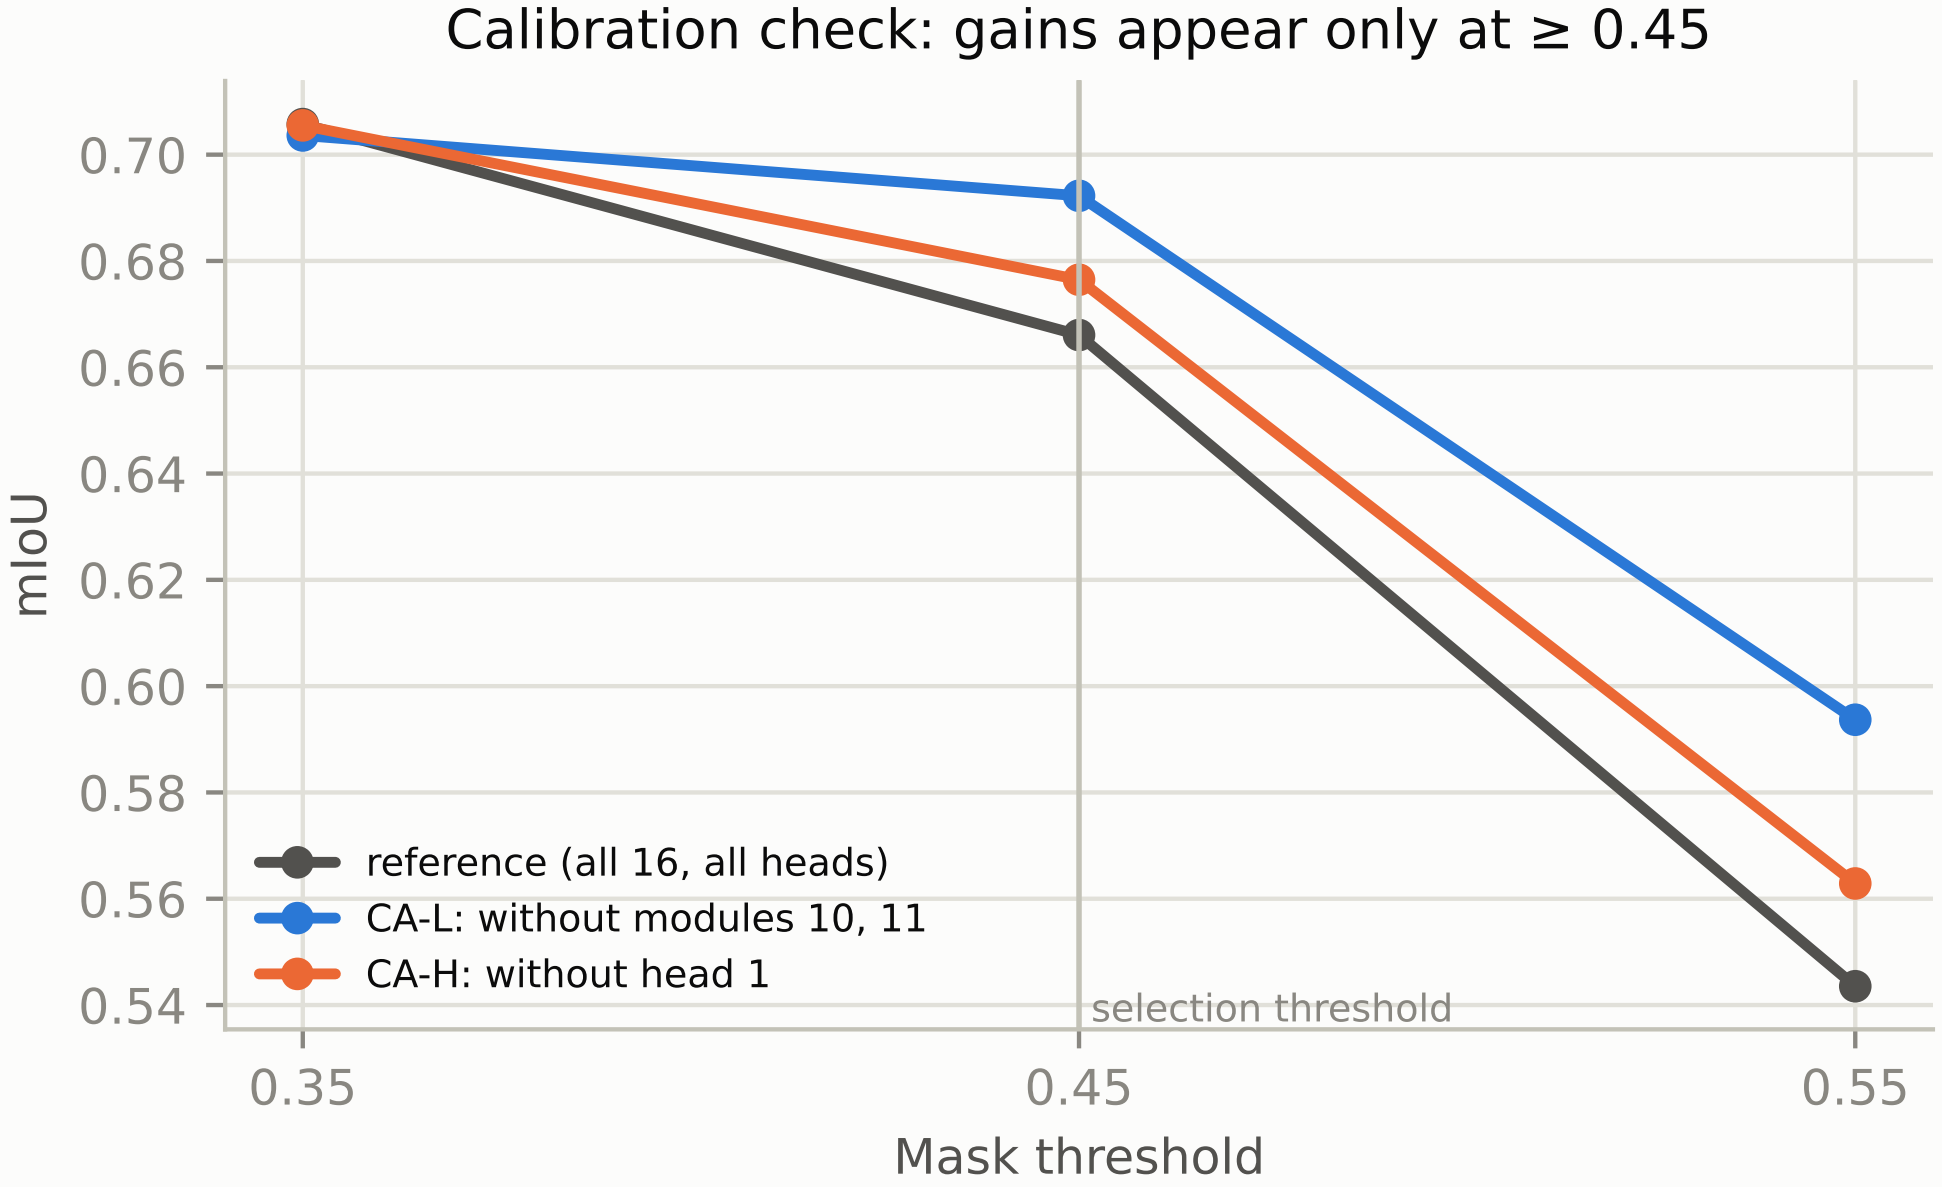
Calibration check: gains appear only at ≥ 0.45
mIoU
0.70
0.68
0.66
0.64
0.62
0.60
0.58
0.56
0.54
reference (all 16, all heads)
CA-L: without modules 10, 11
CA-H: without head 1
selection threshold
0.35
0.45
0.55
Mask threshold