

**HISTOGRAM OF GRADIENT ORIENTATIONS OF EEG SIGNAL
PLOTS FOR BRAIN COMPUTER INTERFACES**

por
Rodrigo Ramele



EN CUMPLIMIENTO PARCIAL DE LOS
REQUISITOS PARA OPTAR AL GRADO DE
DOCTOR EN INGENIERÍA INFORMATICA

DEL

INSTITUTO TECNOLÓGICO DE BUENOS AIRES
BUENOS AIRES, ARGENTINA
30 DE NOVIEMBRE, 2018

INSTITUTO TECNOLÓGICO DE BUENOS AIRES

DEPARTAMENTO DE DOCTORADO

Los aquí suscriptos certifican que han asistido a la presentación oral de la Tesis
“Histogram of Gradient Orientations of EEG Signal Plots for Brain Computer Interfaces” cuyo autor es **Rodrigo Ramele** completando parcialmente, los requerimientos exigidos para la obtención del Título de **Doctor en Ingeniería Informatica**.

Fecha: 30 de Noviembre, 2018

Directores:

Dr. Juan Miguel Santos

Dra. Ana Julia Villar

Tribunal de Tesis:

Dra. Jurado

Dr. Jurado

Dr. Jurado

INSTITUTO TECNOLÓGICO DE BUENOS AIRES

Fecha: **30 de Noviembre, 2018**

Autor: **Rodrigo Ramele**

Título: **Histogram of Gradient Orientations of EEG Signal Plots for
Brain Computer Interfaces**

Departamento: **Doctorado**

Título Académico: **Doctor en Ingeniería Informatica** Convocatoria: **Mes Año**

Por la presente se otorga permiso al Instituto Tecnológico de Buenos Aires (ITBA) para: (i) realizar copias de la presente Tesis y para almacenarla y/o conservarla en el formato, soporte o medio que la Universidad considere conveniente a su discreción y con propósitos no-comerciales; y, (ii) a brindar acceso público a la Tesis para fines académicos no lucrativos a los individuos e Instituciones que así lo soliciten (incluyendo, pero no limitado a la reproducción y comunicación al público no comercial de toda o parte de la Tesis, a través de su sitios o páginas Web o medios análogos que en el futuro se desarrollen).

A excepción de lo autorizado expresamente en el párrafo precedente, me reservo los demás derechos de publicación y, en consecuencia, ni la Tesis ni extractos de la misma podrán ser impresos o reproducidos de otro modo sin mi previo consentimiento otorgado por escrito.

Declaro que he obtenido la autorización para el uso de cualquier material protegido por las leyes de propiedad intelectual mencionado o incluido en la tesis (excepto pasajes cortos, transcripciones, citas o extractos que solo requieran ser referenciados o citados por escrito) y que el uso que se ha hecho de estos está expresamente reconocido por las leyes aplicables en la materia.

Finalmente, manifiesto que la presente autorización se firma en pleno conocimiento de la Política de Propiedad Intelectual del ITBA y, en forma específica, del Capítulo 2.3. referido a la titularidad de derechos de propiedad intelectual en el ITBA y/o, según el caso, a la existencia de licencias no exclusivas de uso académico o experimental por parte del ITBA de la Tesis o la obra o de las invenciones allí contenidas o derivadas de ella.

Hago entrega en este acto de un ejemplar de la Tesis en formato impreso y otro en formato electrónico.

Firma del Autor

Contents

Abstract	ix
Resumen	xiii
Lists of Publications	xv
Acknowledgements	xvii
List of Acronyms	xx
List of Tables	xxi
List of Figures	xxiv
List of Symbols	xxv
Chapter 1 Introduction	1
1.1 Significance	3
1.2 Summary	4
Chapter 2 Interface between the Computer and the Brain	5
2.1 Brain Computer Interface Model and Architecture	8
2.2 Signal Processing	9
2.3 The Forward and Inverse Model	11
2.4 Brain Signals Measuring Techniques	11
2.5 Electroencephalography	13
2.6 BCI EEG Paradigms	17
2.7 State of the Art of BCI Algorithms for EEG processing	19
2.8 EEG Waveform Analysis	20
2.8.1 EEG Waveform Characterization	20
2.8.2 EEG Waveform Analysis Algorithms	22

Chapter 3 From signals to images	29
3.1 Electroencephalographic Plotting	29
3.2 Signal to Image transformation	30
3.3 Standardized plotting	34
3.4 Autoscaled plotting	34
3.5 Zero-Level	34
3.6 Image Size	35
3.7 EEG Signal Plot	36
3.8 Interpolation	36
3.9 Resolution and Precision	38
Chapter 4 The Histogram of Gradient Orientations of Signal Plots	41
4.1 Introduction	41
4.2 Feature Extraction: Histogram of Gradient Orientations	42
4.3 Keypoint Location	43
4.4 Patch Geometry	44
4.4.1 Oscillatory Processes	47
4.4.2 Transient Events	47
4.5 Classification	47
4.6 BCI Algorithm	48
4.A Implementation Summary	48
Chapter 5 Alpha Wave: inhibition signal	53
5.1 Introduction	53
5.2 Materials and Methods	54
5.2.1 Dataset I - Emotiv EPOC alpha waves own dataset	54
5.2.2 Dataset II - AlphaNet Dataset	56
5.2.3 Parameters	56
5.3 Results	57
5.4 Conclusion	58
Chapter 6 Motor Imagery: the hunt for a greek letter	61
6.1 Introduction	61

6.2	Materials and Methods	61
6.3	Results	62
6.4	Conclusion	64
Chapter 7	Event Related Potential: The P300 Wave	65
7.1	Introduction	65
7.2	Materials and Methods	66
7.2.1	Preprocessing Pipeline	67
7.2.2	Speller Matrix letter Identification	69
7.2.3	Experimental Protocol	70
7.3	Results	78
7.4	Conclusion	84
Chapter 8	Epilogue	89
8.1	Conclusion	89
8.2	Future Work	92
Appendix A	BCI en Argentina	95
Appendix B	Walkthrough BCI	99
Appendix C	SIFT	101
Appendix D	Negative Results	103
D.1	Keypoint location	103
D.2	Classification algorithms	103
Bibliography		104

Abstract

Brain Computer Interface (BCI) or Brain Machine Interfaces (BMI), has proved the feasibility of a distinct non-biological communication channel to transmit information from the Central Nervous System (CNS) to a computer device. Promising success has been achieved with invasive BCI, though biocompatibilities issues and the complexity and risks of surgical procedures are the main drive to enhance current non-invasive technologies.

Electroencephalography (EEG) is the most widespread method to gather information from the CNS in a non-invasive way. Clinical EEG has traditionally focused on temporal waveforms, but signal analysis methods which follow this path has been overshadow in BCI research.

This thesis propose a method and framework to analyze the waveform, the shape of the EEG signal, using the histogram of gradient orientations, a fruitful technique from Computer Vision which is used to characterize image local features. Inspiration comes from what traditionally electroencephalographers have been doing for almost a century: visually inspecting raw EEG signal plots.

This technique can be outlined in five steps, (1) signal preprocessing, (2) signal segmentation, (3) transformation on a channel by channel basis of each signal segment into a binary image of a signal plot, (4) assignment of keypoint location on a position over the newly created image depending on the physiological phenomena under study and finally (5) the calculation of the histogram of gradient orientations using finite differences from the image around this keypoint. This method generates a feature, a normalized 128-dimension descriptor. This feature is used to compare the signal segments that were used to generate them, hence to analyze the underlying cognitive phenomena.

The validity of the method is verified by studying three cognitive patterns. First, Visual Occipital Alpha Waves are analyzed. An experimental protocol is designed and a dataset is produced using a commercial-grade EEG device. Additionally, the ability of the method to capture oscillatory processes is verified by analyzing a public dataset. Moreover, this methodology is extended to study a related oscillatory process: Motor Imagery Rolandic Mu rhythms. The performance of the method to discriminate right vs left motor imagery

against a public dataset of healthy subjects, is verified. Results are reported.

Finally, the method is modified to capture transient events, particularly the P300 Event Related Potential (ERP). A description on how to extract the ERP from the EEG segment is offered, and a detailed depiction of how to implement a P300-Based BCI Speller application is outlined. Its performance is verified by processing a public dataset of Amyotrophic Lateral Sclerosis (ALS) patients and contrasted against an own dataset produced in-house replicating the same experimental conditions. Results are compared against other methods referenced in the bibliography

The benefits of the approach presented here are twofold, (1) it has a universal applicability because the same basic methodology can be applied to detect different patterns in EEG signals with applications to BCI and (2) it has the potential to foster close collaboration with physicians and electroencephalograph technicians because this direction of work follows the established procedure of the clinical EEG community of analyzing waveforms by their shapes.

Resumen

Las interfaces BCI (Brain Computer Interfaces, interfaces cerebro computadora) o BMI (Brain Machine Interfaces, interfaces cerebro máquina) han surgido como un nuevo canal de comunicación entre el cerebro y las computadoras, máquinas o robots, distinto de los canales biológicos estándar. Se han obtenido resultados prometedores en el empleo de la variante invasiva de BCI pero, además de los problemas de biocompatibilidad, los procedimientos quirúrgicos requeridos son complejos y riesgosos. Estas razones, han impulsado las mejoras de las tecnologías no invasivas.

La electroencefalografía (EEG) es el método más difundido para obtener información del sistema nervioso central de manera no invasiva. La electroencefalografía clínica se ha enfocado tradicionalmente en el estudio de las formas de ondas temporales, pero los métodos de procesamiento de señales que exploren esta metodología han sido ignorados en las investigaciones sobre BCI.

Esta tesis propone un método y un marco para analizar las formas de las señales de EEG utilizando los histogramas de gradientes orientados, una técnica de visión por computadora que es utilizada para identificar y clasificar características locales en regiones de una imagen. Este procedimiento está inspirado en lo que tradicionalmente los técnicos electroencefalógrafos han realizado por casi un siglo: inspeccionar visualmente los registros electroencefalográficos.

El método propuesto puede resumirse en 5 pasos, (1) preprocesamiento de la señal cruda, (2) segmentación de la señal, (3) obtención de una gráfica blanco y negro de la señal canal por canal, (4) asignación de una localización dentro de la imagen para posicionar un parche de un determinado tamaño y escala dependiendo del fenómeno cognitivo en estudio, y (5) cálculo del histograma de los gradientes orientados de la intensidades de los pixeles usando diferencias finitas. Este mecanismo genera un vector de 128 dimensiones, que se utiliza para comparar los segmentos de señales entre sí, y que permite entonces analizar el fenómeno cognitivo subyacente.

La validez del método se verifica estudiando tres patrones cognitivos. Primero se analizan las ondas alfa de la corteza visual occipital sobre dos conjuntos de registros: uno obtenido a partir de la aplicación de un protocolo experimental y mediante la utilización de un

dispositivo electroencefalográfico digital de uso comercial, y otro obtenido de una base de datos pública de registros electroencefalográficos. Segundo, se analiza otro tipo de onda oscilatoria conocida como ritmo Mu correspondiente a la corteza motora que puede ser también activada si el sujeto imagina una actividad motora. Se reporta la efectividad del método para discriminar entre la actividad de la corteza motora derecha e izquierda en base al estudio de otro conjunto de registros públicos de pacientes sanos. Los resultados son reportados y publicados.

Finalmente, el método propuesto se utiliza para estudiar eventos transitorios, particularmente, el potencial evocado P300. La eficiencia del sistema es verificada mediante el procesamiento de un conjunto de registros públicos de pacientes con esclerosis lateral amiotrófica, y corroborada contra un conjunto de registros de sujetos sanos obtenidos de manera experimental, replicando el mismo protocolo. Para ambos conjuntos de registros, se realiza una descripción detallada de cómo extraer este potencial de la señal de EEG, y se implementa un procesador de texto basado en P300 para comparar el desempeño del método propuesto respecto de otros citados en la bibliografía.

Los beneficios de esta propuesta se resumen en, (1) tiene una aplicación potencialmente universal, debido que el mismo tipo de metodología puede ser aplicada para detectar cualquier tipo de patrón obtenido en la señal de EEG con potenciales aplicaciones a BCI, y (2) ofrece la posibilidad de incentivar la colaboración y utilización de estas técnicas en la clínica médica especializada en electroencefalografía ya que esta perspectiva basada en el estudio de las formas de onda de las señales, es un procedimiento conocido y ya establecido por esa comunidad.

Lists of Publications

Conference Proceedings,

- Ramele, R., A.J.Villar, and J.M.Santos."A Brain Computer Interface Classification Method Based on SIFT Descriptors." VI Latin American Congress on Biomedical Engineering CLAIB 2014, Paraná, Argentina 29,30,31 October 2014. Springer International Publishing, 2015.
- Ramele, R., A. J. Villar, and J. M. Santos. "A Brain Computer Interface Classification Method Based on Signal Plots." 4th Winter Conference on Brain Computer Interfaces, Yongpyong, Korea, February 2016. IEEE Signal and Processing, 2016.

Peer-reviewed Journals,

- Ramele, R., A. J. Villar, and J. M. Santos. "Histogram of Gradient Orientations of Signal Plots applied to P300 Detection", Frontiers in Neuroscience, Special Issue:"Computational Methodologies in Brain Imaging and Connectivity: EEG and MEG Applications" (Under Review)
- Ramele, R., A. J. Villar, and J. M. Santos. "EEG Waveform Analysis of P300 ERP with applications to Brain Computer Interfaces", MDPI Brain Sciences Journal, Special Issue:"Brain-Computer Interfaces for Human Augmentation" (Under Review)

Poster Presentations,

- Ramele, R., A. J. Villar, and J. M. Santos. Poster Presentation: "Assistive Brain Computer Interfaces", HYPER Workshop 2011, La Alberca, Salamanca, Spain, Sept 18-23, 2011.
- Ramele, R., A. J. Villar, and J. M. Santos. Poster Presentation: "Towards a Cognitive Monitoring BCI Application for Assistive Robotics", COGCOMP 2013, Stirling, Scotland, UK, Aug 25-30, 2013.
- Ramele, R., A. J. Villar, and J. M. Santos. Poster Presentation: "Histogram of Gradient Orientations of Signal Plots applied to Brain Computer Interfaces", BCI Society Conference "BCIs: Not Getting Lost in Translation", Asilomar, CA, USA, May 21-25, 2018.

Acknowledgements

Es un falacia creer que existe alguna actividad en nuestra vida que la hacemos solos. Todos nosotros tenemos una interminable lista de personas a quienes le debemos agradecimiento, desde el primer segundo respirado hasta el último, y especialmente por aquellos actos ciclópeos que nos demandan todo lo que tenemos.

List of Acronyms

The following abbreviations are used in this thesis:

- ALS: Anterior Lateral Sclerosis
- EEG: electroencephalography
- BCI: Brain Computer Interfaces
- BMI: Brain Machine Interfaces
- BNCI: Brain-Neural Computer Interfaces
- SNR: Signal to Noise Ratio
- CNS: Central Nervous System
- DC: Direct Current
- ERP: Event-Related Potential
- P300: Positive deflection at 300 ms
- ITR: Information Transfer Rate
- BTR: Bit Transfer Rate
- SIFT: Scale Invariant Feature Transform
- SHCC: Slope Horizontal Chain Code
- PE: Permutation Entropy
- MP: Matching Pursuit
- ICU: Intensive Care Unit
- EKG: Electrocardiogram
- PAA: Period Amplitude Analysis
- SVM: Support Vector Machine
- NBNN: Naive Bayes Near Neighbor

List of Tables

3.1	Reference Values for Precision and Resolution	39
7.1	Single Channel Character Recognition Rates for ALS patient's Dataset	78
7.2	Single Channel Character Recognition Rates for Healthy Subject's Dataset	79
7.3	Character Recognition Rates for ALS patient's dataset	80
7.4	Character Recognition Rates for Healthy Subject's Dataset	81
7.5	Pseudo-real Dataset Speller Performance	85
7.6	Dataset IIb BCI Competition II (2003) Speller Performance	85

List of Figures

2.1	BCI Block Diagram	9
2.2	Neuroanatomical structures of the brain	10
2.3	EEG Volume Conduction	12
2.4	Sample Multichannel EEG signal	14
2.5	Electrode Locations	15
2.6	Wearable portable Digital Electroencephalograph	15
3.1	EEG Signal Mapping to Images	31
3.2	Image Coordinate System	32
3.3	Signal plot of an impulse response	35
3.4	Signal Plotting: Interpolation	37
4.1	Histogram of Gradient Orientations for ERP	44
4.2	Keypoint Locations	45
4.3	Patch Geometry	46
4.4	NBNN Classification	50
4.5	NBNN Classification	51
5.1	Alpha Waves Wiggles	54
5.2	Spectrum components obtained by the FFT of Alpha Waves	55
5.3	EPOC Emotiv Alpha Waves Dataset	56
5.4	Power Spectral Density of the Dataset I	57
5.5	Dataset I Classification Rate	58
5.6	PhysioNet Dataset Classification Rate	58
6.1	Motor Imagery Experimental Protocol	63
6.2	Motor Imagery Accuracy	64
7.1	P300 Speller Matrix	66
7.2	P300 Speller Matrix Letter Identification	67
7.3	g.Tec Device	73

7.4	P300 ERP Template	74
7.5	Pseudo-real Dataset EEG Streams	76
7.6	P300 Averaged Segments for a single-intensification sequence	77
7.7	ALS Patients Dataset P300 Performance Curves	80
7.8	P300 Classification Boxplots	81
7.9	Sample P300 Patches	82
7.10	Experiment I Pseudo-real Dataset Speller Performance	83
7.11	Experiment II Pseudo-real Dataset Speller Performance	84
7.12	Experiment III Pseudo-real Dataset Speller Performance	84
7.13	Dataset IIb BCI Competition II (2003) Speller Performance	86

List of Symbols

N	Sample points
F_s	Sampling Frequency
w	Signal Segment Size
γ	Signal Amplitude Scale Factor
γ_t	Time Scale Factor
kp	Keypoint
S_t	Horizontal Patch Scale
S_v	Vertical Patch Scale
\mathbf{S}_x	Patch Width
\mathbf{S}_y	Patch Height
d	Descriptor
Δ_s	Pixels in unit scale
kp_d	Keypoint Density
λ	Signal Span
$\Delta\mu V$	Peak-to-peak Amplitude
W_x	Image Width
H_y	Image Height
bpc	Best Performing Channel
k_a	Intensification Sequences Repetitions
C	Number of available channels

Chapter 1

Introduction

The brain is a machine with the sole purpose to respond appropriately to external and internal events, and to spread its own presence into the environment where it belongs ¹. Hence, the brain needs to communicate and it posses mainly two natural ways to do it: hormonal or neuromuscular. When those natural channels are interrupted, they are not available or when it needs to increase or enhance the communication alternatives, a new artificial communication channel which is not based on natural pathways, is needed. It is based, instead, on a new technology feat that decode the information from the CNS and transmit it directly to a computer or machine.

Brain Computer Interface, BCI, is a system that measures brainwaves and converts them into artificial output that replaces, restores, enhances, supplements and improves natural brain output and changes the ongoing interactions between the Central Nervous System and its external or internal environment [126]. Brain Machine Interface (BMI) generally refers to invasive devices. Brain Neural Computer Interfaces (BNCI) may refer to devices that do not exclusively use information from the CNS, they also may use any kind of biological signal that can be harnessed with the purpose of volitionally transmit information. Above all, every kind of BCI system is after all a communication device.

There are five motives behind BCI: the **first** is the aging of societies: estimated for 2025, 800 millions people will be over 65 years old, and 2/3 of them on developing countries [68]. This may lead to an increased tendency to develop diseases that affect motor pathways and require some form of assistance from technology. The **second** reason is the digital world that calls for more methods of interactions. This digital society [32] demands more mechanisms to interpret the surrounding world and to translate human intentions through digital gadgets. Additionally, the advancement of smart wearable devices that can be used

¹The sensorimotor Hypothesis [129, 126] and The Extended Mind Thesis [23]

over the skin is also pushing the frontiers to go deeper into the body to find there useful information. The **third** motive is the impulse of neuroscience research and the advances that this discipline is having worldwide. The **fourth** reason is the potentialities of BCI as a clinical tool which can help to diagnose diseases, as aid in the field of neurorehabilitation, or to provide neurofeedback. The **fifth**, final and most important motive, the reason behind Brain Computer Interfaces, is the still unfulfilled societal promise of social inclusion of people with disabilities. It is known that the ability to walk and live independently is a key indicator of psychological and physical health, and we have to do all we can to provide the technological tools to achieve this goal [94, 24, 126, 54].

In line with the aforementioned motives, there are several applications currently under development for BCI. People affected by any kind of neurodegenerative diseases, particularly those affected by advanced stages of Amyotrophic Lateral Sclerosis (ALS) with locked-in syndrome may find in BCIs the only remaining alternative to communicate. Other applications targeted for the general population include alertness monitoring, telepresence, gaming, education, art, human augmentation [130] biometric identification, virtual reality avatar, assistive robotics and education. Novel niches where this new communication channel can be useful are found routinely [79]. In spite of all this hype [38], there is still a long way ahead. This area advanced rapidly but the complexity of brain signals in all their forms is still a big problem to tackle.

Electroencephalography (EEG) is the most widespread device to capture electrical brain information in a non-invasive and portable way, and it is the most used device in BCI research and applications. The clinical and historical tactic to analyze EEG signals were based on detecting visual patterns out of the EEG trace or polygraph[107]: multichannel signals were extracted and continuously plotted over a piece of paper. Electroencephalographers or Electroencephalography technician have decoded and detected patterns along the signals by visually inspecting them [103]. Nowadays clinical EEG still entails a visually interpreted test [107].

In contrast, automatic processing, or quantitative EEG, was based first on analog electronic devices and later on computerized digital processing methods [57]. They implemented mathematically and algorithmically complex procedures to decode the information with good results [130]. The best materialization of the automatic processing of EEG signals rests precisely in the BCI discipline, where around 71.2% is based on noninvasive EEG [44].

Hence, the traditional strategy of analyzing the electroencephalography by signal shapes

on plots, was mainly overshadow in BCI research, and the waveform of the EEG was replaced by procedures that were difficult to link to existing clinical EEG knowledge.

On the other hand, the study of biological visual sensory system provided insights and models that are very useful to understand brain functions. Additionally, they serve as inspiration to develop Computer Vision algorithms that aimed to reproduce a similar level of accuracy as those obtained by biological beings, including humans. The Histogram of Gradient Orientations is one successful method from Computer Vision useful to image recognition that aims to mimetically reproduce how the visual cortex discriminate shapes.

This thesis tries to unravel the following question: is it possible to analyze and discriminate electroencephalographic signals by automatic processing the shape of the waveforms using the Histogram of Gradient Orientations ?

To do that, this thesis unfolds as follows: Chapter 2 gives details of what is Brain Computer Interfaces and the particularities of the first window of the electric mind: the EEG. It also covers the state of the art in the methods that explore the waveform automatically. The Chapter 3 provides an overview on the procedure to construct a plot representing the signal. Chapter 4 is the core of this thesis and describes the Histogram of Gradient Orientations and how it can be used to process one-dimensional signals. Next, results and experimental procedures are described to analyze EEG signals and implement BCI paradigms: Alpha Waves are covered in Chapter 5 and Motor Imagery in Chapter 6. The P300 Wave is studied in Chapter 7. Future Work and Conclusions are addressed in Chapter 8.

1.1 Significance

This thesis propose

- A procedure to construct analyzable 2D-images based on one-dimensional signals.
- A mapping procedure to link time-series characteristics based on feature of the 2D-image representation.
- A feature extraction method for EEG signals that can be used objectively to construct a representation of the waveform.
- A classification algorithm that can be used effectively with these features.

1.2 Summary

- What is this all about?: a method to analyze EEG signals based on extracting local features from their 2D image plot representation.
- What will be found in this thesis?: a point of view that emphasizes the importance of providing mechanisms that help to understand signals based on how they look like on plots.
- Does it work?: It works when the waveform contains the discriminating information. If a person is able to discriminate the signals, this method would also do that.
- Can it be used?: Yes, it can. The developed software is open-source and it can be used out-of-the-box. It is particular useful when an intelligible automatic classification procedure is required.


Chapter 2

Interface between the Computer and the Brain

...the brain is not a passive decoder of information but a dynamic and distributed modeler of a reality...

Nicolelis

With Vidal's work in 1970s, Brain-Computer Interfaces started as a technological amusement, and it steadily moved toward a mature and highly researched area of work. Outstanding success has been achieved with invasive BCI, i.e. with surgically implanted electrodes. Success stories have been made public like Braingate's implant on Jan Scheuermann, Cathy Hutchinson and Dennis Degray [86]. Other works include the total reproduction of arm movement [51], the restoration of reaching and grasping movements through a brain-controlled muscle stimulation device on a person with tetraplegia [2] and the remote control of a manipulator by a macaque using brainwave information [125] albeit of persistent biocompatibility issues and the pervasive complexity and risks of surgical procedures. One noteworthy aspect of this novel communication channel is the ability to transmit information from the central nervous system to a computer device and from there use that information to control a wheelchair [18], as input to a speller application [45], in a Virtual Reality environment [71] or as aiding tool in a rehabilitation procedure [61]. Other novel applications include the real-time control of flight simulators [82] and the implementation of neuroadaptive interfaces where the computer detects the correctness of a given command based on brainwave analysis [132]. Overall, the holy grail of BCI is to implement a new complete and alternative pathway to restore lost locomotion [126].

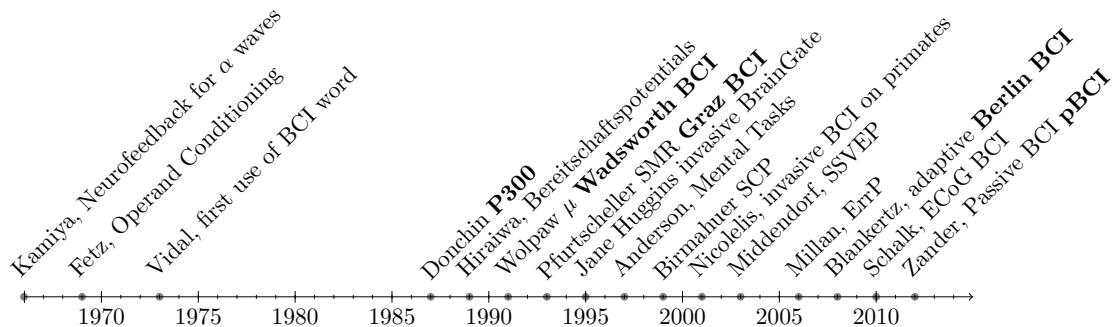

This graphic shows a brief chronology of the main events in BCI history, starting from the early works on Neurofeedback in the 70s and walking through the different paradigms. In recent years, this discipline has gained mainstream public awareness with worldwide challenge competitions like Cybathlon [97, 83] and even been broadcasted during the inauguration ceremony of the 2014 Soccer World Cup. New developments are approaching the out-of-the-lab high-bar and they are starting to be used in real world environments [44, 53]. Moreover, BCI research had rampantly been advanced accomplishing a BCI Society, a BCI Journal, BCI Award, annual conference meetings, practical applications, myriads of startups companies and even included in the Gartner Hype Cycle [38].

From its root as assistive technology it has now expanded to include several application niches like temporal induced disability, neuroergonomics, early detection of human error, affective computing, biometric authentication, telepresence (improvement of haptic interface), cyberinfrastructure and assistive robotics. Intensive Care Units (ICU) and Disorders of Consciousness (DoC) [6] (detection of remaining brain activity in comatose patients) are recent disciplines where BCI is showing tremendous prospects and possible applications.

Their adoption as a clinical tool is still years ahead. Stroke rehabilitation is the only area where clinical trials for BCI are being conducted. It is understood that the neurofeedback provided by a BCI interface improves the prognosis of motor rehabilitation [5].

BCI Definition (circa 2018)

Definition 2.0.1. *A system that measures central nervous system activity and converts it into artificial output that replaces, restores, enhances, supplements, or improves natural CNS output and thereby changes the ongoing interactions between the CNS and its external and internal environment [126].*

Despite all this, its primary objective, its core motive of moving into real applications for disabled people has yet to come [16, 60, 3]. They still lack the necessary robustness, and

its performance is well behind any other method of human computer interaction, including any kind of detection of residual muscular movement [24]. Among the many and current challenges of BCI [16] one which is still perennial is precisely their inability to be used and applied outside the BNCI community and specifically in clinical context.

Quoting experts in the field,

"We yet have an impractical and inaccessible exotica for very specific user groups"
(Allison 2010)

"Effectiveness of non-invasive BCI systems remain limited. . ." (Wolpaw 2011)

"...to ponder if BCIs are really promising and helpful, or if they are simple a passing rod, reinforced by their sci-fi side..." (Lotte 2016)

The feasibility of the system has been proved but there are several challenges in BCI that need to be tackled. They can be summarizing as increasing the ITR, the pervasive low signal-to-noise ratio of brainwaves, particularly of noninvasive signals [69], the reliability of the system, its portability, and the usability of the system [123], and at the same time decreasing the setup, the training and calibration time and the subject's inter/intra variability. The search for practical, relevant, and invariant *features* that convey good-enough information about the underlying cognitive process is still a goal to be achieved [88]. Ethical aspects of BCI [130] must also be considered and handled: cybersecurity threats and privacy concerns, agency and identity issues that might be occurring by deleterious plasticity with BCI users and the strict peg to the *Primum non nocere*¹ mandate.

Hybrid BCI, or Brain Neural Computer Interface, are BCI devices that use not only signals from the CNS, they utilize any kind of available biosignal that can be volitionally modulated to transmit information (this is called dependant BCI). On the other hand, when the pace of the BCI is regulated by external stimulus it is called synchronous and when the user choose their own pace to transmit information, it is often called asynchronous or self-paced BCI.

Recent years have seen an incredible advance of passive BCI, pBCI [131]. The original definition of BCI did not include passive modalities but per definition 2.0.1 it is now part of this discipline. The important aspect is that passive technologies do not entail necessary the volitional requirement to transmit information. EEG-based passive BCI is a promising and

¹*First, do not harm*, in reference to the Hippocratic Oath

advancing area of research and of commercial applications.

2.1 Brain Computer Interface Model and Architecture

The draft architecture of a BCI system can be summarized in Fig 2.1. A volitional control, a will to transmit information, is exerted by a user. A brain signal acquisition device captures his/her signals using a measurement modality. This module obtains the brainwaves and the information is digitalized and transmitted to a computer device. Signal preprocessing is applied to eliminate nuisances and artifacts and to enhance the Signal to Noise Ratio (SNR), or to apply spatial or frequency filters. In the next step, a *feature* is carefully constructed in order to differentiate at least between two different mental states. Finally a classification step is applied to derive the actual information bit out of the system. An application system uses this information to affect some external device. By visual or any other sensory means, the feedback is fed back to the user and a loop is finally closed.

The central point of this system is called the *Brain Machine Dilemma* [126]. The underlying idea is that the BCI system adapts to the user's thinking patterns but at the same time the brain is adapting to what the system is doing, and changing their own signals in the process. This is the reason why it is often called, a *co-adaptive system*, where two different intelligent devices, one biological and the other electronic, try to adapt to each other.

Let X be a multichannel digital signal $X \in \mathbb{R}^{C \times N}$, with N being the length of the digitalized signal in sample points, and C is the number of available channels. This signal matrix is

$$X = \begin{bmatrix} X(1, 1) & \cdots & X(n, 1) & \cdots & X(N, 1) \\ \vdots & & \vdots & & \vdots \\ X(1, c) & \cdots & X(n, c) & \cdots & X(N, c) \\ \vdots & & \vdots & & \vdots \\ X(1, C) & \cdots & X(n, C) & \cdots & X(N, C) \end{bmatrix}. \quad (2.1)$$

The n-column $\mathbf{x}(n)$ of this matrix is a vector for a sample point n in digital time for every available channel. Additionally, $x(n, c)$ is a c-row with the multichannel signal as a scalar time-series for a particular channel c .

The basic model of any BCI is to take this multichannel digital signal $\mathbf{x}(n)$, and transform it to an output control signal $y(n)$ which can be a scalar or binary function. The BCI system

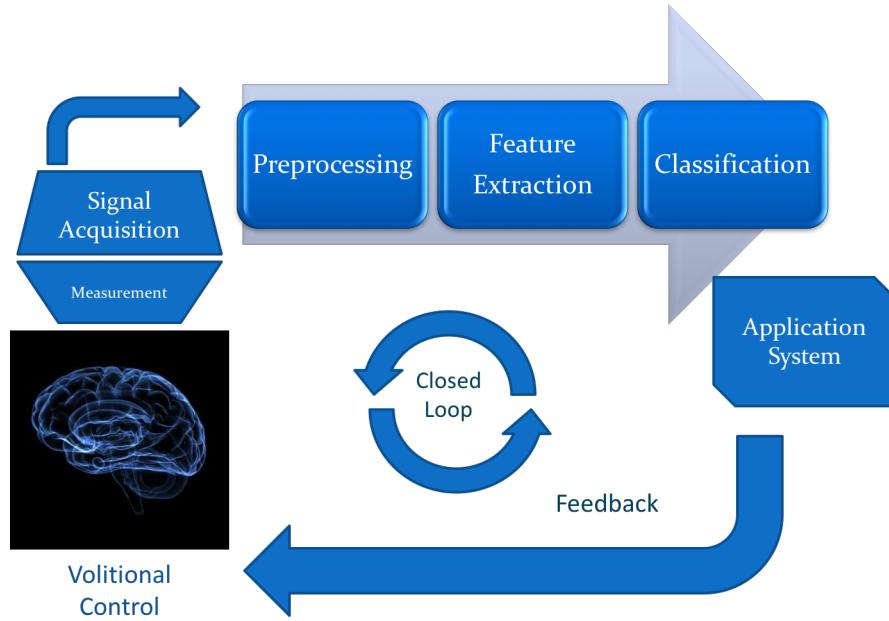


Figure 2.1: General components of a BCI system.

can be modeled as the transformation T , which operates on the equation

$$y(n) = T[\mathbf{x}(n)]. \quad (2.2)$$

What a BCI system must do, is to take at least a single bit of information out of $y(n)$ and use that information to derive some action.

2.2 Signal Processing

From this signal processing point of view, BCIs are:

- Causal: $y(n) = T[\mathbf{x}(m)]$, where $m \leq n$. The action of a BCI system depends on the history of the captured brainwaves.
- Dynamic: $y(n) = T[\mathbf{x}(m), \dot{\mathbf{x}}(m), \ddot{\mathbf{x}}(m), \dots]$. A BCI system is dynamic, where the output function do not depend only on the current value being observed, it does depend on its dynamic interactions.
- Time invariant: $y(n) = T[\mathbf{x}(n)] \Rightarrow y(n-p) = T[\mathbf{x}(n-p)]$. The output of a BCI system does not depend on the particular time frame where it is being used. However, Adaptive BCI, which do adapt to the user behavior are in general time variant.

- Nonlinear: a system is linear when $T[a_1\mathbf{x}(n) + a_2\mathbf{x}(n)] = a_1T[\mathbf{x}(n)] + a_2T[\mathbf{x}(n)]$. Due to brainwave complexity, BCI systems are not linear.
- Multirate or broadband [77]: The energy of brainwave spectrum is not confined to a certain band, and almost all frequency channels convey some information.

There are several filters that can be applied to the system to eliminate artifacts, enhance the signal, and to ease the detection of the discriminative information.

Static filters like square or logarithmic, were traditionally used in analog signal processing and are currently already embedded in the measuring device. Wiener and Kallman filters are usually applied to invasive techniques [49]. The filter, particularly when it is linear, can be viewed as the matrix M in:

$$y(n) = MT[\mathbf{x}(n)] \quad (2.3)$$

Spatial filters are carefully adapted to the arrangement of sensors around or within the head and they emphasize the spatial structure of the information that is being captured. The head is divided in anatomical regions and electrode locations around the head are arranged according to neuroanatomical planes or axes (Figure 2.2).

Spectral filters, on the other hand, do consider brainwaves as a digital signal, and they perform different transformations based on the spectral information contained within the signal $\mathbf{x}(n)$. They can be combined and aggregated creating *filter banks* to enhance signal quality.

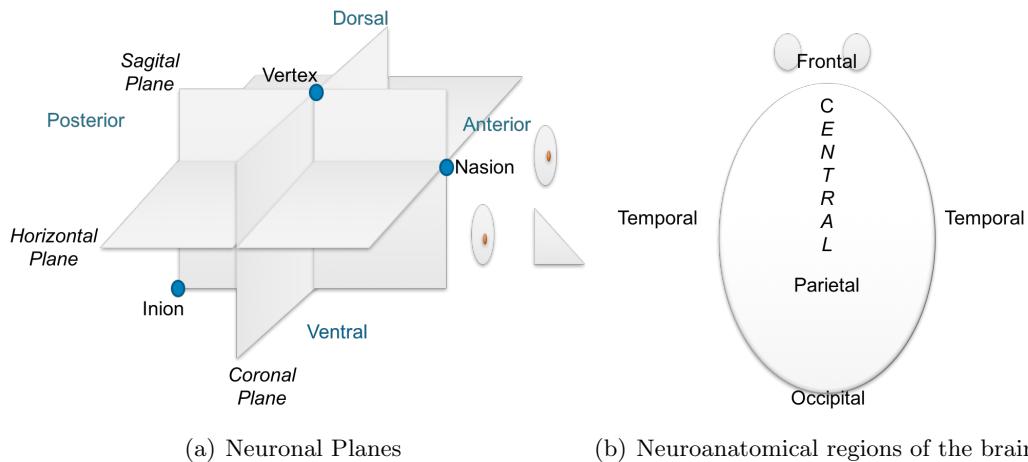


Figure 2.2: Neuronal Planes regularly used in neuroscience research. In BCI they are used to understand electrode location and spatial filters.

2.3 The Forward and Inverse Model

Brainwaves are obtained via sensors. Each one of them captures only a part or a version of the information. However, whatever is actually happening inside the brain can be only recovered indirectly from the *sensor space*. From there, the information can be traced back to the real landscape where the information source is located, inside the *source space*. This is a regular problem found in engineering and it is not different in BCI. *Calculating* the signal on each a sensor from a projection of a known source of information from within the head is called *The Forward Problem*[87, 126] and doing the opposite, *estimating* the contributions of different sources to whatever activity is found on sensors is called *The Inverse Problem*. Although the latter is a complex ill-posed problem, it is more relevant in BCI because it allows to determine source origins that can be mapped more directly to cognitive activities.

Particularly for noninvasive electrophysiological modalities, an additional problem makes things harder. Due to its electromagnetic properties, the brain acts like conductive gel, and any signal that is generated inside the brain is irradiated to every direction and it can influence every sensor regardless of its position. This is called *Volume conduction* [79, 17] and can be visualized in Figure 2.3.

2.4 Brain Signals Measuring Techniques

The measuring technique determines the most important taxonomic differentiation in BCI, according to the methodology that is applied to extract the information from the CNS. All of them have been used so far for BCI applications.

1. EEG Electroencephalography: it is based on the electrical potential detected at the scalp. It is explained in detail in Section 2.5.
2. ECoG Electrocorticography: the electrodes are located bellow the skull and above the cortex, on the exposed region of the brain. Thus, a craniotomy is required. It offers a very high temporal resolution, broader bandwidth and much better spatial resolution than EEG. This modality has allowed very good performance in complex BCI schemes like speech synthesis from direct neural signals [50].
3. MEG Magnetoencephalography: when active neurons generate electric currents, minuscule magnetic fields are generated. It is considered complementary to EEG and ECoG, due to the fact that it is sensitive to neurons firing parallel to the scalp,

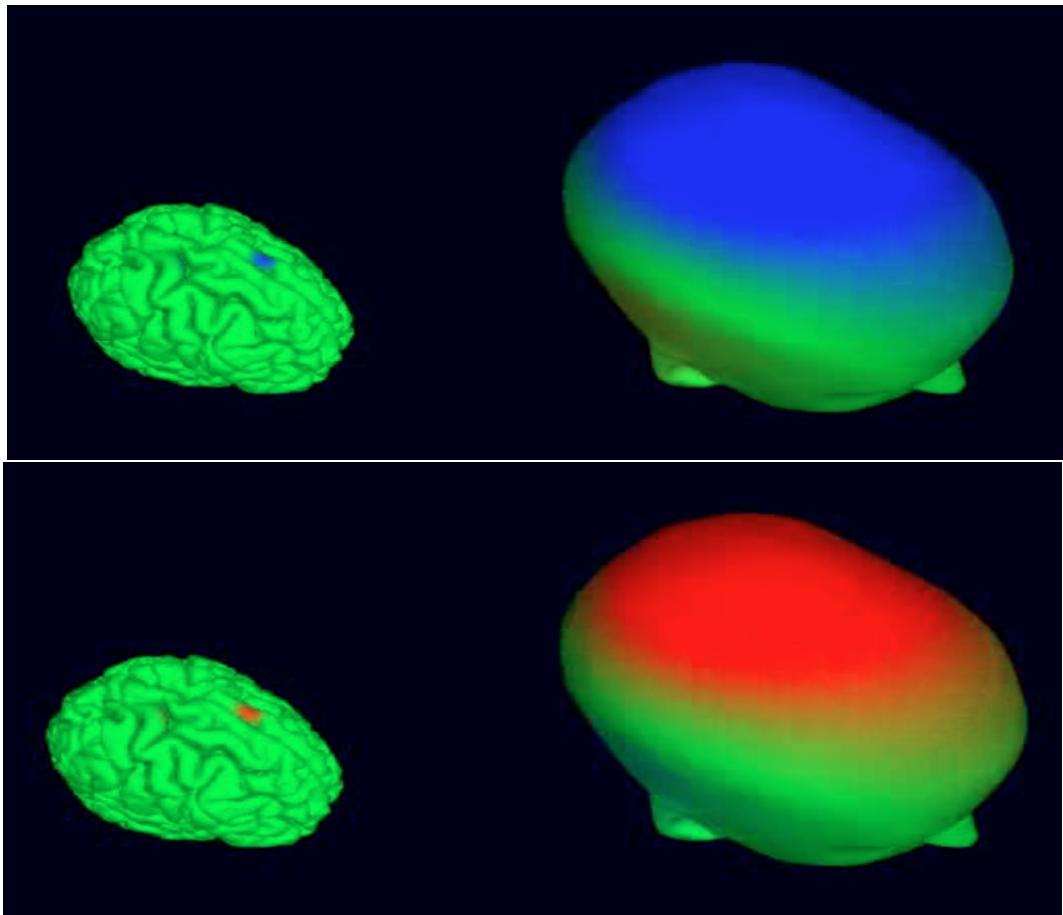


Figure 2.3: A source signal with positive/negative polarity is generated in a very specific region of the brain but due to volume conduction their influence affects a widespread area of the scalp where sensors are located (Image of the brain from Swartz Center for Computational Neuroscience).

which are hard to detect in EEG and MEG. Although MEG equipment is bulky and room-size, recent advances [12] are aiming to develop portable and wearable versions.

4. PET Positron Emission Tomography: this radio nuclear measuring device, use a tracer molecule like fludeoxyglucose, which emits positrons. Positrons interacts with biological tissue generating photons in exact opposite directions. The tracer is spread around the body and the brain, and its concentration is higher in those areas where active neuron firing is being conducted which requires more glucose [78].
5. fMRI functional Magnetic Resonance Imaging: this noninvasive, non-portable measuring techniques, measures the so-called BOLD response: the Blood Oxygen Level-Dependent contrast. This is based on the principle that firing neurons generates an imbalance of oxyhemoglobin and deoxyhemoglobin which can be detected on the magnetic resonator, with a very high spatial accuracy.
6. fNIR functional Near Infra Red Spectroscopy: it also measures the concentration changes of oxy/deoxy-hemoglobin using light pulses of near-infrared wavelengths. The different types of hemoglobin molecules absorb these light frequencies at different rates. It is an indirect measure of brain activity. Although it provides very good spatial localization, temporal localization is hindered by the hemodynamic response [78].
7. INR Intracortical Neuron Recordings. Particularly LFP (iEEG, intracranial EEG[17]) and microelectrodes [2] (e.g. Utah array).

ECoG and INR are invasive technologies that require a neurosurgery or craniotomy. The implantation of electrodes is performed inside the skull for the former, and inside the brain for the latter. All the remaining measuring techniques are external or noninvasive.

2.5 Electroencephalography

Above all, electroencephalography, is the most widespread method to gather information from the CNS in a non-invasive way. It is of particular interest in BCI mainly because of its non-invasiveness, its optimal time resolution and acceptable spatial resolution. Moreover, it is portable, cheap, wearable and can be more easily integrated into fashionable designs aimed for real users, which prefer cap-like devices [54].

The electroencephalography consists on the measurement of small variations of electrical voltage over the scalp. This represents the summed activity of post-synaptic potentials

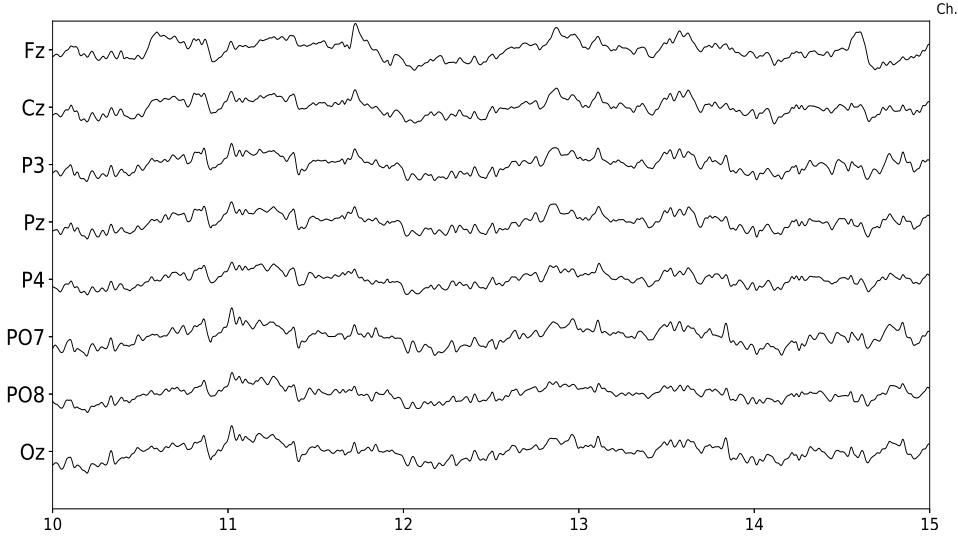


Figure 2.4: Sample EEG signal obtained from (g.Nautilus, g.Tec, Austria). Time axis is in seconds and five seconds are displayed. The eight channels provided by this device are shown.

PSPs of pyramidal neurons located perpendicular to the scalp [79]. Only one percent of synchronized activity of pyramidal neurons are stronger than the remaining desynchronized neurons [103] and explain ninety-nine percent of the signals obtained from EEG. This technique is one of the most widespread used methods to capture brain signals and was initially developed by Hans Berger in 1924 and has been extensively used for decades to diagnose neural diseases and other medical conditions.

The first characterization that Dr. Berger detected was the Visual Cortical Alpha Wave, the *Berger Rythm* [57]. He understood that the amplitude and shape of this rhythm was coherently associated to a cognitive action (eyes closing). We should ask ourselves if the research advancement that came after that discovery would have happened if it weren't so evident that the shape alteration was due to a very simple and verifiable cognitive process.

The EEG signal is a highly complex multi-channel time-series. It can be modeled as a linear stochastic process with great similarities to noise [111]. It is measured in microvolts, and those slight variations are contaminated with heavy endogenous artifacts and exogenous spurious signals.

The device that captures these small variations in current potentials over the scalp is called the electroencephalograph (Figure 2.6). Electrodes are located in predetermined positions over the head, usually embedded in saline solutions to facilitate the electrophysiological interface and are connected to a differential amplifier with a high gain which allowed the

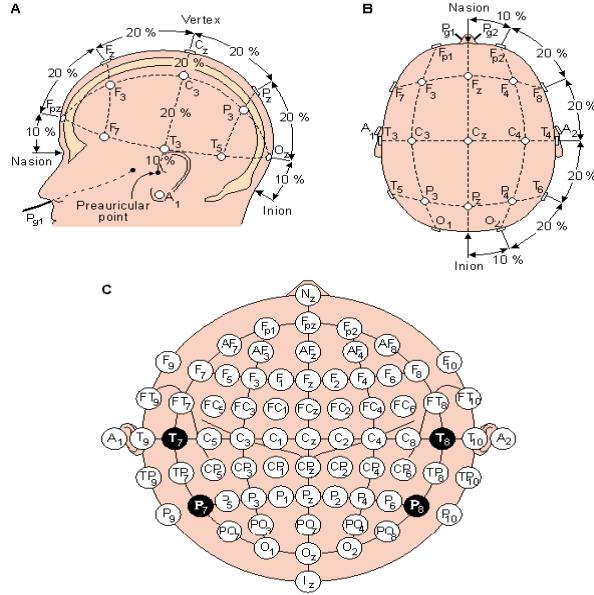


Figure 2.5: International 10-20 system that standardize electrode locations over the scalp.



Figure 2.6: Digital and wearable electroencephalographs.

measurement of tiny signals. Although initially analog devices were developed and used, nowadays digital versions connected directly to a computer are pervasive. A detailed explanation on the particularities and modeling of EEG can be obtained from [55], and a description of its electrophysiological aspects from [46].

Overall, EEG signals can be described by their phase, amplitude, frequency and *waveform*. The following components regularly characterize EEG signals:

- Artifacts: These are signal sources which are not generated from the CNS, but can be detected from the EEG signal. They are called endogenous or physiological when they are generated from a biological source like face muscles, ocular movements, etc., and exogenous or non-physiological when they have an external electromagnetic source like

line induced currents or electromagnetic noise [124]. Ambulatory studies or out-of-the lab studies introduces artifacts that are derived from the person movement, from any kind of muscular electrical stimulator on rehabilitation treatments and also from other devices in hybrid BCI, or multi-modal BCIs.

- Non-Stationarity: the statistical parameters that describe the EEG as a random process are not conserved through time, i.e. its mean and variance, and any other higher-order moments are not time-invariant [57].
- DC drift and trending: in EEG jargon, which is derived from concepts of electrical amplifiers theory, Direct Current (DC) refers to very low frequency components of the EEG signal which varies around a common center, usually the zero value. DC drift means that this center value drifts in time. Although sometimes considered as a nuisance that needs to get rid of, it is known that very important cognitive phenomena like slow cortical potentials or slow activity transients in infants do affect the drift and can be used to understand some particular brain functioning [119, 103].
- Basal EEG activity: the EEG is the compound summation of myriads of electrical sources from the CNS. These sources generate a baseline EEG which shows continuous activity with a small or null relation with any concurrent cognitive activity or task.
- Intra-subject and Inter-subject variability: electroencephalographic signals vary greatly from person to person. Additionally, EEG can be affected by the person's behavior like sleep hygiene, caffeine intake, smoking habit or alcohol intake previously to the signal measuring procedure [35].

Regarding how the EEG activity can be related to an external stimulus that is affecting the subject, it can be considered as

- Spontaneous: generally treated as noise or basal EEG.
- Evoked: activity that can be detected synchronously after some specific amount of time from the onset of the stimulus. This is usually referred as time-locked. In contrast to the previous one, it is often called induced activity.

Additionally, according to the existence of a repeated rhythm, the EEG activity can be understood as

- Rhythmic: EEG activity consisting in waves of approximately constant frequency. It is often abbreviated RA (regular rhythmic activity). They are loosely classified by their frequencies, and their naming convention was derived from the original naming used by Hans Berger himself:
 - Delta (0-4 Hz)
 - Theta (4-8 Hz)
 - Alpha Waves (10 Hz)
 - Sigma (12-16 Hz)
 - Beta (12-30 Hz)
 - Gamma (30-100 Hz)
 - Omega (60-120 Hz)
 - Rho (250 Hz) hippocampal
 - Sigma Thalamocortical burst (600 Hz) [36].

The last three are hardly encountered in conventional EEG [119].

- Arrhythmic: EEG activity in which no stable rhythms are present.
- Dysrhythmic: Rhythms and/or patterns of EEG activity that characteristically appear in patient groups and rarely seen in healthy subjects.

The number of electrodes and their positions over the scalp determines a spatial structure: signal elements can be generalized, focal or lateralized, depending on in which channel (i.e. electrode) they are found.

2.6 BCI EEG Paradigms

BCI Paradigms are referred to noninvasive EEG-based BCI configurations that can be used to transmit volitional information. The popularity of EEG (71.2% of the BCI projects submitted to BCI Award 2016 were with EEG) [44] pushed the adoption of paradigms exclusively for noninvasive BCI. Their chronology can be found at the beginning of the Chapter. They can be roughly [21] described as:

1. Steady State Evoked Potentials: the basis for this paradigm is that when a subject attends certain stimulus, the dominant frequency component contained in the stimulus source can be found in the brain waves. When stimulus sources are light, this is called SSVEP and the signals are prominent in occipital regions. A similar process can be obtained with auditory stimulus, in which case they are called SSAEPs, or with somatosensory stimulation (i.e. tactile) and it is called SSSEP. By using different stimulus sources with different frequencies the one that is **selectively attended** by a subject can be inferred based on the main frequency component found on the EEG trace.
2. Bereitschaftspotentials, Readiness Potential or Movement-Related Potentials: these signals are slow cortical potential that can appear when a subject is just about to engage in a movement related activity. They are related to a general desynchronization prior to movement onset. They are used in BCI as triggering markers.
3. Motor Imagery ERD/ERS: the imagery, i.e. the mental visualization of movement without actually performing it, triggers a neurophysiological response which is very similar to the one obtained when the movement is physically performed. Frequencies on the α range of EEG are desynchronized prior to movement imagery, and synchronized afterwards. At the same time, β frequencies are resynchronized and increase in power after motor imagery. A subject can learn to think about moving a feet or moving a limb, and transfer a bit from this thinking patterns. This paradigm requires intensive training from subjects. This is further explained in Chapter 6.
4. P300: the positive deflection at 300 ms is activated by a cognitive experiment called the oddball paradigm and can be used to detect which symbol a subject is paying attention on a flickering matrix. By exploiting this information, a speller application can be implemented. This important signal is explained in details in Chapter 7.
5. Mental Tasks: mental tasks like rotation 3D objects in the head, or calculating arithmetic operations can be used to generate signals that can be detected and used to transfer a bit.
6. Slow Cortical Potentials: these are very slow shifts in the electrical activity found in the cortex, of a very low frequency. They can be modulated by **operand conditioning** protocols.

7. Error Potentials: when a person recognizes that an error was committed during a task, a recognizable signal called ErrP can be detected along the EEG trace, time-locked to the onset when the error information is fed back to the person. This very important potential is used in BCI applications to enhance the identification of false positives and to improve the overall interaction between the subject and the computer.

These paradigms have been exploited in the most popular BCI configurations, the Wadsworth BCI, the Graz BCI, the Berlin BCI and the Tübingen BCI. These platforms introduced pragmatic enhancements and solutions to use these paradigms to implement more practical devices [79] [103].

2.7 State of the Art of BCI Algorithms for EEG processing

According to general layout of a BCI system, Figure 2.1, specific algorithms or techniques are required for both the feature extraction and classification step. The most relevant features used nowadays in BCI are:

- Time points: the sequence of time series, often, concatenated in time or space.
- Band Power: frequency based features.
- Complexity: based on complexity measurements like entropy, or fractal.
- Statistical: Auto-regressive parameters or covariances matrix.

The most successfull used and verified classification methods for BCI [70] can be described as linear versions of machine learning tools. Particularly, Support Vector Machines SVM, Linear Discriminant Analysis LDA and its variant SWLDA. SWLDA is relevant for two reasons: the first is that the stepwise identification of features improves the selection criteria and also the spatial filter that this procedure encompass. Additionally, from a pragmatic perspective, this method is included in the popular BCI2000 [101] package and is the default option for the identification of event related potentials. Spatial filters have also being incorporated and have shown substantial improvements in classification accuracies: the canonical Common Spatial Patterns CSP for the identification of Motor Imagery as well as the xDAWN algorithm for P300 identification.

In recent years (circa 2018) classification accuracies in BCI have improved but the focus was not centered on any particular classification algorithm. Instead, current contributions

concentrate their efforts on how these algorithms are used [69]. Recent works can be described as:

- Ensemble classifiers: SVM ensembles [91] and variants of random forest [108]. Features are segmented and divided and the forest performs a classification step on aggregated parts, maximizes classification accuracies.
- Cross-paradigm BCI: the use of a reinforced signal with ErrP feedback or the use of SSVEP in combination with P300 detection [69].
- Adaptive classifiers: the parameters of the classifiers are adapted continuously and online adapting to the natural variation of the EEG signals [69].
- Transfer learning: transfer the calibration information obtained by users to new subjects. This aims to ease the issue of the intra-subject variability in BCI, and to reduce the set-up and calibration times of a BCI system.
- RGC Riemann Geometry Classifiers: the EEG stream is directly mapped onto a geometrical space equipped with a suitable Riemannian metric. Hence, further data manipulation is carried out following principles of Riemannian geometry which yields very good results in terms of accuracies.
- Tensor-based BCI [?]: the EEG data is viewed as a multidimensional matrix, a tensor. The BCI problem is considered as an optimization problem that can be solved with sparsity and nonnegativity constraints.
- Deep learning [114]: deep learning is a very successful technique driven by the increased computational power of current computer devices. Deep learning techniques have also been applied to BCI applications.

2.8 EEG Waveform Analysis

This section describes the procedures that are used to analyze EEG signals waveforms and the automatic procedures that were developed with this purpose.

2.8.1 EEG Waveform Characterization

The shape of the signal, the waveform, can be defined as the graphed line that represents the signal's amplitude plotted against time. It can also be called EEG biomarker, EEG

pattern, motifs, signal shape, signal form and a morphological signal [57].

The signal context is crucial for waveform characterization, both in a spatial and in a temporal domain [57]. Depending on the context, some specific waveform can be considered as noise while in other cases is precisely the element which has a cognitive functional implication.

A waveform can have a characteristic shape, a rising or falling phase, a pronounced plateau or it may be composed of ripples and wiggles. In order to describe them, they are characterized by its amplitude, the arch, whether they have (non)sinusoidal shape, by the presence of an oscillation or imitating a sawtooth (e.g. Motor Cortical Beta Oscillations). The characterization by their sharpness is also common, particularly in Epilepsy, and they can also be identified by their resemblance to spikes (e.g. Spike-wave discharge).

Other depictions may include, subjective definitions of sharper, arch comb or wicket shape, rectangular, containing a decay phase or voltage rise, peaks and troughs, short term voltage change around each extrema in the raw trace. Derived ratios and indexes can be used as well like peak and trough sharpness ratio, symmetry between rise and decay phase and slope ratio (steepness of the rise period to that of the adjacent decay period). For instance, wording like "Central trough is sharper and more negative than the adjacent troughs" are common in the literature.

Other regular characterizations which are based on shape features may include:

- Attenuation: Also called suppression or depression. Reduction of amplitude of EEG activity resulting from decreased voltage. When activity is attenuated by stimulation, it is said to have been "blocked" or to show "blocking".
- Hypersynchrony: Seen as an increase in voltage and regularity of rhythmic activity, or within the alpha, beta, or theta range. The term suggest an increase in the number of neural elements contributing to the rhythm and a synchronization of neurons with similar firing patterns [17].
- Paroxysmal: Activity that emerges from background with a rapid onset, reaching (usually) quite high voltage and ending with an abrupt return to lower voltage activity.
- Monomorphic: Distinct EEG activity appearing to be composed of one dominant activity.
- Polymorphic: Distinct EEG activity composed of multiple frequencies that combine to form a complex waveform.

- Transient. An isolated wave or pattern that is distinctly different from background activity.

The traditional clinical approach consists in analyzing the paper strip that is generated by the plot of the signal obtained from the device. Expert technician and physicians analyze visually the plots looking for specific patterns that may give a hint of the underlying cognitive process or pathology. Atlases and guidelines were created in order to help in the recognition of these complex patterns. Even Video-electroencephalography scalp recordings are routinely used as a diagnostic tools [39]. The clinical EEG research has also focused on temporal waveforms, and a whole branch of electrophenomenology has arisen around EEG *graphoelements* [103].

Sleep Research has been studied in this way by performing Polysomnographic recordings (PSG) [98], where the different sleep stages are evaluated by visually marking waveforms or graphoelements in long-running electroencephalographic recordings, looking for patterns based on standardized guidelines. Visual characterization includes the identification or classification of certain waveform components, or transient events, based on a subjective characterization (e.g. positive or negative peak polarity) or the location within the strip. It is regular to establish an amplitude difference between different waveforms from which a relation between them is established and a structured index are created (e.g. sleep K-Complex is well characterized based on rates between positive vs. negative amplitude) [115]. Other relevant EEG patterns for sleep stage scoring are alpha, theta, and delta waves, sleep spindles, polysplindles, vertex sharp waves (VSW), and sawtooth waves (REM Sleep).

Moreover, EEG data acquisition is a key procedure during the assessment of patients with focal Epilepsy for potential seizure surgery, where the source of the seizure activity must be reliably identified. The onset of the epileptic seizure is defined as the first electrical change seen in the EEG rhythm which can be visually identified from the context and it is verified against any clinical sign indicating seizure onset. The Interictal Epileptiform Discharges (IEDs) are visually identified from the paper strip, and they are also named according to their shape: spike, spike and wave or sharp-wave discharges[15].

2.8.2 EEG Waveform Analysis Algorithms

Shape or waveform analysis methods are considered as nonparametric methods. They explore signal's time-domain metrics or even derive more complex indexes or features from it [112].

One of the earliest approach to automatically process EEG data is the Peak Picking

method. Although of limited usability, peak picking has been used to determine latency of transient events in EEG [58, 133]. Straightforward in its implementation, it consists in selecting a simple component based on the expected location of its more prominent deflection [84]. Evoked Potentials (EPs) and Event Related Potentials (ERPs) are transient component that may arise as a brain response to an external visual, tactile or auditory stimulus. Particularly, EPs are regularly used to assess auditory response in infants. ERPs are characterized by their most prominent peaks, where the name of many of the EEG features evoke directly a peak within the component, e.g. P300 or P3a, P3b or N100. This leads to a natural procedure to classify them visually by selecting appropriate peaks and matching their positions and amplitudes in an orderly manner. The letter provides the polarity (Positive or Negative) and the numbering shows the time referencing the stimulus onset, or the ordinal position of each peak (first, second, etc). Finally, the trailing letter is added to describe different variants of components that initially were considered one.

A related method is used in [4] where the area under the curve of the EEG is summarized to derive a feature. This was even used in the seminal work of Farwell and Donchin on P300 [34, 126]. Additionally, a logarithmic graph of the peak-to-peak amplitude which is called amplitude integrated EEG (aEEG) [105] is used nowadays in Neonatal Intensive Care Units.

Other works on EEG explored the idea to extend human capacities analyzing EEG waveforms [63] where a feature from the amplitude and frequency of its signal and its derivative in time-domain is used. Moreover, other works explored the use of Mathematical Morphology [128], where the time-domain structure of contractions and dilations were studied. Finally the proposals of Burch, Fujimori, Uchida and the Period Amplitude Analysis (PAA) [116] algorithm are few of the earliest proposals where the idea of capturing the shape of the signal were established.

Pursuit algorithms refer, in their many variants, as blind source separation [122] techniques that assume the EEG signal as a linear combination of different sparse sources extracted from a template's dictionary. Matching Pursuit *MP* [75], the most representative of this algorithms, is a greedy variant that decomposes a signal into a linear combination of waveforms, called atoms, that are well localized in time and frequency [20]. This method has been used to identify epileptogenetic patterns from EEG traces [120].

Another method that explores the waveform is Bond and Pompe Permutation Entropy [8]. This has been extensively used in EEG processing, with applications on Anesthesia, Sleep Stage evaluation and increasingly for Epilepsy pre-ictal detection . This method generates

a code based on the orderly arrangement of sequential samples, and then derives a metric which is based on the number of times each sequence is found on the signal. This numeric value can be calculated as information entropy [80].

A related method is Slope Horizontal Chain Code and Slope Chain Code (SCC) [4]. This algorithm proceeds by generating a coding scheme from a sequence of sample points. This encoding is based on the angle between the horizontal line on a 2D-plane and any segment produced by two consecutive sample points, regarding them as coordinates on that plane. Similar works were provided in Local Binary Patterns (1-D LNBP, 1D-LBP and LBP)[56] algorithms. Finally, the Merging of Increasing and Decreasing Sequences (MIDS) [134] do not generate a feature but it provides a filter or not heterogeneous downsampling scheme which is based on the waveform structure.

The method presented in this Thesis generates a feature that can be classified. Likewise, all these methods provide a feature that can be used as a template, whereas all of them are based on metrics that can be extracted from the shape of the signal. The notation $f = \{f_i\}_1^n$ or $f = \{f_i\}_{i \in J}$ will be used to describe the concatenation of scalar values to form a multidimensional feature vector $f = \{f_1, f_2, \dots, f_n\}$. These features can be used to create dictionaries or template databases. These templates provide the basis for the pattern matching algorithm and offline classification.

Details for the most relevant methods are provided in the following sections. The notation $x(n)$ is used to represent the c-row EEG matrix $x(n, c)$ for a given fixed channel c .

Matching Pursuit - MP 1 and MP 2

Pursuit algorithms refer, in their many variants, as blind source separation [122] techniques that assume the EEG signal as a linear combination of different sparse sources extracted from a template's dictionaries. Matching Pursuit *MP* [75], the most representative of these algorithms, is a greedy variant that decomposes a signal into a linear combination of waveforms, called atoms, that are well localized in time and frequency [20]. Given a signal, this optimization technique, tries to find the indexes of m atoms and their weights (contributions) that minimize,

$$\varepsilon = \left\| x(n) - \sum_{i=1}^m w_i g_i(n) \right\| \quad (2.4)$$

which is the error between the signal and its approximation constructed by the weighted w_i

atoms g_i , and calculating the euclidean norm $\|\cdot\|_2$. The algorithm goes by first setting the approximating signal \tilde{x}_0 as the original signal itself,

$$\tilde{x}_0(n) = x(n) \quad (2.5)$$

and setting the iterative counter s as 1. Hence, it searches recurrently the best template out of the dictionary that matches current approximation.

$$g_s = \arg \max_{g_i} \left| \sum_{n=1}^N \tilde{x}_{s-1}(n) g_i(n) \right| \quad (2.6)$$

where g_i are all the available scaled, translated and modulated atoms from the dictionary. The operation $|\cdot|$ corresponds to the absolute value of the inner product. This step determines the atom selection process, and their contribution is calculated based on

$$w_s = \frac{\sum_{n=1}^N \tilde{x}_{s-1}(n) g_s(n)}{\|g_s\|^2} \quad (2.7)$$

with s representing the index of the selected atom g_s and $\|\cdot\|$ its euclidean norm. Finally the contribution of each atom is subtracted from the next approximation [25, 100, 75]

$$\tilde{x}_s(n) = \tilde{x}_{s-1}(n) - w_s g_s(n) \quad (2.8)$$

The stopping criteria can be established based on a limiting threshold on Equation 2.4 or based on a predetermined number of steps and selected atoms. Two variants of this algorithm are evaluated. In *MP 1* the dictionary is constructed with the normalized templates directly extracted from the real signal segments which is a straightforward implementation of the pattern matching technique. In *MP 2* the coefficients of Daubechies least-asymmetric wavelet with 2 vanishing moments atoms are used to construct the dictionary [120]. For the first version, the matching against the template is evaluated according to Equation 2.4 directly, whereas for the latter each feature is crafted by decomposing the signal in its coefficients and building, an eventually sparse, vector with them:

$$f = \left\{ w_i \right\}_1^m \quad (2.9)$$

where D is the size of the dictionary.

Permutation Entropy - PE

Bond and Pompe Permutation Entropy has been extensively used in EEG processing, with applications on Anesthesia, Sleep Stage evaluation and increasingly for Epilepsy pre-ictal detection [8]. This method generates a code based on the orderly arrangement of sequential samples, and then derives a metric which is based on the number of times each sequence is found along the signal. This numeric value can be calculated as information entropy [80]. Let's consider a signal on a window of length W represented by the sample points

$$(x_1, x_2, \dots, x_W) \quad (2.10)$$

and resampled by τ intervals, starting from the sampling point n , doing

$$(x_n, x_{n+\tau}, x_{n+2\tau}, \dots, x_{n+(m-1)\tau}). \quad (2.11)$$

This sequence is of order m , which is the number of sample points used to derive the ordinal element called π . There are $m!$ ways in which this sequence can be orderly arranged, according to the position that each sample point holds within the sequence in a strict order relationship. For example if $m = 3$, and the first sample point is the bigger, the second is the smaller and the third one is in the middle, the ordinal element π corresponds to $(3, 1, 2)$. Thus, along the signal window there can be at most k different ordinal (and overlapping) elements π_s

$$(\pi_1, \pi_2, \dots, \pi_k) \quad (2.12)$$

with $k = W - (m-1)\tau$. The probability density function pdf for all the available permutations of order m should be $\mathbf{p} = (p_1, p_2, \dots, p_{m!})$ with $\sum_{i=1}^{m!} p_i = 1$.

Hence, the time series window is mapped to a new set of k ordinal elements, and the pdf can be calculated by the empirical permutation entropy,

$$p_i = \frac{1}{k} \sum_{s=1}^k [\pi_s = \pi_i] \quad (2.13)$$

with $1 \leq i \leq m!$. The Iverson Bracket $[.]$ resolves to 1 when their logical proposition argument is true, 0 otherwise. Therefore, for each i only those ordinal elements π_s that were effectively found along the signal are counted to estimate p_i , and zero elsewhere. The

empirical permutation entropy can be calculated from the histogram as,

$$H(\mathbf{p}) = \sum_{i=1}^{m!} p_i \log \frac{1}{p_i}. \quad (2.14)$$

The implemented code was derived from [117], and the model description from [9]. This procedure produces a scalar number for the given signal window of size W . To derive a feature, a sliding window procedure must be implemented to cover an entire segment of length N . Thus, the length of the feature is $N - (W + \tau(m - 1))$.

$$f = \left\{ H(\mathbf{p})_u \right\}_{W+\tau m}^N. \quad (2.15)$$

with u varying on a sample by sample basis along the signal, starting from the specified index.

Slope Horizontal Chain Code - SHCC

This algorithm [4] proceeds by generating a coding scheme from a sequence of sample points. This encoding is based on the angle between the horizontal line on a 2D-plane and any segment produced by two consecutive sample points, regarding them as coordinates on that plane.

A signal of length N , can be represented by a list of ordered-pairs e ,

$$e = [(x, y)_1, (x, y)_2, \dots, (x, y)_N] \quad (2.16)$$

and it can be divided into G different blocks. These blocks are obtained by resampling the original signal from the index

$$G = \lfloor n + (m\Delta) + 0.5 \rfloor \quad (2.17)$$

with n being the original sampling index on $1 \leq n \leq N$ and $\lfloor \cdot \rfloor$ being the floor operation, i.e. rounding of the number argument to the closest smaller integer number. On the other hand, Δ can be obtained by

$$\Delta = \left\lceil \frac{N}{G+1} \right\rceil \quad (2.18)$$

with $G < N$ and using instead $\lceil \cdot \rceil$ as the ceil operation, the rounding to the closest bigger integer number. Lastly, the value m can be derived from

$$m = \text{sign}\left(\frac{N-1}{\Delta}\right) \left\lceil \left| \frac{N-1}{\Delta} \right| \right\rceil. \quad (2.19)$$

This resampling produces a new sequence of values,

$$e' = [(x', y')_1, \dots, (x', y')_s, \dots, (x', y')_G]. \quad (2.20)$$

The next step is the normalization of each ordered-pair as vectors $\mathbf{x}' = (x'_1, \dots, x'_G)$ and $\mathbf{y}' = (y'_1, \dots, y'_G)$ according to

$$\hat{\mathbf{x}} = \frac{\mathbf{x}' - \min(\mathbf{x}')\mathbf{1}}{\max(\mathbf{x}') - \min(\mathbf{x}')} \quad (2.21)$$

$$\hat{\mathbf{y}} = \frac{\mathbf{y}' - \min(\mathbf{y}')\mathbf{1}}{\max(\mathbf{y}') - \min(\mathbf{y}')} \quad (2.22)$$

with $\mathbf{1}$ being the vector of length G with all their components equal to 1. Hence, the scalar components \hat{x}_s of $\hat{\mathbf{x}}$, and \hat{y}_s of $\hat{\mathbf{y}}$, with s varying between 1 and G are effectively normalized to $\hat{x}_s, \hat{y}_s \in [0, 1]$.

Finally, the feature is constructed by calculating the point-to-point slope against the horizontal plane,

$$f = \left\{ \frac{\hat{y}_s - \hat{y}_{s-1}}{\hat{x}_s - \hat{x}_{s-1}} \right\}_2^G \quad (2.23)$$

Chapter 3

From signals to images

A regular practice in image processing is to analyze images as bidimensional signals. In this Thesis the opposite is done and signals are studied by how they are represented on images. This chapter describes the procedure to plot an image from the digital EEG signal. This image is used to extract a feature which represents the waveform, the structure of the signal on a plot. By analyzing this feature, we hypothesize that the underlying cognitive process can be detected and it can be used to implement a brain-computer communication device.

3.1 Electroencephalographic Plotting

The plotting of the EEG is intrinsically mixed with the nuisances of the electroencephalography itself. Plotting proceed by using a chart recorded with a single pen [59]. Voltages are represented on a vertical axis while time is represented on the horizontal axis, in a Cartesian arrangement. The most salient characteristics of a plot are:

1. Sensitivity: also termed gain due the amplification procedure. Its units are $\frac{mV}{mm}$. In the digital form, it is $\frac{\mu V}{pixel}$.
2. Epoch/Paper speed: the time span that is represented in a single screen. For paper strips it is usually $10s$. In its digital counterpart is $\frac{w}{pixel}$ with w being the length in milliseconds of the signal segment.

Additionally, on analog plotting montage is essential, though digital plotting allows flexible montage configuration from software. Montage can be monopolar or bipolar. On monopolar montages each electrode obtains the potential difference against a common reference. With bipolar montages, electrodes are paired, eventually in chained configurations, and the potential difference is obtained between each pair of electrodes [15].

Neuroimaging

With the advent of digital computers and the digital revolution, plotting has become imaging. Neuroimaging [37] means mapping activity or structure to neuroanatomical regions.

There are currently three categories of neuroimaging: *structural* which includes CT (Computed Tomography), MRI (Magnetic Resonance Imaging) and DTI (Diffusion Tensor Imaging), *functional*, which encompass EEG, MEG (Magnetoencephalography), fMRI (functional MRI) PET (Positron Emission Tomography), SPECT (Single Positron Emission Computed Tomography), NIRS (Near-Infrared Spectroscopy) and *chemical* which involves special dyes which are sensible to neuron firing.

3.2 Signal to Image transformation

The EEG signal is represented by

$$x(n, c) \quad (3.1)$$

where n are sample points digitalized at sampling frequency F_s . This is a multichannel signal, for c varying between $1 \leq c \leq C$. Each one of this channels is assigned a name according to the 10-20 international system (see Figure 2.5), and there are C available channels. The sample index n varies between 1 and N . The span of the signal λ is the length in milliseconds of the waveform under study.

The length of segment N in sample units, the sampling frequency F_s in Hz and the segment length w in seconds are related by

$$N = \lfloor F_s w \rfloor. \quad (3.2)$$

To extract features from an image, it should be first constructed. The straightforward way to do it, replicating the analog or digital EEG plotting, is to draw a line on a contrast background. This line represents the voltage amplitude of a channel c in relation to a reference zero-level $z(c)$, with a positive deflection going upwards and downwards for negative deflection. Figure 3.1 shows an example of an EEG signal segment plot. This image is a black-and-white binary image. The color selection is arbitrary (white for the line, black for the background), but it has some implications in terms of the feature extraction procedure that will be described in Section 4.2.



Figure 3.1: Sample EEG signal plot. For this sample image, the length of the signal is 1s, which is 250 sample points. The height of the image is 73 pixels, which is the peak-to-peak amplitude of the signal segment. Channel Oz of baseline EEG activity is being shown.

This chapter mostly deal with the coordinates transformation that need to be enforced while converting the signal into a plot. Figure 3.2 shows the image coordinate system where the (z_1, z_2) represents the horizontal and vertical location, and the $(0, 0)$ value is the upper-left position of the image.

Let c_i be a given constant channel, and n_i be a constant sample point in digital time, the values of $I(z_1, z_2)$ are obtained for n varying between 1 and N or c varying between 1 and C . In order to convert the EEG original signal $x(n, c)$ into the image $I(z_1, z_2)$, the following six alternatives can be used:

1. Channel-by-channel binary image

The standard plotting, on a black-and-white image with lines representing voltage amplitude.

$$I^{(c_i)}(z_1, z_2) = \begin{cases} 255 & \text{if } z_1 = n; z_2 = x(n, c_i) + z(c_i) \\ 0 & \text{otherwise.} \end{cases} \quad (3.3)$$

The signal plotted by this procedure is inverted on the image. So it is necessary to multiply $x(n, c_i)$ by (-1) to invert it before plotting.

2. Channel-by-channel greyscale image

The voltage amplitudes are represented in greyscale, that could range between 0 and 255. The function $\phi(\cdot)$ is a bounded linear mapping between $[0, 255]$

$$I^{(c_i)}(z_1, z_2) = \begin{cases} \phi(x(n, c_i)) & \text{if } z_1 = n; z_2 = z(c_i) \\ 0 & \text{otherwise.} \end{cases} \quad (3.4)$$

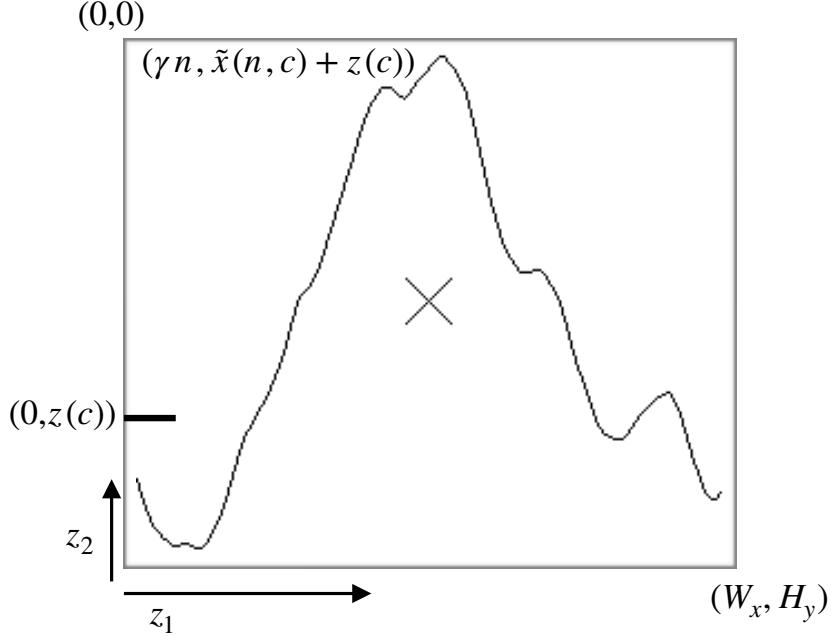


Figure 3.2: The image coordinate system and the mapping from the signal segment. The origin is the $(0, 0)$ position at the upper-left corner of the image. Time is represented as sample points on the horizontal axis, and the amplitude in μV is shown on the vertical axis. Image height H_y and width W_x are obtained based on signal parameters. The signal's zero-level $z(c)$ is the vertical location where the signal zero value is located. The plot of the signal is obtained by first setting the sample points on the predetermined image locations according to equation 3.15 and then applying a discrete interpolation algorithm to connect them with straight lines.

3. Multichannel full greyscale image

The image is greyscale. Voltage amplitudes are represented by the pixel content and each channel is represented on the vertical axis. The height of the signal is equal to the number of channels. This is used in Neuroimaging [37] plots of ERP events.

$$I(z_1, z_2) = \begin{cases} \phi(x(n, c)) & \text{if } z_1 = n; z_2 = c \end{cases} . \quad (3.5)$$

4. Multichannel stationary binary image

The horizontal axis of the image is not time, but it is the number of the channel instead. In this representation different contributions from different channels can be

explored at the same time, but time dynamics is lost.

$$I^{(n_i)}(z_1, z_2) = \begin{cases} 255 & \text{if } z_1 = c; z_2 = x(n_i, c) + z(n_i) \\ 0 & \text{otherwise.} \end{cases} \quad (3.6)$$

In this case, the vertical position where the signal's zero value is located, $z(n_i)$, is calculated across the different channels and fixed for a discrete time point n_i .

5. Multichannel stationary greyscale image

This is a variant of the previous one, where the horizontal axis also represent the channel, and the zero-level is also calculated for a fixed sample point. In this form, the intensity of the contribution of each channel is represented by the greyscale pixel value. Combined with head models and forward projection solutions this is the methodology used to represent scalp heatmaps [41].

$$I^{(n_i)}(z_1, z_2) = \begin{cases} \phi(x(n_i, c)) & \text{if } z_1 = c; z_2 = z(n_i) \\ 0 & \text{otherwise.} \end{cases} \quad (3.7)$$

6. Channel by channel full greyscale image

This is similar to a raster plot [25] but the greyscale image representing voltages in pixel intensities can be replicated or epoched H times, which at the same time is the height of the image. The selection of this value depends on the number of epochs or repetitions to show. In this case, the mapping is

$$I^{(c_i)}(z_1, z_2) = \begin{cases} \phi(x(n, c_i)) & \text{if } z_1 = n; z_2 = H \end{cases}. \quad (3.8)$$

To analyze effectively an EEG signal, many signal segments must be produced. Hence, the transformation from signal to image is continuously repeated, and many images need to be crafted for the EEG signal under analysis. How to determine the size of all the images so that they can be effectively compared between them ? The first option is to regularize the signal and fit in an equal size for every image. An alternative choice is to autoscale every image according to the zero-level position. Figure 3.3 shows two sample artificial impulse signals and their alternative transformation into images.

3.3 Standardized plotting

The *z-score* is a widely used method to regularize a signal [134].

This standardization procedure is defined for $1 \leq n \leq N$ and $1 \leq c \leq C$ by doing

$$\tilde{x}(n, c) = \frac{x(n, c) - \bar{x}(c)}{\hat{\sigma}(c)} \quad (3.9)$$

where $x(n, c)$ is the multichannel EEG signal segment for the sample point n and for channel c . The values

$$\bar{x}(c) = \frac{1}{N} \sum_{n=1}^N x(n, c)$$

and

$$\hat{\sigma}(c) = \left\{ \frac{1}{N-1} \sum_{n=1}^N [x(n, c) - \bar{x}(c)]^2 \right\}^{\frac{1}{2}}$$

are the mean and estimated standard deviation of $x(n, c), 1 \leq n \leq N$, for each channel c .

Figure 3.3(a) shows an impulse signal and their standardized representation.

3.4 Autoscaled plotting

This plotting scheme allows each image to adapt to the underlying signal. The height is set at twice the value of the zero-level, and the signal mean is subtracted from the original signal, producing a vertical displacement, according to the following Equation,


$$\tilde{x}(n, c) = x(n, c) - \bar{x}(c) \quad (3.10)$$

Figure 3.3(b) shows the results of the plotting for an impulse signal. Equation 3.10 has the advantage that any low frequency component, particularly the EEG DC drift is eliminated, due to the fact that plot of the signal is always centered on each image.


3.5 Zero-Level

The zero-level $z(c)$ is the image vertical position where the signal's zero value has to be situated in order to fit the entire signal within the image for each channel c :

$$z(c) = \left\lfloor \frac{\max_n \tilde{x}(n, c) - \min_n \tilde{x}(n, c)}{2} \right\rfloor - \left\lfloor \frac{\max_n \tilde{x}(n, c) + \min_n \tilde{x}(n, c)}{2} \right\rfloor \quad (3.11)$$

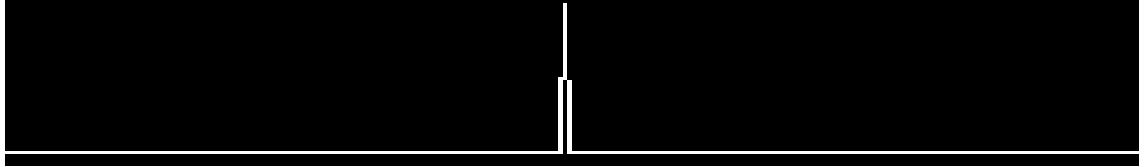

(a) An artificial signal pulse and their plotting representation. The signal is standardized and the height of the image is determined according to the peak-to-peak amplitude, which is the same for every image and equal to γ .

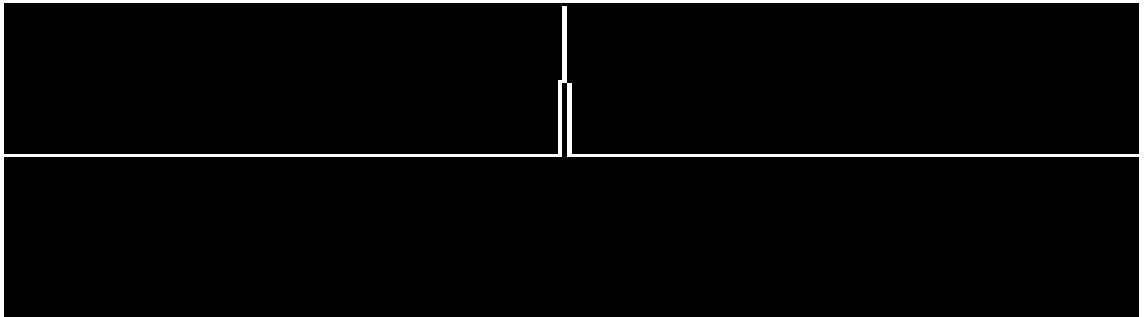

(b) The plotted image height is twice the zero-level. In this case, the height is also determined according to the peak-to-peak amplitude of each segment, proportional to γ , and not constant. Transformed images do not have the same height, but the zero-level is always located at half the height of the image.

Figure 3.3: Signal plotting schemes.

where the minimization and maximization are carried out for n varying between $1 \leq n \leq N$, and $\lfloor \cdot \rfloor$ denote the rounding to the smaller nearest integer of the number. This value represents the vertical location on the image where the signal goes to zero.

3.6 Image Size

Height

The height of the image is calculated according to the peak-to-peak amplitude of the signal segment,

$$H_y = \max |\gamma \tilde{x}(n, c)| - \min |\gamma \tilde{x}(n, c)| \quad (3.12)$$

while for the autoscalable version, it is just twice the value of the zero-level.

$$H_y = 2 z(c) \quad (3.13)$$

Width

The width, on the other hand, is obtained based on the length of the signal segment, scaled by the γ_t time factor,

$$W_x = \gamma_t N \quad (3.14)$$

3.7 EEG Signal Plot

Once the regularization procedure, and the size and the scale of the image are defined, a binary image $\mathcal{I}^{(c)}$ can be constructed from a variant of the method specified in 3.3 according to


$$\mathcal{I}^{(c)}(z_1, z_2) = \begin{cases} 255 & \text{if } z_1 = \gamma_t n \text{ and } z_2 = \lfloor \gamma \tilde{x}(n, c) \rceil + z(c) \\ 0 & \text{otherwise} \end{cases} \quad (3.15)$$

where $1 \leq c \leq C$ and $1 \leq n \leq N$. The amplitude scale factor γ and time scale factor γ_t are used to determine the image size and at the same time the image resolution. This scheme produces a black-and-white plot of the signal with 255 being white and 0 black. There is one image per channel per segment.


3.8 Interpolation

Equation 3.15 produces a set of isolated pixels over the image $\mathcal{I}^{(c)}$. To produce the plot $I^{(c)}$, the Bresenham [14, 93] algorithm is used to digitally interpolate straight lines between each pair of consecutive pixels. Figure 3.4(a) shows an image plot constructed by only using the sample points, while (b) shows the digital interpolation produced by the Bresenham algorithm.


On Figure 3.4(c) the same signal can be observed produced when the time scaling factor γ_t is increased to 4. It can be noticed that there are very sharp edges around sample pixels. This can lead to a quantization of histogram gradients that will be discussed in the next Chapter. To reduce this sharpness of the signal on the plot, an alternative procedure is to use

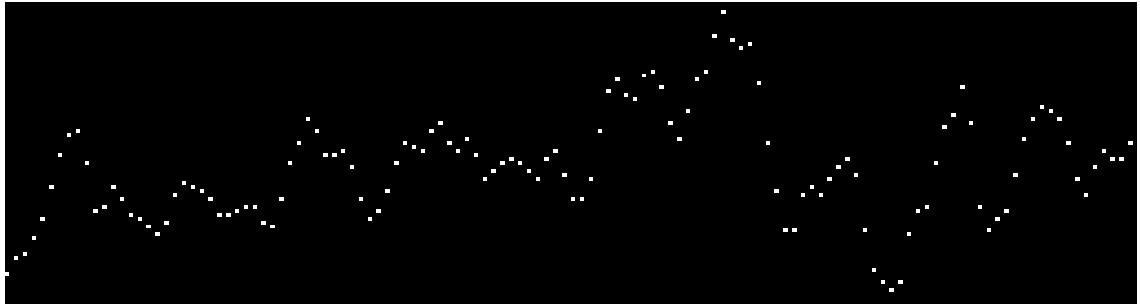


(a) Sample points are located on the image according to Equation 3.15.

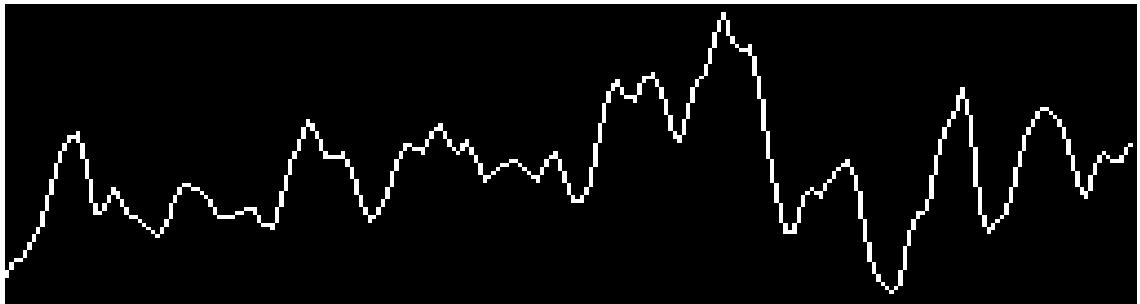

(b) Sample points are linearly interpolated in a discrete procedure using the Bresenham algorithm.

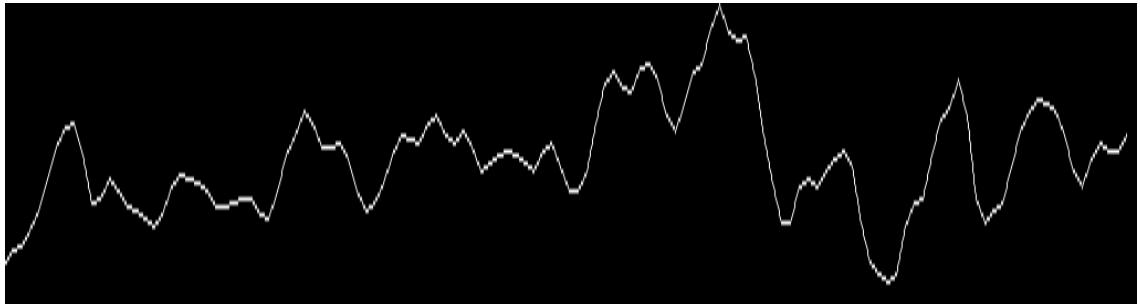

(c) The digital signal is scaled 4 times ($\gamma_t = 4$) and the generated sample points are interpolated using the Bresenham algorithm.

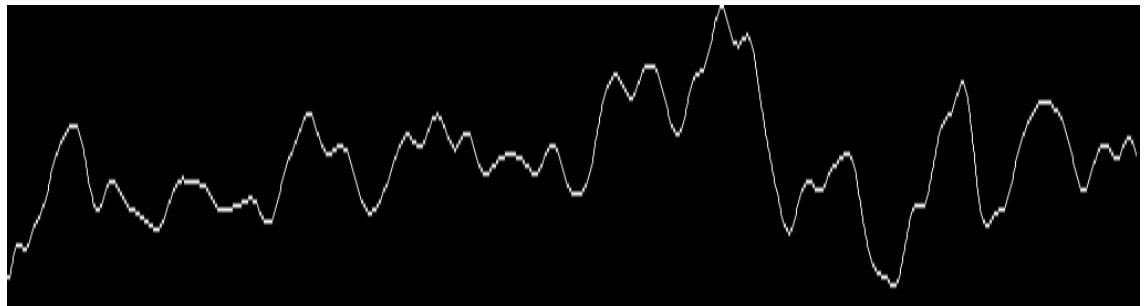

(d) The digital signal is upsampled 4 times and the generated sample points are interpolated using the Bresenham algorithm.

Figure 3.4: Generated images based on different interpolation schemes.

a smoothing interpolation of the signal $\tilde{x}(n, c)$ using splines. Instead of just situating time point values at a bigger step according to Equation 3.15, intermediate values are computed according to a linear, quadratic or cubic interpolation, hence smoothing the curve around each point. The result of this interpolation can be seen on Figure 3.4(d), where the edges around each sample point are more rounded. This procedure is similar to what the Matlab's **resample** function does which also includes an antialiasing FIR lowpass filter.

Special care must be taken by the presence of artifacts around the signal endpoints, at the edges of the image. Those regions are excluded from further analysis.

3.9 Resolution and Precision

The resolution [25] of the image transformation can be determined based on the characteristics of the digital signal and the parameter selection.

On the horizontal axis of the image, one pixel is equivalent \equiv to

$$1P_x \equiv \frac{1}{F_s \gamma_t} [\text{s}] \quad (3.16)$$

where F_s is the sampling frequency in Hertz, and γ_t is the time scale factor. This gives a value in seconds. For example, for Figure 3.1 where the length is 0.65s , the sampling frequency is 200Hz , and $\gamma_t = 1$, which gives a resolution of $1P_x \equiv 0.0077\text{s}$.

Consistently, on the vertical axis, one pixel is analogous to

$$1P_y \equiv \frac{1}{\gamma} [\mu\text{V}] \quad (3.17)$$

where γ is the amplitude scale factor. As EEG time-series are digitalized in μV , this is the unit of choice. In Figure 3.1, 1 vertical pixel represents exactly $1\mu\text{V}$.

Regarding the *Precision*, discrete EEG time-series are floating-point numbers and the image is constructed based on discrete and integer pixels. Image's pixel values (z_1, z_2) are obtained according to Equation 3.15. Thus, on the horizontal axis, z_1 , no discretization is needed because time is already digitalized in sample units. Hence, there is no loss of precision in time from the one generated by the digital device.

$$z_1 = \gamma_t n. \quad (3.18)$$

On the other hand, on the vertical axis, pixels are discretized according to

$$z_2 = \lfloor \gamma \tilde{x}(n, c) \rceil \quad (3.19)$$

where γ is the amplitude scale factor parameter, which also affects the height of the image in Equation 3.12. A rounding operation $\lfloor \cdot \rceil$ is applied to obtain an integer representation. Hence, precision is lost on the voltage amplitude. Additionally, the dynamic range of the digital capturing device is reduced to what is actually needed for each segment. Table 3.1 show some reference values.

Table 3.1: Reference Values for Precision and Resolution

γ	$1P_x$	Decimal Precision	γ_t	$1P_y$
1	$1\mu V$	NN	1	$\frac{1}{F_s} s$
2	$\frac{1}{2}\mu V$	$NN \pm 0.5$	2	$\frac{1}{2} \frac{1}{F_s} s$
3	$\frac{1}{3}\mu V$	$NN \pm 0.3$	3	$\frac{1}{3} \frac{1}{F_s} s$
10	$\frac{1}{10}\mu V$	$NN.N$	10	$\frac{1}{10} \frac{1}{F_s} s$
100	$\frac{1}{100}\mu V$	$NN.NN$	100	$\frac{1}{100} \frac{1}{F_s} s$

Chapter 4

The Histogram of Gradient Orientations of Signal Plots

This Chapter introduces the EEG feature extraction procedure based on the Histogram of Gradient Orientations. This method is grounded on an extension and modification of the SIFT [72] Descriptor which is used in Computer Vision to extract and map local regions of an image. At the same time, this Chapter brings to completion the previous one, describing how to mine the information from the Plot and build a feature out of it.

4.1 Introduction

The work of Edelman, Intrator and Poggio [33] on how the visual cortex sense features was the inspiration to the development of an algorithm to identify and decode salient local information from image regions. The Scale Invariant Feature Transform (SIFT) method is composed of two parts, the SIFT Detector and the SIFT Descriptor. The first is the procedure to identify relevant areas of an image. The second is the procedure to describe and characterize a region of an image using the Histogram of Gradient Orientations¹. The SIFT algorithm is biomimetically inspired in how the visual cortex detects shapes by analyzing orientations [33]. The patch description is also based on the Theory of Receptive Fields and other related ideas [67].

¹It should not to be confused with HOG [29], the Histogram Of Gradients which is another method from Computer Vision based on similar ideas. Actually, the descriptor part of the SIFT Method has no specific name, but as it is based on building a histogram of gradient orientations, that is the reason why it is described here in that way.

4.2 Feature Extraction: Histogram of Gradient Orientations

The basic procedure is composed of,

1. Keypoints **kp** are located on an image of a signal plot.
2. A region of an image, a patch, is located using keypoints as centers. Each patch has a horizontal S_t and vertical scale S_v , which determines the size in pixels \mathbf{S}_x and \mathbf{S}_y , along the horizontal and vertical axis respectively.
3. Form each patch, a descriptor **d** is derived which is used as a representation of the graphical information contained within the patch.

On the image generated by the procedure detailed in previous Chapter, a keypoint **kp** is placed on a pixel (x_{kp}, y_{kp}) over the image plot and a window around the keypoint is considered. A local image patch of size $\mathbf{S}_x \times \mathbf{S}_y$ pixels is constructed by dividing the window in 16 blocks. It is arranged in a 4×4 grid and the pixel **kp** is the patch center. Figure 4.1(a) shows a plot of a signal, a keypoint in red at the center and the surrounding patch.

A local representation of the signal shape within the patch can be described by obtaining the gradient orientations on each of the 16 blocks and creating a histogram of gradients. In order to calculate the histogram, the interval $[0 - 360]$ of possible angles is divided in 8 bins, each one at 45 degrees.

Hence, for each spacial bin $i, j = \{0, 1, 2, 3\}$, corresponding to the indexes of each block $B_{i,j}$, the orientations are accumulated in a 3-dimensional histogram h through the following equation:

$$h(\theta, i, j) = \sum_{\mathbf{p}} \omega_{\text{ang}}(\angle J(\mathbf{p}) - \theta) \omega_{ij}(\mathbf{p} - \mathbf{kp}) |J(\mathbf{p})| \quad (4.1)$$

where \mathbf{p} is a pixel from within the patch, θ is the angle bin with $\theta \in \{0, 45, 90, 135, 180, 225, 270, 315\}$, $|J(\mathbf{p})|$ is the norm of the gradient vector in the pixel \mathbf{p} and it is computed using finite differences and $\angle J(\mathbf{p})$ is the angle of the gradient vector. The scalar $\omega_{\text{ang}}(\cdot)$ and vector $\omega_{ij}(\cdot)$ functions are linear interpolations used by [72] and [121] to provide a weighting contribution to eight adjacent bins. They are calculated as

$$\omega_{ij}(\mathbf{v}) = \omega\left(\frac{v_x - x_i}{3 \sqrt{2} S_t}\right) \omega\left(\frac{v_y - y_i}{3 \sqrt{2} S_v}\right) \quad (4.2)$$

$$\omega_{\text{ang}}(\alpha) = \sum_{r=-1}^1 \omega\left(\frac{8\alpha}{2\pi} + 8r\right) \quad (4.3)$$

where x_i and y_i are the spatial bin centers located in $x_i, y_i = \{-\frac{3}{2}, -\frac{1}{2}, \frac{1}{2}, \frac{3}{2}\}$. The function parameter $\mathbf{v} = (v_x, v_y)$ is a vector variable and α a scalar variable. On the other hand, r is an integer that can vary freely between $[-1, 1]$ and allows the argument α to be unconstrained in terms of its values in radians. The interpolating function $\omega(\cdot)$ is defined as:

$$\omega(z) = \max(0, |z| - 1). \quad (4.4)$$

These binning functions conform a trilinear interpolation that has a combined effect of sharing the contribution of each oriented gradient between their eight adjacent bins in a tridimensional cube in the histogram space, and zero everywhere else.

Lastly, the fixed value of 3 on Equation 4.2 is a magnification factor, a fixed parameter. The multiplication by $\sqrt{2}$ on the same equation is related to the unit length of the patch Δ_s which is described in the section 4.4. As the patch has 16 blocks and 8 bin angles are considered, a feature **d** called *descriptor* of 128 dimension is obtained. This technique is a modification of Lowe's SIFT Descriptor method.

Figure 4.1 shows an example of a patch and a scheme of the histogram computation. In (A) a plot of the signal and the patch centered around the keypoint is shown. In (B) the possible orientations on each patch are illustrated. Only the upper-left four blocks are visible. The first eight orientations of the first block, are labeled from 1 to 8 clockwise. The orientations of the second block $B_{1,2}$ are labeled from 9 to 16. This labeling continues left-to-right, up-down until the eight orientations for all the sixteen blocks are assigned. They form the corresponding **kp**-descriptor of 128 coordinates. Finally, in (C) an enlarged image plot is shown where the oriented gradient vector for each pixel can be seen.

4.3 Keypoint Location

The keypoint **kp** location must be accurately specified in order to establish the region from the signal where the waveform is located.

For the horizontal position, the localization of the keypoint is based on a priori information, based on the characteristics of the event under study. For instance, ERPs have a specific timing that can be explored to elucidate in which position the expected signal pattern will be generated.

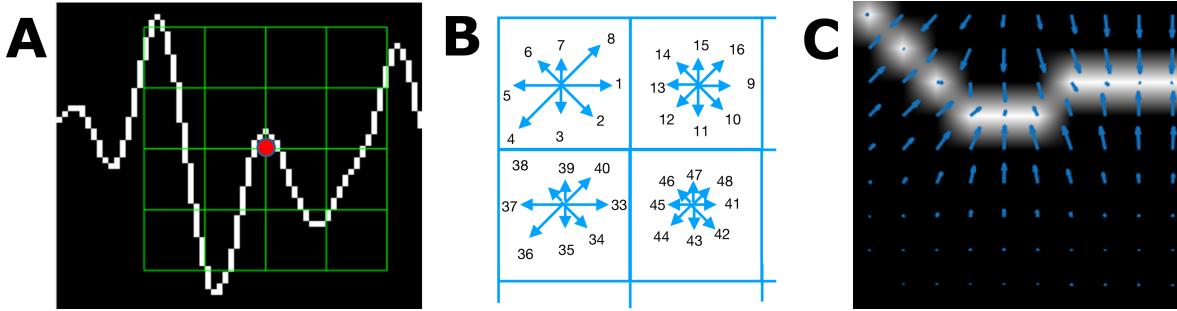


Figure 4.1: (A) Example of a plot of the signal, a keypoint and the corresponding patch. (B) A scheme of the orientation's histogram computation. Only the upper-left four blocks are visible. The first eight orientations of the first block, are labeled from 1 to 8 clockwise. The orientation of the second block $B_{1,2}$ is labeled from 9 to 16. This labeling continues left-to-right, up-down until the eight orientations for all the sixteen blocks are assigned. They form the corresponding descriptor of 128 coordinates. The length of each arrow represent the value of the histogram on each direction for each block. (C) Vector field of oriented gradients. Each pixel is assigned an orientation and magnitude calculated using finite differences.

Additionally, there can be more than just one keypoint and patch located over the signal plot. This is particular important for oscillatory processes where many waveforms are contained within the same signal segment. This needs to be addressed by defining a keypoint density parameter **kpa**.


Regarding the Vertical Location, there are two options. The first one is along the signal, exactly on the sample points calculated by the Equation 3.15. The second is on a fixed position over the zero-level as described by 3.11. Figure 4.2(a) show the former while on (b) the latter can be spotted.

4.4 Patch Geometry


The Horizontal Patch Scale S_t determines the size of the patch on the image horizontal axis, and it is related to the span λ of the waveform to analyze according to

$$S_t = \frac{\lambda}{\Delta_s} \frac{F_s \gamma_t}{\Delta_s} \quad (4.5)$$

where F_s is the sample frequency, γ_t is the time scale factor and Δ_s is the unit length of the patch which determines the pixel conversion factor. This value depends on the actual implementation of the Histogram of Gradient Orientations of the SIFT method. In this case, its value is $\Delta_s = \sqrt{2} 3 5$, where 3 is the fixed magnification factor.

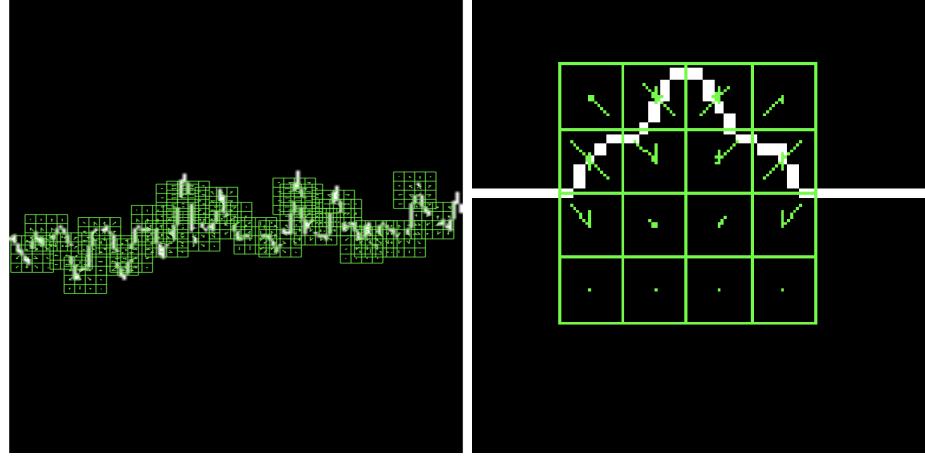

(a) Fixed size patches are located all along the EEG signal trace at a given keypoint density $\mathbf{kp_d}$.
(b) A patch is used to map an artificial signal using an autoscale plotting scheme, and mapping the entire waveform within the patch. The keypoint is located on the zero-level $z(c)$ value.

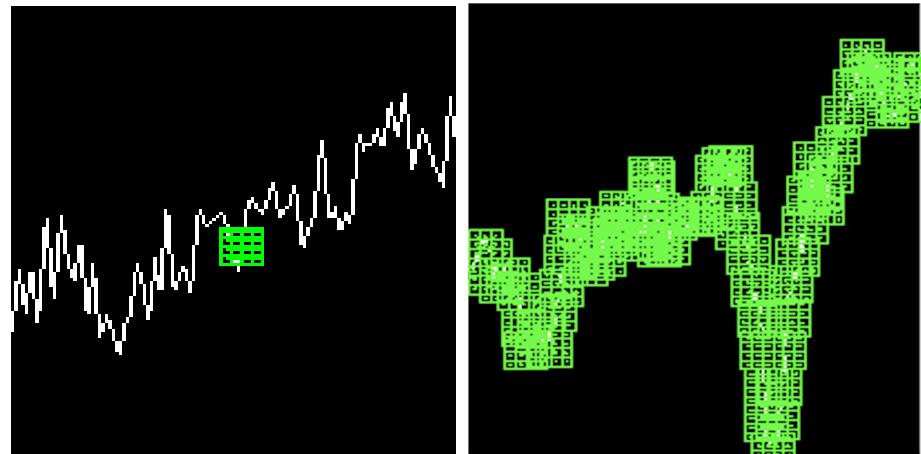

(c) Only one fixed size patches are used on a very specific position of the signal trace.
(d) An entire signal is mapped with fixed size patches with a very high keypoint density $\mathbf{kp_d}$.

Figure 4.2: Four different alternatives of keypoint locations and patch geometry.

On the other hand, on the vertical axis, the vertical patch scale depends on the peak-to-peak amplitude $\Delta\mu V$, and the amplitude scale factor γ , as

$$S_v = \frac{\Delta\mu V \gamma}{\Delta_s}. \quad (4.6)$$

The vertical scale can be dynamically adjusted according to the peak-to-peak amplitude of each segment, or it can be set fixed. This is more appropriate if the underlying signal is

bounded which is the case if the standardized procedure described in 3.3 is applied.

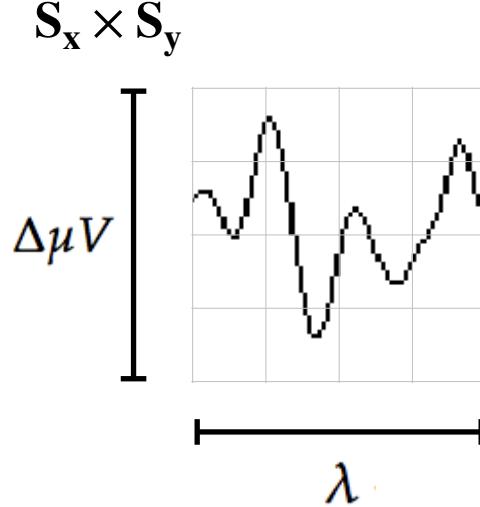


Figure 4.3: The scale of local patch is selected in order to capture the whole transient event. The size of the patch is $\mathbf{S}_y \times \mathbf{S}_x$ pixels. The vertical size consists of 4 blocks of size \mathbf{S}_y pixels which should be high enough as to contain the signal $\Delta\mu V$, the peak-to-peak amplitude of the signal component. The horizontal size includes 4 blocks up to \mathbf{S}_x and should cover the entire duration in seconds of the signal waveform, λ .

Figure 4.3 shows the different parameters of the patch and how they are related to the underlying signal. Once these parameters are set, the size in pixels of the patch can be obtained in both dimensions. Hence, the Horizontal Patch Size in pixels is

$$\mathbf{S}_x = \Delta_s S_t + 1. \quad (4.7)$$

On the other hand, the vertical patch size in pixels can be calculated from

$$\mathbf{S}_y = \Delta_s S_v + 1 \quad (4.8)$$

where Δ_s being the unit length of the patch. The parameters S_t and S_v are the horizontal and vertical patch scale. This region is arranged in a 4×4 grid and the pixel **kp** is the patch center. For instance, for a given set of values of $S_v = 1$ and $S_t = 1$, the patch is a squared region on the image of size 22 pixels.

The patch size cannot be bigger than the image itself, whose width is W_x and its height is H_y . This is reflected by the following two inequalities that restrict the size of the patch

according to

$$\frac{W_x - 1}{\Delta_s} \geq S_t, \quad (4.9)$$

on the horizontal axis, and on the vertical axis,

$$\frac{H_y - 1}{\Delta_s} \geq S_v. \quad (4.10)$$

4.4.1 Oscillatory Processes

For these patterns, the central idea is to locate keypoints, and their patches, all along the signal trace, filling the entire signal segments with all the possible patches. In this case, the keypoint density \mathbf{kp}_d determines the step at which a keypoint is located along the trace of the signal, unit sample after unit sample. Care must be taken close to the margins, where there should be a gap to avoid locating incomplete patches. This can be observed in Figure 4.2(a).

4.4.2 Transient Events

For transient events, descriptors are treated as representatives of the single transient waveforms. This lead to usually just one keypoint that is located in a meaningful position along the horizontal axis. Additionally, for autoscale plotting, the zero level can be used to localize keypoints.

4.5 Classification

A discriminative [126] semi-supervised classification method based on Naive Bayes Nearest Neighbor (NBNN) [11] is applied to classify EEG signals using the features provided by the calculated descriptors. One problem that frequently arises when using local features is how to go back from the classification of those local characteristics to the image where those descriptors come from. The NBNN technique overcomes this problem by comparing each image against a whole label class which is characterized by the set of descriptors q that are closest to each one of the descriptors of the query image \mathbf{d}_i . This algorithm is very easy to implement, and is based on the following Equation:

$$\hat{L} = \arg \min_L \sum_{\mathbf{d}_i^{(bpc)}} \sum_{q \in N_T(\mathbf{d}_i^{(bpc)})} \|q - \mathbf{d}_i^{(bpc)}\|^2. \quad (4.11)$$

The estimated class label \hat{L} of a query image is calculated as the class label L that minimize the summation of the distance between each descriptor $\mathbf{d}_i^{(bpc)}$ that belongs to the query image and its corresponding near neighbor $N_T(\mathbf{d}^{(bpc)})$ descriptor for each class. Figure ?? show a scheme of how this classification method works.

The *bpc* is the Best Performing Channel. This value is determined in the calibration step of the BCI algorithm when the spatial performance is assessed to determine on which channel the performance is maximized [22].

4.6 BCI Algorithm

In brief, based on segmented signals from at least two labeled classes, a set of images is first generated. For each image, keypoints are localized and descriptors are extracted during the training or calibration step of a BCI procedure and they are grouped in KD-tree [72] structures for each one of the classes. Additionally, the spatial performance is evaluated and the *bpc* value is computed.

Hence, given a new unlabeled signal segment, an image plot is generated as well, their keypoints localized and their descriptors extracted. They are fed into Equation 4.11 in order to determine the class which minimizes the summation and thus provide the information bit to the BCI controller.

4.A Implementation Summary

This section provides a mapping cheat-sheet to convert and obtain the parameters of the algorithm for a given set of signal parameters.

The input signal parameters are N, F_s, λ and the peak-to-peak amplitude $\Delta\mu V$ of the waveform to study. The unit length of the patch is $\Delta_s = \sqrt{2} 15$ and as has been earlier mentioned, depends on the particular SIFT implementation.

Output parameters are: $\gamma \ \gamma_t \ H_y \ W_x \ S_t \ S_v \ \mathbf{S}_y \ \mathbf{S}_x \ \mathbf{k}\mathbf{p}$

Mappings:

Amplitude scale factor

$$\gamma \equiv \frac{H_y}{\Delta\mu V}$$

Time scale factor

$$\gamma_t \equiv \frac{W_x}{F_s w}$$

Restriction on the waveform time scale

$$\frac{W_x - 1}{\sqrt{2} 15} \geq S_t$$

Restriction on the waveform amplitude scale

$$\frac{H_y - 1}{\sqrt{2} 15} \geq S_v$$

Horizontal Patch scale

$$S_t = \frac{\lambda F_s \gamma_t}{\Delta_s}$$

Vertical Patch scale

$$S_v = \frac{\Delta \mu V \gamma}{\Delta_s}$$

Time to sample point conversion

$$n = \lfloor F_s \Delta_t \rfloor \gamma_t$$

Horizontal Patch size in pixels


$$\mathbf{S}_x = \Delta_s S_t + 1$$

Vertical Patch Size in pixels


$$\mathbf{S}_y = \Delta_s S_v + 1$$

Span of a Patch

$$\Delta_t = \frac{S_t \Delta_s}{F_s \gamma_t}$$

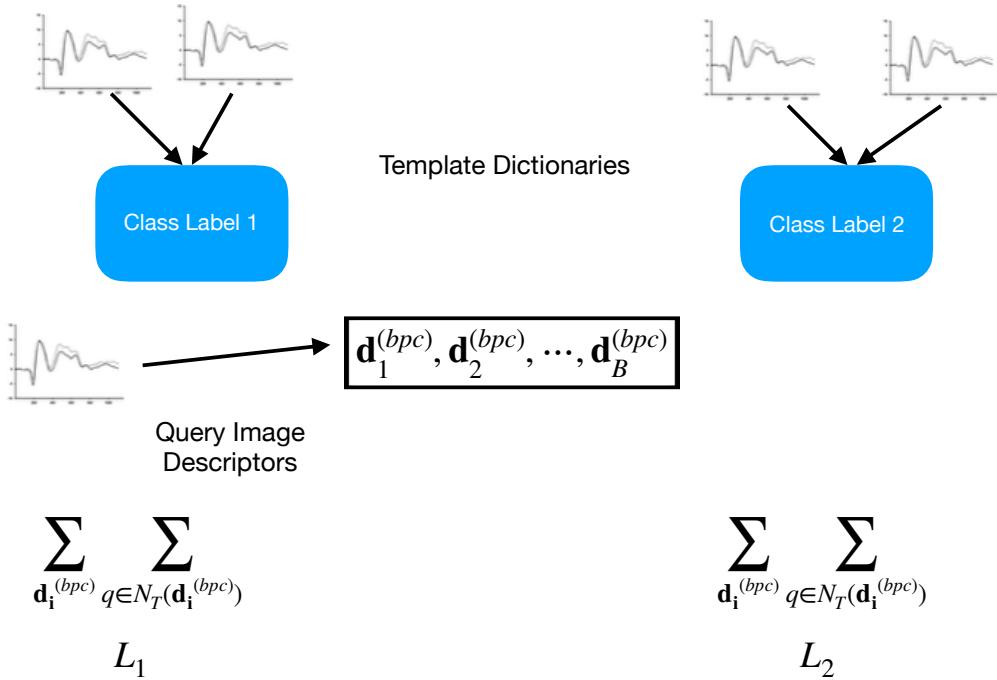


(a) Two Dictionaries contain templates descriptors for two different classes. A set of query descriptors are extracted from a new image that needs to be categorized.

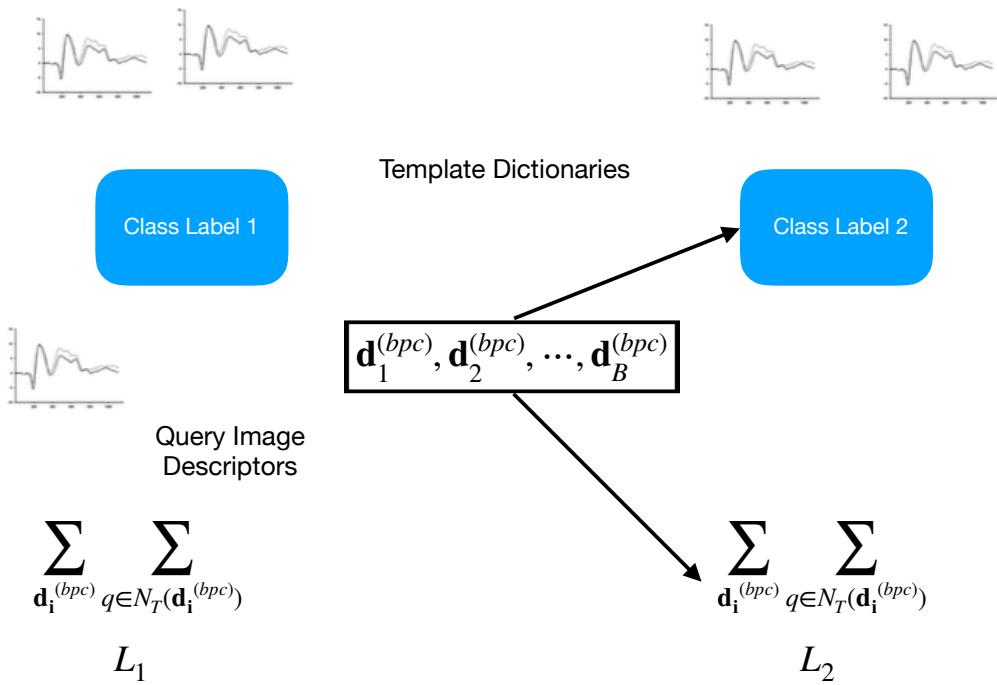


(b) Distances from every descriptor \mathbf{d}_i are calculated against the closest one from the Dictionary of Class 2. Distances summations are accumulated.

Figure 4.4: NBNN Classification Scheme

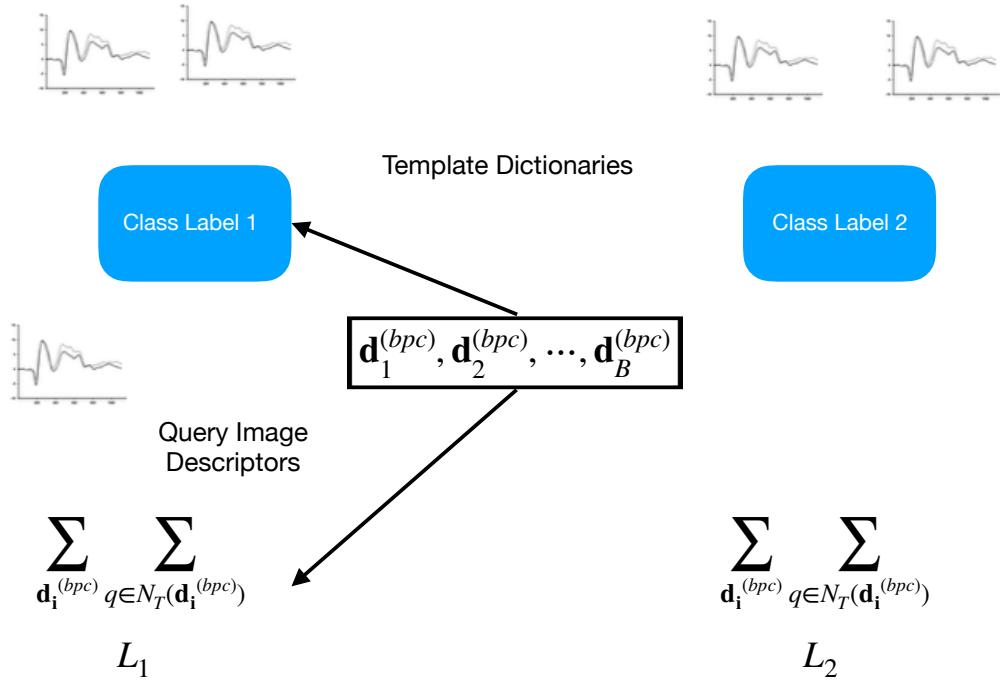

(a) Distance values from every descriptor \mathbf{d}_i are calculated against the closest one from the Dictionary of Class 1. Distances summations are accumulated.

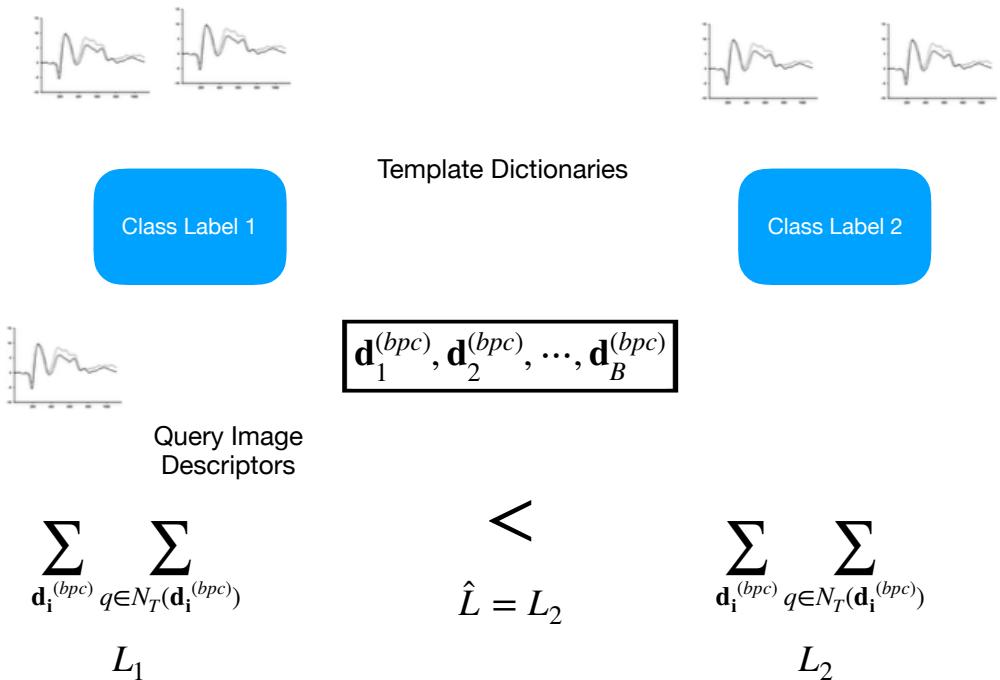

(b) The two different summation values are compared against each other. The summation that achieved the lesser value is the one that more closely resembles the set of templates, thus is the one predicted by the classification algorithm.

Figure 4.5: NBNN Classification Scheme

Chapter 5

Alpha Wave: inhibition signal

The electroencephalogram represents a continuous curve with continuous oscillations in which... one can distinguish larger first order waves with an average duration of 90 milliseconds...

Berger


This Chapter describes the experiments performed over a well-established but still mysterious EEG cognitive signal: The Berger Rhythm or Visual Occipital Alpha Waves. An own dataset of resting subjects with and without alpha blocking is produced and the details of their generation are outlined. Additionally, an experiment on a public Dataset is also delineated. Conclusions and discussion are described in the last section.

5.1 Introduction

Alpha Waves were the first signals ever spotted from the Electroencephalography. They are regularly characterized as 10Hz, or more broadly between the frequency band of 8-12 Hz. They are physiologically consistent across subjects, though it has been reported inter- and intra- variations with functional cognitive implications [47]. Moreover, they are associated with synchronous inhibitory processes and attention shifting [99]. They tend to be more prominent while subject's eyes are closed and appear stronger in occipital regions, around O_1 and O_2 [126, 110]. These waves are also called Prominent Posterior Alpha or Posterior Dominant Rhythm due to their pervasiveness in EEG [103, 47].

Figure 5.1 shows two records of 8-channels signals. Figure 5.1(a) contains the registered alpha waves of a subject with their eyes open while the (b) contains the same information

with their eyes closed. The characteristic pattern of wiggles can be spotted in the latter, while their absence entails the blocking of alpha waves in the former [7].

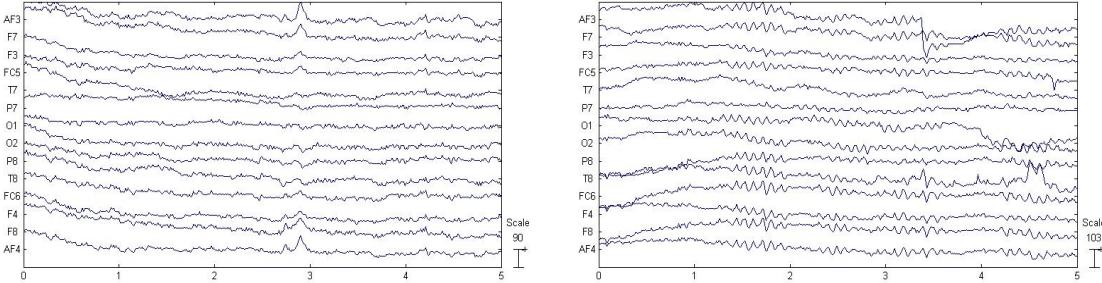

(a) EEG signals of a relaxed healthy subject with their eyes open.
(b) EEG signals of the same relaxed subject with their eyes closed. Alpha Waves wiggles can be spotted since the first second.

Figure 5.1: Five seconds of EEG signals obtained from the Emotiv EPOC device. Fourteen channels are shown.


This important rhythm is an oscillatory process. As such, it is understood and studied in the frequency-domain. Figure 5.2 show the results of applying the Fast Fourier Transform to two different segments of 10s length. For each segment, the Power Spectral Density is calculated and their values are shown on the vertical axis. Frequency values are shown on the horizontal axis. On Figure (a) no particular frequency component can be spotted. However, on Figure (b) the prevalence of the 10-Hz alpha wave component can be observed.

5.2 Materials and Methods

These experiments consist in performing a binary classification of EEG signal segments between the two defined classes. Class 2 is assigned to segments containing significant alpha waves (i.e. eyes closed), whereas class 1 identifies those where these signals are blocked (i.e. eyes open).

5.2.1 Dataset I - Emotiv EPOC alpha waves own dataset

The first dataset is gathered using the EEG EPOC Emotiv Headset. Although this is a commercial-grade device, it provides an acceptable price-performance ratio and it has been used to investigate basic EEG processes [31, 30]. In order to obtain the multichannel raw EEG signal, a C++ SDK library provided by the manufacturer is used and an in-house

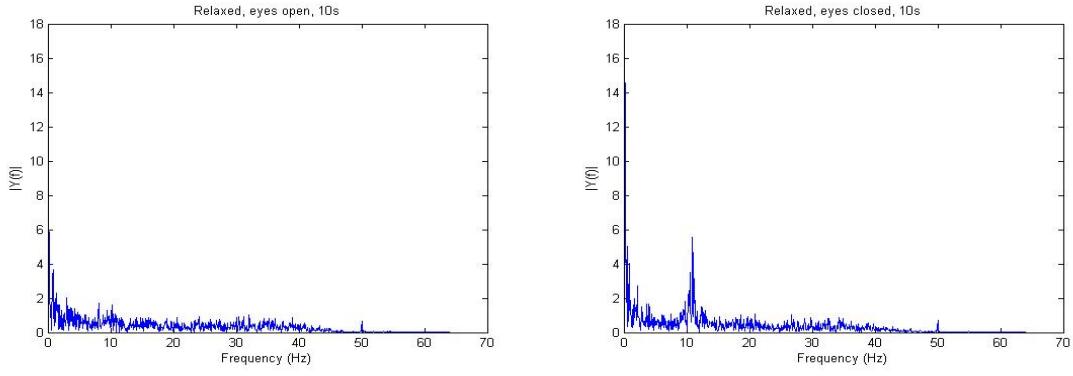

(a) Subject was sit, relaxed in front of the Computer Monitor with his eyes open. (b) Subject was sit, relaxed in front of the Computer Monitor with his eyes closed. A strong 10Hz component can be observed.

Figure 5.2: Spectrum components of a 10s signal segment of a subject with their eyes open. Horizontal axis shows different frequencies while the vertical axis represents the PSD. In both diagrams a 50Hz line component can be visualized.

software program is developed. This device has 14 channels, and a sampling rate of 128 Hz[110]. Available channels are AF3, F7, F3, FC5, T7, P7, O1, O2, P8, T8, FC6, F4, F8, AF4. Ten healthy subjects between ages 20-50 are recruited and they accept to wear the device and to participate in the experiments.

A 30 minutes procedure is required to adjust the headset to each user, in order to decrease the impedance on each electrode (below $5\text{k}\Omega$). This is achieved by physically adjusting the headset position over the scalp, and by embedding each electrode electrode pad in saline solution. Once the set up is finished, each subject is instructed to sit in a relaxed position. Subsequently, she/he is commanded to watch the screen for 15 seconds, trying to avoid, as much as possible, to abruptly move its body or head. During that time, a single-trial of 10 seconds-length window of EEG signals data is transferred to a PC and logged into standard binary files. After a 5 minutes pause, the subject is asked to close the eyes avoiding any movement while keeping the same pose for another batch of 15 seconds. Again, 10 seconds of EEG information are transferred and logged into the PC. This finally produce a dataset of 10 subjects, 2 classes per subject, composed of 14 channels, 10-seconds length or 1280 samples per window. These windows are further divided into 10 segments per class and per subject.

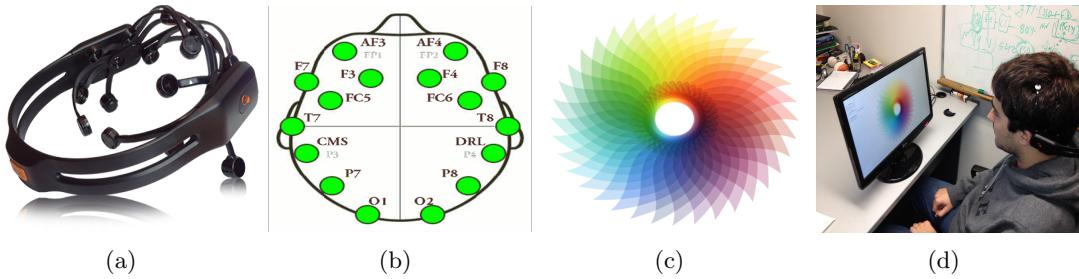


Figure 5.3: (a) EPOC Emotiv consumer-grade 14-channels Wireless EEG.(b) This device has a fixed set of positions according to the 10-20 International System.(c) While resting and sitting comfortable in a chair, subjects had to fixate their sight to the center of this image which was being displayed on a computer monitor, 1 meter away from the subject.(d) Subject performing the experiment described to produce the Dataset described in 5.2.1

5.2.2 Dataset II - AlphaNet Dataset

Additionally, the performance of HIST was tested against the public dataset EEG Motor Movement/Imagery Dataset of the PhysioNet effort published and maintained by the NHS [101, 40].


Baseline records and motor/imagery tasks were performed by 109 healthy volunteers, using the BCI2000 system [101]. At the same time 64-channel EEG records were registered where each subject completed 14 tasks, called Runs. The first two are the baseline calibration tasks, of relevance for this Chapter. These Runs 1 and 2 are each one-minute records of resting subjects with eyes open and eyes closed. From these records, 60 segments of 1-second length are further extracted per subject. Class labeling is the same as Dataset I. The experiment was performed on 25 of the 109 subjects.

5.2.3 Parameters

Descriptors are extracted from all the generated images, from both classes, and they are used to classify images in a 10-fold cross-validation procedure. Keypoint localization is determined according to Section 4.3 by following the trace of the signal, with a $\mathbf{k}_{pd} = 1$. The NBNN classification method described in Section 4.5 is used. The parameter γ is set to 1, as well as γ_t .

5.3 Results

Dataset I was controlled and verified by processing it with a 8-12Hz band-pass filter, and calculating the average power spectral density across subjects for each channels. It can be observed on Figure 5.4(a) that values corresponding to class 2 (eyes closed) are always higher than the values obtained for class 1 (eyes open). On the other hand, for the sake of illustration, a scatter plot of the obtained segment's PSD for O1 vs O2 for Subject 2 is shown, where a clear separation of classes can be devised. In brief, there is discriminative information in the frequency-domain.

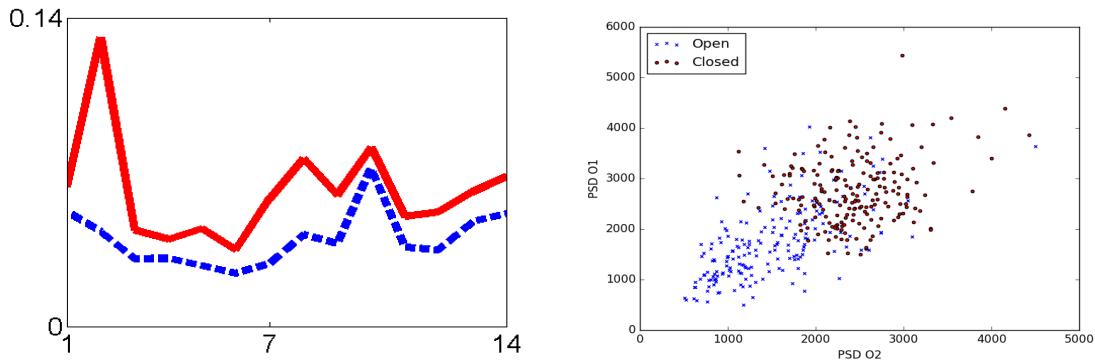

(a) PSD averaged across 10 subjects for each channel. (b) Scatterplot of PSD for the channel O1 vs O2. Values for Class 2 (red) are always higher than values for Class 1 (blue). There is a separation of classes between the red (class 2) and blue (Class 1) dots.

Figure 5.4: Verification and control of the obtained Dataset I.

Results of applying a 10-Fold Cross Validation procedure on the entire set of labeled descriptors is shown on Figure 5.5. Descriptors from different subjects were used as part of the different training set to classify unknown images, so the obtained accuracy level was subject-independent. Moreover, a classification level with average above 70% was obtained in Occipital channels.

For the Dataset II, an accuracy median higher than 70% for 25 subjects, also on occipital channels O1, Oz, O2 and Iz (numbered 61 to 64) is obtained while discriminating Runs 1 and 2 (Baseline eyes open vs Baseline eyes closed). This information can be devised on Figure 5.6 (a) where boxplots of the averaged classification accuracies for all the subjects are represented. On the other hand, Figure 5.6(b) shows the 10-Fold Validated Accuracy for one random subject. A higher accuracy in the classification of the signals can also be seen over occipital channels.

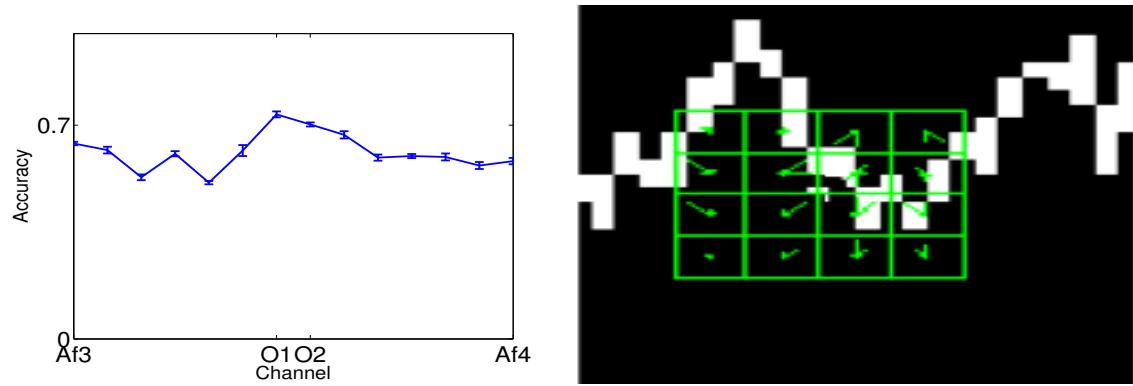


Figure 5.5: The classification accuracy is maximum on occipital channels O1 and O2. The descriptor size is 12x12 pixels which corresponds to a variation of $\Delta\mu V = 12$ microvolts in the signal amplitude during $\lambda = 0.09$ seconds.

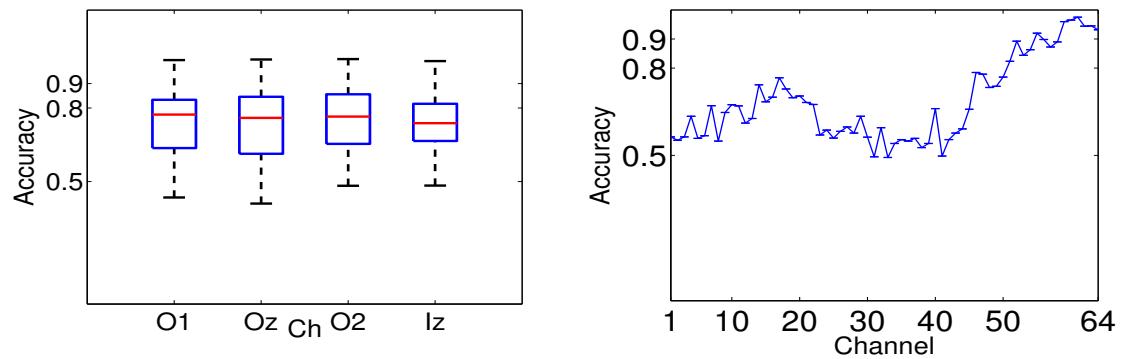


Figure 5.6: Classification Accuracy for discriminating windows of 1s ($N = 160$) of EEG for Alpha Waves differences between subjects with eyes opened and closed.

5.4 Conclusion

It is known and it was verified here that the discriminative information in EEG alpha waves is mostly contained in the frequency-domain. In spite of this, there is enough discriminative information to classify alpha waves signals solely on the information contained on the wiggles of the plot that is captured by the HIST method presented in this Thesis. Offline Alpha Waves presence was detected from plots of single segments of EEG signals with an accuracy level 10-fold cross validated of 70%.

It was also showed and proved here that there is information within the plot of a signal related to 8-12 Hz oscillatory alpha waves is higher around the occipital region and that an automated procedure which analyze visually the image structure can detect them. This important oscillatory rhythm has many connections with shifting of attention and with volitional changes and is of quite relevance in BCI research. Particularly, the BCI paradigm of Covert Spatial Visual Attention is a further area of research for this method due to the fact that it is entirely based on analyzing alpha waves. Moreover, the posterior rythm has many implications outside the field of BCI and is very important to assess healthy EEG patterns. The exact meaning of alpha waves is still debated[1] and this basic procedure can open the possibility to explore it under a different perspective and verify if they can be effectively tied to some unexpected form of volitional control which may be effective for BCI understanding and improvement.

Chapter 6

Motor Imagery: the hunt for a greek letter

...utilizing the brain signals in
man-computer dialogue.

Vidal

6.1 Introduction

Motor Imagery is an EEG or ECoG based BCI paradigm originated on changes of SMR, sensorimotor rhythms, that are altered when a person engages in motor behavior, but it can also be elicited when a person imagines to perform any movement. Particularly, the Rolandic wicket rhythm, the μ rhythm, is of the same frequency (e.g. 8-12 Hz) of visual occipital alpha waves, but from a spatially different location (posterior frontal and anterior parietal areas)[126]. Although SMR patterns presents a high inter- and intra-subjects variability regarding the signal features required to identify them, an Event Related Desynchronization/Synchronization of μ rhythm is in general consistent across subjects, regardless of the specificity of the imagined movement (i.e. what is being imagined to move).

6.2 Materials and Methods

In order to verify if this ERD/ERS could be detected by the method presented in this Thesis, i.e. by automatically extracting the information from the signal plots, a BCI Simulation is performed against the public Motor Imagery Dataset 002-2014, published by BNCI-Horizon 2020 website and initiative [108]. This dataset is composed of 8 runs for 14 participants.

The first 5 runs are used for training without feedback, and the remaining 3 runs are used to test the results. The original online experiment was performed with 20 trials on each run, 10 corresponding to imagining moving the right hand and the other 10 to feet movement. Figure 6.1 schematize the protocol and the structure of this published dataset. This BCI simulation experiment is divided in two. In the first simulation, baseline signals, corresponding to the 1st second of each trial are compared against right hand motor imagery, which is 4.5 seconds ahead of the beginning of each trial. Signal segments of 1-second length are processed for 10 trials for each of 5 runs and their descriptors are extracted for both classes. The second BCI simulation is similar but only extracting trials corresponding to feet movement imagery.

BCI Simulation or Cross Validation?

The brain signals decoding branch of BCI Research inherits practices from Machine Learning and a cross-validation procedure is a common practice. However, in terms of the data extracted from the brain of a person who is learning and changing how to perform a certain operation, it violates time dynamics to use information extracted from forward experiences to derive outputs in the past.

The idea of implementing a BCI Simulation is not very well defined in BCI research, but their practice, without naming it, has been the regular approach for BCI Competitions. The idea is to use an offline dataset simulating what would have happened if the system have been tested in real-time following the same sequence of operations that what was used to generate the dataset.

Regardless, of any definition, the Online Validation with feedback of any BCI system is the unquestioned Gold Standard of the discipline [126].

6.3 Results

Binary classification accuracies are calculated based on the output of the BCI simulation on the remaining 3 runs for each participant, in a single-trial approach: for each sampled segment of 1-second length, classification based on the classification algorithm described in 4.5 is applied and a match or mismatch is obtained. Results are shown in Figure 6.2 where for right-hand detection *RH*, average accuracies of around 70% are obtained for the channel C3, the best-performing channel *bpc*, coincidentally with the contralateral structure of the imagined movement. On the other hand, the binary classification accuracy for feet imagery detection *FM*, achieves in all the channels accuracies of just above chance level.

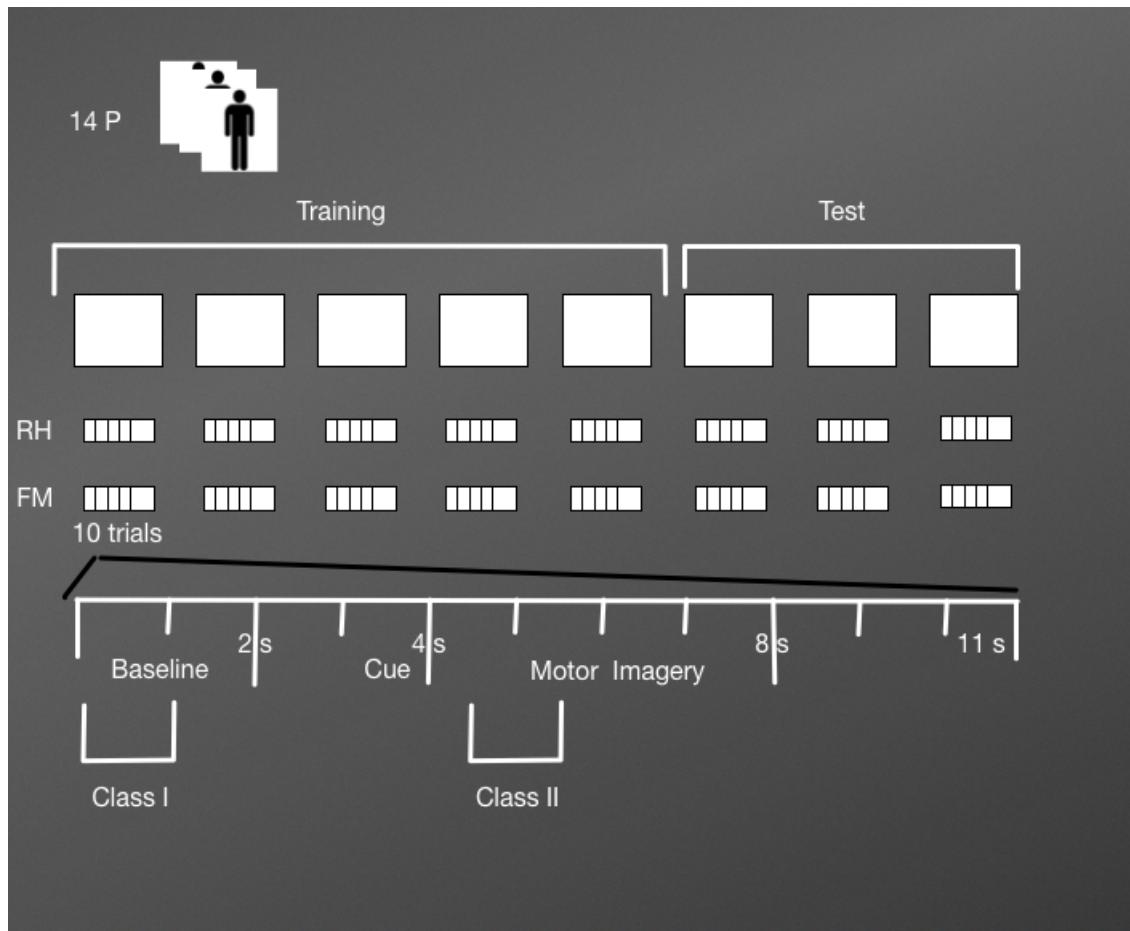


Figure 6.1: Fourteen voluntary Participants performed 5 sessions of training and 3 sessions of testing. On each session each subject had 10 trials to perform Right Hand Motor Imagery and 10 trials for Feet Movement. At the same time, each trial has a 2-seconds baseline and a 4-seconds section to perform the imagery task. For each BCI Simulation, Class 1 is defined from EEG information obtained from the baseline section, while Class 2 is based on extracting segments from the imagery section of the EEG signal.

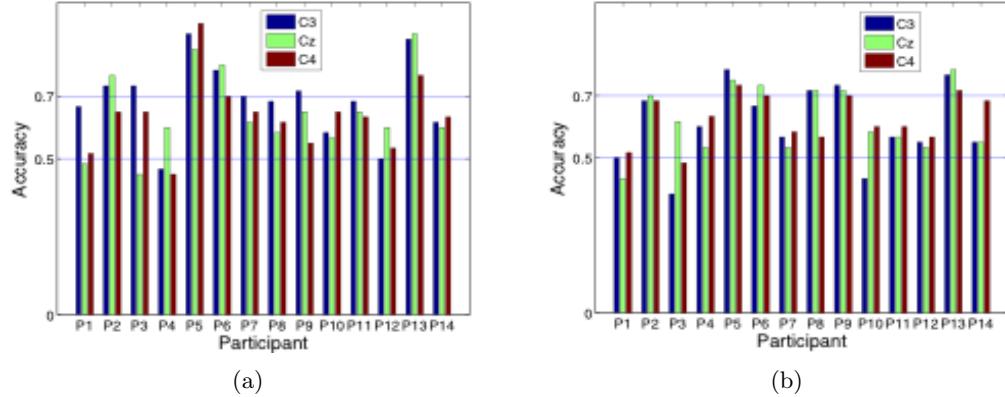


Figure 6.2: Classification Accuracy for discriminating segments of 1s ($N = 512$) of EEG for Motor Imagery detection BCI simulation. (a) Accuracy values for channels C3, Cz and C4 for the 14 participants of the described MI dataset discriminating between baseline and right-hand imagery. (b) The same procedure for feet imagery. Accuracy levels averaged to 70% are obtained only for right-hand movement on the contralateral channel C3. The horizontal S_t and vertical S_v patch scale are adjusted to 6

6.4 Conclusion

Offline BCI Simulation of single trial asynchronous triggering for right hand MI based on signal plots is implemented with a level of success of 70% for 7 out of 14 Participants. Single trial asynchronous triggering of BCI can be implemented with this paradigm, particularly for right-hand motor imagery. The name μ rhythm was precisely coined because the shape of the waves have some resemblance to the greek letter [26]. Additionally, in line with previous chapter results, though the differentiation information is contained in the frequency domain, the method based on the Histogram of Gradient Orientation detected differences in the shape of the signals. Coincidentally with results obtained from Alpha Waves, there is information that is mapped in the structure of the waveform, at least for frequencies on the 10 Hz range, which characterize both types of waves.

Chapter 7

Event Related Potential: The P300 Wave

Talking off the top of your head....

Farwell and Donchin

7.1 Introduction

The P300 [34, 64] is a positive deflection of the EEG signal which occurs around 300 ms after the onset of a rare and deviant stimulus that the subject is expected to attend. It is produced under the oddball paradigm [126] and it is consistent across different subjects. It has a lower amplitude ($\pm 5\mu V$) compared to basal EEG activity, reaching a Signal to Noise Ratio (SNR) of around -15 db estimated based on the amplitude of the P300 response signal divided by the standard deviation of the background EEG activity [52].

This signal can be cleverly utilized to implement a speller application by means of a Speller Matrix. Farwell and Donchin P300 Speller [34] is one the most used BCI paradigms to implement a thought translation device and to send commands to a computer in the form of selected letters, similar to typing on a virtual keyboard. This procedure exploits this cognitive phenomena by detecting along the EEG trace of a person which is focusing on a sequence of two different visual flashing stimulus, the distinctive P300 transient component each time the expected stimulus flashes. On the P300 Speller, rows and columns of a 6×6 matrix flash randomly but only the flashing of a column or row where the letter that a user is focusing will trigger concurrently the P300 ERP.

Figure 7.1 shows an example of the Speller Matrix used in the OpenVibe open source software [95], where the flashes of rows and columns provide the deviant stimulus required

to elicit this physiological response. Each time a row or a column that contains the desired letter flashes, the corresponding synchronized EEG signal should also contain the P300 signature and by detecting it, the selected letter can be identified.

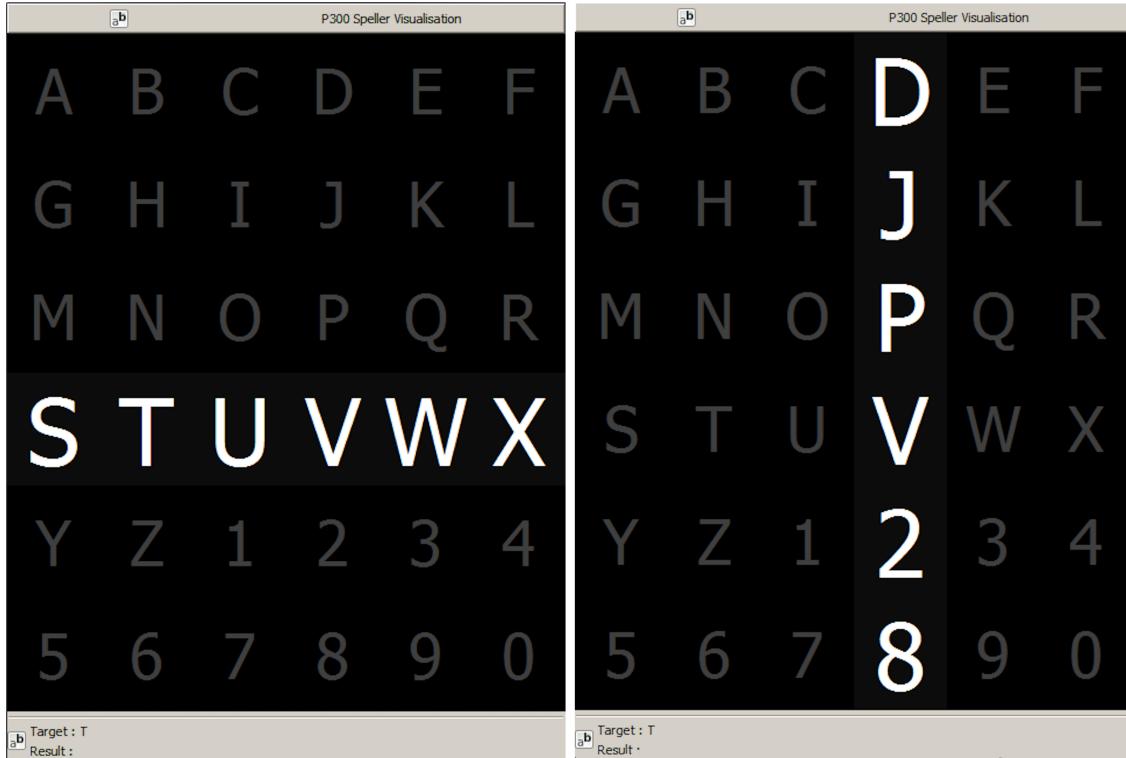


Figure 7.1: Example of the 6×6 Speller Matrix used in the study obtained from the OpenVibe software. Rows and columns flash in random permutations.

7.2 Materials and Methods

In this section, the signal preprocessing, the ERP Extraction, and the Speller Matrix identification are described. Figure 7.2 outlines a scheme of this process. Additionally, the experiments that were conducted, are also expounded.

Up to this point, EEG signals were treated in *raw* form. The reason being, the oscillatory processes that were studied contain a waveform that could be detected from raw signal plots. However, this is not the case with the P300 Wave, and a preprocessing step, and more importantly an enhancement of the SNR though signal averaging, is in general mandatory to extract the ERP waveform.

7.2.1 Preprocessing Pipeline

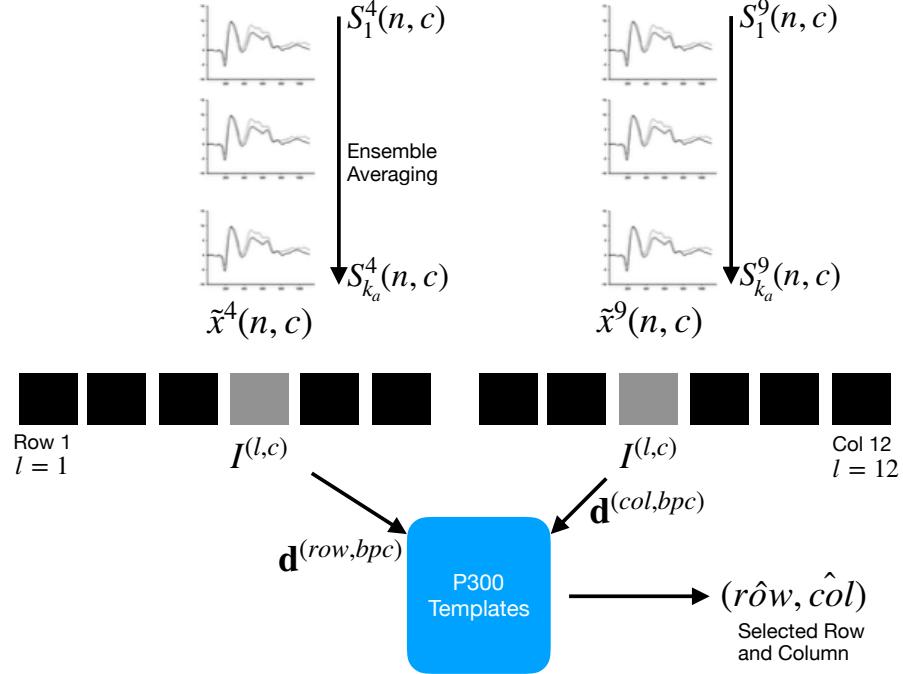


Figure 7.2: For each column and row, an averaged, standardized and scaled signal $\tilde{x}^l(n, c)$ is obtained from the segments S_i^l corresponding to the k_a intensification sequences with $1 \leq i \leq k_a$ and location l varying between 1 and 12. From the averaged signal, the image $I^{(l,c)}$ of the signal plot is generated and each descriptor is computed. By comparing each descriptor against the set of templates, the P300 ERP can be detected, and finally the desired letter from the matrix can be inferred.

The data obtained by the capturing device is digitalized and a multichannel EEG signal is constructed. The 6 rows and 6 columns of the Speller Matrix are intensified providing the visual stimulus. The number of a row or column is a location. A sequence of twelve randomly permuted locations l conform an intensification sequence. The whole set of twelve intensifications is repeated k_a times.

- **Signal Enhancement:** This stage consists of the enhancement of the SNR of the P300 pattern above the level of basal EEG. The pipeline starts by applying a notch filter to the raw digital signal, a 4th degree 10 Hz lowpass Butterworth filter and finally a decimation with a Finite Impulse Response (FIR) filter of order 30 from the original sampling frequency down to 16 Hz [65].
- **Artifact Removal:** For every complete sequence of 12 intensifications of 6 rows and

6 columns, a basic artifact elimination procedure is implemented by removing the entire sequence when any signal deviates above/below $\pm 70\mu V$.

- **Segmentation:** For each of the 12 intensifications of one intensification sequence, a segment S_i^l of a window of t_{max} seconds of the multichannel signal is extracted, starting from the stimulus onset, corresponding to each row/column intensification l and to the intensification sequence i . As intensifications are permuted in a random order, the segments are rearranged corresponding to row flickering, labeled 1-6, whereas those corresponding to column flickering are labeled 7-12. Two of these segments should contain the P300 ERP signature time-locked to the flashing stimulus, one for the row, and one for the column.
- **Signal Averaging:** The P300 ERP is deeply buried under basal EEG so the standard approach to identify it is by point-to-point averaging the time-locked stacked signal segments. Hence the values which are not related to, and not time-locked to the onset of the stimulus are canceled out [66].

Balanced Information Transfer Rate

The procedure described in 7.2.1 determines the operation of any P300 Speller. In order to obtain an improved signal in terms of its SNR, repetitions of the sequence of row/column intensification are necessary. And, at the same time, as long as more repetitions are needed, the ability to transfer information faster is diminished, so there is a trade-off that must be acutely determined [65].

In brief, the procedure to obtain the point-to-point averaged signal goes as follows:

1. Highlight randomly the rows and columns from the matrix. There is one row and one column that should match the letter selected by the subject.
2. Repeat step 1 k_a times, obtaining the $1 \leq l \leq 12$ segments $S_1^l(n, c), \dots, S_{k_a}^l(n, c)$, of the EEG signal where the variables $1 \leq n \leq n_{max}$ and $1 \leq c \leq C$ correspond to sample points and channel, respectively. The parameter C is the number of available EEG channels whereas N is the segment length and F_s is the sampling frequency. The parameter k_a is the number of repetitions of intensifications and it is an input parameter of the algorithm.

3. Compute the Ensemble Average by

$$x^l(n, c) = \frac{1}{k_a} \sum_{i=1}^{k_a} S_i^l(n, c) \quad (7.1)$$

for $1 \leq n \leq n_{max}$ and for the channels $1 \leq c \leq C$. This provide an averaged signal $x^l(n, c)$ for the twelve locations $1 \leq l \leq 12$.

7.2.2 Speller Matrix letter Identification

P300 ERP Extraction

Segments corresponding to row flickering are labeled 1-6, whereas those corresponding to column flickering are labeled 7-12. The extraction process has the following steps:

- **Step A:** First highlight rows and columns from the matrix in a random permutation order and obtain the Ensemble Average as detailed in steps 1, 2 and 3 in Section 7.2.1.
- **Step B:** Plot the signals $\tilde{x}^l(n, c)$, $1 \leq n \leq n_{max}$, $1 \leq c \leq C$, according to Section 3.7 in order to generate the images $I^{(l,c)}$ for rows and columns $1 \leq l \leq 12$.
- **Step C:** Obtain the descriptors $\mathbf{d}^{(l,c)}$ for rows and columns from $I^{(l,c)}$ in accordance to the method described in Section 4.2.

Calibration

A trial, as defined by the BCI2000 platform [101], is every attempt to select just one letter from the speller. A set of trials is used for calibration and once the calibration is complete it can be used to identify new letters from new trials.

During the calibration phase, two descriptors $\mathbf{d}^{(l,c)}$ are extracted for each available channel, corresponding to the locations l of a selection of one previously instructed letter from the set of calibration trials. These descriptors are the P300 templates, grouped together in a template set called T^c . The set is constructed using the steps described in Section 7.2.1 and the steps A, B and C of the P300 ERP extraction process.

Additionally, the best performing channel, bpc is identified based on the the channel where the best Character Recognition Rate is obtained.

Letter identification

In order to identify the selected letter, the template set T^{bpc} is used as a database. Thus, new descriptors are computed and they are compared against the descriptors belonging to the calibration template set T^{bpc} .

- **Step D:** Match to the calibration template T^{bpc} by computing

$$\hat{r}ow = \arg \min_{l \in \{1, \dots, 6\}} \sum_{q \in N_T(\mathbf{d}^{(l,bpc)})} \left\| q - \mathbf{d}^{(l,bpc)} \right\|^2 \quad (7.2)$$

and

$$\hat{col} = \arg \min_{l \in \{7, \dots, 12\}} \sum_{q \in N_T(\mathbf{d}^{(l,bpc)})} \left\| q - \mathbf{d}^{(l,bpc)} \right\|^2 \quad (7.3)$$

where $N_T(\mathbf{d}^{(l,bpc)})$ is defined as $N_T(\mathbf{d}^{(l,bpc)}) = \{\mathbf{d} \in T^{bpc} / \text{is the k-nearest neighbor of } \mathbf{d}^{(l,bpc)}\}$ for the best performing channel. This set is obtained by sorting all the elements in T^{bpc} based on distances between them and $\mathbf{d}^{(l,bpc)}$, choosing the k with smaller values, with k a parameter of the algorithm. This procedure is an adapted version of the k-NBNN algorithm [11] described in Section 4.5, to the letter identification required in the BCI-Based P300 Speller implementation.

By computing the aforementioned equations, the letter of the matrix can be determined from the intersection of the row $\hat{r}ow$ and column \hat{col} . Figure 7.2 shows a scheme of this process.

7.2.3 Experimental Protocol

To verify the validity of the proposed framework and method over transients events, the public dataset 008-2014 [96] published on the BNCI-Horizon website [16] by IRCCS Fondazione Santa Lucia, is used. A BCI Simulation is performed to decode the spelled words from the provided signals.

Additionally, an own dataset with the same experimental conditions is generated. A different BCI Simulation is implemented and the decoding of letters is performed.

In order to verify how this method performs against similar methods that also use the structure of the waveform, a P300 ERP template, obtained from a ALS patients dataset,

is superimposed into a distinct EEG stream. This trace was experimentally obtained by a subject which was observing the flashing of the stimulus matrix during a P300 Speller procedure but did not engage in focusing on any letter in particular. Everything is there, except the P300 ERP component. Along the EEG stream, the markers information was used to localize the *True* segments where the P300 should have been found, and those timing locations are used to superimpose the extracted ERP waveform. By implementing this pseudo-real approach, it is possible to effectively control null-signals and to adjust the shape of this evoked potential in accordance to similar procedures used in other works [84, 58, 90].

Finally, the performance of the method presented in this Thesis is tested against one of the dataset published by the BCI Competitions.

P300 ALS Public Dataset

The experimental protocol used to generate this dataset is explained in [96] but can be summarized as follows: 8 subjects with confirmed diagnoses but on different stages of ALS disease, were recruited and accepted to perform the experiments. The Visual P300 detection task designed for this experiment consisted of spelling 7 words of 5 letters each, using the traditional P300 Speller Matrix [34]. The flashing of rows and columns provide the deviant stimulus required to elicit this physiological response. The first 3 words are used for calibration and the remaining 4 words, for testing with visual feedback. A trial is every attempt to select a letter from the speller. It is composed of signal segments corresponding to $k_a = 10$ repetitions of flashes of 6 rows and $k_a = 10$ repetitions of flashes of 6 columns of the matrix, yielding 120 repetitions. Flashing of a row or a column is performed for 0.125 s, following by a resting period (i.e. inter-stimulus interval) of the same length. After 120 repetitions an inter-trial pause is included before resuming with the following letter.

The recorded dataset was sampled at 256 Hz and it consisted of a scalp multichannel EEG signal for electrode channels Fz, Cz, Pz, Oz, P3, P4, PO7 and PO8, identified according to the 10-20 International System, for each one of the 8 subjects. The recording device was a research-oriented digital EEG device (g.Mobilab, g.Tec, Austria) and the data acquisition and stimuli delivery were handled by the BCI2000 open source software [101].

In order to assess and verify the identification of the P300 response, subjects are instructed to perform a copy-spelling task. They have to fix their attention to successive letters for copying a previously determined set of words, in contrast to a free-running operation of the speller where each user decides on its own what letter to choose.

P300 for healthy subjects

We replicate the same experiment on healthy subjects using a wireless digital EEG device (g.Nautilus, g.Tec, Austria). Figure 7.3 shows the front and back of the g.Tec head cap and two subjects performing this experiment. The experimental conditions are the same as those used for the previous dataset, as detailed in section 7.2.3. The produced dataset is available in a public online repository [92].

Participants are recruited voluntarily and the experiment is conducted anonymously in accordance with the Declaration of Helsinki published by the World Health Organization. No monetary compensation is handed out and all participants agree and sign a written informed consent. This study is approved by the *Departamento de Investigación y Doctorado, Instituto Tecnológico de Buenos Aires (ITBA)*. All healthy subjects have normal or corrected-to-normal vision and no history of neurological disorders. The experiment is performed with 8 subjects, 6 males, 2 females, 6 right-handed, 2 left-handed, average age 29.00 years, standard deviation 11.56 years, range 20-56 years.

EEG data is collected in a single recording session. Participants are seated in a comfortable chair, with their vision aligned to a computer screen located one meter in front of them. The handling and processing of the data and stimuli is conducted by the OpenVibe platform [95].

Gel-based active electrodes (g.LADYbird, g.Tec, Austria) are used on the same positions Fz, Cz, Pz, Oz, P3,P4, PO7 and PO8. Reference is set to the right ear lobe and ground is preset as the AFz position. Sampling frequency is slightly different, and is set to 250 Hz, which is the closest possible to the one used with the other dataset.



Figure 7.3: The g.Tec device, wearable and wireless g.Nautilus headset. Subjects wearing the g.LADYbird cap.

P300 Pseudo-Real Dataset Generation

The template ERP is acquired from the Subject Number 8 of the public dataset 008-2014 [96] published on the BNCI-Horizon website [16] by IRCCS Fondazione Santa Lucia. Segments from the EEG signal containing the ERP are extracted for the trial number 2, and they are point-to-point coherently averaged. This P300 ERP can be seen in Figure 7.4.

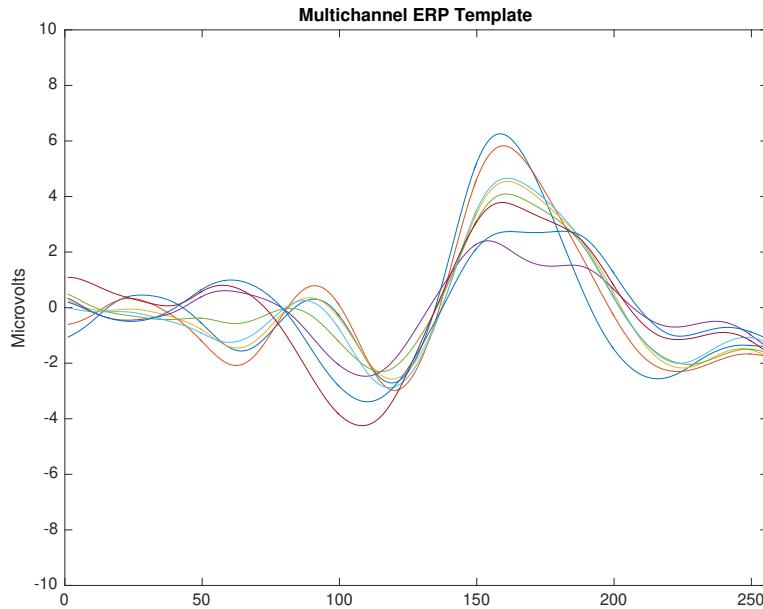


Figure 7.4: ERP Template obtained from the coherent point-to-point ensemble average from the signals of Subject Number Eight of the BNCI Horizon public dataset 008-2014. The template is 1s long which is 256 sample points, and the eight channels are superimposed with different colors. The P3b component can be seen around the sample index 150 and 200.

An EEG stream with null-P300 signal is obtained by the following procedure: A subject participant is recruited voluntarily and the experiment is conducted anonymously in accordance with the Declaration of Helsinki published by the World Health Organization. No monetary compensation is handed out and she/he agrees and signs a written informed consent. This study is approved by the *Departamento de Investigación y Doctorado, Instituto Tecnológico de Buenos Aires (ITBA)*. The participant is healthy and have normal or corrected-to-normal vision and no history of neurological disorders. This voluntary subject is aged between 20-30 years old. EEG data is collected in a single recording session. She/He is seated in a comfortable chair, with her/his vision aligned to a computer screen located one meter in front of her/him. The handling and processing of the data and stimuli is

conducted by the OpenVibe platform [95]. Gel-based active electrodes (g.LADYbird, g.Tec, Austria) are used on locations Fz, Cz, Pz, Oz, P3,P4, PO7 and PO8 according to the 10-20 international system. Reference is set to the right ear lobe and ground is preset as the AFz position. Sampling frequency is set to 250 Hz.

The participant is instructed to passively watch the flashing screen while not focusing on any particular letter. The experimental conditions are the same as those described for previous datasets. A questionnaire is handed out at the end of the experiment with questions about how the participant felt during it, without giving more details.

Figure 7.5 shows a 5s sample of the EEG trace obtained with the MNE library [41]. Channel S represents the twelve different stimulus markers (columns or rows) while channel L represent the label (*True* vs *False*). Labels are represented by square signals. *False* segments are marked with single amplitude square signals while *True* segments are identified by double-amplitude square signals. Subfigure (a) shows the signals before the ERP template is superimposed while subfigure (b) shows the same signals with the superimposed ERP template. At first-sight, differences are really hard to spot visually. Subfigures (c) and (d) show only one second of channels Cz and L from the same segment. The superimposed ERP can be devised enclosed by the vertical bars, around 31.5s, where in (d) the peak is slightly bigger. Figure 7.6 shows the obtained ensemble average ERPs as result of superimposing the template signal into the EEG stream, time-locked to the stimulus onset. These 12 point-to-point averaged segments correspond to the first trial of the EEG stream.

The following experiments are conducted with this dataset.

- Experiment 1 - Letter Identification Performance: the letter identification performance of each one of these methods on the artificially generated pseudo-real dataset.
- Experiment 2 - Latency Noise: Instead of superimposing the P300 ERP over the EEG trace at the exact locations where stimulus onsets are situated, an artificial latency lag is added. The lagging value is picked from a uniform distribution $U(0, 0.4)$ [s] ranging from 0 to 0.4 of the 1s segment size [28].
- Experiment 3 - Component Amplitude Noise: the amplitude of the main P3b component of the ERP template is randomly altered. This component is defined to be located from the stimulus onset between 148 ms up to 996 ms which is around 840 ms long. This waveform element, multiplied by a gain factor, is subtracted from the original template. This gain factor between 0 and 1 is drawn from a uniform distribution

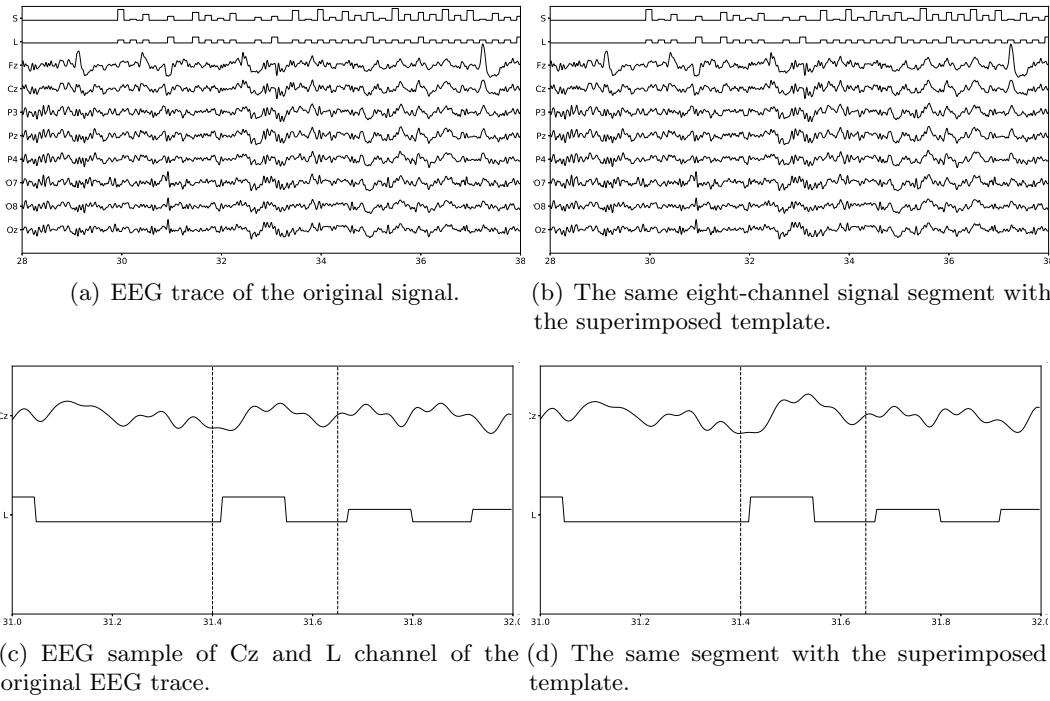


Figure 7.5: Eight-channel EEG signal without and with the superimposed ERP Template. The channel L, the mark which identifies where to superimpose the P300 ERP, is shown as well as the channel S which identifies the stimulus that was presented. On (c) and (d) the small variation that was introduced by the superimposition of the ERP can be seen enclosed by the vertical bars, where the slope of the bump on subplot (d) is slightly bigger

$U(0, 1)$. Additionally this subtracted waveform is multiplied by a Gaussian window with a support of the same length [48]. This avoids adding any discontinuity into the artificial generated signal.

The classification method Support Vector Machine SVM with a linear kernel, is added for comparison as control using a feature f constructed by normalizing the signal on each channel [65]. This method has been proved efficient in decoding P300 in several BCI Competitions [62].

All these experiments are executed using a Cross-Validation procedure dividing the letter to spell in two sets, preserving the structure of the letter identification trials. Spelling letters are scrambled while the order and group of each intensification sequence is preserved.

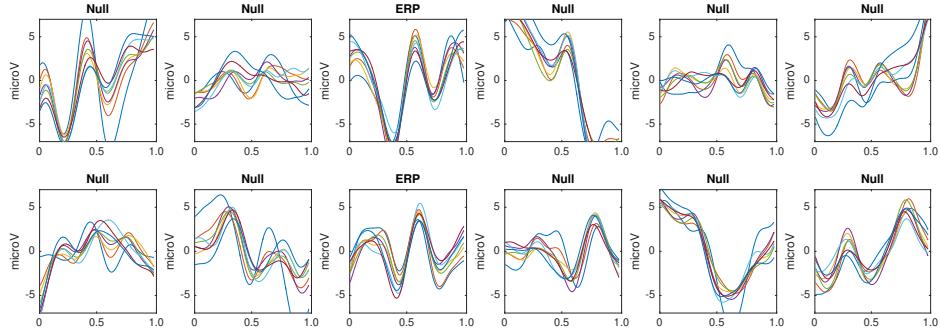


Figure 7.6: Point-to-point averaged signals for the first letter identification trial. The ERP is superimposed on classes 3 and 9. Class 3 is obtained while averaging the segments where the row of the speller matrix is intensified whereas class 9 is calculated from the intensification of the corresponding column.

P300 Dataset IIb BCI Competition II (2003)

Finally the performance at letter identifications for the method proposed on this Thesis and the other similar methods described in 2.8.2 is evaluated by performing an offline BCI Simulation on the Dataset IIb of the BCI Competition II (2003) [10]. The protocol of this dataset is very similar to what was used to obtain the pseudo-real dataset. The sampling frequency of this dataset is 240, the number of letters are 73 where the first 42 are used to create the template dictionary for all the methods and the remaining 31 are used to test the character recognition rate performance. Additionally, in this dataset the number of available intensification number sequences k_a is 15.

Parameters

The P300 event can have a span λ of 400 ms and its peak-to-peak amplitude $\Delta\mu V$ can reach $10\mu V$ [94]. Hence it is necessary to utilize a signal segment of size $w = 1$ second. In order to compute the patch parameters, Equations 4.5 and 4.6 are used to determine the value of 3 for the horizontal patch scale S_t as well as the vertical patch scale S_v .

As the peak-to-peak amplitude is small, to have a better resolution, the amplitude scales parameter are selected to be $\gamma = 4$, and $\gamma_t = 4$. With this configuration, the local patch and the descriptor can identify events of $9 \mu V$ of amplitude, with a span of $\lambda = 0.56$ seconds. This also determines that 1 pixel represents $\frac{1}{\gamma} = \frac{1}{4}\mu V$ on the vertical direction, and $\frac{1}{F_s \gamma} = \frac{1}{64}$ seconds on the horizontal direction. The keypoints **kp** are located

at $(x_{k_p}, y_{k_p}) = (0.55F_s \gamma, z^l(c)) = (35, z^l(c))$ for the corresponding channel c and location l (see Equation 3.11). In this way the whole transient event is captured.

Lastly, the number of channels C is equal to 8 for the first three datasets and the number of intensification sequences k_a is fixed to 10. The parameter k used to construct the set $N_T(\mathbf{d}^{(l,c)})$ is assigned to $k = 7$, which was found empirically to achieve better results. In addition, the norm used on Equations 7.2 and 7.3 is the cosine norm, and descriptors are normalized to $[-1, 1]$.

7.3 Results

Table 7.1 shows the results of applying the Histogram of Gradient Orientations (HIST) algorithm to the subjects of the public dataset of ALS patients. The percentage of correctly spelled letters is calculated while performing an offline BCI Simulation. From the seven words for each subject, the first three are used for calibration, and the remaining four are used for testing. The best performing channel bpc is informed as well. The target ratio is 1 : 36; hence theoretical chance level is 2.8%. It can be observed that the best performance of the letter identification method is reached in a dissimilar channel depending on the subject being studied. Table 7.1 and 7.2 show for comparison the obtained performance rates using single-channel signals with the Support Vector Machine (SVM) [102] classifier. This method is configured to use a linear kernel. The best performing channel bpc , where the best letter identification rate was achieved, is also depicted.

Table 7.1: Character recognition rates for the public dataset of ALS patients using the Histogram of Gradient (HIST) calculated from single-channel plots. Performance rates using single-channel signals with the SVM classifier are shown for comparison. The best performing channel bpc for each method is visualized

Participant		bpc	HIST	bpc	Single Channel SVM
1		Cz	35%	Cz	15%
2		Fz	85%	PO8	25%
3		Cz	25%	Fz	5%
4		PO8	55%	Oz	5%
5		PO7	40%	P3	25%
6		PO7	60%	PO8	20%
7		PO8	80%	Fz	30%
8		PO7	95%	PO7	85%

The Information Transfer Rate (ITR), or Bit Transfer Rate (BTR), in the case of reactive

Table 7.2: Character recognition rates for the own dataset of healthy subjects using the Histogram of Gradient (HIST) calculated from single-channel plots. Performance rates using single-channel signals with the SVM classifier are shown for comparison. The best performing channel *bpC* for each method is visualized.

Participant	<i>bpC</i>	HIST	<i>bpC</i>	Single Channel SVM
1	Oz	40%	Cz	10%
2	PO7	30%	Cz	5%
3	P4	40%	P3	10%
4	P4	45%	P4	35%
5	P4	60%	P3	10%
6	Pz	50%	P4	25%
7	PO7	70%	P3	30%
8	P4	50%	PO7	10%

BCIs [126] depends on the amount of signal averaging required to transmit a valid and robust selection. Figure 7.7 shows the performance curves for varying intensification sequences for the subjects included in the dataset of ALS patients. It can be noticed that the percentage of correctly identified letters depends on the number of intensification sequences that are used to obtain the averaged signal. Moreover, when the number of intensification sequences tend to 1, which corresponds to single-intensification character recognition, the performance is reduced. As mentioned before, the SNR of the P300 obtained from only one segment of the intensification sequence is very low and the shape of its P300 component is not very well defined.

In Table 7.2 the results obtained for 8 healthy subjects are shown. It can be observed that the performance is above chance level. It was verified that HIST method has an improved performance at letter identification than SVM that process the signals on a channel by channel strategy (Wilcoxon signed-rank test, $p = 0.004$ for both datasets).

Tables 7.3 and 7.4 are presented in order to compare the performance of the HIST method versus a multichannel version of the Stepwise Linear Discriminant Analysis (SWLDA) and SVM classification algorithms for both datasets. The feature was formed by concatenating all the channels [65]. SWLDA is the methodology proposed by the ALS dataset's publisher. Since authors [96] did not report the Character Recognition Rate obtained for this dataset, we replicate their procedure and include the performance obtained with the SWLDA algorithm at letter identification. As can be observed in Figure 7.8, It was verified for the dataset of ALS patients that it has similar performance against other methods like SWLDA or SVM, which use a multichannel feature (Quade test with $p = 0.55$) whereas for the dataset of

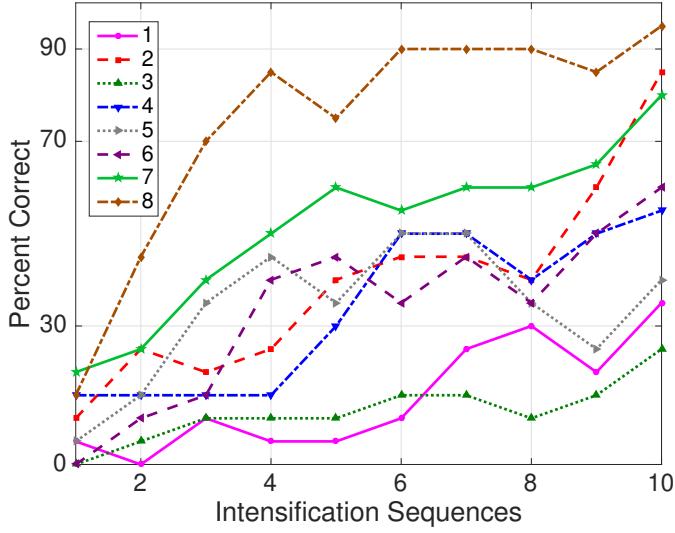


Figure 7.7: Performance curves for the eight subjects included in the dataset of ALS patients. Three out of eight subjects achieved the necessary performance to implement a valid P300 speller.

Table 7.3: Character recognition rates and the best performing channel bpc for the public dataset of ALS patients using the Histogram of Gradient (HIST) (repeated here for comparison purposes). Performance rates obtained by SWLDA and SVM classification algorithms with a multichannel concatenated feature.

Participant	bpc for HIST	HIST	Multichannel SWLDA	Multichannel SVM
1	Cz	35%	45%	40%
2	Fz	85%	30%	50%
3	Cz	25%	65%	55%
4	PO8	55%	40%	50%
5	PO7	40%	35%	45%
6	PO7	60%	35%	70%
7	PO8	80%	60%	35%
8	PO7	95%	90%	95%

healthy subjects significant differences were found (Quade test with $p = 0.02$) where only the HIST method achieved a different performance than SVM (with multiple comparisons, significant difference of level 0.05).

The P300 ERP consists of two overlapping components: the P3a and P3b, the former with frontocentral distribution while the later stronger on centroparietal region [89]. Hence, the standard practice is to find the stronger response on the central channel Cz [96]. However,

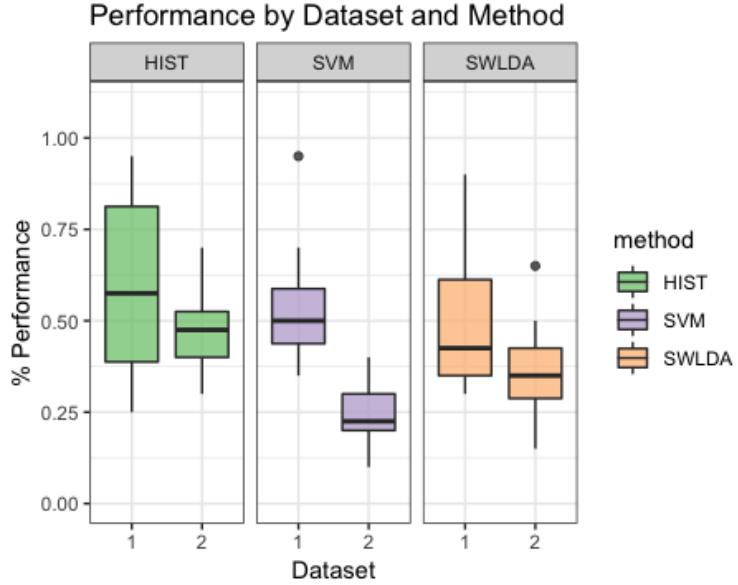


Figure 7.8: Obtained boxplots for the given algorithms.

Table 7.4: Character recognition rates and the best performing channel *bpc* for the own dataset of healthy subjects using the Histogram of Gradient (HIST) (repeated here for comparison purposes). Performance rates obtained by SWLDA and SVM classification algorithms with a multichannel concatenated feature.

Participant	<i>bpc</i> for HIST	HIST	Multichannel SWLDA	Multichannel SVM
1	Oz	40%	65%	40%
2	PO7	30%	15%	10%
3	P4	40%	50%	25%
4	P4	45%	40%	20%
5	P4	60%	30%	20%
6	Pz	50%	35%	30%
7	PO7	70%	25%	30%
8	P4	50%	35%	20%

[65] show that the response may also arise in occipital regions. We found that by analyzing only the waveforms, occipital channels PO8 and PO7 show higher performances for some subjects.

As subjects have varying *latencies* and *amplitudes* of their P300 components, they also have a varying stability of the *shape* of the generated ERP [78]. Figure 7.9 shows 10 sample P300 templates patches for patients 8 and 3 from the dataset of ALS patients. It can be discerned that in coincidence with the performance results, the P300 signature is more clear

and consistent for subject 8 (A) while for subject 3 (B) the characteristic pattern is more difficult to perceive.

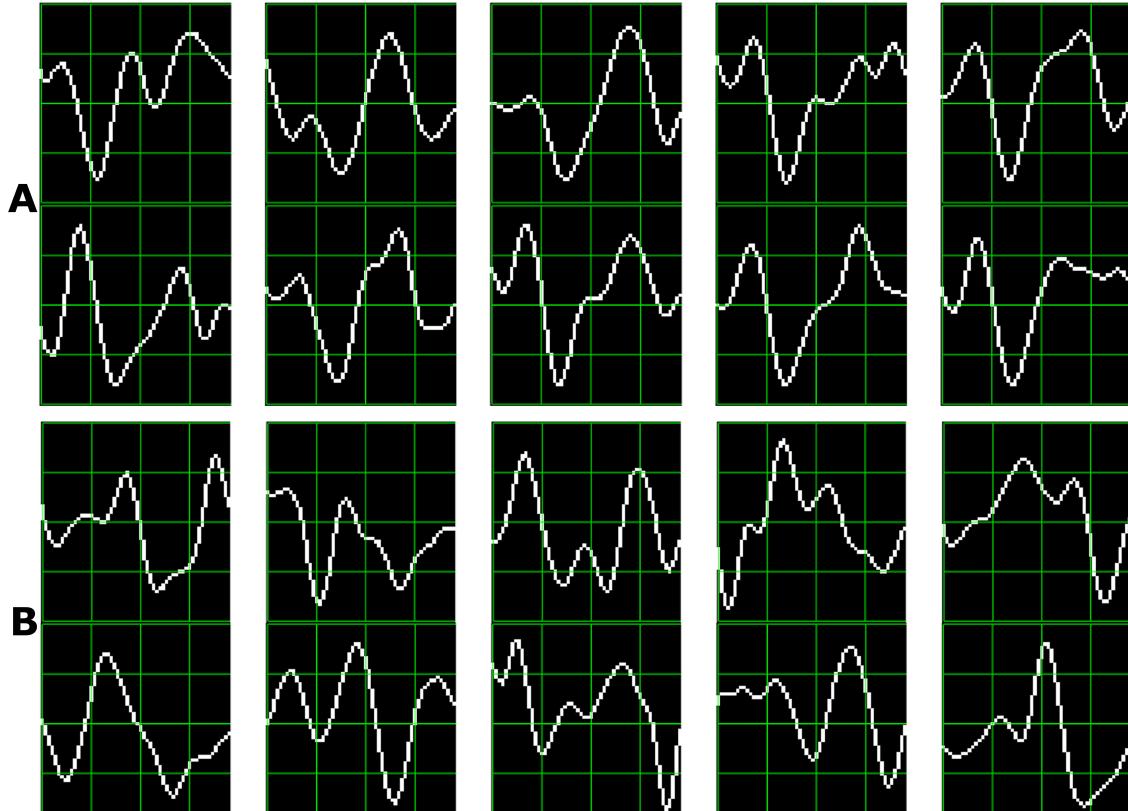


Figure 7.9: Ten sample P300 template patches for subjects 8 (A) and 3 (B) of the ALS Dataset. Downward deflection is positive polarity.

Additionally, the stability of the P300 component waveform has been extensively studied in patients with ALS [104, 73, 81, 74, 76] where it was found that these patients have a stable P300 component, which were also sustained across different sessions. In line with these results we do not find evidence of a difference in terms of the performance obtained by analyzing the waveforms (HIST) for the group of patients with ALS and the healthy group of volunteers (Mann-Whitney U Test, $p = 0.46$). Particularly, the best performance is obtained for a subject from the ALS dataset for which, based on visual observation, the shape of they P300 component is consistently identified.

It is important to remark that when applied to binary images obtained from signal plots, the feature extraction method described in Section 4.2 generates sparse descriptors. Under this subspace we found that using the cosine metric yielded a significant performance improvement. On the other hand, the unary classification scheme based on the NBNN

algorithm proved very beneficial for the P300 Speller Matrix. This is due to the fact that this approach solves the unbalance dataset problem which is inherent to the oddball paradigm [113].

Regarding Experiments 1,2 and 3 for the third Dataset, results are shown in Table 7.5 and in Figure 7.10, 7.11 and 7.12. Table 7.5 shows the performance while identifying each letter of the standard P300 Speller Matrix, and the *bpc*, the channel where the best performance is attained. Figure 7.10 shows the performance curves for six algorithms under comparison. Each one represents the percentage of letters that is actually predicted by the algorithms using a cross-validation procedure. As previously described the data is continuously divided in two sets, where the first 15 letters are used to derive the dictionary of templates while the remaining 20 letters are used to measure the letter identification performance. This is repeated one hundred times, and performances averaged. Figure 7.11 shows the same results for the Experiment 2, where a noisy latency lag was included. Finally, Figure 7.12 represents the performance values obtained for the Experiment 3, when the amplitude of the P3b component of the template is randomly attenuated.

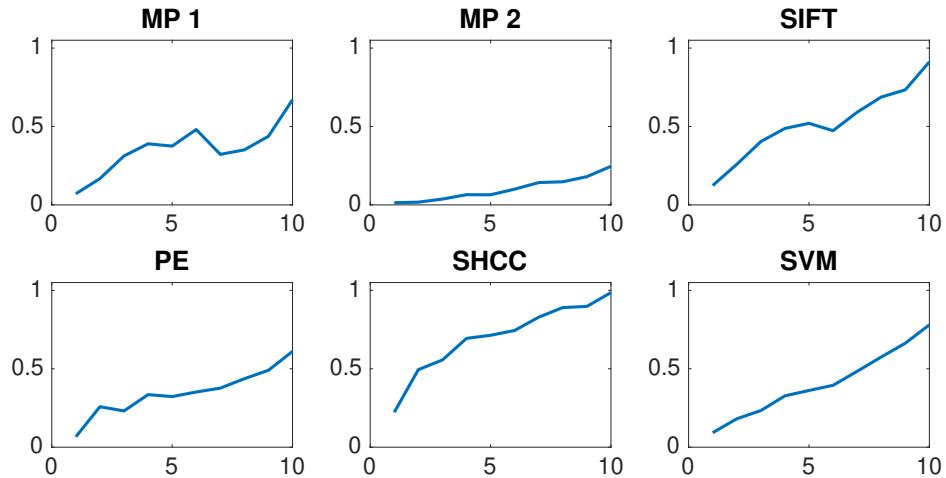


Figure 7.10: Speller performance obtained for each method for the Experiment 1. Y-axis shows performance accuracy while X-axis shows the number of intensification sequences used to calculate the point-to-point signal average.

Finally, results obtained for the dataset BCI Competition 2003 IIb are shown in Figures 7.13 and in Table 7.6. For this experiment the number of available intensification sequences is 15.

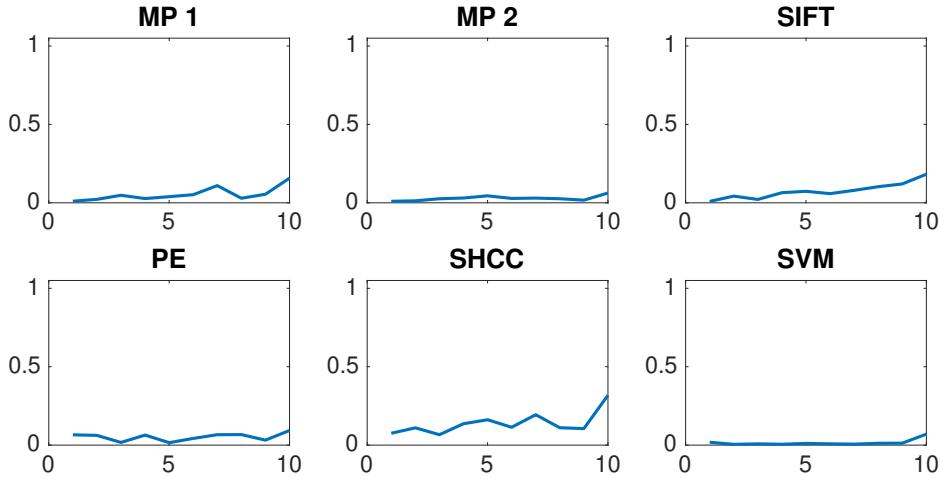


Figure 7.11: Speller performance obtained for each method while latencies are artificially added to each single-intensification segment corresponding to the Experiment 2. The achieved performance is significantly reduced for all methods. Y-axis shows letter identification performance while X-axis shows the number of intensification sequences used to calculate the ensemble average.

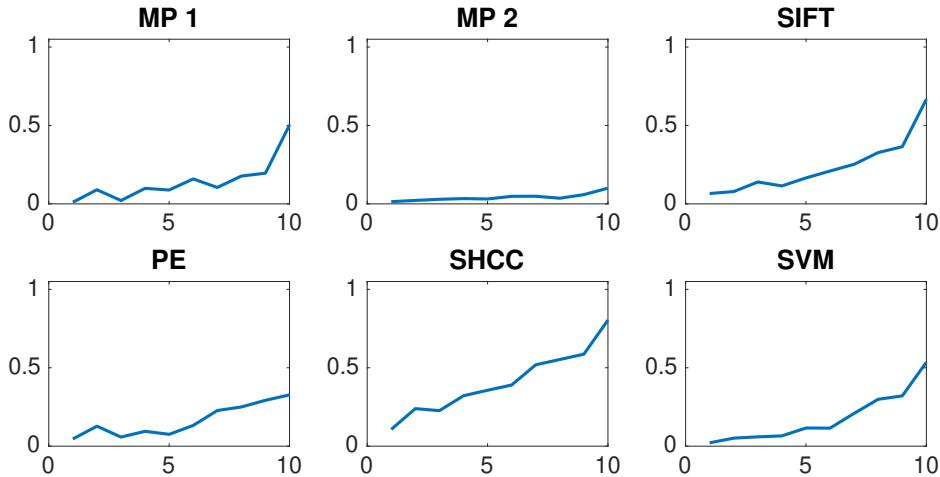


Figure 7.12: Speller performance obtained for the Experiment 3 while the amplitudes of the P3b component of the superimposed ERP is randomly reduced. Y-axis shows performance accuracy while X-axis shows the number of intensification sequences.

7.4 Conclusion

The usage of the Histogram of Gradient Orientations to implement a valid P300-Based BCI Speller application is expounded. Additionally, its validity is evaluated using a public dataset

Table 7.5: Speller classification performance obtained for all the waveform-based algorithms: MP Matching Pursuit, SIFT Scale Invariant Feature Transform, PE Permutation Entropy and SHCC Slope Horizontal Code Chain. Additionally, the control algorithm SVM Support Vector Machines is included for comparison. All the methods process the signal on a channel-by-channel basis, hence the best performing channel is also shown. In this case with absence of null-signals, it can be interpreted as the channel that adds less noise to the ERP template. All the methods used 10 intensification sequences to coherently average the trials to obtain the averaged signal.

Method	Channel	Performance		
		Experiment 1	Experiment 2	Experiment 3
MP 1	PO8	67%	15%	50%
MP 2	PO7	24%	6%	10%
SIFT	PO8	91%	18%	66%
PE	Cz	61%	9%	32%
SHCC	P4	98%	31%	80%
SVM	PO8	78%	7%	53%

Table 7.6: Speller classification performance obtained for the dataset IIb of the BCI Competition II (2003) for each one of the algorithms using 15 repetitions of intensification sequences. The first 42 trials are used for training to build the template dictionary and the remaining 31 for testing. The channel where the best performance is attained, is also shown.

Method	Channel	Performance
MP 1	FC2	50%
MP 2	CPz	22%
SIFT	Cz	67%
PE	PO8	22%
SHCC	Cz	61%
SVM	C1	32%

of ALS patients and an own dataset of healthy subjects. The method is compared against other approaches based on a shared similar idea and the results are presented. Finally, the method is used on a public dataset of a BCI Competition.

It is verified that this method has an improved performance at letter identification than other methods that process the signals on a channel by channel strategy, and it even has a comparable performance against other methods like SWLDA or SVM, which uses a multichannel feature. Furthermore, this method has the advantage that shapes of waveforms can be analyzed in an objective way. We observed that the shape of the P300 component is more stable in occipital channels, where the performance for identifying letters is higher. We additionally verified that ALS P300 signatures are stable in comparison to those of healthy

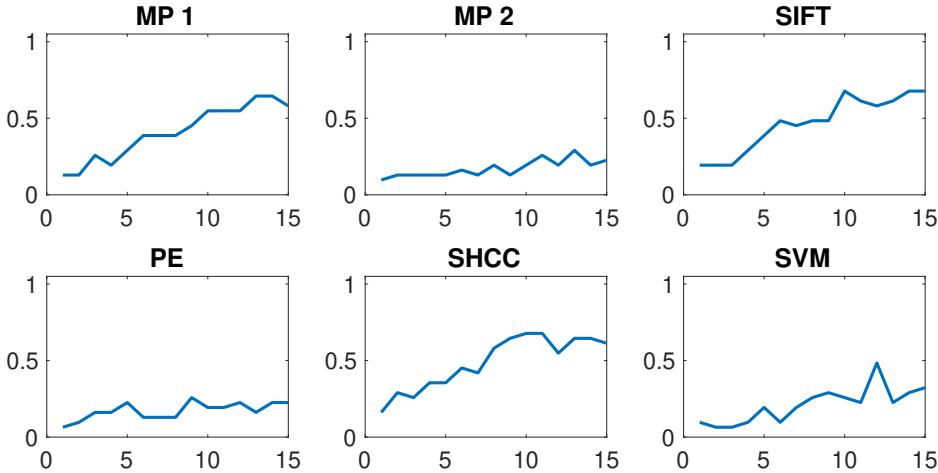


Figure 7.13: Speller performance obtained for the Dataset IIb of the BCI Competition II (2003) for each one of the algorithms. An offline BCI Simulation is performed using the first 42 trials as training and the remaining 31 as testing. The horizontal axis show the number of intensification sequences, from 0 to 15 for this dataset, while the vertical axis show the performance rate.

subjects.

We believe that the use of descriptors based on histogram of gradient orientation, presented in this work, can also be utilized for deriving a shape metric in the space of the P300 signals which can complement other metrics based on time-domain as those defined by [74]. It is important to notice that the analysis of waveform shapes is usually performed in a qualitative approach based on visual inspection [104], and a complementary methodology which offer a quantitative metric will be beneficial to these routinely analysis of the waveform of ERPs.

The goal of this Chapter is to answer the question if a P300 component could be solely determined by inspecting automatically their waveforms. We conclude affirmatively, though two very important issues still remain:

First, the stability of the P300 in terms of its shape is crucial: the averaging procedure, montages, the signal to noise ratio and spatial filters all of them are non-physiological factors that affect the stability of the shape of the P300 ERP. We tested a preliminary approach to assess if the morphological shape of the P300 of the averaged signal can be stabilized by applying different alignments of the stacked segments (see Figure 7.2) and we verified that there is a better performance when a correct segment alignment is applied. We applied Dynamic Time Warping (DTW) [19] to automate the alignment procedure but we were

unable to find a substantial improvement. Further work to study the stability of the shape of the P300 signature component needs to be addressed.

The second problem is the amplitude variation of the P300. We propose a solution by standardizing the signal, shown in Equation 3.9. It has the effect of normalizing the peak-to-peak amplitude, moderating its variation. It has also the advantage of reducing noise that was not reduced by the averaging procedure. It is important to remark that the averaged signal variance depends on the number of segments used to compute it [118]. The standardizing process converts the signal to unit signal variance which makes it independent of the number k_a of signals averaged. Although this is initially an advantageous approach, the standardizing process reduces the amplitude of any significant P300 complex diminishing its automatic interpretation capability.

Considering other methods inspired on the same idea, we verified that similar performance results are obtained for the methods *SHCC*, *SIFT* and *MP-1* and that it is also possible to obtain discriminating information from the underlying signal based exclusively on an automated method of processing the waveforms. Moreover, the possibilities of finding overcomplete dictionaries for matching pursuit sparse representation based on obtained signal templates, could also be considered an area of future improvement [42].

Chapter 8

Epilogue

In the first Chapter, the following question was posed: is it possible to analyze and discriminate Electroencephalographic signals by automatic processing the shape of the waveforms using the Histogram of Gradient Orientations ?

We conclude affirmatively, and remark the following points:

- EEG Waveforms can be analyzed by this method.
- Oscillatory processes can be studied by the shape of the plots.
- The stability of ERP components can be studied objectively with HIST.

The scientific or technological endeavor has been enlightened many times by the connection of initially unrelated topics. At the conclusion of this work, we have the feeling that there are many potential benefits from the application of this technique and that there are many areas that could be improved from this work and extensions. This is the topic of this last, final, and conclusive, Chapter.

8.1 Conclusion

Among other applications of Brain Computer Interfaces, the goal of the discipline is to provide communication assistance to people affected by neuro-degenerative diseases, who are the most likely population to benefit from BCI systems and EEG processing and analysis [126].

A method to analyze EEG signals based on the waveform characterization, is presented. The proposed procedure transforms the signal into an image, plots the signal on it, and analyzes their local structure using the Histogram of Gradient Orientations. Aiming to offer

a BCI implementation, this technique is adapted to perform a feature extraction procedure. Finally an additional classification scheme is outlined.

This method is verified on EEG oscillatory processes. An experiment with ten subjects and using a commercial-grade device, is conducted. The application of the method effectively detects Alpha Waves from signals, differentiating two mental states. It is also proved on a public dataset. The prevalence of these signals in occipital areas is determined by a higher accuracy obtained for those brain regions.

The applicability of the method is extended to study transient signals, particularly the P300 ERP, due to their importance, and widespread adoption in BCI. Moreover, a method to extract the ERP waveform is expounded and used to recognize it from EEG signals by analyzing their waveform shape. An additional experiment on eight healthy subjects is performed but using a research-grade EEG device, specifically designed for this discipline. The procedure is tested against the produced dataset and, a usable level of accuracy is obtained. A BCI simulation is also implemented against a public dataset of ALS patients where it is verified that the waveform of the P300 is stable regardless of the health condition, offering an alternative method to study waveform stability. A pseudo-real dataset is created to test and control for regular issues with ERP extraction procedures and the method proposed here is additionally contrasted against a set of other four alternative methods which are inspired in analyzing EEG waveforms. It is found that this method achieved higher or equal performance values than the other methods.

This technique has the following benefits,

1. Universal Applicability
2. Objective Waveform Metric
3. Foster clinical interaction.
4. Clinical-Tool Making
5. Intelligible Property and BCI Reliability

Universal Applicability The Histogram of Gradient Orientation method has a potential universal applicability, because the same basic methodology can be applied to detect different patterns in EEG signals with applications to BCI. The search for meaningful or cognitive waveforms, or *cognemes* is a very important issue in BCI, Neuroscience Research and

Neurophysiology. Automatic classification of patterns in EEG that are specifically identified by their shapes like K-Complex, Vertex Waves, Positive Occipital Sharp Transient [107] are a prospect future work to be considered.

Objective Waveform Metric Descriptors are a direct representation of the shape of signal waveforms. Hence, they can be used to build databases of quantitative descriptions of known waveforms and improve atlases, which are currently based on qualitative descriptions of signal shapes.

Foster clinical collaboration In our opinion, the best benefit of the presented method is that a closer collaboration of the field of BCI with physicians can be fostered, since this procedure intent to imitate human visual observation. After all analyzing waveforms by their waveform shapes is a established procedure of the clinical EEG community. One of the main goals of the BCI discipline is to provide assistance to patients and to provide alternative tools to be used in diagnostics and rehabilitation procedure. This requires a clinical focus which is often neglected in BCI research.

Clinical tool-making The method presented in this thesis offers the ability to identify waveforms shapes in an exhaustive manner. This can eventually provide assistance to physicians to localize EEG patterns, specially in long recordings periods, frequent in clinical sleep studies or Neonatal ICU. Additionally, it can be used for artifact removal which is performed on many occasions by visually inspecting signals.

Intelligible Property and BCI Reliability BCI reliability is yet an unfulfilled goal in this discipline [126]. The convenience of analyzing or including metrics about the shape of the EEG, is that clinical EEG diagnosis may support a vast set of already understood knowledge which is based on identifying EEG patterns by their shape and that can steer towards a more robust implementation of BCI devices.

Moreover, this conventional clinical method of observing the waveform is understood to be subjective and laborious because results depend on the technicians' experience and expertise. At the same time, it is a subjective time-consuming task, with long-learning curves, requires specialized personnel, and it has significant error rates [114]. These problems has pushed for the adoption of more automated means of decoding the signals [111]. This trend pointed to the initial development of quantitative EEG, which however didn't replaced clinically the traditional approach which is still widespread: the Gold standard in clinical EEG is still *Eye Ball* [127, 114].

We believe that the adoption of a *hybrid* methodology which can process the signal

automatically, but at the same time, maintains an inherent intelligible property [13] that can be mapped to existing procedures, and above all, can maintain the clinician trust on the system behavior, is beneficial to Clinical Practice, Neuroscience and BCI research.

8.2 Future Work

Regarding future work, there are potential areas that could be improved upon the presented methodology:

1. Multichannel extension
2. Scale space analysis on EEG for keypoint localization
3. Neuroimaging
4. Ensemble classifiers
5. Computer vision interdisciplinary work
6. Other areas

Multichannel extension The methods described in section 2.8.2 and the one proposed here analyze the waveform of a single channel. The nature of the proposal is to analyze the shape of single waveforms obtained from just one channel. However, for automatic interpretation of the signal it is known that multichannel extension is necessary. Hence, a multichannel extension should likely be beneficial to the usage of the proposed methodology [42].

Scale space analysis of EEG for keypoint localization This work focused on the waveform representation but another important area is waveform detection. The theory of Scale Space developed for the SIFT Detector is an important area for future study that has not been explored thoughtfully in the EEG or BCI literature.

Neuroimaging Many tools for Computer Vision are being used in Neuroscience to devise methods to understand brain function. The Histogram of Gradient Orientations can be explored from this same perspective due to their visually relevant nature.

Ensemble classifiers The Histogram of Gradient Orientations method has the advantage that they can map a visual component with a clinical meaning to a feature with an objective representation. Thus, compound classifiers or ensemble of features can be further explored to improve accuracies. Successful approaches in Computer Vision or Pattern

Recognition in other areas use them [27] with a significant enhancement of the classification performances [43].

Computer Vision interdisciplinary work Furthermore, the extensive body of research from Computer Vision on SIFT provides a fruitful path to explore in order to achieve faster and improved algorithms to automatically detect EEG characteristics which are suitable for classification. Other image processing feature extraction methods like SURF, GLOH, RANSAC could also be considered.

Other areas The HIST method, after all, is solely analyzing waveforms, so they can be explored in other disciplines where the structure or shape of the waveform is of relevance. Analyzing signals by their waveforms is relative common in chemical analysis [106], seismic analysis in Geology [85], and quantitative financial analysis. Electrocardiogram EKG, on the other hand, has been extensively processed and studied analyzing the waveform structure [109].

Appendix A

BCI en Argentina

El propósito de este apéndice es ofrecer información del estado de esta disciplina en Argentina. La inevitable omisión de trabajos o grupos específicos de ninguna manera ha sido adrede, y se solicita las pertinentes disculpas. Este relevamiento fue realizado durante el transcurso del desarrollo de esta tesis, y probablemente tenga una visión desde el mundo de las Ingenierías, lo cual es un sesgado abordaje en esta tremadamente interdisciplinaria disciplina.

Los pioneros en Argentina son los trabajos en la Universidad de La Plata, y los trabajos de la UNER. Estos últimos desarrollaron en el 2006 las primeras Jornadas Argentinas sobre Interfaces Cerebro-Computadora y las replicaron en el JAICC 2009.

- UNER, Faculta de Ingeniería, LIRINS,(Oro Verde) Bioingeniería Dr. Gerardo Gentilleti
 - <http://cortex.loria.fr/Projects/STIC-AmSud-BCI>,
 - http://www.bioingenieria.edu.ar/postgrado/index.php?option=com_content&view=category&id=72&Itemid=61
 - Otros investigadores: Guerenstein, Pablo; Carolina B. Tabernig (BCI-FES system for neuro-rehabilitation of stroke patients [LINK](#))
- FRN: Fundación Rosarina de Neuro-Rehabilitación, Medicina y Rehabilitación, Dr. Carlos Ballario
 - BCI-FES
 - Stroke Neurorehabilitation
 - Trabajan con la Empresa Interactive Dynamics.

- UBA, Facultad de Ingeniería, Laboratorio de Sergio Lew (<http://www.fi.uba.ar/es/node/1442>) , "Instituto de Ingeniería Biomédicas" / Dr. Sergio Lew
 - BCI Invasivo principalmente (trabajan cerca de Zanutto).
- UBA, Ingeniería, Laboratorio de Sistemas Inteligentes Dr. Jorge Ierache <http://laboratorios.fi.uba.ar/lsi/>.
 - Control de robots por bioseñales, detección de emociones.
- UBA, Exactas, <https://liaa.dc.uba.ar/> Applied Artificial Intelligence Lab Dr. Agustín Gravano / Dr. Diego Fernandez Slezak
 - Tesis de grado Arneodo.
 - Otros investigadores: Alejandro Sabatini
- INAUT, Instituto Nacional de Automática, San Juan, / Dr. Carlos Soria, Dr. Eugenio Orosco BCI Robótica (BCI híbridos, robótica asistiva) Trabajan con Teodiano Freire Bastos en Brasil www.ncbi.nlm.nih.gov Otros investigadores: Mst. Ing. Fernando Auat Cheeín E-mail: fauat@inaut.unsj.edu.ar
- Instituto Argentino de Matemáticas Alberto Calderon / Bioing. Sergio Liberczuk, Dr. Bruno Cernuschi Frías Matemáticas y modelado del problema inverso.
- ITBA, / CiC del Dr Juan Santos, <http://www.itba.edu.ar/es/id/centros/cic-centro-de-inteligencia-computacional> Proyecto Doctorado Robótica Asistiva BCI Neurorehabilitación, Rodrigo Ramele http://www.unsam.edu.ar/tss/controlar-maquinas-con-el-pensamiento/978-3-319-13117-7_142
- UNC, Universidad Nacional de Córdoba Trabajo Final de Ingeniería: <http://www.electronicosonline.com/2013/07/08/crean-jovenes-argentinos-interface-cerebral-para-discap> Carrera de Ingeniería Biomédica: Ing. Diego Beltramone
- UNLP, LEICI / Dr. Enrique Spinelli (<http://www.ing.unlp.edu.ar/leici/esp/pspinelli.html>) Electrónica. Tesis de Grado de García Pablo: <http://sedici.unlp.edu.ar/handle/10915/3800631605> Tesis de Maestría de Andrea Noelia Bermudez Cicchino 31605 Cesar Caiafa (trabajó con Cichocki) <http://ccaiafa.wixsite.com/cesar>

- Universidad Nacional de Tucuman, Instituto Superior de Investigaciones Biológicas (INSIBIO) www.lamein.org Investigación sobre alternativas de codificación neural de los sistemas sensoriales. Investigadores responsables: Dr. Carmelo Felice, Mst. Ing. Fernando Farfán E-mail: cfelice@herrera.unt.edu.ar, ffarfan@herrera.unt.edu.ar
- Laboratorio de Investigación y Desarrollo en Nuevas Tecnologías (LIDeNTec) - ANSES Desarrollo de BCI Investigadores responsables: Dr. Mario Mastriani E-mail: mmastri@gmail.com
- INECO: Cercanía con BCI pero no parece ser el foco de lo que hacen. Eugenia Hesse Agustín Ibañez
- IBCN Silvia Kochen http://www.ibcn.fmed.uba.ar/200_grupos-lab-epilepsia-kochen.html
- Instituto Ferrero de Neurología y Sueño. Fundación Argentina de Estudio del Cerebro. Publicaron un excelente libro en castellano de *Análisis Computado de EEG*.

Appendix B

Walkthrough BCI

Hjorth Parameters

Fractal Dimension

AR Modelling

AAR Modelling

Spatial Filtering

EEG based on Bayesian Learning

Trade-off between resolution, range and storage capacity.

range min-max Resolution Range / bitrange

Quantization noise: due to the rounding or truncation which is performed in an ADC converter.

Layers

Skin: 1mm Fat: 2 mm Skull: 7 mm Dura: 1mm CSF: 2mm Brain: 40 mm

Patients suffering from ALS degeneration of nerve cell that control voluntary muscles.

Severe cerebral palsy is a non-progressive but not unchanging, disorder of movement and posture that is the consequence of lesions or anomalies of the brain arising in the early stages of its development

MDN, Motor neuron disease actually describes a group of very similar conditions that affect motor neurons. ALS is the most common type upper motor neurons (brain spinal cord) lower motor neurons (spinal cord to muscles).

Lou Gehrig's disease in the US, MND in the UK

SCI spinal cord injury less than 5 percent recover locomotion

Brain Stem stroke fatal can derive in locked-in state.

bci for assistive technologies book

Appendix C

SIFT

The history of Scale Space tracks back to Witkin 1983, where it was applied to time series. He highlighted the Spatial Coincidental assumption. Basically, the number of zero crossing of the first derivative is reduced with increasing scale.

Biomimetic Applications

This method is actually composed on two submethods: the first is the keypoint localization, while the second is the histogram of gradient orientations, which is the basis for this thesis.

bla bla bla

Aca tambien voy a mandar detalles de la implementacion. como por ejemplo los detalles de como funciona vlfeat y las modificaciones.

- <https://bitbucket.org/itba/hist>
- <https://github.com/faturita/BciVisualToolbox>
- <https://github.com/faturita/vlfeat>
- <https://github.com/faturita/GuessMe>

Datasets

- P300-Dataset <https://www.kaggle.com/rramele/p300samplingdataset>, Registered as public scientific resource in the public Database SciCrunch, RRID: SCR_015977.
- P300 Template (routput.mat) and P300-null signal subject (P300-Subject-21.mat) at the CodeBase Repository <https://goo.gl/MzNNkn>.

Blogs

- The following blog was maintained during the development of this Thesis: <http://monostuff.logdown.com/>.

Appendix D

Negative Results

This is a list of noncurated things that we tested and didnt work.

D.1 Keypoint location

Keypoint location using the SIFT Detector.

The reason being there are two many descriptors that are generated and the important regions on the image are not salient in terms of angles per se.

Esto provoco que nos inclinacemos a eventos de BCI sincronicos.

D.2 Classification algorithms

El esquema natural con siftmatch y con el BagOfWords. RootSIFT

NBNN funcional barbero como algoritmo, y tambien el uso de la distancia coseno.

Varinates pesadas. Clasificacion binaria. SMOTE. MAD para el averaging. DTW para mejorar la sincronización.

Bibliography

- [1] Minkyu Ahn, Hohyun Cho, Sangtae Ahn, and Sung Chan Jun, *High theta and low alpha powers may be indicative of BCI-illiteracy in motor imagery*, PloS one **8** (2013), no. 11, 1–11.
- [2] A. Bolu Ajiboye, Francis R. Willett, Daniel R. Young, William D. Memberg, Brian A. Murphy, Jonathan P. Miller, Benjamin L. Walter, Jennifer A. Sweet, Harry A. Hoyer, Michael W. Keith, P. Hunter Peckham, John D. Simeral, John P. Donoghue, Leigh R. Hochberg, and Robert F. Kirsch, *Restoration of reaching and grasping movements through brain-controlled muscle stimulation in a person with tetraplegia: a proof-of-concept demonstration*, The Lancet **389** (2017), no. 10081, 1821–1830.
- [3] Brendan Z. Allison, Stephen Dunne, Robert Leeb, José Del R. Millán, and Anton Nijholt (eds.), *Towards Practical Brain-Computer Interfaces*, Biological and Medical Physics, Biomedical Engineering, Springer Berlin Heidelberg, Berlin, Heidelberg, 2013.
- [4] Montserrat Alvarado-González, Edgar Garduño, Ernesto Bribiesca, Oscar Yáñez-Suárez, and Verónica Medina-Bañuelos, *P300 Detection Based on EEG Shape Features*, Computational and Mathematical Methods in Medicine **2016** (2016), 1–14.
- [5] Kai Keng Ang, Cuntai Guan, Karen Sui Geok Chua, Beng Ti Ang, Christopher Wee Keong Kuah, Chuanchu Wang, Kok Soon Phua, Zheng Yang Chin, and Haihong Zhang, *A large clinical study on the ability of stroke patients to use an EEG-based motor imagery brain-computer interface*, Clinical EEG and Neuroscience **42** (2011), no. 4, 253–258.
- [6] Jitka Annen, Séverine Blandiaux, Nicolas Lejeune, Mohamed A. Bahri, Aurore Thibaut, Woosang Cho, Christoph Guger, Camille Chatelle, and Steven Laureys, *BCI performance and brain metabolism profile in severely brain-injured patients without response to command at bedside*, Frontiers in Neuroscience **12** (2018), no. 6, 370.
- [7] Erol Başar, *A review of alpha activity in integrative brain function: Fundamental physiology, sensory coding, cognition and pathology*, International Journal of Psychophysiology **86** (2012), no. 1, 1–24.
- [8] Christoph Bandt and Bernd Pompe, *Permutation Entropy: A Natural Complexity Measure for Time Series*, Physical Review Letters **88** (2002), no. 17, 1–17.
- [9] Sebastian Berger, Gerhard Schneider, Eberhard F Kochs, and Denis Jordan, *Permutation entropy: Too complex a measure for EEG time series?*, Entropy **19** (2017), no. 12, 1–20.
- [10] B Blankertz, *Documentation second wadsworth BCI dataset P300 evoked potentials data acquired using BCI2000 P300 Speller Paradigm*, 2002.

- [11] Oren Boiman, Eli Shechtman, and Michal Irani, *In defense of nearest-neighbor based image classification*, 26th IEEE Conference on Computer Vision and Pattern Recognition, CVPR (2008), no. i, 10–18.
- [12] Elena Boto, Niall Holmes, James Leggett, Gillian Roberts, Vishal Shah, Sofie S Meyer, Leonardo Duque Muñoz, Karen J Mullinger, Tim M Tierney, Sven Bestmann, Gareth R Barnes, Richard Bowtell, and Matthew J Brookes, *Moving magnetoencephalography towards real-world applications with a wearable system*, Nature **555** (2018), 657.
- [13] M Bragg, *The Challenge of Crafting Intelligible Intelligence*, ACM Symposium on User Interface Software and Technology, 2018.
- [14] J. E. Bresenham, *Algorithm for computer control of a digital plotter*, IBM Systems Journal **4** (1965), no. 1, 25–30.
- [15] Jeffrey W Britton, Lauren C Frey, Jennifer L Hopp, Pearce Korb, Mohamad Z Koubeissi, William E Lievens, Elia M Pestana-Knight, and Erik K St. Louis, *Electroencephalography (EEG): An Introductory Text and Atlas of Normal and Abnormal Findings in Adults, Children, and Infants*, 2016.
- [16] Clemens Brunner, Benjamin Blankertz, Febo Cincotti, Andrea Kübler, Donatella Mattia, Felip Miralles, Anton Nijholt, and Begonya Otal, *BNCI Horizon 2020 – Towards a Roadmap for Brain / Neural Computer Interaction*, Lecture Notes in Computer Science **8513** (2014), no. 1, 475–486.
- [17] György Buzsáki, Costas A. Anastassiou, and Christof Koch, *The origin of extracellular fields and currents-EEG, ECoG, LFP and spikes*, Nature Reviews Neuroscience **13** (2012), no. 6, 407–420.
- [18] Tom Carlson and Jose del R. Millan, *Brain-Controlled Wheelchairs: A Robotic Architecture*, IEEE Robotics & Automation Magazine **20** (2013), no. 1, 65–73.
- [19] S. Casarotto, A.M. Bianchi, S. Cerutti, and G.A. Chiarenza, *Dynamic time warping in the analysis of event-related potentials*, IEEE Engineering in Medicine and Biology Magazine **24** (2005), no. 1, 68–77.
- [20] S. Chandran KS, A. Mishra, V. Shirhatti, and S. Ray, *Comparison of Matching Pursuit algorithm with other signal processing techniques for computation of the time-frequency power spectrum of brain signals*, Journal of Neuroscience **36** (2016), no. 12, 3399–3408.
- [21] U. Chaudhary, N. Birbaumer, and A. Ramos-Murguialday, *Chapter 5 - brain-computer interfaces in the completely locked-in state and chronic stroke*, Brain-Computer Interfaces: Lab Experiments to Real-World Applications (Damien Coyle, ed.), Progress in Brain Research, vol. 228, Elsevier, 2016, pp. 131 – 161.
- [22] Ricardo Chavarriaga, Melanie Fried-Okne, Sonja Kleih, Fabien Lotte, and Reinhold Scherer, *Heading for new shores! Overcoming pitfalls in BCI design*, Brain-Computer Interfaces **4** (2017), no. 1-2, 60–73.

- [23] Andy Clark, *Supersizing the Mind: Embodiment, Action, and Cognitive Extension*, vol. 66, Philosophy of mind; Philosophy of mind series, no. 7, Oxford University Press, 2008.
- [24] M Clerc, L Bougrain, and F Lotte, *Brain-computer interfaces, Technology and applications 2(Cognitive Science)*, ISTE Ltd. and Wiley, 2016.
- [25] Mike X Cohen, *Analyzing Neural Time Series Data: Theory and Practice*, MIT Press, 2014.
- [26] Scott R. Cole and Bradley Voytek, *Brain Oscillations and the Importance of Waveform Shape*, Trends in Cognitive Sciences **21** (2017), no. 2, 137–149.
- [27] Antonio Criminisi and Jamie Shotton, *Decision forests for computer vision and medical image analysis*, Springer Science & Business Media, 2013.
- [28] P. Da Pelo, M. De Tommaso, A. Monaco, S. Stramaglia, R. Bellotti, and S. Tangaro, *Trial latencies estimation of event-related potentials in EEG by means of genetic algorithms*, Journal of Neural Engineering **15** (2018), no. 2, 026016.
- [29] Navneet Dalal and Bill Triggs, *Histograms of oriented gradients for human detection*, Proceedings - IEEE Computer Society Conference on Computer Vision and Pattern Recognition, CVPR 2005, vol. I, IEEE, 2005, pp. 886–893.
- [30] Maarten De Vos and Stefan Debener, *Mobile eeg: Towards brain activity monitoring during natural action and cognition*, International Journal of Psychophysiology **91** (2014), no. 1, 1–2.
- [31] Stefan Debener, Falk Minow, Reiner Emkes, Katharina Gandras, and Maarten de Vos, *How about taking a low-cost, small, and wireless EEG for a walk?*, Psychophysiology **49** (2012), no. 11, 1617–21.
- [32] Esther Dyson, *Release 2.1: A design for living in the digital age*, 1st ed., Broadway Books, 1998.
- [33] S Edelman, N Intrator, and T Poggio, *Complex cells and object recognition*, Unpublished manuscript (1997), 1–12.
- [34] L. A. Farwell and E. Donchin, *Talking off the top of your head: toward a mental prosthesis utilizing event-related brain potentials*, Electroencephalography and Clinical Neurophysiology **70** (1988), no. 6, 510–523.
- [35] Faranak Farzan, Sravya Atluri, Matthew Frehlich, Prabhjot Dhami, Killian Kleffner, Rae Price, Raymond W. Lam, Benicio N. Frey, Roumen Milev, Arun Ravindran, Mary Pat McAndrews, Willy Wong, Daniel Blumberger, Zafiris J. Daskalakis, Fidel Vila-Rodriguez, Esther Alonso, Colleen A. Brenner, Mario Liotti, Moyez Dharsee, Stephen R. Arnott, Kenneth R. Evans, Susan Rotzinger, and Sidney H. Kennedy, *Standardization of electroencephalography for multi-site, multi-platform and multi-investigator studies: Insights from the canadian biomarker integration network in depression*, Scientific Reports **7** (2017), no. 1, 7473.

- [36] T. Fedele, H. J. Scheer, G. Waterstraat, B. Telenczuk, M. Burghoff, and G. Curio, *Towards non-invasive multi-unit spike recordings: Mapping 1kHz EEG signals over human somatosensory cortex*, Clinical Neurophysiology **123** (2012), no. 12, 2370–2376.
- [37] Walter J. Freeman and Rodrigo Quian Quiroga, *Imaging brain function with EEG: Advanced temporal and spatial analysis of electroencephalographic signals*, Springer New York, New York, NY, 2013.
- [38] Inc. Gartner, *Gartner hype 2015*, 2015 (accessed September 3, 2018), <https://www.gartner.com/newsroom/id/3114217%0A>.
- [39] B. Giagante, S. Oddo, W. Silva, D. Consalvo, E. Centurion, L. D'Alessio, P. Solis, P. Salgado, E. Seoane, P. Saidon, and S. Kochen, *Clinical-electroencephalogram patterns at seizure onset in patients with hippocampal sclerosis*, Clinical Neurophysiology **114** (2003), no. 12, 2286–2293.
- [40] A. L. Goldberger, L. A. N. Amaral, L. Glass, J. M. Hausdorff, P. Ch. Ivanov, R. G. Mark, J. E. Mietus, G. B. Moody, C.-K. Peng, and H. E. Stanley, *PhysioBank, PhysioToolkit, and PhysioNet : Components of a New Research Resource for Complex Physiologic Signals*, Circulation **101** (2000), no. 23, e215–e220.
- [41] Alexandre Gramfort, Martin Luessi, Eric Larson, Denis A. Engemann, Daniel Strohmeier, Christian Brodbeck, Roman Goj, Mainak Jas, Teon Brooks, Lauri Parkkonen, and Matti Hämäläinen, *MEG and EEG data analysis with MNE-Python*, Frontiers in Neuroscience **7** (2013), no. 7, 267.
- [42] Rémi Gribonval, Holger Rauhut, Karin Schnass, and Pierre Vandergheynst, *Atoms of all channels, unite! Average case analysis of multi-channel sparse recovery using greedy algorithms*, Journal of Fourier Analysis and Applications **14** (2008), no. 5-6, 655–687.
- [43] Shenkai Gu and Yaochu Jin, *Heterogeneous classifier ensembles for EEG-based motor imaginary detection*, 2012 12th UK Workshop on Computational Intelligence, UKCI 2012, IEEE, sep 2012, pp. 1–8.
- [44] Christoph Guger, Brendan Z Allison, and Mikhail A Lebedev, *Brain Computer Interface Research: A State of the Art Summary 6 - Introduction*, Brain Computer Interface Research: A State of the Art Summary 6, Springer, 2017, pp. 1–8.
- [45] Christoph Guger, Shahab Daban, Eric Sellers, Clemens Holzner, Gunther Krausz, Roberta Carabalona, Furio Gramatica, and Guenter Edlinger, *How many people are able to control a P300-based brain-computer interface (BCI)?*, Neuroscience Letters **462** (2009), no. 1, 94–98.
- [46] Marcelo Alejandro Haberman and Enrique Mario Spinelli, *A multichannel EEG acquisition scheme based on single ended amplifiers and digital DRL*, IEEE Transactions on Biomedical Circuits and Systems **6** (2012), no. 6, 614–618.
- [47] Saskia Haegens, Helena Cousijn, George Wallis, Paul J. Harrison, and Anna C. Nobre, *Inter- and intra-individual variability in alpha peak frequency*, NeuroImage **92** (2014), 46–55.

- [48] Fredric J. Harris, *On the Use of Windows for Harmonic Analysis with the Discrete Fourier Transform*, Proceedings of the IEEE **66** (1978), no. 1, 51–83.
- [49] Bin He, *Neural engineering: Second edition*, KA-PP, 2013.
- [50] C. Herff, G. Johnson, L. Diener, J. Shih, D. Krusienski, and T. Schultz, *Towards direct speech synthesis from ecog: A pilot study*, 2016 38th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC), Aug 2016, pp. 1540–1543.
- [51] Hochberg, Serruya, Friehs, Mukand, Saleh, Capla, Branner, Chen, Penn, and Donoghue, *Neuronal ensemble control of prosthetic devices by a human with tetraplegia*, Nature **442** (2006), no. 7099, 164–171.
- [52] L. Hu, A. Mouraux, Y. Hu, and G. D. Iannetti, *A novel approach for enhancing the signal-to-noise ratio and detecting automatically event-related potentials (ERPs) in single trials*, NeuroImage **50** (2010), no. 1, 99–111.
- [53] Jane E. Huggins, Ramses E. Alcaide-Aguirre, and Katya Hill, *Effects of text generation on P300 brain-computer interface performance*, Brain-Computer Interfaces **3** (2016), no. 2, 112–120.
- [54] Jane E. Huggins, Aisha A. Moinuddin, Anthony E. Chiodo, and Patricia A. Wren, *What would brain-computer interface users want: Opinions and priorities of potential users with spinal cord injury*, Archives of Physical Medicine and Rehabilitation **96** (2015), no. 3, S38–S45.
- [55] Alice F. Jackson and Donald J. Bolger, *The neurophysiological bases of EEG and EEG measurement: A review for the rest of us*, Psychophysiology **51** (2014), no. 11, 1061–1071.
- [56] Abeg Kumar Jaiswal and Haider Banka, *Local pattern transformation based feature extraction techniques for classification of epileptic EEG signals*, Biomedical Signal Processing and Control **34** (2017), 81–92.
- [57] Ben H. Jansen, *Quantitative analysis of electroencephalograms: is there chaos in the future?*, International Journal of Bio-Medical Computing **27** (1991), no. 2, 95–123.
- [58] Piotr Jaśkowski and Rolf Verleger, *An evaluation of methods for single-trial estimation of P3 latency*, Psychophysiology **37** (2000), no. 2, 153–162.
- [59] J. Jestic, P. Fitch, R. W. Gilliatt, and R. G. Willison, *Automatic and rapid visual analysis of sleep stages and epileptic activity. A preliminary report*, Electroencephalography and Clinical Neurophysiology **43** (1977), no. 3, 438–441.
- [60] Camille Jeunet, Alison Cellard, Sriram Subramanian, Martin Hachet, Bernard N'Kaoua, and Fabien Lotte, *How Well Can We Learn With Standard BCI Training Approaches? A Pilot Study.*, 6th International Brain-Computer Interface Conference (Graz, Austria), September 2014.

- [61] Fabricio A Jure, Lucía C Carrere, Gerardo G Gentiletti, and Carolina B Tabernig, *BCI-FES system for neuro-rehabilitation of stroke patients*, Journal of Physics: Conference Series **705** (2016), no. 1, 012058.
- [62] Matthias Kaper, Peter Meinicke, Ulf Grossekathofer, Thomas Lingner, and Helge Ritter, *BCI competition 2003 - Data set IIb: Support vector machines for the P300 speller paradigm*, IEEE Transactions on Biomedical Engineering **51** (2004), no. 6, 1073–1076.
- [63] F Klein, *A waveform analyzer applied to the human EEG*, IEEE Transactions on Biomedical Engineering **23** (1976), no. 3, 246–252.
- [64] K. H. Knuth, *Differentially Variable Component Analysis: Identifying Multiple Evoked Components Using Trial-to-Trial Variability*, Journal of Neurophysiology **95** (2006), no. 5, 3257–3276.
- [65] Dean J. Krusienski, Eric W. Sellers, François Cabestaing, Sabri Bayoudh, Dennis J. McFarland, Theresa M. Vaughan, and Jonathan R. Wolpaw, *A comparison of classification techniques for the P300 Speller*, Journal of Neural Engineering **3** (2006), no. 4, 299–305.
- [66] Nanying Liang and Laurent Bougrain, *Averaging techniques for single-trial analysis of oddball event-related potentials*, 4th International Brain-Computer . . . (2008), 1–6.
- [67] Tony Lindeberg, *A computational theory of visual receptive fields*, Biological Cybernetics **107** (2013), no. 6, 589–635.
- [68] Peter Lloyd-Sherlock, *Population ageing in developed and developing regions: Implications for health policy*, Social Science and Medicine **51** (2000), no. 6, 887–895.
- [69] F. Lotte, L. Bougrain, A. Cichocki, M. Clerc, M. Congedo, A. Rakotomamonjy, and F. Yger, *A review of classification algorithms for EEG-based brain-computer interfaces: A 10 year update*, Journal of Neural Engineering **15** (2018), no. 3, 031005.
- [70] F. Lotte, M. Congedo, A. Lécuyer, F. Lamarche, and B. Arnaldi, *A review of classification algorithms for EEG-based brain-computer interfaces*, 2007.
- [71] F. Lotte, J. Faller, and C. Guger, *Combining BCI with Virtual Reality: Towards New Applications and Improved BCI*, Proceedings of the 6th International Conference on Foundations of Digital Games, Springer, Berlin, Heidelberg, 2013, pp. 1–24.
- [72] G Lowe, *SIFT - The Scale Invariant Feature Transform*, International Journal **2** (2004), 91–110.
- [73] Tomohiro Madarame, Hisaya Tanaka, Takenobu Inoue, Minoru Kamata, and Motoki Shino, *The development of a brain computer interface device for amyotrophic lateral sclerosis patients*, Conference Proceedings - IEEE International Conference on Systems, Man and Cybernetics, IEEE, oct 2008, pp. 2401–2406.

- [74] Joseph N. Mak, Dennis J. McFarland, Theresa M. Vaughan, Lynn M. McCane, Phillipa Z. Tsui, Debra J. Zeitlin, Eric W. Sellers, and Jonathan R. Wolpaw, *EEG correlates of P300-based brain-computer interface (BCI) performance in people with amyotrophic lateral sclerosis*, Journal of Neural Engineering **9** (2012), no. 2, 1–11.
- [75] Stephane G. Mallat and Zhifeng Zhang, *Matching Pursuits With Time-Frequency Dictionaries*, IEEE Transactions on Signal Processing **41** (1993), no. 12, 3397–3415.
- [76] Lynn M McCane, Susan M Heckman, Dennis J McFarland, George Townsend, Joseph N Mak, Eric W Sellers, Debra Zeitlin, Laura M Tenteromano, Jonathan R Wolpaw, and Theresa M Vaughan, *P300-based brain-computer interface (BCI) event-related potentials (ERPs): People with amyotrophic lateral sclerosis (ALS) vs. age-matched controls*, Clinical Neurophysiology **126** (2015), no. 11, 2124–2131.
- [77] Kai J. Miller, *Broadband spectral change: Evidence for a macroscale correlate of population firing rate?*, Journal of Neuroscience **30** (2010), no. 19, 6477–6479.
- [78] Chang S. Nam, Yueqing Li, and Steve Johnson, *Evaluation of P300-based brain-computer interface in real-world contexts*, International Journal of Human-Computer Interaction **26** (2010), no. 6, 621–637.
- [79] Nam, C., Nijholt, A., Lotte, F (ed.), *Brain-Computer Interfaces Handbook*, CRC Press, Boca Raton, jan 2018.
- [80] Nicoletta Nicolaou and Julius Georgiou, *Permutation entropy: A new feature for brain-computer interfaces*, 2010 IEEE Biomedical Circuits and Systems Conference, BioCAS 2010, IEEE, nov 2010, pp. 49–52.
- [81] Femke Nijboer and Ursula Broermann, *Brain-Computer Interfaces for Communication and Control in Locked-in Patients*, Brain-Computer Interfaces: Revolutionizing Human-Computer Interaction, Springer Berlin Heidelberg, 2009, pp. 185–201.
- [82] Amin Nourmohammadi and Mohammad Jafari, *A Survey on Unmanned Aerial Vehicle Remote Control Using Brain- Computer Interface*, IEEE Transactions on Human-Machine Systems (2018), no. May, 1–12.
- [83] Domen Novak, Roland Sigrist, Nicolas J. Gerig, Dario Wyss, René Bauer, Ulrich Götz, and Robert Riener, *Benchmarking Brain-Computer Interfaces Outside the Laboratory: The Cybathlon 2016*, Frontiers in Neuroscience **11** (2018), 15.
- [84] Guang Ouyang, Andrea Hildebrandt, Werner Sommer, and Changsong Zhou, *Exploiting the intra-subject latency variability from single-trial event-related potentials in the P3 time range: A review and comparative evaluation of methods*, Neuroscience and Biobehavioral Reviews **75** (2017), 1–21.
- [85] Thomas J Owens, George Zandt, and Steven R Taylor, *Seismic evidence for an ancient rift beneath the Cumberland Plateau, Tennessee: A detailed analysis of broadband teleseismic P waveforms*, Journal of Geophysical Research: Solid Earth **89** (1984), no. B9, 7783–7795.

- [86] Chethan Pandarinath, Paul Nuyujukian, Christine H. Blabe, Brittany L. Sorice, Jad Saab, Francis R. Willett, Leigh R. Hochberg, Krishna V. Shenoy, and Jaimie M. Henderson, *High performance communication by people with paralysis using an intracortical brain-computer interface*, eLife **6** (2017), 1–12.
- [87] Lucas C. Parra, Christoforos Christoforou, Adam D. Gerson, Mads Dyrholm, An Luo, Mark Wagner, Marios G. Philiastides, and Paul Sajda, *Spatiotemporal linear decoding of brain state*, IEEE Signal Processing Magazine **25** (2008), no. 1, 107–115.
- [88] S. Perdikis, R. Leeb, J. Williamson, A. Ramsay, M. Tavella, L. Desideri, E. J. Hoogerwerf, A. Al-Khadairy, R. Murray-Smith, and J. D R Millán, *Clinical evaluation of BrainTree, a motor imagery hybrid BCI speller*, Journal of Neural Engineering **11** (2014), no. 3, 12.
- [89] John Polich, *Updating P300: An integrative theory of P3a and P3b*, oct 2007, pp. 2128–2148.
- [90] R. Quian Quiroga and H. Garcia, *Single-trial event-related potentials with wavelet denoising*, Clinical Neurophysiology **114** (2003), no. 2, 376–390.
- [91] Alain Rakotomamonjy and Vincent Guigue, *BCI Competition III: Dataset II- Ensemble of SVMs for BCI P300 Speller*, IEEE Transactions on Biomedical Engineering **55** (2008), no. 3, 1147–1154.
- [92] R Ramele, A J Villar, and J M Santos, *P300-Dataset RRID:SCR_015977*, <https://www.kaggle.com/rramele/p300samplingdataset>, 2017.
- [93] R. Ramele, A.J. Villar, and J.M. Santos, *BCI classification based on signal plots and SIFT descriptors*, 2016 4th International Winter Conference on Brain-Computer Interface (BCI), IEEE, feb 2016, pp. 1–4.
- [94] Rajesh P. N. Rao, *Brain-computer interfacing : an introduction*, Cambridge University Press, 2013.
- [95] Yann Renard, Fabien Lotte, Guillaume Gibert, Marco Congedo, Emmanuel Maby, Vincent Delannoy, Olivier Bertrand, and Anatole Lécuyer, *OpenViBE: An Open-Source Software Platform to Design, Test, and Use Brain–Computer Interfaces in Real and Virtual Environments*, Presence: Teleoperators and Virtual Environments **19** (2010), no. 1, 35–53.
- [96] Angela Riccio, Luca Simione, Francesca Schettini, Alessia Pizzimenti, Maurizio Inghilleri, Marta Olivetti Belardinelli, Donatella Mattia, and Febo Cincotti, *Attention and P300-based BCI performance in people with amyotrophic lateral sclerosis*, Frontiers in Human Neuroscience **7** (2013), no. 11, 732.
- [97] Robert Riener and Linda J. Seward, *Cybathlon 2016*, 2014 IEEE International Conference on Systems, Man, and Cybernetics (SMC) (2014), 2792–2794.
- [98] Andrea Rodenbeck, Ralf Binder, Peter Geisler, Heidi Danker-Hopfe, Reimer Lund, Friedhart Raschke, Hans Günther Weiß, and Hartmut Schulz, *A review of sleep EEG*

- patterns. Part I: A compilation of amended rules for their visual recognition according to Rechtschaffen and Kales*, Somnologie **10** (2006), no. 4, 159–175.
- [99] Sanei and Chambers, *EEG signal processing*, John Wiley & Sons, 2008.
 - [100] Saeid Sanei and J.A. Chambers, *EEG Signal Processing*, Wiley, 2007.
 - [101] G. Schalk, D. J. McFarland, T. Hinterberger, N. Birbaumer, and J. R. Wolpaw, *BCI2000: a general-purpose brain-computer interface (BCI) system.*, IEEE Transactions on Bio-medical Engineering **51** (2004), no. 6, 1034–43.
 - [102] Bernhard Scholkopf and Alexander J Smola, *Learning with kernels: support vector machines, regularization, optimization, and beyond*, MIT press, 2001.
 - [103] Donald L Schomer and Fernando Lopes Da Silva, *Niedermeyer's Electroencephalography: Basic Principles, Clinical Applications, and Related Fields*, vol. 1, Oxford University Press, 2010.
 - [104] Eric W Sellers, Andrea Kübler, and Emanuel Donchin, *Brain-computer interface research at the University of South Florida cognitive psychophysiology laboratory: The P300 speller*, IEEE Transactions on Neural Systems and Rehabilitation Engineering **14** (2006), no. 2, 221–224.
 - [105] Nidhi Agrawal Shah and Courtney Jane Wusthoff, *How to use: Amplitude-integrated EEG (aEEG)*, Archives of Disease in Childhood: Education and Practice Edition **100** (2015), no. 2, 75–81.
 - [106] Douglas A Skoog, Donald M West, F James Holler, and Stanley R Crouch, *Analytical chemistry: an introduction*, Saunders College Publishing, 2000.
 - [107] J Stern and J Engel Jr, *Atlas of EEG Patterns*, Wolters Kluwer, 2005.
 - [108] David Steyrl, Reinhold Scherer, Josef Faller, and Gernot R Müller-Putz, *Random forests in non-invasive sensorimotor rhythm brain-computer interfaces: a practical and convenient non-linear classifier.*, Biomedizinische Technik. Biomedical engineering (2015), 77–86.
 - [109] G. Stockman, L Kanal, and M.C. Kyle, *Structural pattern recognition of carotid pulse waves using a general waveform parsing system*, Communications of the ACM **19** (1976), no. 12, 688–695.
 - [110] Arkadiusz Stopczynski, Carsten Stahlhut, Jakob Eg Larsen, Michael Kai Petersen, and Lars Kai Hansen, *The smartphone brain scanner: a portable real-time neuroimaging system.*, PloS one **9** (2014), no. 2, 10.
 - [111] N. V. Thakor and S. Tong, *Advances in Quantitative Electroencephalogram Analysis Methods*, Annual Review of Biomedical Engineering **6** (2004), no. 1, 453–495.
 - [112] N.V. Thakor, *Quantitative EEG analysis methods and clinical applications*, Artech House Series Engineering in Medicine and Biology, 2009.

- [113] Roni Tibon and Daniel A. Levy, *Striking a balance: Analyzing unbalanced event-related potential data*, Frontiers in Psychology **6** (2015), no. 5, 15.
- [114] Marleen C. Tjepkema-Cloostermans, Rafael C.V. de Carvalho, and Michel J.A.M. van Putten, *Deep learning for detection of focal epileptiform discharges from scalp EEG recordings*, Clinical Neurophysiology **129** (2018), no. 10, 2191–2196.
- [115] Sunao Uchida, Irwin Feinberg, Jonathan D. March, Yoshikata Atsumi, and Tom Maloney, *A comparison of period amplitude analysis and FFT power spectral analysis of all-night human sleep EEG*, Physiology and Behavior **67** (1999), no. 1, 121–131.
- [116] Sunao Uchida, Masato Matsuura, Shigeki Ogata, Takuji Yamamoto, and Naoyuki Aikawa, *Computerization of Fujimori's method of waveform recognition a review and methodological considerations for its application to all-night sleep EEG*, Journal of Neuroscience Methods **64** (1996), no. 1, 1–12.
- [117] Valentina Unakova and Karsten Keller, *Efficiently Measuring Complexity on the Basis of Real-World Data*, Entropy **15** (2013), no. 10, 4392–4415.
- [118] Wim Van Drongelen, *Signal processing for neuroscientists: an introduction to the analysis of physiological signals*, Academic press, 2006.
- [119] Sampsa Vanhatalo, Juha Voipio, and Kai Kaila, *Full-band EEG (FbEEG): An emerging standard in electroencephalography*, Clinical Neurophysiology **116** (2005), no. 1, 1–8.
- [120] L Vareka, *Matching pursuit for P300-based brain-computer interfaces*, 35th International Conference on Telecommunications and Signal Processing, TSP - Proceedings (2012), no. 2, 513–516.
- [121] Andrea Vedaldi and Brian Fulkerson, *VLCFeat - An open and portable library of computer vision algorithms*, Design **3** (2010), no. 1, 1–4.
- [122] E. Vincent and Y. Deville, *Handbook of Blind Source Separation - Independent Component Analysis and Applications*, Elsevier, 2010.
- [123] Sophie Wang, C. Janice Hsu, Lauren Trent, Tiffany Ryan, Nathan T. Kearns, Eugene F. Civillico, and Kimberly L. Kontson, *Evaluation of Performance-Based Outcome Measures for the Upper Limb: A Systematic Review*, Pm&R (2018), 1–16.
- [124] Wouter D. Weeda, Raoul P P P Grasman, Lourens J. Waldorp, Maria C. van de Laar, Maurits W. van der Molen, and Hilde M. Huizenga, *A fast and reliable method for simultaneous waveform, amplitude and latency estimation of single-trial EEG/MEG data*, PLoS ONE **7** (2012), no. 6, 1–12.
- [125] Wessberg, Stambaugh, Kralik, Beck, Laubach, Chapin, Kim, Biggs, Srinivasan, and Nicolelis, *Real-time prediction of hand trajectory by ensembles of cortical neurons in primates*, Nature **408** (2000), no. 6810, 361–365.
- [126] Wolpaw Elizabeth Wolpaw, Jonathan R, *Brain-Computer Interfaces: Principles and Practice*, Oxford University Press, 2012.

- [127] D. F. Wulsin, J. R. Gupta, R. Mani, J. A. Blanco, and B. Litt, *Modeling electroencephalography waveforms with semi-supervised deep belief nets: Fast classification and anomaly measurement*, Journal of Neural Engineering **8** (2011), no. 3, 15.
- [128] Tomonari Yamaguchi, Mitsuhiro Fujio, Katsuhiro Inoue, and Gert Pfurtscheller, *Design method of morphological structural function for pattern recognition of EEG signals during motor imagery and cognition*, 2009 4th International Conference on Innovative Computing, Information and Control, ICICIC 2009, IEEE, dec 2009, pp. 1558–1561.
- [129] Robert Maxwell Young, *Mind, brain, and adaptation in the nineteenth century: Cerebral localization and its biological context from Gall to Ferrier*, Oxford University Press, USA, 1970.
- [130] Rafael Yuste, Sara Goering, Blaise Agüeray Arcas, Guoqiang Bi, Jose M. Carmena, Adrian Carter, Joseph J. Fins, Phoebe Friesen, Jack Gallant, Jane E. Huggins, Judy Illes, Philipp Kellmeyer, Eran Klein, Adam Marblestone, Christine Mitchell, Erik Parens, Michelle Pham, Alan Rubel, Norihiro Sadato, Laura Specker Sullivan, Mina Teicher, David Wasserman, Anna Wexler, Meredith Whittaker, and Jonathan Wolpaw, *Four ethical priorities for neurotechnologies and AI*, Nature **551** (2017), no. 7679, 159–163.
- [131] Thorsten O. Zander, Christian Kothe, Sabine Jatzev, and Matti Gaertner, *Enhancing Human-Computer Interaction with Input from Active and Passive Brain-Computer Interfaces*, Brain-Computer Interfaces: Applying our Minds to Human-Computer Interaction, Springer, London, 2010, pp. 181–199.
- [132] Thorsten O. Zander, Laurens R. Krol, Niels P. Birbaumer, and Klaus Gramann, *Neuroadaptive technology enables implicit cursor control based on medial prefrontal cortex activity*, Proceedings of the National Academy of Sciences **113** (2016), no. 52, 14898–14903.
- [133] Dandan Zhang and Yuejia Luo, *The P1 latency of single-trial ERPs estimated by two peak-picking strategies*, Proceedings - 2011 4th International Conference on Biomedical Engineering and Informatics, BMEI 2011 **2** (2011), 882–886.
- [134] Jian Zhang, Junzhong Zou, Min Wang, Lanlan Chen, Chunmei Wang, and Guisong Wang, *Automatic detection of interictal epileptiform discharges based on time-series sequence merging method*, Neurocomputing **110** (2013), 35–43.