



| FCC TEST REPORT FCC 47 CFR Part 15C Industry Canada RSS-210 Digital transmission systems operating within the 2400 – 2483.5 MHz band | | | | | | | | | | | | | | | | |
|---|---|---------------------|--------------------------|--|-----------|-------------|--|------------------|-----|--|-----------------------------|------|--|--|----------------------|------------------|
| Report Reference No. | G0M-1305-2859-TFC247W-V02 | | | | | | | | | | | | | | | |
| Testing Laboratory | Eurofins Product Service GmbH | | | | | | | | | | | | | | | |
| Address | Storkower Str. 38c 15526 Reichenwalde Germany | | | | | | | | | | | | | | | |
| Accreditation |   A2LA Accredited Testing Laboratory, Certificate No.: 1983.01 FCC Filed Test Laboratory, Reg.-No.: 96970 IC OATS Filing assigned code: 3470A | | | | | | | | | | | | | | | |
| Applicant's name | Bang & Olufsen Medicom A/S | | | | | | | | | | | | | | | |
| Address | Gimsinglundvej 20 7600 Struer DENMARK | | | | | | | | | | | | | | | |
| Test specification: | Standard..... : 47 CFR Part 15C KDB Publication No. 558074 RSS-210, Issue 8, 2010-12 RSS-Gen, Issue 3, 2010-12 ANSI C63.4:2009 | | | | | | | | | | | | | | | |
| Equipment under test (EUT): | <table border="0"> <tr> <td>Product description</td> <td colspan="2">Electronic Auto-injector</td> </tr> <tr> <td>Model No.</td> <td colspan="2">betaCONNECT</td> </tr> <tr> <td>Hardware version</td> <td colspan="2">B11</td> </tr> <tr> <td>Firmware / Software version</td> <td colspan="2">None</td> </tr> <tr> <td></td> <td>FCC-ID: 2AAGY-BETAC1</td> <td>IC: 3775E-BETAC1</td> </tr> </table> | Product description | Electronic Auto-injector | | Model No. | betaCONNECT | | Hardware version | B11 | | Firmware / Software version | None | | | FCC-ID: 2AAGY-BETAC1 | IC: 3775E-BETAC1 |
| Product description | Electronic Auto-injector | | | | | | | | | | | | | | | |
| Model No. | betaCONNECT | | | | | | | | | | | | | | | |
| Hardware version | B11 | | | | | | | | | | | | | | | |
| Firmware / Software version | None | | | | | | | | | | | | | | | |
| | FCC-ID: 2AAGY-BETAC1 | IC: 3775E-BETAC1 | | | | | | | | | | | | | | |
| Test result | Passed | | | | | | | | | | | | | | | |

Possible test case verdicts:


- neither assessed nor tested: N/N
- required by standard but not appl. to test object.....: N/A
- required by standard but not tested.....: N/T
- not required by standard for the test object: N/R
- test object does meet the requirement.....: P (Pass)
- test object does not meet the requirement.....: F (Fail)

Testing:


Date of receipt of test item: 2013-07-01

Date (s) of performance of tests: 2013-07-02 – 2013-07-03

Compiled by: Antje Bartusch

Tested by (+ signature).....: Wilfried Treffke 

(Testing Manager)

Approved by (+ signature): Christian Weber 

(Test Lab Manager)

Date of issue: 2013-11-13

Total number of pages.....: 82

General remarks:

The test results presented in this report relate only to the object tested.

The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.

Additional comments:

Version History

| Version | Issue Date | Remarks | Revised by |
|---------|------------|-----------------------------|------------|
| 01 | 2013-08-30 | Initial Release | |
| 02 | 2013-11-13 | Calibration dates corrected | C. Weber |

REPORT INDEX

| | | |
|----------|---|-----------|
| 1 | EQUIPMENT (TEST ITEM) DESCRIPTION | 5 |
| 1.1 | Photos – Equipment External | 6 |
| 1.2 | Photos – Equipment internal | 7 |
| 1.3 | Photos – Test setup | 8 |
| 1.4 | Supporting Equipment Used During Testing | 9 |
| 1.5 | Test Modes | 10 |
| 1.6 | Test Equipment Used During Testing | 11 |
| 1.7 | Sample emission level calculation | 12 |
| 2 | RESULT SUMMARY | 13 |
| 3 | TEST CONDITIONS AND RESULTS | 14 |
| 3.1 | Test Conditions and Results – Occupied Bandwidth | 14 |
| 3.2 | Test Conditions and Results – 6 dB Bandwidth | 18 |
| 3.3 | Test Conditions and Results – Maximum peak conducted power | 22 |
| 3.4 | Test Conditions and Results – Power spectral density | 24 |
| 3.5 | Test Conditions and Results – AC power line conducted emissions | 25 |
| 3.6 | Test Conditions and Results – Band edge compliance | 28 |
| 3.7 | Test Conditions and Results – Conducted spurious emissions | 31 |
| 3.8 | Test Conditions and Results – Transmitter radiated emissions | 35 |
| 3.9 | Test Conditions and Results – Receiver radiated emissions | 37 |
| ANNEX A | Transmitter radiated spurious emissions | 39 |
| ANNEX B | Receiver radiated spurious emissions | 75 |

1 Equipment (Test item) Description

| | | |
|-----------------------------|--|-------------------------------------|
| Description | Electronic Auto-injector | |
| Model | betaCONNECT | |
| Serial number | None | |
| Hardware version | B11 | |
| Software / Firmware version | None | |
| FCC-ID | 2AAGY-BETAC1 | |
| IC | 3775E-BETAC1 | |
| Equipment type | Radio module | |
| Radio type | Transceiver | |
| Radio technology | Bluetooth 4.0 Low Energy | |
| Operating frequency range | 2402 - 2480 MHz | |
| Assigned frequency band | 2400 - 2483.5 MHz | |
| Main test frequencies | F _{LOW} | 2402 MHz |
| | F _{MID} | 2440 MHz |
| | F _{HIGH} | 2480 MHz |
| Spreading | None | |
| Modulations | GFSK | |
| Number of channels | 40 | |
| Channel spacing | 2MHz | |
| Number of antennas | 1 | |
| Antenna | Type | integrated |
| | Model | 2450AT18B100 |
| | Manufacturer | Johanson Technology |
| | Gain | -0.5 dBi (manufacturer declaration) |
| Manufacturer | Bang & Olufsen Medcom A/S Gimsinglundvej 20 7600 Struer DENMARK | |
| Power supply | V _{NOM} | 3.7 VDC |
| | V _{MIN} | 3.3 VDC |
| | V _{MAX} | 4.2 VDC |
| AC/DC-Adaptor | Model | ASUC30e-050100 |
| | Vendor | Aquilstar Precision Industrial |
| | Input | 100-240VAC, 50-60Hz |
| | Output | 5.0V |

1.4 Supporting Equipment Used During Testing

| Product Type* | Device | Manufacturer | Model No. | Comments |
|---|--------|--------------|-----------|----------|
| None | | | | |
| <p>*Note: Use the following abbreviations:</p> <p>AE : Auxiliary/Associated Equipment, or</p> <p>SIM : Simulator (Not Subjected to Test)</p> <p>CABL : Connecting cables</p> | | | | |

1.5 Test Modes

| Mode # | Description | |
|--------------|---------------------|---|
| Transmit | General conditions: | EUT powered by laboratory power supply. |
| | Radio conditions: | Mode = standalone transmit Spreading = None Modulation = GFSK Data rate = 1 Mbps Bandwidth = 2 MHz Duty cycle = 100 % Power level = Maximum |
| Receive | General conditions: | EUT powered by laboratory power supply. |
| | Radio conditions: | Mode = standalone receive (scan mode) Spreading = None Modulation = GFSK |
| AC-Powerline | General conditions: | EUT powered by commercial Laptop |
| | Radio conditions: | Mode = Transmit Spreading = None |

1.6 Test Equipment Used During Testing

| Occupied Bandwidth | | | | | |
|--------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Spectrum Analyzer | R&S | FSP 30 | EF00312 | 2013-01 | 2014-01 |

| 6dB Bandwidth | | | | | |
|-------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Spectrum Analyzer | R&S | FSP 30 | EF00312 | 2013-01 | 2014-01 |

| Maximum peak conducted power | | | | | |
|------------------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Spectrum Analyzer | R&S | FSP 30 | EF00312 | 2013-01 | 2014-01 |

| Power spectral density | | | | | |
|------------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Spectrum Analyzer | R&S | FSP 30 | EF00312 | 2013-01 | 2014-01 |

| Band edge compliance | | | | | |
|----------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Spectrum Analyzer | R&S | FSP 30 | EF00312 | 2013-01 | 2014-01 |

| Conducted spurious emissions | | | | | |
|------------------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Spectrum Analyzer | R&S | FSP 30 | EF00312 | 2013-01 | 2014-01 |

| Radiated spurious emissions | | | | | |
|-----------------------------|--------------|--------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Semi-anechoic chamber | Frankonia | AC 5 | EF00395 | - | - |
| Spectrum Analyzer | R&S | FSIQ26 | EF00242 | 2013-06 | 2014-06 |
| Biconical Antenna | R&S | HK 116 | EF00012 | 2013-02 | 2016-02 |
| LPD Antenna | R&S | HL 223 | EF00187 | 2011-02 | 2014-02 |
| LPD Antenna | R&S | HL 025 | EF00327 | 2013-02 | 2016-02 |

| AC powerline conducted emissions | | | | | |
|----------------------------------|--------------|---------|------------|-----------|----------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| AMN | R&S | ESH2-Z5 | EF00182 | 2012-10 | 2014-10 |
| AMN | R&S | ESH3-Z5 | EF00036 | 2012-11 | 2014-11 |
| EMI Test Receiver | R&S | ESCS 30 | EF00295 | 2012-08 | 2013-08 |

Test Report No.: G0M-1305-2859-TFC247W-V02

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dB μ V. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB μ V/m). The FCC limits are given in units of μ V/m. The following formula is used to convert the units of μ V/m to dB μ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 \cdot \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

$$\begin{array}{rclcl} \text{Reading} & + & \text{AF} & = & \text{Net Reading} & : & \text{Net reading - FCC limit} & = & \text{Margin} \\ 21.5 \text{ dB}\mu\text{V} & + & 26 \text{ dB} & = & 47.5 \text{ dB}\mu\text{V/m} & : & 47.5 \text{ dB}\mu\text{V/m} - 57.0 \text{ dB}\mu\text{V/m} & = & -9.5 \text{ dB} \end{array}$$

2 Result Summary

| FCC 47 CFR Part 15C, IC RSS-210 | | | | |
|--|---|--|--------|--------------------|
| Product Specific Standard Section | Requirement – Test | Reference Method | Result | Remarks |
| RSS-Gen 4.6.1 | Occupied Bandwidth | RSS-Gen 4.6.1 | N/R | Informational only |
| FCC § 15.247(a)(2) IC RSS-210 § A8.2 | 6dB Bandwidth | KDB Publication No. 558074 | PASS | |
| FCC § 15.247(b)(3) IC RSS-210 § A8.4 | Maximum peak conducted power | KDB Publication No. 558074 | PASS | |
| FCC § 15.247(e) IC RSS-210 § A8.2 | Power spectral density | KDB Publication No. 558074 | PASS | |
| 47 CFR 15.207 RSS-Gen 7.2.4 | AC power line conducted emissions | KDB Publication No. 558074 / ANSI C63.4 | PASS | |
| FCC § 15.247(d) IC RSS-210 § A8.5 | Band edge compliance | KDB Publication No. 558074 | PASS | |
| FCC § 15.247(d) IC RSS-210 § A8.5 | Conducted spurious emissions | KDB Publication No. 558074 | PASS | |
| FCC § 15.247(d) FCC § 15.209 IC RSS-210 A8.5 IC RSS-Gen 4.9 IC RSS-Gen 7.2.5 | Transmitter radiated spurious emissions | KDB Publication No. 558074 / ANSI C 63.4 | PASS | |
| IC RSS-Gen 4.10 IC RSS-Gen 6.1 | Receiver radiated spurious emissions | ANSI C 63.4 | PASS | |
| Remarks: | | | | |

3 Test Conditions and Results

3.1 Test Conditions and Results – Occupied Bandwidth


| Occupied Bandwidth acc. IC RSS-Gen | | | Verdict: PASS |
|---|---|----------|--------------------------|
| Test according to measurement reference | Reference Method | | |
| | RSS-Gen 4.6.1 | | |
| Test frequency range | Tested frequencies | | |
| | F _{LOW} / F _{MID} / F _{HIGH} | | |
| Limits | | | |
| None (Informational only) | | | |
| Test setup | | | |
| <div><div>Spectrum Analyzer</div><div>EUT</div></div> | | | |
| Test procedure | | | |
| <div>1. EUT set to test mode (Communication tester is used if needed)</div> <div>2. Span set to at least twice the emission spectrum</div> <div>3. Resolution bandwidth set to 1 % of span</div> <div>4. Occupied Bandwidth (99 %) measurement with spectrum analyzer built in measurement function</div> | | | |
| Test results | | | |
| Channel | Frequency [MHz] | Mode | Occupied Bandwidth [kHz] |
| F _{LOW} | 2402 | Transmit | 1.065 |
| F _{MID} | 2440 | Transmit | 1.017 |
| F _{HIGH} | 2480 | Transmit | 1.009 |
| Comments: | | | |

Occupied Bandwidth – F_{Low}

RSS Gen

Occupied Bandwidth

EUT Electronic Auto-injector
Model betaCONNECT
Approval Holder Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage Tnom / Vnom
Test Site / Operator Eurofins Product Service GmbH / Mr. Treffke
Test Specification 4.4.1 Occupied Bandwidth
Comment 1 Channel.: 2402 MHz
Comment 2 A spectrum analyzer with an integrated 99% power bandwidth function is used
Comment 3 GFSK

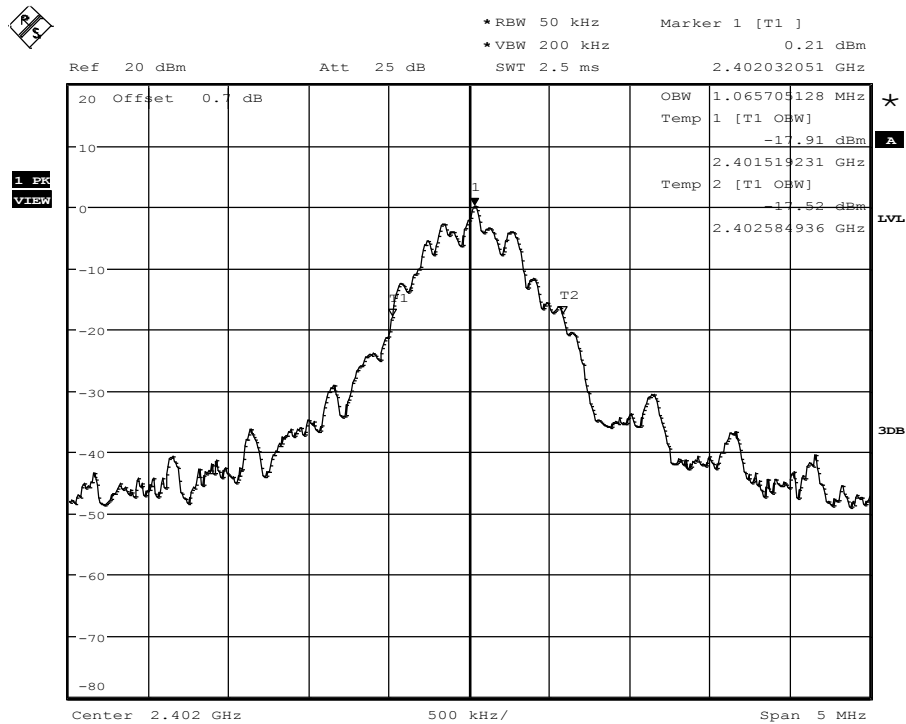

Occupied bandwidth: 1065.7 KHz


Date: 2.JUL.2013 14:00:10

Occupied Bandwidth – F_{MID}

RSS Gen

Occupied Bandwidth

EUT Electronic Auto-injector
Model betaCONNECT
Approval Holder Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage Tnom / Vnom
Test Site / Operator Eurofins Product Service GmbH / Mr. Treffke
Test Specification 4.4.1 Occupied Bandwidth
Comment 1 Channel.: 2440 MHz
Comment 2 A spectrum analyzer with an integrated 99% power bandwidth function is used
Comment 3 GFSK

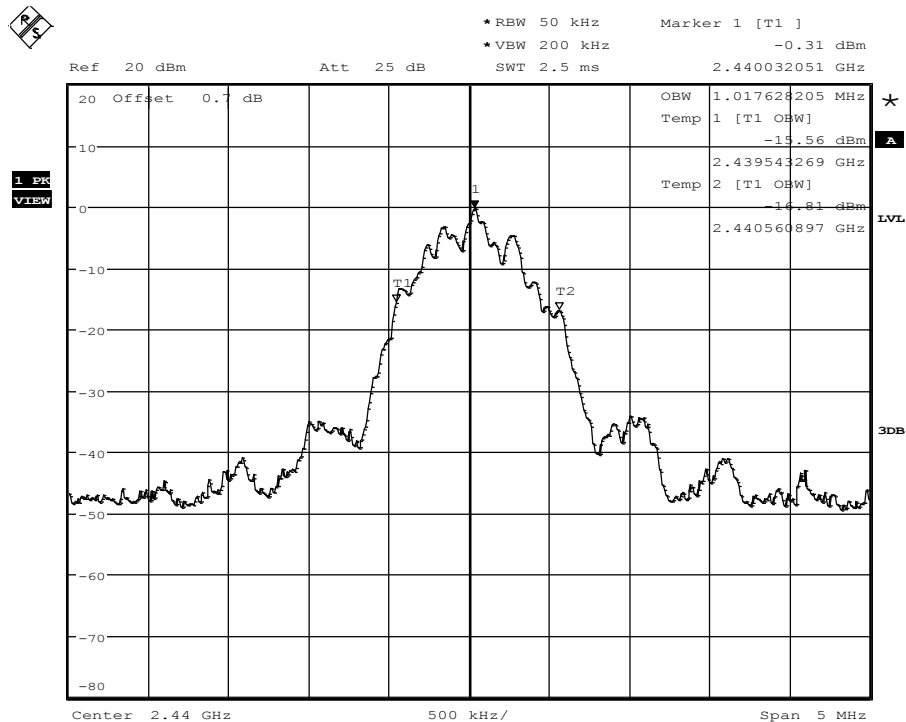


Occupied bandwidth: 1017.6 KHz

Date: 2.JUL.2013 14:01:37

Occupied Bandwidth – F_{HIGH}

RSS Gen Occupied Bandwidth

| | |
|-----------------------|---|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | 4.4.1 Occupied Bandwidth |
| Comment 1 | Channel.: 2480 MHz |
| Comment 2 | A spectrum analyzer with an integrated 99% power bandwidth function is used |
| Comment 3 | GFSK |

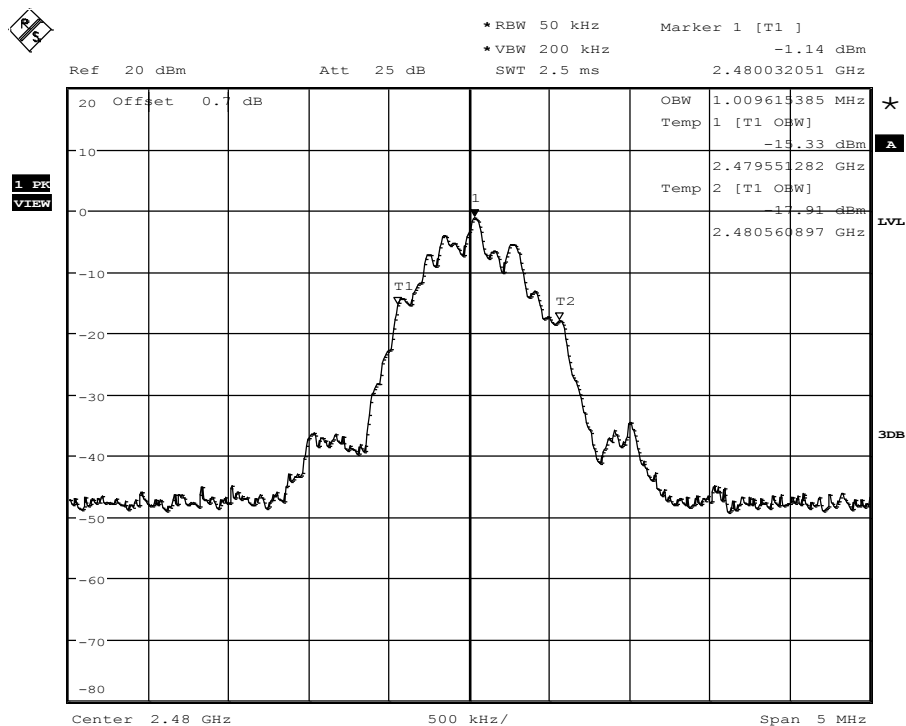

Occupied bandwidth: 1009.6 KHz

Date: 2.JUL.2013 14:03:07

3.2 Test Conditions and Results – 6 dB Bandwidth


| 6dB Bandwidth acc. FCC 15.247 / IC RSS-210 | | | | Verdict: PASS | |
|---|-----------------|---|----------------------|---------------|--------|
| EUT requirement rule parts and clause | | Reference | | | |
| | | FCC 15.247(a)(2) / IC RSS-210 A8.2 | | | |
| Test according to measurement reference | | Reference Method | | | |
| | | FCC KDB Publication No. 558074 | | | |
| Test frequency range | | Tested frequencies | | | |
| | | F _{LOW} / F _{MID} / F _{HIGH} | | | |
| Limits | | | | | |
| Limit | | | | | |
| ≥ 500kHz | | | | | |
| Test setup | | | | | |
| <div><div>Spectrum Analyzer</div><div>EUT</div></div> | | | | | |
| Test procedure | | | | | |
| <div>1. EUT set to test mode</div> <div>2. Span set to at least twice the emission spectrum</div> <div>3. Detector set to peak and max hold and RBW is set to 100 kHz</div> <div>4. Envelope peak value of emission spectrum is selected</div> <div>5. Marker on envelope of spectrum is set to level of -6 dB to the left of the peak</div> <div>6. Marker on envelope of spectrum is set to level of -6 dB to the right of the peak</div> <div>7. 6 dB Bandwidth is determined by marker frequency separation</div> | | | | | |
| Test results | | | | | |
| Channel | Frequency [MHz] | Mode | 6 dB Bandwidth [kHz] | Limit [kHz] | Result |
| F _{LOW} | 2402 | Transmit | 668.963 | 500 | PASS |
| F _{MID} | 2440 | Transmit | 668.907 | 500 | PASS |
| F _{HIGH} | 2480 | Transmit | 663.221 | 500 | PASS |
| Comments: | | | | | |

6 dB Bandwidth – F_{Low}

FCC part 15.247 (a)2

Minimum 6 dB Bandwidth

| | |
|-----------------------|--|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | FCC part 15.247 (a)2 |
| Comment 1 | Minimum 6 dB Bandwidth |
| Comment 2 | Channel 2402 MHz, GFSK |
| Comment 3 | procedure 8.1 DTS BW (558074 D01 DTS) |

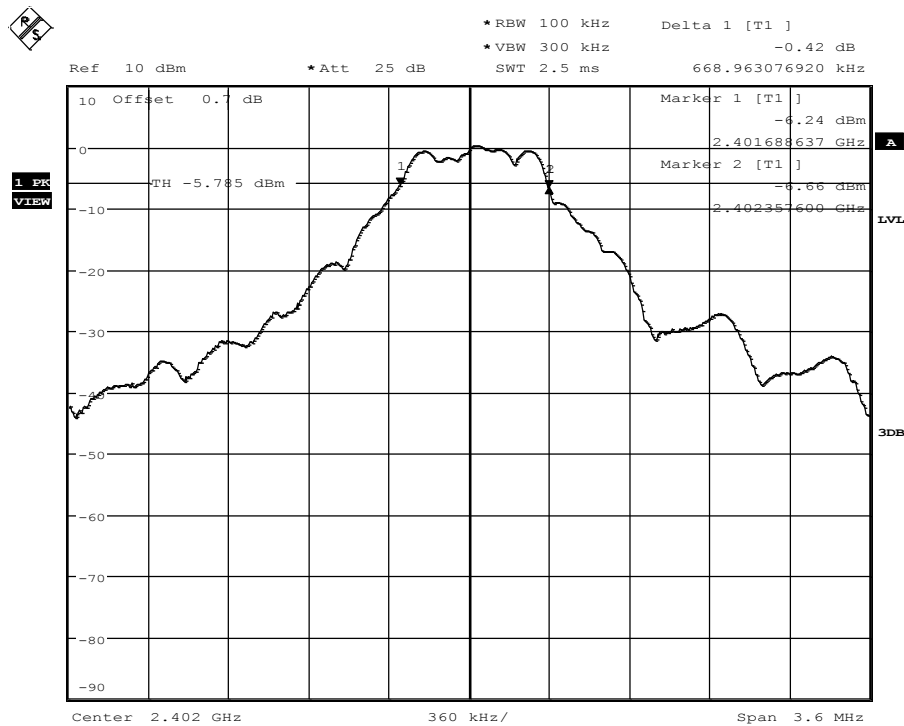

6 dB bandwidth: 669 KHz > 500 KHz; verdict: PASS


Date: 2.JUL.2013 13:35:44

6 dB Bandwidth – F_{MID}

FCC part 15.247 (a)2

Minimum 6 dB Bandwidth

| | |
|-----------------------|--|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | FCC part 15.247 (a)2 |
| Comment 1 | Minimum 6 dB Bandwidth |
| Comment 2 | Channel 2440 MHz, GFSK |
| Comment 3 | procedure 8.1 DTS BW (558074 D01 DTS) |

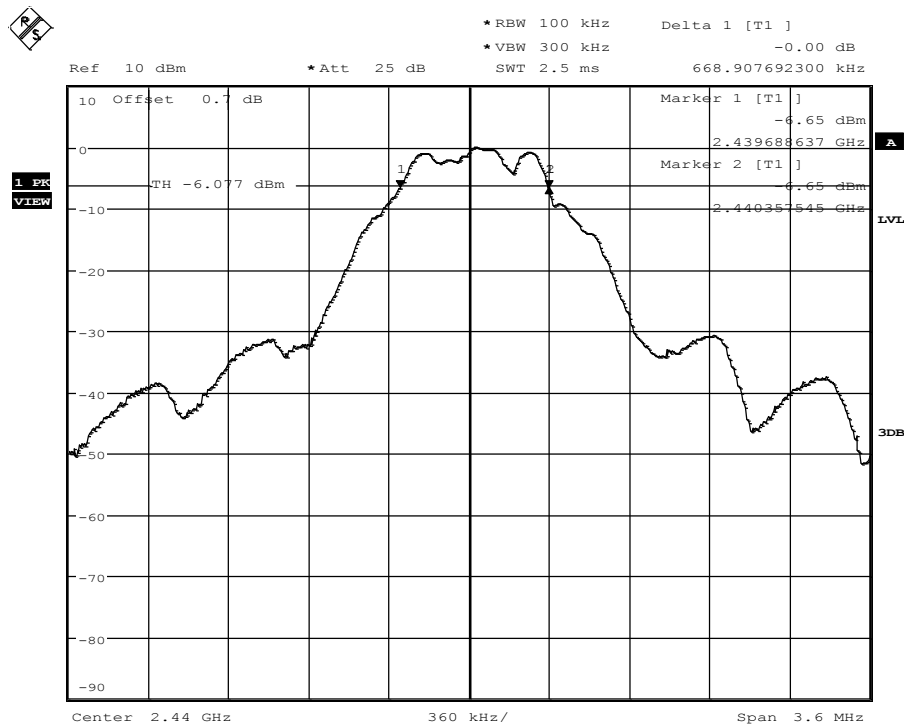

6 dB bandwidth: 668.9 KHz > 500 KHz; verdict: PASS


Date: 2.JUL.2013 13:32:55

6 dB Bandwidth – F_{HIGH}

FCC part 15.247 (a)2

Minimum 6 dB Bandwidth


| | |
|-----------------------|--|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | FCC part 15.247 (a)2 |
| Comment 1 | Minimum 6 dB Bandwidth |
| Comment 2 | Channel 2480 MHz, GFSK |
| Comment 3 | procedure 8.1 DTS BW (558074 D01 DTS) |

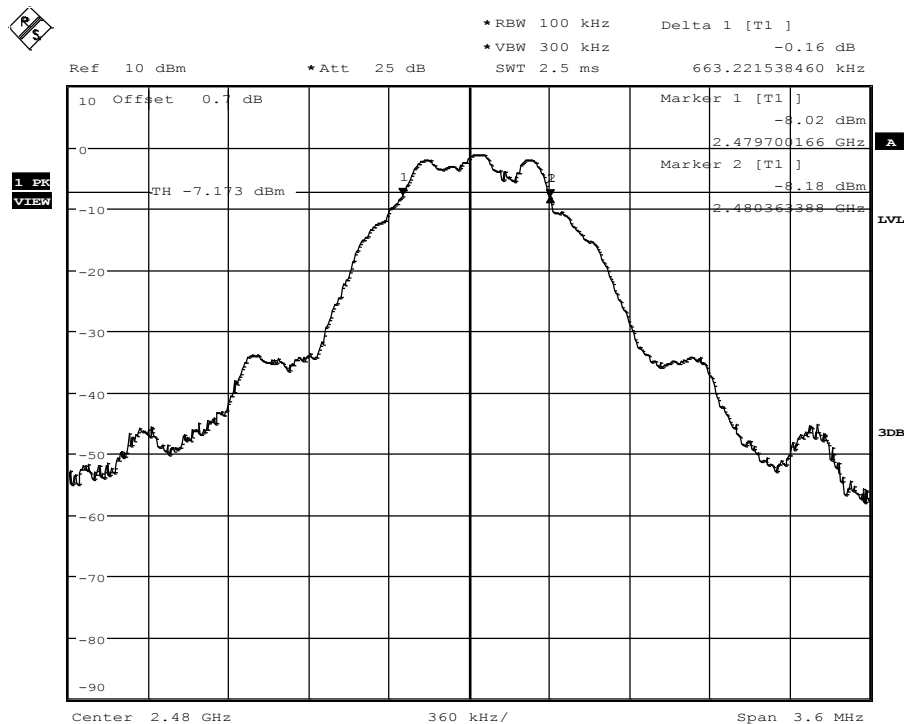

6 dB bandwidth: 663.2 KHz > 500 KHz; verdict: PASS

Date: 2.JUL.2013 13:37:15

3.3 Test Conditions and Results – Maximum peak conducted power
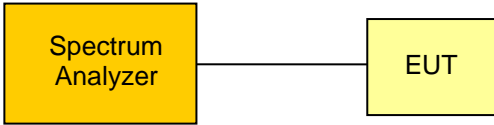
| Maximum peak conducted power acc. FCC 15.247 / IC RSS-210 | | Verdict: PASS |
|---|---|---------------|
| EUT requirement rule parts and clause | Reference | |
| | FCC 15.247(b)(3) / IC RSS-210 A8.4 | |
| Test according to measurement reference | Reference Method | |
| | FCC KDB Publication No. 558074 | |
| Test frequency range | Tested frequencies | |
| | $F_{\text{LOW}} / F_{\text{MID}} / F_{\text{HIGH}}$ | |
| Measurement mode | Peak | |
| Maximum antenna gain | -0.5 dBi \Rightarrow Limit correction = 0 dB | |
| Limits | | |
| 1 W (30 dBm) | | |
| The conducted output power limit specified above is based on the use of antennas with directional gains that do not exceed 6 dBi. If transmitting antennas of directional gain greater than 6 dBi are used, the conducted output power from the intentional radiator shall be reduced below the stated values in the table, as appropriate, by the amount in dB that the directional gain of the antenna exceeds 6 dBi. | | |
| Test setup | | |
|  | | |
| Test procedure | | |
| <ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Center frequency set to test channel center frequency 3. Span set to twice the 20 dB bandwidth and detector to peak and max hold 4. Resolution bandwidth is set to 3 MHz 5. Peak conducted power is determined from peak of spectrum envelope | | |

| Test results | | | | | | | |
|-------------------|-----------------|------------------------|----------|------------------|----------------|-------------|-------------|
| Channel | Frequency [MHz] | Voltage | Mode | Peak power [dbm] | Peak power [W] | Limit [dBm] | Margin [dB] |
| F _{LOW} | 2402 | V _{NOM} = 3.7 | Transmit | 0.21 | 0.001 | 30 | -29.79 |
| F _{MID} | 2442 | V _{MIN} = 3.3 | Transmit | 0.21 | 0.001 | 30 | -29.79 |
| F _{HIGH} | 2480 | V _{MAX} = 4.2 | Transmit | 0.20 | 0.001 | 30 | -29.80 |
| F _{LOW} | 2402 | V _{NOM} = 3.7 | Transmit | -0.3 | 0.001 | 30 | -30.30 |
| F _{MID} | 2442 | V _{MIN} = 3.3 | Transmit | -0.28 | 0.0009 | 30 | -30.28 |
| F _{HIGH} | 2480 | V _{MAX} = 4.2 | Transmit | -0.29 | 0.0009 | 30 | -30.29 |
| F _{LOW} | 2402 | V _{NOM} = 3.7 | Transmit | -1.21 | 0.0007 | 30 | -31.21 |
| F _{MID} | 2442 | V _{MIN} = 3.3 | Transmit | -1.21 | 0.0007 | 30 | -31.21 |
| F _{HIGH} | 2480 | V _{MAX} = 4.2 | Transmit | -1.22 | 0.0007 | 30 | -31.22 |
| Comment: | | | | | | | |

3.4 Test Conditions and Results – Power spectral density

| Power spectral density acc. FCC 15.247 / IC RSS-210 | | | | | Verdict: PASS | |
|---|-----------------|---|----------------------|--------------------------|------------------|-------------|
| EUT requirement rule parts and clause | | Reference | | | | |
| | | FCC 15.247(e) / IC RSS-210 A8.2 | | | | |
| Test according to measurement reference | | Reference Method | | | | |
| | | FCC KDB Publication No. 558074 | | | | |
| Test frequency range | | Tested frequencies | | | | |
| | | F _{LOW} / F _{MID} / F _{HIGH} | | | | |
| Measurement mode | | Peak | | | | |
| Limits | | | | | | |
| 8 dBm / 3 kHz | | | | | | |
| Test setup | | | | | | |
| <div><div>Spectrum Analyzer</div><div>EUT</div></div> | | | | | | |
| Test procedure | | | | | | |
| <div>1. EUT set to test mode (Communication tester is used if needed)</div> <div>2. Center frequency set to test channel center frequency</div> <div>3. Span is set large enough to capture maximum emissions in passband, RBW is set to 3kHz</div> <div>4. Peak power density is determined from peak emission of envelope</div> | | | | | | |
| Test results | | | | | | |
| Channel | Frequency [MHz] | Test mode | Peak frequency [MHz] | Peak power density [dBm] | Limit [dBm/3kHz] | Margin [dB] |
| F _{LOW} | 2402 | Transmit | 2402.045 | -15.02 | 8.0 | -23.02 |
| F _{MID} | 2440 | Transmit | 2440.035 | -15.6 | 8.0 | -23.60 |
| F _{HIGH} | 2480 | Transmit | 2480.045 | -16.5 | 8.0 | -24.50 |
| Comments: | | | | | | |

3.5 Test Conditions and Results – AC power line conducted emissions

| Power line conducted emissions acc. FCC 47 CFR 15.207 / IC RSS-Gen | | | | Verdict: PASS | |
|--|-------------------|-----------------------|----------------|---------------|--|
| Test according referenced standards | | Reference Method | | | |
| | | ANSI C63.4 | | | |
| Fully configured sample scanned over the following frequency range | | Frequency range | | | |
| | | 0.15 MHz to 30 MHz | | | |
| Points of Application | | Application Interface | | | |
| AC Mains | | LISN | | | |
| EUT test mode | | AC power line | | | |
| Limits and results | | | | | |
| Frequency [MHz] | Quasi-Peak [dBμV] | Result | Average [dBμV] | Result | |
| 0.15 to 5 | 66 to 56* | PASS | 56 to 46* | PASS | |
| 0.5 to 5 | 56 | PASS | 46 | PASS | |
| 5 to 30 | 60 | PASS | 50 | PASS | |
| Comments: | | | | | |
| * Limit decreases linearly with the logarithm of the frequency. | | | | | |


Conducted Emissions

EMI voltage test in the ac-mains according to FCC 15B

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
EUT Name: Electronic Auto-injector
Model: betaCONNECT
Test Site: Eurofins Product Service GmbH
Operator: Mr. Handrik
Test Conditions: Tnom: 22°C, Unom: 120 V AC (AC/DC adaptor: ASUC30e-050100)
LISN: ESH2-Z5 N
Mode: active; motor with load; charging, Bluetooth link
Test Date: 2013-07-02
Note:

Index 4

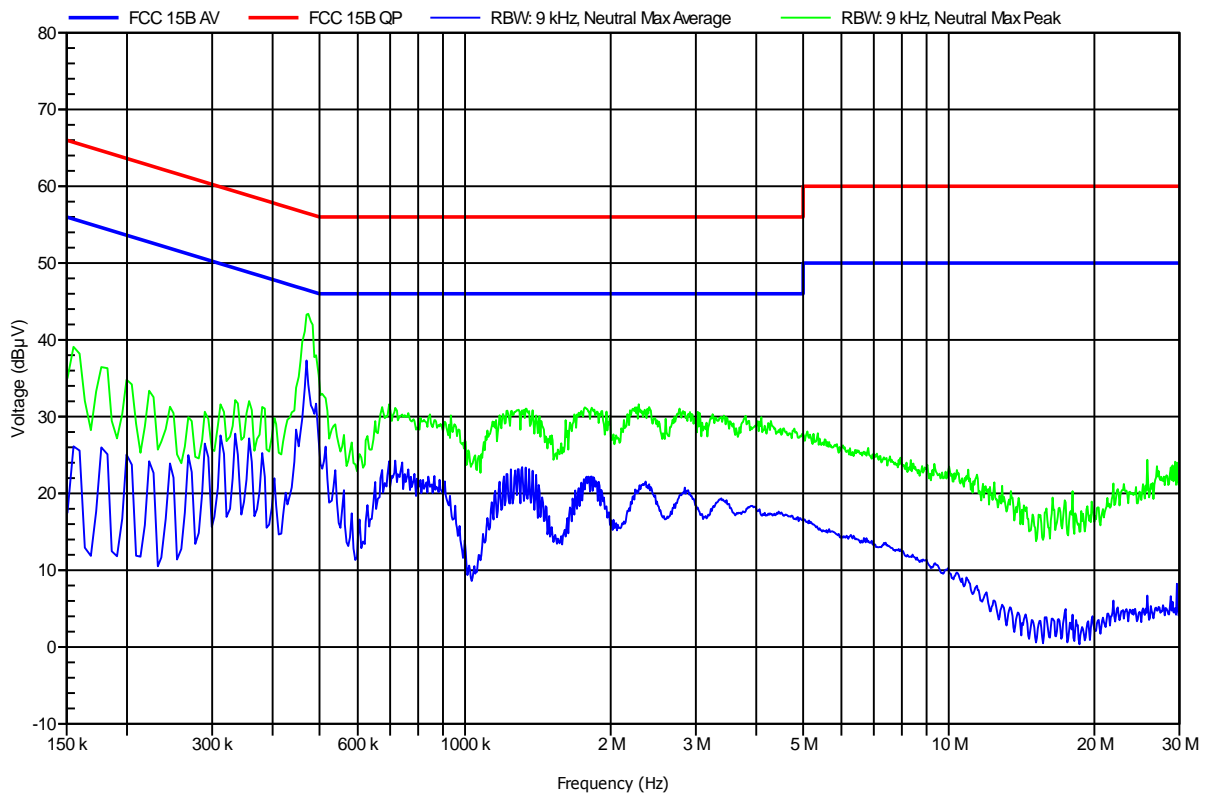


Conducted Emissions

EMI voltage test in the ac-mains according to FCC 15B

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Handrik
 Test Conditions: Tnom: 22°C, Unom: 120 V AC (AC/DC adaptor: ASUC30e-050100)
 LISN: ESH2-Z5 L
 Mode: active; motor with load; charging, Bluetooth link
 Test Date: 2013-07-02
 Note:

Index 5

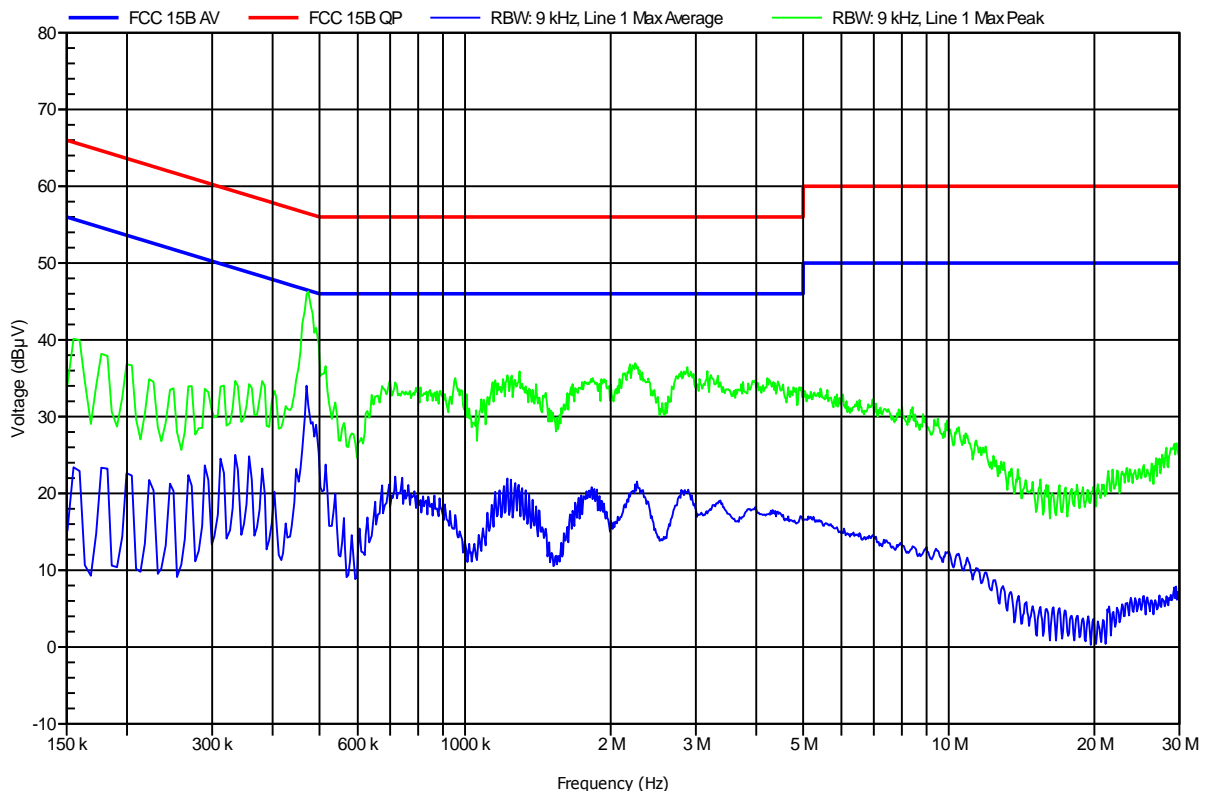

Test Report No.: G0M-1305-2859-TFC247W-V02

Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

3.6 Test Conditions and Results – Band edge compliance


| Band-edge compliance acc. FCC 15.247 / IC RSS-210 | | | | Verdict: PASS | |
|---|-----------------|--------------------------------------|--|---------------|-------------|
| EUT requirement rule parts and clause | | Reference | | | |
| | | FCC 15.247(d) / IC RSS-210 A8.5 | | | |
| Test according to measurement reference | | Reference Method | | | |
| | | FCC KDB Publication No. 558074 | | | |
| Test frequency range | | Tested frequencies | | | |
| | | F _{LOW} / F _{HIGH} | | | |
| Measurement mode | | Peak | | | |
| Limits | | | | | |
| Limit | | | Condition | | |
| ≤ -20 dB / 100 kHz | | | Peak power measurement detector = Peak | | |
| ≤ -30 dB / 100 kHz | | | Peak power measurement detector = RMS | | |
| Test setup | | | | | |
| <div><div>Spectrum Analyzer</div><div>EUT</div></div> | | | | | |
| Test procedure | | | | | |
| 1. EUT set to test mode (Communication tester is used if needed) 2. Span set around lower band edge and detector is set to peak and max hold 3. Resolution bandwidth is set to 100 kHz 4. Markers are set to peak emission levels within frequency band and outside frequency band 5. Band edge attenuation is determined from level difference | | | | | |
| Test results | | | | | |
| Channel | Frequency [MHz] | Mode | Level [dBc] | Limit [dBc] | Margin [dB] |
| F _{LOW} | 2402 | Transmit | -40.61 | -20 | -20.61 |
| F _{HIGH} | 2480 | Transmit | -41.73 | -20 | -21.73 |
| Comments: | | | | | |

Band-edge compliance

FCC part 15.247

Band-edge compliance of RF conducted emissions

| | |
|-----------------------|--|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | FCC part 15 section 247(c) |
| Comment 1 | Band-edge compliance |
| Comment 2 | Channel.: 2402 MHz |
| Comment 3 | GFSK |

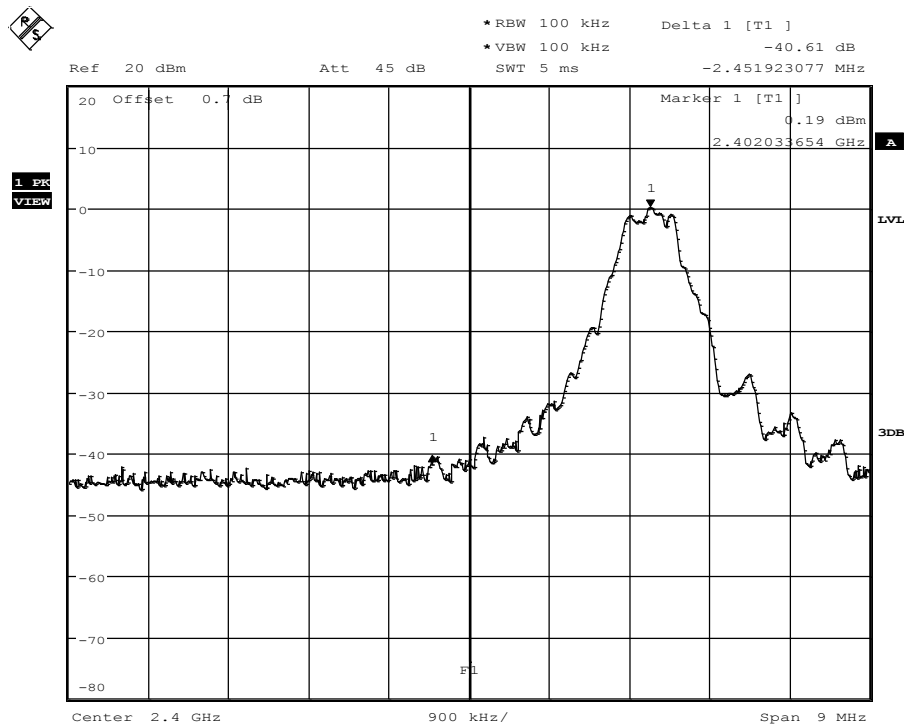

Limit: Marker Delta value >20 dB; Result: PASS


Date: 2.JUL.2013 14:07:14

Band-edge compliance

FCC part 15.247

Band-edge compliance of RF conducted emissions

| | |
|-----------------------|--|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | FCC part 15 section 247(c) |
| Comment 1 | Band-edge compliance |
| Comment 2 | Channel.: 2480 MHz |
| Comment 3 | GFSK |

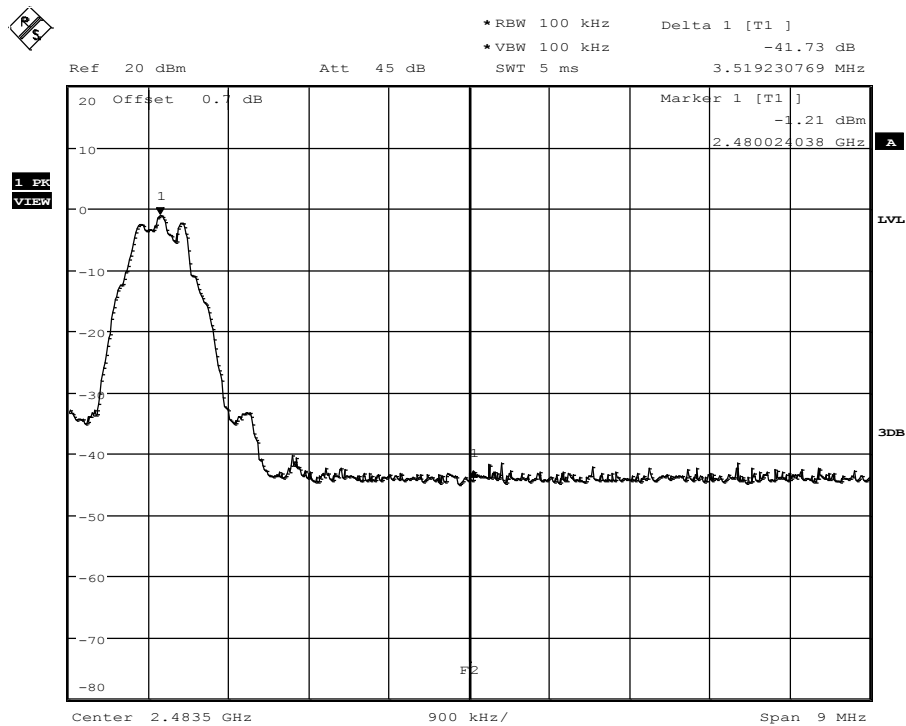

Limit: Marker Delta value >20 dB; Result: PASS

Date: 2.JUL.2013 14:05:01


3.7 Test Conditions and Results – Conducted spurious emissions

| Conducted spurious emissions acc. FCC 15.247 / IC RSS-210 | | | | | | Verdict: PASS | |
|--|-----------------|----------|------------------------------------|--|------------------|---------------|-------------|
| EUT requirement rule parts and clause | | | Reference | | | | |
| | | | FCC 15.247(d) / IC RSS-210 A8.5 | | | | |
| Test according to measurement reference | | | Reference Method | | | | |
| | | | FCC KDB Publication No. 558074 | | | | |
| Test frequency range | | | Tested frequencies | | | | |
| | | | 10 MHz – 10 th Harmonic | | | | |
| Measurement mode | | | Peak | | | | |
| Limits | | | | | | | |
| Limit | | | | Condition | | | |
| ≤ -20 dB / 100 kHz | | | | Peak power measurement detector = Peak | | | |
| ≤ -30 dB /100 kHz | | | | Peak power measurement detector = RMS | | | |
| Test setup | | | | | | | |
| <div><div>Spectrum Analyzer</div><div>EUT</div></div> | | | | | | | |
| Test procedure | | | | | | | |
| <div>1. EUT set to test mode (Communication tester is used if needed)</div> <div>2. Span it set according to measurement range</div> <div>3. Resolution bandwidth is set to 100 kHz and detector to peak and max hold</div> <div>4. Markers are set to peak emission levels within frequency band</div> <div>5. Emission level is determined by second marker on emission peak</div> <div>6. Attenuation is determined from level difference</div> | | | | | | | |
| Test results | | | | | | | |
| Channel | Frequency [MHz] | Mode | Emission [MHz] | Emission Level [dbm] | Peak power [dBm] | Limit [dBm] | Margin [dB] |
| F _{LOW} | 2402 | Transmit | 4800.74 | -41.72 | -0.16 | -20.16 | -21.56 |
| F _{MID} | 2440 | Transmit | 4884.78 | -41.70 | -1.43 | -21.4 | -20.30 |
| F _{HIGH} | 2480 | Transmit | 4968.83 | -40.09 | -1.77 | -21.8 | -18.29 |
| Comments: | | | | | | | |

Conducted spurious emissions – F_{Low}

FCC part 15.247 (d)
Spurious Emissions


EUT Electronic Auto-injector
Model betaCONNECT
Approval Holder Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage Tnom / Vnom
Test Site / Operator Eurofins Product Service GmbH / Mr. Treffke
Test Specification FCC part 15.247 (d)
Comment 1 Spurious Emissions conducted
Comment 2 Channel 2402 MHz
Comment 3 Emissions in non-restricted frequency bands 558074 D01 Meas Guidance

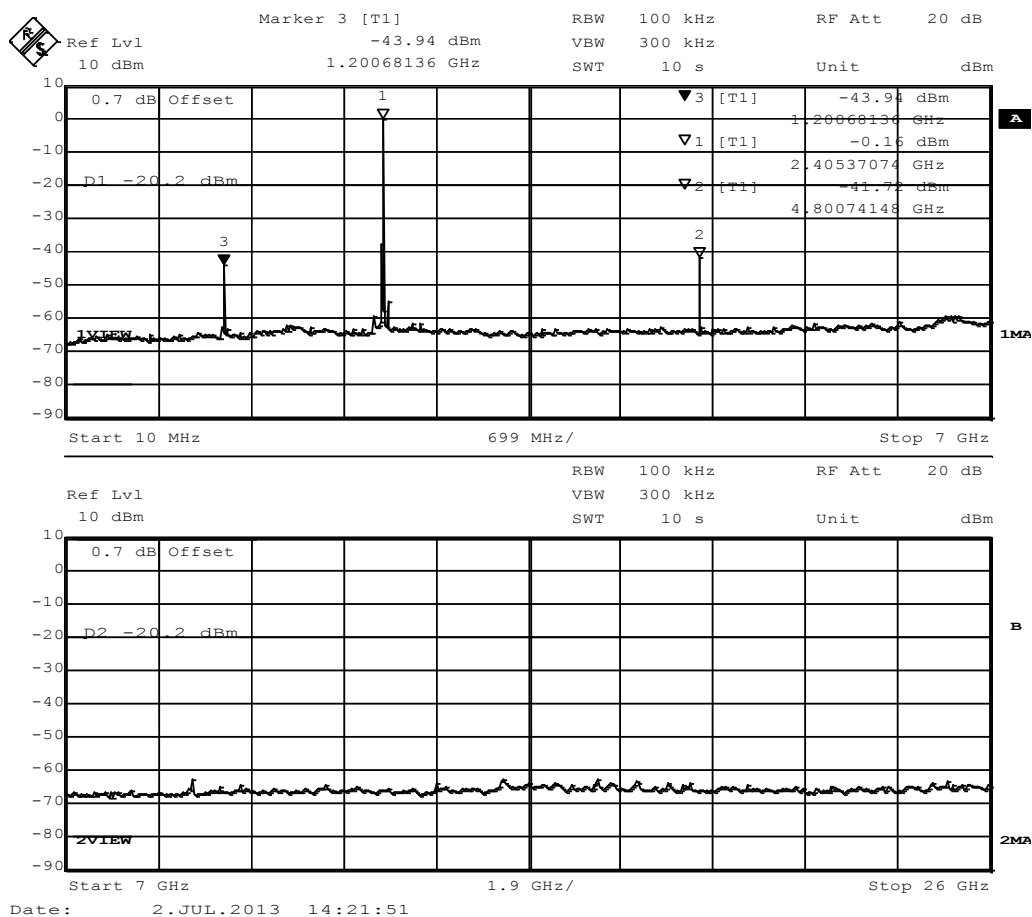

Conducted spurious emissions – F_{MID}

FCC part 15.247 (d)
Spurious Emissions


| | |
|-----------------------|--|
| EUT | Electronic Auto-injector |
| Model | betaCONNECT |
| Approval Holder | Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859 |
| Temperature / Voltage | Tnom / Vnom |
| Test Site / Operator | Eurofins Product Service GmbH / Mr. Treffke |
| Test Specification | FCC part 15.247 (d) |
| Comment 1 | Spurious Emissions conducted |
| Comment 2 | Channel 2440 MHz |
| Comment 3 | Emissions in non-restricted frequency bands 558074 D01 Meas Guidance |

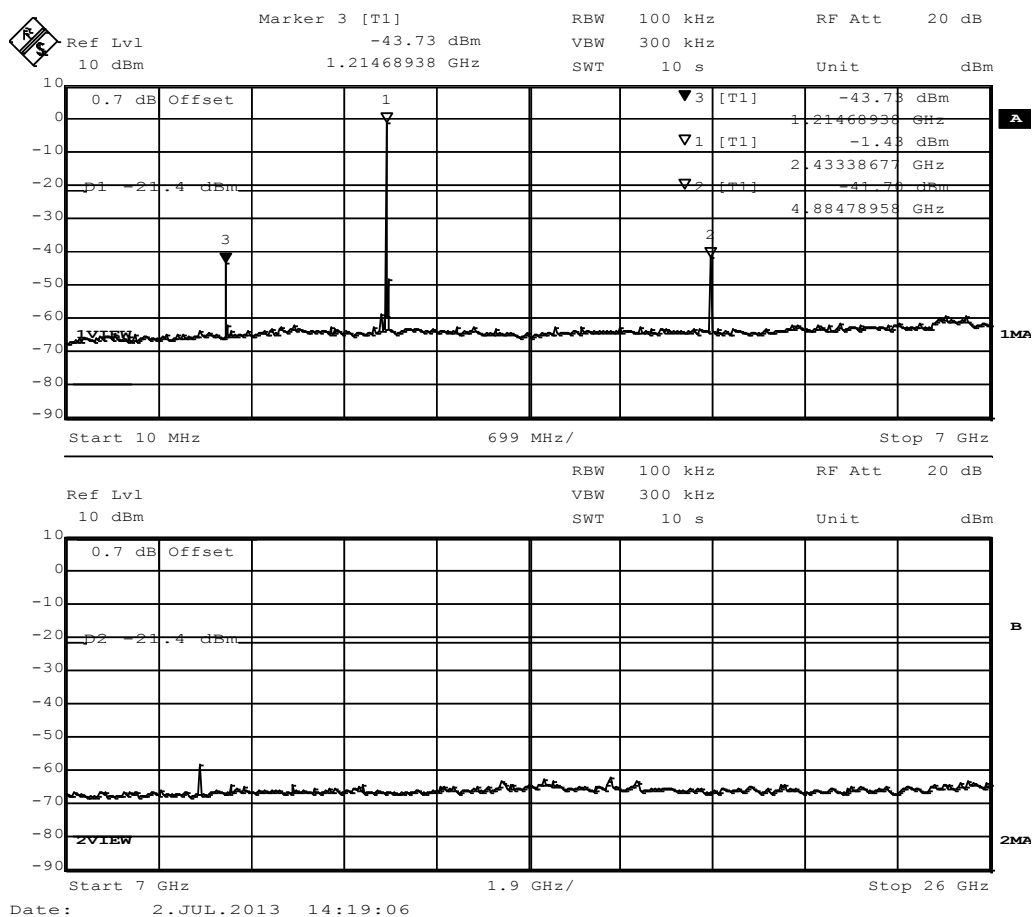

Conducted spurious emissions – F_{HIGH}

FCC part 15.247 (d)
Spurious Emissions


EUT Electronic Auto-injector
Model betaCONNECT
Approval Holder Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage Tnom / Vnom
Test Site / Operator Eurofins Product Service GmbH / Mr. Treffke
Test Specification FCC part 15.247 (d)
Comment 1 Spurious Emissions conducted
Comment 2 Channel 2480 MHz
Comment 3 Emissions in non-restricted frequency bands 558074 D01 Meas Guidance

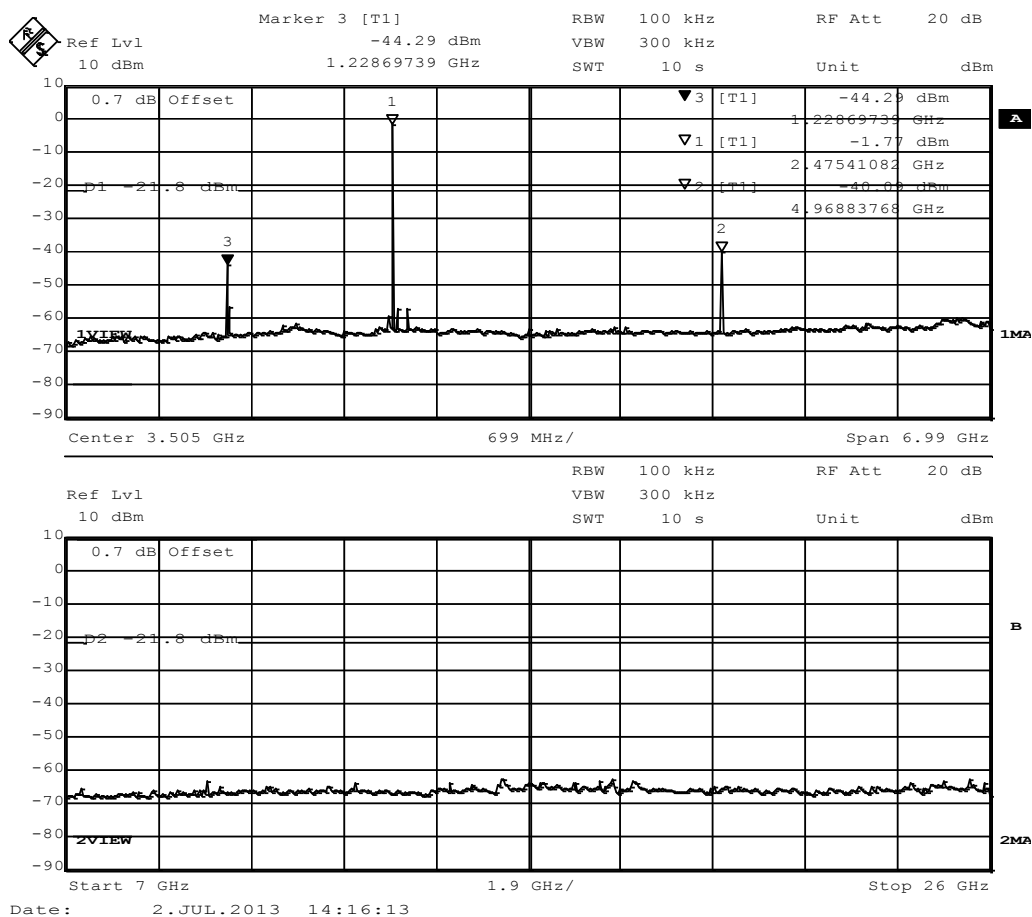

3.8 Test Conditions and Results – Transmitter radiated emissions


| Transmitter radiated emissions acc. FCC 47 CFR 15.247 / IC RSS-210 | | | | Verdict: PASS |
|--|---|--------------|----------------|--------------------|
| Test according referenced standards | Reference Method | | | |
| | FCC 15.247(d) / IC RSS-210 A8.5 | | | |
| Test according to measurement reference | Reference Method | | | |
| | FCC KDB Publication No. 558074 / ANSI C63.4 | | | |
| Test frequency range | Tested frequencies | | | |
| | 30 MHz – 10 th Harmonic | | | |
| Limits | | | | |
| Frequency range [MHz] | Detector | Limit [µV/m] | Limit [dBµV/m] | Limit Distance [m] |
| 30 – 88 | Quasi-Peak | 100 | 40 | 3 |
| 88 – 216 | Quasi-Peak | 150 | 43.5 | 3 |
| 216 – 960 | Quasi-Peak | 200 | 46 | 3 |
| 960 – 1000 | Quasi-Peak | 500 | 54 | 3 |
| > 1000 | Average | 500 | 54 | 3 |

Radiated emissions which fall in the restricted bands, as defined in Section 15.205(a), must also comply with the radiated emission limits specified in Section 15.209(a) (see Section 15.205(c)). When average radiated emission measurements are specified, including average emission measurements below 1000 MHz, there also is a limit on the peak level of the radio frequency emissions. The limit on peak radio frequency emissions is 20 dB above the maximum permitted average emission limit applicable to the equipment under test.
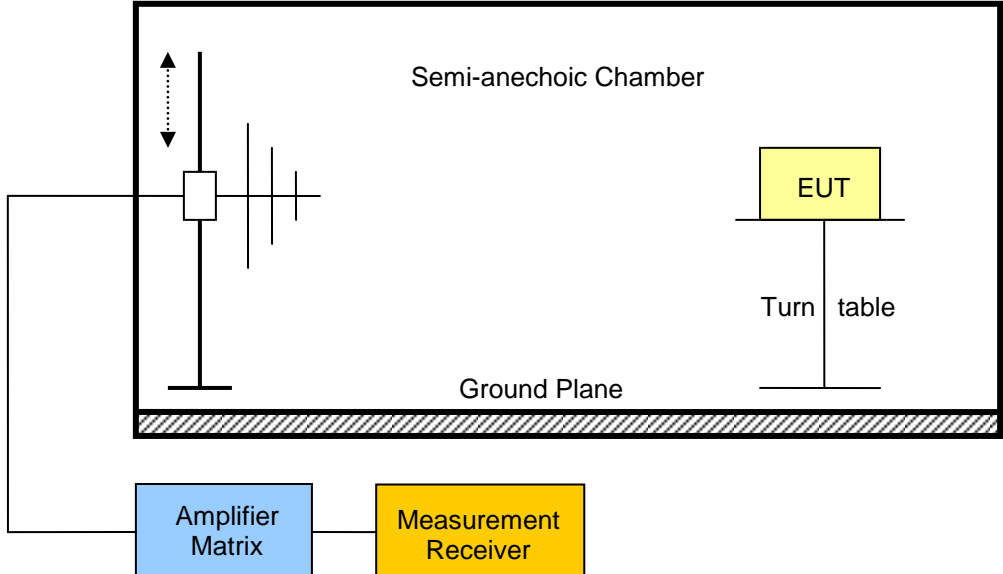
| Test setup | |
|--|--|
|  | |

| Test procedure | | | | | | | | | |
|---|-----------------|----------|----------------|----------------|------|------|----------------|------------------|-------------|
| <ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Markers are set to peak emission levels within restricted bands | | | | | | | | | |
| Test results | | | | | | | | | |
| Channel | Frequency [MHz] | Mode | Emission [MHz] | Level [dBμV/m] | Det. | Pol. | Limit [dBμV/m] | Limit dist. [m]* | Margin [dB] |
| F _{LOW} | 2402 | Transmit | 37.804 | 31.02 | pk | ver | 40.00 | 3 | -08.98 |
| F _{LOW} | 2402 | Transmit | 2336 | 37.94 | pk | hor | 74.00 | 3 | -36.06 |
| F _{LOW} | 2402 | Transmit | 4804 | 54.81 | pk | hor | 74.00 | 3 | -19.19 |
| F _{LOW} | 2402 | Transmit | 4804 | 53.00 | avg | hor | 54.00 | 3 | -01.00 |
| F _{LOW} | 2402 | Transmit | 4804 | 52.68 | pk | ver | 74.00 | 3 | -21.32 |
| F _{LOW} | 2402 | Transmit | 4804 | 50.31 | avg | ver | 54.00 | 3 | -03.69 |
| F _{MID} | 2440 | Transmit | 4880 | 51.60 | pk | ver | 74.00 | 3 | -22.40 |
| F _{MID} | 2440 | Transmit | 4880 | 48.82 | avg | ver | 54.00 | 3 | -05.18 |
| F _{HIGH} | 2480 | Transmit | 2483.5 | 46.20 | pk | hor | 74.00 | 3 | -27.80 |
| Comments: | | | | | | | | | |

3.9 Test Conditions and Results – Receiver radiated emissions
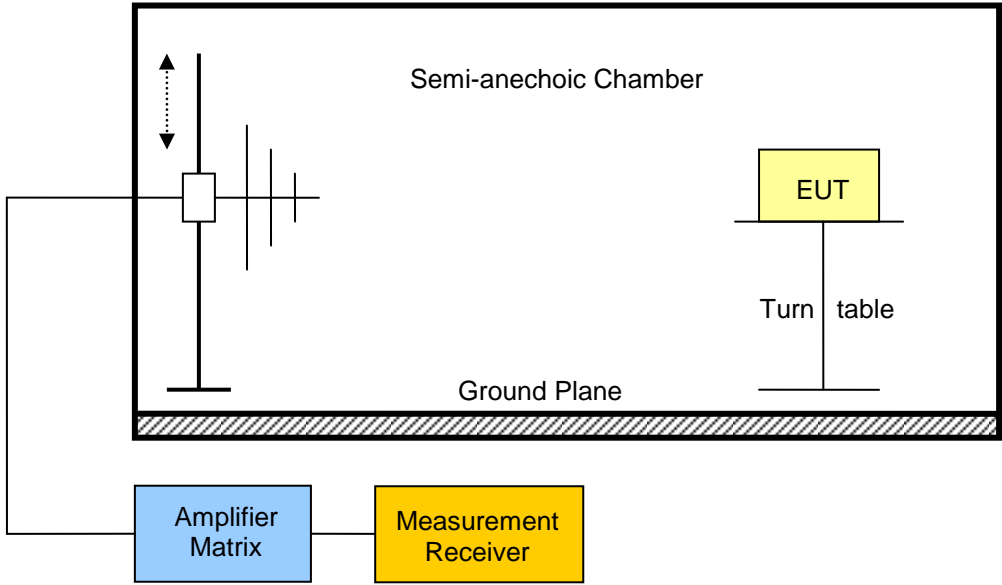
| Receiver radiated emissions acc. IC RSS-210 | | | | Verdict: PASS |
|--|-----------------------------------|--------------|----------------|--------------------|
| Test according referenced standards | Reference Method | | | |
| | IC RSS-210 A8.5 | | | |
| Test according to measurement reference | Reference Method | | | |
| | ANSI C63.4 | | | |
| Test frequency range | Tested frequencies | | | |
| | 30 MHz – 3 th Harmonic | | | |
| EUT test mode | Receive | | | |
| Limits | | | | |
| Frequency range [MHz] | Detector | Limit [µV/m] | Limit [dBµV/m] | Limit Distance [m] |
| 30 – 88 | Quasi-Peak | 100 | 40 | 3 |
| 88 – 216 | Quasi-Peak | 150 | 43.5 | 3 |
| 216 – 960 | Quasi-Peak | 200 | 46 | 3 |
| 960 – 1000 | Quasi-Peak | 500 | 54 | 3 |
| > 1000 | Average | 500 | 54 | 3 |
| Test setup | | | | |
|  | | | | |

| Test procedure | | | | | | | |
|--|-----------------|----------------|-------------------------------|-----------------------------|------|--------------------|---------------------|
| <ol style="list-style-type: none"> 1. EUT set to receive mode (Communication tester is used if needed) 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Markers are set to peak emission levels | | | | | | | |
| Test results | | | | | | | |
| Channel | Frequency [MHz] | Emission [MHz] | Emission Level [dB μ V/m] | Emission Level [μ V/m] | Det. | Limit [μ V/m] | Margin [μ V/m] |
| F _{MID} | 2440 | 32.715 | 31.65 | 38.24 | pk | 100 | -61.76 |
| F _{MID} | 2440 | 59.86 | 34.24 | 51.52 | pk | 100 | -48.48 |
| F _{MID} | 2440 | 551.297 | 27.33 | 23.25 | pk | 200 | -176.75 |
| F _{MID} | 2440 | 575.25 | 26.43 | 20.97 | pk | 200 | -179.03 |
| Comments: * Physical distance between EUT and measurement antenna. ** Emission level corresponds to ambient noise floor | | | | | | | |


ANNEX A Transmitter radiated spurious emissions

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

| | |
|-----------------------|---|
| Manufacturer: | Bang & Olufsen Medicom A/S |
| EUT Name: | Electronic Auto-injector |
| Model: | betaCONNECT |
| Test Site: | Eurofins Product Service GmbH |
| Operator: | Mr. Treffke |
| Test Conditions: | Tnom: 20°C, Vnom: 3.7V DC lithium battery |
| Antenna: | Rohde & Schwarz HK 116, Horizontal |
| Measurement distance: | 3 m |
| Mode: | TX; ch. 0 |
| Test Date: | 2013-07-03 |
| Note: | worst case |

Index 74

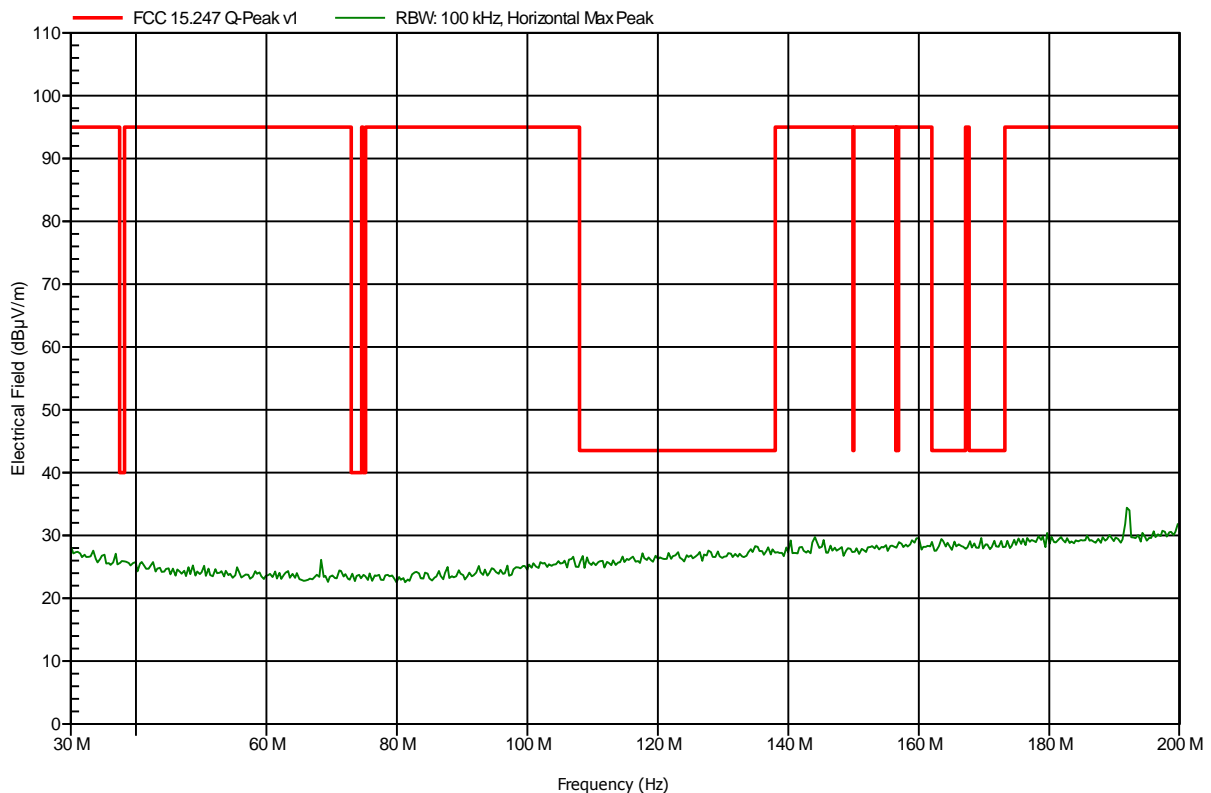


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HK 116, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note: worst case

Index 75

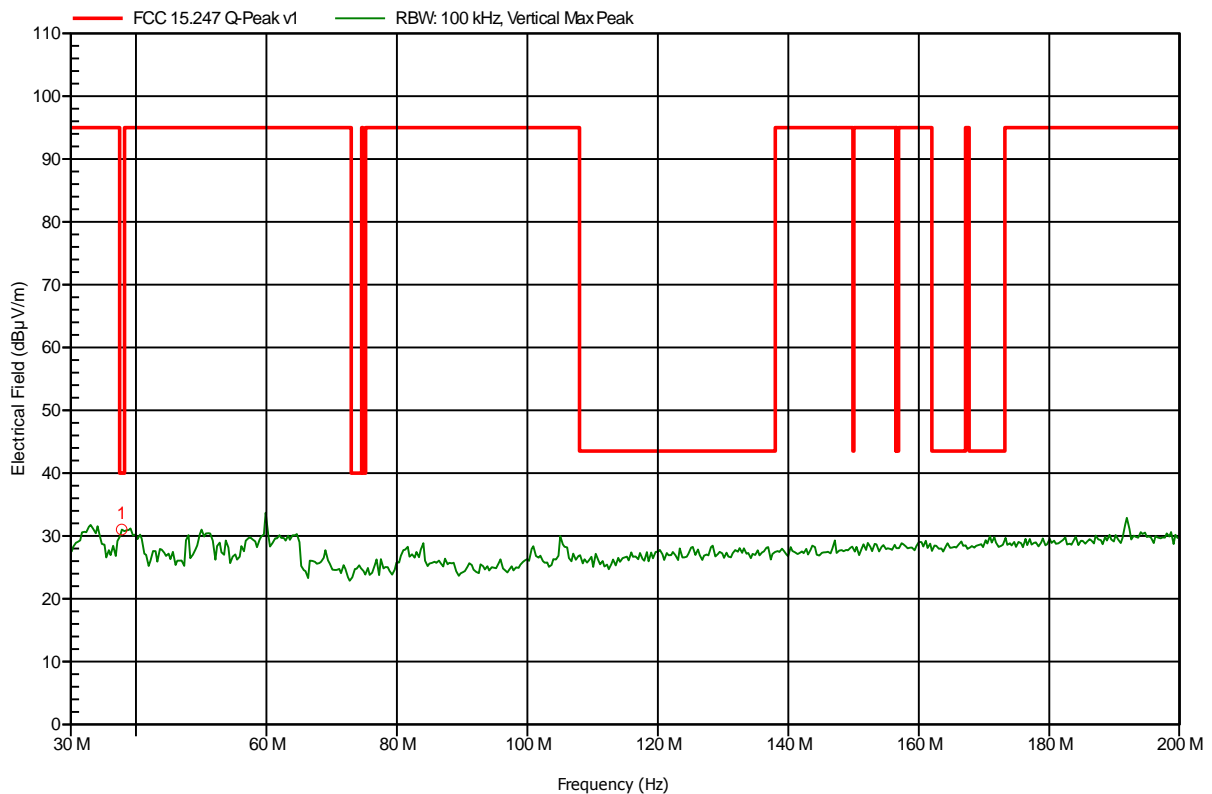


| Frequency | Peak | Peak Limit | Peak Difference | Peak Status |
|------------|--------------|------------|-----------------|-------------|
| 37.804 MHz | 31.02 dBµV/m | 40 dBµV/m | -8.98 dB | Pass |

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

| | |
|-----------------------|---|
| Manufacturer: | Bang & Olufsen Medicom A/S |
| EUT Name: | Electronic Auto-injector |
| Model: | betaCONNECT |
| Test Site: | Eurofins Product Service GmbH |
| Operator: | Mr. Treffke |
| Test Conditions: | Tnom: 20°C, Vnom: 3.7V DC lithium battery |
| Antenna: | Rohde & Schwarz HL 223, Horizontal |
| Measurement distance: | 3 m |
| Mode: | TX; ch. 0 |
| Test Date: | 2013-07-03 |
| Note: | |

Index 71

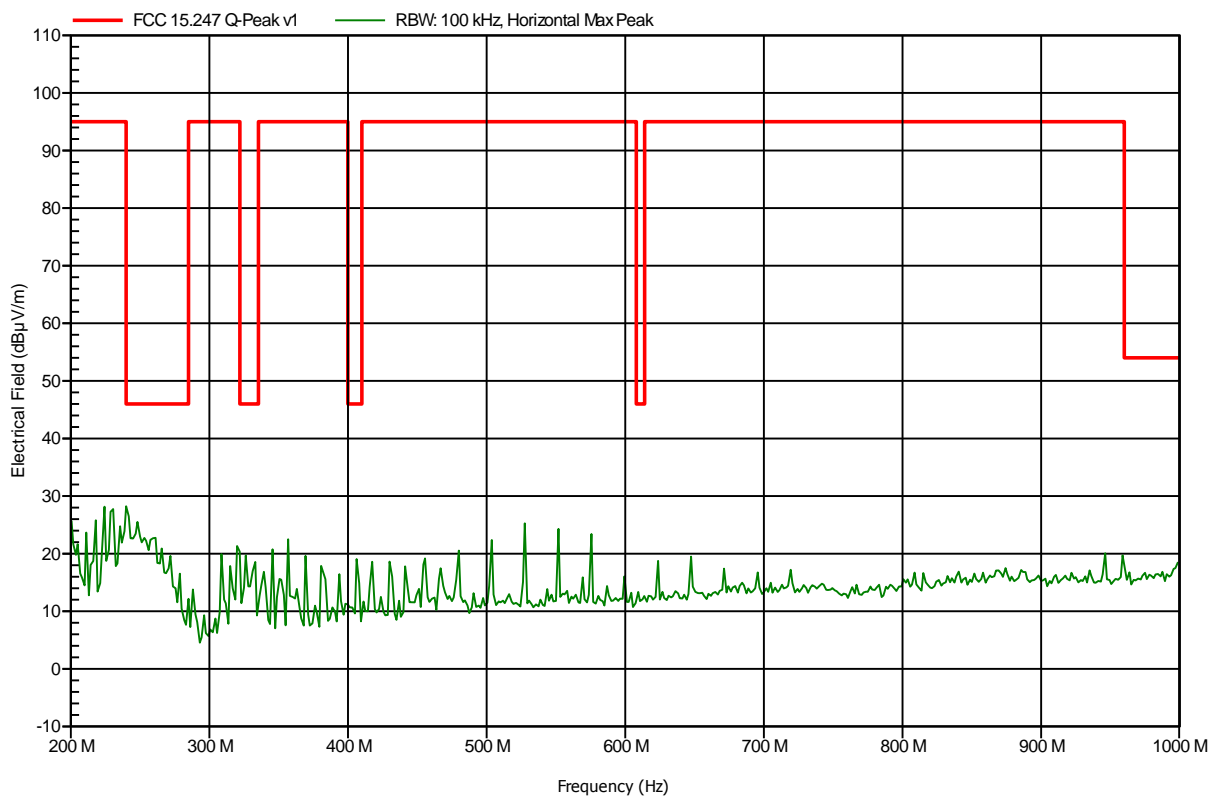


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 223, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 68

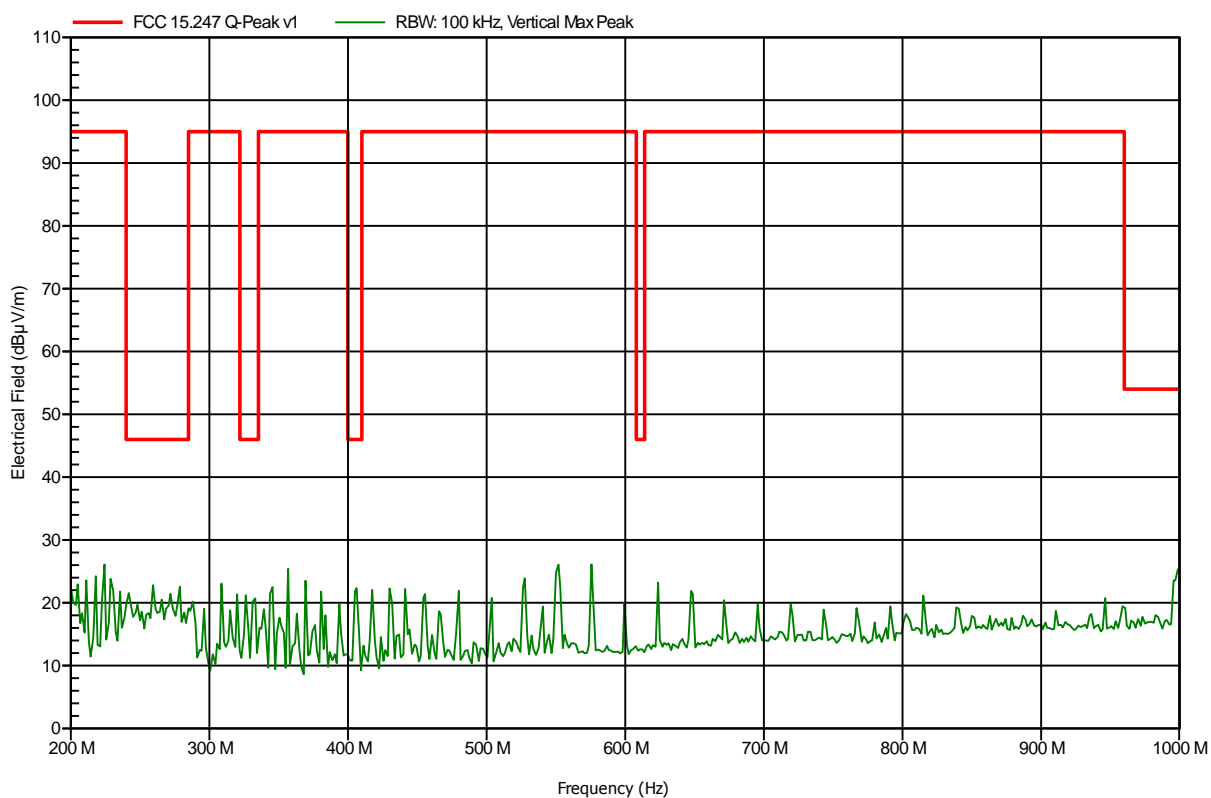


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 41

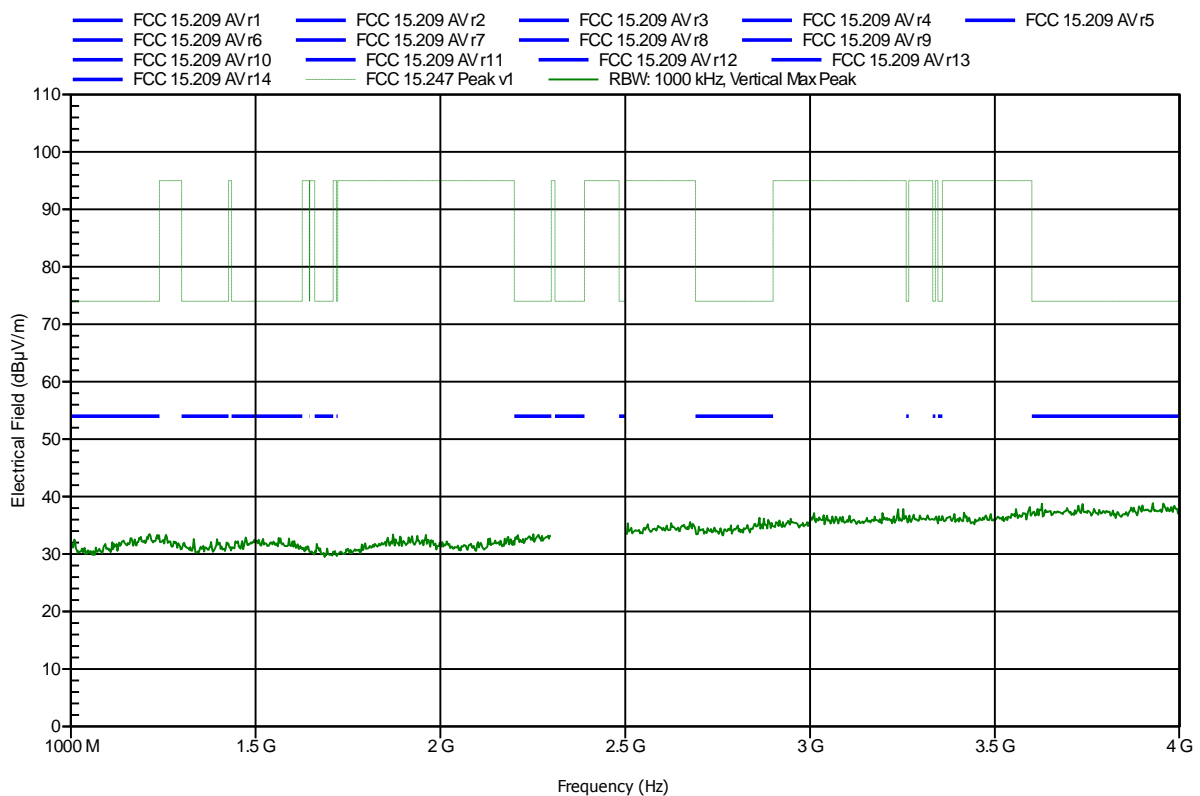


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 38

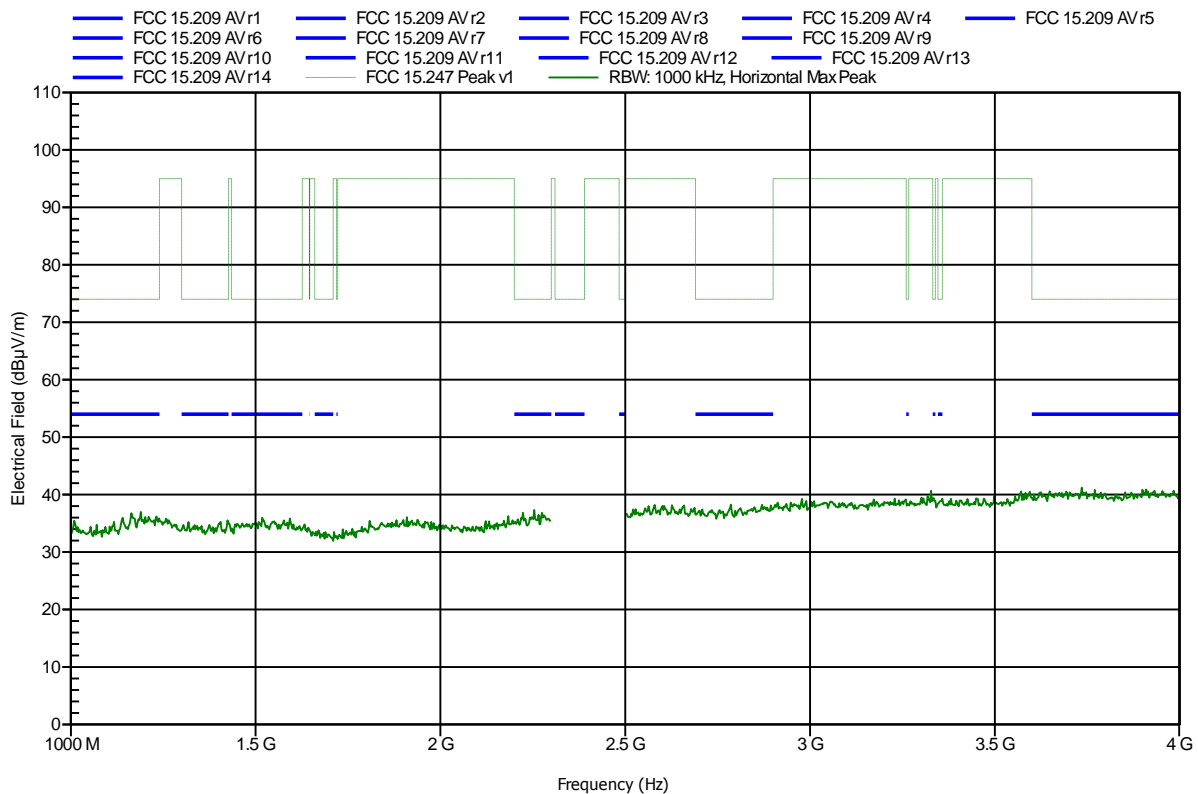


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note: lower bandedge

Index 39

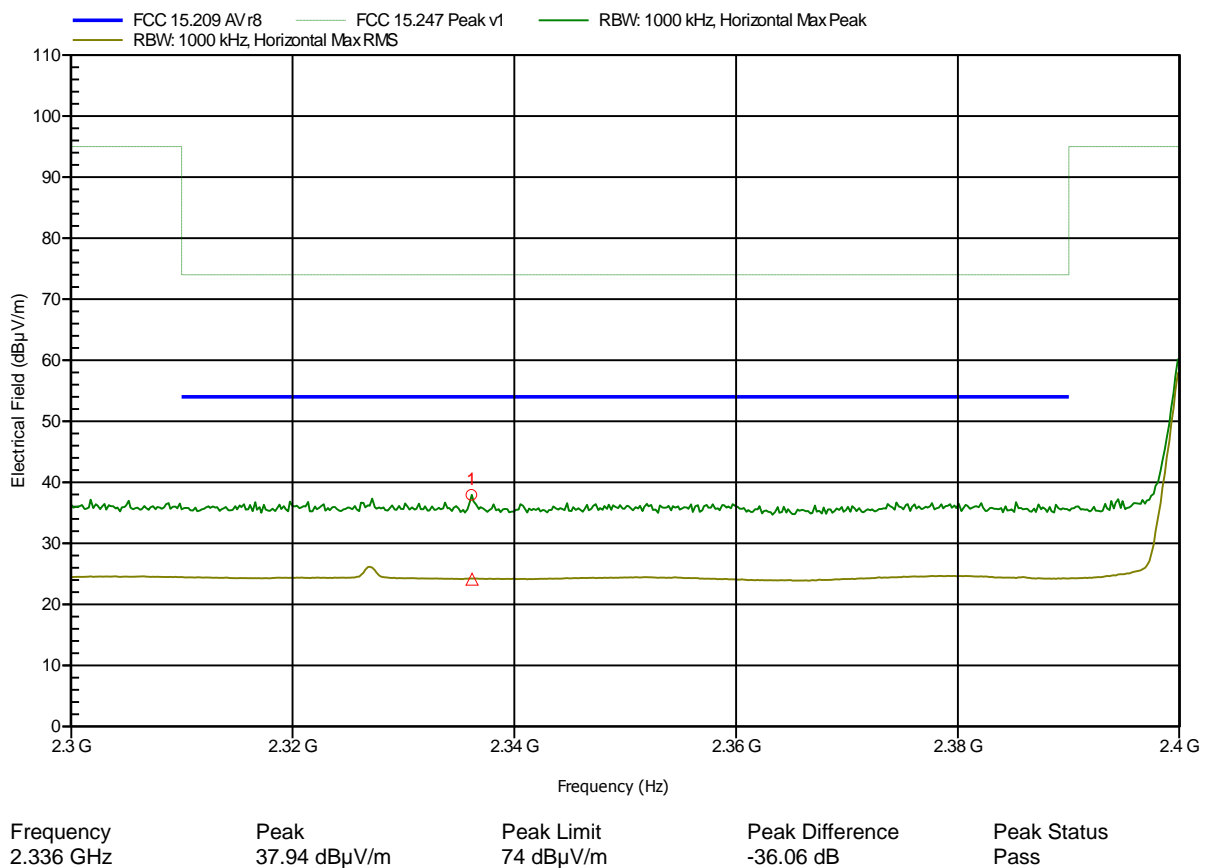


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note: lower bandedge

Index 42

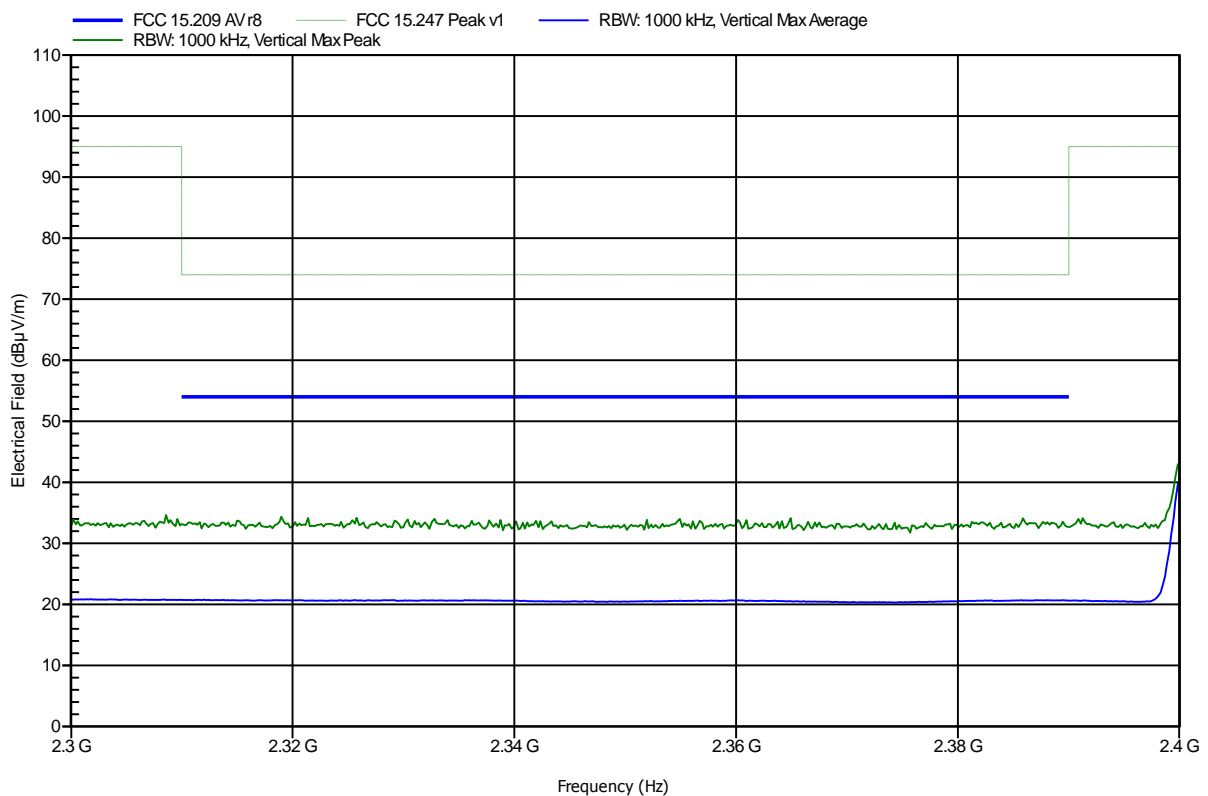


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 40

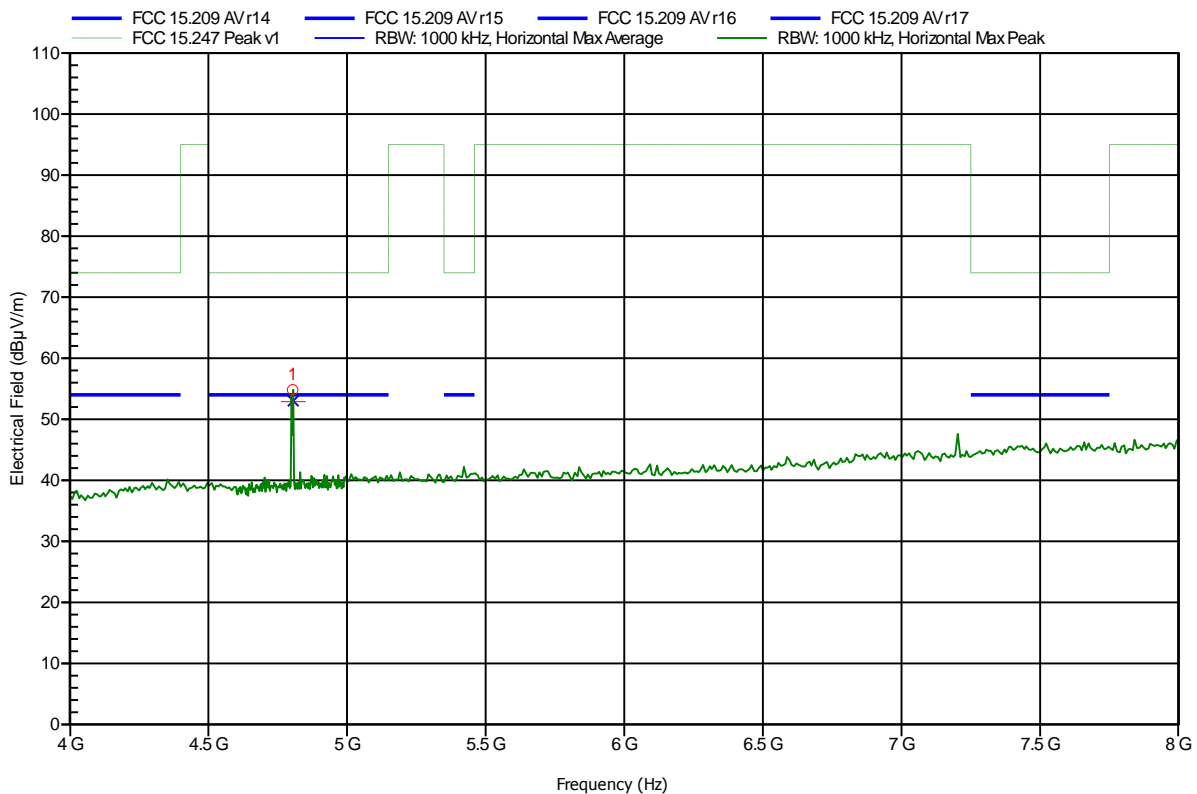


| | | | | |
|------------------------|----------------------|----------------------------|------------------------------|------------------------|
| Frequency 4.804 GHz | Peak 54.81 dBuV/m | Peak Limit 74 dBuV/m | Peak Difference -19.19 dB | Peak Status Pass |
| Frequency 4.804 GHz | Average 53 dBuV/m | Average Limit 54 dBuV/m | Average Difference -1 dB | Average Status Pass |

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 43

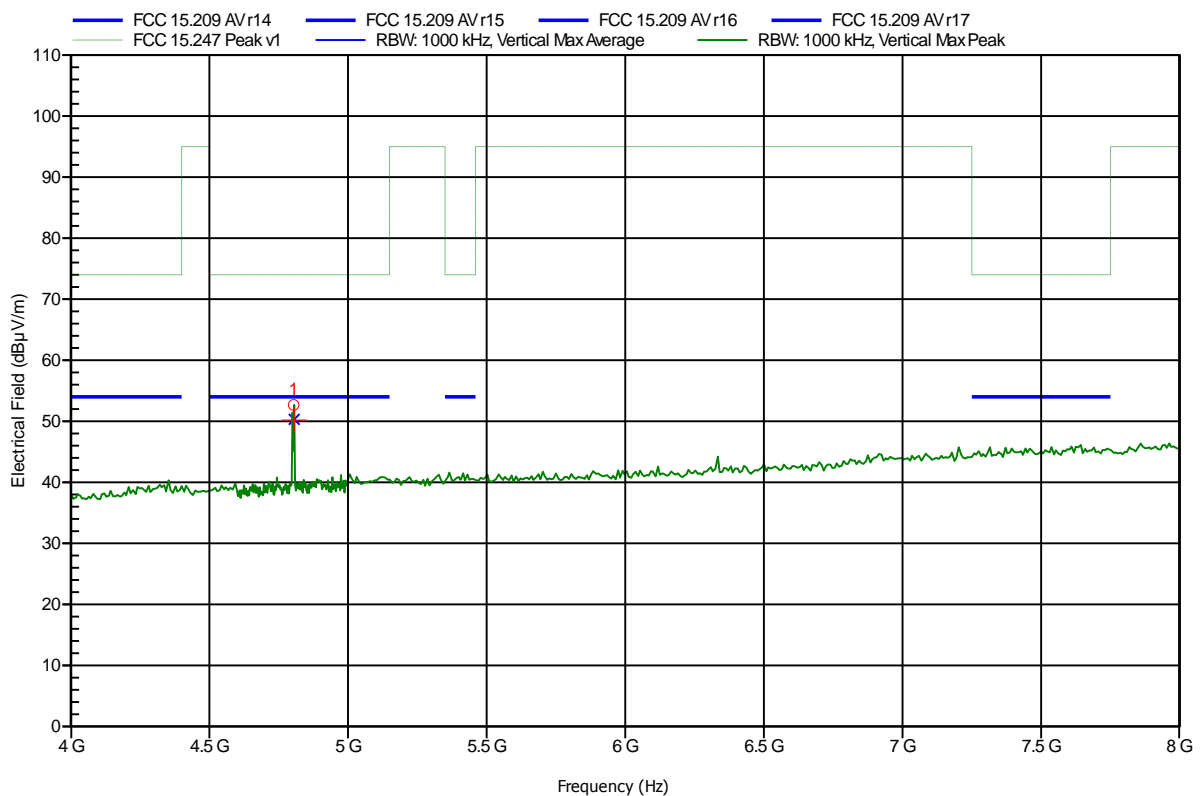


| | | | | |
|------------------------|-------------------------|----------------------------|--------------------------------|------------------------|
| Frequency 4.804 GHz | Peak 52.68 dBuV/m | Peak Limit 74 dBuV/m | Peak Difference -21.32 dB | Peak Status Pass |
| Frequency 4.804 GHz | Average 50.31 dBuV/m | Average Limit 54 dBuV/m | Average Difference -3.69 dB | Average Status Pass |

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 54

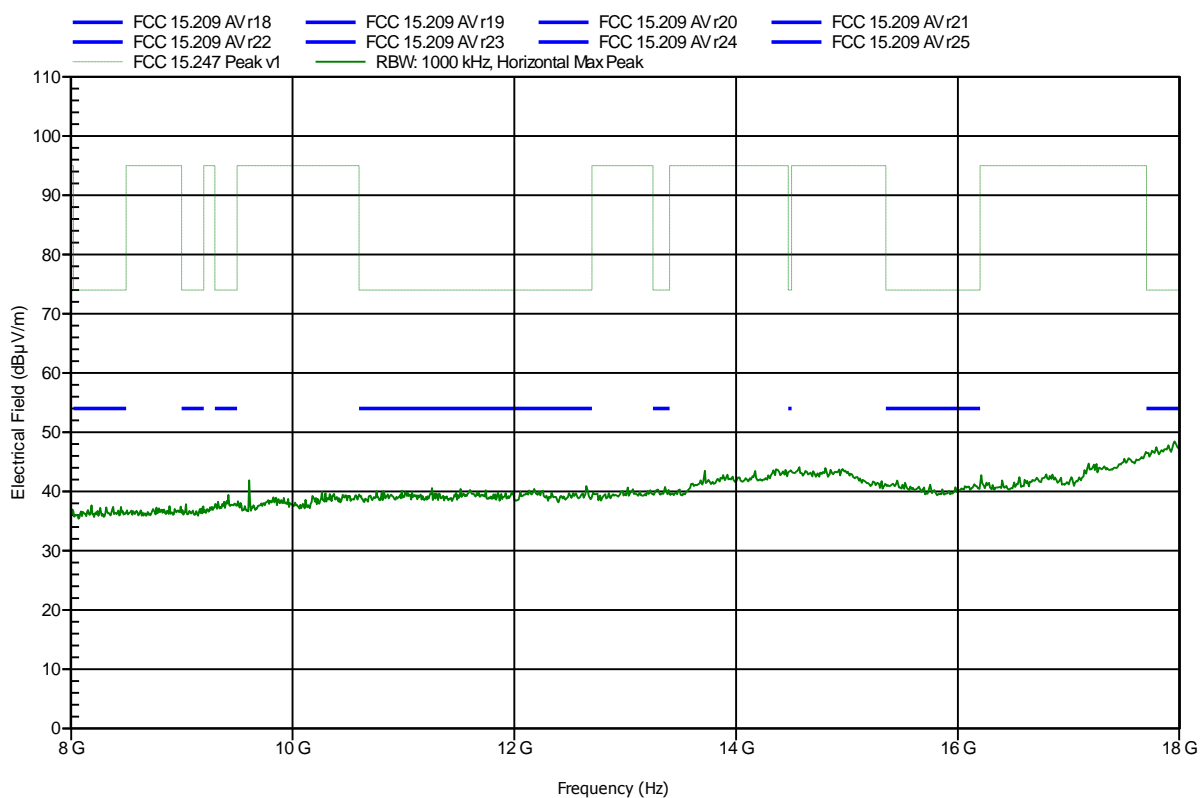


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 56

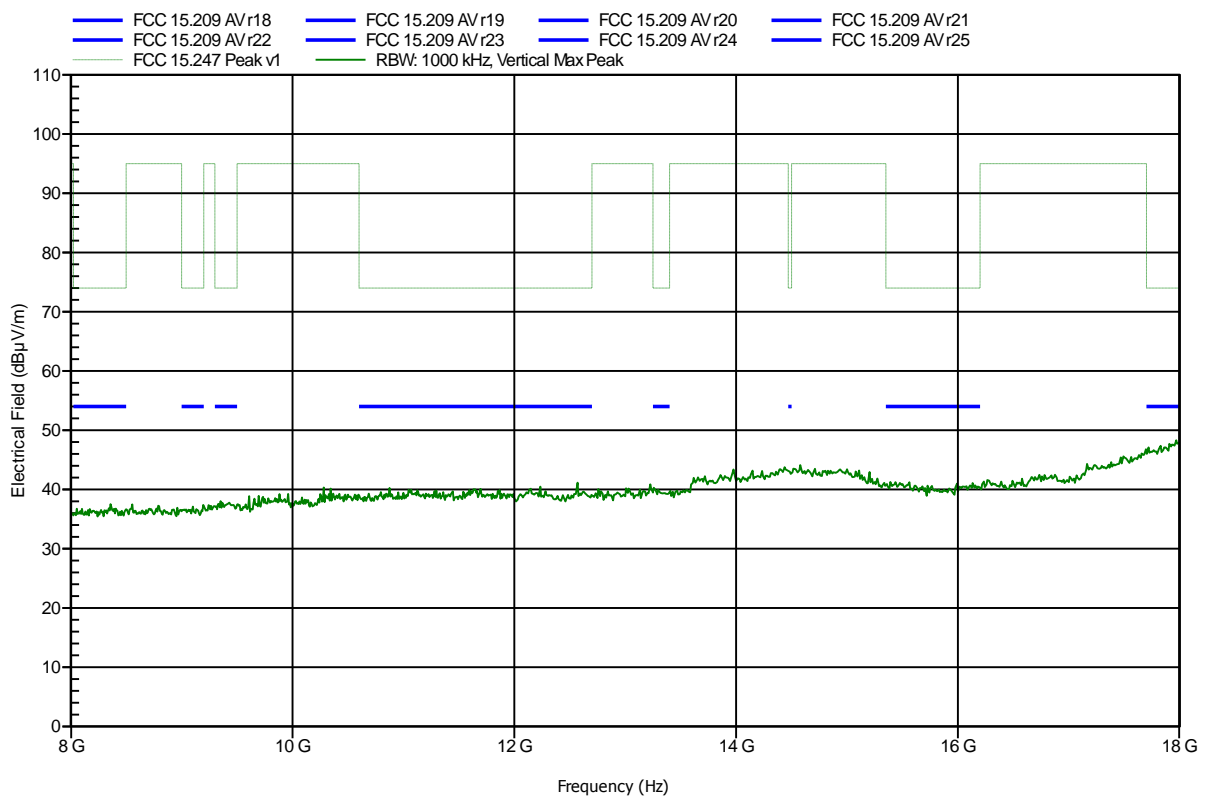


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Horizontal
 Measurement distance: 100 cm
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 55

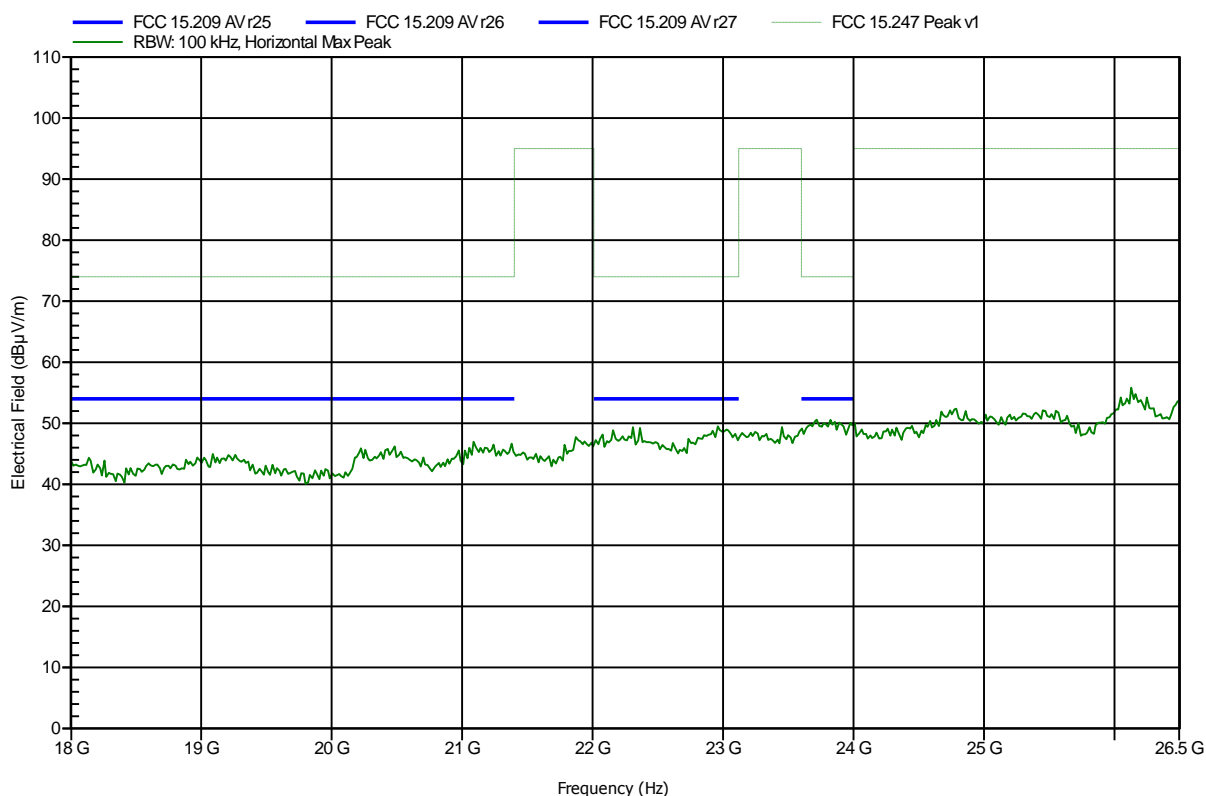


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Vertical
 Measurement distance: 100 cm
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 57

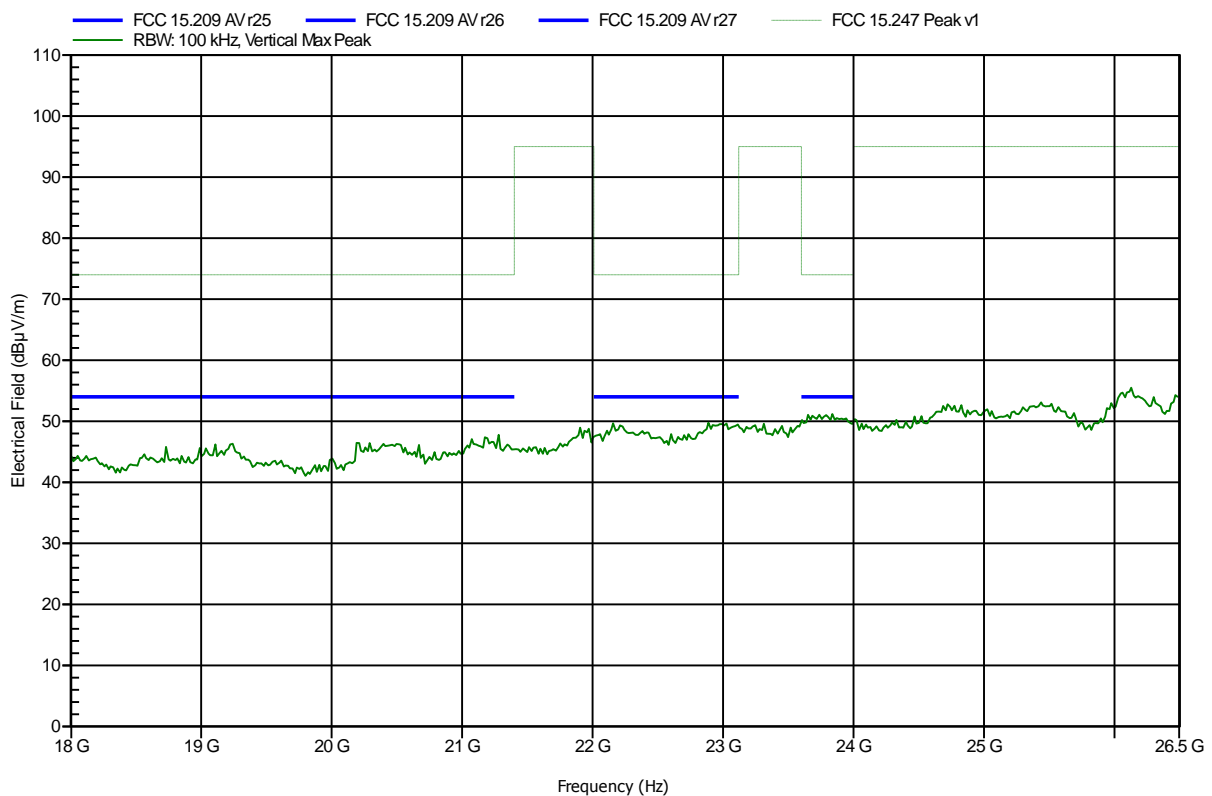


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

| | |
|-----------------------|---|
| Manufacturer: | Bang & Olufsen Medicom A/S |
| EUT Name: | Electronic Auto-injector |
| Model: | betaCONNECT |
| Test Site: | Eurofins Product Service GmbH |
| Operator: | Mr. Treffke |
| Test Conditions: | Tnom: 20°C, Vnom: 3.7V DC lithium battery |
| Antenna: | Rohde & Schwarz HL 223, Horizontal |
| Measurement distance: | 3 m |
| Mode: | TX; ch. 19 |
| Test Date: | 2013-07-03 |
| Note: | |

Index 70

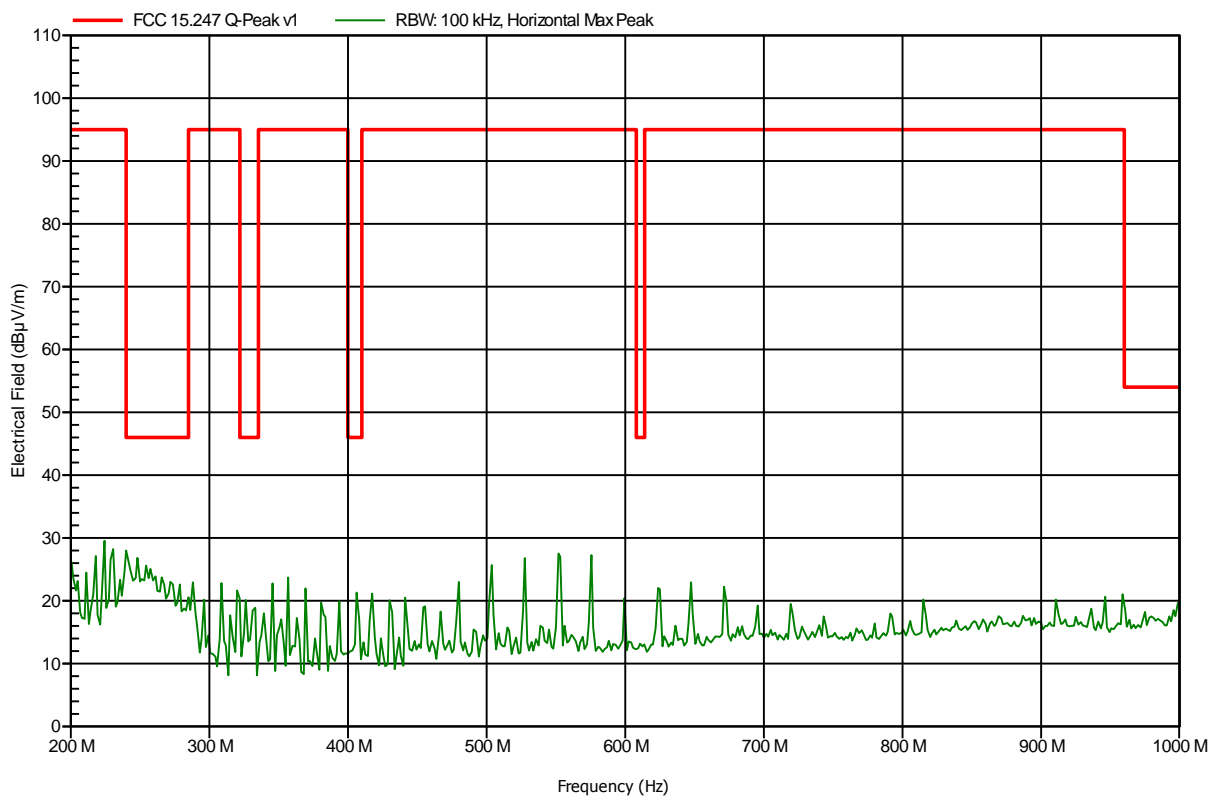


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 223, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 69

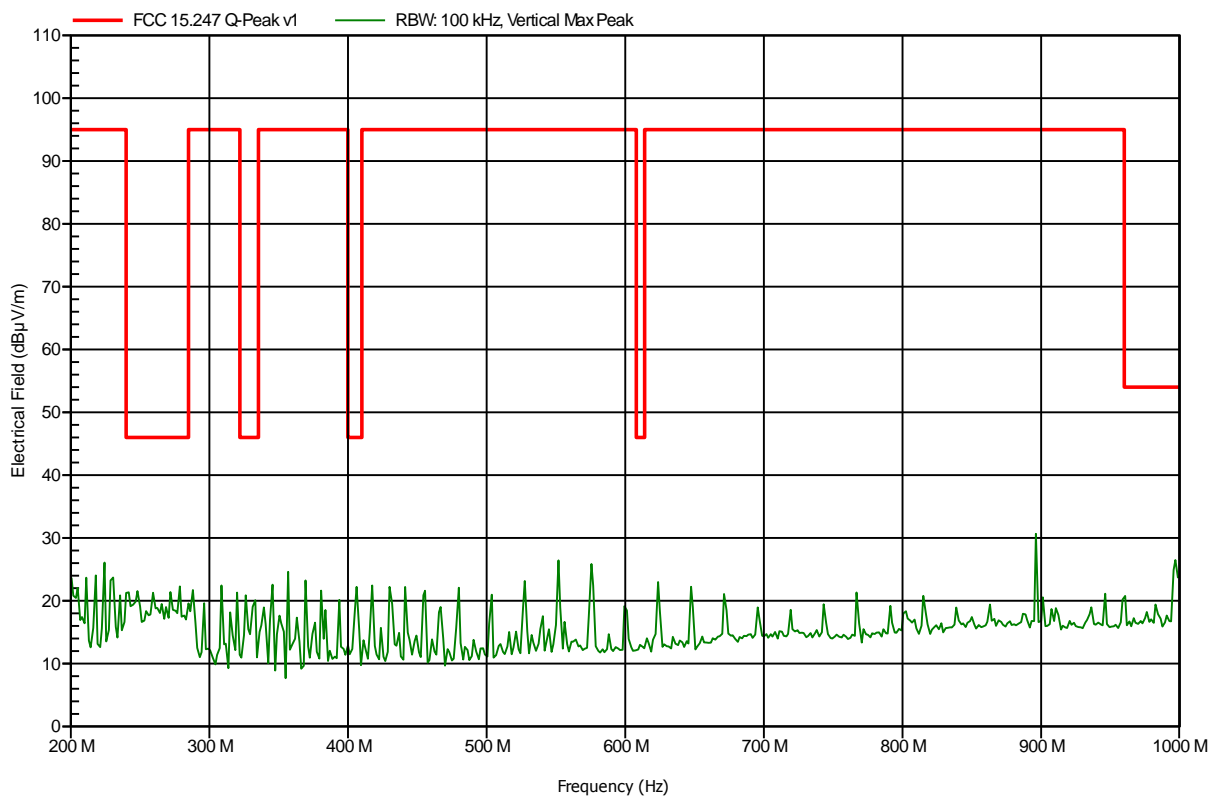


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 44

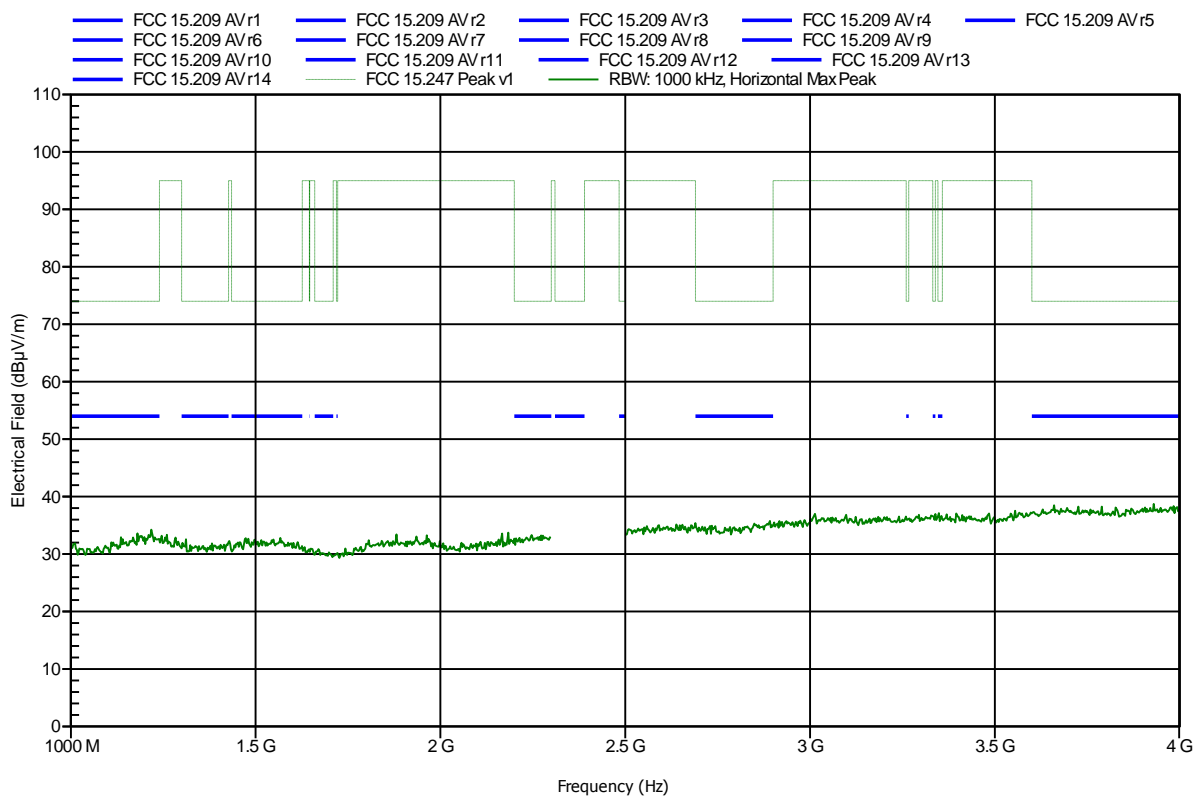


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 46

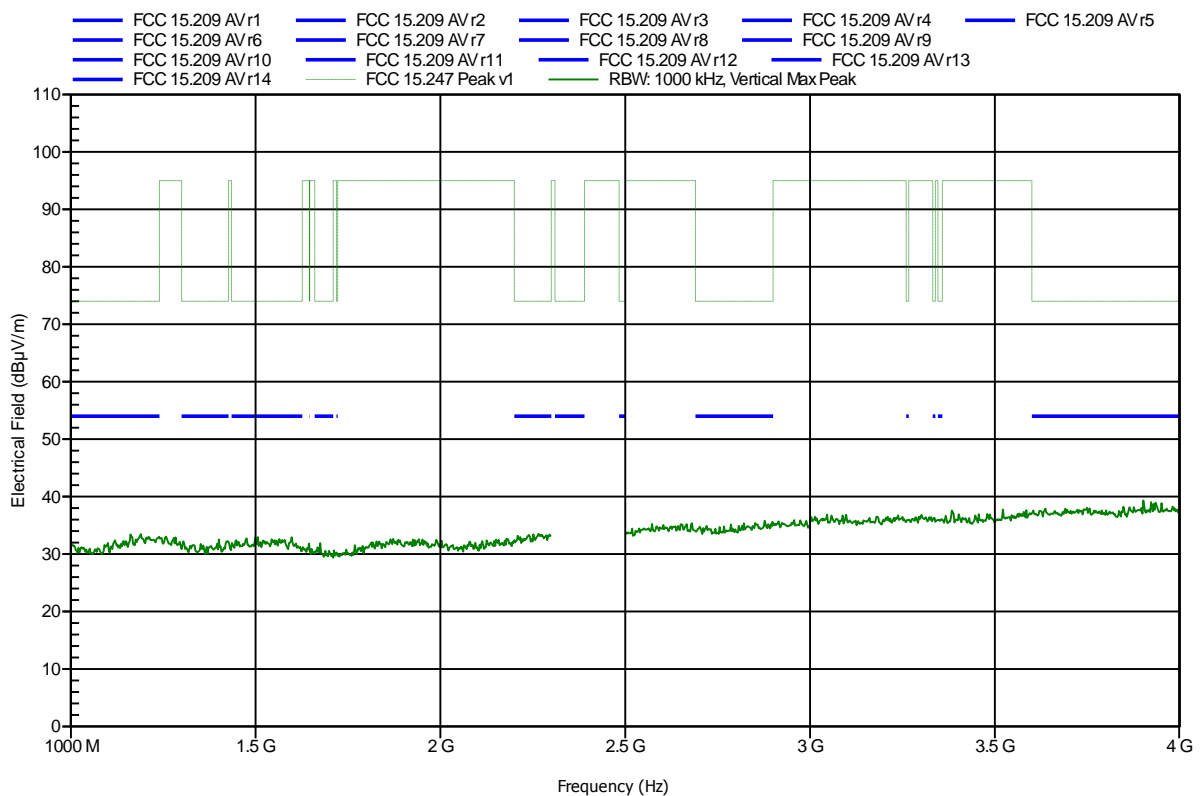


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 45

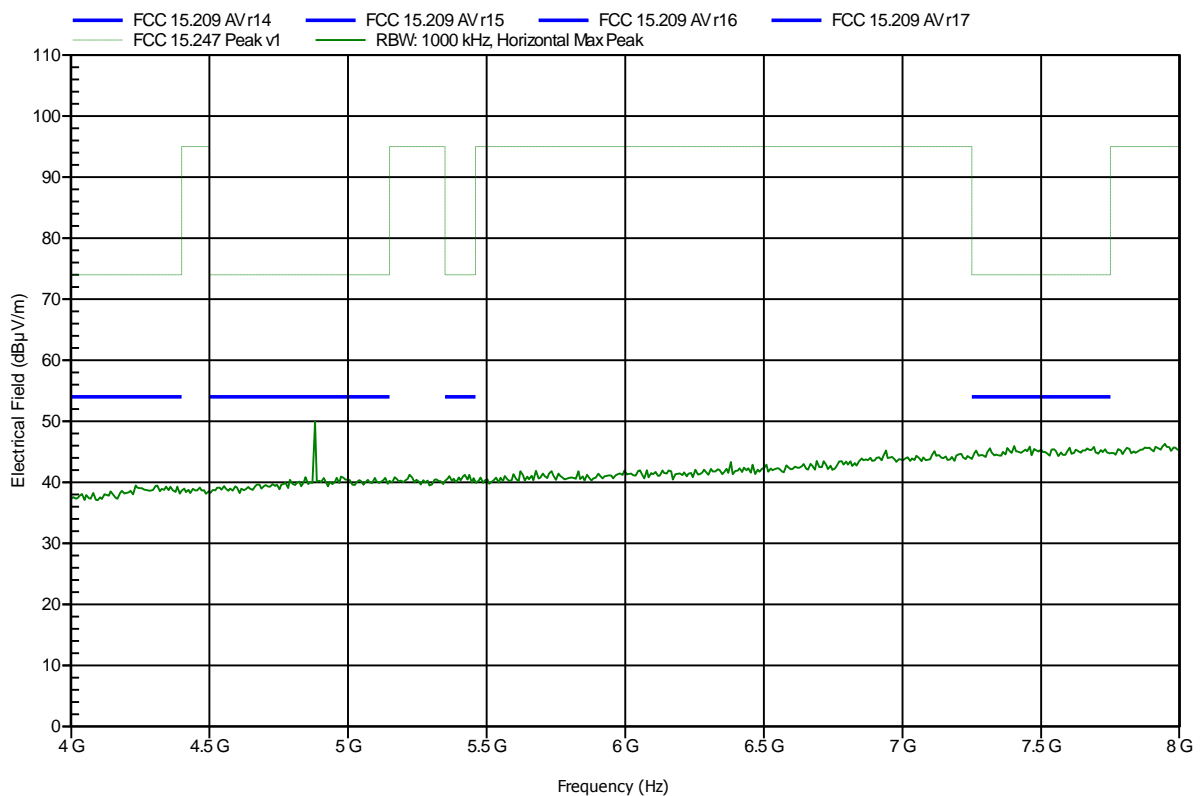


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 47

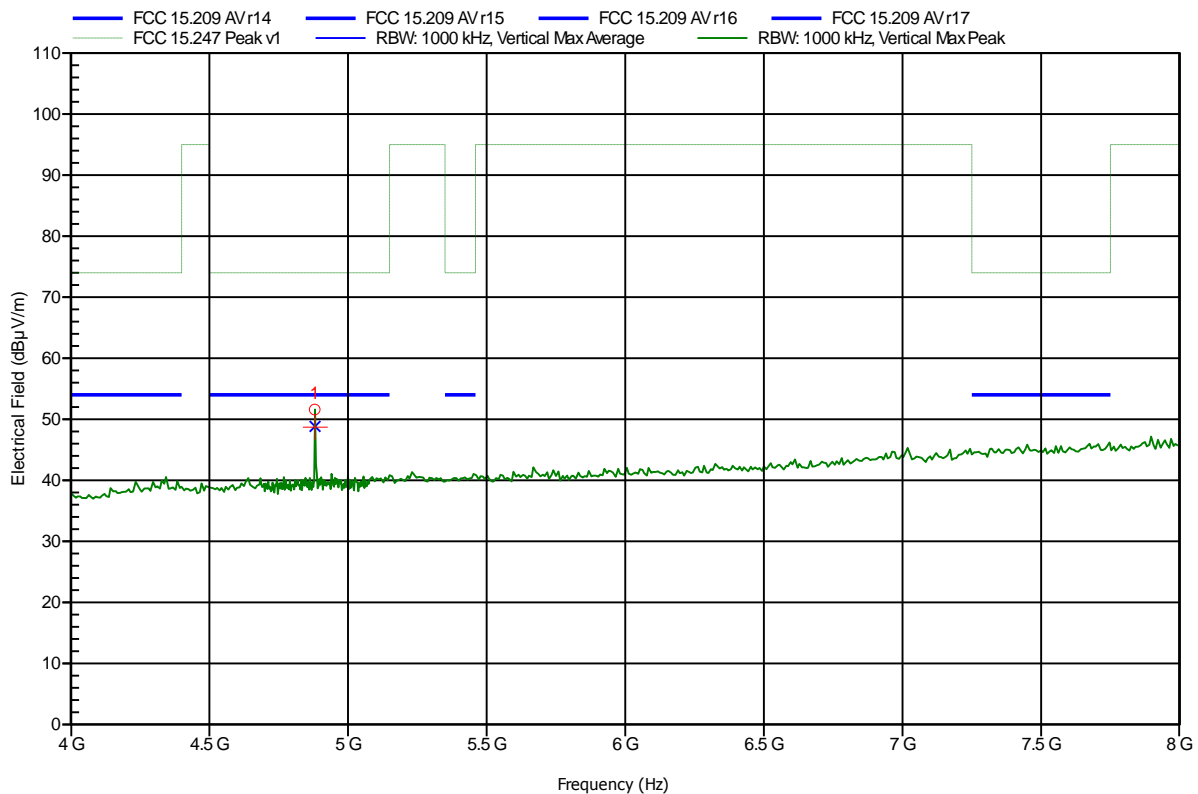


| | | | | |
|-----------------------|-------------------------------|----------------------------------|--------------------------------|------------------------|
| Frequency 4.88 GHz | Peak 51.6 dB μ V/m | Peak Limit 74 dB μ V/m | Peak Difference -22.4 dB | Peak Status Pass |
| Frequency 4.88 GHz | Average 48.82 dB μ V/m | Average Limit 54 dB μ V/m | Average Difference -5.18 dB | Average Status Pass |

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 58

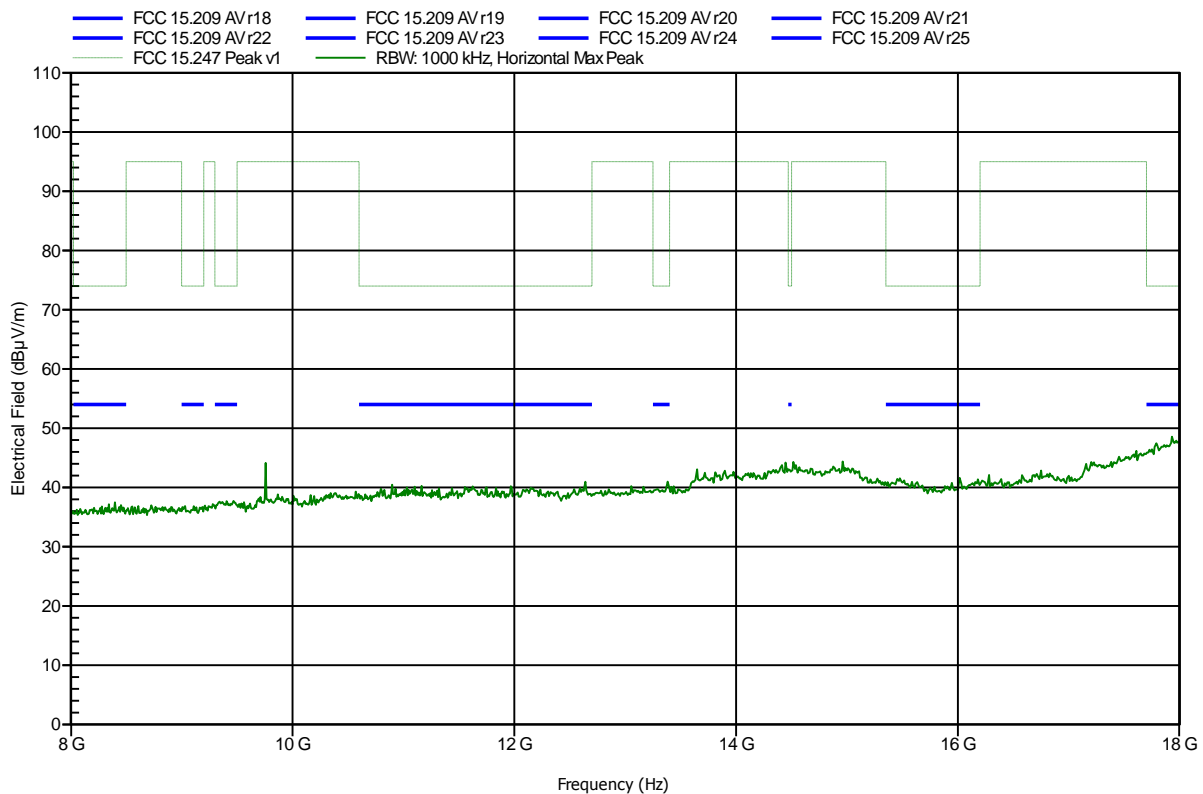


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 61

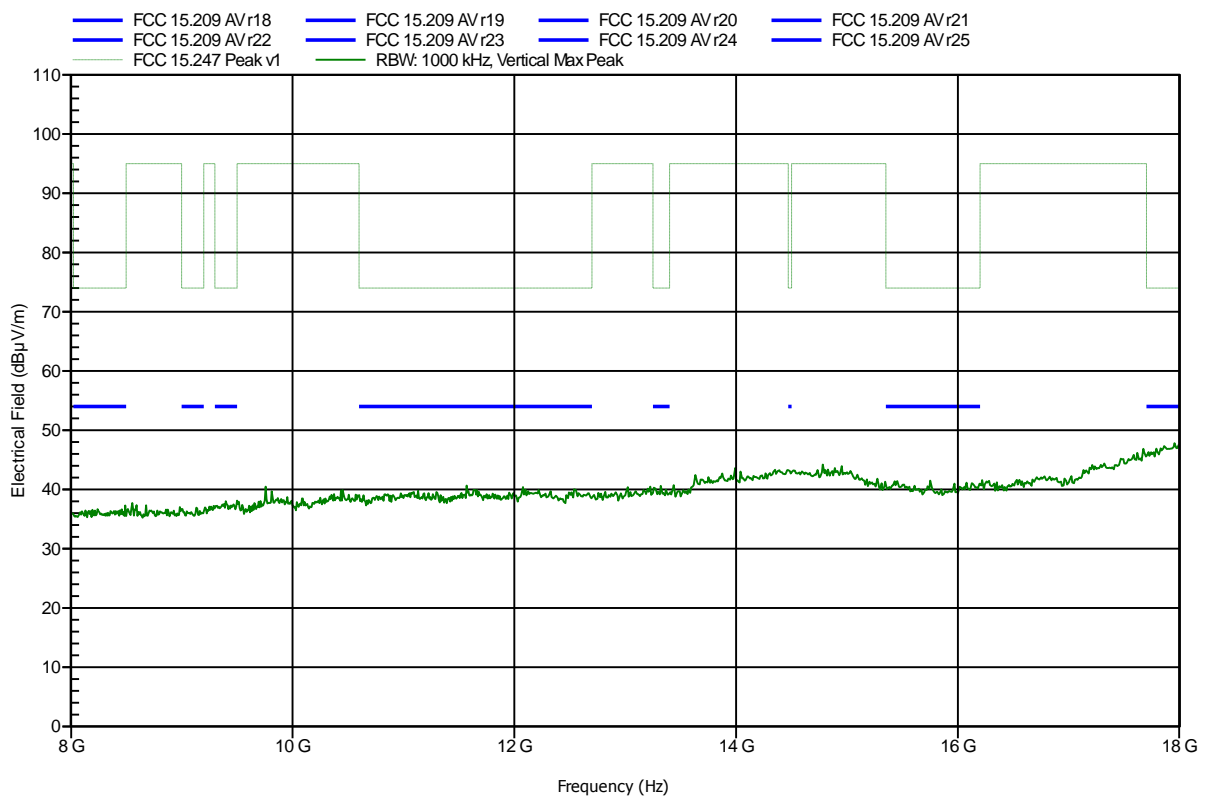


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Horizontal
 Measurement distance: 100 cm
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 59

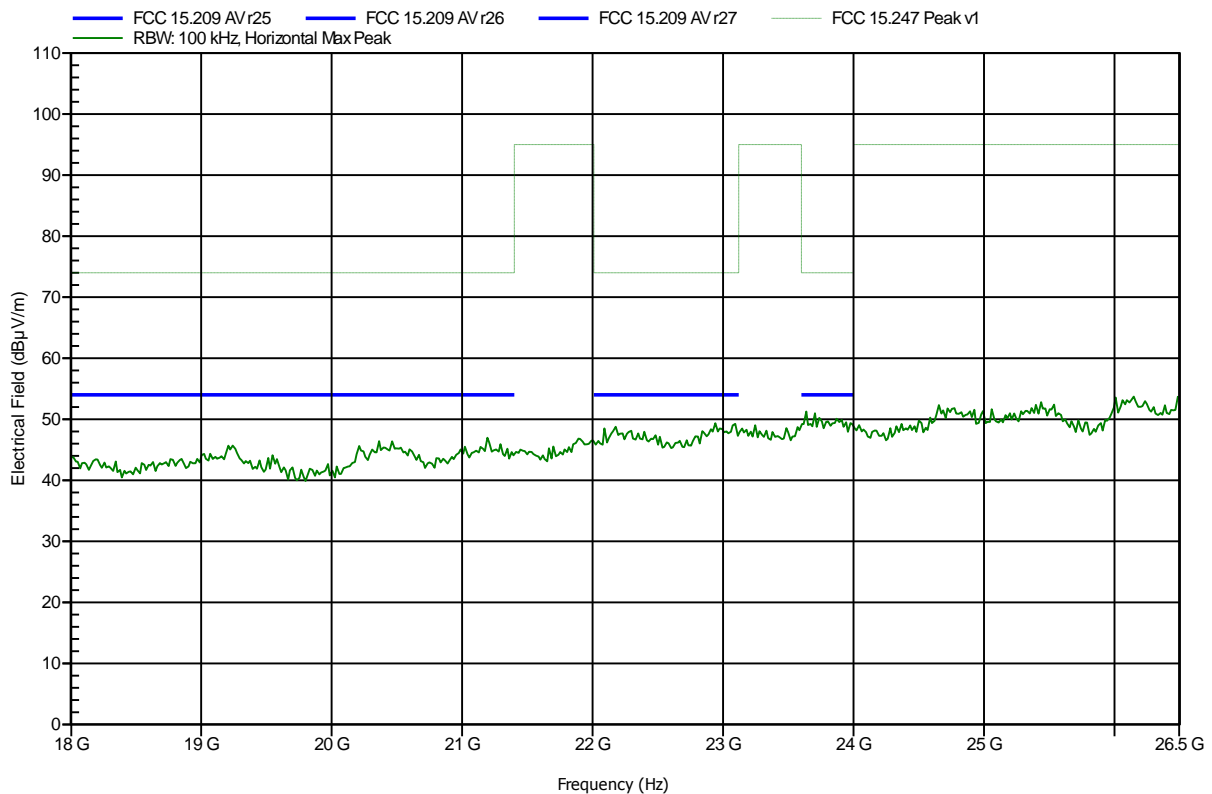


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Vertical
 Measurement distance: 100 cm
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 62

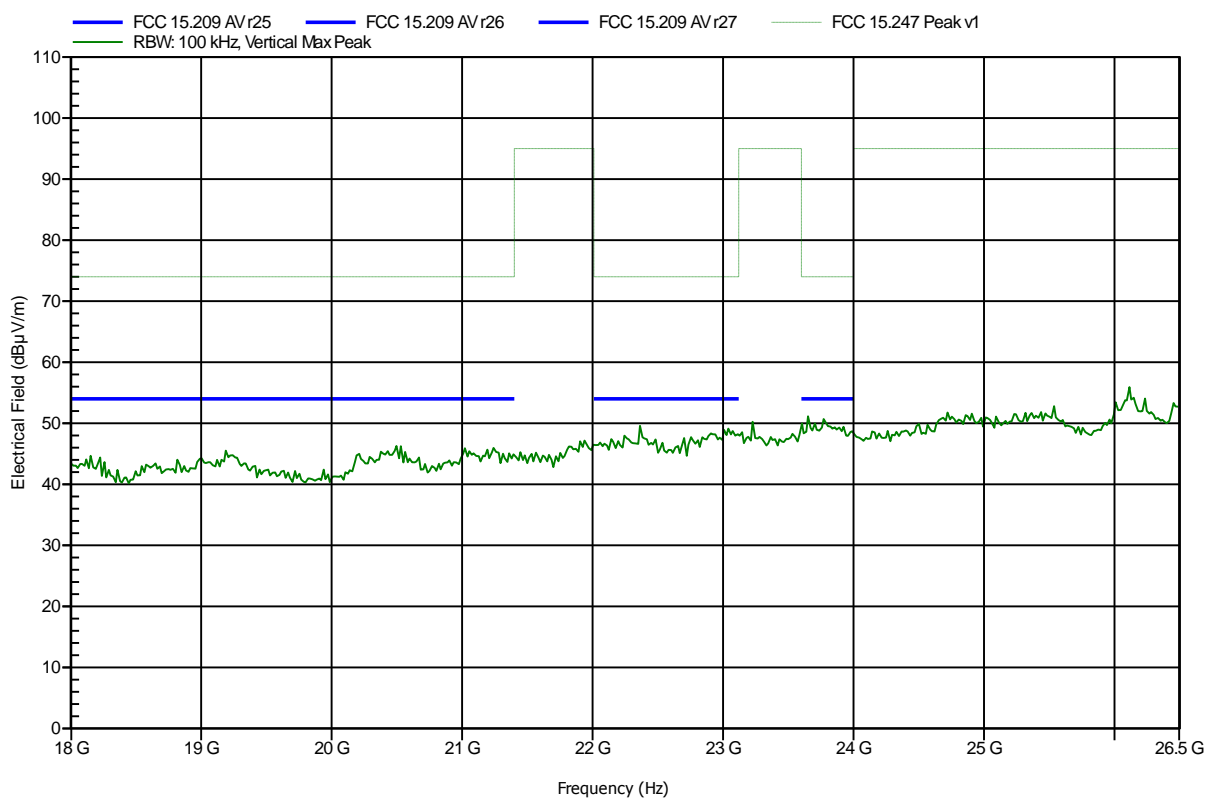


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 223, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 72

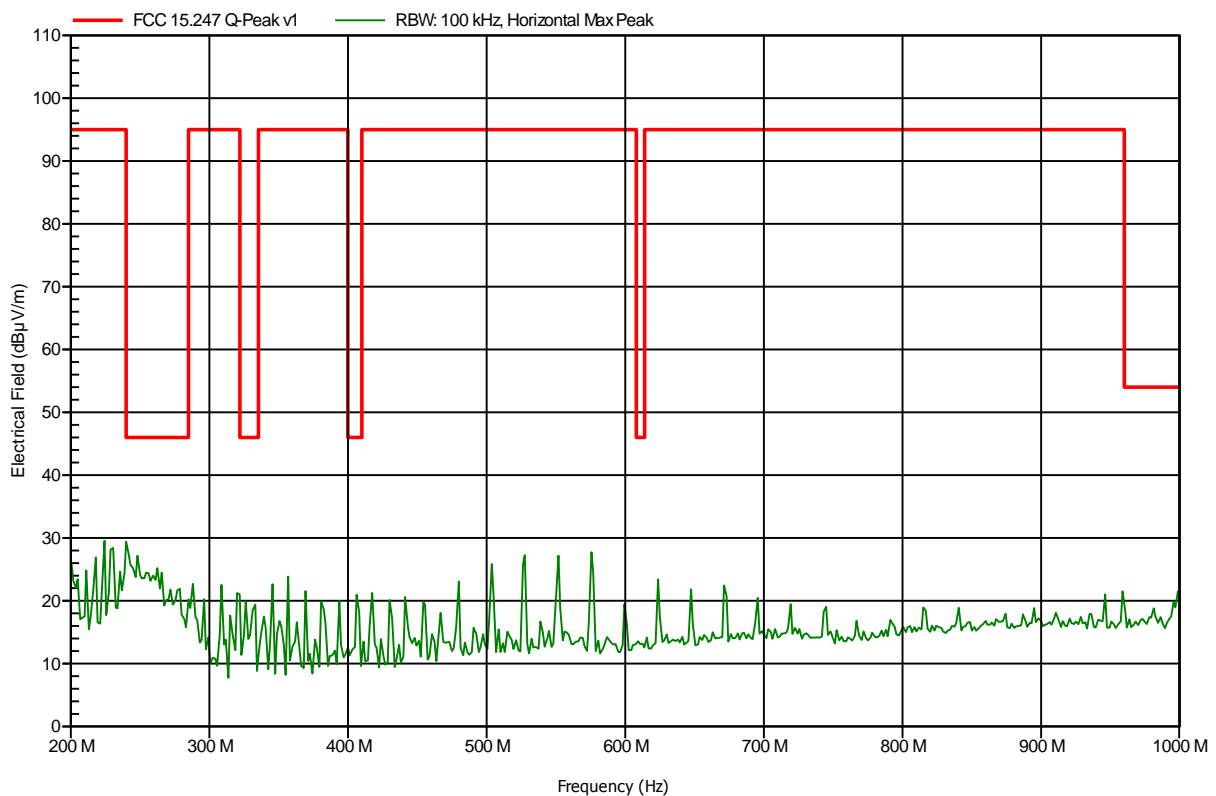


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

| | |
|-----------------------|---|
| Manufacturer: | Bang & Olufsen Medicom A/S |
| EUT Name: | Electronic Auto-injector |
| Model: | betaCONNECT |
| Test Site: | Eurofins Product Service GmbH |
| Operator: | Mr. Treffke |
| Test Conditions: | Tnom: 20°C, Vnom: 3.7V DC lithium battery |
| Antenna: | Rohde & Schwarz HL 223, Vertical |
| Measurement distance: | 3 m |
| Mode: | TX; ch. 39 |
| Test Date: | 2013-07-03 |
| Note: | |

Index 73

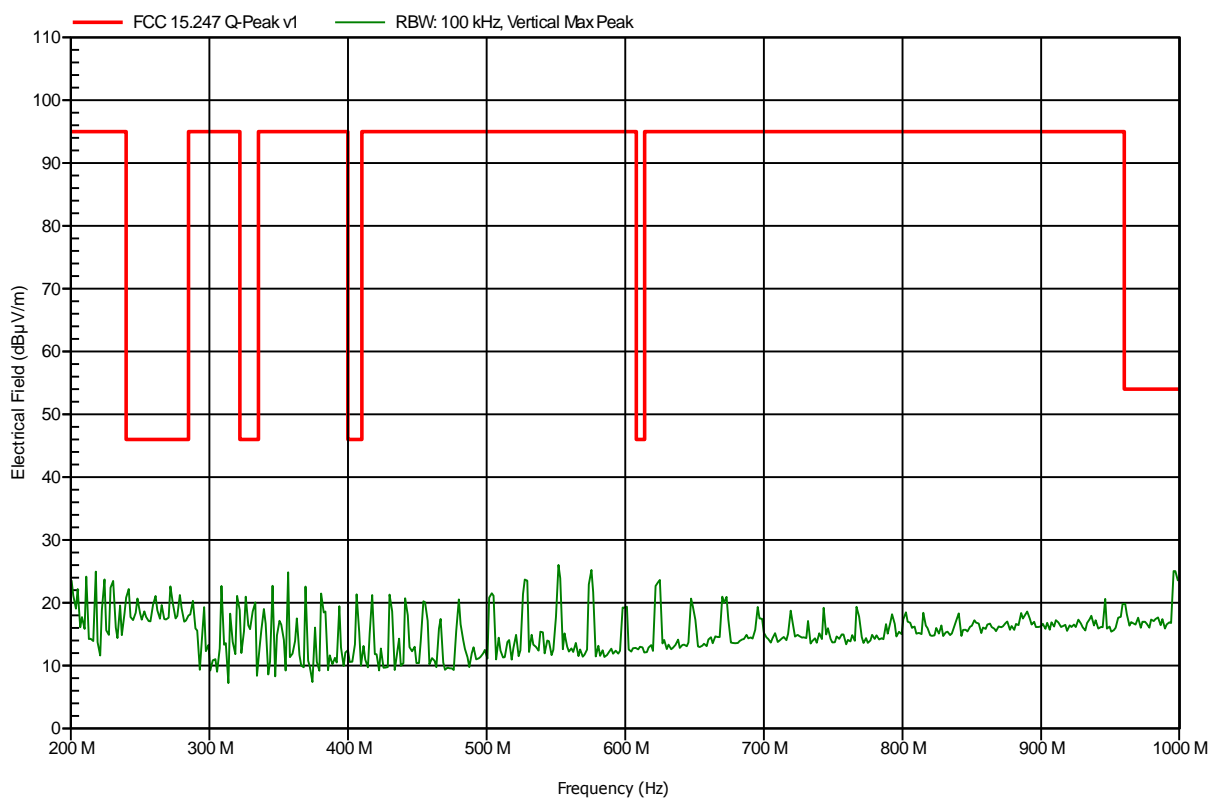


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 48

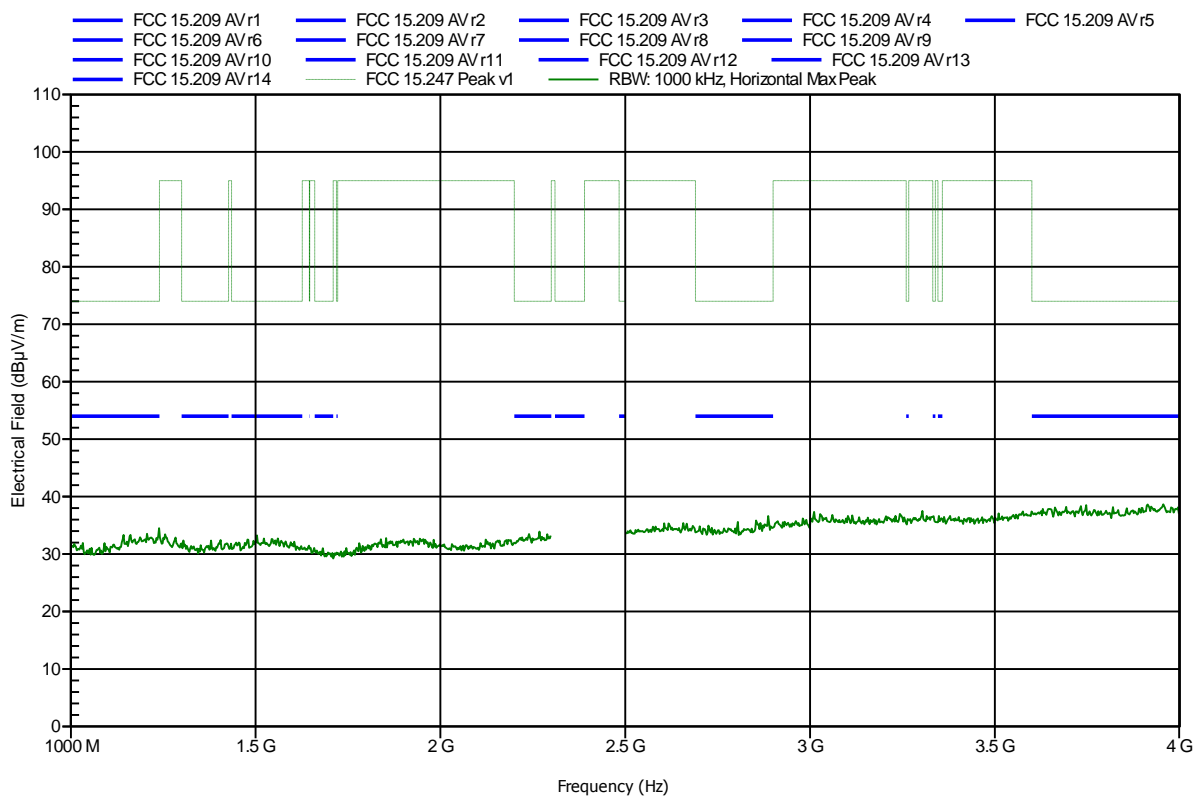


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 51

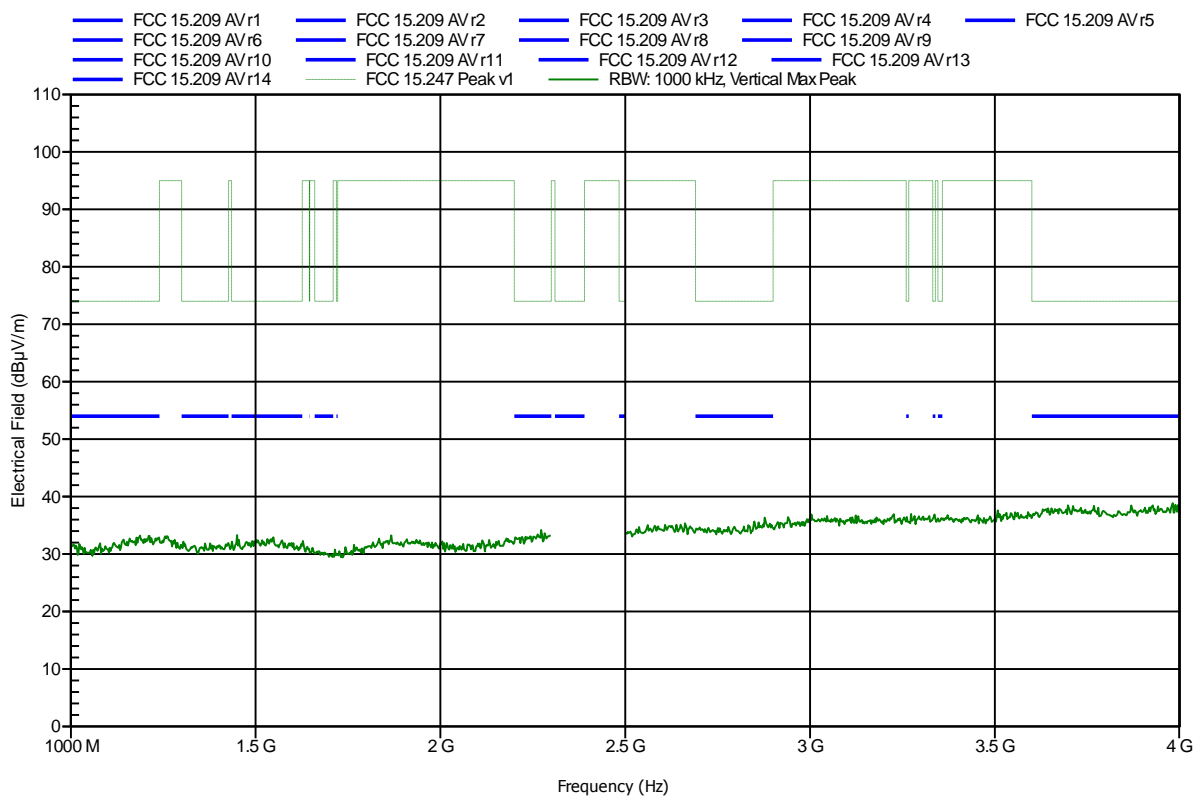


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note: upper bandedge

Index 49

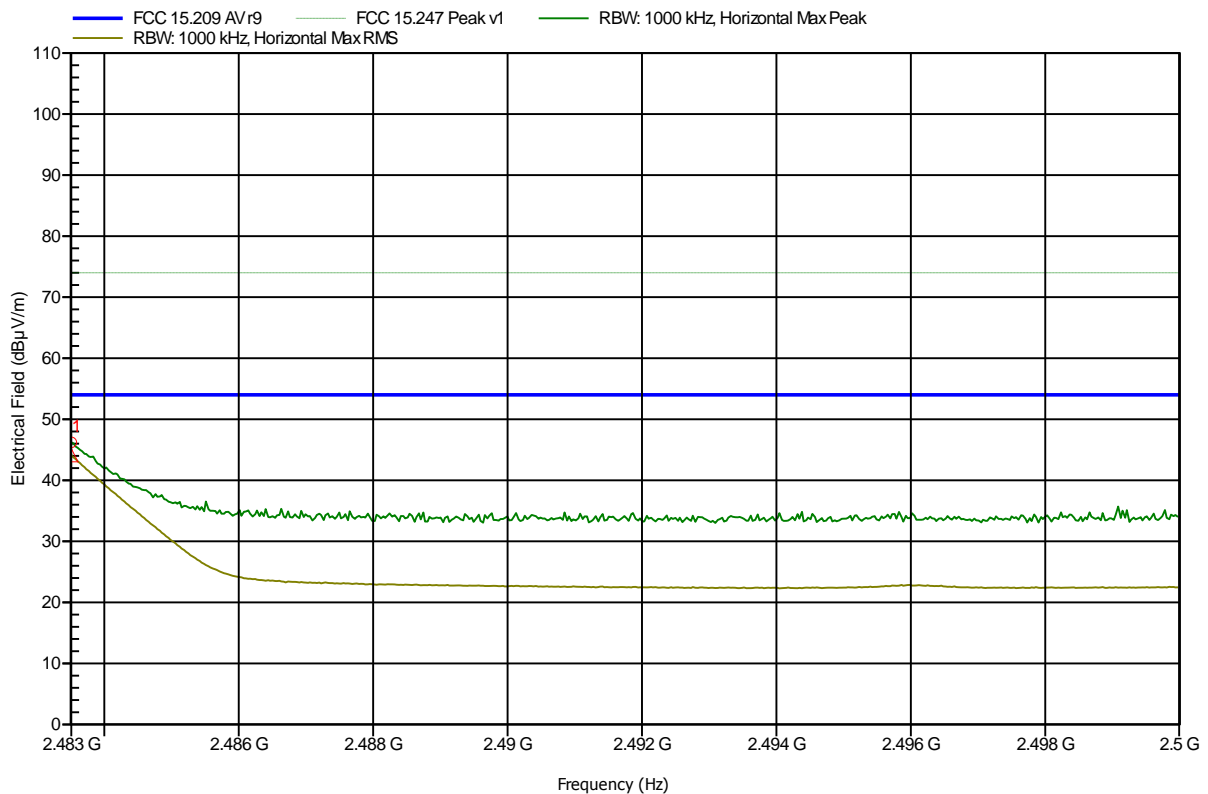


| Frequency | Peak | Peak Limit | Peak Difference | Peak Status |
|------------|-------------|------------|-----------------|-------------|
| 2.4835 GHz | 46.2 dBuV/m | 74 dBuV/m | -27.8 dB | Pass |

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note: upper bandedge

Index 52

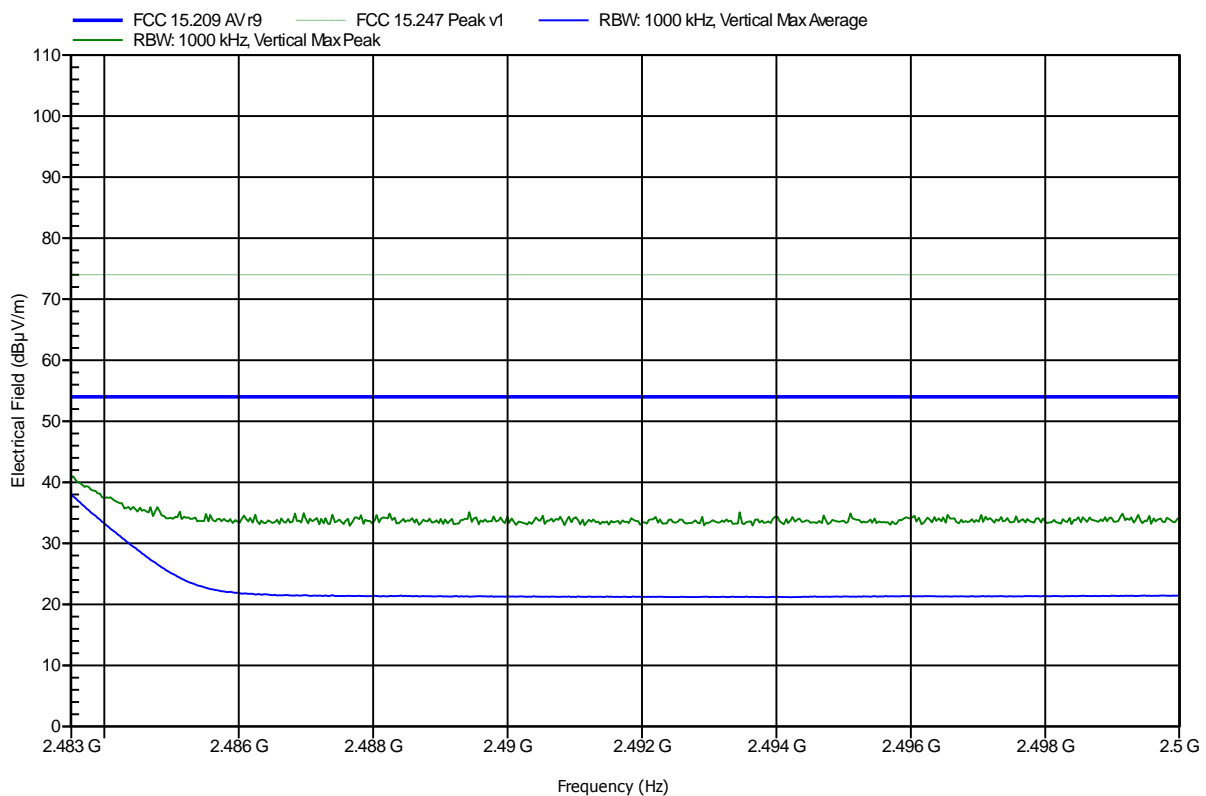


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 50

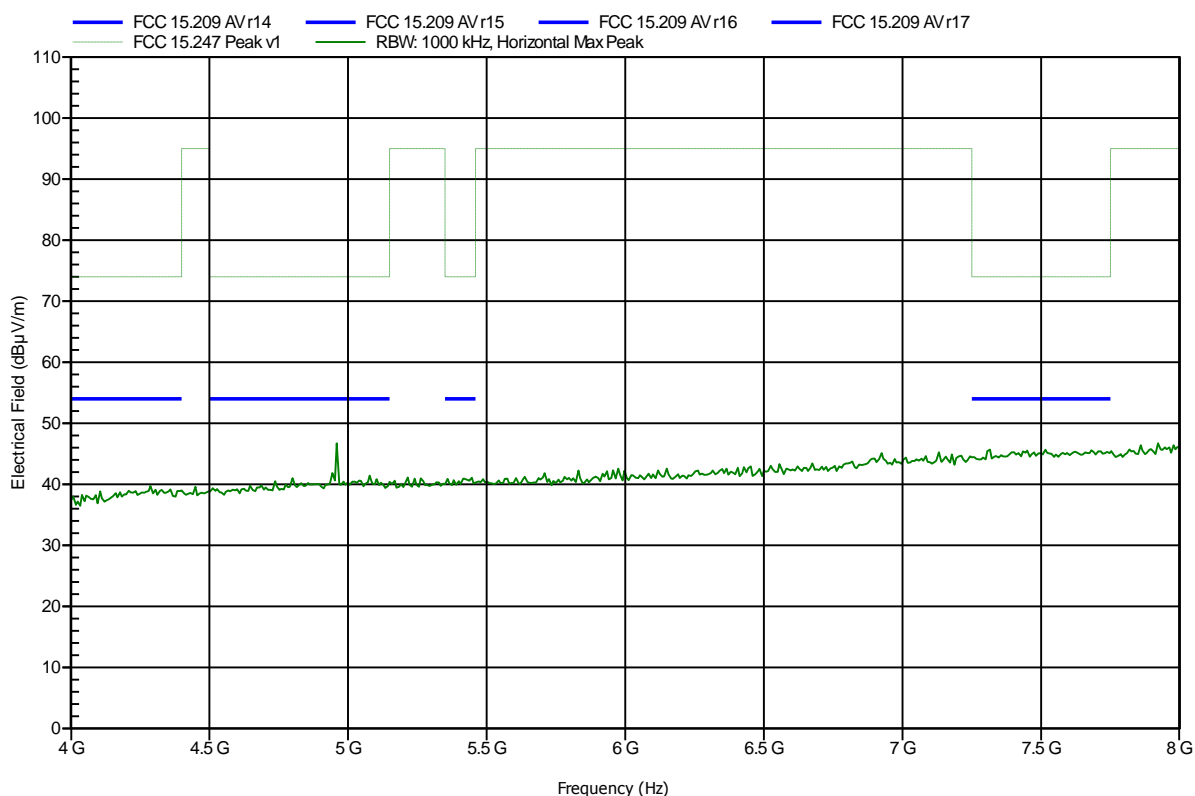


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 53

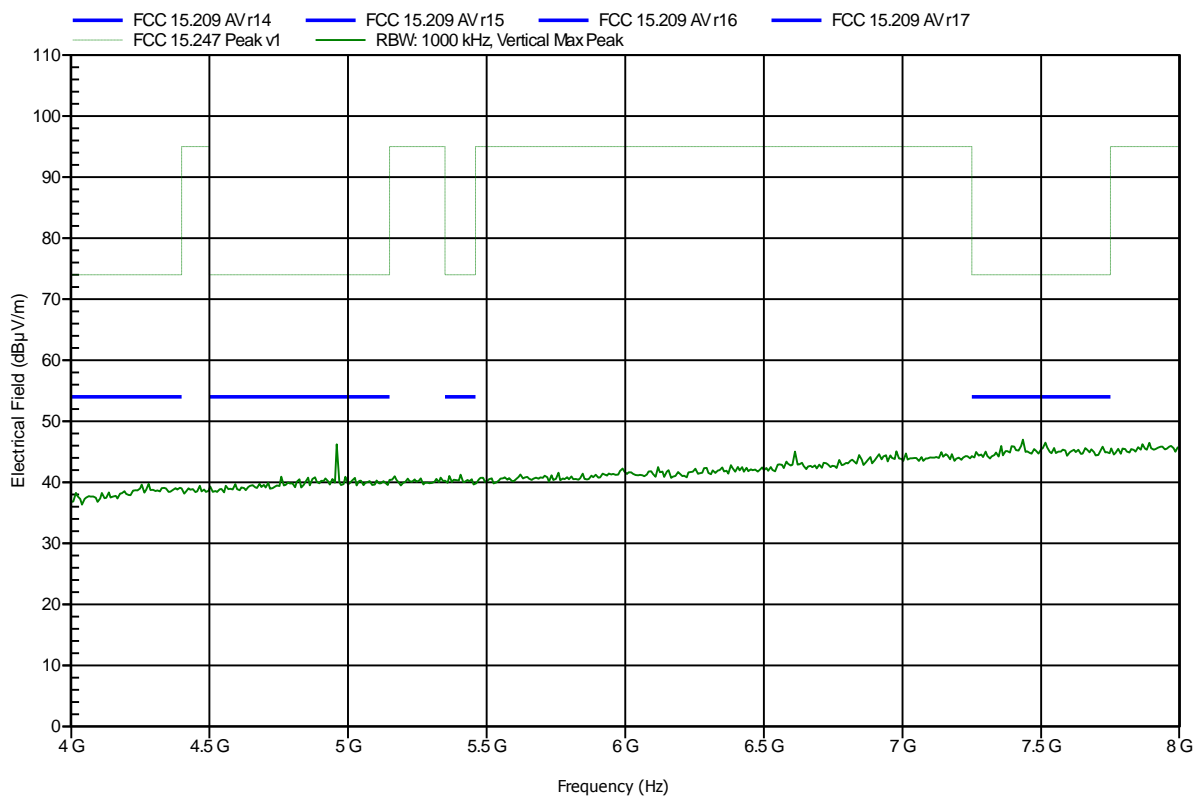


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 63

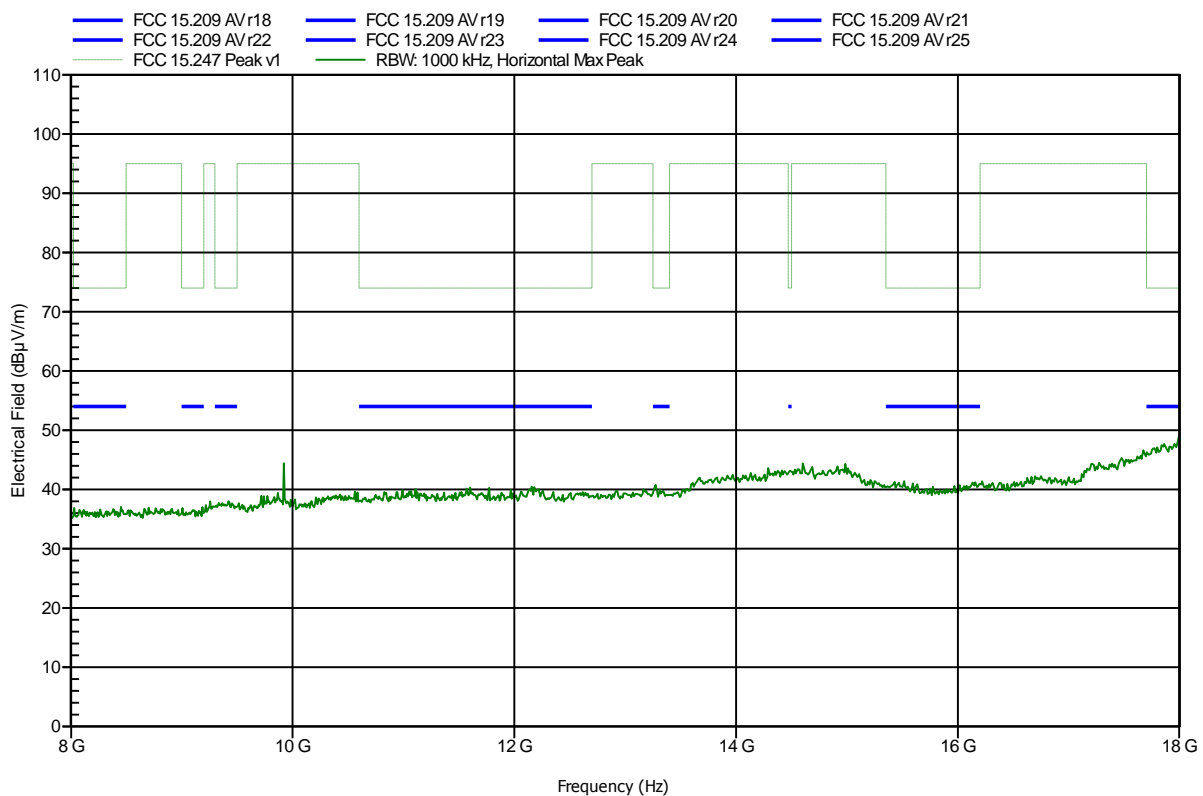


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 65

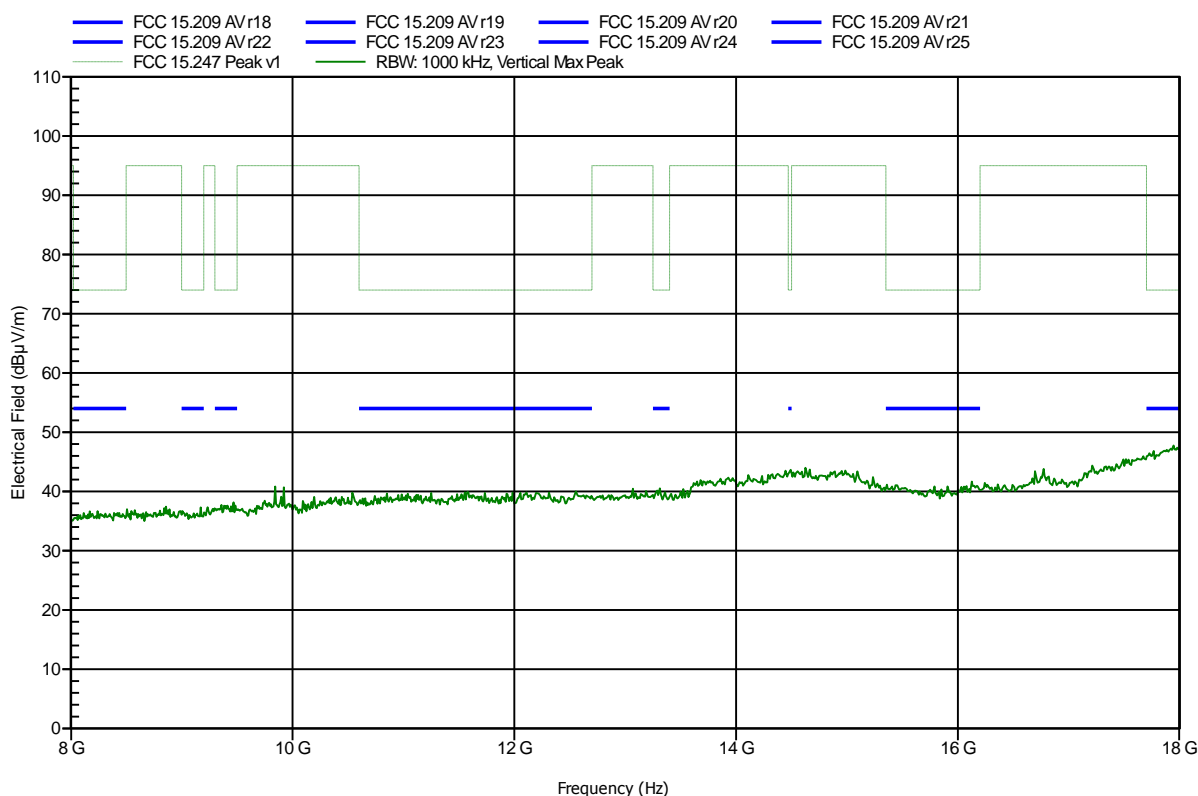


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Horizontal
 Measurement distance: 100 cm
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 64

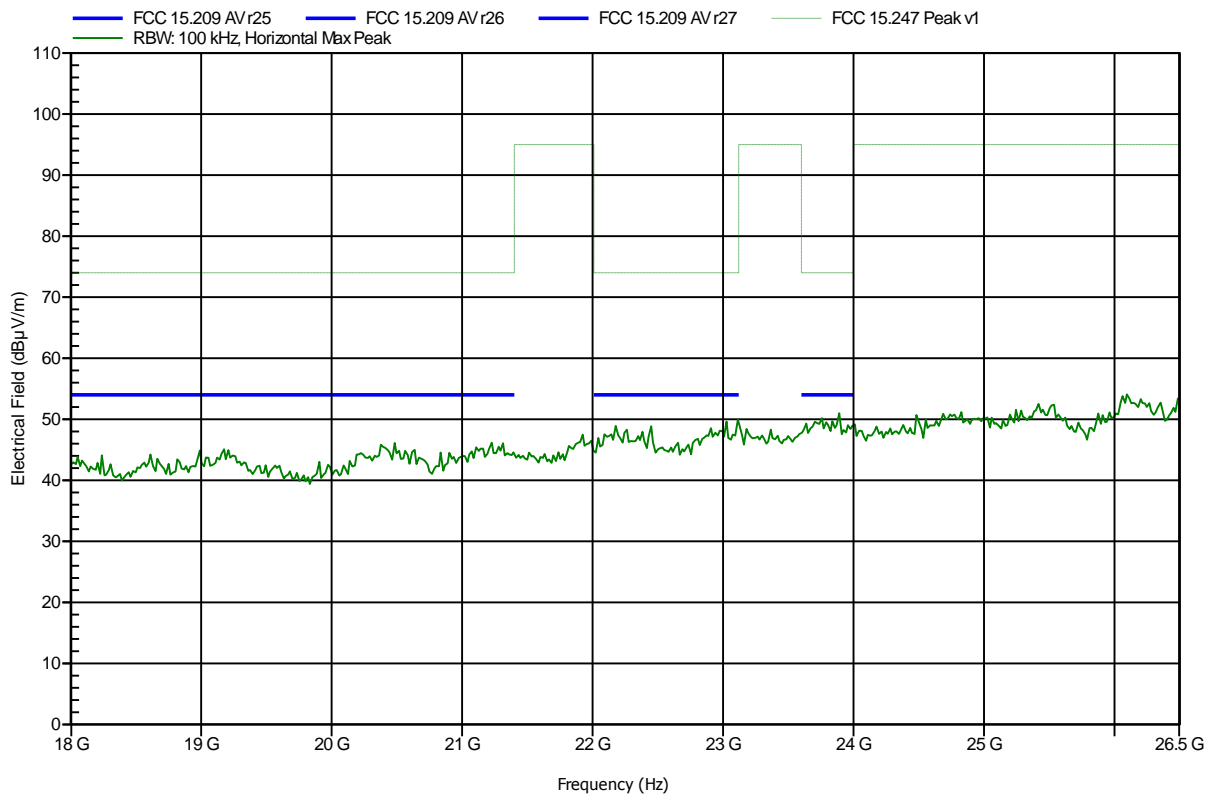


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Vertical
 Measurement distance: 100 cm
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 66

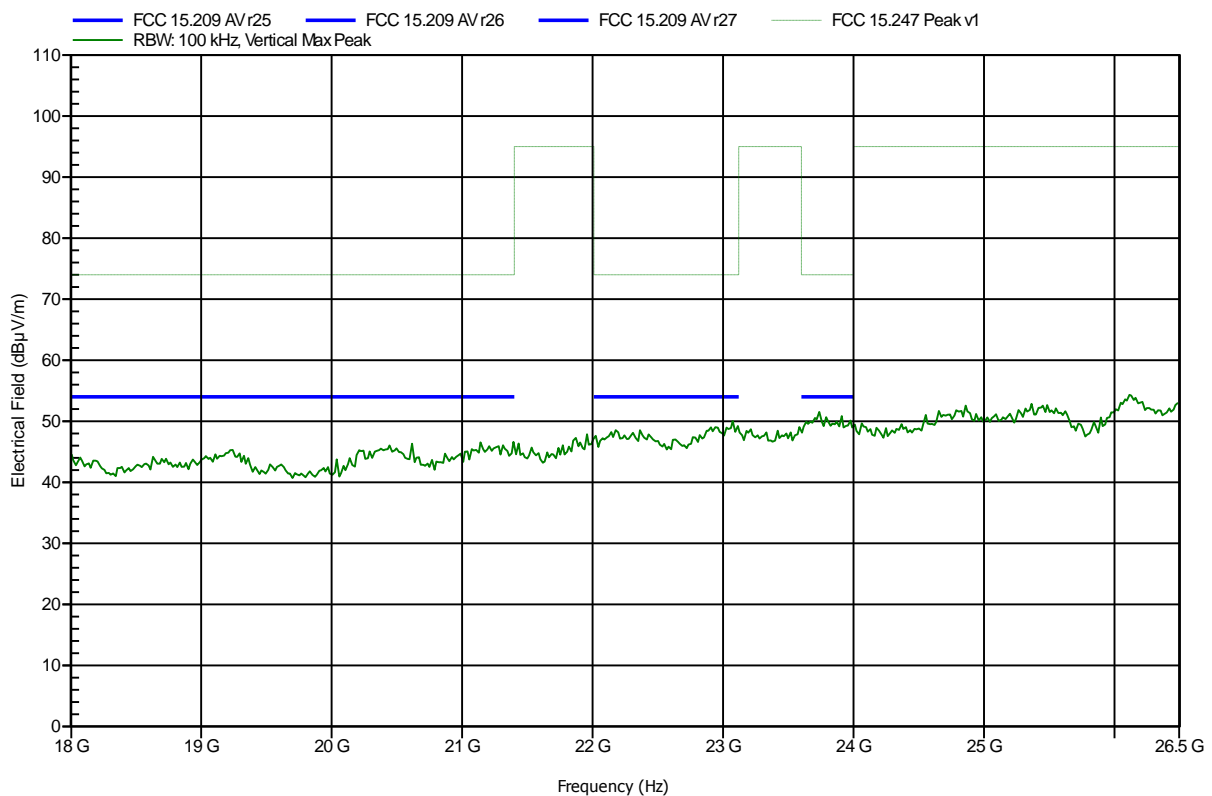


ANNEX B Receiver radiated spurious emissions

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HK 116, Horizontal
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 76

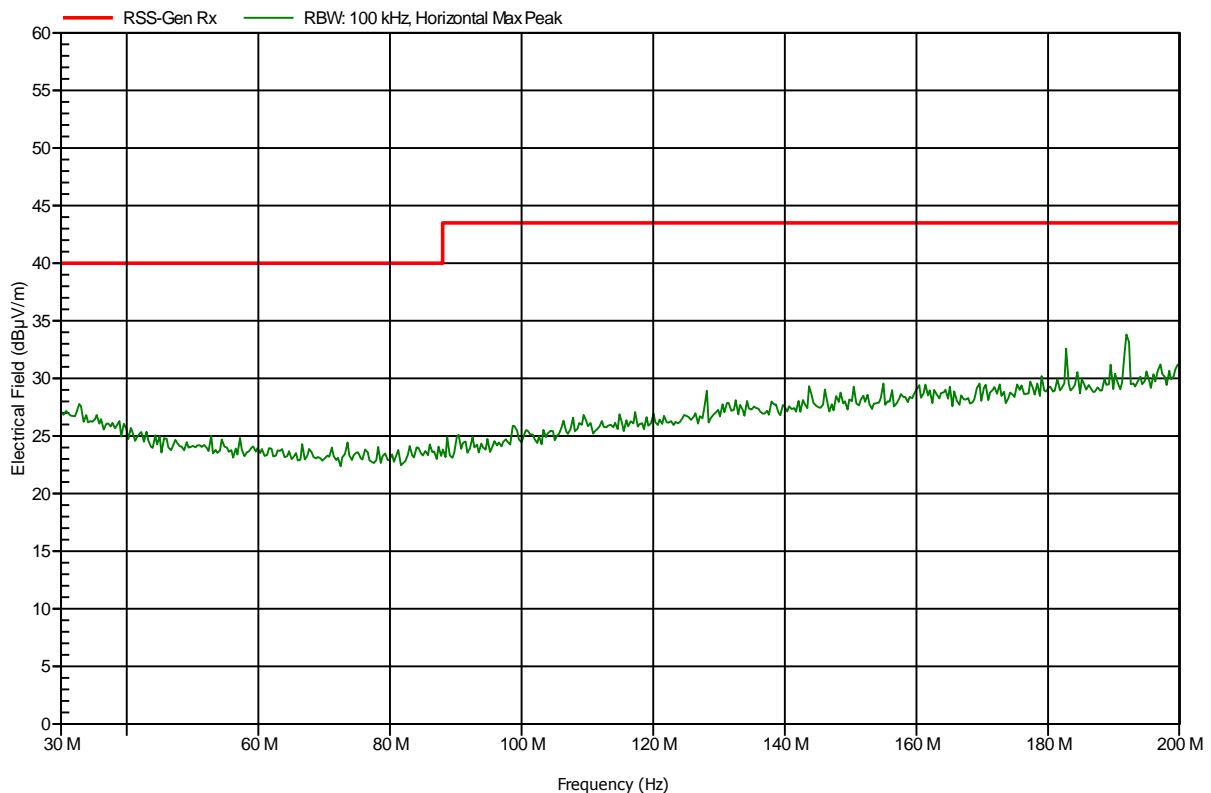


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HK 116, Vertical
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 77

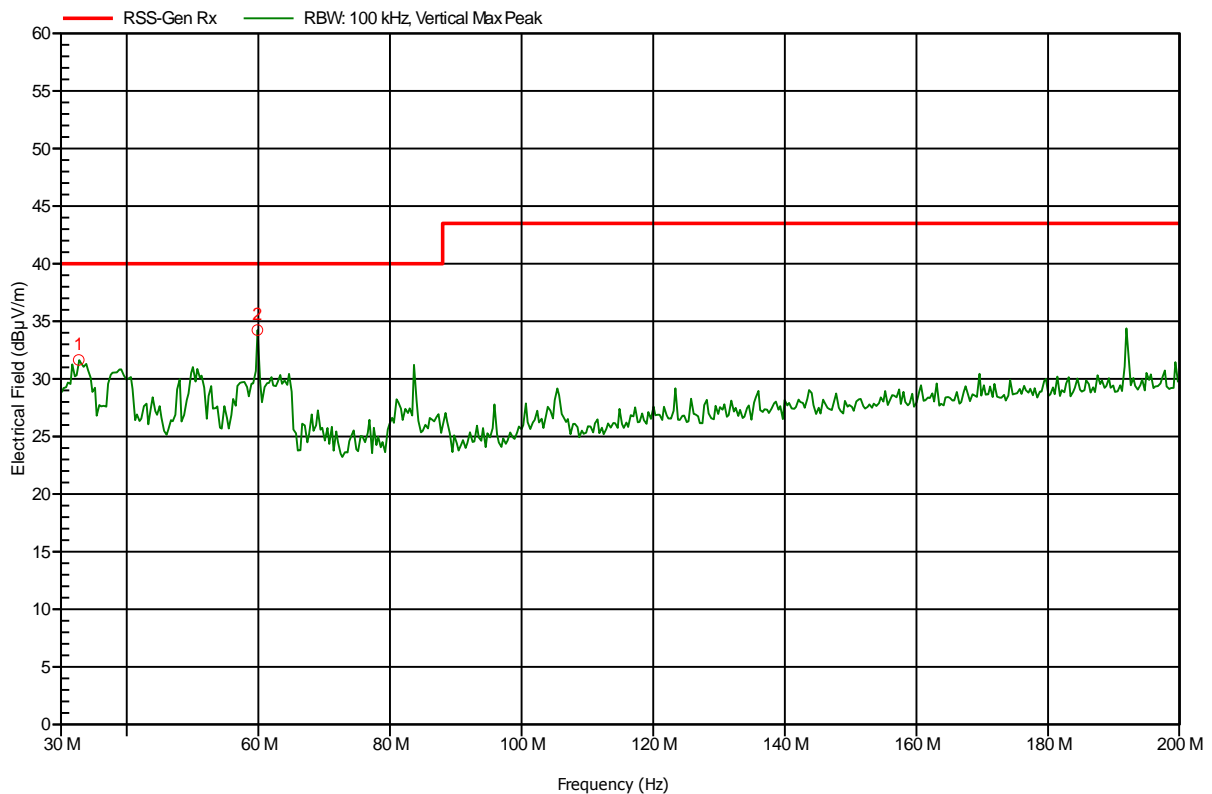


| Frequency | Peak | Peak Limit | Peak Difference | Status |
|------------|--------------|------------|-----------------|--------|
| 32.715 MHz | 31.65 dBµV/m | 40 dBµV/m | -8.35 dB | Pass |
| 59.86 MHz | 34.24 dBµV/m | 40 dBµV/m | -5.76 dB | Pass |

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 223, Horizontal
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 78

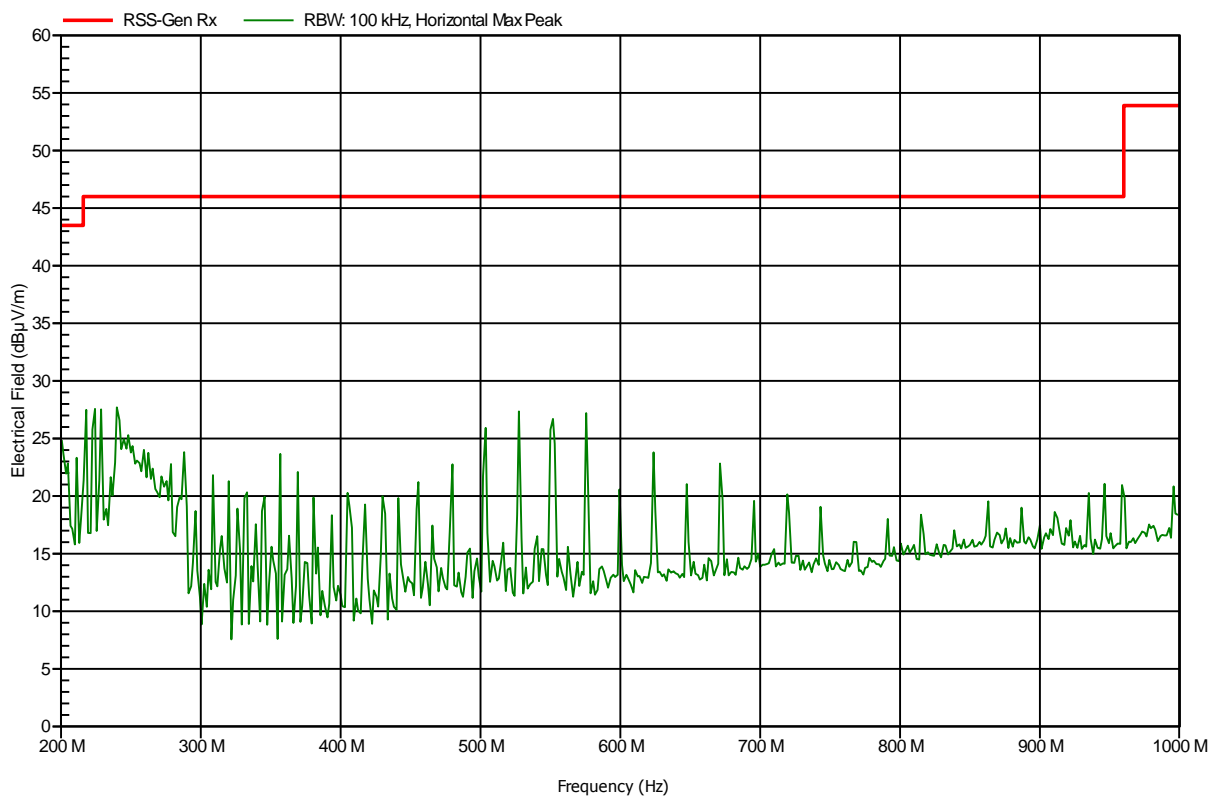


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 223, Vertical
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 79

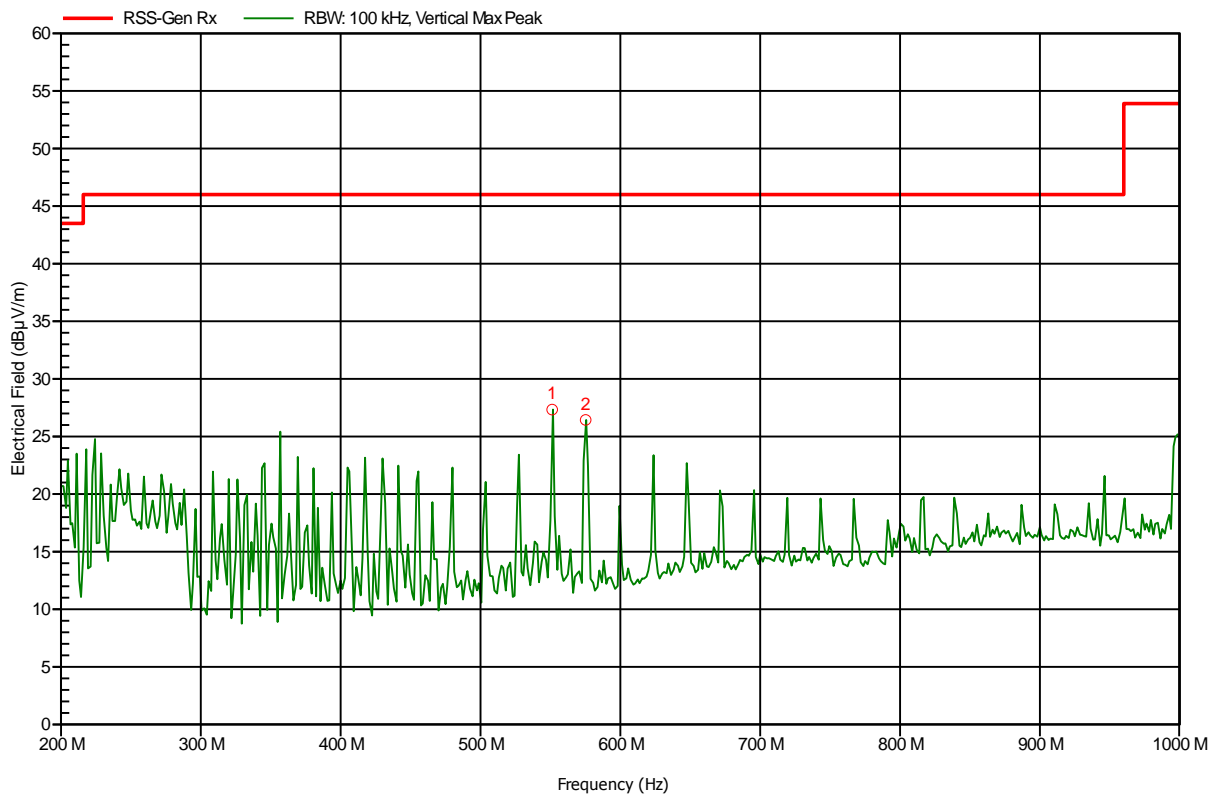


| Frequency | Peak | Peak Limit | Peak Difference | Status |
|-------------|--------------|------------|-----------------|--------|
| 551.297 MHz | 27.33 dBµV/m | 46 dBµV/m | -18.67 dB | Pass |
| 575.25 MHz | 26.43 dBµV/m | 46 dBµV/m | -19.57 dB | Pass |

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medcom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 80

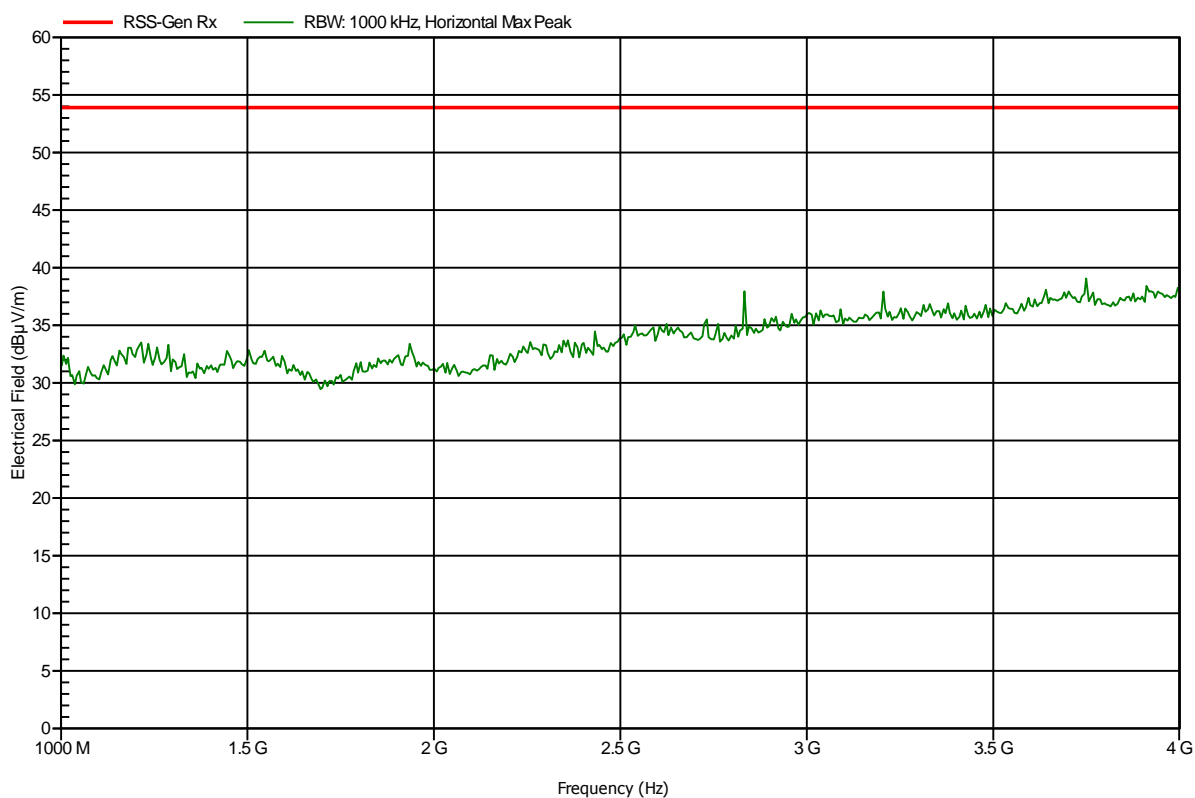


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 82

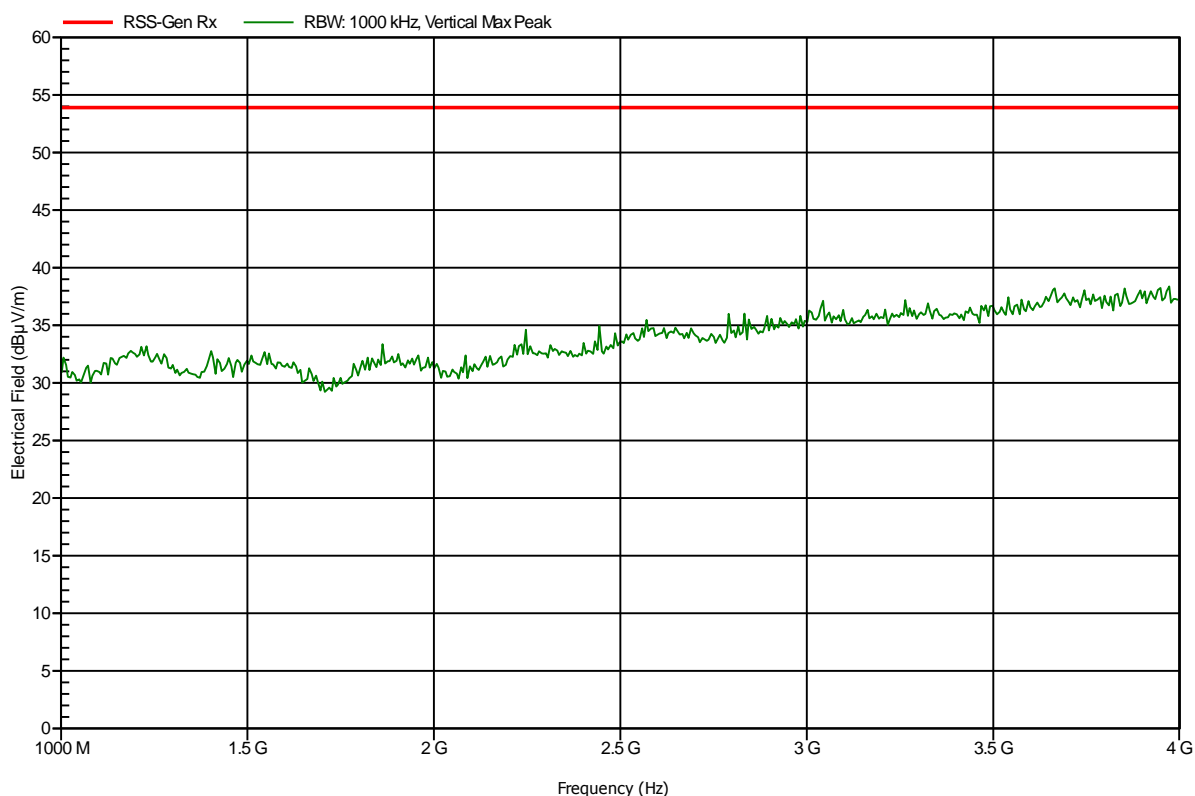


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 81

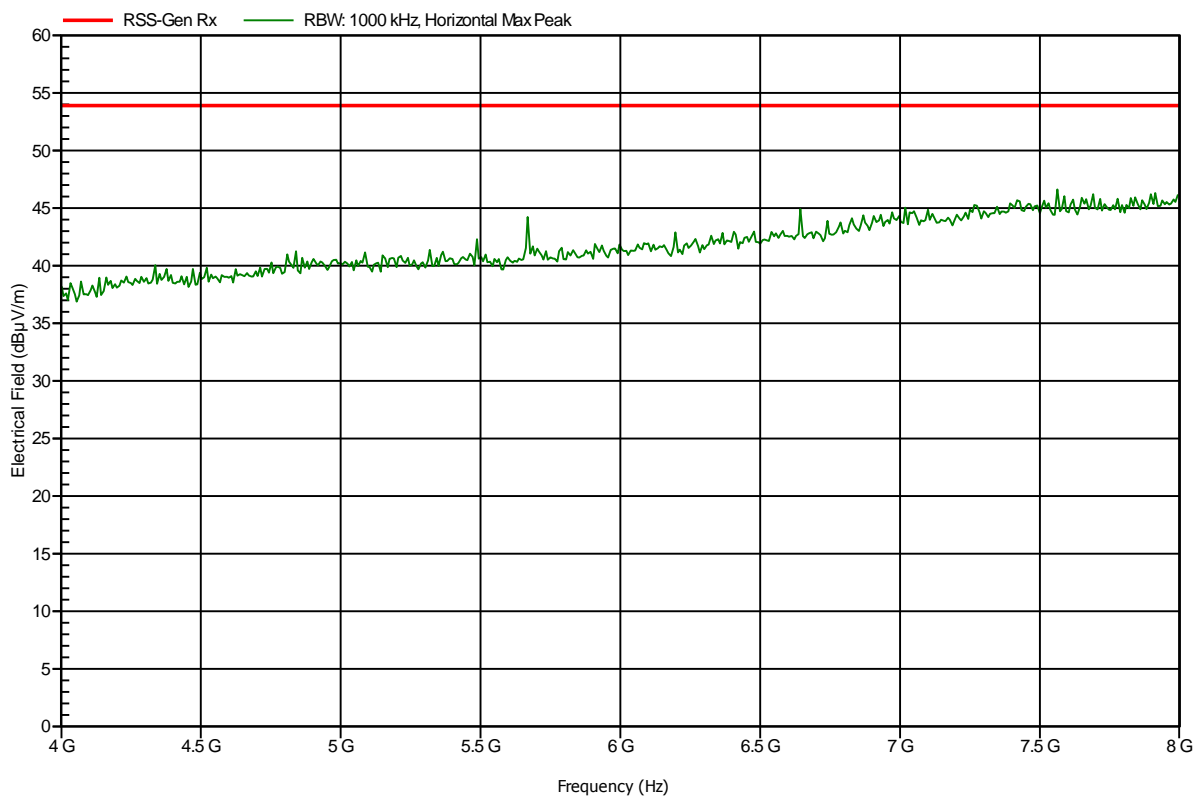

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 83

