Huntleigh Healthcare Ltd.
Diagnostic Products Division
35 Portmanmoor Road, Cardiff, CF24 5HN, U.K.
Tel: +44 (0)29 20485885
Fax: -44 (0) 29 20492520
www.huntleigh-diagnostics.com

REF SF1-SL   Made in UK

SN

CLASSIFIED c (UL) us   EXXXXXX

IP30

Reciever Unit
FCC ID: 2ABOQ-SF1SL
IC ID: 11744A-SF1SL
Model: SF1-SL

CTG

This device complies with part 15 of the FCC/IC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Operation of this equipment requires the prior coordination with a frequency coordinator designated by the FCC for the Wireless Medical Telemetry Service.

100-240V ∼ 10-20VA
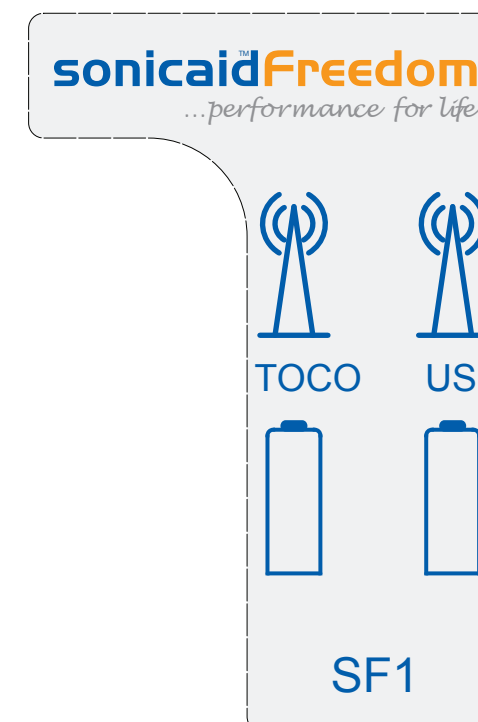50-60Hz

Rear Panel Label
Background: Pantone Cool Grey 1C
Text and Graphics: Blue Pantone 286C
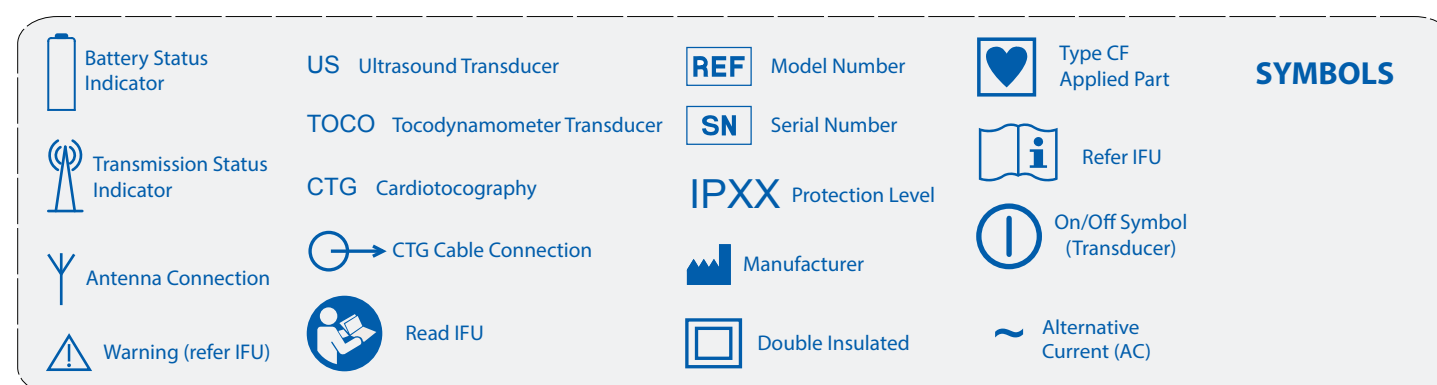Clear Window 34 x 5.6
2 holes 6.7 (shown solid black)
1 hole 12.5 (shown solid black)

sonicaid Freedom
...performance for life

TOCO   US

SF1

Front Panel Label
Background: Pantone Cool Grey 1C
Text and Graphics: Pantone Blue 286C,
Pantone Orange144C & Cool Grey 9C

SYMBOLS

Battery Status Indicator

Transmission Status Indicator

Antenna Connection

Warning (refer IFU)

US Ultrasound Transducer
TOCO Tocodynamometer Transducer
CTG Cardiotocography
CTG Cable Connection
Read IFU

REF Model Number
SN Serial Number
IPXX Protection Level
Manufacturer
Double Insulated

Type CF Applied Part
Refer IFU
On/Off Symbol (Transducer)
∼ Alternative Current (AC)

Top Panel Label
Background: Pantone Cool Grey 1C
Text and Graphics: Pantone Blue 286C,

Freedom US Label Set
778348-J