#### Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-CN (Auden)

Certificate No: ER3-2528 Mar16

### CALIBRATION CERTIFICATE

Object

ER3DV6 - SN:2528

Calibration procedure(s)

QA CAL-02.v8, QA CAL-25.v6

Calibration procedure for E-field probes optimized for close near field

evaluations in air

Calibration date:

March 24, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ER3DV6	SN: 2328	12-Oct-15 (No. ER3-2328_Oct15)	Oct-16
DAE4	SN: 789	16-Mar-15 (No. DAE4-789_Mar15)	Mar-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Signature Name Function Calibrated by: Michael Weber Laboratory Technician Approved by: Katja Pokovic Technical Manager

Issued: March 26, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

NORMx,y,z DCP sensitivity in free space diode compression point

CF

crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

A, B, C, D Polarization φ

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e.,  $\vartheta = 0$  is normal to probe axis

Connector Angle

information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

 a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005

b) CTIA Test Plan for Hearing Aid Compatibility, Rev 3.0, November 2013

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 for XY sensors and θ = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

# Probe ER3DV6

SN:2528

Manufactured: Calibrated:

April 26, 2010 March 24, 2016

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

ER3DV6 - SN:2528 March 24, 2016

### DASY/EASY - Parameters of Probe: ER3DV6 - SN:2528

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)$	1.91	1.64	1.88	± 10.1 %
DCP (mV) <sup>B</sup>	100.4	100.0	100.6	

**Modulation Calibration Parameters** 

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	Х	0.0	0.0	1.0	0.00	241.7	±3.8 %
Name of the		Υ	0.0	0.0	1.0		204.6	
		Z	0.0	0.0	1.0	1.	210.6	1.14
10011- CAB	UMTS-FDD (WCDMA)	Х	3.44	68.1	19.4	2.91	148.1	±0.5 %
		Υ	3.26	66.7	18.6		121.9	. ***
		Z	3.21	66.4	18.3		126.2	
10021- DAB	GSM-FDD (TDMA, GMSK)	Х	25.68	100.0	28.9	9.39	133.9	±2.5 %
J. P. Park		Υ	23.94	99.3	29.4	1.5	107.6	
		Ζ	30.24	99.8	29.5		140.3	
10039- CAB	CDMA2000 (1xRTT, RC1)	Х	4.84	66.5	19.1	4.57	112.8	±0.7 %
		Υ	5.00	66.9	19.3		126.6	
		Z	4.88	66.4	18.8		130.5	,
10081- CAB	CDMA2000 (1xRTT, RC3)	Х	4.17	67.2	19.4	3.97	149.3	±0.7 %
		Υ	3.93	65.4	18.3		120.7	
		Z	3.98	65.9	18.5		125.3	
10295- AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	Х	19.24	99.6	39.5	12.49	116.7	±3.5 %
		Υ	19.55	99.0	39.2		139.0	
***************************************		Z	20.01	95.9	36.9		109.7	


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

Certificate No: ER3-2528\_Mar16 Page 4 of 10

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

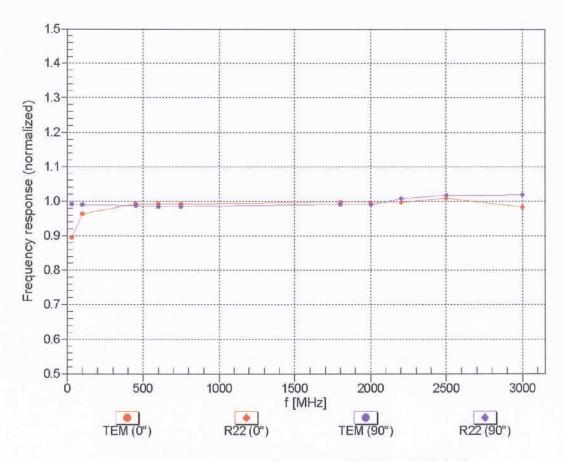



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

### Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

f=600 MHz,TEM,0°

f=2500 MHz,R22,0°

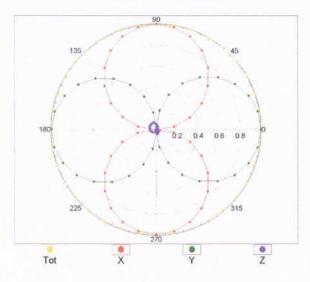


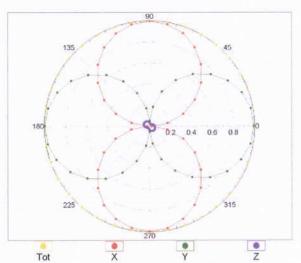


### Receiving Pattern ( $\phi$ ), $\vartheta = 90^{\circ}$


f=600 MHz,TEM,90°

f=2500 MHz,R22,90°

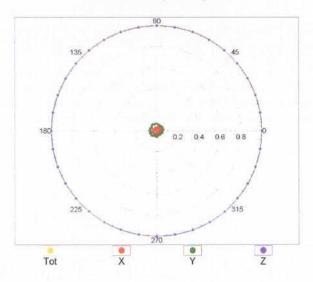




### Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

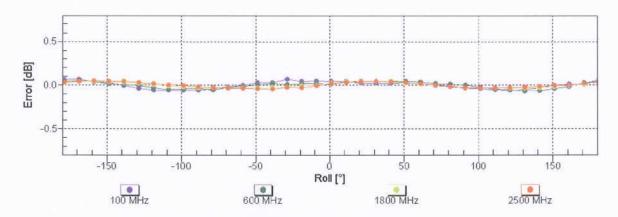


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


### Receiving Pattern ( $\phi$ ), $\vartheta = 90^{\circ}$

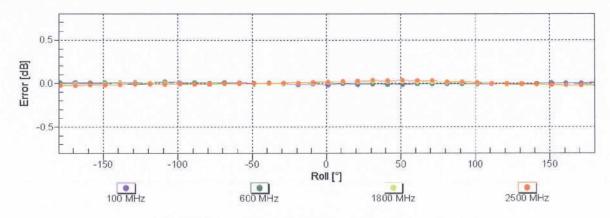

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

### Dynamic Range f(E-field) (TEM cell , f = 900 MHz)

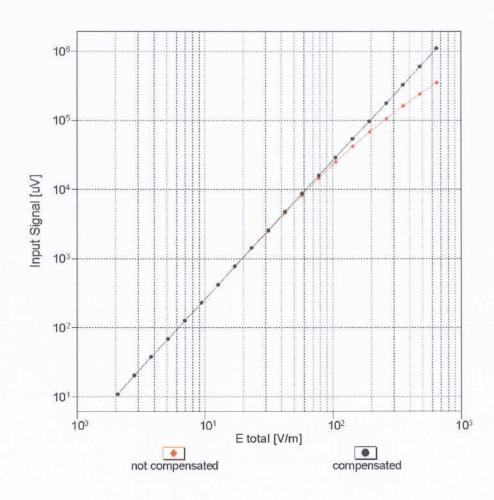


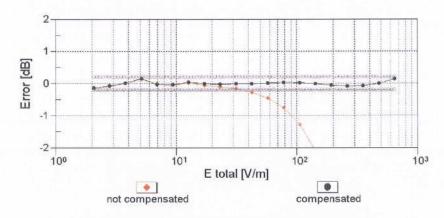


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

### **Deviation from Isotropy in Air**

Error ( $\phi$ ,  $\vartheta$ ), f = 900 MHz

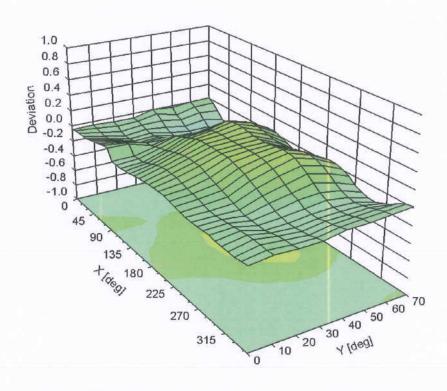



Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

### DASY/EASY - Parameters of Probe: ER3DV6 - SN:2528

### **Other Probe Parameters**

Sensor Arrangement	 Rectangular
Connector Angle (°)	-18.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	 8 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm
<u> </u>	1

### Appendix E. Product Equality Declaration

SPORTON INTERNATIONAL (SHENZHEN) INC.

TEL: 86-755-8637-9589 FAX: 86-755-8637-9595 FCC ID: 2ACCJA018  $\begin{array}{lll} \mbox{Page Number} & : \mbox{E1 of E1} \\ \mbox{Report Issued Date} & : \mbox{Aug. 10}, 2016 \end{array}$ 

Report No.: HA670106A

Report Version : Rev. 01



5F, C building, No. 232, Liang Jing Road ZhangJiang High-Tech Park, Pudong Area Shanghai, P.R. China. 201203 TEL: +86(0)21 61460666 FAX: +86(0)21 61460602

### Declaration of changes from Initial to Variant

General: 6055A is a variant product of 6055U

#### SOFTWARE MODIFICATIONS:

Protocol Stack changes: No

> MMS/STK/USAT/USIM changes: No

> DM/SUPL/VT/FUMO/SWP/HCI: Yes (6055A does not support DM/FUMO)

Other changes detailed:

1. Enable FDD band17

2. Add UICC base NFC

#### HARDWARE MODIFICATIONS:

> Band changes: No

> PCB Layout changes: No

> Main RF components changes:

	Antenna	AP	Modem	Transceiver	Power Amplifier	Rx SAW Filter	ASM
GSM850	No	No	No	No	No	No	No
GSM900	No	No	No	No	No	No	No
GSM1800	No	No	No	No	No	No	No
GSM1900	No	No	No	No	No	No	No

	Antenna	AP	Modem	Transceive r	Power Amplifier	Tx SAW Filter	Duplexe r	ASM
UMTS band X	No	No	No	No	No	No	No	No

	Ante nna	AP	Mode m	Transcei ver	Power Amplifier	Tx SAW Filter	Rx SAW Filter	Duplexe r	ASM
LTE Band x	No	No	No	No	No	No	No	No	No
LTE Band x	No	No	No	No	No	No	No	No	No

	Antenna	AP	Modem	Transceiver	Power Amplifie r	Balun	Band pass filter	Diplexer
Bluetooth	No	No	No	No	No	No	No	No

Wi-Fi No No No No No No

- > FM changes: No
- > LCD/ Speaker/ Camera/ Vibrator changes: No (indicated the changed items if yes)
- Other changes detailed: Reduce 2db power in band 7.

#### MECHANICAL MODIFICATIONS:

- > Use new metal front/back cover or keypad: No
- Mechanical shell changes: Whole size of EUT: No Distance of Ear reference point to bottom of handset: No Other trinkets to change the surface of handset: No
- > Other changes detailed:
  - 1. Different logo on backcover.

#### APPROVED BY:

Project Manager: Frede

Signature: 8.10.

Date: