


Dipole900 insertion loss and impedance Annual check



Head 900

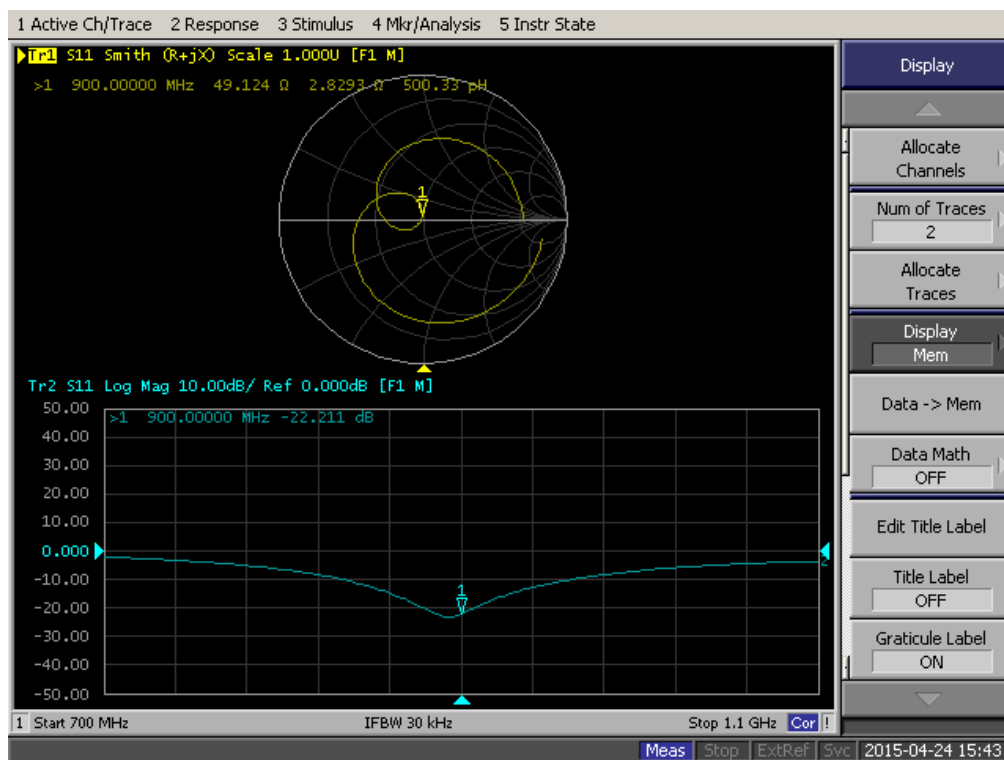


Head 900

Original calibration: Return Loss: -22.3; Impedance: 49.2

Annual check: Return Loss: -22.2; Impedance: 49.1



Body 900

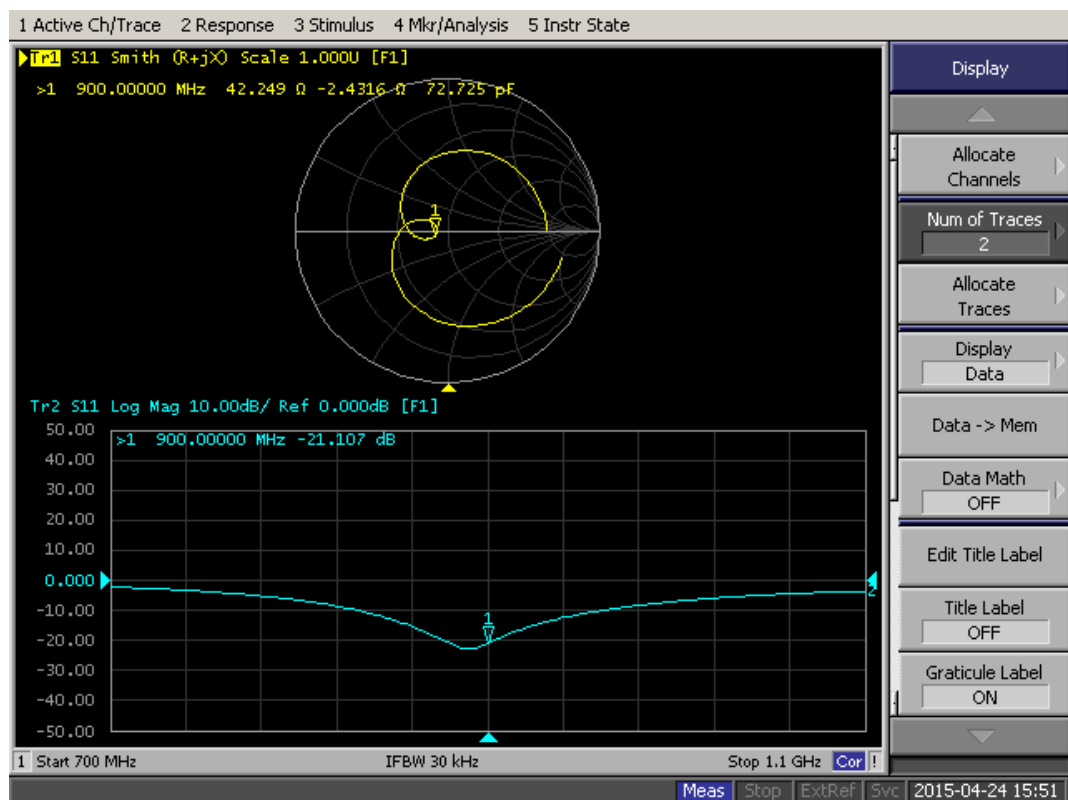

Body 900

Original calibration: Return Loss: -21.3; Impedance: 42.1

Annual check: Return Loss: -21.1; Impedance: 42.2