

ANNEX 2 TO TEST REPORT # EMCC-140157ACBB, 2015-08-05**PHOTOGRAPHS OF EQUIPMENT UNDER TEST (EUT)****EQUIPMENT UNDER TEST:**


Trade Name:	RFID Module
Type Designation(s):	B40421
Serial Number:	Sample #4: 0018 14/24 Sample #6: 0042 14/24
Equipment Class:	Low Power Transceiver
Manufacturer:	Beckman Coulter Biomedical GmbH
Address:	Sauerbruchstraße 50 81377 München Germany
Phone:	+49 89 579589-3606
Fax:	+49 89 579589-3505

RELEVANT STANDARD(S): 47 CFR 15.225**MEASUREMENT PROCEDURE:**


<input checked="" type="checkbox"/> RSS-Gen Issue 4	<input checked="" type="checkbox"/> ANSI C63.10-2013	<input type="checkbox"/> Other
---	--	--------------------------------

Test of Beckman Coulter RFID Module type B40421 to 47 CFR 15.225 and RSS-210 Issue 8


1 PHOTOS OF TEST SAMPLES

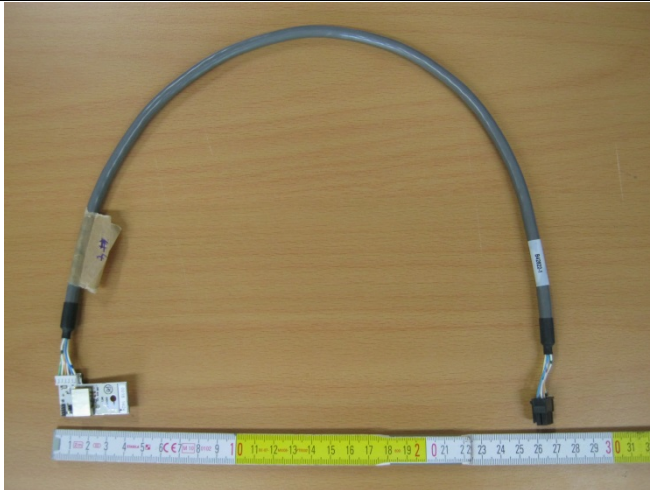

Sample #4 with cable

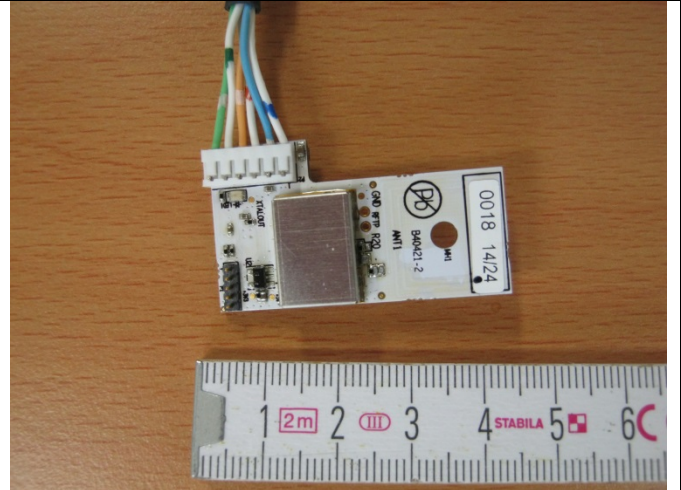


Sample #4, board side 1

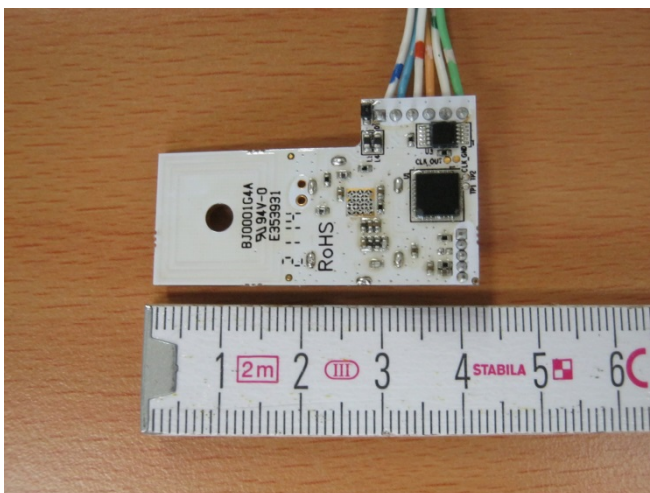


Sample #4, board side 2



Sample #6 (CW mode), with cable

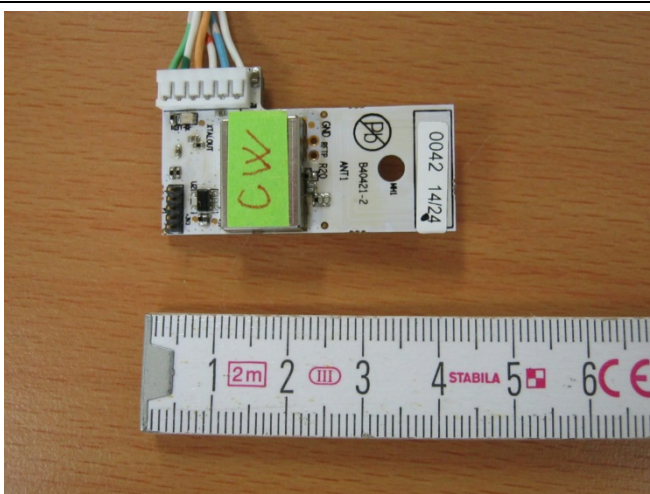

Sample #6 (CW mode), board side 1

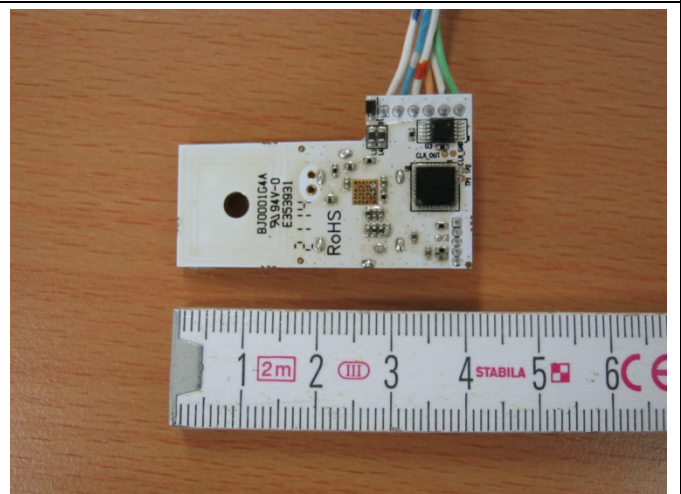

Sample #6 (CW mode), board side 2