

ANNEX 2 TO TEST REPORT # EMCC-140157ACAB, 2015-08-07

PHOTOGRAPHS OF EQUIPMENT UNDER TEST (EUT)

EQUIPMENT UNDER TEST:

Trade Name:	RFID Module
Type Designation(s):	B40420
Serial Number:	Sample #1 0086 14/26
	Sample #3: 0095 14/26
	Sample #7: 0023 14/26
Equipment Class:	Low Power Transceiver
Manufacturer:	Beckman Coulter Biomedical GmbH
Address:	Sauerbruchstraße 50
	81377 München
	Germany
Phone:	+49 89 579589-3606
Fax:	+49 89 579589-3505


RELEVANT STANDARD(S): 47 CFR 15.225

MEASUREMENT PROCEDURE:


☒ RSS-Gen Issue 4 ☒ ANSI C63.10-2013 ☐ Other

Test of Beckman Coulter RFID Module type B40420 to 47 CFR 15.225 and RSS-210 Issue 8


1 PHOTOS OF TEST SAMPLES

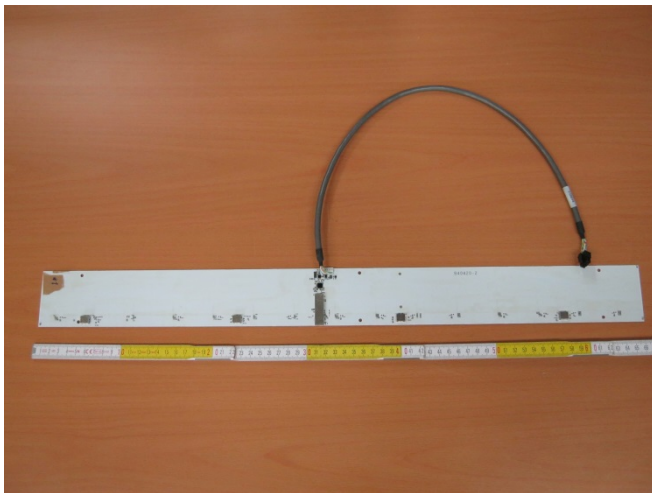


Sample #1 back view

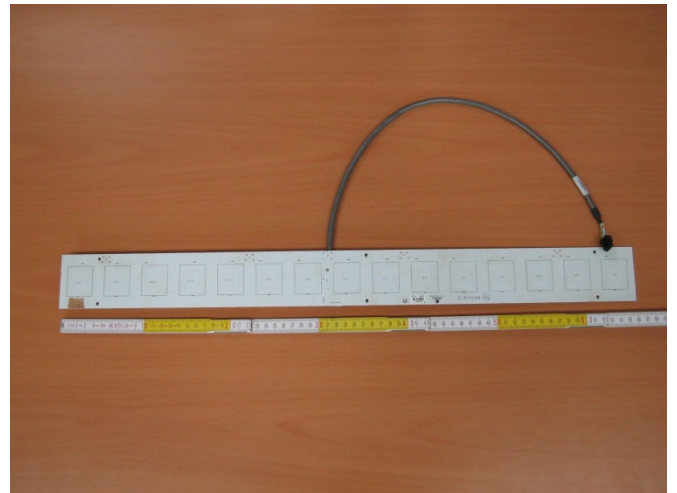

Sample #1 top view

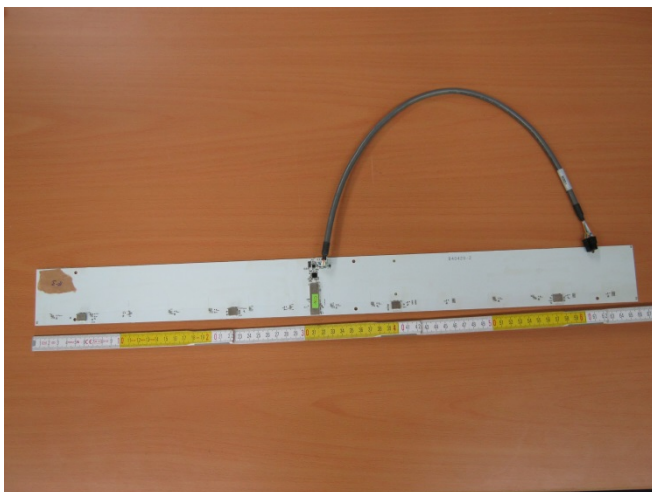


Sample #3 (CW mode) back view

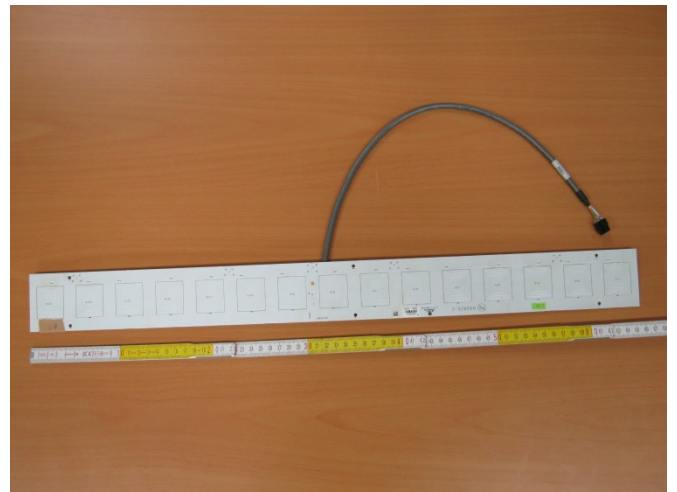

Sample #3 (CW mode) top view



Sample #7 with dummy load, back view

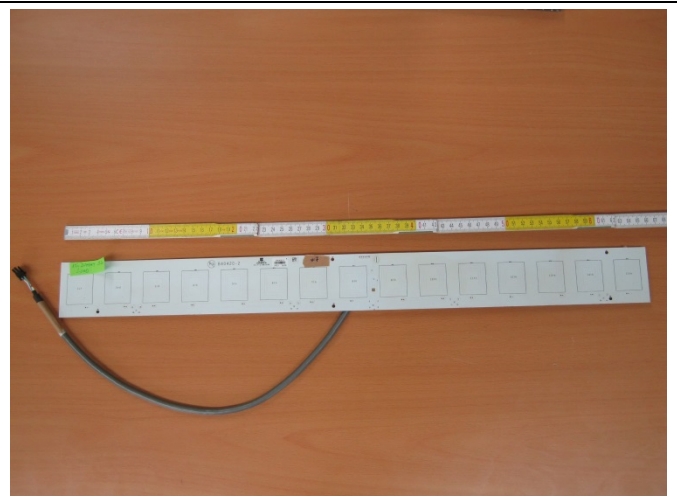

Sample #7 with dummy load, top view