A.5: Conducted Spurious Emission

Test Graphs

Channel Bandwidth: 1.4 MHz

(Channel Bandwidth: 1.4 MHz)_LCH_QPSK_1RB#0

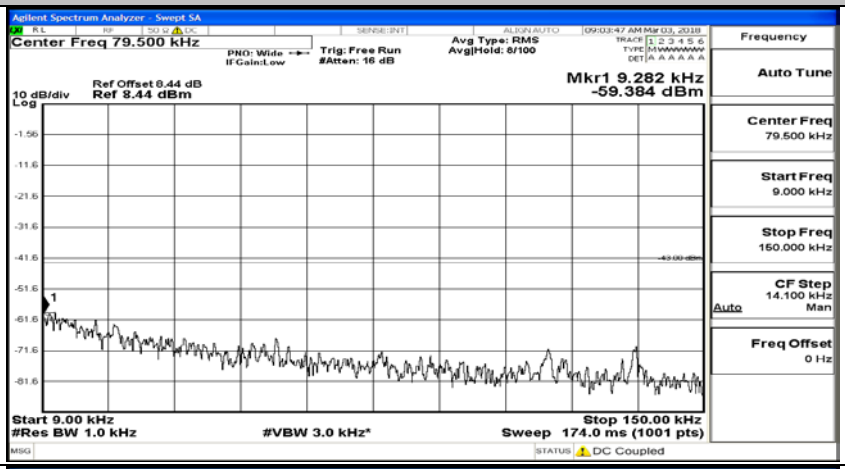

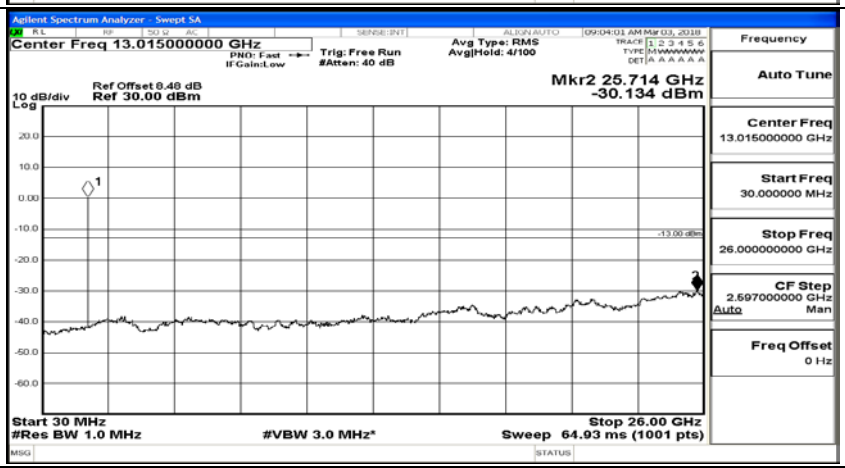

(Channel Bandwidth: 1.4 MHz)_LCH_QPSK_6RB#0

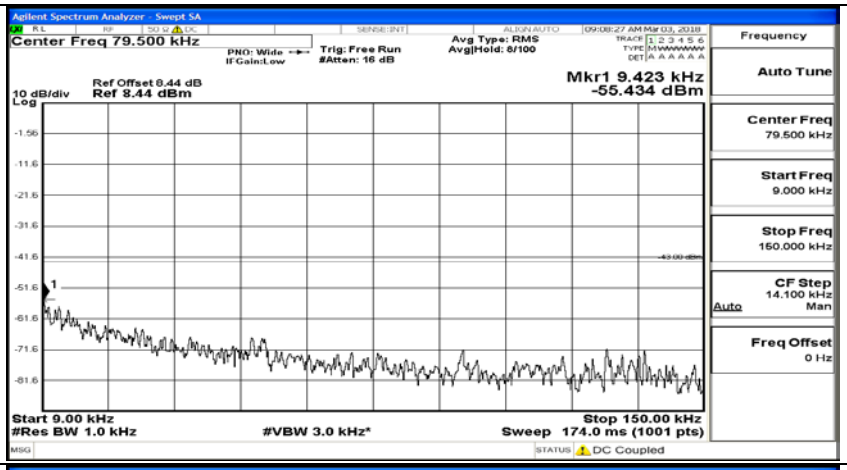
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:08:27 AM Mar 03, 2018
Mkr1 9.423 kHz
-55.434 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:08:35 AM Mar 03, 2018
Mkr1 8.598 MHz
-42.338 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

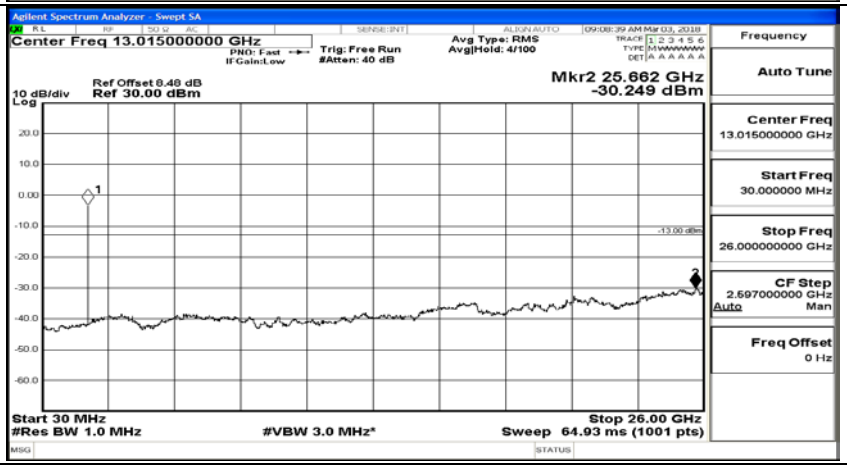
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:08:39 AM Mar 03, 2018
Mkr2 25.662 GHz
-30.249 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_MCH_QPSK_1RB#0
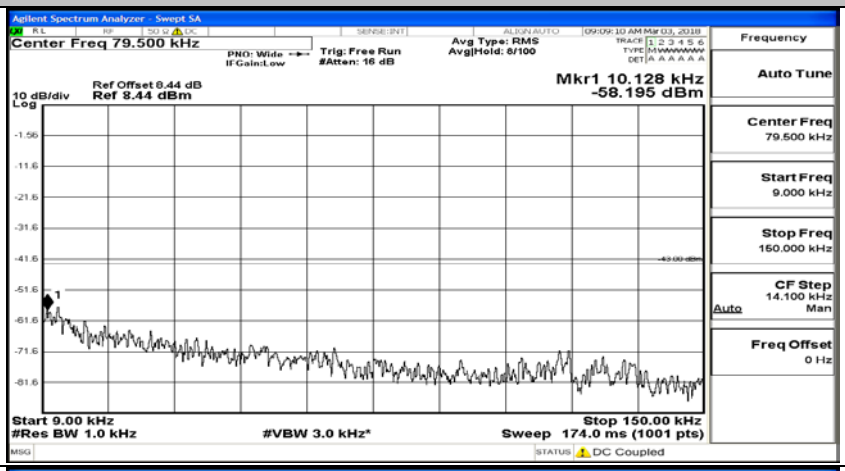
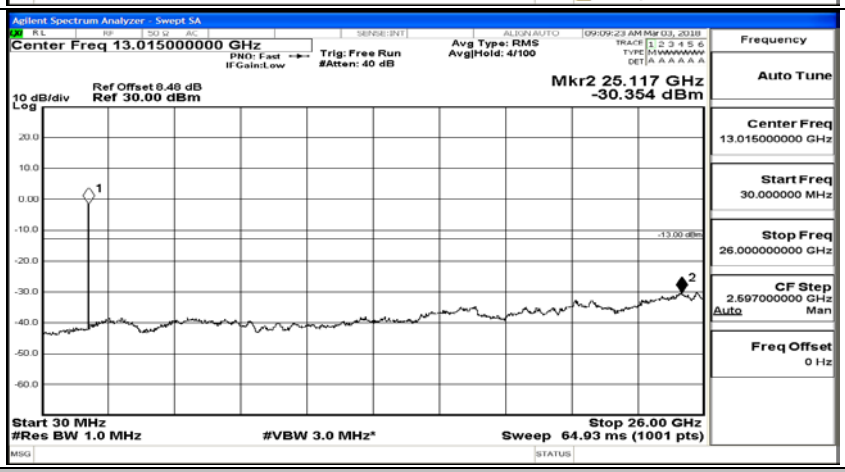
(Channel Bandwidth: 1.4 MHz)_MCH_QPSK_6RB#0

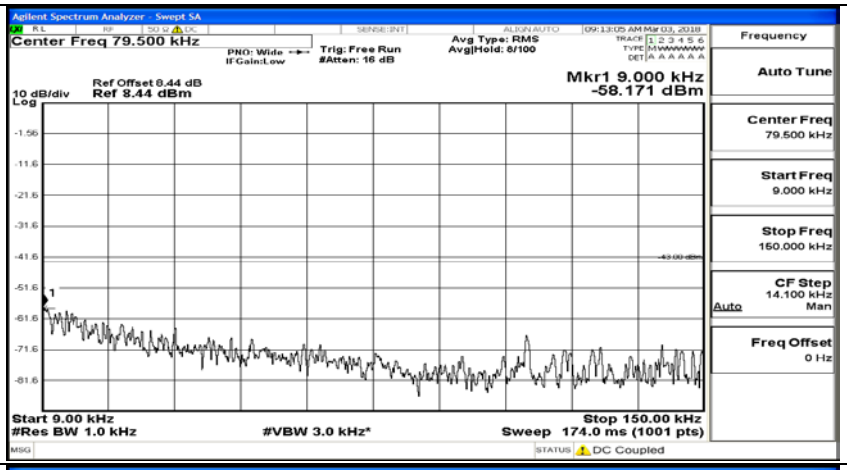
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:13:05 AM Mar 03, 2018
Mkr1 9.000 kHz
-58.171 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:13:14 AM Mar 03, 2018
Mkr1 8.418 MHz
-41.559 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

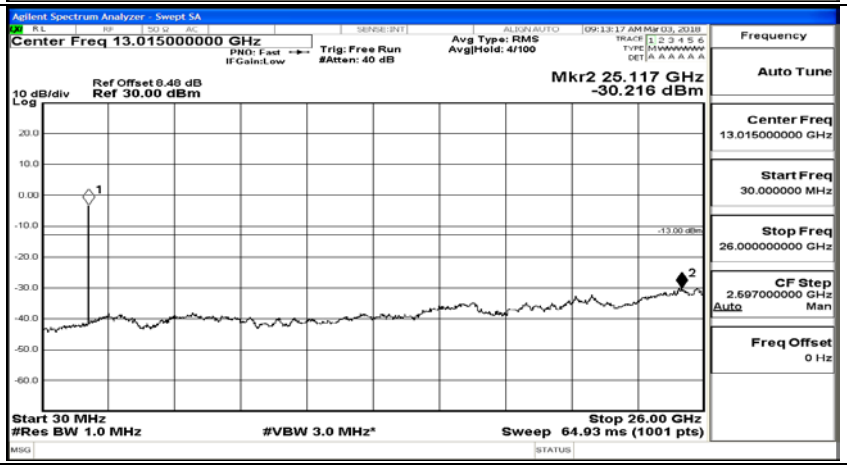
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:13:17 AM Mar 03, 2018
Mkr2 25.117 GHz
-30.216 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_HCH_QPSK_1RB#0
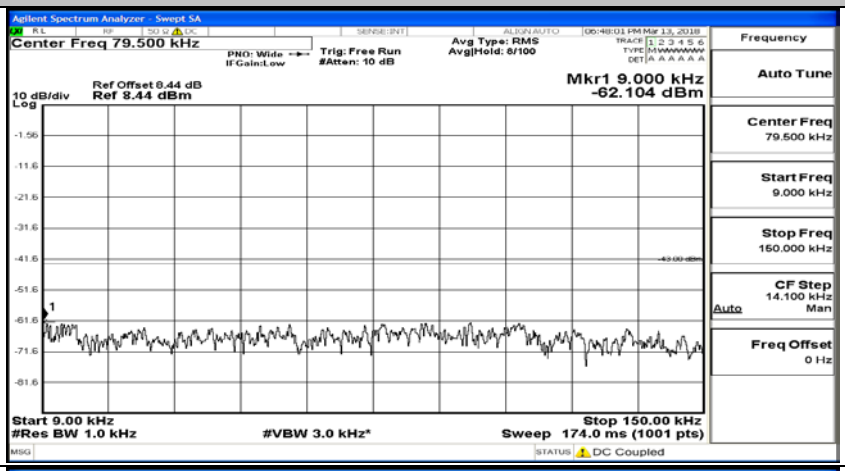
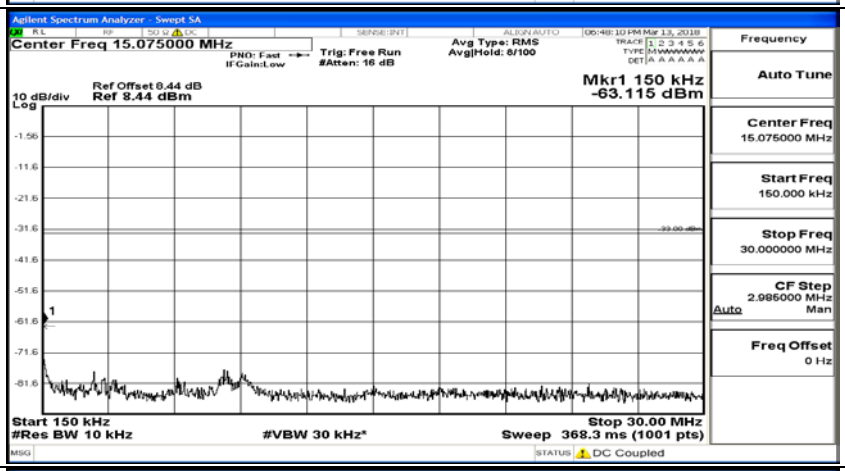
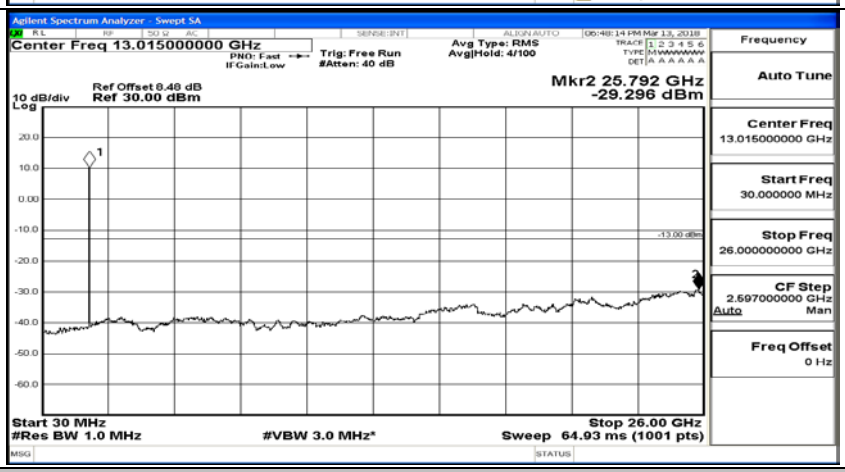
(Channel Bandwidth: 1.4 MHz)_HCH_QPSK_6RB#0

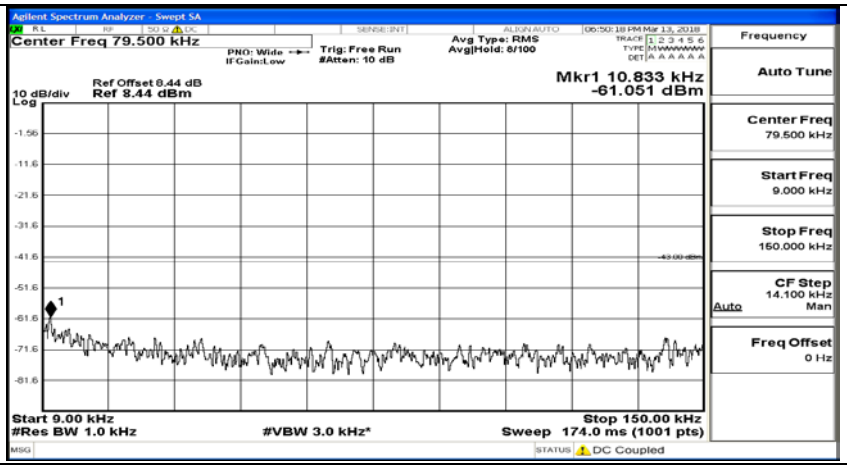
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 8/100
06:50:18 PM Mar 13, 2018
Mkr1 10.833 kHz
-61.051 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

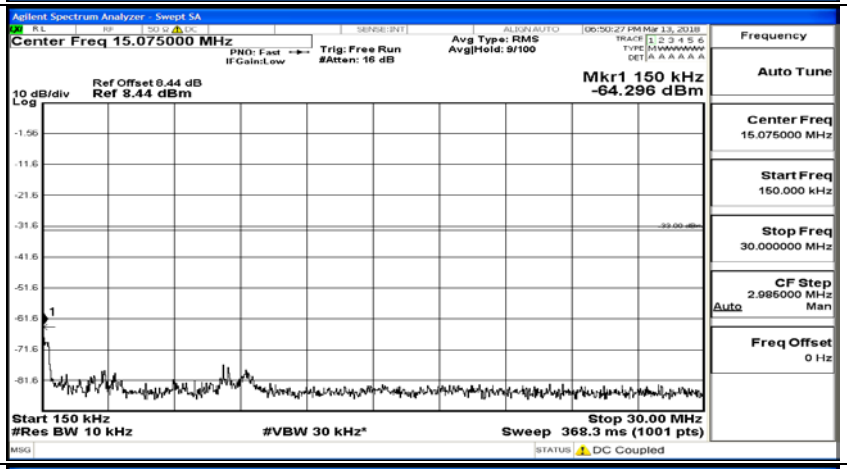
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
06:50:27 PM Mar 13, 2018
Mkr1 150 kHz
-64.296 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

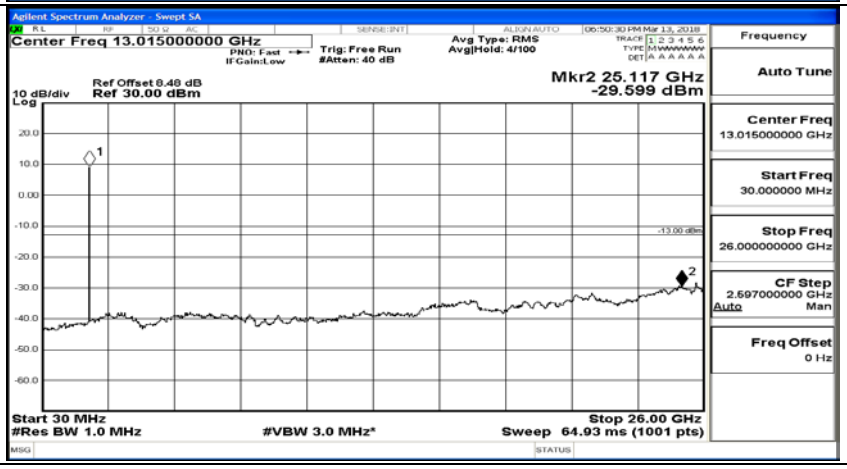
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
06:50:30 PM Mar 13, 2018
Mkr2 25.117 GHz
-29.599 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_LCH_16QAM_1RB#0
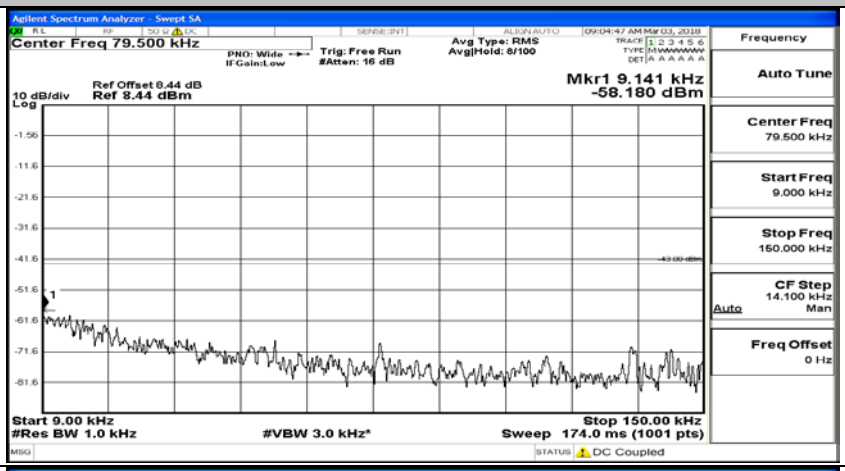
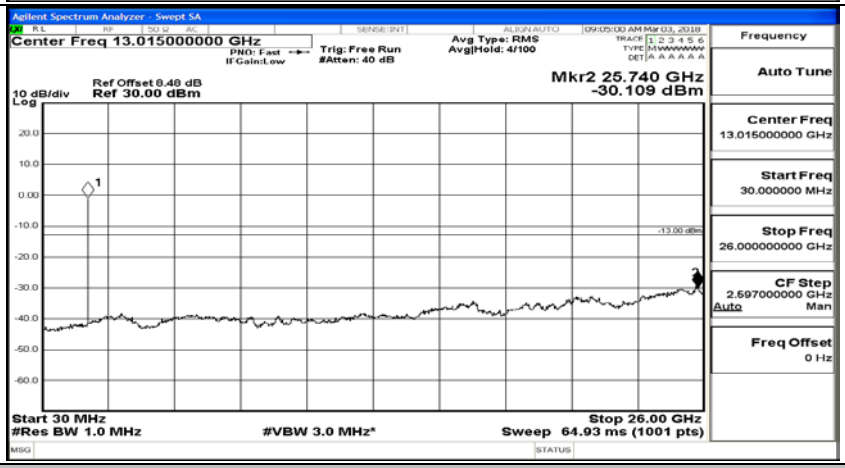
(Channel Bandwidth: 1.4 MHz)_LCH_16QAM_6RB#0

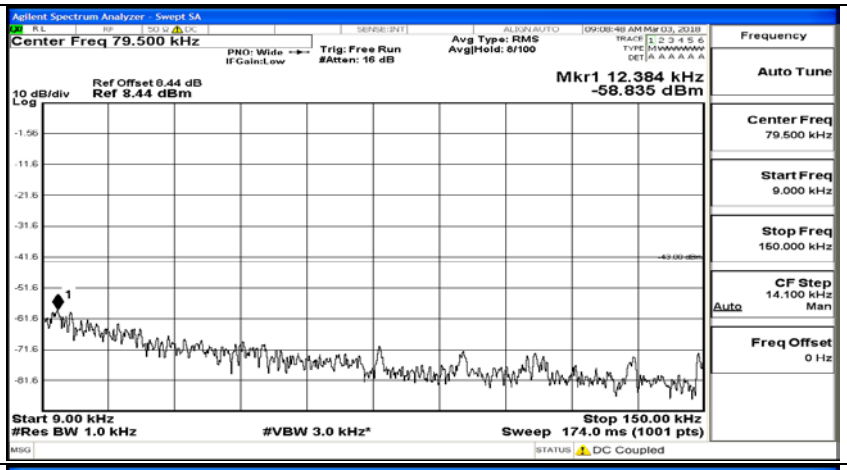
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:08:48 AM Mar 03, 2018
Mkr1 12.384 kHz
-58.835 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:08:57 AM Mar 03, 2018
Mkr1 8.269 MHz
-42.468 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

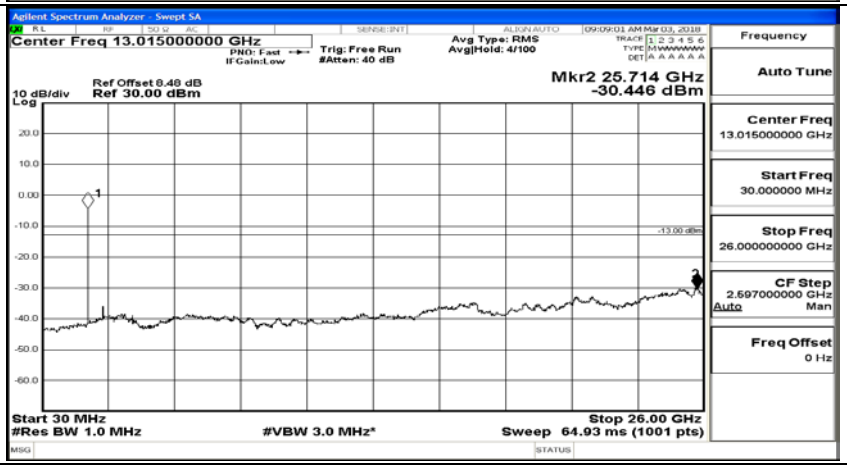
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:09:01 AM Mar 03, 2018
Mkr2 25.714 GHz
-30.446 dBm
Ref Offset 8.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_MCH_16QAM_1RB#0
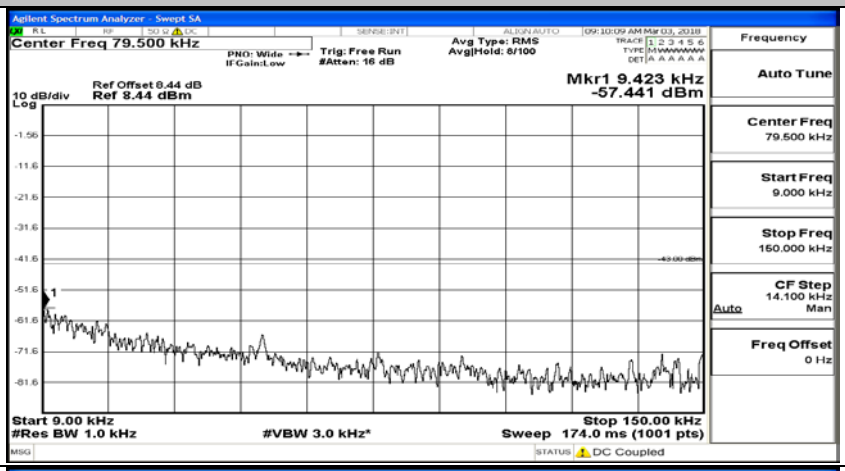
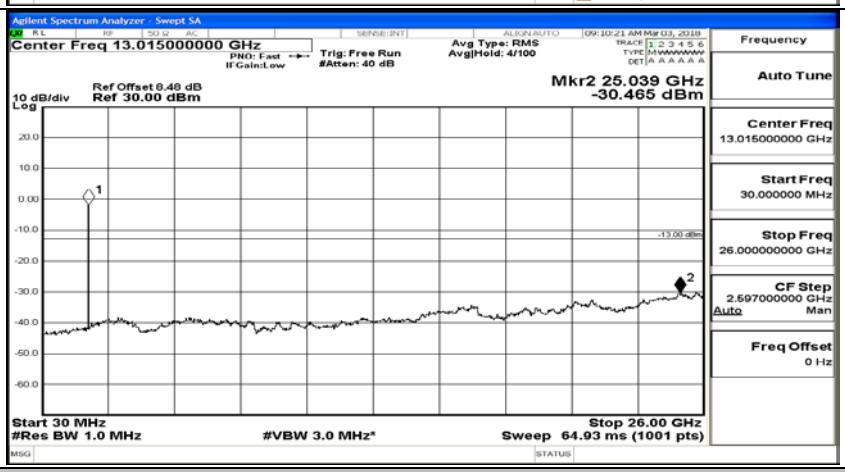
(Channel Bandwidth: 1.4 MHz)_MCH_16QAM_6RB#0

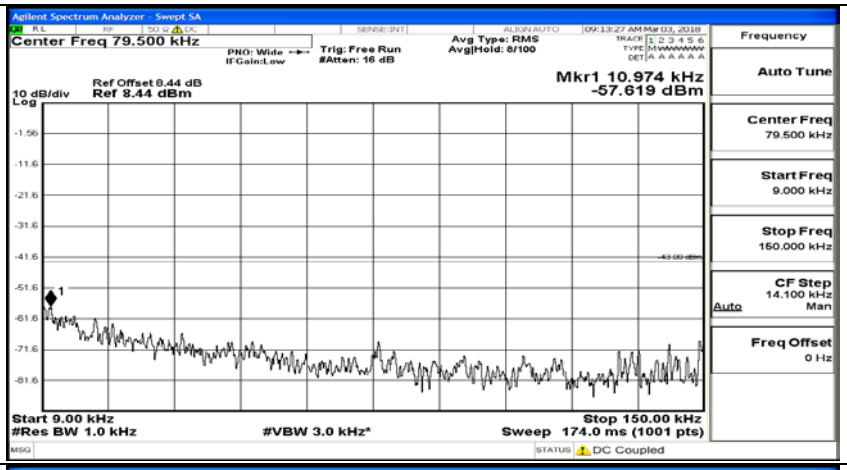
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:13:27 AM Mar 03, 2018
Mkr1 10.974 kHz
-57.619 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:13:35 AM Mar 03, 2018
Mkr1 8.329 MHz
-40.746 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

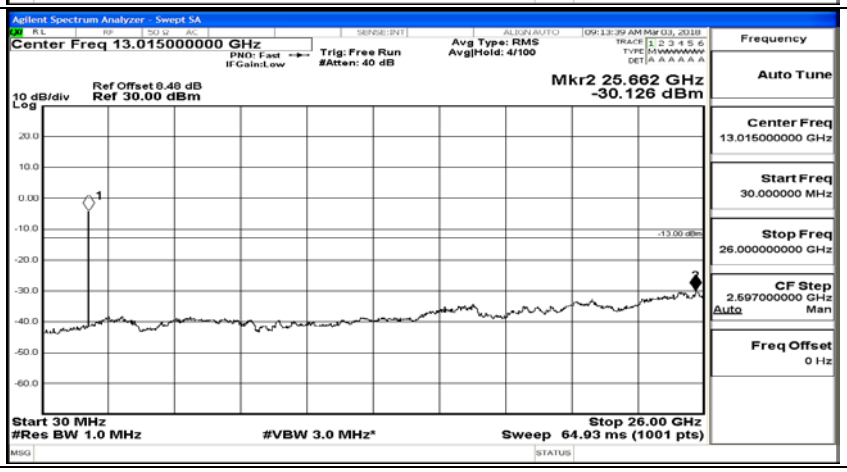
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:13:39 AM Mar 03, 2018
Mkr2 25.662 GHz
-30.126 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_HCH_16QAM_1RB#0
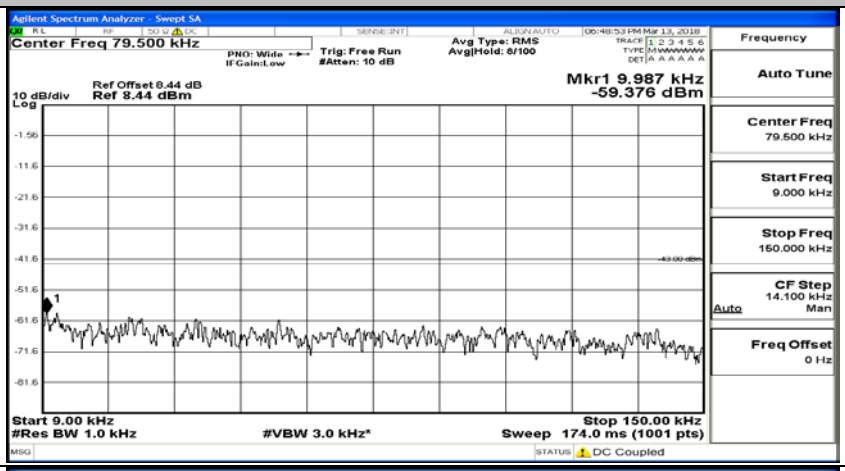
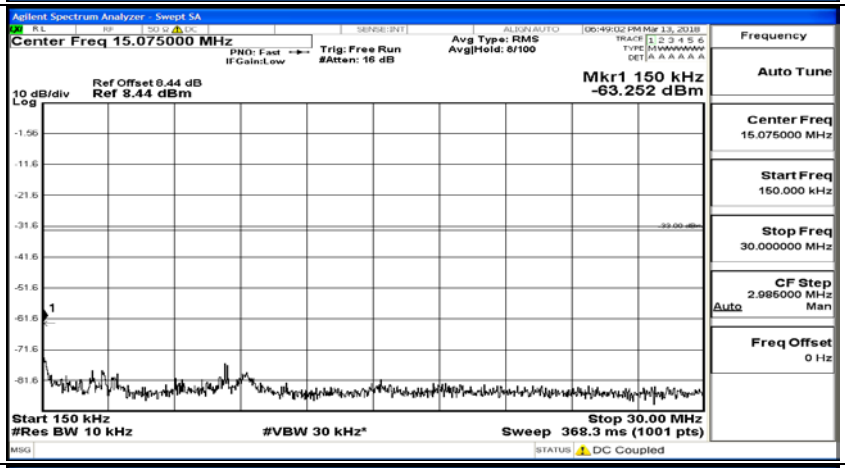
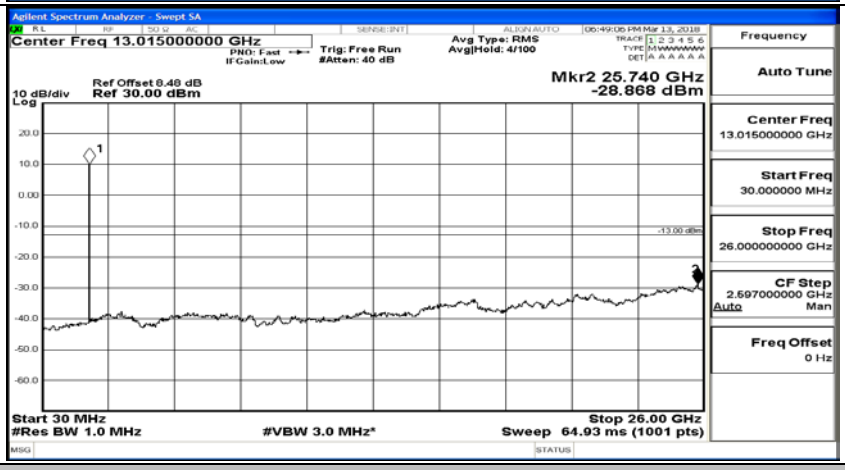
(Channel Bandwidth: 1.4 MHz)_HCH_16QAM_6RB#0

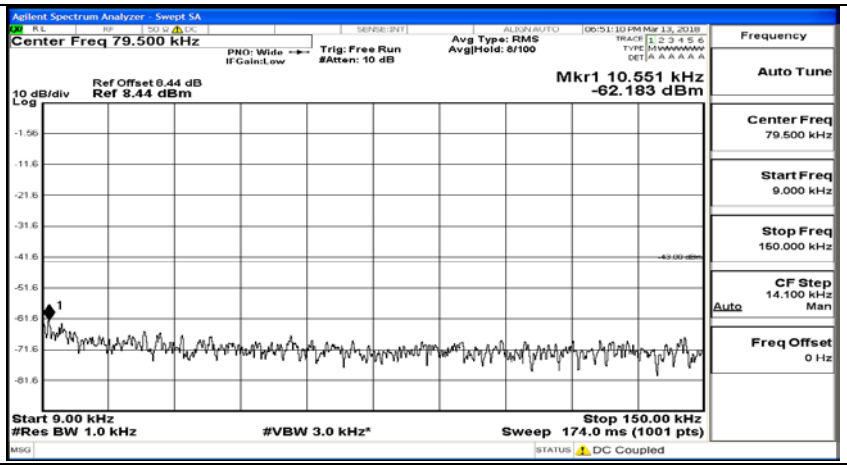
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 8/100
06:51:10 PM Mar 13, 2018
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
Mkr1 10.551 kHz
-62.183 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

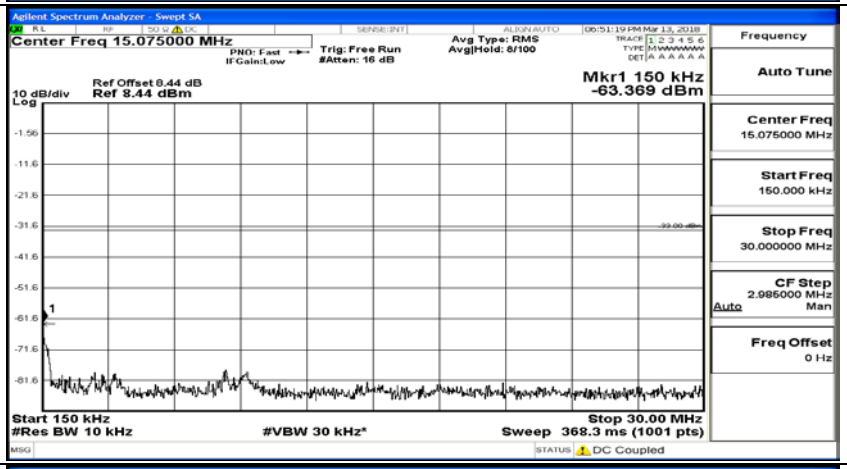
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
06:51:19 PM Mar 13, 2018
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
Mkr1 150 kHz
-63.369 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

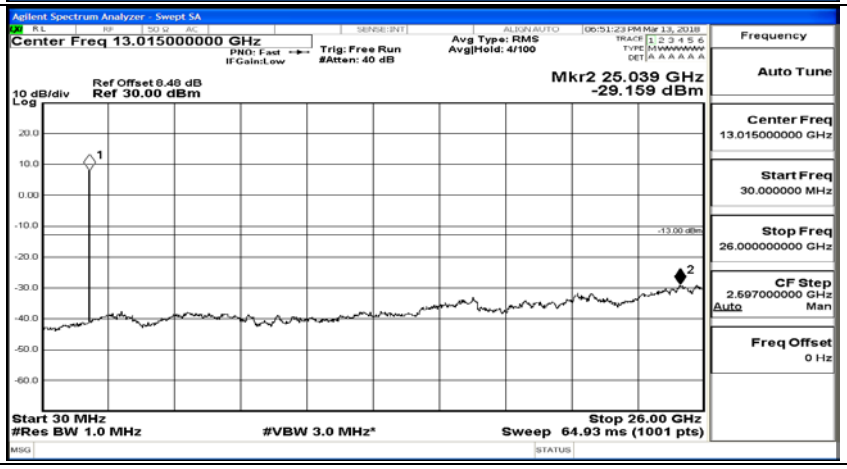
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
06:51:23 PM Mar 13, 2018
Ref Offset 8.48 dB
10 dB/div
Log
Ref 30.00 dBm
Mkr2 25.039 GHz
-29.159 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 3 MHz

(Channel Bandwidth: 3 MHz)_LCH_QPSK_1RB#0
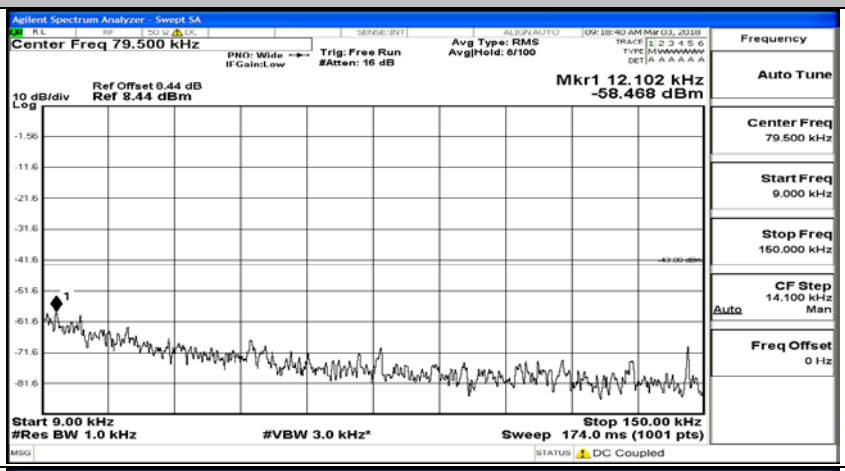
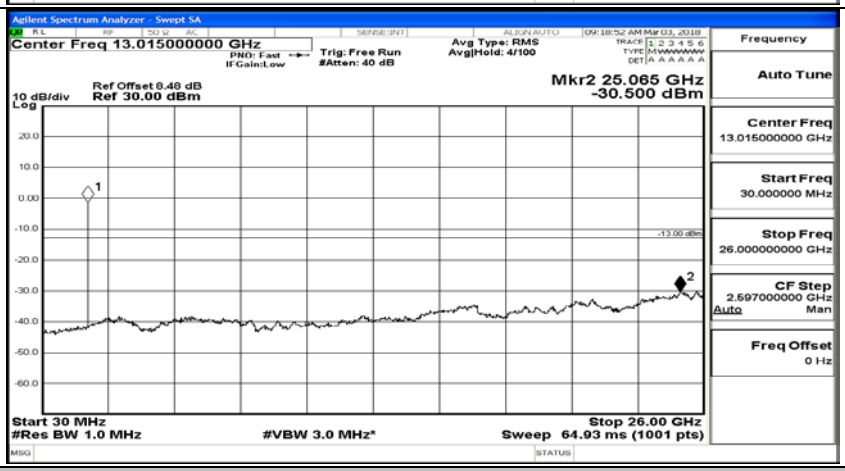
(Channel Bandwidth: 3 MHz)_LCH_QPSK_15RB#0

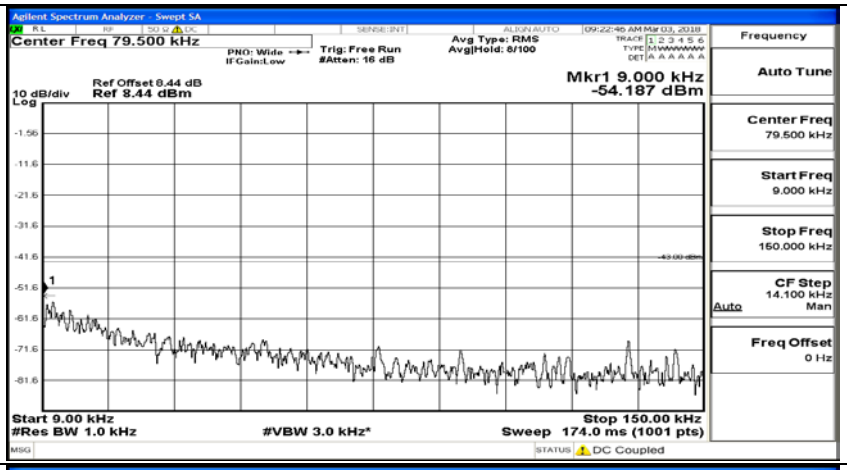
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:22:46 AM Mar 03, 2018
Mkr1 9.000 kHz
-54.187 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:22:55 AM Mar 03, 2018
Mkr1 8.418 MHz
-41.056 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

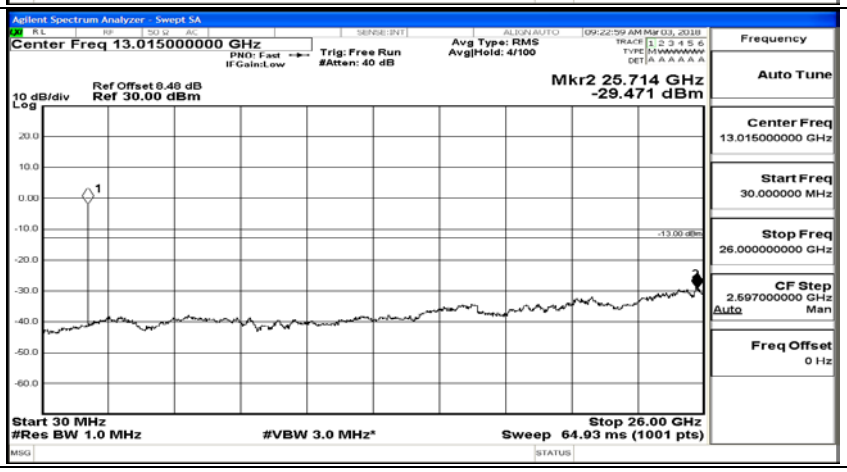
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:22:59 AM Mar 03, 2018
Mkr2 25.714 GHz
-29.471 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_MCH_QPSK_1RB#0
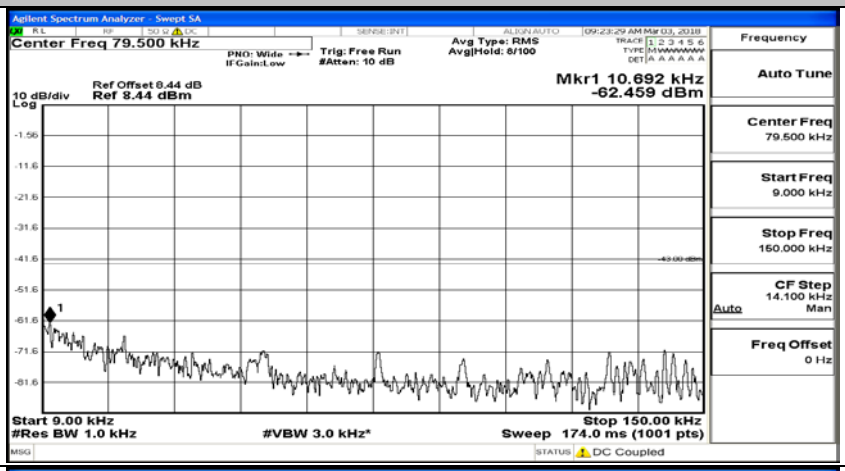
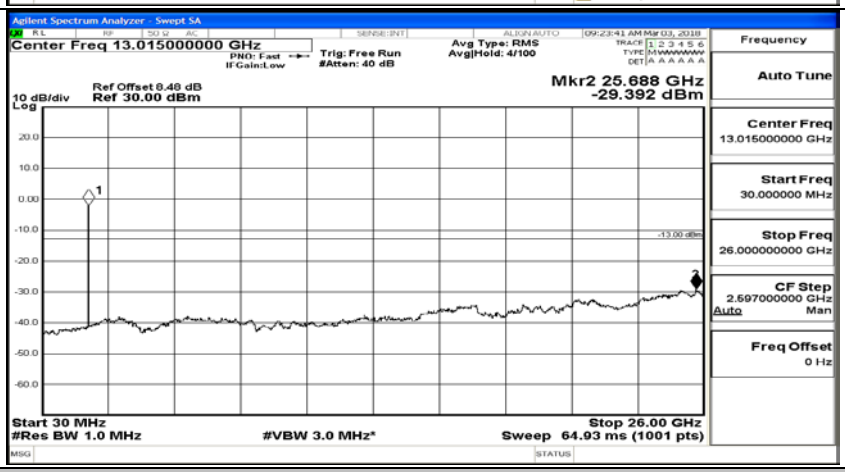
(Channel Bandwidth: 3 MHz)_MCH_QPSK_15RB#0

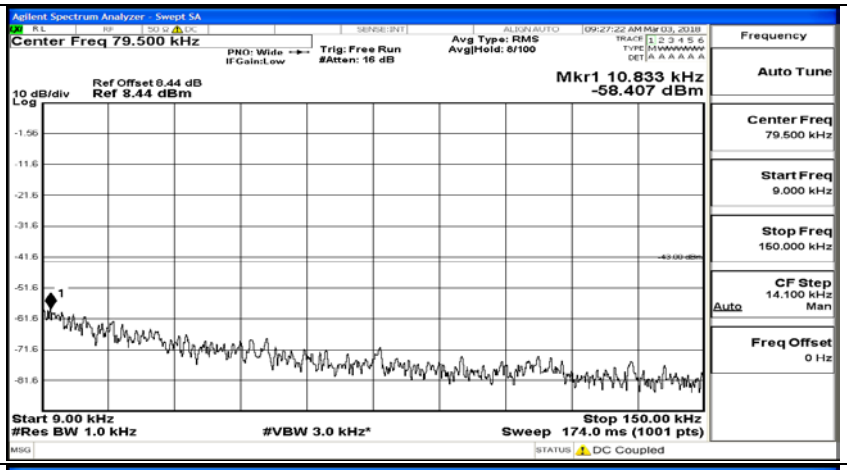
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:27:22 AM Mar 03, 2018
Mkr1 10.833 kHz
-58.407 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:27:31 AM Mar 03, 2018
Mkr1 8.329 MHz
-41.055 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

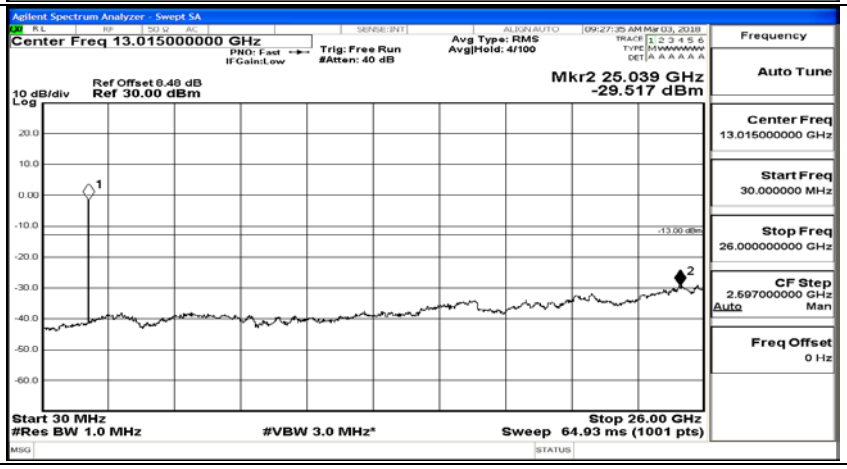
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:27:35 AM Mar 03, 2018
Mkr2 25.039 GHz
-29.517 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_HCH_QPSK_1RB#0
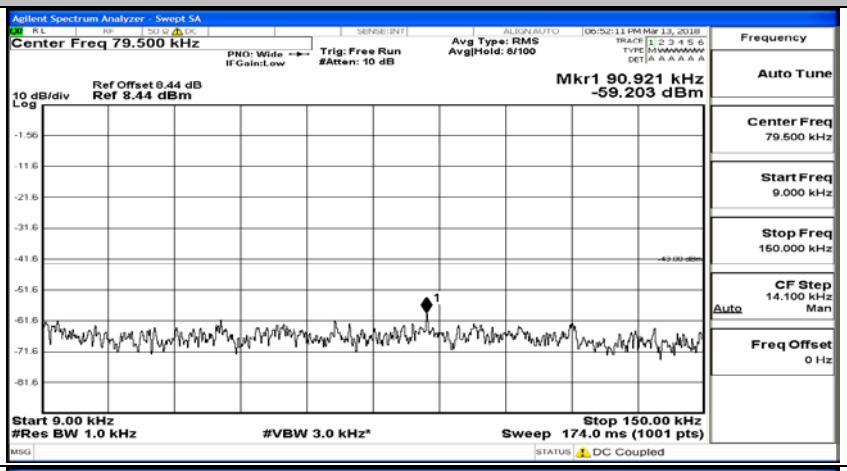
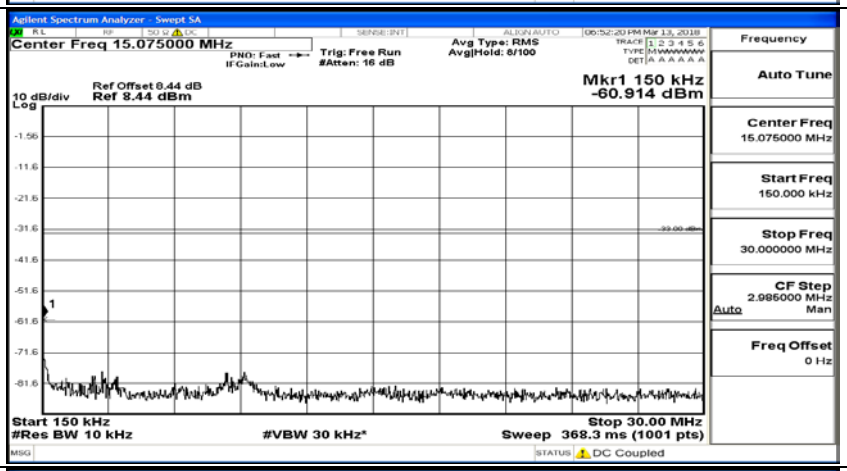
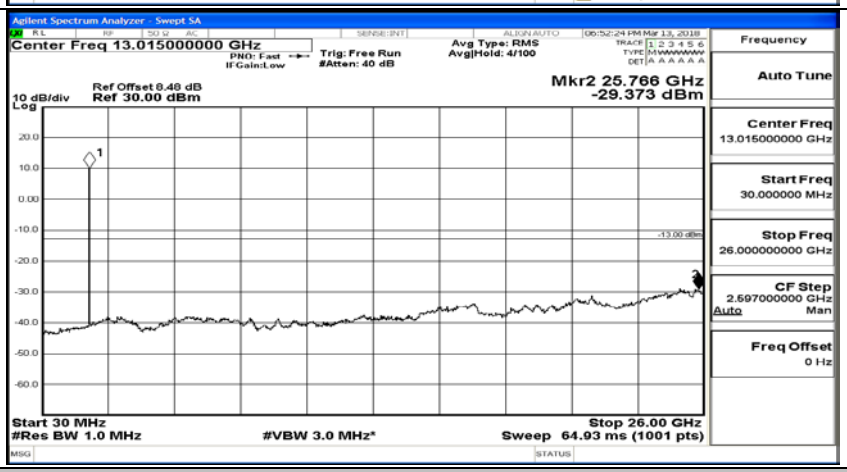
(Channel Bandwidth: 3 MHz)_HCH_QPSK_15RB#0

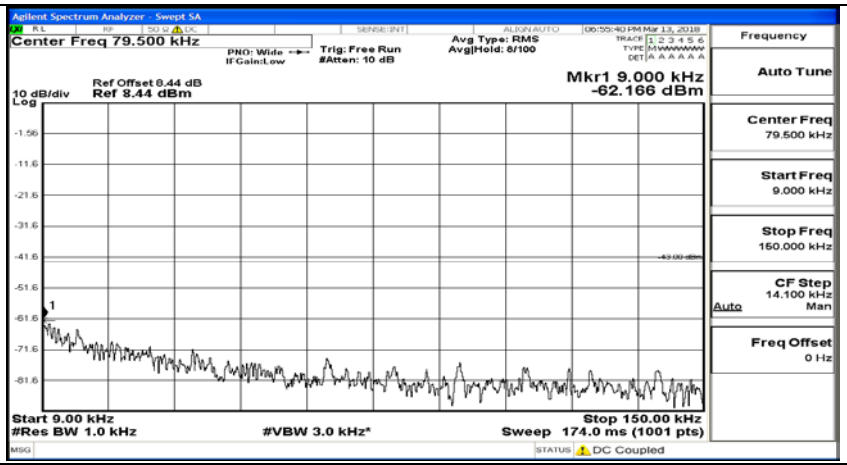
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 8/100
06:55:40 PM Mar 13, 2018
Mkr1 9.000 kHz
-62.166 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

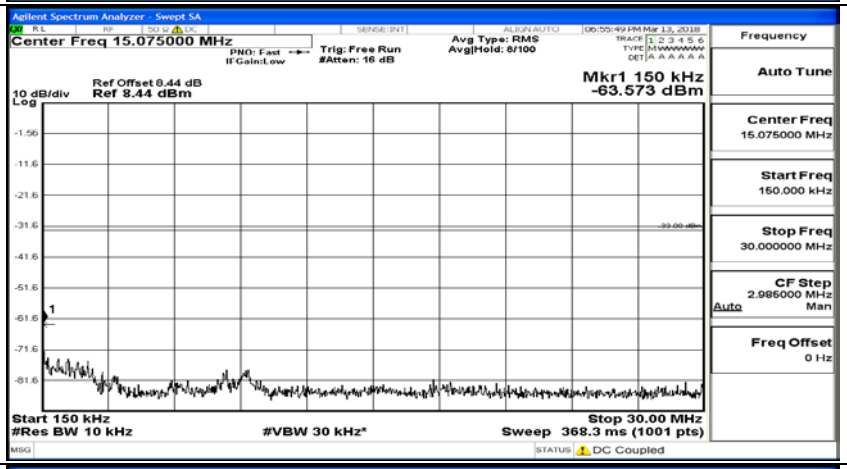
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
06:55:49 PM Mar 13, 2018
Mkr1 150 kHz
-63.573 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

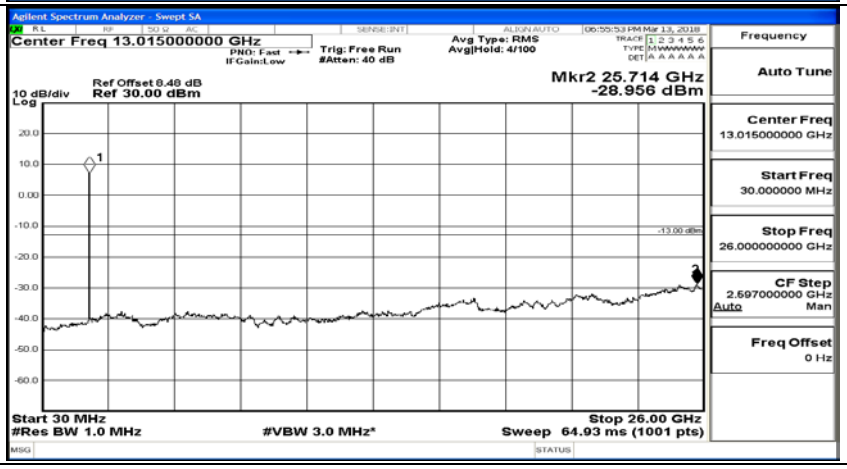
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
06:55:53 PM Mar 13, 2018
Mkr2 25.714 GHz
-28.956 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_LCH_16QAM_1RB#0
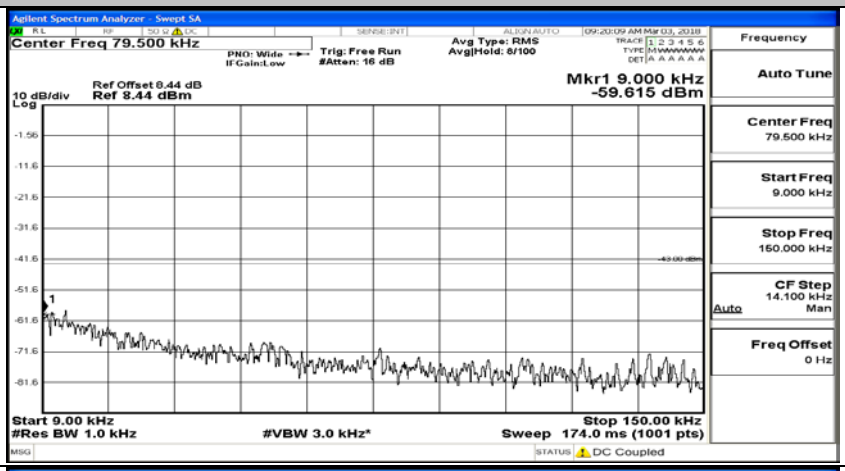
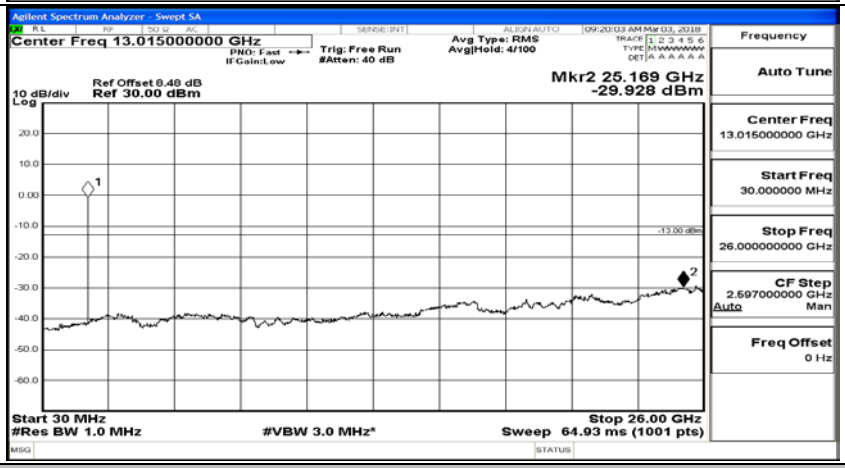
(Channel Bandwidth: 3 MHz)_LCH_16QAM_15RB#0

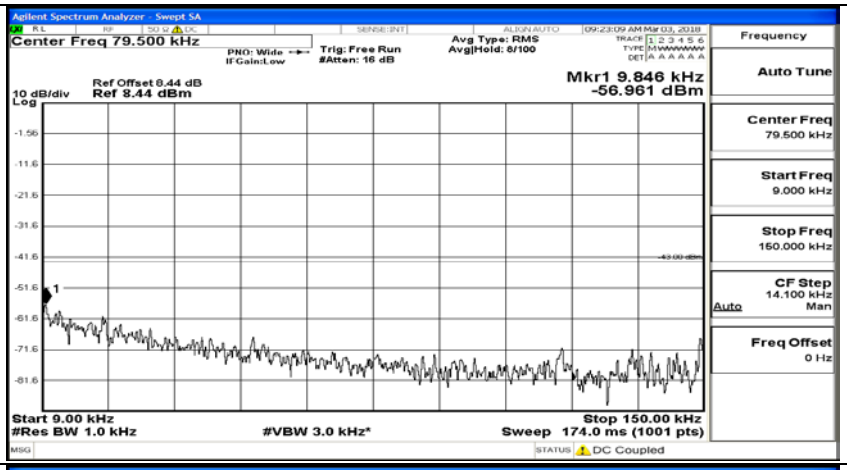
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:23:09 AM Mar 03, 2018
Mkr1 9.846 kHz
-56.961 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:23:18 AM Mar 03, 2018
Mkr1 478 kHz
-42.662 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

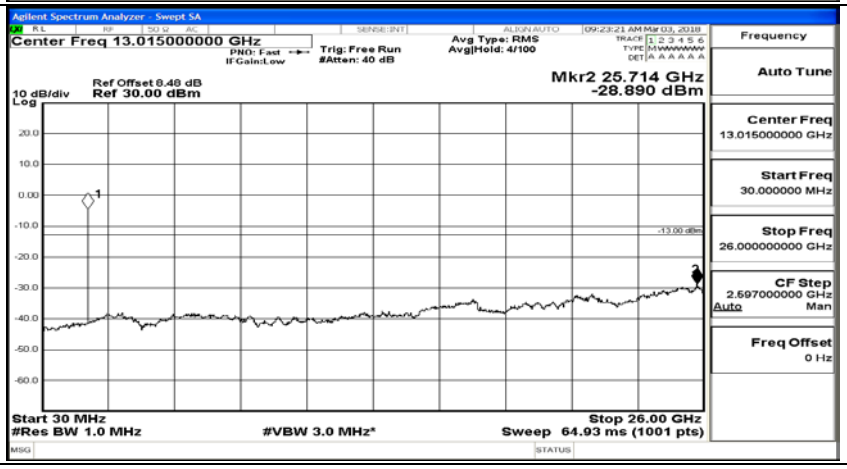
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:23:21 AM Mar 03, 2018
Mkr2 25.714 GHz
-28.890 dBm
Ref Offset 8.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_MCH_16QAM_1RB#0
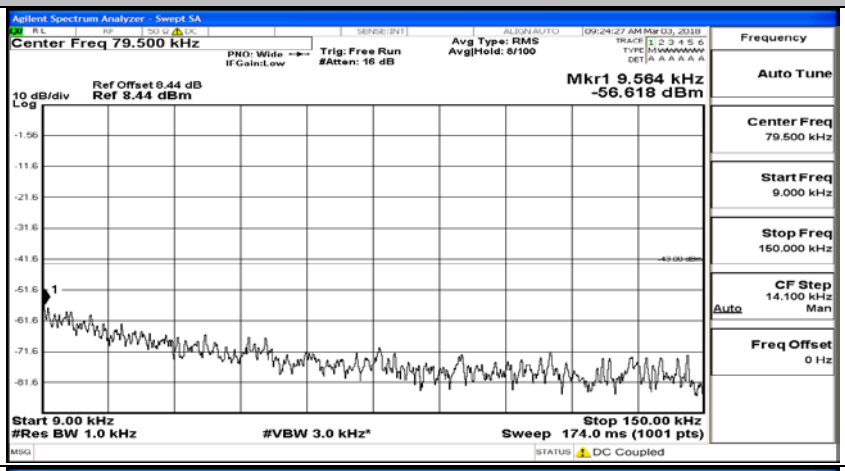
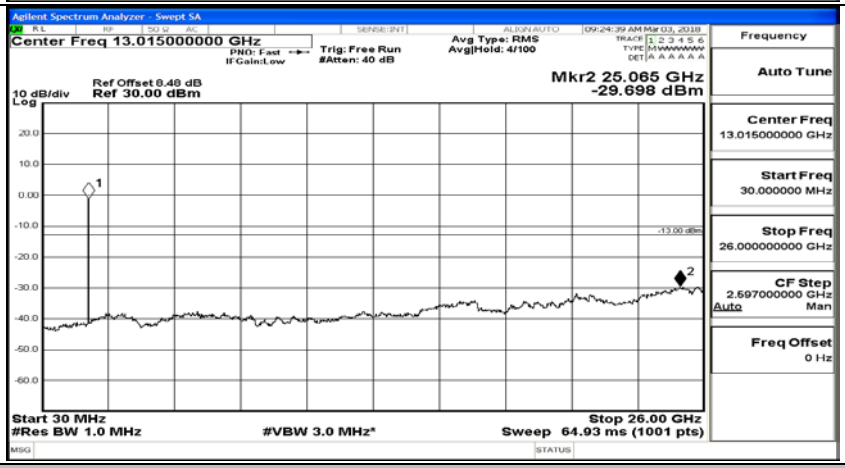
(Channel Bandwidth: 3 MHz)_MCH_16QAM_15RB#0

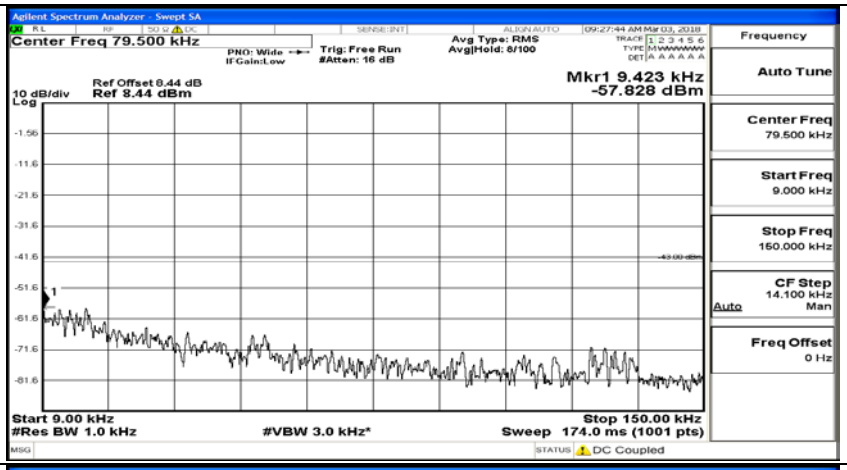
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:27:44 AM Mar 03, 2018
Mkr1 9.423 kHz
-57.828 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:27:53 AM Mar 03, 2018
Mkr1 8.508 MHz
-38.651 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

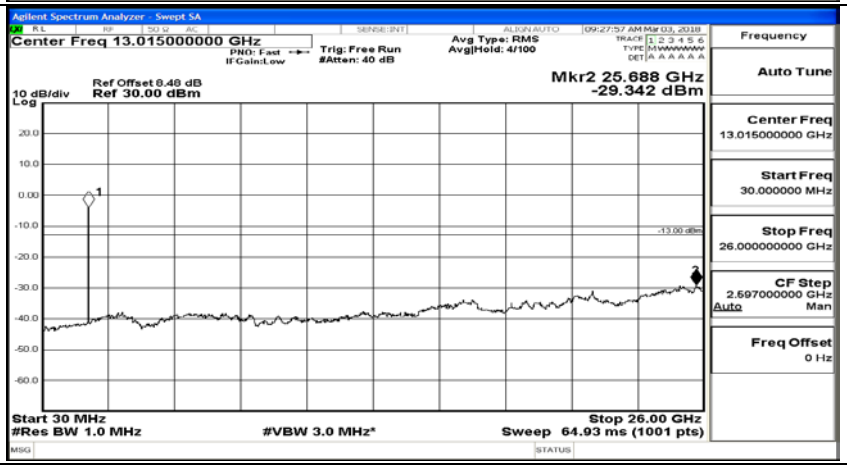
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:27:57 AM Mar 03, 2018
Mkr2 25.688 GHz
-29.342 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_HCH_16QAM_1RB#0
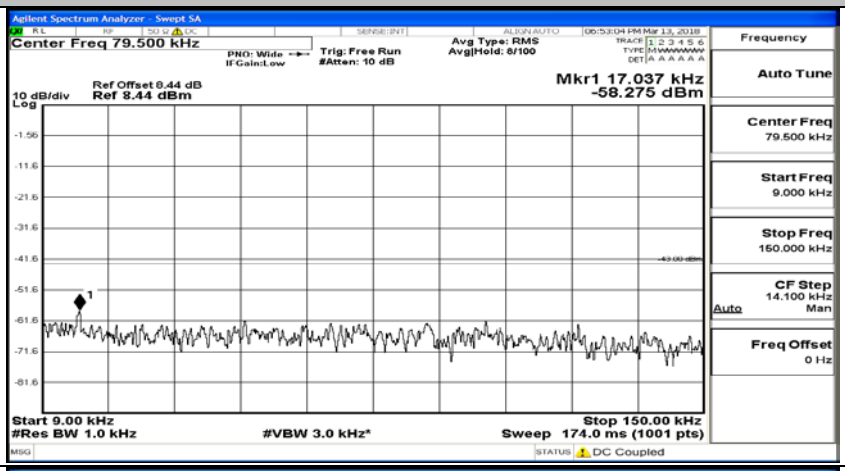
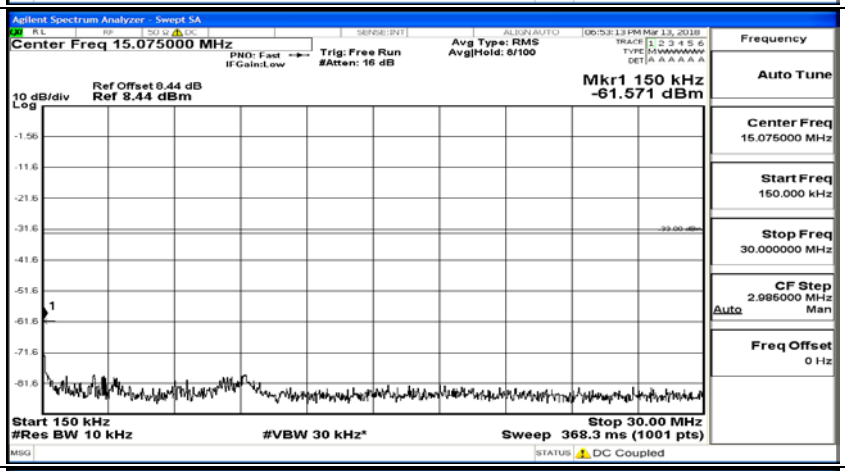
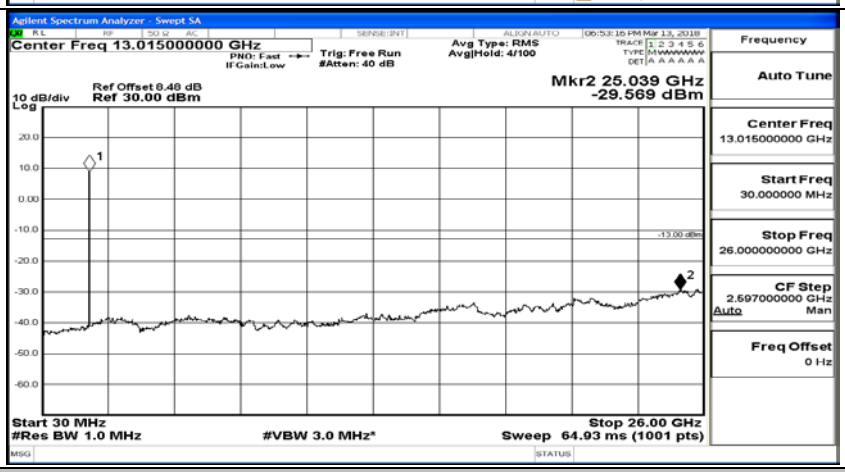
(Channel Bandwidth: 3 MHz)_HCH_16QAM_15RB#0

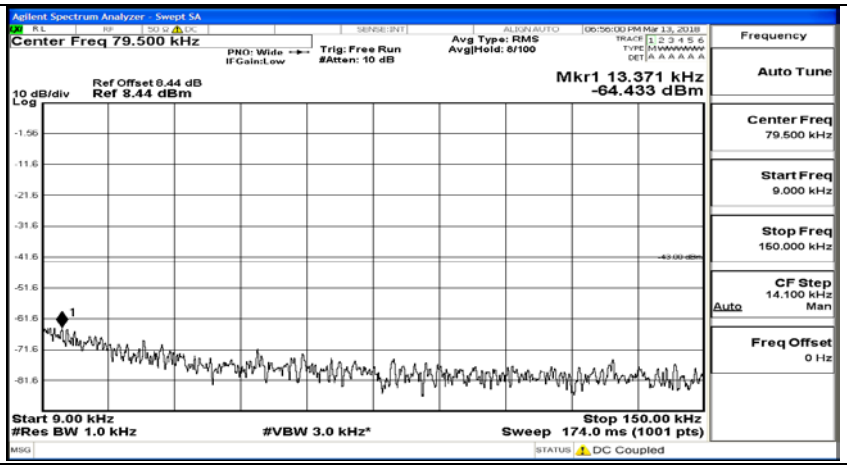
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 8/100
06:56:00 PM Mar 13, 2018
Mkr1 13.371 kHz
-64.433 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

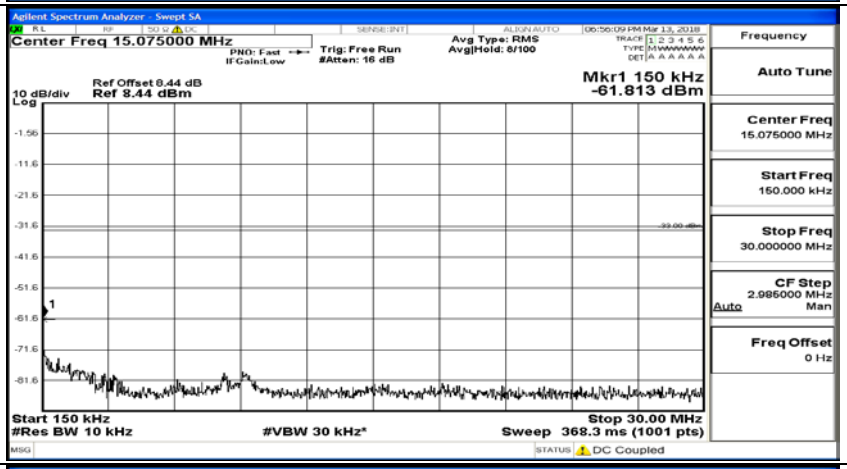
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
06:56:09 PM Mar 13, 2018
Mkr1 150 kHz
-61.813 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

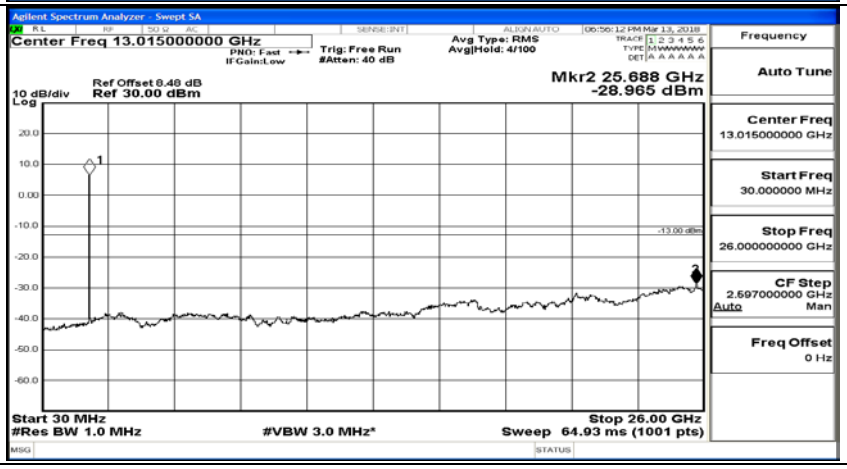
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
06:56:12 PM Mar 13, 2018
Mkr2 25.688 GHz
-28.965 dBm
Ref Offset 9.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 5 MHz

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#0
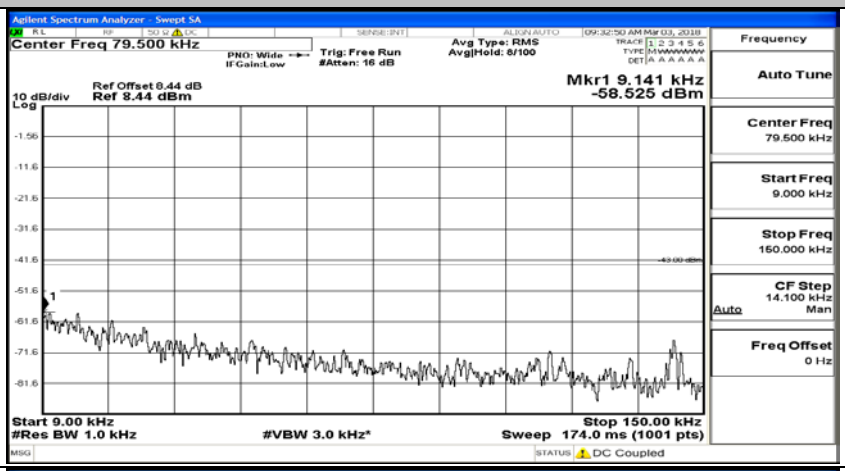
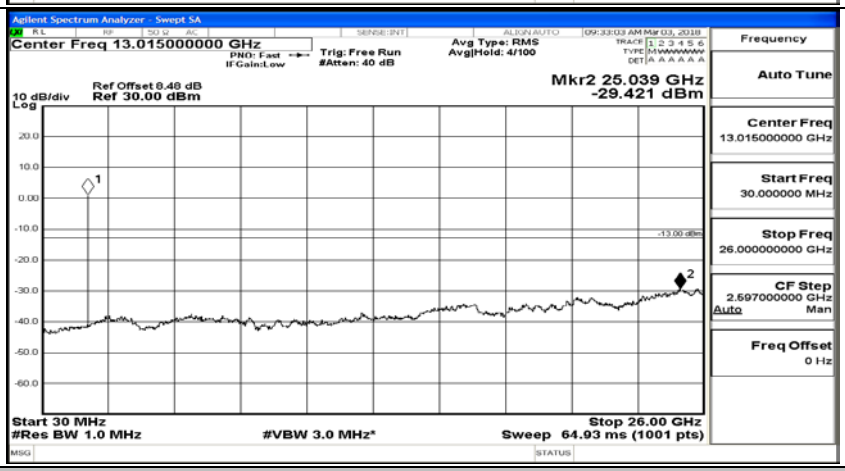
(Channel Bandwidth: 5 MHz)_LCH_QPSK_25RB#0

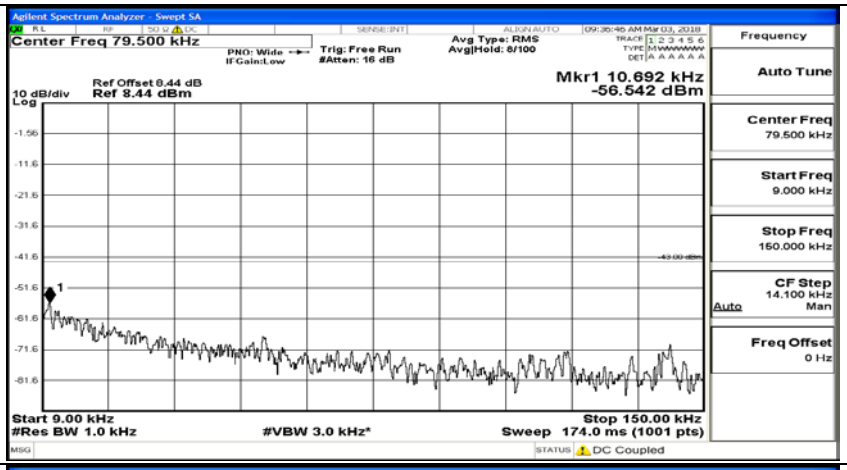
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:36:46 AM Mar 03, 2018
Mkr1 10.692 kHz
-56.542 dBm
Ref Offset 8.44 dB
10 dB/div
Ref 8.44 dBm
Log
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
09:36:55 AM Mar 03, 2018
Mkr1 8.359 MHz
-41.516 dBm
Ref Offset 8.44 dB
10 dB/div
Ref 8.44 dBm
Log
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

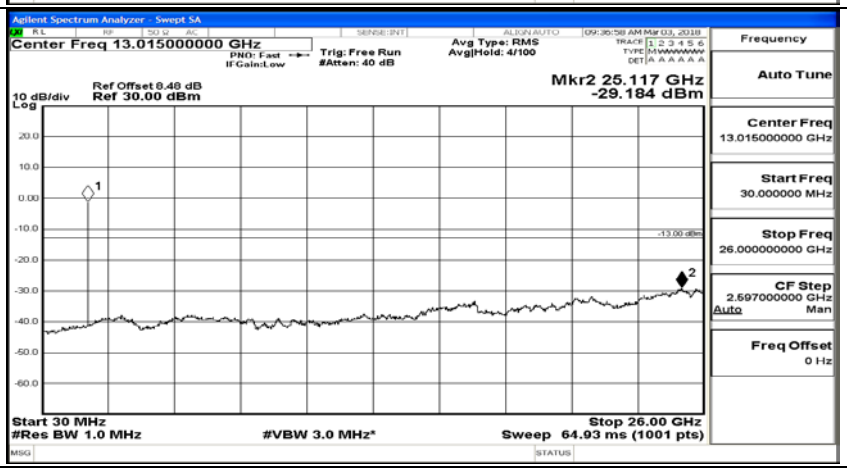
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
09:36:58 AM Mar 03, 2018
Mkr2 25.117 GHz
-29.184 dBm
Ref Offset 9.48 dB
10 dB/div
Ref 30.00 dBm
Log
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#0
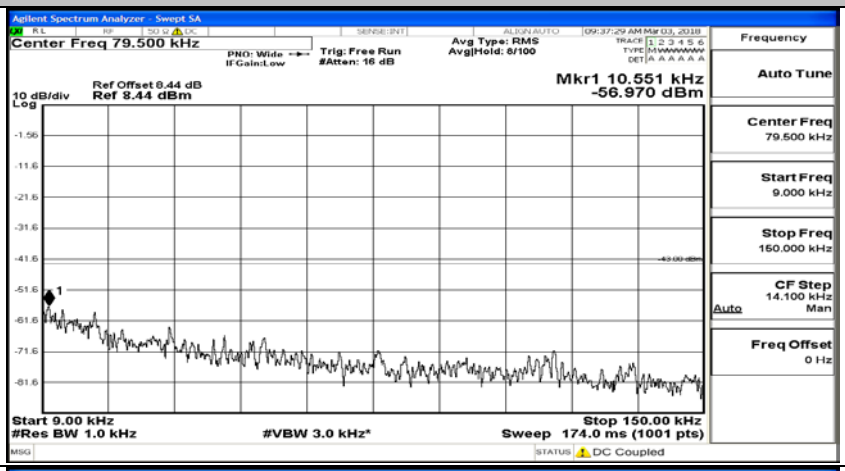
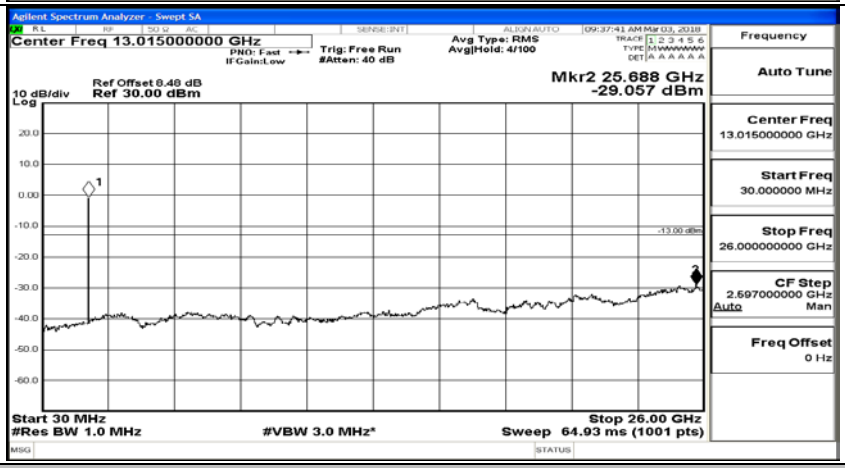
(Channel Bandwidth: 5 MHz)_MCH_QPSK_25RB#0

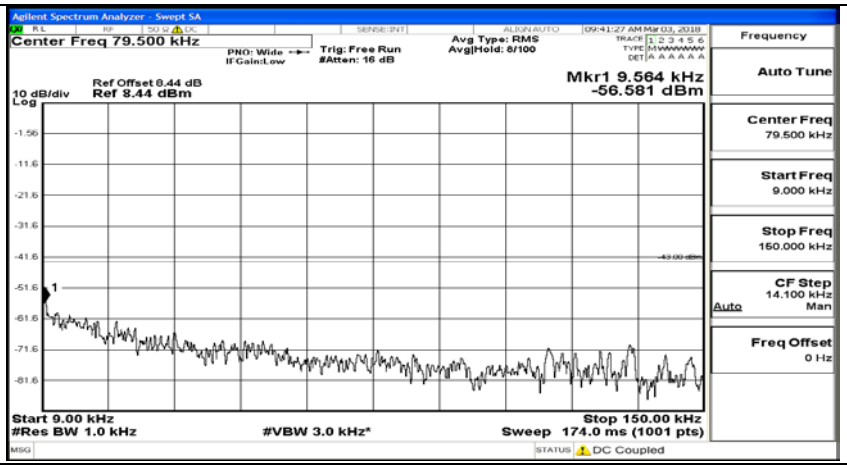

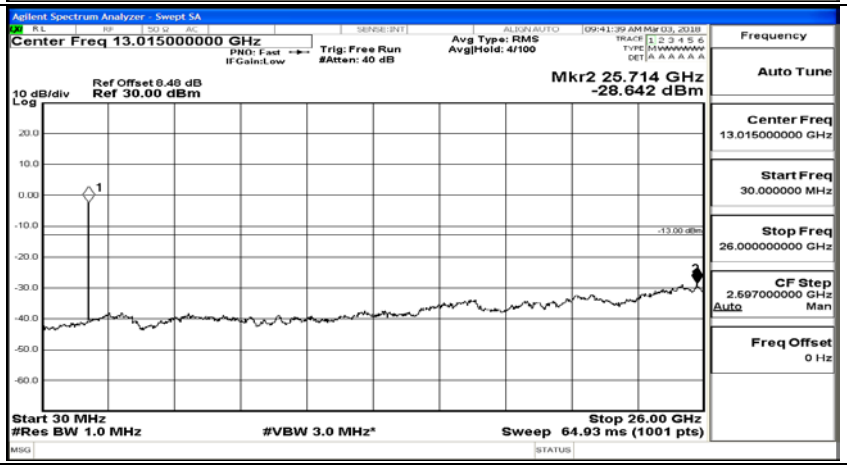

(Channel Bandwidth: 5 MHz)_HCH_QPSK_1RB#0

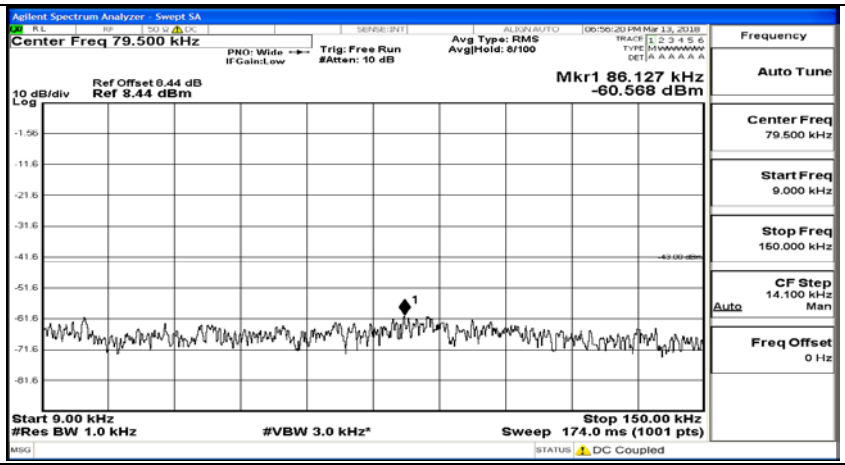

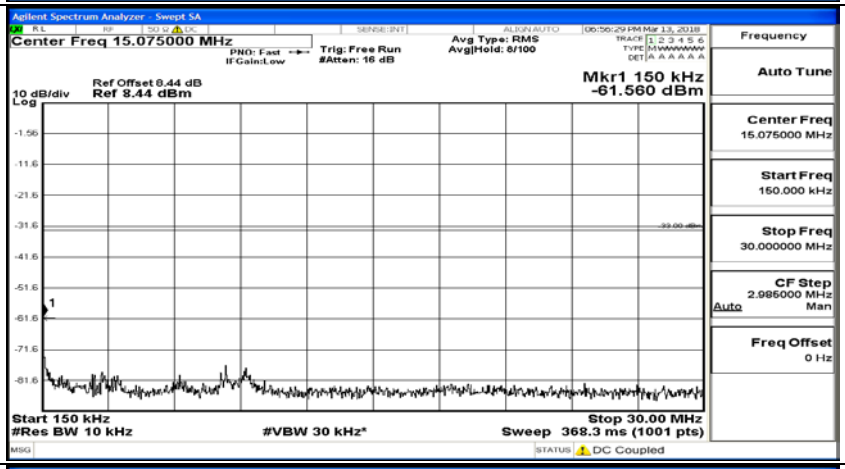

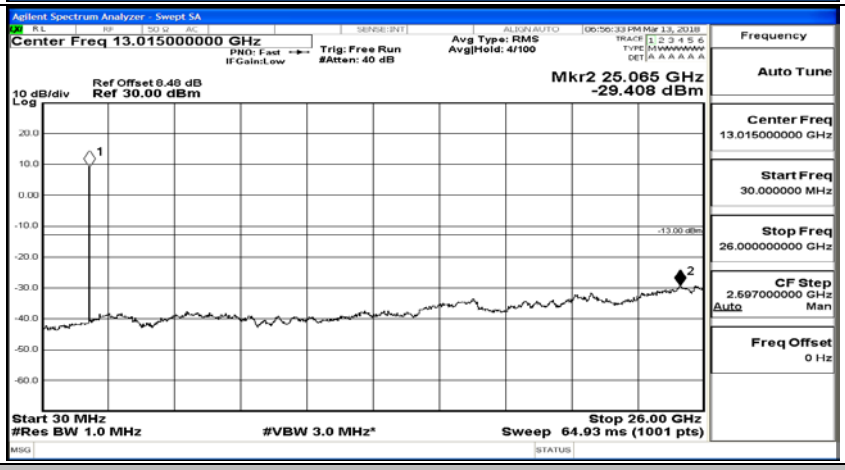

(Channel Bandwidth: 5 MHz)_HCH_QPSK_25RB#0

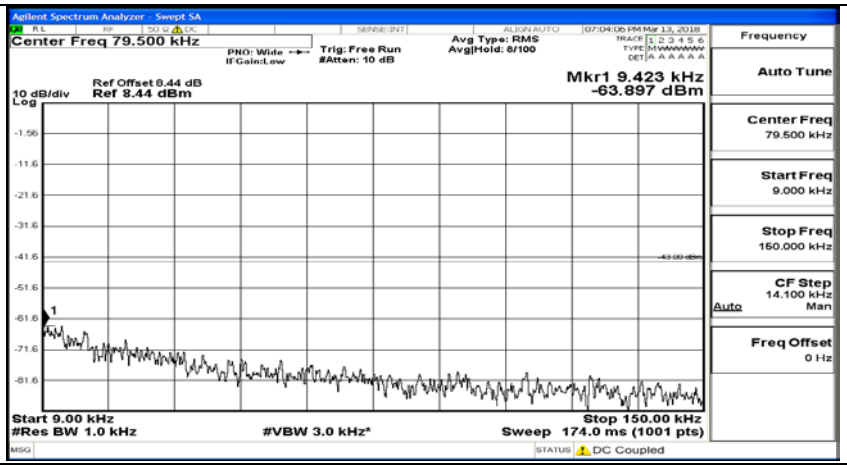
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 8/100
07:04:06 PM Mar 13, 2018
Mkr1 9.423 kHz
-63.897 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.0 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

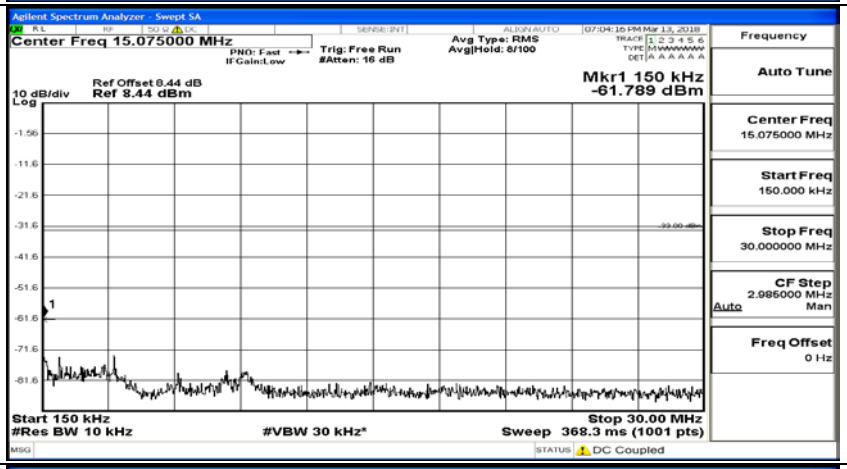
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 8/100
07:04:16 PM Mar 13, 2018
Mkr1 150 kHz
-61.789 dBm
Ref Offset 8.44 dB
10 dB/div
Log
Ref 8.44 dBm
-1.56
-11.6
-21.6
-31.6
-41.6
-51.6
-61.6
-71.6
-81.6
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.3 ms (1001 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

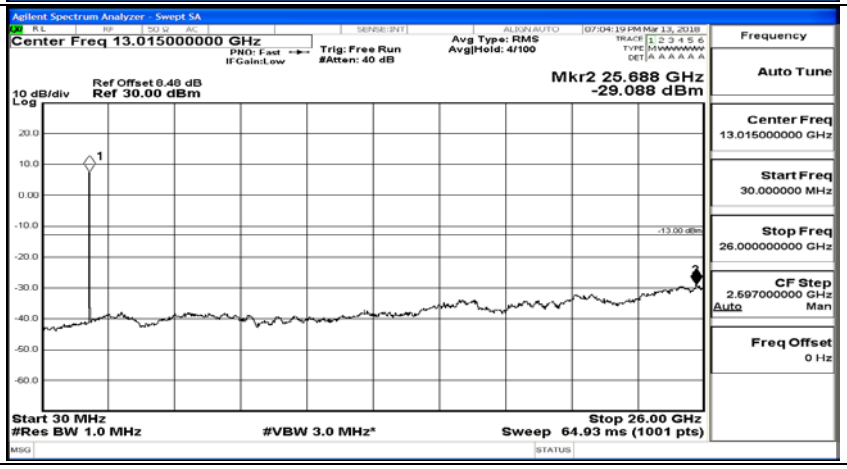
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 4/100
07:04:19 PM Mar 13, 2018
Mkr2 25.688 GHz
-29.088 dBm
Ref Offset 8.48 dB
10 dB/div
Log
Ref 30.00 dBm
20.0
10.0
0.00
-10.0
-20.0
-30.0
-40.0
-50.0
-60.0
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.93 ms (1001 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.697000000 GHz
Auto
Man
Freq Offset
0 Hz