



Appendix D

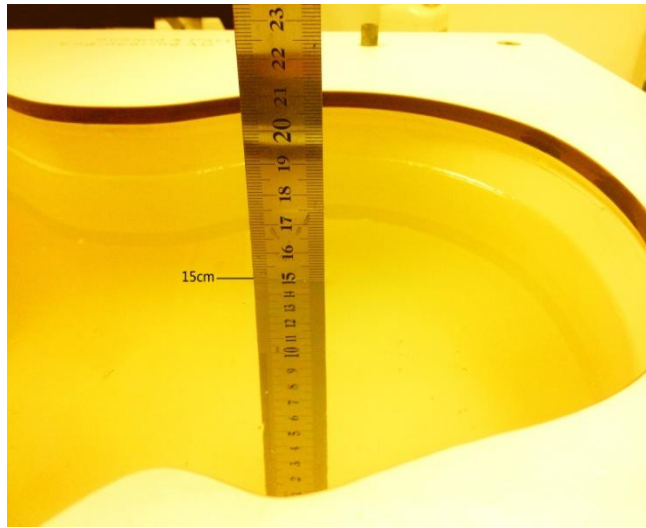
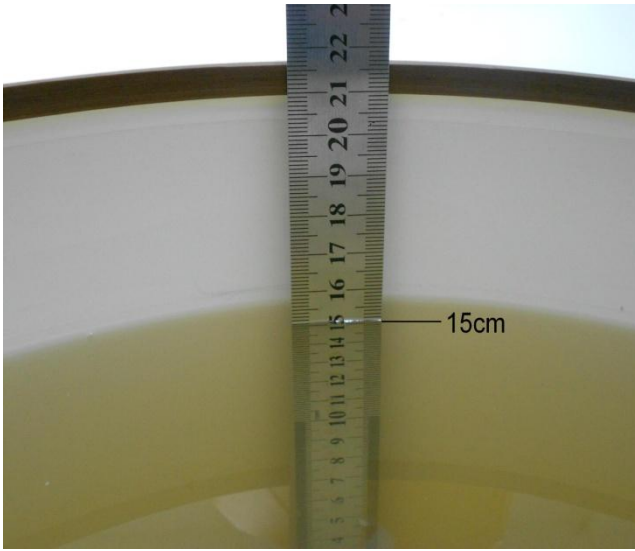
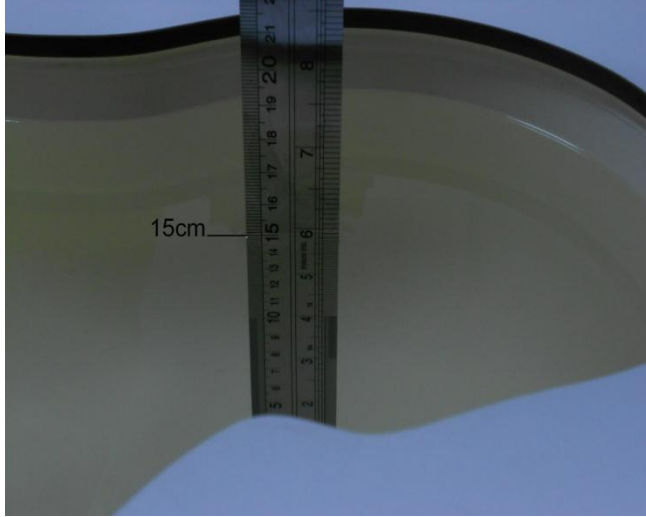
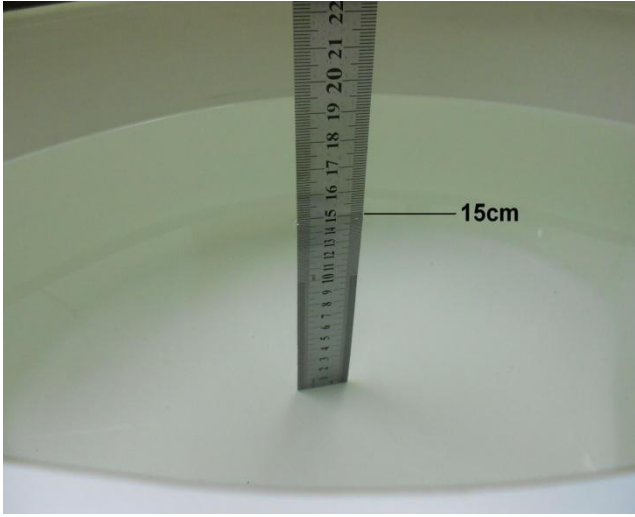
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Body 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Body 1900</p>
	

3. Photographs of EUT test position

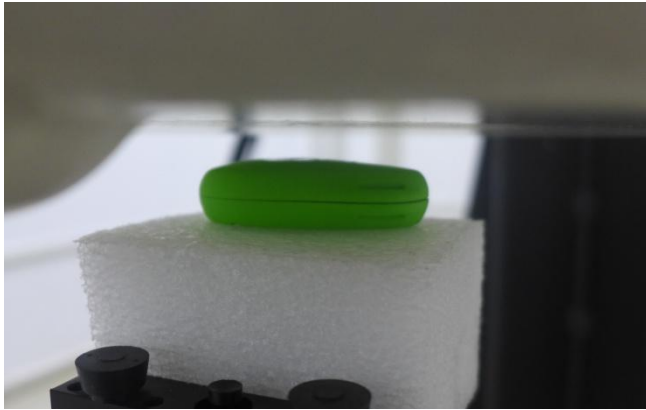
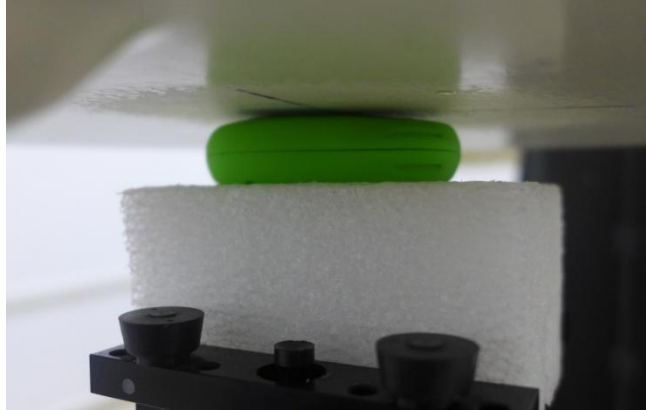
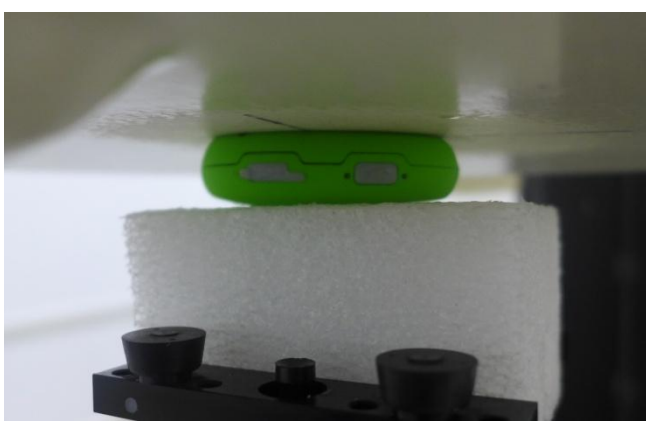

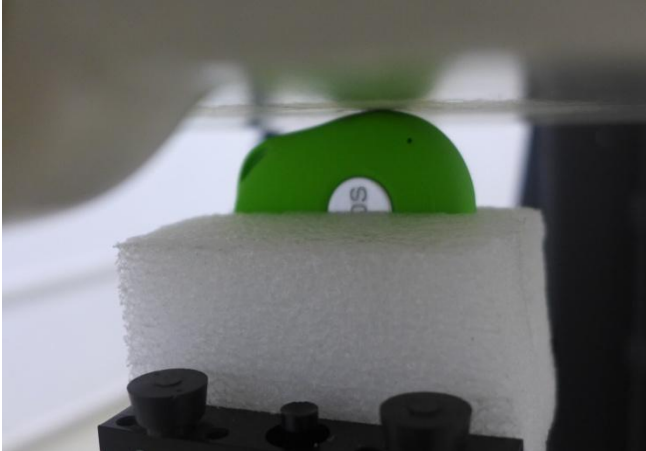
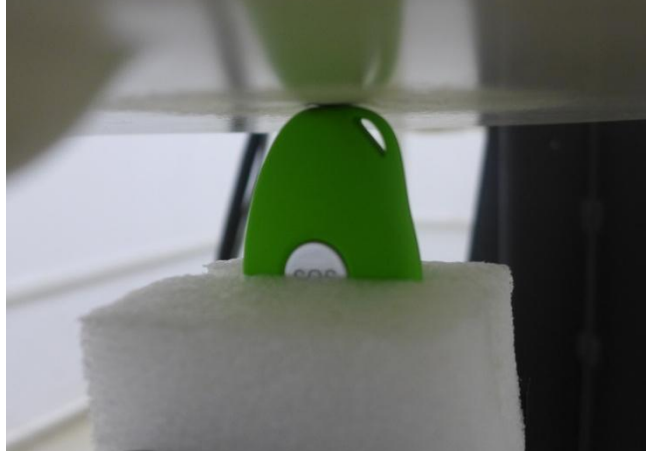

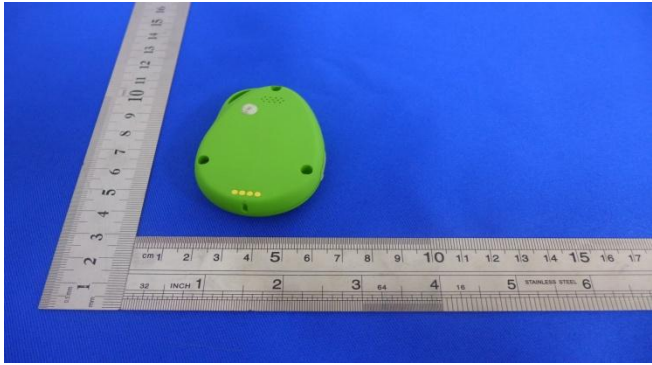

<p>Photo 5: Front to face 10mm</p>	<p>Photo 6: Front side 0mm</p>
	
<p>Photo 7: Back side 0mm</p>	<p>Photo 8: Left side 0mm</p>
	
<p>Photo 9: Right side 0mm</p>	<p>Photo 10: Top side 0mm</p>
	



Photo 11: Bottom side 0mm	NA
	NA

4. EUT Constructional Details

Photo 12: Front View	Photo 13: Back View
	
Photo 14: Accessory	N/A
	<p>N/A</p>