

GSH R5228 Owner's Manual

Language: English

Unit: mg/dL

Market: US

VERSION	Date	By
M01A1Draft	2016/11/01	Karen Yeh from FDA Single Patient version BMU5228BTB_5228BT-M02A4



IMPORTANT SAFETY INFORMATION

Federal Communication Commission Interference Statement

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC Caution: Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate this equipment.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

IMPORTANT NOTE:

Radiation Exposure Statement:

The product comply with the US portable RF exposure limit set forth for an

uncontrolled environment and are safe for intended operation as described in this manual. The further RF exposure reduction can be achieved if the product can be kept as far as possible from the user body or set the device to lower output power if such function is available.

This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

- Please use this device only for the intended use described in this user guide.
- Before using this system to test your blood glucose, please read instructions thoroughly and practice the test when you first use this system. Do a quality check on the system by following the instructions and consult with healthcare professionals for questions or problems.
- Be aware of the safety of young children or handicapped persons near you when you conduct a glucose test using this system.
- Please keep the test strip vial away from children. The test strips and vial cap can present a choking hazard.
- GSH test strips can only be used with the *GSH* glucose meter.

Precaution

The meter and lancing device are for single patient use. Do not share them with anyone including other family members!

Do not use on multiple patients!

All parts of the kit are considered biohazardous and can potentially transmit infectious diseases, even after all cleaning and disinfection procedures have been performed.

For further information, please refer to below:

FDA Public Health Notification: Use of Fingerstick Devices on More than One Person Poses Risk for Transmitting Bloodborne Pathogens: Initial Communication” (2010)

<http://www.fda.gov/MedicalDevices/Safety/AlertsandNotices/ucm224025.htm>

CDC Clinical Reminder: Use of Fingerstick Devices on More than One Person Poses Risk for Transmitting Bloodborne Pathogens” (2010)

<http://www.cdc.gov/injectionsafety/Fingerstick-DevicesBGM.html>

- **Lancet**
Never share a lancet with anyone. Always use a new, sterile lancet; lancets are

for single use only.

- **Lancing Devices**

Lancing devices should never be used for more than one person. Lancing devices are re-useable, and the lifetime cleaning does not affect its performance.

- **Test Strips**

GSH Glucose test strips are intended for single use only. They should be disposed of in an appropriate container according to your healthcare provider's instructions.

- **Meter**

GSH Blood Glucose Monitoring System Model R5228 should only be used for testing single patient.

- Please test your blood glucose using the meter and the test strips with the same reference number as labeled on the outer box of meter and the test strips.

Limitations

1. Do not use for neonatal blood glucose testing or use the system for the diagnosis or screening of diabetes.
2. Alternate site testing should not be used for CGM calibration or for insulin dose calculations.
3. Hematocrit in the range of 20~60% does not affect the glucose results.
4. Cholesterol level up to 500 mg/dL(12.9 mmol/L) and Triglycerides up to 3,000 mg/dL(99.3mmol/L) have been shown not to affect glucose results.
5. Interference was observed for therapeutic levels of Glutathione.
6. Certain substances occurring in the blood naturally, such as uric acid, or from normal therapeutic treatments (Ascorbic acid, L-Dopa, Tolazamide and Gentisic acid) will not significantly affect results. However, higher concentrations in blood may cause incorrect results.
7. There is no significant interference in the presence of galactose, maltose, or fructose observed in blood glucose test.
8. Do not test blood glucose during or soon after xylose absorption test. Xylose in the blood can give falsely elevated results.
9. The test strips may be used at altitudes up to 10,744 feet (3,275 m) without an effect on test results.
10. Persons suffering from severe dehydration should not be tested using a capillary whole blood sample.
11. Test results below 70 mg/dL(3.9 mmol/L) indicate low blood glucose (hypoglycemia). Test results greater than 240 mg/dL (13.3 mmol/L) indicate high blood glucose (hyperglycemia). If you get results below 70 mg/dL(3.9 mmol/L)or above 240 mg/dL(13.3 mmol/L), repeat the test, and if the results are still below 70 mg/dL(3.9 mmol/L)or above 240 mg/dL(13.3 mmol/L), please consult your healthcare professional immediately².
12. Not for use on critically ill patients, patients in shock, dehydrated patients or hyper-osmolar patients.

TABLE OF CONTENTS

Understanding Your New System

Introduction	2-3
Test Principle	3
Appearance and Key Functions of the Meter	4
LCD Screen Overview	5
Installing/Replacing the Batteries	6
Settings (Date/Time/Alarm/Measuring Unit/Memory Deletion)	7-9

Performing a Control Test

About Control Solution Tests	10
Running a Control Solution Test	11-12

Testing Your Blood Sugar

Alternate Site Testing	13
How to Obtain a Blood Sample	14-15
Running a Blood Glucose Test	16-17
Recalling the Memory and Viewing the Average	18-19
Expected Values	20
Transmitting Results	20

Maintenance and Troubleshooting

Maintenance of Your System	21-24
Troubleshooting	25-26
Customer Service	27

Important Additional Information

Specifications	28
Ordering Supplies	28
Warranty Information	29

NOTE: For information about the name of the manufacturer of the lancing device and the lancets, please refer to the package inserts that came with your starter kits.

Understanding Your New System

Introduction

Intended Use / Indications for Use

The *GSH* Blood Glucose Monitoring System (Model R5228) is intended to be used for the quantitative measurement of glucose in fresh capillary whole blood drawn from the fingertips or forearm. The *GSH* Blood Glucose Monitoring System (Model R5228) is intended to be used by a single person and should not be shared.

The *GSH* Blood Glucose Monitoring System (Model R5228) is intended for self-testing outside the body (in vitro diagnostic use) by people with diabetes at home as an aid in monitoring the effectiveness of a diabetes control program.

The *GSH* Blood Glucose Monitoring System (Model R5228) should not be used for the diagnosis of or screening of diabetes or for neonatal use. Alternative site testing should be done only during steady state times (when glucose is not changing rapidly). The *GSH* Test Strips are for use with the *GSH* Blood Glucose Meter to quantitatively measure glucose in fresh capillary whole blood drawn from the fingertips or forearm.

The *GSH* Control Solutions are for use with the *GSH* Blood Glucose Monitoring System (Model R5228) as a quality control check to verify that the meter and test strips are working together properly.

Contents of the System

This User Guide has been prepared to describe the proper use of the *GSH* Blood Glucose Monitoring System Model R5228. Please read this User Guide and the package insert that comes with the *GSH* Glucose Test Strips before testing. The system is available either as a meter alone or as a kit. If you have a meter only, you can purchase the system supplies from your system provider. Please provide to your system provider with the 4 digit system reference number marked on the packaging box when you purchase supplies.

The starter kit of *GSH* Blood Glucose Monitoring System Model R5228 includes the following items:

1. *GSH* Glucose Meter with 2 AAA batteries
2. User Guide
3. Log Book
4. Carrying Case
5. *GSH* Glucose Test Strips
6. *GSH* Control Solution (Level II)
7. Sterile Lancets
8. Lancing Device
9. Package Inserts for Test Strips, Control Solution, and Lancets/Lancing Device


A single level control solution (Level II) is provided in the "Starter Kit," and no control solution is included in the "Meter Only" kit. You may purchase *GSH* Control Solution Level I, Level II or III from your system provider if needed.

The *GSH* Glucose Meter uses *GSH* Glucose Test Strips. Neither the meter nor the test strips will work when used with any other brand of glucose products.

Test Principle


When glucose reacts with the reagents on the test strips, an electrical current is produced, which is proportional to the glucose concentration in the blood sample. The glucose concentration is calculated by the meter and based on the current measured.

Appearance and Key functions of the meter

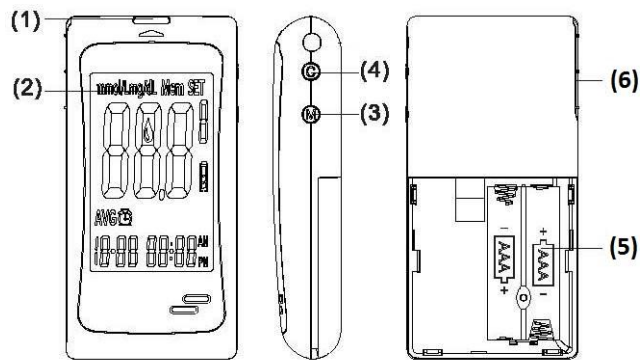

1. Test strip slot - When the strip is inserted into the slot, the meter will automatically turn on.
2. LCD Display - Guide you through the test using symbols and simple messages.
3. M Key - Power ON/OFF, also for memory recalling mode, please refer to manual for detailed function description.
4. C Key - Setting mode, please refer to manual for detailed function description.
5. Battery Compartment - Where batteries are located.
6. Ejector - Remove used strip.


LCD Screen Overview

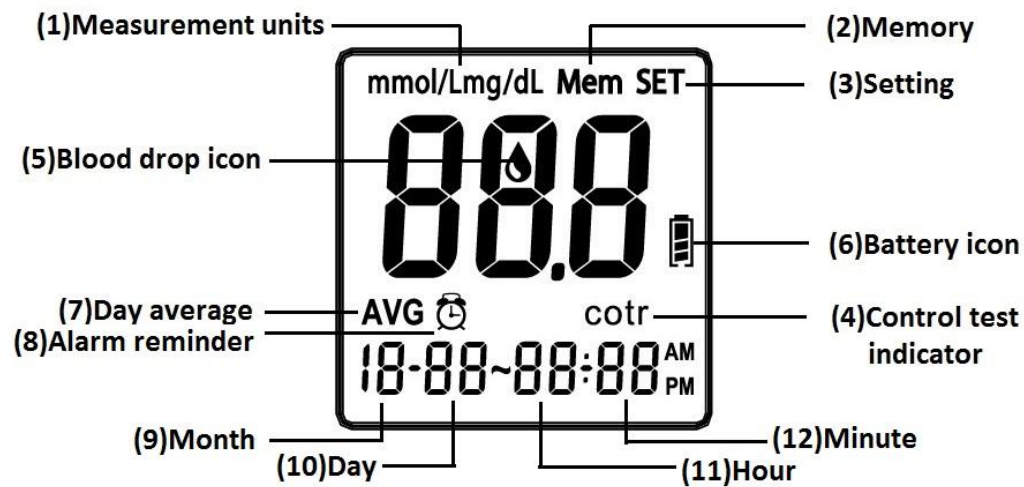

1. Appears with the test result either in mg/dL or in mmol/L.
2. Appears when you recall the memory.
3. Appears when you are in setting mode.
4. Appears for control solution test flag.
5. Indicates the meter is ready to take the blood sample when it flashes.
6. Indicates the battery status.
7. Indicates current displayed result is an average.
8. Appears when alarm is on.
9. Month
10. Day
11. Hour
12. Minute

Installing/Replacing the Batteries

1. Turn off the meter by pressing "M" button and hold for 2 seconds before replacing the batteries. Slide down the battery cover on the back of the meter by pushing the cover in the direction of the arrow and put the cover aside.
2. Remove the two used batteries.
3. Insert 2 new batteries with correct +/- direction.
(Battery: AAA 1.5V 2 Alkaline 24A LR03)
4. Put the battery cover back in place by pushing the cover in the opposite direction of the arrow to close the cover into position.

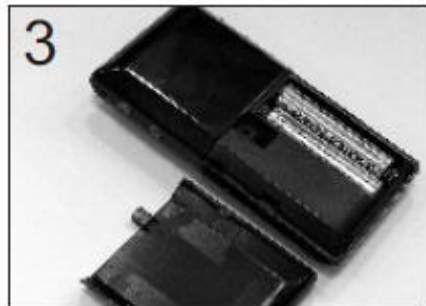

NOTE:

1. It is suggested that batteries need to be replaced when the battery icon appears empty. If you keep using the meter, the battery icon will start flashing and an error message E_3 will appear on the screen.
2. Note that replacing the battery will not reset the stored testing results.
3. You need to reset the time and date after the batteries are replaced.
4. If there is any unexpected symbol on the display, please follow the above procedure to replace the batteries again.
5. Please dispose of batteries according to your local ordinances.

Settings (Date/Time/Alarm/Measuring Unit/ Memory

Deletion)

With the meter in off position, please press M key and hold until the LCD screen displays a flashing “16” digits which represent the last two digits of the Year. The meter is now in the setting mode.

1. **Set the Year** - Press **C** key to adjust the year until the desired year is displayed and then press the **M** key to confirm the year setting. When pressing the **C** key, the year will be adjusted in the range of 2016 to 2030. After the year setting is confirmed, you will see the month segment flashing on the screen. (Please see Figure 1.)
2. **Set the Month** - Press **C** key to adjust the month until the desired month is displayed and then press the **M** key to confirm the month setting. You will then see the day segment is flashing on the screen. (Please see Figure 2.)
3. **Set the Day** - Press **C** key to adjust the day until the desired day appears and then press the **M** key to confirm the day setting. You will then see the hour segment is flashing on the LCD screen. (Please see Figure 3.)
4. **Set the Hour** - Press **C** key to adjust the hour until the desired hour appears on the screen and then press the **M** key to confirm the setting. You will then see the minute segment is flashing on the screen. (Please see Figure 4.)
5. **Set the Minute** - Press **C** key to adjust the minute until the desired minute appears on the screen and then press the **M** key to confirm the setting. You will then see an “AL” displayed on the screen center. (Please see Figure 5.)
6. **Set the Alarm Reminder** – Press **C** key to toggle between the alarm reminder setting and no-setting mode. If you see the LCD display a small flashing icon of alarm clock in the lower left corner with a time segment display, it means that you are in the alarm setting mode. (Please see Figure 6.)

If you see only AL without the icon of the small alarm clock, it means that you are not in the alarm setting mode. Press **M** key to confirm the alarm setting mode. If you select the alarm setting mode, alarm clock icon will stop flashing and the hour of the time segment will start flashing. Press **C** key until the desired alarm hour appears and then press **M** key to confirm the hour setting. Then the minute segment will start flashing. Press **C** key until the desired minute appears on the screen and then press **M** key to confirm the minute

setting. You will see the measuring unit flashing on the upper left corner of the LCD display. (Please see Figure 7.).

7. **Set the measurement unit** – Press **C** key to toggle between mg/dL and mmol/L measurement units. Press **M** key to confirm the setting. You will see a “dEL” displayed in the center of the screen. (Please see Figure 8.)

The unit of measurement-mg/dL-is the standard unit of measurement in the U.S.

8. **Delete Memory** – Press **C** key to toggle between a flashing “dEL” for memory deletion and a non-flashing “dEL”. If you want to delete all memory, press **M** key while the “dEL” is flashing. If you do not want to delete all memory, press **M** key when the “dEL” is not flashing. Once the M key is pressed, the LCD display will turn off automatically after 2 seconds.



NOTE: Your meter can show results either in “mg/dL” or “mmol/L” units. Mg/dL is the correct unit used in the United States, please contact the manufacturer if your meter does not display mg/dL when you turn it on. The factory set default for the meter is mg/dL.

In the event that the meter loses power or the batteries are changed, the factory set default is mg/dL. It is very important to use the correct unit of measurement to properly manage your diabetes. If you live in the United States, you should use mg/dL. If you are testing in mg/dL, your results will never have a decimal point. If you live outside the United States and use the metric system, you should use mmol/L.

Your result will ALWAYS have a decimal point.

NOTE:

1. When you change the date and time backward, you will not change the test results in the meter memory.
2. You need to move through the year, month, day, hour, minutes, alarm, unit, and dEL to save the meter settings and turn off the meter.
3. The average readings in the meter memory are calculated from the results obtained during the 7, 14, 28, 60, and 90 calendar days preceding the current date and time settings.

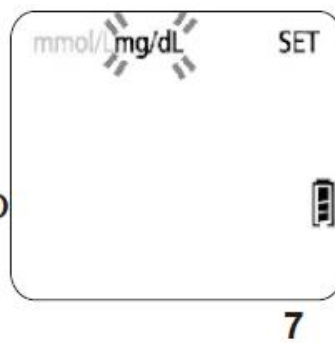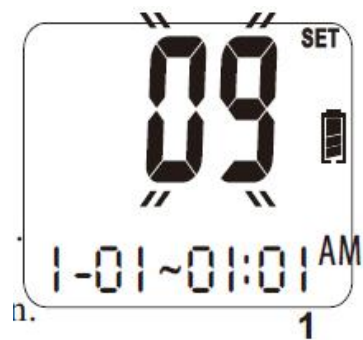

Performing a Control Test


About Control Solution Tests

GSH Control Solution contains a known amount of glucose and is used to confirm that the meter and test strips are working properly. A control solution test should be performed every time a new vial of test strips are opened, or whenever you suspect that the meter or test strips may not be functioning properly.

1. The Control Solution range is found on the bottle of the *GSH* test strips and NOT the control solution itself (see Figure 1).
Note: The ranges in Figure 1 are examples only and not the ranges that you should refer to.
2. Gently roll the control bottle in the palm of your hands to thoroughly mix the control solution content (see Figure. 2).
3. Discard the first drop as crystallization may occur.
4. Place a drop of the control solution either on a hard surface or the “dimple” of the control solution cap (see Figure 3).
5. Place the meter into “**Control**” mode when performing a control test so the readings do NOT get averaged with your other readings.



1 m

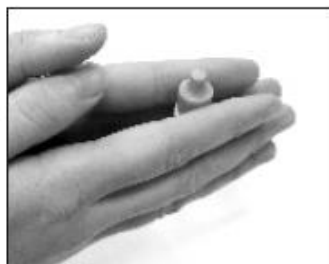

2




3

Running a Control Solution Test

IMPORTANT:

Always make sure you press C key for Control Solution test, otherwise the control solution test result will be stored in the memory, and affect your "AVG" results.

1. Insert a strip into the meter. A full LCD screen will be displayed briefly and then a blood drop icon appears.
2. Press the **C** key, and the meter will display a letter "cotr" on the screen, indicating the control test mode. The test result will not be stored in the memory.
3. Squeeze a small amount of Control Solution on a flat surface and apply to the front edge of the test strip.
4. Wait for 5 seconds, and the meter will display the result.
5. Remove the used strip by hand or by pushing the ejector and the meter will power off.

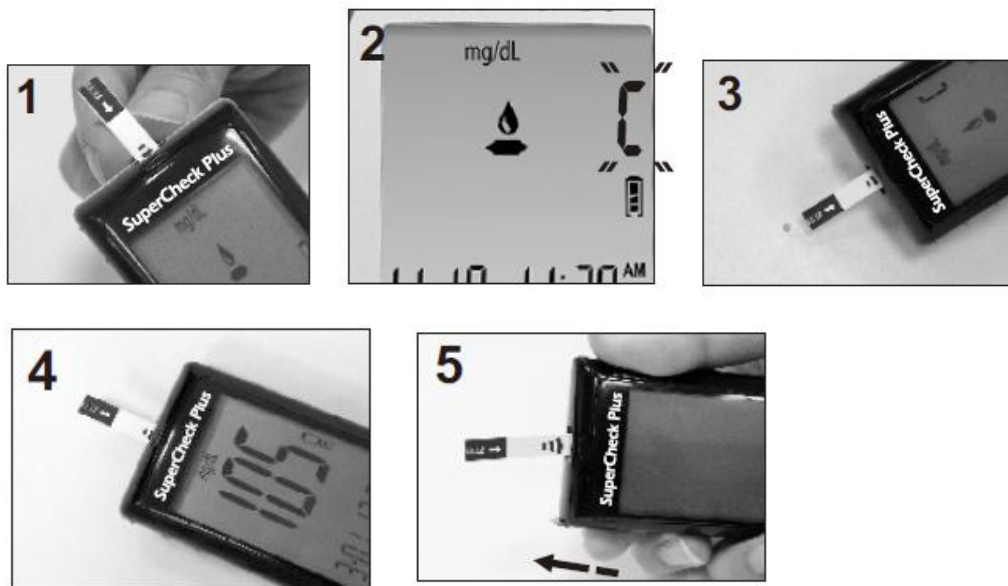

IMPORTANT!!!

1. If the meter, test strips and control solutions are moved from one temperature to another, allow thirty (30) minutes for them to adjust to the new temperature before performing a control test.
2. You must push the C key to distinguish the control solution test from the blood glucose test. Do not perform the blood test in Control Solution mode. (If you perform the blood test in Control Solution mode, the test result will not be stored.)
3. Use only *GSH* Control Solution with the *GSH* Glucose Meter.

4. *GSH* Control Solution is used to check that the meter and the test strips are working together as a system and that you are performing the test correctly.
5. *GSH* Control Solution contains a known amount of glucose that reacts with test strips. The Level I, Level II and III Control Solutions are intended to check the monitoring system in different measurement ranges.
6. Shake the vial, discard the first drop of control solution, and wipe off the dispenser tip to ensure a good sample and an accurate result.
7. Use only for 3 months after first opening. Record the open date on the Control Solution vial. Discard after 3 months.
8. Compare your Control Solution test results with the expected range printed on the test strip vial label. If your glucose control results fall outside the expected range; repeat the test. Results that repeatedly fall outside the expected range may indicate:
 - (1) You may not be doing the test correctly; repeat the test, by shaking the control solution vial well and carefully following instructions. Please make sure the test is done within the temperature range.
 - (2) The Control Solution is expired or contaminated.
 - (3) The test strips are damaged or outdated.
 - (4) You may have applied the Control Solution before the blood drop appears on the screen. This will cause incorrect glucose measurement.
 - (5) Meter malfunction

Testing Your Blood Sugar

Alternate Site Testing (AST)

What is AST?

Sampling from anatomical sites (parts of the body) other than the fingertip to check the blood glucose levels. This system allows you to test on the forearm when glucose is not changing rapidly.

There are important limitations to AST. Please consult your healthcare professional before you use AST.

What is the advantage?

It is more painful feeling when taking blood sample from fingertips because fingertips have many nerve endings. Other body sites do not have as many nerve endings, so you will not feel as much pain as at the fingertip.

When to use AST ?

Medication, stress, illness, food and exercise can affect blood glucose levels. Capillary whole blood at the fingertip can reflect test changes faster than capillary blood at other sites of body. If you test your blood glucose level during or immediately after a meal, physical exercise or stressful events, take the blood sample from your fingertip instead of from other sites.

Use AST only:

1. 2 hours or more after taking insulin;
2. 2 hours or more after a meal;
3. 2 hours or more after exercise.

Do not use AST if you are aware that your glucose level is not as stable as usual, or if you think you have hypoglycemia (low blood sugar) or hyperglycemia (high blood sugar).

Do not use AST if you think your blood glucose is low and if your AST results do not match the way you feel.

AST should not be used to calibrate CGMs or in insulin dose calculation.

How to Obtain a Blood Sample




IMPORTANT:

1. The meter and lancing device are for single patient use. Do not share them with anyone including other family members! Do not use on multiple patients!
2. All parts of the kit are considered biohazardous and can potentially transmit infectious diseases, even after all cleaning and disinfection procedures have been performed.
3. Only the single-use lancing device and lancet should be used with *GSH* meter.
4. Users should wash hands thoroughly with soap and water after handling the meter, lancing device, or test strips. Please follow the cleaning and disinfection procedure on page 21 of this user guide.

GSH Meter requires a small blood drop to perform a test. You may obtain your blood sample from a fingertip or forearm. Be sure to wear a new pair of gloves before obtaining blood sample from each patient. Read the instructions of lancing device carefully before obtaining blood sample.

From Fingertip



1. Wash hands in warm, soapy water. Be sure to rinse and dry well.
2. Hold the lancing device firmly against the side of a finger and retrieve the loaded single use lancing device.
3. Gently massage the finger, if needed, to help obtain a round drop of blood.
4. Do not smear the blood sample. Proceed with blood test.

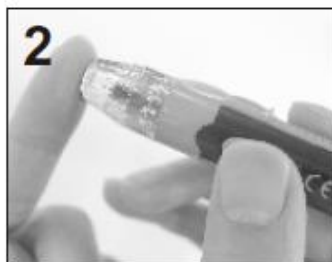

From Forearm

1. Select a soft, fleshy area on forearm that is clean and dry. Make sure it is away from bone and free of visible veins and hair.
2. Massage the selected area gently to increase blood flow to the puncture site. Clean the test location with soap and water. Be sure to rinse and dry well.

3. Press and hold the loaded single use lancing device against the forearm firmly and press the release button.
4. Wait a few seconds until a blood drop forms. Make sure you have sufficient blood to fill the test strip. Be careful not to smear the blood sample and proceed with blood test.

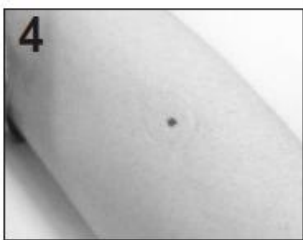


Running a Blood Glucose Test

1. Open the app on your cell phone and turn the Bluetooth function on.
2. Open the test strip vial. Take one new test strip out of the vial and recap the vial quickly and firmly (see Figure 1).
3. While the meter is off, insert a test strip into the meter's strip slot in the right direction. The meter will turn on with a full screen display, and a blood drop icon will be blinking on the screen. If no action is taken in 2 minutes, the meter will turn off automatically (see Figure 2).
4. Use a single lancing device to take a blood sample from the fingertip or forearm (see Figure 3).
5. Apply a small blood drop (● actual size) to the front edge of the test strip, and the blood should be pulled into the test strip before the meter begins to count down. Do not push your finger against the test strip or try to apply a smeared blood sample (see Figure 4).
6. The meter will count down from 5 to 1 and test result will be displayed on the screen.
7. Right after test result is displayed the meter's Bluetooth function will be turned on and you will see "bLE" and test time flashing alternately (see Figure 5). Once the meter is connected to the app, test result will be transferred to the app

automatically. Check the app to make sure the test result has been received. If the transfer failed, the test result will be transferred next time when you perform a test successfully.

8. Remove the used test strip by hand or by pushing the ejector button. The meter will turn off and the test result is stored automatically (see Figure 6).
9. Wash your hands thoroughly with soap and water after handling the meter, lancing device, or test strips.

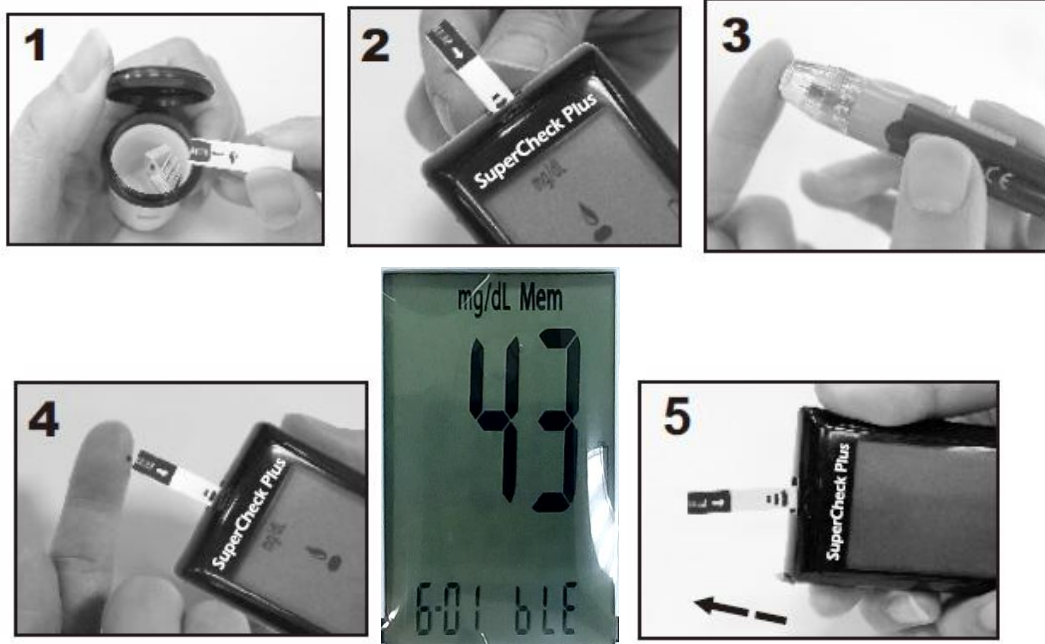

Important:

1. Never reuse a test strip or a lancet. An "E_5" error message will be displayed in the center of screen if a used strip is inserted into the meter.
2. Discard the test strip and lancet immediately in a puncture-proof container with a lid after use.
3. If the meter and test strips are moved from one temperature to another, allow thirty (30) minutes for them to adjust to the new temperature before performing a blood test.

Recalling the Memory and Viewing the Average

A. Using the Meter Memory

The test results for blood sample will be stored in the memory automatically. The meter can store up to 500 of the most recent test results. You can also view the average of test results for various periods of 7, 14, 28, 60 and 90 days. The control solution test results will not be stored in memory.

(Note: Please make sure that you press C key when you run a Control Solution test, so that the control test result will not be added to memory.)

B. Recalling the Test Results from the Meter Memory

1. With meter off, press M key to turn on the meter, the meter will display the total number of test data stored in memory. Then the screen will display "001" as the sequential number of the most recent test result in memory. The memorized test data will be displayed next. If there is no memorized result in the meter, "---" is displayed and the meter will turn off after 60 seconds if no action is taken. (The meter will display "---" if no previous results were memorized.)
2. The screen will display each of the memorized test data in sequence. Press M and C key to review your test results in memory forwards and backwards.
3. To turn off the meter, press M key for 2 seconds, or the meter will turn off automatically after 60 seconds of no activity.

C. Viewing the Average (AVG) of Test Data in Memory

1. To display the average (AVG) test result, please turn meter off. Press C and M keys at the same time and hold for about 2 seconds, wait for AVG displayed on screen, then release the two buttons. The meter will be in the average mode with "AVG" font displayed.
2. When the "AVG" is flashing at the lower left corner of screen, the number 7 will be displayed under AVG and the average of the last 7 days test results will be displayed in the center of the screen. The number of tests done in the last 7 days will be also displayed at the lower right corner of screen. If you want to see the average of 14, 28, 60 and 90 days, keep pressing the M key to move the LCD display forward from 7 day average to 90 day average. The average display will move from 90 days backward to 7 days if you continue to press C key.
3. Press the M key and hold for 2 seconds to exit the recall mode and turn off

the meter, or the meter will automatically power off after 60 seconds.

4. When “---” is displayed, showing that there are no test results in memory.

Calculations:

The 7 days average is the average of the last 7 day test results. The 14 days average is the average of last 14 day test results. The 28 days average is the average of last 28 day test results. The 60 days average is the average of last 60 day test results. The 90 days average is the average of last 90 day test results.

NOTE:

1. HI/LO results are not stored in the memory.
2. Do not insert the strip into the meter when you want to recall the test result

Expected Values Reference¹

Blood glucose levels normally will vary from time to time depending on food intake, medication dosages, health, stress or exercise. Consult your physician or healthcare professional for the target glucose value appropriate for you.

Expected plasma blood glucose values for normal, nondiabetic adults are as follows.

Before eating	<100mg/dL
---------------	-----------

Two hours after meals	<140mg/dL
-----------------------	-----------

GSH meter gives plasma equivalent results.

Transmitting Results

Your *GSH* Blood Glucose Meter transfers test result every time when a test is performed successfully. You will need to install an app to your device to receive the test result. Please read the app manual that comes with this meter for instructions. You can also check with your distributor for the app download and install option.

The meter does not play any message during the data transmission, but you can check the app on your device to confirm if the test result is received. The meter still keeps the results in the memory after transmitting.

Maintenance and Troubleshooting

Maintenance of your system

Please, treat this meter with proper care, and keep it in good condition. Store your meter in its case, in a clean dry place at 35.6~86°F (2~30°C).

Cleaning and Disinfecting Your Meter and Lancing Device

Cleaning and disinfecting your meter and lancing device is important to prevent the spread of infectious diseases.

Cleaning is the physical removal of dirt (e.g. dust, grease, and touch contaminants) from the external surfaces of meter and lancing device. By keeping your meter and lancing device clean, you help ensure that it is working properly and that no dirt gets in the device. Cleaning allows for successful, subsequent disinfection.

Disinfection is a process that destroys pathogens, such as viruses and other microorganisms on the external surfaces of meter and lancing device. By disinfecting your meter and lancing device, you help ensure that no infection is passed when you or others come in contact with your meter and lancing device.

Clorox® Bleach Germicidal Wipes (EPA Reg. No. 67619-12) have been shown to be safe for use with the meter and lancing device and that these wipe should be used for both cleaning and disinfection.

Cleaning and Disinfection Instructions

We recommend users to clean and disinfect the meter and lancing device at least once per week. Please keep the meter free of dirt, dust, bloodstain, and water stains. Using two wipes, follow the cleaning instruction first and the disinfection instruction second to clean and disinfect your meter.

Cleaning: Do the cleaning step first to remove heavy soil and touch contaminants left on the surface of your meter. Use a germicidal wipe to clean your meter. All blood and other body fluids must be thoroughly cleaned before disinfection by the germicidal wipe.

Disinfection: After cleaning, use a germicidal wipe and thoroughly wet all the surface

of your meter, including the strip lot and other connection ports. Treated area must remain visibly wet for a full 1 minute. Let the devices air dry completely before turning it on (30 seconds or so).



Do:

- Make sure the meter is in OFF mode during cleaning and disinfection.
- Keep the test strip vial tightly closed when performing the cleaning and disinfection procedures because the fumes from the disinfectant may affect the performance of the strip.
- Stop using the devices and contact your customer service if any of the following signs of deterioration are noted after each cleaning and disinfection cycle:

For meter:

- The meter does not turn on.
- The meter's screen has been cracked or clouded.
- Any meter's functions are abnormal.
- Any buttons have stopped working.

For lancing device:

- Any button or moving part has stopped working.
- The device is cracked.
- The device does not yield an adequate blood drop.

Please call the Customer Service at Toll Free 1-888-887-4772 (EST 9:00AM~5:00PM /Mon. to Fri.) for support.

Do Not:

- Get any liquid in the test strip slot and other connection ports.
- Spray any cleaning solution directly on to the meter.
- Put the meter under water or liquid.
- Pour liquid into the meter.

NOTE:

1. If the meter is being operated by a second person who is providing testing

assistance to the user, the meter and lancing device should be cleaned and disinfected prior to use by the second person.

2. Be sure to wash your hands with soap and warm water, rinse and dry thoroughly after handling the meter, lancing device or test strips.

Cleaning and Disinfection Frequency

11,000 validated cycles for the meter and lancing device were done; 11,000 cycles of cleaning and 11,000 cycles of disinfection were included. 5 cycles of cleaning per day and 1 cycle of disinfection per week allow the user to use the device for 3 year use life.

Cleaning Frequency:

5 cycles/day x 365 days/year x 3 year use life.

=5475 cycles of cleaning < 11,000 validated cycles of cleaning.

Disinfection Frequency:

1 cycle/week x 52 weeks/year x 3 year use life.

=156 cycles of disinfection < 11,000 validated cycles of disinfection.

3 year use life for properly cleaning and disinfection.

After 3 years, the meter and lancing device must be replaced with a new meter and a new lancing device.

To purchase Clorox® Bleach Germicidal Wipes (EPA Reg. No. 67619-12), you can find the nearest Clorox Sales Representative at Clorox's global website, <http://www.cloroxprofessional.com/products/clorox-germicidal-wipes/at-a-glance/>. In addition, you can purchase them at <http://www.amazon.com>, <http://www.grainger.com/category/cleaning/ecatalog/N-bi4>, or other online retail sites.

NOTE:

Unless you cannot purchase the wipes recommend above, you may consider purchasing the other similar disinfectant products with the EPA registration number of 6719-12.

Troubleshooting:

Following is a summary of all Error Messages. These messages help to identify certain problems, but do not appear in all cases when a problem has occurred. Improper use may cause an inaccurate result without producing an error message or a symbol. In the event of a problem, refer to the information in the table under Solution.

Error messages:

E_1: The temperature is too low.

E_2: The temperature is too high.

E_3: Battery Low.

E_4: Memory damaged.

E_5: The strip is wet or used.

E_6: Error in meter or strip.

E_7: The blood sample is not sufficient.

HI: The glucose level is too high.

LO: The glucose level is too low.

NOTE: Your meter can show results either in “mg/dL” or “mmol/L” units. Mg/dL is the typical unit used in the United States, please contact the manufacturer if your meter does not display mg/dL when you turn it on. The factory set default for the meter is mg/dL.

In the event that the meter loses power or the batteries are changed, the factory set default is mg/dL. It is very important to use the correct unit of measurement to properly manage your diabetes. If you live in the United States, you should use mg/dL. If you are testing in mg/dL, your results will never have a decimal point. If you live outside the United States and use the metric system, you should use mmol/L.

Your result will ALWAYS have a decimal point.

Problem	Possible Cause	Solution
(1) The meter displays an E_1 error message.	The meter is operating in an ambient temperature below 10 °C or 50°F which is the lowest range of operating temperature.	Repeat the test after the meter and strip are placed in a warmer environment and allow the meter to warm up for a while before retesting.
(2) The meter displays an E_2 error message.	The meter is operating in an ambient temperature above 40 °C or 104°F which is the upper limit of operating temperature.	Repeat the test after the meter and strip are placed in a cooler environment and allow the meter to cool down for a period before retesting.
(3) The meter displays an E_3 error message.	The battery is too low to operate the meter.	Please replace the two AAA batteries.
(4) The meter displays an E_4 error message.	The memory chip of the meter could be damaged or malfunctioning.	The meter can perform the glucose measuring without storing the test results into the meter's memory. Please write down the test results into the data logger before you call a customer service representative.
(5) The meter displays an E_5 error message.	1. If you apply the sample before blood drop icon appears on the screen. 2. The inserted test strip has been wet or used.	Please check the test strip to see if it is damaged or used. In either case, please discard the strip and repeat the test using a new strip.
(6) The meter displays an E_6 error message.	The meter is not working properly, either because of a defective meter or a defective strip.	Repeat the test with a new test strip. If E_6 continues to show up on screen, please call a customer service representative.
(7) The meter displays an E_7 error message.	The blood sample is not sufficient.	Please re-test by inserting a new test strip ensuring an adequate amount of blood comes into contact with the test strip.

<p>(8)</p> <p>The meter displays HI on screen.</p>	<p>The test result is higher than the measuring range of 600 mg/dL (33.3 mmol/L).</p>	<p>Test again following the user guide for correct glucose measurement process. If you see HI again, please call your medical doctor for advice immediately.</p>
<p>(9)</p> <p>The meter displays LO on the screen.</p>	<p>The test result is lower than the measuring range of 20 mg/dL (1.1 mmol/L).</p>	<p>Test again following the user guide for correct glucose measurement process. If you see LO again, please call your medical doctor for advice immediately.</p>

Customer Service

If you need assistance with your *GSH* Blood Glucose Monitoring System Model R5228, please contact:

Biotest Medical Corporation

No. 3-2 Chien-kuo Road, TEPZ Tantz, Taichung 427

Taiwan R.O.C.

TEL: 886-4-2532 6668

For U.S.A. 1-888-887-4772

Hours: 9 AM to 5 PM EST/Mon. to Fri.

Outside of these times, contact your healthcare professional for medical issues or advice.

For questions related to your health condition, please call your doctor or healthcare professional.

Important Additional Information

Specifications

Test: Glucose

Sample: Capillary whole blood

Principle of the test method: Amperometric, FAD- glucose dehydrogenase

Test sites: Fingertip, forearm

Measurement time: 5 seconds

Measurement Range: 20 - 600 mg/dL (1.1 - 33.3mmol/L)

Batteries: 2 x AAA 1.5 V Alkaline 24A LR03

Operating Condition:

10 - 40°C (50 - 104°F)

20 - 80% RH (non-condensing)

Storage/Transportation Condition:

2 - 30°C (35.6 - 86°F)

20 - 80% RH (non-condensing)

Width: 50 mm

Length: 100 mm

Thickness: 20 mm

Weight: ~72g

Memory: 500 measurement results with date and time

Auto power off after 2 minutes without action when a strip is inserted, or 60 seconds if there is no strip inserted.

Federal Communication Commission Interference Statement

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

FCC Caution: Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate this equipment.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

IMPORTANT NOTE:

Radiation Exposure Statement:

The product comply with the US portable RF exposure limit set forth for an uncontrolled environment and are safe for intended operation as described in this manual. The further RF exposure reduction can be achieved if the product can be kept as far as possible from the user body or set the device to lower output power if such function is available.

This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

Ordering Supplies

To order supplies, please contact:

Biotest Medical Corporation

No. 3-2 Chien-kuo Road, TEPZ Tantz, Taichung 427

Taiwan R.O.C.

TEL: 886-4-2532 6668

For U.S.A. 1-888-887-4772

Hours: 9 AM to 5 PM EST/Mon. to Fri.

(Outside of these times, contact your healthcare professional for medical issues or advice.)

Warranty Information

Your *GSH* Glucose Meter is warranted to be free of defects in materials and workmanship for one year from the date of the original purchase.

This warranty does not cover device failure due to owner misuse or negligence, or normal wear and tear.

If you have a question about your *GSH* Glucose Meter or this warranty, please contact:

Biotest Medical Corporation

No. 3-2 Chien-kuo Road, TEPZ Tantz, Taichung 427

Taiwan R.O.C.

TEL: 886-4-2532 6668

For U.S.A. 1-888-887-4772

Hours: 9 AM to 5 PM EST/Mon. to Fri.

(Outside of these times, contact your healthcare professional)

Reference:

1. American Diabetes Association: Diabetes Care, January 2016, Volume 39 (Suppl. 1) S13 – S22.

2. American Diabetes Association-Diabetes Forecast website information:

<http://www.forecast.diabetes.org/diabetes-101/hyperglycemia>

<http://www.forecast.diabetes.org/diabetes-101/hypoglycemia>