

---

## APPENDIX B EUT TEST POSITION PHOTOS


---

### Liquid depth $\geq 15\text{cm}$


Phantom: SAM (30deg probe tilt) with CRP v5.0\_20150321; Type: QD000P40CD; Serial: TP:1874




**Vertical-Front Setup Photo (5mm)**

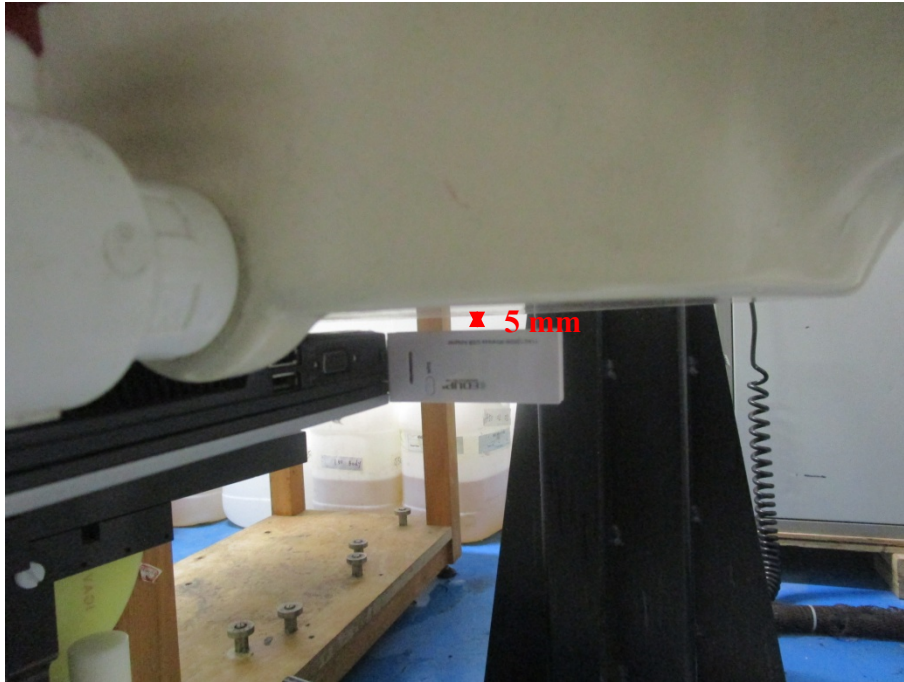

**Horizontal-Down Setup Photo (5mm)**

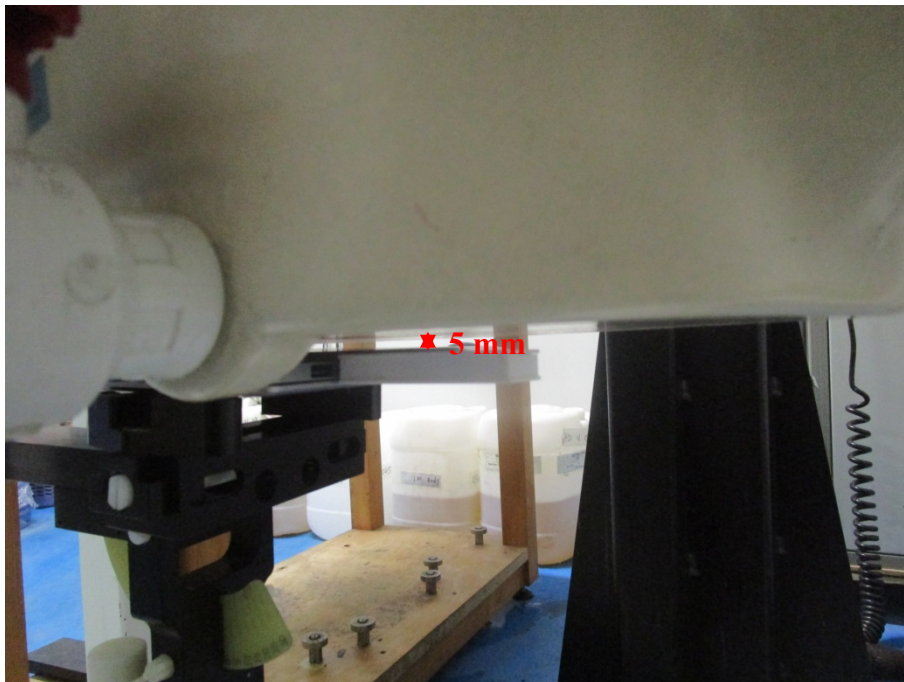

**Body Top Setup Photo (5mm)**

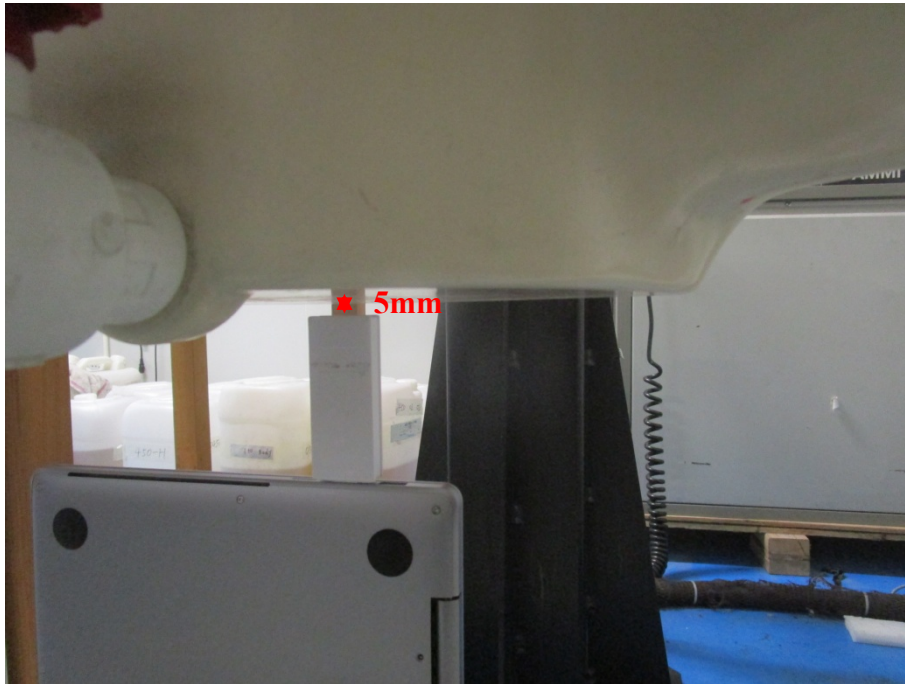

**Horizontal-Up(Adding USB extension cable) Setup Photo (5mm)**



**Vertical-Back (Adding USB extension cable) Setup Photo (5mm)**

