



# CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 F-mail: cttl@chinattl.com



Client

Sporton\_TW

Certificate No:

Z16-97124

# CALIBRATION CERTIFICATE

Object

D835V2 - SN: 4d200

Calibration Procedure(s)

FD-Z11-2-003-01

Calibration Procedures for dipole validation kits

Calibration date:

August 23, 2016

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	27-Jun-16 (CTTL, No.J16X04777)	Jun-17
Power sensor NRP-Z91	101547	27-Jun-16 (CTTL, No.J16X04777)	Jun-17
Reference Probe EX3DV4	SN 3617	26-Aug-15(SPEAG,No.EX3-3617_Aug15)	Aug-16
DAE4	SN 777	26-Aug-15(SPEAG,No.DAE4-777_Aug15)	Aug-16
Secondary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	01-Feb-16 (CTTL, No.J16X00893)	Jan-17
Network Analyzer E5071C	MY46110673	26-Jan-16 (CTTL, No.J16X00894)	Jan-17

Name

Function

Signatura

Calibrated by:

Zhao Jing

SAR Test Engineer

34

Reviewed by:

Qi Dianyuan

SAR Project Leader

2 Mils

Approved by:

Lu Bingsong

Deputy Director of the laboratory

Issued: August 26,12016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured

# Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

### Additional Documentation:

e) DASY4/5 System Handbook

# Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z16-97124 Page 2 of 8



### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1258
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

**Head TSL parameters** 

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.0 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.37 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	9.39 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.56 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	6.19 mW /g ± 20.4 % (k=2)

**Body TSL parameters** 

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.9 ± 6 %	0.98 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.43 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	9.65 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.62 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	6.44 mW /g ± 20.4 % (k=2)

Certificate No: Z16-97124 Page 3 of 8

### **Appendix**

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.0Ω- 3.39jΩ	
Return Loss	- 29.4dB	

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.1Ω- 5.27jΩ	
Return Loss	- 23.3dB	

### General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG

Certificate No: Z16-97124 Page 4 of 8

### DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d200

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: f = 835 MHz;  $\sigma = 0.915$  S/m;  $\varepsilon_r = 41.98$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Center Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(9.56, 9.56, 9.56); Calibrated: 8/26/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2015-08-26
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7372)

Date: 08.23.2016

# Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 58.36V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.53 W/kg

SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.56 W/kg

Maximum value of SAR (measured) = 3.00 W/kg

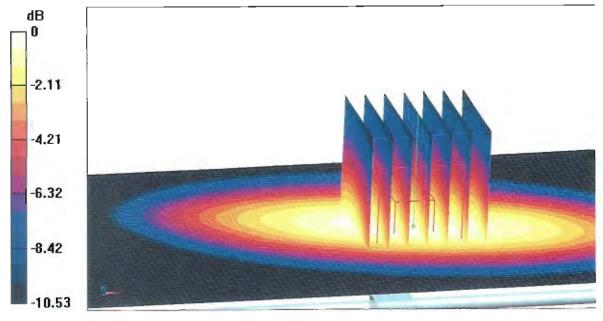


0 dB = 3.00 W/kg = 4.77 dBW/kg

Certificate No: Z16-97124 Page 5 of 8



# Impedance Measurement Plot for Head TSL

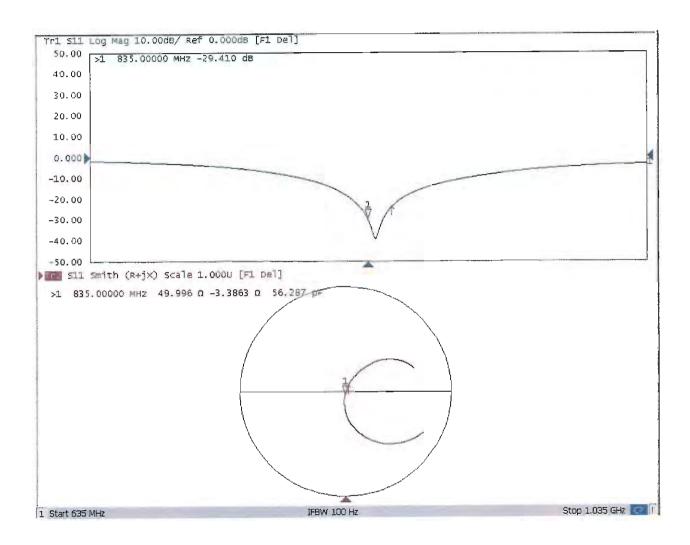



### DASY5 Validation Report for Body TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d200

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: f = 835 MHz;  $\sigma = 0.978$  S/m;  $\varepsilon_r = 54.86$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(9.71,9.71, 9.71); Calibrated: 8/26/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2015-08-26
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7372)

Date: 08.23.2016

# Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 55.53 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 3.54 W/kg

SAR(1 g) = 2.43 W/kg; SAR(10 g) = 1.62 W/kg


Maximum value of SAR (measured) = 3.04 W/kg

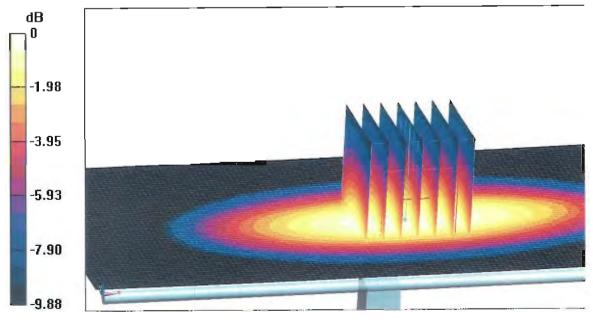

0 dB = 3.04 W/kg = 4.83 dBW/kg



# Impedance Measurement Plot for Body TSL

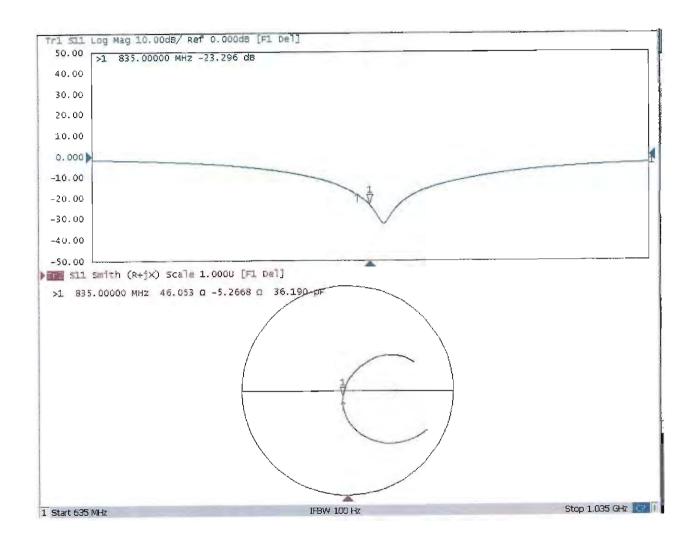

Certificate No: Z16-97124

## **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: D1750V2-1068\_Nov16

# CALIBRATION CERTIFICATE

Object D1750V2 - SN:1068

Calibration procedure(s) QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date: November 16, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).

The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 7349	15-Jun-16 (No. EX3-7349_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17
	Name	Function	Signature
Calibrated by:	Claudio Leubler	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	el u

Issued: November 17, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

### **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1750 MHz ± 1 MHz	

# **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.1 ± 6 %	1.37 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.20 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	36.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.88 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.5 W/kg ± 16.5 % (k=2)

**Body TSL parameters**The following parameters and calculations were applied.

The following parameters and calculations were appr	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.4	1.49 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.7 ± 6 %	1.49 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		-400

# SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	· · · · · · · · · · · · · · · · · · ·
SAR measured	250 mW input power	9.04 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	36.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.85 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	19.4 W/kg ± 16.5 % (k=2)

Certificate No: D1750V2-1068\_Nov16

# Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.4 Ω + 3.9 jΩ
Return Loss	- 27.9 dB

# **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	47.1 Ω + 2.7 jΩ
Return Loss	- 27.8 dB

### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.221 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG	
Manufactured on	June 15, 2010	

Page 4 of 8

Certificate No: D1750V2-1068\_Nov16

### **DASY5 Validation Report for Head TSL**

Date: 16.11.2016

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1068

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: f = 1750 MHz;  $\sigma = 1.37 \text{ S/m}$ ;  $\varepsilon_r = 39.1$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

### DASY52 Configuration:

Probe: EX3DV4 - SN7349; ConvF(8.46, 8.46, 8.46); Calibrated: 15.06.2016;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 30.12.2015

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

# Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.4 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 16.8 W/kg


SAR(1 g) = 9.2 W/kg; SAR(10 g) = 4.88 W/kg

Maximum value of SAR (measured) = 14.0 W/kg

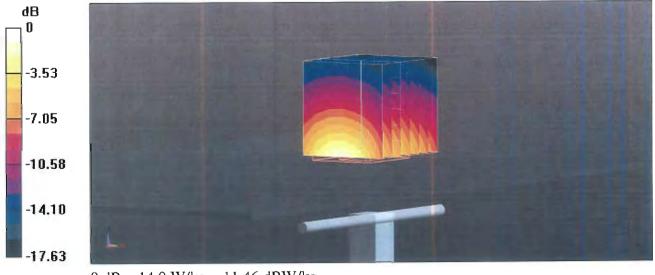

0 dB = 14.0 W/kg = 11.46 dBW/kg

# Impedance Measurement Plot for Head TSL

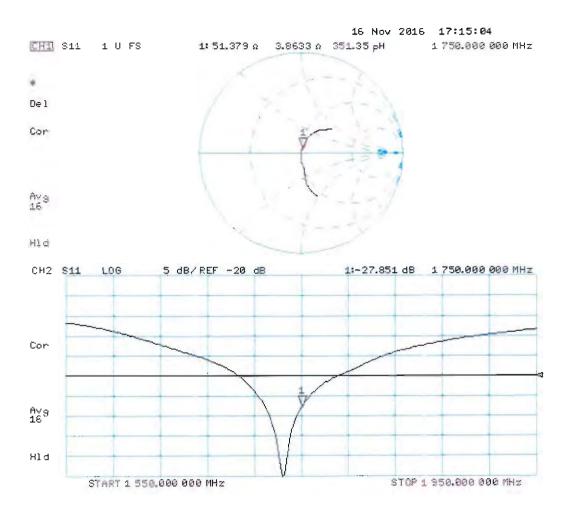

### **DASY5 Validation Report for Body TSL**

Date: 16.11.2016

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN:1068

Communication System: UID 0 - CW; Frequency: 1750 MHz

Medium parameters used: f = 1750 MHz;  $\sigma = 1.49 \text{ S/m}$ ;  $\varepsilon_r = 53.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

### DASY52 Configuration:

Probe: EX3DV4 - SN7349; ConvF(8.25, 8.25, 8.25); Calibrated: 15.06.2016;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 30.12.2015

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

• DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

# Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.57 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 15.8 W/kg


SAR(1 g) = 9.04 W/kg; SAR(10 g) = 4.85 W/kg

Maximum value of SAR (measured) = 13.5 W/kg



0 dB = 13.5 W/kg = 11.30 dBW/kg

# Impedance Measurement Plot for Body TSL

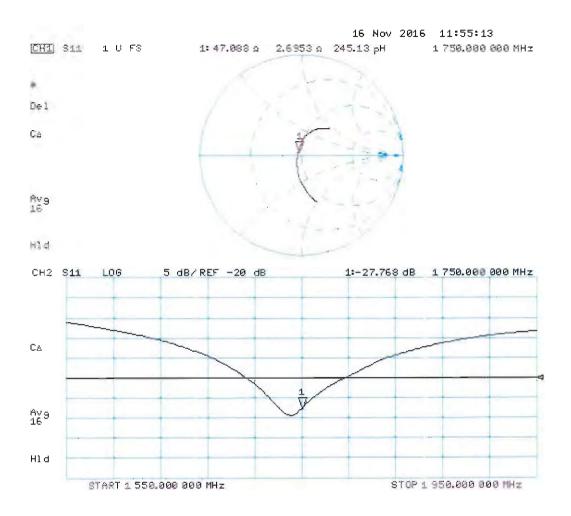

# Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura **Swiss Calibration Service** 

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: D1900V2-5d041\_Sep16

# CALIBRATION CERTIFICATE

Object

D1900V2 - SN:5d041

Calibration procedure(s)

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

September 30, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	IÐ#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 7349	15-Jun-16 (No. EX3-7349_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (No. 217-02223)	In house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Jun-15)	In house check: Oct-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16
	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	a l
Approved by:	Katja Pokovic	Technical Manager	RUL

Issued: September 30, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z

not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d041\_Sep16 Page 2 of 8

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

**Head TSL parameters**The following parameters and calculations were applied.

The tonowing parameters and earloans note app.	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.5 ± 6 %	1.40 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.5 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.33 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.4 W/kg ± 16.5 % (k=2)

**Body TSL parameters** 

The following parameters and calculations were applied.

The following parameters and ealequations were appropriately	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.6 ± 6 %	1.49 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

# SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.58 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	38.8 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.10 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.6 W/kg ± 16.5 % (k=2)

Page 3 of 8 Certificate No: D1900V2-5d041\_Sep16

# Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.5 Ω + 8.0 jΩ
Return Loss	- 21.8 dB

# Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.7 Ω + 7.6 jΩ
Return Loss	- 22.1 dB

## General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 04, 2003

Certificate No: D1900V2-5d041\_Sep16

## **DASY5 Validation Report for Head TSL**

Date: 28.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.4 \text{ S/m}$ ;  $\varepsilon_r = 40.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

### DASY52 Configuration:

Probe: EX3DV4 - SN7349; ConvF(7.99, 7.99, 7.99); Calibrated: 15.06.2016;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 30.12.2015

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

# Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 108.5 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 19.0 W/kg


SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.33 W/kg

Maximum value of SAR (measured) = 15.7 W/kg

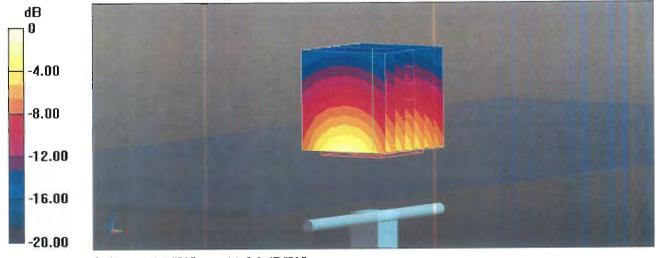

0 dB = 15.7 W/kg = 11.96 dBW/kg

# Impedance Measurement Plot for Head TSL

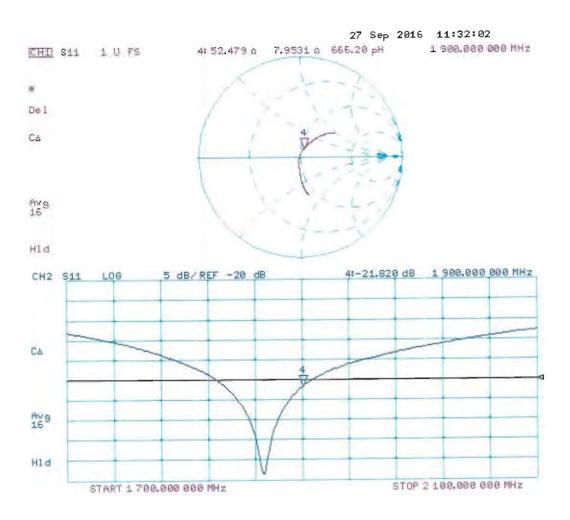

## **DASY5 Validation Report for Body TSL**

Date: 30.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.49 \text{ S/m}$ ;  $\varepsilon_r = 53.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

### DASY52 Configuration:

Probe: EX3DV4 - SN7349; ConvF(8.03, 8.03, 8.03); Calibrated: 15.06.2016;

• Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 30.12.2015

• Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

# Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.7 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 16.7 W/kg


SAR(1 g) = 9.58 W/kg; SAR(10 g) = 5.1 W/kg

Maximum value of SAR (measured) = 14.3 W/kg



0 dB = 14.3 W/kg = 11.55 dBW/kg

# Impedance Measurement Plot for Body TSL

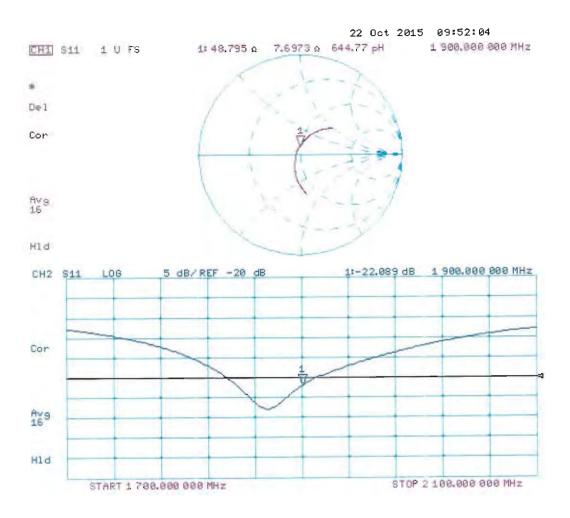



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Fax: +86-10-62304633-2504 Tel: +86-10-62304633-2079 E-mail: cttl@chinattl.com

Http://www.chinattl.cn

Client

Sporton TW





Certificate No: Z16-97130

## CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 736

Calibration Procedure(s)

FD-Z11-2-003-01

Calibration Procedures for dipole validation kits

Calibration date:

August 30, 2016

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	01-Jul-15 (CTTL, No.J15X04256)	Jun-16
Power sensor NRP-Z91	101547	01-Jul-15 (CTTL, No.J15X04256)	Jun-16
Reference Probe EX3DV4	SN 3801	29-Jun-16(SPEAG,No.EX3-3801_Jun16)	Jun-17
DAE4	SN 777	22-Aug-16(CTTL-SPEAG,No.Z16-97138)	Aug-17
Secondary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	01-Feb-16 (CTTL, No.J16X00893)	Jan-17
Network Analyzer E5071C	MY46110673	26-Jan-16 (CTTL, No.J16X00894)	Jan-17

Name Signature **Function** Calibrated by: Zhao Jing SAR Test Engineer Reviewed by: Qi Dianyuan SAR Project Leader Approved by: Lu Bingsong Deputy Director of the laboratory

Issued: Septembler 1, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z16-97130

Page 1 of 8



Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z16-97130 Page 2 of 8



### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1258
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

# **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.1 mW /g ± 20.8 % (k=2)
SAR averaged over 10 ${\it cm}^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	25.0 mW /g ± 20.4 % (k=2)

### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.0 ± 6 %	1.93 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	52.1 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $$ $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.10 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	24.4 mW /g ± 20.4 % (k=2)

Certificate No: Z16-97130 Page 3 of 8

### **Appendix**

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.5Ω+ 4.99jΩ
Return Loss	- 25.3dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.0Ω+ 4.65jΩ
Return Loss	- 25.7dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.053 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z16-97130



### **DASY5 Validation Report for Head TSL**

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 736

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma = 1.812 \text{ S/m}$ ;  $\epsilon r = 39.54$ ;  $\rho = 1000 \text{ kg/m}3$ 

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3801; ConvF(6.67, 6.67, 6.67); Calibrated: 6/29/2016;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/22/2016
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7372)

Date: 08.30.2016

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 103.9 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 26.9 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.24 W/kg

Maximum value of SAR (measured) = 20.2 W/kg

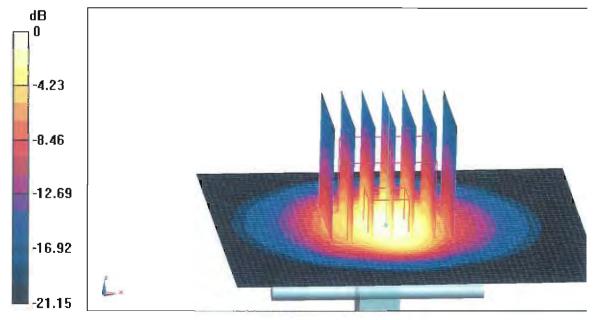


0 dB = 20.2 W/kg = 13.05 dBW/kg

Certificate No: Z16-97130 Page 5 of 8



# Impedance Measurement Plot for Head TSL

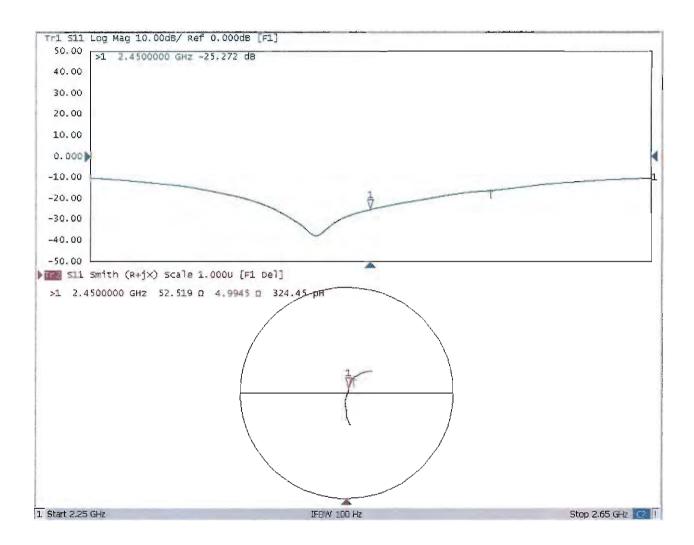



### DASY5 Validation Report for Body TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 736

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma = 1.933 \text{ S/m}$ ;  $\varepsilon_r = 51.96$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Center Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3801; ConvF(6.88, 6.88, 6.88); Calibrated: 6/29/2016;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/22/2016
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7372)

Date: 08.30.2016

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 95.98 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 26.1 W/kg

SAR(1 g) = 13 W/kg; SAR(10 g) = 6.1 W/kg

Maximum value of SAR (measured) = 19.6 W/kg

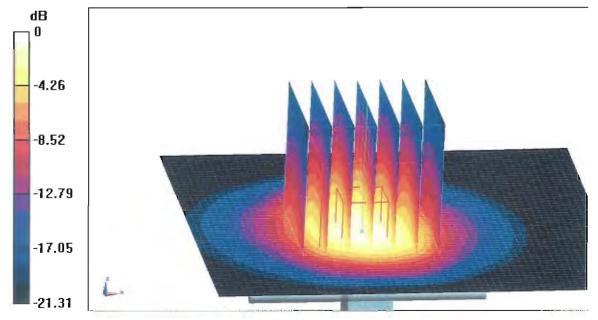


0 dB = 19.6 W/kg = 12.92 dBW/kg

Certificate No: Z16-97130 Page 7 of 8



# Impedance Measurement Plot for Body TSL

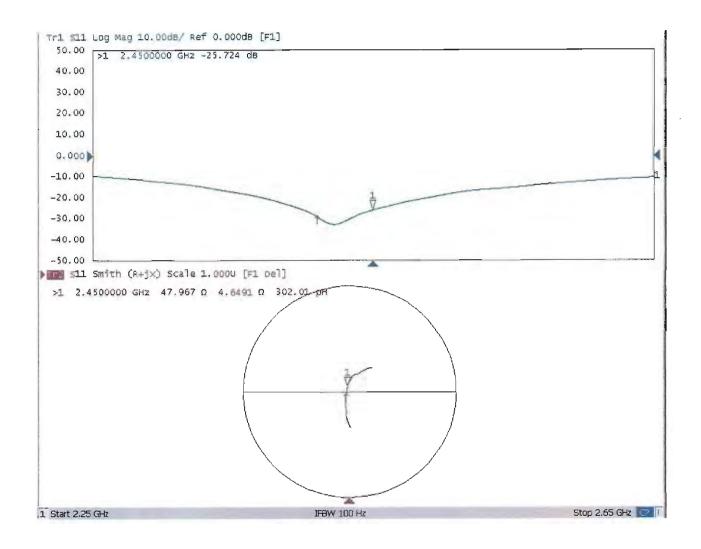





Client

Sporton TW

**Certificate No:** 

Z16-97132

## **CALIBRATION CERTIFICATE**

Object

D2600V2 - SN: 1008

Calibration Procedure(s)

FD-Z11-2-003-01

Calibration Procedures for dipole validation kits

Calibration date:

August 30, 2016

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 $\pm$ 3)  $^{\circ}$ C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	01-Jul-15 (CTTL, No.J15X04256)	Jun-16
Power sensor NRP-Z91	101547	01-Jul-15 (CTTL, No.J15X04256)	Jun-16
Reference Probe EX3DV4	SN 3801	29-Jun-16(SPEAG,No.EX3-3801_Jun16)	Jun-17
DAE4	SN 777	22-Aug-16(CTTL-SPEAG,No.Z16-97138)	Aug-17
Secondary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	01-Feb-16 (CTTL, No.J16X00893)	Jan-17
Network Analyzer E5071C	MY46110673	26-Jan-16 (CTTL, No.J16X00894)	Jan-17

Name

**Function** 

Signaturo

Calibrated by:

Zhao Jing

SAR Test Engineer

是

Reviewed by:

Qi Dianyuan

SAR Project Leader

Approved by:

Lu Bingsong

Deputy Director of the laboratory

Issued: September 1, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z16-97132

Page 1 of 8



Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z16-97132 Page 2 of 8



### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1258
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2600 MHz ± 1 MHz	

### **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.4 ± 6 %	1.97 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	56.8 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	_
SAR measured	250 mW input power	6.40 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	25.6 mW /g ± 20.4 % (k=2)

### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.5	2.16 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.2 ± 6 %	2.18 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.9 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	55.2 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.28 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	25.0 mW /g ± 20.4 % (k=2)

Certificate No: Z16-97132 Page 3 of 8

### **Appendix**

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.3Ω- 1.82jΩ
Return Loss	- 31.8dB

### **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	45.8Ω- 1.91jΩ
Return Loss	- 26.4dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.046 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

	20512
Manufactured by	SPEAG

Certificate No: Z16-97132 Page 4 of 8



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 Http://www.chinattl.cn

#### DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1008

Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2600 MHz;  $\sigma = 1.974 \text{ S/m}$ ;  $\epsilon r = 39.43$ ;  $\rho = 1000 \text{ kg/m}3$ 

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3801; ConvF(6.64, 6.64, 6.64); Calibrated: 6/29/2016;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/22/2016
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7372)

Date: 08.30.2016

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 107.4 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 30.0 W/kg

SAR(1 g) = 14.2 W/kg; SAR(10 g) = 6.4 W/kg

Maximum value of SAR (measured) = 22.1 W/kg

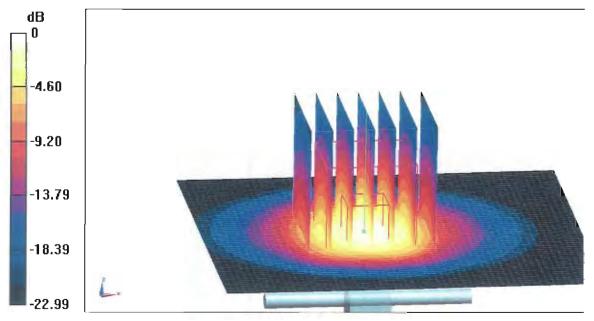


0 dB = 22.1 W/kg = 13.44 dBW/kg

Certificate No: Z16-97132 Page 5 of 8



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 Http://www.chinattl.en

#### Impedance Measurement Plot for Head TSL

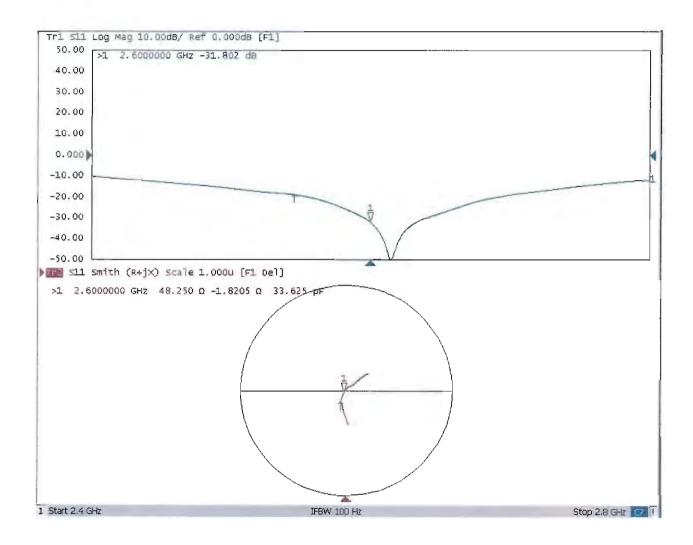



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.cn

#### DASY5 Validation Report for Body TSL

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1008

Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2600 MHz;  $\sigma = 2.184 \text{ S/m}$ ;  $\varepsilon_r = 52.15$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3801; ConvF(6.7, 6.7,6.7); Calibrated: 6/29/2016;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/22/2016
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7372)

Date: 08.30.2016

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 94.70 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 28.8 W/kg

SAR(1 g) = 13.9 W/kg; SAR(10 g) = 6.28 W/kg

Maximum value of SAR (measured) = 21.3 W/kg

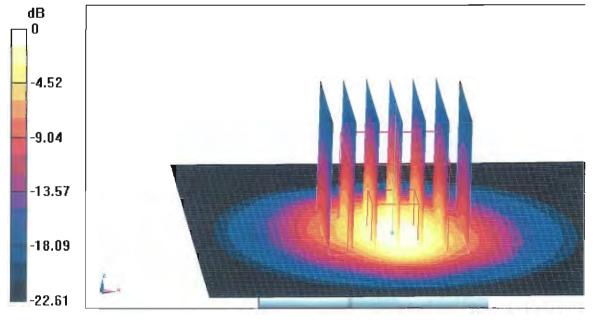


0 dB = 21.3 W/kg = 13.28 dBW/kg

Certificate No: Z16-97132 Page 7 of 8



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tcl: +86-10-62304633-2079 Fax: +86-10-62304633-2504 Http://www.chinattl.cn

#### Impedance Measurement Plot for Body TSL

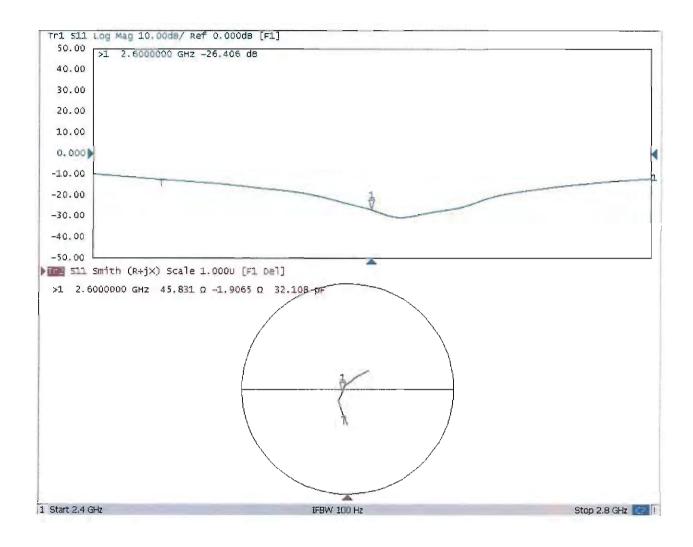

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: D5GHzV2-1006\_Sep16

#### CALIBRATION CERTIFICATE

Object D5GHzV2 - SN:1006

Calibration procedure(s) QA CAL-22.v2

Calibration procedure for dipole validation kits between 3-6 GHz

Calibration date: September 27, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Certificate No: D5GHzV2-1006\_Sep16

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-16 (No. 217-02295)	Apr-17
Reference Probe EX3DV4	SN: 3503	30-Jun-16 (No. EX3-3503_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (No. 217-02222)	In house check: Oct-16
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (No. 217-02223)	In house check: Oct-16
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Jun-15)	In house check: Oct-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16
	Name	Function	Signature
Calibrated by:	Claudio Leubler	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	RK

Issued: September 27, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Page 1 of 12

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A

not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### **Additional Documentation:**

Certificate No: D5GHzV2-1006\_Sep16

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0  mm, dz = 1.4  mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5750 MHz ± 1 MHz	

#### Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.5 ± 6 %	4.59 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL at 5250 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.13 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.6 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 19.5 % (k=2)

#### Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.0 ± 6 %	4.93 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.47 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.8 W / kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.40 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.7 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006\_Sep16 Page 3 of 12

#### Head TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.8 ± 6 %	5.08 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL at 5750 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.5 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.7 W/kg ± 19.5 % (k=2)

Body TSL parameters at 5250 MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.4 ± 6 %	5.52 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL at 5250 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.59 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	75.5 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.2 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006\_Sep16

#### Body TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.8 ± 6 %	6.00 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.90 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	78.6 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	_
SAR measured	100 mW input power	2.22 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	22.0 W/kg ± 19.5 % (k=2)

#### Body TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.5 ± 6 %	6.21 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL at 5750 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.50 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	74.6 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2. <u>10 W/kg</u>
SAR for nominal Body TSL parameters	normalized to 1W	20.8 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006\_Sep16

# Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL at 5250 MHz

Impedance, transformed to feed point	55.6 Ω - 6.5 jΩ
Return Loss	- 21.8 dB

#### Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	57.5 Ω - 4.7 jΩ
Return Loss	- 21.7 dB

#### Antenna Parameters with Head TSL at 5750 MHz

Impedance, transformed to feed point	59.2 Ω + 5.8 jΩ
Return Loss	- 20.1 dB

### Antenna Parameters with Body TSL at 5250 MHz

Impedance, transformed to feed point	55.5 Ω - 3.4 jΩ
Return Loss	- 24.2 dB

### Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	59.3 Ω - 1.9 jΩ
Return Loss	- 21.2 dB

## Antenna Parameters with Body TSL at 5750 MHz

Impedance, transformed to feed point	58.8 Ω + 8.9 jΩ
Return Loss	- 18.8 dB
Hetalit Loss	

### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.201 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 28, 2003

Certificate No: D5GHzV2-1006\_Sep16 Page 6 of 12

#### **DASY5 Validation Report for Head TSL**

Date: 27.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1006

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used: f = 5250 MHz;  $\sigma = 4.59$  S/m;  $\varepsilon_r = 34.5$ ;  $\rho = 1000$  kg/m<sup>3</sup> Medium parameters used: f = 5600 MHz;  $\sigma = 4.93$  S/m;  $\varepsilon_r = 34.0$ ;  $\rho = 1000$  kg/m<sup>3</sup> Medium parameters used: f = 5750 MHz;  $\sigma = 5.08$  S/m;  $\varepsilon_r = 33.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

#### DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.42, 5.42, 5.42); Calibrated: 30.06.2016, ConvF(4.89, 4.89, 4.89); Calibrated: 30.06.2016, ConvF(4.85, 4.85, 4.85); Calibrated: 30.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

# Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 72.67 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 29.4 W/kg

SAR(1 g) = 8.13 W/kg; SAR(10 g) = 2.32 W/kg

Maximum value of SAR (measured) = 18.2 W/kg

# Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 72.60 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 33.1 W/kg

SAR(1 g) = 8.47 W/kg; SAR(10 g) = 2.4 W/kg

Maximum value of SAR (measured) = 19.7 W/kg

# Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,


dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 70.56 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 33.0 W/kg


SAR(1 g) = 8.14 W/kg; SAR(10 g) = 2.3 W/kg

Maximum value of SAR (measured) = 19.2 W/kg

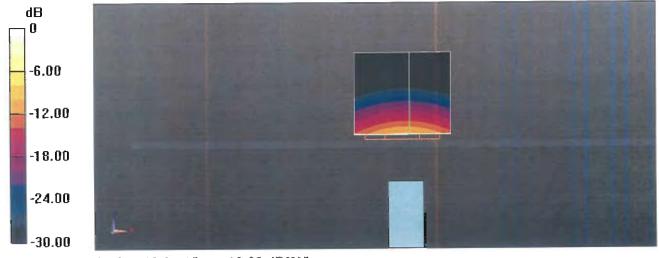

0 dB = 19.2 W/kg = 12.83 dBW/kg

#### Impedance Measurement Plot for Head TSL

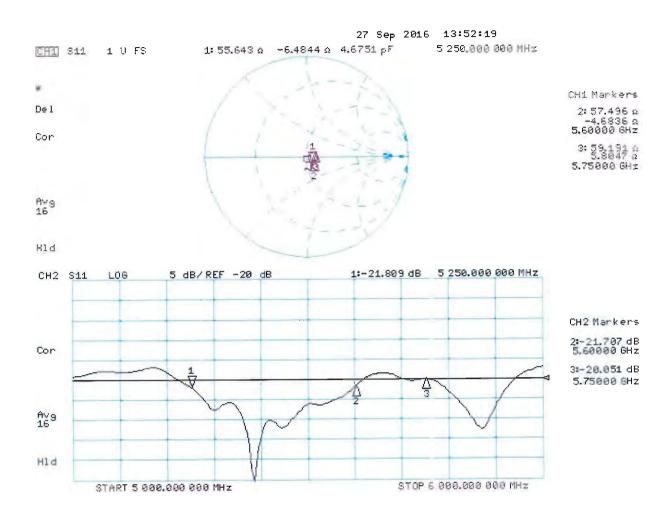

#### **DASY5 Validation Report for Body TSL**

Date: 26.09.2016

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1006

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used: f = 5250 MHz;  $\sigma = 5.52$  S/m;  $\varepsilon_r = 47.4$ ;  $\rho = 1000$  kg/m<sup>3</sup> Medium parameters used: f = 5600 MHz;  $\sigma = 6.00$  S/m;  $\varepsilon_r = 46.8$ ;  $\rho = 1000$  kg/m<sup>3</sup> Medium parameters used: f = 5750 MHz;  $\sigma = 6.21$  S/m;  $\varepsilon_r = 46.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

#### DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(4.85, 4.85, 4.85); Calibrated: 30.06.2016, ConvF(4.35, 4.35, 4.35); Calibrated: 30.06.2016, ConvF(4.3, 4.3, 4.3); Calibrated: 30.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

# Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 66.79 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 28.8 W/kg

SAR(1 g) = 7.59 W/kg; SAR(10 g) = 2.13 W/kg

Maximum value of SAR (measured) = 17.9 W/kg

# Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.00 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 32.5 W/kg

SAR(1 g) = 7.9 W/kg; SAR(10 g) = 2.22 W/kg

Maximum value of SAR (measured) = 19.0 W/kg

# Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,


dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.64 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 32.2 W/kg


SAR(1 g) = 7.5 W/kg; SAR(10 g) = 2.1 W/kg

Maximum value of SAR (measured) = 18.5 W/kg

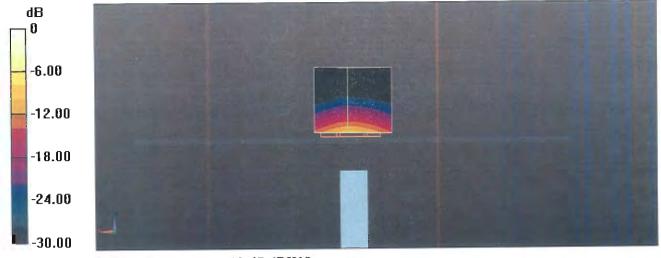

0 dB = 18.5 W/kg = 12.67 dBW/kg

# Impedance Measurement Plot for Body TSL

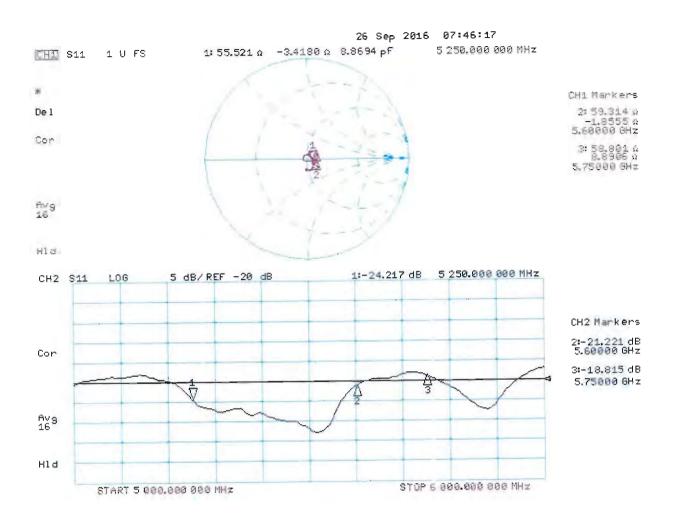

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton - ICC (Auden)

Accreditation No.: SCS 0108

Certificate No: DAE4-1424\_Feb17

#### CALIBRATION CERTIFICATE

Object DAE4 - SD 000 D04 BM - SN: 1424

Calibration procedure(s) QA CAL-06.v29

Calibration procedure for the data acquisition electronics (DAE)

Calibration date:

February 16, 2017

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	09-Sep-16 (No:19065)	Sep-17
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	05-Jan-17 (in house check)	In house check: Jan-18
			In house check: Jan-18

Name

Adrian Gehring

Function

Technician

Approved by:

Calibrated by:

Fin Bomholt

Deputy Technical Manager

1

Issued: February 16, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-1424\_Feb17 Page 1 of 5

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement. Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

#### **DC Voltage Measurement**

A/D - Converter Resolution nominal

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	403.134 ± 0.02% (k=2)	403.619 ± 0.02% (k=2)	403.192 ± 0.02% (k=2)
Low Range	3.96929 ± 1.50% (k=2)	3.99683 ± 1.50% (k=2)	3.98424 ± 1.50% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	358.0°±1°

Certificate No: DAE4-1424\_Feb17 Page 3 of 5

# Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	200030.67	-2.60	-0.00
Channel X	+ Input	20005.85	1.13	0.01
Channel X	- Input	-20002.78	2.30	-0.01
Channel Y	+ Input	200031.94	-1.24	-0.00
Channel Y	+ Input	20003.46	-1.30	-0.01
Channel Y	- Input	-20006.16	-1.09	0.01
Channel Z	+ Input	200032.25	-1.01	-0.00
Channel Z	+ Input	20004.24	-0.48	-0.00
Channel Z	- Input	-20006.86	-1.71	0.01

Low Range		Reading (µV)	Difference (μV)	Error (%)
Channel X	+ Input	2001.70	0.52	0.03
Channel X	+ Input	201.06	-0.00	-0.00
Channel X	- Input	-198.66	0.27	-0.13
Channel Y	+ Input	2001.37	0.26	0.01
Channel Y	+ Input	199.96	-1.04	-0.52
Channel Y	- Input	-199.87	-0.90	0.45
Channel Z	+ Input	2000.87	-0.15	-0.01
Channel Z	+ Input	199.84	-1.10	-0.55
Channel Z	- Input	-200.34	-1.29	0.65

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

<del></del> -	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-0.52	-2.04
	- 200	2.53	1.37
Channel Y	200	-13.45	-13.66
	- 200	11.80	11.67
Channel Z	200	-9.10	-8.91
	- 200	6.53	6.23

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

D7.67 1110 acc. 6111	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	2.89	-3.75
Channel Y	200	8.71		4.32
Channel Z	200	9.71	6.36	<u>-</u>

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Briton model of the first of th	High Range (LSB)	Low Range (LSB)
Channel X	15953	15468
Channel Y	15877	15900
Channel Z	15869	13329

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input  $10M\Omega$ 

Average (μV)		min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.70	-0.82	2.12	0.47
Channel Y	-0.67	-2.05	0.88	0.54
Channel Z	-1.55	-2.34	-0.03	0.37

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)		
Supply (+ Vcc)	+7.9		
Supply (- Vcc)	-7.6		

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1424\_Feb17 Page 5 of 5

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton - TW (Auden)

Certificate No: DAE3-495\_May16

Accreditation No.: SCS 0108

0	A		ID	DA	TI	AM	CER	TIE	10	AT	E
U	н	٧.	ID	n	N. P.	VIV	ULI		IV		_

Object DAE3 - SD 000 D03 AD - SN: 495

Calibration procedure(s) QA CAL-06.v29

Calibration procedure for the data acquisition electronics (DAE)

Calibration date: May 27, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22  $\pm$  3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	09-Sep-15 (No:17153)	Sep-16
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	05-Jan-16 (in house check)	In house check: Jan-17
Calibrator Box V2.1		05-Jan-16 (in house check)	In house check: Jan-17

Name Function Signature

Calibrated by:

R.Mayoraz

Technician

Technician

Approved by: Fin Bomholt Deputy Technical Manager

Issued: May 27, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE3-495\_May16

Page 1 of 5

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

#### Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

#### **Methods Applied and Interpretation of Parameters**

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement. Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

#### **DC Voltage Measurement**

A/D - Converter Resolution nominal

High Range:

1LSB =

6.1μV ,

full range = -100...+300 mV

Low Range:

1LSB =

61nV ,

full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	х	Υ	Z
High Range	404.392 ± 0.02% (k=2)	405.369 ± 0.02% (k=2)	405.725 ± 0.02% (k=2)
Low Range	3.95295 ± 1.50% (k=2)	3.99096 ± 1.50% (k=2)	3,96580 ± 1.50% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	78.0 ° ± 1 °

Certificate No: DAE3-495\_May16

# Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range		Reading (μV)	Difference (μV)	Error (%)
Channel X +	Input	199996.62	1.58	0.00
Channel X +	Input	20000.74	-0.12	-0.00
Channel X -		-19996.44	4.68	-0.02
Channel Y +	Input	199995.94	1.53	0.00
Channel Y +	Input	20002.54	1.56	0.01
Channel Y -	Input	-19999.75	1.29	-0.01
Channel Z +	Input	199992.83	-1.82	-0.00
Channel Z +	Input	20002.61	1.74	0.01
Channel Z -		-19998.46	2.69	-0.01

Low Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	2001.48	0.75	0.04
Channel X	+ Input	201.55	0.46	0.23
Channel X	- Input	-198.32	0.30	-0.15
Channel Y	+ Input	2000.13	-0.57	-0.03
Channel Y	+ Input	200.91	-0.45	-0.22
Channel Y	- Input	-199.30	-0.77	0.39
Channel Z	+ Input	1999.63	-0.96	-0.05
Channel Z	+ Input	200.82	-0.44	-0.22
Channel Z	- Input	-199.88	-1.27	0.64

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	3.18	2.27
	- 200	-2.19	-3.80
Channel Y	200	0.69	0.05
	- 200	-0.39	-0.92
Channel Z	200	2.28	2.22
	- 200	-4.44	-4.68

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

-	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	-0.76	-2.16
Channel Y	200	7.44	-	-0.52
Channel Z	200	5.77	5.68	<u></u> _

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15817	17431
Channel Y	15765	17509
Channel Z	15903	17029

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MO

Input Tolvisz	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	-0.15	-1.92	1.72	0.56
Channel Y	0.33	-0.86	2.13	0.60
Channel Z	-1.62	-2.91	-0.07	0.62

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

ripat Hoolotalloo (Typ.	Zeroing (kOhm)	Measuring (MOhm)	
Channel X	200	200	
Channel Y	200	200	
Channel Z	200	200	

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	<u>+14</u>
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE3-495\_May16 Page 5 of 5

Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: DAE4-1399\_Nov16

Accreditation No.: SCS 0108

### IBRATION CERTIFICATE

DAE4 - SD 000 D04 BM - SN: 1399 Object

QA CAL-06.v29 Calibration procedure(s)

Calibration procedure for the data acquisition electronics (DAE)

November 17, 2016 Calibration date:

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	09-Sep-16 (No:19065)	Sep-17
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	05-Jan-16 (in house check)	In house check: Jan-17
Calibrator Box V2.1	SE UMS 006 AA 1002	05-Jan-16 (in house check)	In house check: Jan-17
	•		

Calibrated by:

Name

Function

Signature

Dominique Steffen

Technician

Approved by:

Fin Bomholt

Deputy Technical Manager

Issued: November 17, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: DAE4-1399\_Nov16

Page 1 of 5

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

#### Glossary

DAE

Certificate No: DAE4-1399\_Nov16

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement. Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

#### **DC Voltage Measurement**

A/D - Converter Resolution nominal

1LSB = High Range:

 $6.1 \mu V$  , 1LSB =

full range = -100...+300 mV

Low Range:

61nV ,

full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	403.601 ± 0.02% (k=2)	403.860 ± 0.02% (k=2)	403.715 ± 0.02% (k=2)
Low Range	3.98192 ± 1.50% (k=2)	3.99210 ± 1.50% (k=2)	3.98028 ± 1.50% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	302.5°±1°

Page 3 of 5 Certificate No: DAE4-1399\_Nov16

# Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	199995.88	1.05	0.00
Channel X	+ Input	20002.28	0.87	0.00
Channel X	- Input	-19998.50	2.29	-0.01
Channel Y	+ Input	199993.59	-1.44	-0.00
Channel Y	+ Input	20000.11	-1.26	-0.01
Channel Y	- Input	-20001.82	-0.91	0.00
Channel Z	+ Input	199995.29	-0.07	-0.00
Channel Z	+ Input	19998.72	-2.63	-0.01
Channel Z	- Input	-20002.93	-1.99	0.01

Low Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	2001.09	-0.18	-0.01
Channel X	+ Input	201.99	0.26	0.13
Channel X	- Input	-197.66	0.46	-0.23
Channel Y	+ Input	2001.13	-0.06	-0.00
Channel Y	+ Input	200.58	-0.99	-0.49
Channel Y	- Input	-198.74	-0.44	0.22
Channel Z	+ Input	2001.38	0.15	0.01
Channel Z	+ Input	200.84	-0.68	-0.34
Channel Z		-199.07	-0.83	0.42

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-4.94	-6.62
-	- 200	8.38	6.51
Channel Y	200	-6.22	-6.54
	- 200	5.04	4.27
Channel Z	200	-6.68	-6.74
	- 200	4.86	5.05

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	4.65	-1.72
Channel Y	200	9.38	-	6.88
Channel Z	200	8.80	6.72	<u> </u>

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15826	16053
Channel Y	16118	16526
Channel Z	15887	15918

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

input Tolvisz	Std. Deviation (µV)			
Channel X	0.11	-0.73	0.73	0.27
Channel Y	-0.19	-1.32	1.76	0.44
Channel Z	-0.78	-2.06	0.51	0.41

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

ilput nesistance (Typi	Measuring (MOhm)	
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

# Calibration Laboratory of Schmid & Partner

Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton - TW (Auden)

Accreditation No.: SCS 0108

S

C

S

Certificate No: DAE4-778\_May16

# **CALIBRATION CERTIFICATE**

Object

DAE4 - SD 000 D04 BM - SN: 778

Calibration procedure(s)

QA CAL-06.v29

Calibration procedure for the data acquisition electronics (DAE)

Calibration date:

May 12, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}$ C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	09-Sep-15 (No:17153)	Sep-16
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	05-Jan-16 (in house check)	In house check: Jan-17
Calibrator Box V2.1	SE UMS 006 AA 1002	05-Jan-16 (in house check)	In house check: Jan-17

Calibrated by:

Name Dominique Steffen Function Technician Signature

Approved by:

Fin Bomholt

Deputy Technical Manager

Issued: May 12, 2016

This calibration certificate shall not be reproduced except in full without written approval of the faboratory.

Certificate No: DAE4-778\_May16

Page 1 of 5

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

#### Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

# **Methods Applied and Interpretation of Parameters**

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

# **DC Voltage Measurement**

A/D - Converter Resolution nominal

High Range: 1LSB =

 $LSB = 6.1 \mu V,$ 

full range = -100...+300 mV

Low Range:

1LSB = 61nV,

full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	Х	Y	z
High Range	404.712 ± 0.02% (k=2)	403.516 ± 0.02% (k=2)	405.068 ± 0.02% (k=2)
Low Range	3.98678 ± 1.50% (k=2)	3.96495 ± 1.50% (k=2)	4.00091 ± 1.50% (k=2)

#### **Connector Angle**

Comparing April 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	
Connector Angle to be used in DASY system	270.0°±1°
	<u> </u>

Certificate No: DAE4-778\_May16

# Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range		Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	200032.14	-1.38	-0.00
Channel X	+ Input	20005.68	0.79	0.00
Channel X	- Input	-20003.61	1.31	-0.01
Channel Y	+ Input	200030.28	-3.73	-0.00
Channel Y	+ Input	20006.01	1.25	0.01
Channel Y	- Input	-20003.00	1.89	-0.01
Channel Z	+ Input	200035.46	1.52	0.00
Channel Z	+ Input	20002.36	-2.31	-0.01
Channel Z	- Input	-20008.31	-3.27	0.02

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2001.27	0.01	0.00
Channel X + Input	201.37	0.21	0.10
Channel X - Input	-198.61	-0.02	0.01
Channel Y + input	2001.38	0.24	0.01
Channel Y + Input	200.13	-0.97	-0.48
Channel Y - Input	-198.84	-0.10	0.05
Channel Z + Input	2001.29	0.21	0.01
Channel Z + Input	200.34	-0.69	-0.34
Channel Z - Input	-200.58	-1.74	0.88

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode	High Range	Low Range	
	Input Voltage (mV)	Average Reading (μV)	Average Reading (μV)	
Channel X	200	-4.35	-5.61	
	- 200	7.07	5.78	
Channel Y	200	-1.79	-1.82	
	- 200	0.49	0.20	
Channel Z	200	-12.55	-12.56	
	- 200	10.17	10.19	

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	-0.66	-2.54
Channel Y	200	8.70	-	-0.26
Channel Z	200	3.71	7.16	-

# 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16054	16869
Channel Y	16191	17846
Channel Z	16441	16314

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input  $10M\Omega$ 

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.48	-0.60	1.44	0.42
Channel Y	-0.09	-1.42	2.50	0.58
Channel Z	-1.11	-2.45	-0.19	0.45

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton - TW (Auden)

Certificate No: DAE3-577\_Sep16

Accreditation No.: SCS 0108

C

S

### IBRATION CERTIFICATE

Object

DAE3 - SD 000 D03 AA - SN: 577

Calibration procedure(s)

QA CAL-06.v29

Calibration procedure for the data acquisition electronics (DAE)

Calibration date:

September 28, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	09-Sep-16 (No:19065)	Sep-17
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	05-Jan-16 (in house check)	In house check: Jan-17
Calibrator Box V2.1	1	05-Jan-16 (in house check)	In house check: Jan-17

Name

Function

Calibrated by:

Eric Hainfeld

Technician

Signature

Approved by:

Fin Bomholt

Deputy Technical Manager

Issued: September 28, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

### Glossary

DAE

data acquisition electronics

Connector angle

Certificate No: DAE3-577\_Sep16

information used in DASY system to align probe sensor X to the robot

coordinate system.

### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

### **DC Voltage Measurement**

Low Range:

A/D - Converter Resolution nominal

High Range:

1LSB =

 $\begin{array}{ll} 6.1 \mu V \; , & \qquad \text{full range} = & -100...+300 \; \text{mV} \\ 61 \text{nV} \; , & \qquad \text{full range} = & -1......+3 \text{mV} \end{array}$ 

1LSB =

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.533 ± 0.02% (k=2)	403.512 ± 0.02% (k=2)	403.819 ± 0.02% (k=2)
Low Range	3.92648 ± 1.50% (k=2)	3.94206 ± 1.50% (k=2)	3.96074 ± 1.50% (k=2)

## **Connector Angle**

Connector Angle to be used in DASY system	190.0 ° ± 1 °

Certificate No: DAE3-577\_Sep16

Page 3 of 5

# Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	200038.14	2.56	0.00
Channel X + Input	20010.51	5.45	0.03
Channel X - Input	-20002.01	3.17	-0.02
Channel Y + Input	200032.33	-3.18	-0.00
Channel Y + Input	20006.38	1.35	0.01
Channel Y - Input	-20004.73	0.65	-0.00
Channel Z + Input	200031.49	-4.11	-0.00
Channel Z + Input	20005.92	0.98	0.00
Channel Z - Input	-20007.03	-1.64	0.01

Low Range	<del>-</del>	Reading (μV)	Difference (μV)	Error (%)
Channel X	+ Input	2001.00	-0.10	-0.01
Channel X	+ Input	201.47	0.40	0.20
Channel X	- Input	-198.57	0.28	-0.14
Channel Y	+ Input	2001.38	0.31	0.02
Channel Y	+ Input	200.40	-0.54	-0.27
Channel Y	- Input	-199.63	-0.73	0.37
Channel Z	+ Input	2000.35	-0.56	-0.03
Channel Z	+ Input	199.97	-0.93	-0.46
Channel Z	- Input	-200.50	-1.56	0.79

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-2.76	-4.30
	- 200	6.04	3.73
Channel Y	200	-14.29	-14.35
	- 200	12.74	12.77
Channel Z	200	3.10	2.81
	- 200	-5.90	-5.65

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

_	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	-1.07	-3.44
Channel Y	200	8.43	-	0.12
Channel Z	200	5.44	4.83	

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)	
Channel X	16132	16062	
Channel Y	16099	16321	
Channel Z	16116	15372	

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

11) Olivisz	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.37	-1.07	1.49	0.43
Channel Y	1.21	-0.41	3.21	0.59
Channel Z	-1.38	-2.63	-0.30	0.45

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Certificate No: EX3-3976\_Feb17

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-ICC (Auden)

## **CALIBRATION CERTIFICATE**

Object EX3DV4 - SN:3976

Calibration procedure(s) QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date: February 21, 2017

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Certificate No: EX3-3976\_Feb17

Primary Standards	(D	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: S5277 (20x)	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe ES3DV2	SN: 3013	31-Dec-16 (No. ES3-3013_Dec16)	Dec-17
DAE4	SN: 660	7-Dec-16 (No. DAE4-660_Dec16)	Dec-17
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by:

Claudio Leubler

Claudio Leubler

Enction

Function

Signature

Laboratory Technician

Approved by:

Katja Pokovic

Technical Manager

Issued: February 27, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization φ φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
   NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media, VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-3976\_Feb17 Page 2 of 11

EX3DV4 - SN:3976 February 21, 2017

# Probe EX3DV4

SN:3976

Manufactured:

Calibrated:

November 5, 2013

February 21, 2017

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3976

**Basic Calibration Parameters** 

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) <sup>2</sup> ) <sup>A</sup>	0.48	0.49	0.54	± 10.1 %
DCP (mV) <sup>B</sup>	102.3	101.2	103.1	

Modul	ation Calibration Parameters							
UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	173.0	±3.0 %
		Y	0.0	0.0	1.0		186.1	
		Z	0.0	0.0	1.0		174.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>&</sup>lt;sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

B Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3976 February 21, 2017

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3976

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.9	0.89	10.96	10.96	10.96	0.38	0.95	± 12.0 %
835	41.5	0.90	10.43	10.43	10.43	0.46	0.80	± 12.0 %
900	41.5	0.97	10.28	10.28	10.28	0.49	0.80	± 12.0 %
1750	40.1	1.37	8.93	8.93	8.93	0.33	0.80	± 12.0 %
1900	40.0	1.40	8.62	8.62	8.62	0.39	0.80	± 12.0 %
2000	40.0	1.40	8.61	8.61	8.61	0.29	0.80	± 12.0 %
2450	39.2	1.80	7.83	7.83	7.83	0.32	0.88	± 12.0 %
2600	39.0	1.96	7.60	7.60	7.60	0.36	0.87	± 12.0 %
3700	37.7	3.12	7.60	7.60	7.60	0.25	1.20	± 13.1 %
5250	35.9	4.71	5.56	5.56	5.56	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.98	4.98	4.98	0.40	1.80	± 13. <u>1 %</u>
5750	35.4	5.22	5.16	5.16	5.16	0.40	1.80	± 13.1 %

 $<sup>^{\</sup>rm C}$  Frequency validity above 300 MHz of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to  $\pm$  50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is  $\pm$  10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to  $\pm$  110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the Copy Function of t

the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3976

## Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity F	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	55.5	0.96	10.68	10.68	10,68	0.51	0.80	± 12.0 %
835	55.2	0.97	10.41	10.41	10.41	0.48	0.80	± 1 <u>2.0 %</u>
1750	53.4	1.49	8.57	8.57	8 <u>.5</u> 7	0.37	0.80	± 12.0 %
1900	53.3	1.52	8.31	8.31	8.31	0.41	0.80	± 12.0 %
2450	52.7	1.95	7.93	7.93	7.93	0.30	0.92	± 12.0 %
2600	52.5	2.16	7.59	7.59	7.59_	0.28	0.92	± 12.0 %
3700	51 <u>.</u> 0	3.55	6.84	6.84	6.84_	0.30	1.20	± 13.1 %
5250	48.9	5.36	4.87	4.87	4.87	0.40	1.90	± 13.1 %
5600	48.5	5.77	4.03	4.03	4.03	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.33	4.33	4.33	0.50	1.90	± 13.1 %

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


validity can be extended to ± 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvE uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.


Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

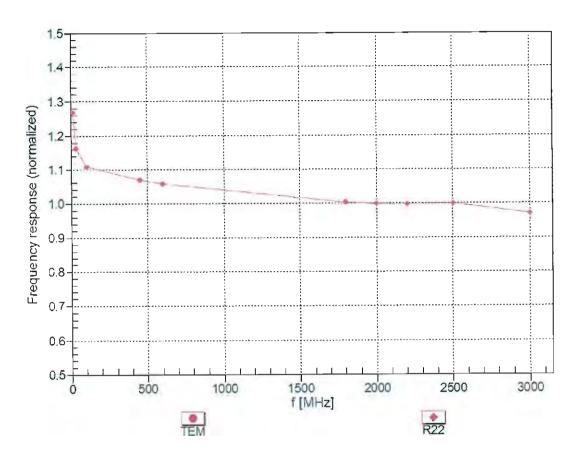

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


# Receiving Pattern ( $\phi$ ), $9 = 0^{\circ}$

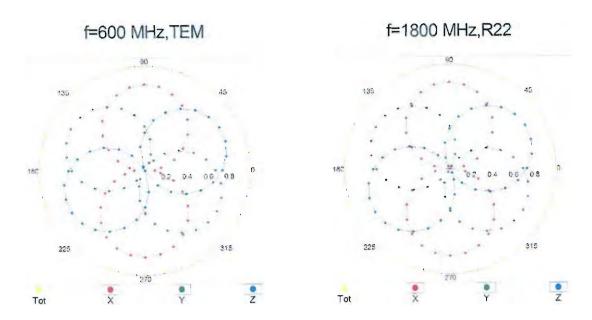


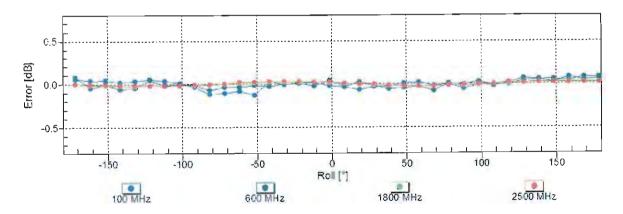

Uncertainty of Axiał Isotropy Assessment:  $\pm 0.5\%$  (k=2)


# Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

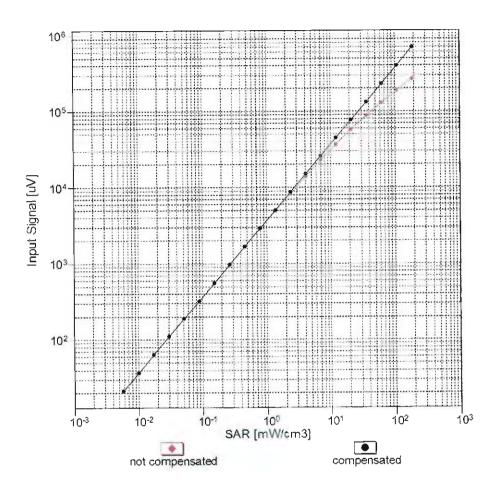

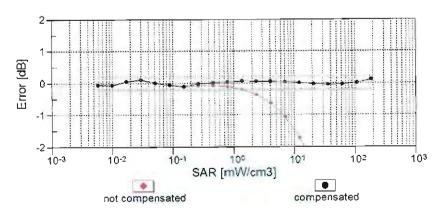



Uncertainty of Linearity Assessment: ± 0.6% (k=2)

## **Conversion Factor Assessment**

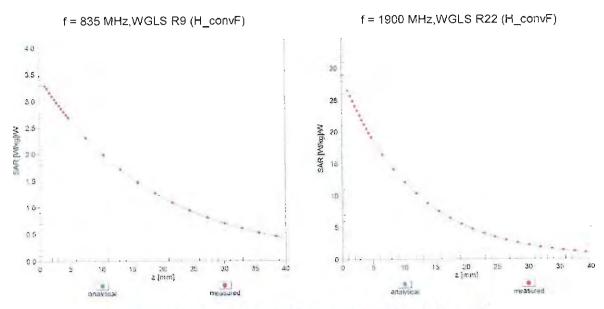

## Deviation from Isotropy in Liquid Error (φ, θ), f = 900 MHz

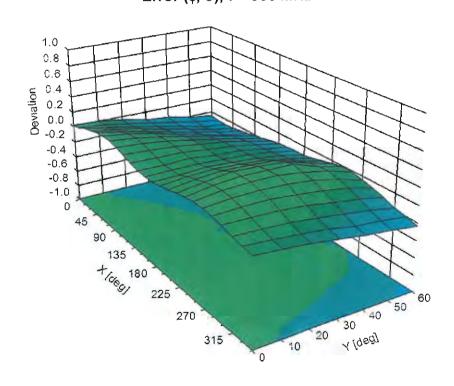



EX3DV4-- SN:3976

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3976

### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	-1.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: EX3-3925\_May16

S

## **CALIBRATION CERTIFICATE**

Object EX3DV4 - SN:3925

Calibration procedure(s) QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date: May 26, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: S5277 (20x)	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe ES3DV2	SN: 3013	31-Dec-15 (No. ES3-3013_Dec15)	Dec-16
DAE4	SN: 660	23-Dec-15 (No. DAE4-660_Dec15)	Dec-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (No. 217-02285/02284)	In house check: Jun-16
Power sensor E4412A	SN: MY41498087	06-Apr-16 (No. 217-02285)	In house check: Jun-16
Power sensor E4412A	SN: 000110210	06-Apr-16 (No. 217-02284)	In house check: Jun-16
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Apr-13)	In house check: Jun-16
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Name Function Signature

Calibrated by: Leif Klysner Laboratory Technician

Approved by: Katja Pokovic Technical Manager

Issued: May 31, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3925\_May16 Page 1 of 11

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z tissue simulating liquid sensitivity in free space

ConvF DCP sensitivity in TSL / NORMx,y,z diode compression point

CF A, B, C, D crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization φ

φ rotation around probe axis

Polarization 9

3 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e.,  $\vartheta = 0$  is normal to probe axis

Connector Angle

information used in DASY system to align probe sensor X to the robot coordinate system

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Methods Applied and Interpretation of Parameters:

- *NORMx,y,z*: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

EX3DV4 - SN:3925 May 26, 2016

# Probe EX3DV4

SN:3925

Manufactured:

March 8, 2013

Calibrated:

May 26, 2016

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3925

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	0.59	0.52	0.50	± 10.1 %
DCP (mV) <sup>8</sup>	96.5	97.9	98.9	

#### **Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>±</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	152.6	±2.7 %
		Y	0.0	0.0	1.0		143.7	
		Z	0.0	0.0	1.0		138.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>&</sup>lt;sup>^</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3925 May 26, 2016

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3925

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.9	0.89	10.37	10.37	10.37	0.48	0.80	± 12.0 %
835	41.5	0.90	9.92	9.92	9.92	0.47	0.81	± 12.0 %
900	41.5	0.97	9.72	9.72	9.72	0.41	0.80	± 12.0 %
1750	40.1	1.37	8.57	8.57	8.57	0.29	0.80	± 12.0 %
1900	40.0	1.40	8.30	8.30	8.30	0.30	0.80	± 12.0 %
2000	40.0	1.40	8.26	8.26	8.26	0.30	0.80	± 12.0 %
2450	39.2	1.80	7.47	7.47	7.47	0.35	0.80	± 12.0 %
2600	39.0	1.96	7.28	7.28	7.28	0.36	0.86	± 12.0 %
3500	37.9	2.91	7.14	7.14	7.14	0.29	1.30	± 13.1 %
5200	36.0	4.66	5.31	5. <u>3</u> 1	5.31	0.35	1.80	± 13.1 %
5300	35.9	4.76	5.15	5.15	5.15	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.66	4. <u>6</u> 6	4.66	0.45	1.80	± 13.1 %
5600	35.5	5.07	4.47	4.47	4.47	0.50	1.80	± 13.1 %
5800	35.3	5.27	4.51	4.51	4.51	0.50	1.80	± 13.1 %

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to

F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConyE uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3925 May 26, 2016

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3925

### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	55.5	0.96	10.18	10.18	10. <u>18</u>	0.49	0.80	± 12.0 %
835	55.2	0.97	9.91	9.91	9.91	0.44	0.88	± 12.0 %
900	55.0	1.05	9.96	9.96	9.96	0.47	0.80	± 12.0 %
1750	53.4	1.49	8.30	8.30	8.30	0.34	0.80	± 12.0 %
1900	53.3	1.52	8.00	8.00	8.00	0.38	0.80	± 12.0 %
2000	53.3	1.52	8.18	8.18	8.18	0.37	0.80	± 12.0 %
2450	52.7	1.95	7.64	7.64	7.64	0.36	0.80	± 12.0 %
2600	52.5	2.16	7.38	7.38	7.38	0.26	0.80	± 12.0 %
3500	51.3	3.31	6.73	6.73	6.73	0.29	1.30	± 13.1 %
5200	49.0	5.30	4.39	4.39	4.39	0.50	1.90	± 13.1 %
5300	48.9	5.42	4.22	4.22	4.22	0.50	1.90	± 13.1 %
5500	48.6	5.65	4.02	4.02	4.02	0.55	1.90	± 13.1 %
5600	48.5	5.77	3.85	3.85	3.85	0.60	1.90	± 13.1 %
5800	48.2	6.00	3.85	3.85	3.85	0.60	1.90	± 13. <u>1</u> %


<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConyE uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

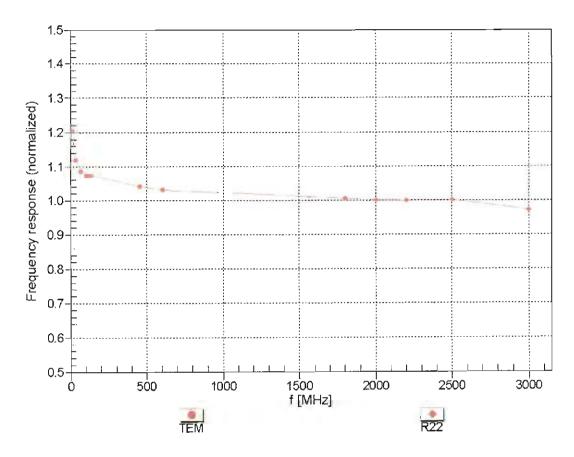


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

EX3DV4- SN:3925 May 26, 2016

# Receiving Pattern ( $\phi$ ), $9 = 0^{\circ}$

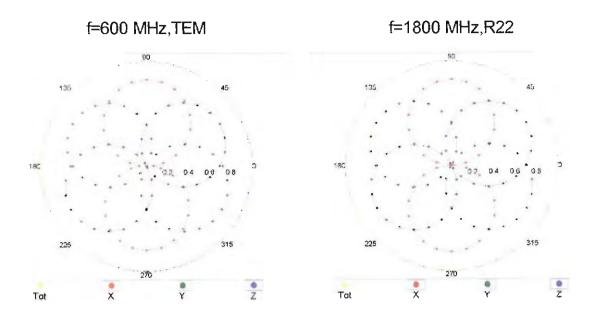

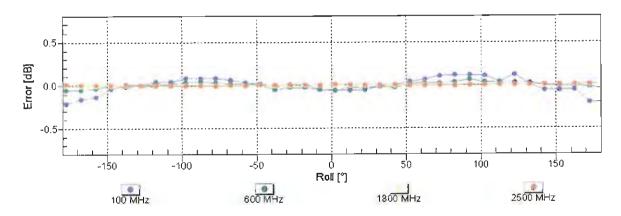


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

May 26, 2016 EX3DV4-SN:3925

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

105 10<sup>4</sup> Input Signal [uV]  $10^{3}$ 102 10 102 10-3 10-2 10-1 100 101  $10^{3}$ SAR [mW/cm3] compensated

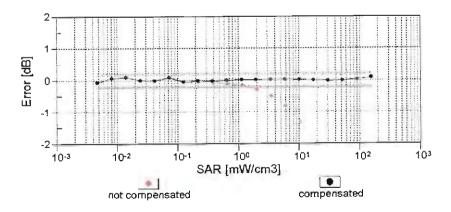


not compensated

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN:3925 May 26, 2016


# **Conversion Factor Assessment**

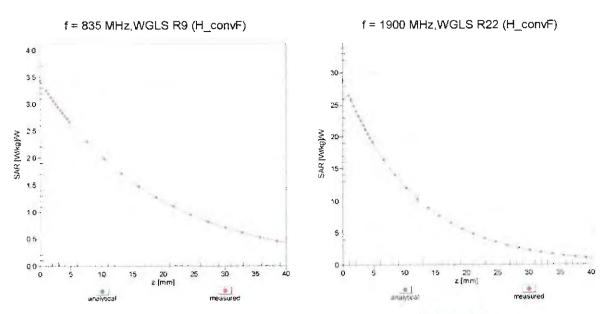

# **Deviation from Isotropy in Liquid**

Error  $(\phi, \vartheta)$ , f = 900 MHz

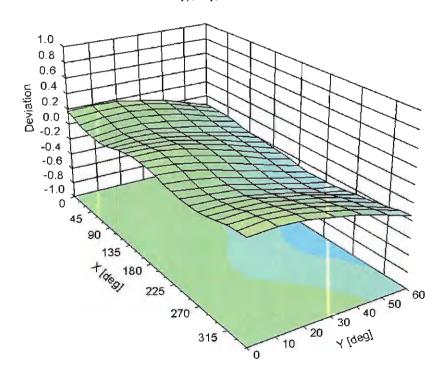



EX3DV4- SN:3925 May 26, 2016

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3925

### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	92.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: EX3-3955\_Nov16

## CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3955

Calibration procedure(s)

QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date:

November 24, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards ID		Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: S5277 (20x)	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe ES3DV2	SN: 3013	31-Dec-15 (No. ES3-3013_Dec15)	Dec-16
DAE4	SN: 660	23-Dec-15 (No. DAE4-660_Dec15)	Dec-16
Secondary Standards	ID and a	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by:

Name Leif Klysner Function Laboratory Technician Signature

Approved by:

Katja Pokovic

Technical Manager

Issued: November 28, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage

Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

Certificate No: EX3-3955\_Nov16

ConvF sensitivity in TSL / NORMx,y,z diode compression point

CF crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization  $\phi$   $\phi$  rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e.,  $\vartheta = 0$  is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

## Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Methods Applied and Interpretation of Parameters:

 NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).

NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
in the stated uncertainty of ConvF.

DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.

 PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics

• Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.

• ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.

 Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.

 Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

 Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required). EX3DV4 – SN:3955 November 24, 2016

# Probe EX3DV4

SN:3955

Manufactured:

August 6, 2013

Calibrated:

November 24, 2016

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

November 24, 2016

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3955

**Basic Calibration Parameters** 

Basic Calibration Parai	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) <sup>2</sup> ) <sup>A</sup>	0.34	0.40	0.31	± 10.1 %
DCP (mV) <sup>B</sup>	100.5	101.5	97.2	

**Modulation Calibration Parameters** 

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc⁻ (k=2)
0	CW	X	0.0	0.0	1.0	0.00	128.6	±3.3 %
		Y	0.0	0.0	1.0		140.6	
		Z	0.0	0.0	1.0		128.8	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>0</sup> Numerical linearization parameter: uncertainty not required.

A The uncertainties of Norm X,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

E Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3955 November 24, 2016

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3955

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.9	0.89	10.65	10.65	10.65	0.49	0.80	± 12.0 %
835	41.5	0.90	10.33	10.33	10.33	0.44	0.80	± 12.0 %
900	41.5	0.97	10.07	10. <u>0</u> 7	10.07	0.34	1.01	± 12.0 %
1750	40.1	1.37	8.68	8.68	8.68_	0.32	0.80	± 12.0 %
1900	40.0	1.40	8.43	8.43	8.43	0.32	0.80	± 12.0 %
2000	40.0	1.40	8.38	8.38	8.38	0.33	0.80	± 12.0 %
2450	39.2	1.80	7.5 <u>6</u>	7.56	7.56	0.24	1.06	± 12.0 %
2600	39.0	1.96	7.28	7.28	7.28	0.30	0.95	± 12.0 %
5250	35.9	4.71	5.04	5.04	5.04	0.40	1.80	± 13.1 9
5600	35.5	5.07	4.50	4.50	4.50_	0.50	1.80	± 13.1 9
5750	35.4	5.22	4.63	4.63	4.63	0.50	1.80	± 13.1 9

Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvE uncertainty for indicated target tissue parameters

the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

November 24, 2016

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3955

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	55.5	0.96	10.42	10.42	10.42	0.38	0.90	± 12.0 %
835	55.2	0.97	10.18	10.18	10.18	0.33	0.97	± 12.0 %
1750	53.4	1.49	8.31	8.31	8.31	0.46	0.80	± 12.0 %
1900	53.3	1.52	8.00	8.00	8.00_	0.30	0.95	± 12.0 %
2450	52.7	1.95	7.65	7. <u>65</u>	7.65	0.39	0.80	± 12.0 %
2600	52.5	2.16	7.42	7.42	7.42	0.37	0.80	± 12.0 %
5250	48.9	5.36	4.51	4.51	4.51	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.91	3.91	3.91	0.55	1.90	± 13.1 %
5750	48.3	5.94	4.12	4.12	4.12	0.55	1.90	± 13.1 %

Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the Control procedure, the control procedure to the control procedure.

the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

November 24, 2016 EX3DV4-SN:3955


# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

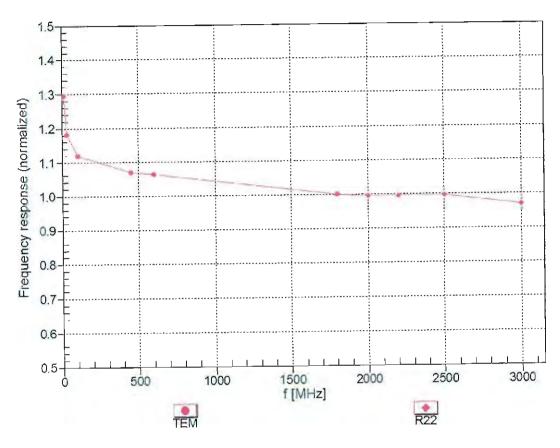


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

November 24, 2016

# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

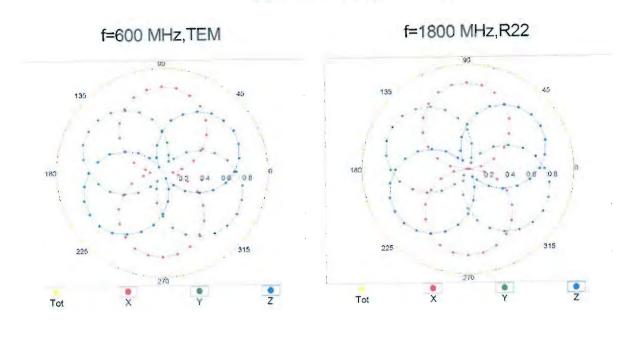


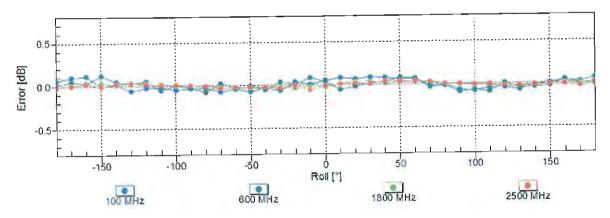


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

November 24, 2016

## Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

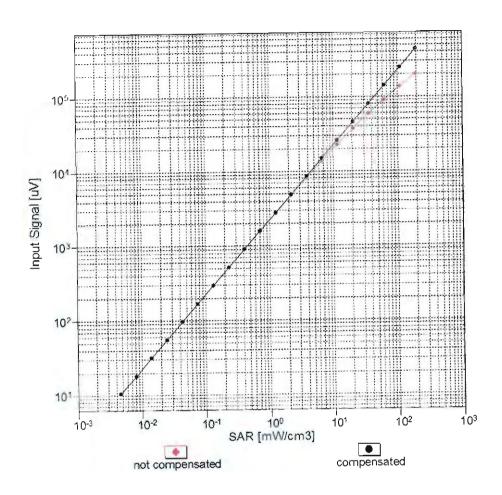


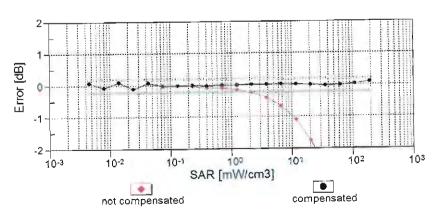

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN:3955 November 24, 2016


# **Conversion Factor Assessment**

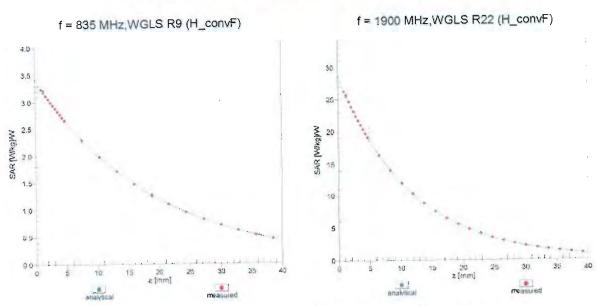

# **Deviation from Isotropy in Liquid**

Error ( $\phi$ ,  $\vartheta$ ), f = 900 MHz

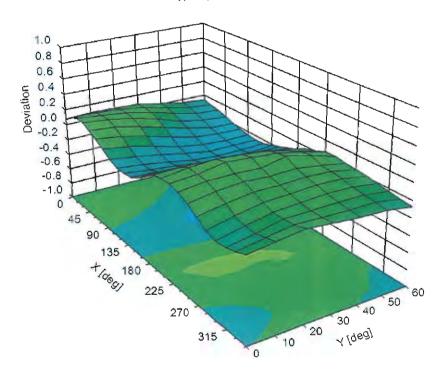



EX3DV4- SN:3955 November 24, 2016

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3955

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	130.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Http://www.chinattl.cn



Sporton TW

Certificate No: Z16-97123

**CNAS L0570** 

## **CALIBRATION CERTIFICATE**

Object ES3DV3 - SN:3270

Calibration Procedure(s)

FD-Z11-2-004-01

Calibration Procedures for Dosimetric E-field Probes

Calibration date:

August 26, 2016

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	27-Jun-16 (CTTL, No.J16X04777)	Jun-17
Power sensor NRP-Z91	101547	27-Jun-16 (CTTL, No.J16X04777)	Jun-17
Power sensor NRP-Z91	101548	27-Jun-16 (CTTL, No.J16X04777)	Jun-17
Reference10dBAttenuato	r   18N50W-10dB	13-Mar-16(CTTL,No.J16X01547)	Mar-18
Reference20dBAttenuato	r 18N50W-20dB	13-Mar-16(CTTL, No.J16X01548)	Mar-18
Reference Probe EX3DV	4 SN 7307	19-Feb-16(SPEAG,No.EX3-7307_Feb16)	Feb-17
DAE4	SN 1331	21-Jan-16(SPEAG, No.DAE4-1331_Jan16)	Jan -17
Secondary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
SignalGeneratorMG3700	4 6201052605	27-Jun-16 (CTTL, No.J16X04776)	Jun-17
Network Analyzer E50710	MY46110673	26-Jan-16 (CTTL, No.J16X00894)	Jan -17
	Name	Function	Signature
Calibrated by:	Yu Zongying	SAR Test Engineer	AM
Reviewed by:	Qi Dianyuan	SAR Project Leader	203/
Approved by:	Lu Bingsong	Deputy Director of the laboratory	Ja wstr
		Issued: August	/ 27, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal A,B,C,D modulation dependent linearization parameters

Polarization  $\Phi$   $\Phi$  rotation around probe axis

Polarization  $\theta$   $\theta$  rotation around an axis that is in the plane normal to probe axis (at measurement center), i

 $\theta$ =0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization  $\theta$ =0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z\* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z:A,B,C are numerical linearization parameters assessed based on the
  data of power sweep for specific modulation signal. The parameters do not depend on frequency nor
  media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z\* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: Z16-97123 Page 2 of 11

# Probe ES3DV3

SN: 3270

Calibrated: August 26, 2016

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

### DASY/EASY – Parameters of Probe: ES3DV3 - SN: 3270

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
$Norm(\mu V/(V/m)^2)^A$	1.09	1.22	1.19	±10.8%
DCP(mV) <sup>B</sup>	100.9	103.3	101.0	

## **Modulation Calibration Parameters**

UID	Communication		Α	В	С	D	VR	Unc
	System Name		dB	dBõV		dB	mV	(k=2)
0	CW	X	0.0	0.0	1.0	0.00	274.7	±2.7%
		Υ	0.0	0.0	1.0		295.4	
		Z	0.0	0.0	1.0		288.4	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

A The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 5 and Page 6).

<sup>&</sup>lt;sup>E</sup> Uncertainly is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

# DASY/EASY - Parameters of Probe: ES3DV3 - SN: 3270

### Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	41.9	0.89	6.19	6.19	6.19	0.50	1.35	±12%
835	41.5	0.90	6.03	6.03	6.03	0.42	1.47	±12%
900	41.5	0.97	6.09	6.09	6.09	0.37	1.61	±12%
1750	40.1	1.37	5.21	5.21	5.21	0.52	1.53	±12%
1900	40.0	1.40	5.08	5.08	5.08	0.55	1.50	±12%
2000	40.0	1.40	4.98	4.98	4.98	0.57	1.47	±12%
2100	39.8	1.49	5.02	5.02	5.02	0.68	1.41	±12%
2450	39.2	1.80	4.51	4.51	4.51	0.73	1.30	±12%
2600	39.0	1.96	4.37	4.37	4.37	0.90	1.13	±12%

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>&</sup>lt;sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>&</sup>lt;sup>G</sup>Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm$  1% for frequencies below 3 GHz and below  $\pm$  2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



## DASY/EASY - Parameters of Probe: ES3DV3 - SN: 3270

### Calibration Parameter Determined in Body Tissue Simulating Media

f [MHz] <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	55.5	0.96	6.09	6.09	6.09	0.50	1.35	±12%
835	55.2	0.97	6.01	6.01	6.01	0.42	1.60	±12%
1750	53.4	1.49	4.95	4.95	4.95	0.50	1.66	±12%
1900	53.3	1.52	4.70	4.70	4.70	0.53	1.64	±12%
2450	52.7	1.95	4.28	4.28	4.28	0.90	1.20	±12%
2600	52.5	2.16	4.12	4.12	4.12	0.90	1.18	±12%

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


<sup>&</sup>lt;sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>&</sup>lt;sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm$  1% for frequencies below 3 GHz and below  $\pm$  2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



# Frequency Response of E-Field


(TEM-Cell: ifi110 EXX, Waveguide: R22)

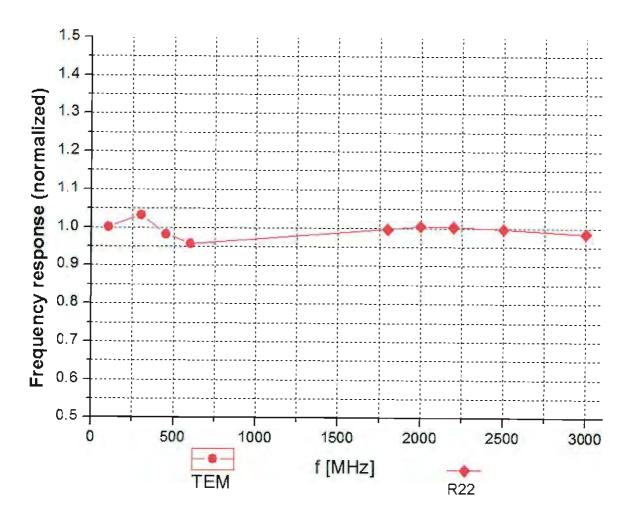

Uncertainty of Frequency Response of E-field: ±7.5% (k=2)




# Receiving Pattern ( $\Phi$ ), $\theta$ =0°

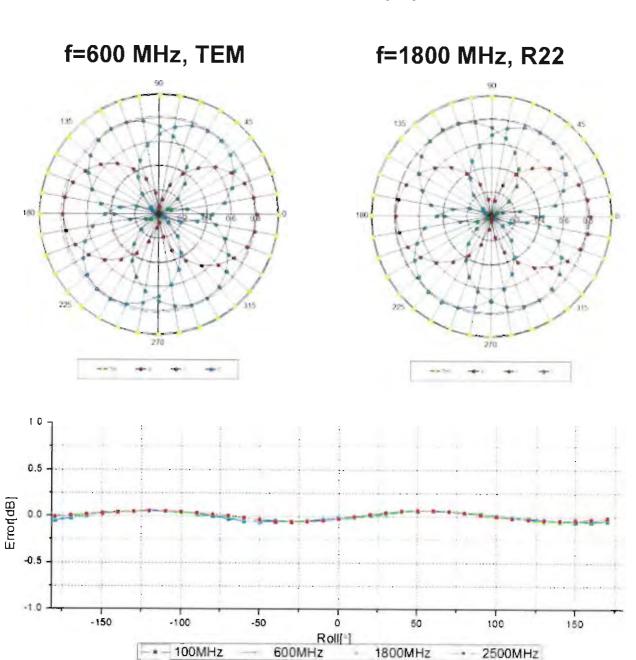

Uncertainty of Axial Isotropy Assessment: ±0.9% (k=2)

Certificate No: Z16-97123 Page 8 of 11

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

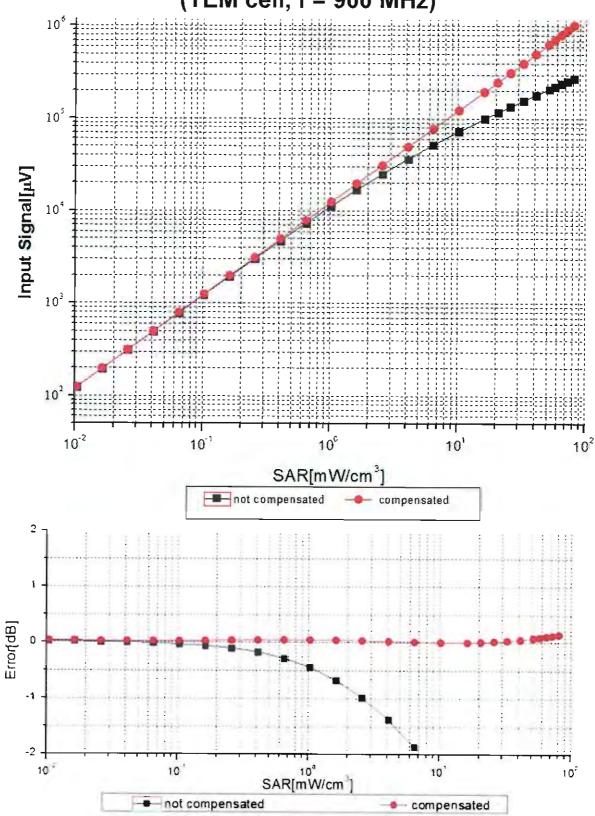


Uncertainty of Linearity Assessment: ±0.9% (k=2)


## **Conversion Factor Assessment**

#### f=900 MHz, WGLS R9(H\_convF)

#### f=1750 MHz, WGLS R22(H\_convF)

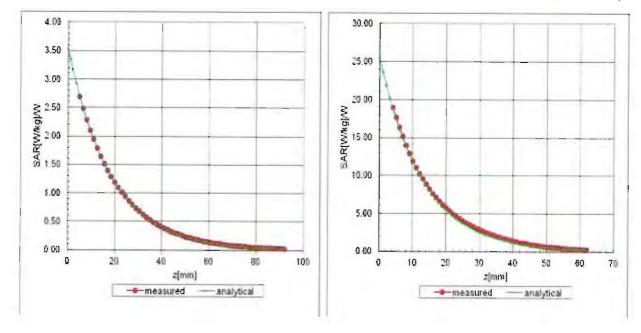


# **Deviation from Isotropy in Liquid**

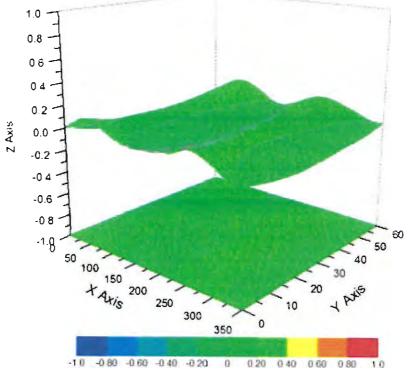

Uncertainty of Spherical Isotropy Assessment: ±2.8% (K=2)

Certificate No: Z16-97123 Page 10 of 11



# DASY/EASY - Parameters of Probe: ES3DV3 - SN: 3270

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	168.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	10mm
Tip Diameter	4mm
Probe Tip to Sensor X Calibration Point	2mm
Probe Tip to Sensor Y Calibration Point	2mm
Probe Tip to Sensor Z Calibration Point	2mm
Recommended Measurement Distance from Surface	3mm

Certificate No: Z16-97123 Page 11 of 11

#### Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

Sporton-TW (Auden)

Certificate No: EX3-3931\_Oct16

#### CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3931

Calibration procedure(s)

QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date:

October 3, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Certificate No: EX3-3931\_Oct16

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: S5277 (20x)	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe ES3DV2	SN: 3013	31-Dec-15 (No. ES3-3013_Dec15)	Dec-16
DAE4	SN: 660	23-Dec-15 (No. DAE4-660_Dec15)	Dec-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr~16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Name Function Signature

Calibrated by: Michael Weber Laboratory Technician

Approved by: Katja Pokovic Technical Manager

Issued: October 4, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

#### Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL NORMx,y,z tissue simulating liquid sensitivity in free space

ConvF DCP sensitivity in TSL / NORMx,y,z diode compression point

CF A, B, C, D crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization φ

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Connector Angle

information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- Techniques", June 2013
  b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

# Probe EX3DV4

SN:3931

Manufactured:

July 24, 2013

Repaired:

September 27, 2016

Calibrated:

October 3, 2016

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

October 3, 2016

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3931

**Basic Calibration Parameters** 

			Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	0.50	0.56	0.47	± 10.1 %
DCP (mV) <sup>B</sup>	99.3	102.3	99.2	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>⊨</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	165.2	±2.2 %
		Y	0.0	0.0	1.0		169.6	
		Z.	0.0	0.0	1.0		158.4	

Note: For details on UID parameters see Appendix.

**Sensor Model Parameters** 

	C1 fF	C2 fF	α V-1	T1 ms.V <sup>-2</sup>	T2 ms.V <sup>-1</sup>	T3 ms	T4 V <sup>-2</sup>	T5 V <sup>-1</sup>	T6
X	39.73	299.4	36.38	13.81	1.099	5.004	0.119	0.351	1.005
Υ	59.82	447.7	35.85	21.83	1.546	5.045	0.719	0.472	1.007
Z	54.23	405.8	35.74	19.34	1.491	5.007	0.433	0.514	1.00 <u>5</u>

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

A The uncertainties of Norm X,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3931

#### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.9	0.89	10.68	10.68	10.68	0.47	0.86	± 12.0 %
835	41.5	0.90	10.35	10.35	10.35	0.43	0.80	± 12.0 %
900	41.5	0.97	10.09	10.09	10.09	0.44	0.86	± 12.0 %
1450	40.5	1.20	8.73	8.73	8.73	0.45	0.80	± 12.0 %
1750	40.1	1.37	8.68	8.68	8.68_	0.37	0. <u>8</u> 0	± 12.0 %
1900	40.0	1.40	8.42	8.42	8.42_	0.34	0.80	± 12.0 %
2000	40.0	1.40	8.43	8.43	8.43	0.37	0.80	± 12.0 %
2300	39.5	1.67	7.94	7.94	7.94	0.28	0.86	± 12.0 %
2450	39.2	1.80	7.60	7.60	7 <u>.</u> 60	0.36	0.84	± 12.0 %
2600	39.0	1.96	7.37	7.37	7.37	0.31	0.97	± 12.0 %
5250	35.9	4,71	5.38	5.38	5.38	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.68	4.68	4.68	0.40	1.80	± 13.1 %
5750	35.4	5.22	4.84	4.84	4.84	0.40	1.80	± 13.1 %

<sup>&</sup>lt;sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

Validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>6</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3931

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	55.5	0.96	10.37	10.37	10.37	0.38	0.97	± 12.0 %
835	55.2	0.97	10.14	10.14	10.14	0.36	0.99	± 12.0 %
1450	54.0	1.30	8.53	8.53	8. <u>5</u> 3	0.31	0.80	± 12.0 %
1750	53. <u>4</u>	1.49	8.45	8.45	8. <u>4</u> 5	0.37	0.80	± 12.0 %
1900	53.3	1.52	8.1 <u>4</u>	8.14	8.14	0.33	0.90	± 12.0 %
2300	52.9	1.81	7.96	7.96	7.96	0.39	0.80	± 12.0 %
2450	52.7	1.95	7.73	7.73	7.73	0.38	0.85	± 12.0 %
2600	52.5	2.16	7.46	7.46	7.46	0.25	0.95	± 12.0 %
5250	48.9	5.3 <u>6</u>	4.57	4.57	4.57	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.71	3.71	3.71	0.60	1.90	± 13.1 %
5750	48.3	5.94	4.01	4.01	4.01	0.60	1.90	± 13.1 %

<sup>&</sup>lt;sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConyE uncertainty for indicated target tissue parameters

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


October 3, 2016 EX3DV4-SN:3931


# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

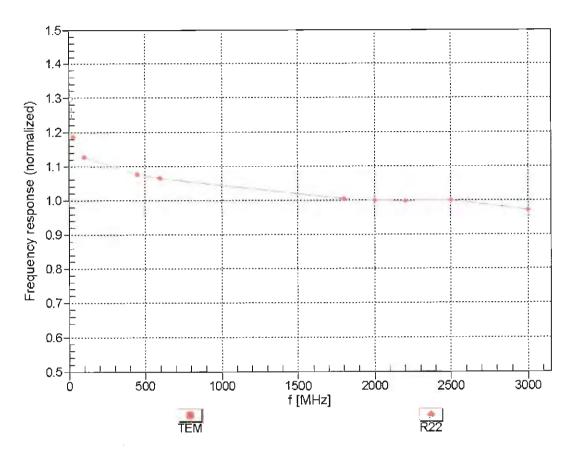

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

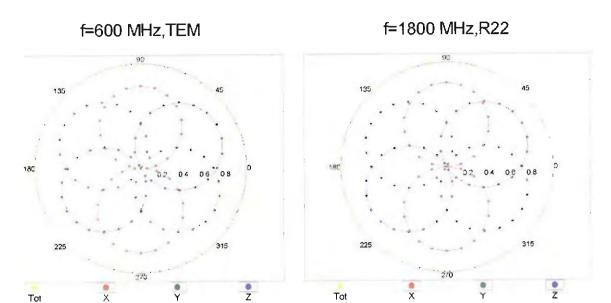


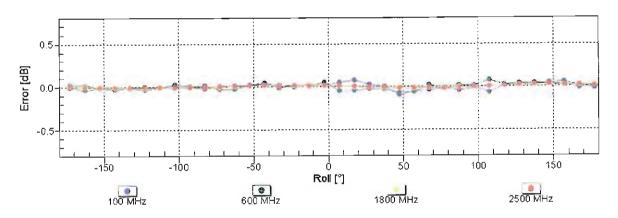

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

## Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

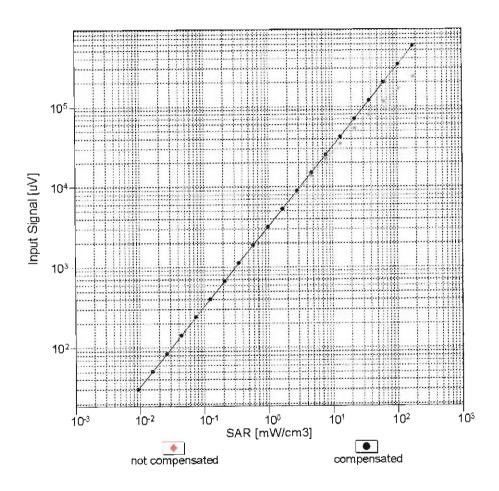


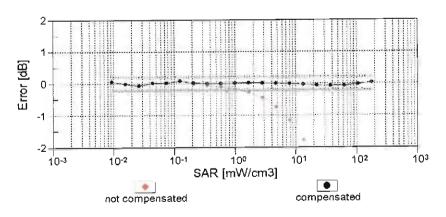

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


October 3, 2016

# **Conversion Factor Assessment**

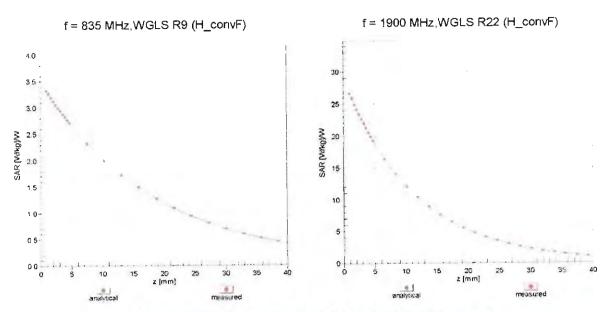

# Deviation from Isotropy in Liquid

Error  $(\phi, \theta)$ , f = 900 MHz

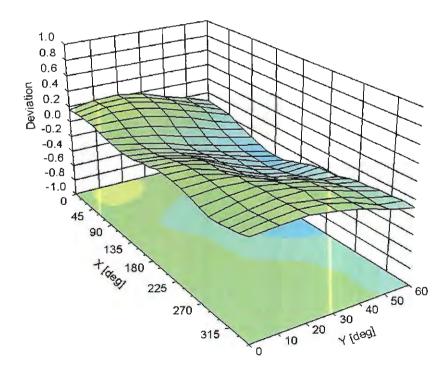

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3931

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	127.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

**Appendix: Modulation Calibration Parameters** 

UID	ix: Modulation Calibration Paral Communication System Name		A dB	B dBõV	С	D dB	VR mV	Max Unc <sup>E</sup> (k=2)
0	CW	Х	0.00	0.00	1.00	0.00	165.2	± 2.2 %
		Υ	0.00	0.00	1.00		169.6	
10010-	CAD Validation (Causes 100ms 10ms)	Z	0.00 3.48	0.00 69.31	1.00 12.63	10.00	158.4 20.0	± 9.6 %
CAA	SAR Validation (Square, 100ms, 10ms)	^	3.40	09.31	12.03	10.00	20.0	± 9.0 %
0/11		Υ	5.87	75.87	16.27		20.0	
		Z	4.02	70.66	13.78		20.0	
10011- CAB	UMTS-FDD (WCDMA)	X	1.30	72.39	18.20	0.00	150.0	± 9.6 %
	<del></del>	Y	1.19 1.01	69.63 66.38	16.77 14.76		150.0 150.0	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	1.24	65.29	16.42	0.41	150.0	± 9.6 %
<del></del>		Υ	1.26	64.91	16.05		150.0	
		Z	1.20	63.67	14.96		150.0	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps)	X	4.82	66.95	17.27	1.46	150.0	± 9.6 %
	_	Y	5.04	66.77	17.23		150.0 150.0	
10021- DAB	GSM-FDD (TDMA, GMSK)	X	4.95 100.00	66.50 114.09	16.90 27.93	9.39	50.0	± 9.6 %
D/ (D		Υ	100.00	118.26	30.54		50.0	
		Z	25.45	96.76	24.27		50.0	
10023- DAB	GPRS-FDD (TDMA, GMSK, TN 0)	X	83.93	111.52	27.32	9.57	50.0	± 9.6 %
	_	Y	99.99	118.26	30.60		50.0 50.0	
10024- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	Z	19.40 100.00	92.86 112.26	23.18 25.94	6.56	60.0	± 9.6 %
DAD		Y	100.00	115.42	28.11		60.0	
		Z	100.00	112.41	26.50		60.0	
10025- DAB	EDGE-FDD (TDMA, 8PSK, TN 0)	Х	5.67	76.70	28.63	12.57	50.0	± 9.6 %
	_	Y	15.06	105.00	40.92 27.63		50.0 50.0	
10026- DAB	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	5.92 9.71	75.84 91.87	32.18	9.56	60.0	± 9.6 %
D) 10	-	Y	18.06	104.69	36.55		60.0	
		Z	11.21	92.21	31. <u>5</u> 5		60.0	
10027- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	Х	100.00	112.68	25.31	4.80	80.0	± 9.6 %
		Z	100.00 100.00	114.88	27.06 25.19		80.0 80.0	
10028- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	100.00	111.26 114.77	25.19	3.55	100.0	± 9.6 %
טייט	<del></del>	Y	100.00	115.72	26.71		100.0	
		Z	100.00	111.32	24.54		100.0	
10029- DAB	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	6.19	82.03	27.36	7.80	80.0	± 9.6 %
		Y	10.55	92.05	31.00		80.0	
10030- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	X	7,5 <u>3</u> 100.00	83.82 110.56	27.35 24.66	5.30	70.0	± 9.6 %
U/V1	<del>                                     </del>	Y	100.00	113.96	26.95		70.0	
		Z	100.00	110.53	25.16		70.0	
10031- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	X	100.00	116.75	24.95	1.88	100.0	± 9.6 %
		Y	100.00	117.62	26.11		100.0	
		Z	100.00	110.75	23.01	<u> </u>	100.0	L

10032-	IEEE 802.15.1 Bluetooth (GFSK, DH5)	Х	100.00	131.18	29.75	1.17	100.0	± 9.6 %
CAA			100.00	405.00	00.00		100.0	
		Y	100.00	125.29	28.26 23.87		100.0	
		Z	100.00	114.95	23.87	5.30	70.0	± 9.6 %
10033- CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)	Х	10.93	90.53		5.30		
*		Υ_	20.55	101.44	27.99		70.0	
		Z	7.67	84.45	21.88		70.0	
10034- CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	Х	5.70	84.58	20.06	1.88	100.0	± 9.6 %
O/M	B1107	Υ	5.85	85.75	22.03		100.0	
		Z	2.95	74.86	17.34		100.0	
10035- CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH5)	Χ	3.92	81.20	18.80	1.17	100.0	± 9.6 %
<u> </u>		Υ	3.48	79.72	19.80		100.0	
		Z	2.10	71.76	15.97		100.0	
10036- CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	X	15.13	95.54	24.90	5.30	70.0	± 9.6 %
0,01		Υ	28.86	107.18	29.66		70.0	
		Z	9.07	87.21	22.88		70.0	
10037- CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	X	4.82	82.50	19.36	1.88	100.0	± 9.6 %
<u> </u>		Ŷ	5.58	85.13	21.78		100.0	
		Z	2.82	74.36	17.11		100.0	
10038- CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	X	4.08	82.09	19.24	1.17	100.0	± 9.6 %
<u> </u>		Y	3.57	80.38	20.14		100.0	
		Z	2.12	72.10	16.20		100.0	
10039- CAB	CDMA2000 (1xRTT, RC1)	X	5.80	88.31	21.06	0.00	150.0	± 9.6 %
CAD	<del></del>	Υ	2.44	75.65	18.16		150.0	
	<del></del>	Z	1.80	71.10	15.73		150.0	
10042- CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4- DQPSK, Halfrate)	X	100.00	110.27	25.32	7.78	50.0	± 9.6 %
CAD	DQF3K, Hallfate)	Y	100.00	114.03	27.70		50.0	
		Ż	32.06	97.64	22.93		50.0	
10044-	IS-91/EIA/TIA-553 FDD (FDMA, FM)	X	0.00	105.67	0.52	0.00	150.0	± 9.6 %
CAA		Y	0.00	101.10	0.34		150.0	
		Z	0.00	94.56	3.16		150.0	_
10048-	DECT (TDD, TDMA/FDM, GFSK, Full	X	11.94	82.95	20.71	13.80	25.0	± 9.6 %
CAA_	Slot, 24)	Y	15.06	89.64	24.59		25.0	
		Z	9.78	81.31	21.11	-	25.0	
10049-	DECT (TDD, TDMA/FDM, GFSK, Double	X	15.54	88.48	21.39	10.79	40.0	± 9.6 %
CAA	Slot, 12)	Y	23.79	97.14	25.51		40.0	
		Z	11.46	84.91	21.03		40.0	
10056-	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	13.32	89.14	23.36	9.03	50.0	± 9.6 %
CAA		Y	16.34	93.59	26.16		50.0	
		Ż	10.18	84.57	22.45		50.0	
10059	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	4.78	77.20	24.69	6.55	100.0	± 9.6 %
10058- DAB	EDGE-FDD (1DWA, 0F3K, 114 0-1-2-3)	Y	7.46	84.92	27.60		100.0	_
		Z	5.76	78.94	24.73	1	100.0	
10059-	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2	X	1.30	66.67	17.10	0.61	110.0	± 9.6 %
CAB	Mbps)	Υ	1.37	66.65	16.91	1	110.0	
		Z	1.27	64.87	15.53	1	110.0	
10060-	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5	X	100.00	139.37	36.42	1.30	110.0	± 9.6 %
CAB	Mbps)	Y	100.00	134.75	34.85		110.0	
		Z	5.80	90.90	23.07		110.0	
		1 4	<u> </u>	30.30	1. 20.01	1		<del></del>

	_							
10061- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	X	4.16	86.26	24.31	2.04	110.0	±9.6 %
		Y	6.78	92.08	26.03		110.0	
		Z	3.18	78.55	20.67		110.0	
10062- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	Х	4.62	66.99	16.77	0.49	100.0	± 9.6 %
		Y	4.83	66.75	16.66		100.0	
		Z	4.75	66.51	16.38		100.0	
10063- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	X	4.64	67.08	16.86	0.72	100.0	± 9.6 %
	- 15.27	Y	4.86	66.87	16.78		100.0	
		Z	4.77	66.60	16.47		100.0	
10064- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	Х	4.89	67.27	17.04	0.86	100.0	± 9.6 %
		Y	5.19	67.18	17.02		100.0	
		Z	5.08	66.89	16.71		100.0	
10065- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	X	4.77	67.14	17.11	1.21	100.0	± 9.6 %
		Y	5.06	67.12	17.13		100.0	
		Z	4.94	66.80	16.79		100.0	
10066- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	Х	4.78	67.15	17.25	1.46	100.0	± 9.6 %
		Y	5.09	67.18	17.31		100.0	
		Z	4.97	66.83	16.94		100.0	
10067- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	X	5.07	67.35	17.68	2.04	100.0	±9.6 %
		Y	5.38	67.26	17.72		100.0	
		Z	5.26	66.92	17.34		100.0	
10068- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps)	X	5.11	67.30	17.84	2.55	100.0	± 9.6 %
		Y	5.48	67.51	18.02		100.0	
		Z	5.34	67.10	17.60		100.0	
10069- CAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	Х	5.18	67.33	18.03	2.67	100.0	± 9.6 %
<u> </u>	,spoy	Y	5.55	67.43	18.19		100.0	
		Z	5.42	67.05	17.77		100.0	
10071- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	4.92	67.02	17.54	1.99	100.0	± 9.6 %
	, , , , , , , , , , , , , , , , , , , ,	Y	5.15	66.91	17.55		100.0	
		Z	5.05	66.61	17.20		100.0	
10072- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	Х	4.89	67.32	17.73	2.30	100.0	± 9.6 %
		Y	5.18	67.36	17.81		100.0	
		Z	5.06	66.97	17.41		100.0	
10073- ÇAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	X	4.97	67.51	18.05	2.83	100.0	± 9.6 %
		Y	5.26	67.57	18.16		100.0	
		Z	5.13	67.15	17.71		100.0	
10074- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	X	4.97	67.45	18.19	3.30	100.0	± 9.6 %
		Y	5.25	67.52	18.35		100.0	
		Z	5.12	67.08	17.88		100.0	
10075- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	X	5.01	67.53	18.46	3.82	90.0	±9.6 %
		Υ	5.35	67.85	18.77		90.0	
		Z	5.20	67.32	18.23		90.0	<del></del>
10076- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	Х	5.05	67.39	18.61	4.15	90.0	± 9.6 %
		Υ	5.33	67 <i>.</i> 57	18.84		90.0	
		Z	5.20	67.09	18.32		90.0	
10077-	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	X	5.08	67.49	18.72	4.30	90.0	± 9.6 %
LOAB								
CAB	(Beceret Bill, et illege)	Y	5.35	67.63	18.93		90.0	

10081-	CDMA2000 (1xRTT, RC3)	X	1.31	72.98	15.39	0.00	150.0	± 9.6 %
CAB		Y	1.11	69.20	15.13		150.0	
		Z	0.87	65.58	12.79		150.0	
10082- CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4- DQPSK, Fullrate)	X	0.85	60.00	5.02	4.77	80.0	± 9.6 %
JAD	DQF3N, 1 dillate)	Y	1.21	60.81	6.24		80.0	
		Z	1.05	60.00	5.50		80.0	
10090- DAB	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	100.00	112.28	25.96	6.56	60.0	± 9.6 %
		Υ	100.00	115.46	28.15		60.0	
		Z	100.00	112.45	26.54	0.00	60.0	± 9.6 %
10097- CAB	UMTS-FDD (HSDPA)	X	2.10	70.95	17.43	0.00	150.0 150.0	± 9.0 %
		Y	1.95	68.39	16.42 15.42		150.0	
		Z	1.81	67.01 70.93	17.43	0.00	150.0	± 9.6 %
10098- CAB	UMTS-FDD (HSUPA, Subtest 2)	X	2.06		16.41		150.0	20.0 //
		Y	1.91	68.38	15.38		150.0	
		Z	1.77 9.76	66.95 91.94	32.20	9.56	60.0	± 9.6 %
10099- DAB	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X		104.66	36.54	<del></del>	60.0	
		Y	18.08	92.22	31.54	<del></del>	60.0	
	1000/ 55 00	Z	11.25 3.35	72.13	17.90	0.00	150.0	± 9.6 %
10100- CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X		71.55	17.33		150.0	
		Y	3.43 3.14	69.99	16.48		150.0	
10101-	LTE-FDD (SC-FDMA, 100% RB, 20	Z	3.14	68.30	16.59	0.00	150.0	± 9.6 %
CAB	MHz, 16-QAM)	Y	3.42	68.10	16.32		150.0	
		Z	3.28	67.37	15.82		150.0	
10102-	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	3.39	68.25	16.67	0.00	150.0	± 9.6 %
CAB	W112, 04-QAW)	Y	3.51	67.99	16.38		150.0	
<del>.</del>		Ż	3.39	67.35	15.92		150.0	
10103- CAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	Х	6.41	75.89	20.51	3.98	65.0	± 9.6 %
0,10		Υ	7.77	77.49	21.00		65.0	
		Z	6.54	74.47	19.52		65.0	
10104- CAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	6.38	73.95	20.45	3.98	65.0	± 9.6 %
		Υ	7.62	75.73	21.18		65.0	
		Z	6.97	74.03	20.17		65.0	0.00
10105- CAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	Х	5.88	72.23	19.98	3.98	65.0	± 9.6 %
		Υ	7.31	74.91	21.13		65.0	
		Z	6.85	73.64	20.32	0.00	65.0	± 9.6 %
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	Х	2.91	71.53	17.82	0.00	150.0	19.0 %
		Y	3.02	70.68	17.15		150.0	-
		Z	2.76	69.18	16.29	0.00	150.0 150.0	± 9.6 %
10109- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	Х	2.95	68.44	16.61	0.00	150.0	2 3.0 70
		Y	3.08	67.93	_	<del> </del>	150.0	
10110-	LTE-FDD (SC-FDMA, 100% RB, 5 MHz,	Z X	2.95	67.17 71.08	15.72 17.59	0.00	150.0	± 9.6 %
CAC	QPSK)	Y	2.47	69.75	16.86		150.0	
		$\frac{1}{Z}$	2.25	68.18	15.88	1	150.0	
10111-	LTE-FDD (SC-FDMA, 100% RB, 5 MHz,	X	2.79	70.36	17.30	0.00	150.0	± 9.6 %
CAC	16-QAM)	Y	2.80	68.64	16.65		150.0	

							1	
10112- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	×	3.07	68.42	16.64	0.00	150.0	± 9.6 %
ψ, το		Υ	3.20	67.83	16.29		150.0	
		Z	3.07	67.16	15.79		150.0	
10113- CAC	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	2.94	70.45	17.39	0.00	150.0	± 9.6 %
07.10	0.1.00.1111	Υ	2.95	68.67	16.72		150.0	
		Z	2.81	67.97	16.15		150.0	
10114- CAB	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	5.09	67.47	16.77	0.00	150.0	± 9.6 %
OVD.	(Nibps, Bi Sit)	Υ	5.23	67.24	16.53		150.0	
		Ż	5.18	67.08	16.35		150.0	
10115- CAB	IEEE 802.11n (HT Greenfield, 81 Mbps, 16-QAM)	X	5.34	67.51	16.78	0.00	150.0	± 9.6 %
		Υ	5.60	67.53	16.67		150.0	
		Z	5.52	67.36	16.50		150.0	
10116- CAB	IEEE 802.11n (HT Greenfield, 135 Mbps, 64-QAM)	X	5.18	67.67	16.79	0.00	150.0	± 9.6 %
		Υ	5.36	67.51	16.58		150.0	
		Z	5.29	67.32	16.39		150.0	
10117- CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	5.07	67.38	16.74	0.00	150.0	± 9.6 %
		Υ	5.24	67.25	16.55		150.0	
		Z	5.16	67.03	16.34		150.0	
10118- CAB	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	Х	5.42	67.71	16.89	0.00	150.0	± 9.6 %
		Y	5.67	67.69	16.76		150.0	
		Z	5.59	67.53	16.59		150.0	
10119- CAB	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	Х	5.17	67.64	16.79	0.00	150.0	± 9.6 %
07.12	_	Y	5.33	67.45	16.57		150.0	
		Z	5.26	67.25	16.37		150.0	
10140- CAB	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	Х	3.41	68.25	16.57	0.00	150.0	± 9.6 %
0.12	111112, 10 00 000	Υ	3.56	67.99	16.30		150.0	
	-	Z	3.43	67.35	15.84		150.0	
10141- CAB	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	3.54	68.37	16.75	0.00	150.0	± 9.6 %
0710	111112, 3 1 32 1117	Υ	3.68	68.01	16.43		150.0	
	-	Ż	3.56	67.45	16.01		150.0	
10142~ CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	2.25	71.96	17.48	0.00	150.0	± 9.6 %
0.10		Υ	2.26	69.83	16.74		150.0	•
		Z	2.02	68.09	15.61		150.0	
10143- CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	Х	2.82	72.22	17.26	0.00	150.0	± 9.6 %
		Υ	2.71	69.55	16.65		150.0	
		Ζ	2.52	68.51	15.83		150.0	
10144- CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	Х	2.29	68.06	14.75	0.00	150.0	± 9.6 %
		Y	2.50	67.47	15.19		150.0	
		Z	2.32	66.44	14.34		150.0	
10145- CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	1.16	65.56	11.35	0.00	150.0	±9.6 %
		Υ	1.65	68.53	14.65		150.0	
		Z	1.36	65.83	12.76		150.0	
10146- CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	1.35	63.40	9.39	0.00	150.0	± 9.6 %
		Υ	3.12	72.00	15.52		150.0	
		Z	2.16	67.04	12.61		150.0	
10147- CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	1.53	64.72	10.19	0.00	150.0	± 9.6 %
		1	4.00	75.00	17.18		150.0	
		Υ	4.03	75.63	17.10		150.0	

10149-	LTE-FDD (SC-FDMA, 50% RB, 20 MHz,	Х	2.96	68.52	16.66	0.00	150.0	± 9.6 %
CAB	16-QAM)	Υ	3.09	67.99	16.32		150.0	
		ż	2.96	67.23	15.77		150.0	
10150- CAB	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	3.08	68.50	16.69	0.00	150.0	± 9.6 %
CAD	04 30 (IVI)	Y	3.21	67.88	16.33		150.0	
		Z	3.08	67.21	15.83		150.0	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	7.03	79.10	21.82	3.98	65.0	± 9.6 %
CAD	QFSK)	Υ	8.21	79.75	22.00		65.0	
	-	Z	7.10	77.15	20.67	_	65.0	_
10152- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	5.92	73.94	20.06	3.98	65.0	± 9.6 %
		Υ	7.21	75.88	21.03		65.0	
		Z	6.48	73.87	19.84		65.0	
10153- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	6.35	75.11	20.94	3.98	65.0	± 9.6 %
		Y	7.55	76.62	21.69		65.0	
		Z	6.87	74.79	20.60		65.0	
10154- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	2.46	71.67	17.92	0.00	150.0	± 9.6 %
		Υ	2.54	70.24	17.15		150.0	
		Ζ	2.30	68.63	16.17		150.0	
10155- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	Х	2.79	70.40	17.33	0.00	150.0	± 9.6 %
	-	Y	2.80	68.64	16.65		150.0	
		Z.	2.66	67.83	16.02		150.0	
10156- CAC	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	Х	2.17	72.73	17.45	0.00	150.0	± 9.6 %
0,10	QI OIT	Υ	2.14	70.24	16.79		150.0	
		Z	1.88	68.21	15.48		150.0	
10157- CAC	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	2.21	69.24	14.98	0.00	150.0	± 9.6 %
CAC	10-QAIN)	Υ	2.36	68.31	15.46		150.0	
		Z	2.15	66.99	14.43		150.0	
10158- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	2.95	70.56	17.46	0.00	150.0	± 9.6 %
070	<u> </u>	Y	2.95	68.72	16.76		150.0	
	-	Z	2.82	68.03	16.20		150.0	
10159- CAC	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	2.36	69.87	15.32	0.00	150.0	± 9.6 %
0/10	04 00 1111)	Υ	2.49	68.78	15.76		150.0	
		Z	2.27	67.50	14.75		150.0	
10160- CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	2.90	70.47	17.47	0.00	150.0	± 9.6 %
		Υ	2.94	69.28	16.77		150.0	
		Z	2.76	68.21	16.07		150.0	
10161- CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	Х	2.98	68.55	16.64	0.00	150.0	± 9.6 %
2, ,_		Υ	3.10	67.79	16.29		150.0	
		Z	2.98	67.13	15.77		150.0	
10162- CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	Х	3.10	68.74	16.76	0.00	150.0	± 9.6 %
J. 12		Y	3.21	67.84	16.35		150.0	
		Z	3.09	67.25	15.86		150.0	
10166- CAC	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	Х	3.31	69.42	19.40	3.01	150.0	± 9.6 %
		Y	3.85	69.94	19.41		150.0	
		Z	3.63	68.92	18.65		150.0	
10167-	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	3.89	72.11	19.78	3.01	150.0	± 9.6 %
LAL					_			
CAC	10 00 111)	Y	4.89	73.20	20.04		150.0	

10168-	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz,	Х	4.43	75.02	21.48	3.01	150.0	± 9.6 %
CAC	64-QAM)							
		Y	5.37	75.20	21.21		150.0	
		Z	4.92	73.76	20.36		150.0	
10169- CAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	2.61	67.65	18.68	3.01	150.0	± 9.6 %
		Y	3.41	71.01	19.90		150.0	
		Z	3.09	68.90	18.61		150.0	
10170- CAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	3.32	73.16	21.10	3.01	150.0	± 9.6 %
		Y	5.09	78.14	22.55		150.0	
		Z	4.27	74.69	20.88		150.0	
10171- AAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	Х	2.74	69.02	18.13	3.01	150.0	± 9.6 %
		Υ	4.10	73.53	19.72		150.0	
		Z	3.48	70.44	18.07		150.0	
10172- CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	5.53	83.56	25.72	6.02	65.0	± 9.6 %
		Y	21.34	105.31	32.41		65.0	
		Z	7.30	84.26	24.94		65.0	
10173- CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	10.58	92.60	26.95	6.02	65.0	± 9.6 %
		Υ	29.30	105.74	30.57		65.0	
		Z	12.37	90.08	25.23		65.0	
10174- CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	7.41	85.53	24.05	6.02	65.0	± 9.6 %
		Y	21.20	98.69	27.99		65.0	
		Z	10.53	86.42	23.55		65.0	
10175- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	Х	2.58	67.36	18.42	3.01	150.0	± 9.6 %
		Υ	3.37	70.66	19.64		150.0	
		Z	3.05	68.56	18.35		150.0	
10176- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	3.33	73.19	21.11	3.01	150.0	± 9.6 %
		Υ	5.10	78.16	22.56		150.0	
		Z	4.27	74.71	20.89		150.0	
10177- CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	2.60	67.50	18.51	3.01	150.0	± 9.6 %
	_	Υ	3.40	70.83	19.75		150.0	
		Z	3.07	68.74	18.46		150.0	
10178- CAC	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	Х	3.30	73.00	21.00	3.01	150.0	± 9.6 %
		Υ	5.02	77.85	22.40		150.0	
		Z	4.22	74.44	20.74		150.0	
10179- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	Х	3.00	71.00	19.50	3.01	150.0	± 9.6 %
		Υ	4.55	75.67	20.98		150.0	
		Z	3.82	72.37	19.31		150.0	
10180- CAC	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	2.73	68.97	18.09	3.01	150.0	± 9.6 %
		Υ	4.08	73.43	19.65		150.0	
		Z	3.47	70.35	18.01		150.0	
10181- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	2.59	67.48	18.51	3.01	150.0	± 9.6 %
		Y	3.39	70.81	19.74		150.0	
		Z	3.07	68.71	18.45		150.0	
10182- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	Х	3.30	72.98	20.99	3.01	150.0	± 9.6 %
***		Υ	5.01	77.82	22.39		150.0	
		Z	4.21	74.41	20.73		150.0	
10183- AAA	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	Х	2.73	68.94	18.08	3.01	150.0	±9.6%
	,	Y	4.07	73.40	19.64		150.0	
		Z	3.46	70.33	18.00	1	150.0	1

October 3, 2016

10184- CAC	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	2.60	67.52	18.53	3.01	150.0	± 9.6 %
	St 010	Υ	3.40	70.86	19.76		150.0	
		Z	3.08	68.76	18.47		150.0	
10185- CAC	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	Х	3.31	73.05	21.03	3.01	150.0	± 9.6 %
JAC	GA(IVI)	Y	5.04	77.90	22.43		150.0	
		Z	4.23	74.49	20.77		150.0	
10186-	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-	X	2.74	69.01	18.12	3.01	150.0	± 9.6 %
AAC	QAM)	Y	4.10	73.47	19.68		150.0	
		Z	3.48	70.39	18.03	_	150.0	
10187- CAC	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	2.61	67.58	18.60	3.01	150.0	± 9.6 %
<u> </u>		Y	3.41	70.90	19.81		150.0	
		Z	3.09	68.80	18.52		150.0	
10188- CAC	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	3.41	73.70	21.42	3.01	150.0	± 9.6 %
OAO	10 38 (11)	Υ	5.24	78.69	22.84		150.0	
	<del></del>	Z	4.38	75.22	21.18		150.0	
10189- AAC	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	Х	2.80	69.41	18.40	3.01	150.0	± 9.6 %
. • . •		Y	4.20	73.97	19.98		150.0	
		Z	3.56	70.83	18.32		150.0	
10193- CAB	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	4.49	67.07	16.51	0.00	150.0	±9.6%
CAD	BI CITY	Υ	4.67	66.69	16.32		150.0	
-		Z	4.59	66.49	16.09		150.0	
10194- CAB	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	Х	4.64	67.34	16.63	0.00	150.0	± 9.6 %
CAD	TO-GO-TIVI)	Υ	4.86	67.05	16.43		150.0	
		Z	4.77	66.83	16.21		150.0	
10195- CAB	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	X	4.68	67.36	16.65	0.00	150.0	± 9.6 %
CAD	04-Q/NVI)	Υ	4.90	67.06	16.44		150.0	
	<del>-</del>	Z	4.82	66.86	16.22		150.0	
10196- CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	4.48	67.10	16.51	0.00	150.0	± 9.6 %
CVD	Br GR)	Υ	4.68	66.78	16.36		150.0	
		Z	4.60	66.57	16.12		150.0	
10197- CAB	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	X	4.66	67.35	16.64	0.00	150.0	± 9.6 %
ŲΛυ.	SQ 1191)	Υ	4.88	67.07	16.45		150.0	
	<del></del>	Z	4.79	66.86	16.22		150.0	
10198- CAB	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	X	4.68	67.37	16.65	0.00	150.0	± 9.6 %
J. LD		Υ	4.91	67.08	16.45		150.0	
		Z	4.82	66.87	16.23		150.0	-
10219- CAB	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	4.44	67.14	16.49	0.00	150.0	± 9.6 %
0,10		Υ	4.63	66.80	16.32		150.0	
		Z	4.55	66.58	16.08		150.0	
10220- CAB	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	X	4.65	67.31	16.63	0.00	150.0	± 9.6 %
J, 10		Υ	4.87	67.06	16.44		150.0	
		Z	4.79	66.83	16.21		150.0	
10221- CAB	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	Х	4.69	67.30	16.64	0.00	150.0	± 9.6 %
UNU		Y	4.91	67.01	16.44		150.0	
		Z	4.83	66.81	16.22		150.0	
10222- CAB	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	5.04	67.37	16.73	0.00	150.0	± 9.6 %
UMU	51 010	+	5.00	07.07	10.55	1	150.0	
		Y	5.22	67.27	16.55		100.0	

10223- CAB	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	Х	5.33	67.57	16.84	0.00	150.0	± 9.6 %
		Υ	5.58	67.57	16.72		150.0	
		Z	5.46	67.24	16.46		150.0	
10224- CAB	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	Х	5.08	67.48	16.71	0.00	150.0	±9.6 %
		Υ	5.27	67.38	16.53		150.0	
		Z	5.19	67.14	16.31		150.0	
10225- CAB	UMTS-FDD (HSPA+)	Х	2.82	67.14	15.84	0.00	150.0	± 9.6 %
		Υ	2.95	66.38	15.78		150.0	
		Z	2.86	65.91	15.30		150.0	
10226- CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	11.41	94.07	27.52	6.02	65.0	± 9.6 %
		Υ	31.67	107.27	31.09		65.0	
		Ż	13.11	91.16	25.67		65.0	
10227- CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	Х	11.04	92.14	26.24	6.02	65.0	± 9.6 %
		Υ	24.12	100.92	28.72		65.0	
		Z	11.71	88.12	24.16		65.0	
10228- CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	Х	7.63	90.07	28.10	6.02	65.0	± 9.6 %
		Υ	23.55	107.62	33.18		65.0	
		Z	10.51	91.21	27.39		65.0	
10229- CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	10.66	92.71	26.99	6.02	65.0	± 9.6 %
		Y	29.42	105.79	30.60		65.0	
		Z	12.45	90.17	25.27		65.0	
10230- CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	10.25	90.80	25.74	6.02	65.0	± 9.6 %
		Υ	22.68	99.76	28.30		65.0	
		Z	11.15	87.26	23.80		65.0	
10231- CAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	Х	7.27	89.04	27.66	6.02	65.0	± 9.6 %
		Y	22.20	106.36	32.73		65.0	
		Z	10.05	90.30	27.01		65.0	
10232- CAB	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	Х	10.64	92.69	26.99	6.02	65.0	± 9.6 %
		Y	29.42	105.80	30.60		65.0	
		Z	12.43	90.15	25.26		65.0	
10233- CAB	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	Х	10.23	90.76	25.73	6.02	65.0	± 9.6 %
		Y	22.67	99.78	28.30		65.0	
		Z	11.14	87.24	23.80		65.0	
10234- CAB	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	Х	6.99	88.15	27.23	6.02	65.0	± 9.6 %
		Υ	20.93	105.02	32.23		65.0	
		Z	9.64	89.40	26. <u>6</u> 0		65.0	
10235- CAB	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	Х	10.65	92.73	27.00	6.02	65.0	± 9.6 %
		Y	29.50	105.86	30.62		65.0	
		Z	12.44	90.18	25.27		65.0	
10236- CAB	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	10.34	90.92	25.77	6.02	65.0	± 9.6 %
		Υ	22.93	99.94	28.35		65.0	_
		Z	11.22	87.34	23.83		65.0	
10237- CAB	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	7.28	89.10	27.69	6.02	65.0	± 9.6 %
		Υ	22.38	106.55	32.79		65.0	
		Z	10.07	90.36	27.03		65.0	
	<del></del>	X	10.61	92.67	26.98	6.02	65.0	± 9.6 %
10238- CAB	LTE-TDD (SC-FDMA, 1 RB, 15 MHz,	^	10.01	32.01				
10238- CAB	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	Y	29.40	105.80	30.59		65.0	

October 3, 2016

		V	40.40	00.72	25.72	6.02	65.0	± 9.6 %
10239- CAB	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	10.19	90.73	25.12	0.02	05.0	± 3.0 %
CAB	04-QAIVI)	Y	22.65	99.78	28.31		65.0	
		Z	11.11	87.22	23.79		65.0	
		_			27.67	6.02	65.0	± 9.6 %
10240- CAB	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	7.26	89.06		0.02		1 9.0 %
5, (6	<u> </u>	Y	22.30	106.48	32.77		65.0	
		Z	10.04	90.32	27.01		65.0	
	TE TOD (OO FDMA FOR DD 4.4 MUZ	X	7.75	81.08	25.21	6.98	65.0	± 9.6 %
10241- CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)							
		Υ	10.21	83.82	26.43		65.0	ļ <u> —</u>
		Z	8.73	80.32	24.52		65.0	
10242- CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	Х	6.80	78.38	24.02	6.98	65.0	± 9.6 %
CAM	04-Q/\(\text{IVI}\)	Y	9.63	82.52	25.83		65.0	
		Ż	8.38	79.47	24.10		65.0	
	. TE TED (00 EDMA 500) DD 111MUT	X	5.61	75.06	23.46	6.98	65.0	± 9.6 %
10243- CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)					0.50		
		Y	7.74	79.46	25.50		65.0	
		Z	6.88	76.70	23.79		65.0	
10244-	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	4.85	72.20	16.09	3.98	65.0	± 9.6 %
CAB	10-04191)	Y	8.02	78.99	20.43		65.0	
		Z	6.19	74.48	17.94		65.0	-
	LITE TOD (00 FD14 500) 00 0141		4.70	71.53	15.74	3.98	65.0	± 9.6 %
10245- CAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X				3.90		2 3.0 70
		Υ	7.89	78.48	20.19		65.0	
		Ζ	6.13	74.10	17.74		65.0	
10246-	LTE-TDD (SC-FDMA, 50% RB, 3 MHz,	X	5.22	76.54	18.28	3.98	65.0	± 9.6 %
CAB	QPSK)	Y	8.14	82.43	21.79		65.0	
		Z	5.87	76.86	19.08		65.0	
						3 00	65.0	± 9.6 %
10247- CAB	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	4.92	73.01	17.55	3.98		± 9.6 %
		Y	6.62	76.59	20.16		65.0	
		Z	5.63	73.71	18.45		65.0	
10248-	LTE-TDD (SC-FDMA, 50% RB, 5 MHz,	X	4.84	72.32	17.23	3.98	65.0	± 9.6 %
CAB	64-QAM)	Y	6.62	76.08	19.95	-	65.0	
						-	65.0	
		Z	5.66	73.31	18.26	2.00		± 9.6 %
10249- CAB	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	Х	7.10	81.85	21.45	3.98	65.0	±9.0 %
<u> </u>		Y	9.09	84.35	23.13		65.0	
		Z	6.82	79.25	20.73		65.0	
10250-	LTE-TDD (SC-FDMA, 50% RB, 10 MHz,	X	6.14	76.72	21.07	3.98	65.0	± 9.6 %
CAB	16-QAM)	Y	7.40	78.29	22.09		65.0	
		Z	6.54	75.95	20.75		65.0	
10251-	LTE-TDD (SC-FDMA, 50% RB, 10 MHz,	X	5.70	74.17	19.61	3.98	65.0	± 9.6 %
CAB	64-QAM)			70.10	00.01	-	OF O	+
		Y	7.04	76.19	20.94		65.0	
		Z	6.27	74.04	19.64		65.0	
10252-	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	Х	7.47	82.32	22.88	3.98	65.0	± 9.6 %
		Y	8.82	83.02	23.29		65.0	
CAB		Y				1.	65.0	
				79 27	21.49	1	00.0	
10253-	LTE-TDD (SC-FDMA, 50% RB, 15 MHz,	Z	7.18 5.82	79.27 73.49	21.49 19.80	3.98	65.0	± 9.6 %
CAB		Z X	7.18 5.82	73.49	19.80	3.98	65.0	± 9.6 %
10253-	LTE-TDD (SC-FDMA, 50% RB, 15 MHz,	Z X Y	7.18 5.82 6.99	73.49 75.20	19.80 20.79	3.98	65.0 65.0	± 9.6 %
10253-	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	Z   X   Y   Z	7.18 5.82 6.99 6.34	73.49 75.20 73.34	19.80 20.79 19.64		65.0 65.0 65.0	
10253- CAB	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)  LTE-TDD (SC-FDMA, 50% RB, 15 MHz,	Z X Y	7.18 5.82 6.99	73.49 75.20	19.80 20.79	3.98	65.0 65.0	± 9.6 %
10253- CAB	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	Z   X   Y   Z	7.18 5.82 6.99 6.34	73.49 75.20 73.34	19.80 20.79 19.64		65.0 65.0 65.0	

10256-   10257-   10258-   10259-   10259-	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)  LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X Y Z X Y Z X	6.71 7.84 6.83 3.47 6.90 5.11 3.38	78.47 79.18 76.67 67.38	21.74 22.03 20.70 12.72	3.98	65.0 65.0 65.0	± 9.6 %
10257- CAA I 10258- CAA I 10259- I	MHz, 16-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4  MHz, 64-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4	Z X Y Z X	6.83 3.47 6.90 5.11	76.67 67.38 76.38	20.70 12.72	3.98	65.0	± 9.6 %
10257- CAA I 10258- CAA I 10259- I	MHz, 16-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4  MHz, 64-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4	Y Z X Y	3.47 6.90 5.11	67.38 76.38	12.72	3.98		± 9.6 %
10257- CAA I 10258- CAA I 10259- I	MHz, 16-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4  MHz, 64-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4	Y Z X	6.90 5.11	76.38		3.98	65.0	± 9.6 %
10257-   CAA   10258-   CAA   10259-   1	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM) LTE-TDD (SC-FDMA, 100% RB, 1.4	Z X Y	5.11					
10258- CAA I	MHz, 64-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4	Z X Y	5.11		18.57		65.0	
10258- CAA I	MHz, 64-QAM)  LTE-TDD (SC-FDMA, 100% RB, 1.4	X		71.48	15.77		65.0	
10258- I CAA I	LTE-TDD (SC-FDMA, 100% RB, 1.4			66.76	12.32	3.98	65.0	± 9.6 %
10259- I	•		6.74	75.67	18.20		65.0	
10259- I	•	Ζ	5.05	70.99	15.48		65.0	
10259-	MHz, QPSK)	X	3.49	70.18	14.59	3.98	65.0	± 9.6 %
		Υ	6.78	79.22	19.98	***	65.0	
		Z	4.80	73.56	17.06		65.0	
0/10	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	5.42	74.50	18.87	3.98	65.0	± 9.6 %
	10 97 (11)	Y	6.93	77.16	20.83		65.0	
		Z	5.98	74.51	19.26		65.0	1
10260-	LTE-TDD (SC-FDMA, 100% RB, 3 MHz,	X	5.41	74.15	18.72	3.98	65.0	± 9.6 %
I	64-QAM)					J.50	65.0	2 0.0 70
		Y	6.95	76.90	20.74			
		Z	6.03	74.34	19.21	0.00	65.0	
	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	Х	6.87	81.15	21.70	3.98	65.0	± 9.6 %
		Υ	8.53	83.00	22.95		65.0	
		Ζ	6.70	78.62	20.83		65.0	
I	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	6.12	76.64	21.02	3.98	65.0	± 9.6 %
	<u>;                                    </u>	Y	7.39	78.26	22.06		65.0	
	<del></del>	Ζ	6.53	75.90	20.71		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	Х	5.69	74.15	19.60	3.98	65.0	± 9.6 %
		Υ	7.03	76.18	20.94		65.0	
		Z	6.26	74.03	19.63		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	7.38	82.08	22.77	3.98	65.0	± 9.6 %
O/ (D		Y	8.75	82.86	23.22		65.0	
		Z	7.12	79.11	21.41		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	5.92	73.94	20.06	3.98	65.0	± 9.6 %
CAB		Υ	7.20	75.88	21.03		65.0	<del></del>
<del></del>	_	-	6.48	73.87	19.85		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	6.35	75.09	20.93	3.98	65.0	± 9.6 %
3		Υ	7.55	76.61	21.68		65.0	_
		Z	6.86	74.78	20.59		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	7.01	79.05	21.80	3.98	65.0	± 9.6 %
5/15		Y	8.19	79.71	21.98	-	65.0	
		Ż	7.09	77.11	20.65		65.0	_
	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	6.54	73.87	20.51	3.98	65.0	± 9.6 %
UND	10 50 101	Y	7.70	75.41	21.18		65.0	_
	<del></del>	ż	7.12	73.89	20.25		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	6.52	73.47	20.39	3.98	65.0	± 9.6 %
VΛD	Wiliz, 07-00 Wij	Υ	7.63	74.96	21.06		65.0	
-		Z	7.08	73.52	20.16		65.0	
	LTE-TDD (SC-FDMA, 100% RB, 15	X	6.72	76.10	20.81	3.98	65.0	± 9.6 %
CAB	MHz, QPSK)		7 77	76.91	21.02		65.0	<del>                                     </del>
_		Y Z	7.77 7.04	75.13	20.02		65.0	<del>-</del>

10274-	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	Х	2.68	67.93	16.00	0.00	150.0	± 9.6 %
CAB	1160.10/	Y	2.70	66.71	15.69		150.0	
		Z	2.60	66.12	15.13		150.0	
10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	1.86	71.35	17.51	0.00	150.0	± 9.6 %
	1(0.4)	Y	1.79	69.27	16.54		150.0	
		Ż	1.60	67.20	15.22		150.0	
10277- CAA	PHS (QPSK)	X	2.51	62.07	7.69	9.03	50.0	± 9.6 %
		Υ	3.60	65.47	10.92		50.0	
	-	Z	3.21	64.00	9.69		50.0	
10278- CAA	PHS (QPSK, BW 884MHz, Rolloff 0.5)	X	4.14	68.90	13.57	9.03	50.0	± 9.6 %
		Υ	8.03	79.56	19.93		50.0	
		Z	5.72	73.56	16.82		50.0	
10279- CAA	PHS (QPSK, BW 884MHz, Rolloff 0.38)	Х	4.23	69.12	13.72	9.03	50.0	± 9.6 %
		Y	8.23	79.82	20.06		50.0	
		Z	5.85	73.80	16.95		50.0	
10290- AAB	CDMA2000, RC1, SO55, Full Rate	Х	2.16	75.12	16.21	0.00	150.0	± 9.6 %
		Υ	1.91	71.91	16.34		150.0	
		Ζ	1.49	68.32	14.21	_	150.0	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	1.24	72.30	15.09	0.00	150.0	± 9.6 %
		Υ	1.08	68.86	14.96		150.0	
		Z	0.85	65.38	12.66		150.0	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	X	13.33	104.67	25.79	0.00	150.0	±9.6 %
		Υ	1.50	74.81	18.02		150.0	
		Ζ	1.03	68.79	14.75		150.0	
10293- AAB	CDMA2000, RC3, SO3, Full Rate	Х	100.00	135.60	33.89	0.00	150.0	± 9.6 %
		Υ	2.41	82.36	21.43		150.0	
		Z	1.44	73.75	17.42		150.0	
10295- AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	Х	11.05	85.41	22.93	9.03	50.0	± 9.6 %
		Υ	8.87	82.92	23.80		50.0	
		Z	7.57	79.23	21.65		50.0	
10297- AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	Х	2.93	71.67	17.91	0.00	150.0	± 9.6 %
		Υ	3.03	70.79	17.22		150.0	
		Z	2.77	69.28	16.35		150.0	
10298- AAB	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	1.80	70.98	15.29	0.00	150.0	± 9.6 %
		Υ	1.94	70.01	16.02		150.0	
		Ζ	1.64	67.53	14.38		150.0	
10299- AAB	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	Х	2.25	68.93	13.39	0.00	150.0	± 9.6 %
		Υ	3.57	73.44	16. <u>9</u> 0		150.0	
		Z	2.68	69.23	14.47		150.0	
10300- AAB	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	Х	1.52	63.47	9.92	0.00	150.0	± 9.6 %
		Υ	2.60	68.00	13.77		150.0	
		Z	2.12	65.38	11.93	ļ	150.0	
10301- AAA	IEEE 802.16e WiMAX (29:18, 5ms, 10MHz, QPSK, PUSC)	Х	4.73	66.14	17.79	4,17	50.0	±9.6 %
		Υ	5.14	66.14	17. <u>9</u> 8		50.0	
		Z	4.87	65.30	17.38		50.0	
10302- AAA	IEEE 802.16e WIMAX (29:18, 5ms, 10MHz, QPSK, PUSC, 3 CTRL symbols)	Х	5.19	66.64	18.43	4.96	50.0	± 9.6 %
		Υ	5.69	67.11	18.91		50.0	
	<del></del>	Z	5.42	66.20	18.24		50.0	

10303- AAA	IEEE 802.16e WiMAX (31:15, 5ms, 10MHz, 64QAM, PUSC)	X	4.96	66.34	18.27	4.96	50.0	± 9.6 %
		Υ	5.48	66.96	18.88		50.0	
		Z	5.20	65.95	18.14		50.0	
10304- AAA	IEEE 802.16e WiMAX (29:18, 5ms, 10MHz, 64QAM, PUSC)	X	4.76	66.23	17.80	4.17	50.0	± 9.6 %
		Y	5.21	66.54	18.19		50.0	
		Z	4.96	65.68	17.56		50.0	
10305- AAA	IEEE 802.16e WiMAX (31:15, 10ms, 10MHz, 64QAM, PUSC, 15 symbols)	X	4.83	70.07	20.50	6.02	35.0	± 9.6 %
		Υ	5.51	71.60	22.16		35.0	
		Z	4.98	69.23	20.55		35.0	
10306- AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 64QAM, PUSC, 18 symbols)	Х	4.91	68.09	19.77	6.02	35.0	± 9.6 %
		Y	5.42	68.18	20.25		35.0	
		Z	5.11	67.47	19.73		35.0	
10307- AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, PUSC, 18 symbols)	X	4.83	68.37	19.78	6.02	35.0	± 9.6 %
		Y	5.47	69.61	21.06		35.0	
		Z	5.07	67.89	19.81		35.0	
10308- AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, PUSC)	Х	4.84	68.69	19.98	6.02	35.0	± 9.6 %
		Y	5.46	69.92	21.24		35.0	
		Z	5.05	68.12	19.96		35.0	
10309- AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, AMC 2x3, 18 symbols)	Х	4.94	68.23	19.88	6.02	35.0	± 9.6 %
	, , , , , , , , , , , , , , , , , , , ,	Y	5.52	68.51	20.43		35.0	
		Z	5.19	67.72	19.88		35.0	-
10310- AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, AMC 2x3, 18 symbols)	X	4.88	68.25	19.79	6.02	35.0	±9.6%
7001	Towning at only mile and, to symbolic	Y	5.44	69.18	20.91		35.0	-
		Z	5.08	67.61	19.74		35.0	
10311- AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	3.31	70.70	17.41	0.00	150.0	± 9.6 %
7001		Y	3.40	70.05	16.83		150.0	
		Z	3.13	68.65	16.04		150.0	
10313- AAA	iDEN 1:3	X	4.31	74.90	16.96	6.99	70.0	± 9.6 %
, , , ,		Y	5.76	76.90	17.84		70.0	
	-	Z	4.08	72.13	15.67		70.0	
10314- AAA	iDEN 1:6	X	7.33	84.94	23.33	10.00	30.0	± 9.6 %
7001		Ý	7.31	83.11	22.80		30.0	
		Z	4.98	76.71	20.14		30.0	
10315- AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)	X	1.15	65.39	16.53	0.17	150.0	±9.6 %
		Υ	1.15	64.64	15.92		150.0	
		Z	1.10	63.46	14.86		150.0	
10316- AAB	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 96pc duty cycle)	Х	4.52	67.01	16.57	0.17	150.0	± 9.6 %
		Y	4.73	66.76	16.44		150.0	
		Ż	4.65	66.51	16.17		150.0	
10317- AAB	IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	Х	4.52	67.01	16.57	0.17	150.0	± 9.6 %
		Y	4.73	66.76	16. <u>44</u>		150.0	
		Z	4.65	66.51	16.17		150.0	
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	Х	4.62	67.36	16.62	0.00	150.0	± 9.6 %
		Y	4.87	67.12	16.43		150.0	
		Z	4.77	66.88	16.19		150.0	
	1555 000 44 MSE: /40MH= 64 OAM	X	5.32	67.33	16.68	0.00	150.0	± 9.6 %
10401-	IEEE 802.11ac WiFi (40MHz, 64-QAM,	``						
10401- AAC	99pc duty cycle)	Y	5.49	67.16	16.50		150.0	_

10402-	IEEE 802.11ac WiFi (80MHz, 64-QAM,	ΓxΤ	5.60	67.66	16.72	0.00	150.0	± 9.6 %
10402- AAC	99pc duty cycle)	^	0.00	07.00				
		Υ	5.79	67.68	16.60		150.0	
		Z	5.72	67. <u>4</u> 7	16.40		150.0	1000
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	2.16	75.12	16.21	0.00	115.0	± 9.6 %
		Y	1.91	71 <u>.9</u> 1	16.34		115.0	
		Ż	1.49	68.32	14.21		115.0	. 0 0 0/
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	Х	2.16	75.12	16.21	0.00	115.0	± 9.6 %
		Υ	1.91	71.91	16.34		115.0	
		Z	1.49	68.32	14.21	0.00	115.0	1000
10406- AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	100.00	127.59	32.37	0.00	100.0	± 9.6 %
		Υ	100.00	123.98	31.83		100.0	
		Z	14.26	95.15	24.05		100.0	
10410- AAA	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	124.06	30.89	3.23	80.0	± 9.6 %
		Y	100.00	119.95	30.07		80.0	
		Z	11.66	89.63	21.52		80.0	1000
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	1.06	64.51	16.01	0.00	150.0	± 9.6 %
, , ,		Y	1.04	63.51	15.25		150.0	
		Z	1.01	62.60	14.33		150.0	
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	X	4.49	67.08	16.58	0.00	150.0	± 9.6 %
		Y	4.67	66.72	16.37		150.0	
		Z	4.59	66.53	16.14		150.0	
10417- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	Х	4.49	67.08	16.58	0.00	150.0	± 9.6 %
<del>/</del>		Ÿ	4.67	66.72	16.37		150.0	
		Z	4.59	66.53	16.14		150.0	
10418- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps, 99pc duty cycle, Long preambule)	X	4.49	67.30	16.63	0.00	150.0	± 9.6 %
		Y	4.65	66.87	16.37		150.0	
		Ž	4.58	66.67	16.15		150.0	
10419- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps, 99pc duty cycle, Short preambule)	×	4.50	67.22	16.62	0.00	150.0	± 9.6 %
		Υ	4.68	66.82	16.38		150.0	
		Z	4.60	66.63	16.16		150.0	
10422- AAA	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	4.61	67.18	16.61	0.00	150.0	± 9.6 %
		Y	4.80	66.83	16.39		150.0	
		Z	4.73	66.64	16.18		150.0	
10423- AAA	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	X	4.75	67.46	16.71	0.00	150.0	± 9.6 %
,		Υ	5.00	67.20	16.53		150.0	
···		Z	4.91	66.98	16.30		150.0	
10424-	IEEE 802.11n (HT Greenfield, 72.2	X	4.68	67.42	16.69	0.00	150.0	± 9.6 %
AAA	Mbps, 64-QAM)	Y	4.91	67.14	16.49		150.0	
		Z	4.82	66.93	16.27		150.0	
10425- AAA	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	5.29	67.59	16.82	0.00	150.0	± 9.6 %
7001		Υ	5.47	67.41	16.61		150.0	
-		Z	5.41	67.25	16.44		150.0	
10426-	JEEE 000 44 - /UT On and ald 00 Mbps	X	5.31	67.68	16.86	0.00	150.0	± 9.6 %
	IEEE 802.11n (HT Greenfield, 90 Mbps,							
10426- AAA	16-QAM)	Y	5.48	67.44	16.63		150.0	

10427- AAA	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	Х	5.29	67.52	16.78	0.00	150.0	± 9.6 %
7001		Y	5.50	67.46	16.63		150.0	
		Z	5.43	67.26	16.43		150.0	
10430- AAA	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	X	4.63	73.67	19.48	0.00	150.0	± 9.6 %
		Υ	4.38	70.39	18.28		150.0	
	-	Z	4.34	70.59	18.21		150.0	
10431- AAA	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	X	4.15	67.84	16.60	0.00	150.0	± 9.6 %
,,,,,,	_	Υ	4.40	67.31	16.45		150.0	
		Z	4.29	67.04	16.16		150.0	
10432- AAA	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	X	4.45	67.57	16.66	0.00	150.0	±9.6 %
		Υ	4.69	67.19	16.47		150.0	
		Z	4.59	66.95	16.22		150.0	
10433- AAA	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	X	4.70	67.46	16.71	0.00	150.0	± 9.6 %
		Υ	4.93	67.18	16.52		150.0	
		Ζ	4.84	66.96	16. <u>29</u>		150.0	
10434- AAA	W-CDMA (BS Test Model 1, 64 DPCH)	Х	4.94	75.22	19.61	0.00	150.0	± 9.6 %
		Υ	4.49	71. <u>19</u>	18.31		150.0	-
		Z	4.45	71.43	18.22		150.0	
10435- AAA	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	123.75	30.75	3.23	80.0	± 9.6 %
		Υ	100.00	119.75	29.98		80.0	
		Z	11.13	88.92	21.27		80.0	
10447- AAA	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	Х	3.46	68.09	15.85	0.00	150.0	± 9.6 %
		Υ	3.73	67.44	16.02		150.0	
		Z	3.59	67.02	15.56		150.0	
10448- AAA	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1, Clippin 44%)	Х	4.01	67.64	16.48	0.00	150.0	± 9.6 %
, , , , ,		Y	4.23	67.09	16.31		150.0	
		Z	4.12	66.82	16.01		150.0	
10449- AAA	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1, Cliping 44%)	X	4.28	67.42	16.58	0.00	150.0	± 9.6 %
7001	Supring 11707	Y	4.48	67.02	16.38		150.0	
		Ż	4.39	66.78	16.12		150.0	
10450- AAA	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.48	67.25	16.58	0.00	150.0	± 9.6 %
7001	Chipping 7 1707	Y	4.66	66.95	16.38		150.0	
		Z	4.58	66.72	16.14		150.0	
10451- AAA	W-CDMA (BS Test Model 1, 64 DPCH, Clipping 44%)	X	3.33	68.18	15.32	0.00	150.0	± 9.6 %
		Y	3.67	67.76	15.79		150.0	
		Z	3.50	67.23	15.24		150.0	
10456- AAA	IEEE 802.11ac WiFi (160MHz, 64-QAM, 99pc duty cycle)	Х	6.23	68.21	17.00	0.00	150.0	± 9.6 %
		Y	6.33	68.03	16.78		150.0	
		Z	6.26	67.85	16.61		150.0	
10457- AAA	UMTS-FDD (DC-HSDPA)	X	3.79	65.76	16.30	0.00	150.0	± 9.6 %
		Y	3.86	65.36	16.10		150.0	
		Z	3.82	65.17	15.85		150.0	
10458- AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	Х	3.05	67.01	14.29	0.00	150.0	± 9.6 %
		Y	3.48	67.05	15.31		150.0	
		Z	3.32	66.56	14.71		150.0	
10459- AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	4.19	65.60	15.56	0.00	150.0	± 9.6 %
		+	+		1 - 3 -		450.0	
		Y	4.63	65.36	16.07		150.0	

10460- AAA	UMTS-FDD (WCDMA, AMR)	X	1.27	75.41	20.14	0.00	150.0	± 9.6 %
<del>////</del>		Υ	1.05	70.71	17.81		150.0	
		Z	0.86	66.76	15.37		150.0	
10461- AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	Х	100.00	127.84	32.72	3.29	80.0	± 9.6 %
	QI ON, OE GODING. NO DIO 117 1959)	Υ	100.00	123.27	31.69		80.0	
_		Z	6.47	83.77	20.46		80.0	
10462- AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	Χ	1.26	63.91	10.22	3.23	80.0	± 9.6 %
, , , ,		Υ	14.90	86.82	19.02		80.0	
		Z	1.81	64.45	10.77		80.0	
10463- AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.85	60.00	7.76	3.23	80.0	± 9.6 %
		Υ	4.74	73.69	14.47		80.0	
		Z	1 <u>.46</u>	62.00	9.21		80.0	
10464- AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	124.65	31.09	3.23	80.0	± 9.6 %
		Y	100.00	121.04	30.50		80.0	
		Z	5.02	79.91	18.70		80.0	
10465- AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16- QAM, UL Subframe=2,3,4,7,8,9)	X	1.13	62.86 	9.67	3.23	80.0	± 9.6 %
·		Y	9.25	81.62	17.45		80.0	
		Z	1.69	63.74	10.38		80.0	
10466- AAA	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64- QAM, UL Subframe=2,3,4,7,8,9)	Х	0.85	60.00	7.71	3.23	80.0	± 9.6 %
<del>,,,,,</del>		Y	3.78	71.31	13.57		80.0	
		Z	1.40	61.59	8.96		80.0	
10467- AAA	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	125.03	31.26	3.23	80.0	± 9.6 %
7001	di ore, de debitatio ajoj eje joj.	Υ	100.00	121.26	30.60		80.0	
		Z	5.32	80.71	18.99		80.0	
10468- AAA	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16- QAM, UL Subframe=2,3,4,7,8,9)	Х	1.17	63.15	9.83	3.23	80.0	± 9.6 %
,,,,,	<u> </u>	Y	10.30	82.81	17.81		80.0	l
		Z	1.71	63.90	10.47		80.0	
10469- AAA	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64- QAM, UL Subframe=2,3,4,7,8,9)	Х	0.85	60.00	7.71	3.23	80.0	± 9.6 %
,,,,,,	<u> </u>	Υ	3.80	71.39	13.60		80.0	
		Z	1.40	61.60	8.96		80.0	
10470- AAA	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	125.05	31.26	3.23	80.0	± 9.6 %
7001	3, 3, 4, 7, 7, 7, 7, 7, 7, 7, 7, 7, 7, 7, 7, 7,	Y	100.00	121.29	30.60		80.0	
		Z	5.31	80.70	18.98		80.0	
10471- AAA	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16- QAM, UL Subframe=2,3,4,7,8,9)	X	1.16	63.09	9.79	3.23	80.0	± 9.6 %
		Υ	10.21	82.69	17.77		80.0	
		Z	1.70	63.86	10.44		80.0	
10472- AAA	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	Х	0.85	60.00	7.70	3.23	80.0	± 9.6 %
	<u> </u>	Υ	3.77	71.31	13.56		80.0	
		Z	1.40	61.57	8.94		80.0	
10473- AAA	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	Х	100.00	125.02	31.24	3.23	80.0	± 9.6 %
		Y	100.00	121.25	30.59		80.0	
		Z	5.30	80.66	18.96		80.0	
10474- AAA	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16- QAM, UL Subframe=2,3,4,7,8,9)	Х	1.15	63.05	9.77	3.23	80.0	± 9.6 %
<del></del>		Y	10.08	82.57	17.73		80.0	
		Z	1.70	63.84	10.43		80.0	
10475- AAA	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	0.85	60.00	7.70	3.23	80.0	± 9.6 %
7007	G 111, 02 00010110 2,0,7,1,10,0/	Y	3.75	71.25	13.54		80.0	_
	T.	1 .	1.39		8.93		80.0	-

10477-	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-	Х	1.12	62.81	9.63	3.23	80.0	± 9.6 %
AAA	QAM, UL Subframe=2,3,4,7,8,9)		0.00	04.00	47.40		00.0	
		Y	9.29	81.66	17.43		80.0	
10.1-0	1 TT TTD (00 FD) (1 TD) (00 N) (1 TD)	Z	1.68	63.69	10.35	0.00	80.0	. 0.0 %
10478- AAA	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64- QAM, UL Subframe=2,3,4,7,8,9)	Х	0.85	60.00	7.69	3.23	80.0	± 9.6 %
		Υ	3.71	71.13	13.49		80.0	
		Z	1.39	61.52	8.91		80.0	
10479- AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	16.34	98.15	26.22	3.23	80.0	± 9.6 %
		Υ	8.05	85.58	23.31		80.0	
		Z	4.44	75.80	19.08		80.0	
10480- AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	Х	8.15	82.28	19.17	3.23	80.0	± 9.6 %
		Y	9.14	82.89	20.82		80.0	
		Z	4.48	72.61	16.42		80.0	
10481- AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	Х	4.98	75.50	16.46	3.23	80.0	± 9.6 %
		Υ	7.94	80.29	19.62		80.0	
		Z	4.00	70.70	15.36		80.0	
10482- AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.11	72.47	16.27	2.23	80.0	± 9.6 %
		Υ	4.49	76.30	19.03		80.0	
		Z	2.84	69.51	15.71		80.0	
10483- AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	Х	3.23	69.48	14.33	2.23	80.0	± 9.6 %
		Y	6.12	77.20	19.06		80.0	_
		Z	3.70	69.78	15.41		80.0	
10484- AAA	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.99	68.30	13.84	2.23	80.0	± 9.6 %
7001	5 : Q: iii, 62 645114116 2,6 <u>1,11,161</u> 67	Υ	5.80	76.19	18.70		80.0	
		Z	3.62	69.26	15.20		80.0	
10485- AAA	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.90	76.03	18.96	2.23	80.0	± 9.6 %
,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,	Q. 014, 02 04 10 10 10 10 10 10 10 10 10 10 10 10 10	Y	4.65	76.77	19.89		80.0	
		Z	3.19	70.88	17.04		80.0	
10486- AAA	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.22	69.78	15.73	2.23	80.0	± 9.6 %
7001	10 00 (01, 02 000)(01,10 2,0,1,110,0)	Υ	4.07	71.59	17.54		80.0	
		Z	3.24	68.15	15.55		80.0	
10487- AAA	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.17	69.19	15.46	2.23	80.0	± 9.6 %
<del>-                                      </del>	04-QAIVI, OE Oubiranie-2,3,4,7,5,5)	Y	4.05	71.16	17.36		80.0	
	<del>-</del>	Ż	3.26	67.91	15.45		80.0	
10488- AAA	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.89	74.31	19.36	2.23	80.0	± 9.6 %
		Υ	4.74	75.31	19.78		80.0	
		Z	3.62	70.94	17.62		80.0	
10489- AAA	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.61	70.11	17.53	2.23	80.0	± 9.6 %
		Υ	4.17	70.61	18.05		80.0	
		Z	3.61	68.29	16.66		80.0	
10490- AAA	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.68	69.86	17.43	2.23	80.0	± 9.6 %
-		Υ	4.25	70.34	17.96		80.0	
		Z	3.72	68.19	16.64		80.0	
	LTE-TDD (SC-FDMA, 50% RB, 15 MHz,	X	3.96	72.11	18.69	2.23	80.0	± 9.6 %
10491- AAA	UPSK. UL Supirame=2.3.4.7.6.91		4 = 4	73.16	19.02		80.0	
10491- _AAA	QPSK, UL_Subframe=2,3,4,7,8,9)	Y	4./4	10.10				
	QPSK, UL Subirame=2,3,4,7,6,9)	Y Z	4.7 <u>4</u> 3.92				80.0	
AAA 10492-	LTE-TDD (SC-FDMA, 50% RB, 15 MHz,	Z X	3.92 3.88	70.03 69.01	17.39 17.48	2.23		±9.6 %
AAA		Z	3.92	70.03	17.39	2.23	80.0	± 9.6 %

10493-	LTE-TDD (SC-FDMA, 50% RB, 15 MHz,	Х	3.93	68.84	17.41	2.23	80.0	± 9.6 %
AAA	64-QAM, UL Subframe=2,3,4,7,8,9)	Y	4.52	69.48	17.82		80.0	
		Z	-	67.81	16.77		80.0	
			4.08	73.69	19.20	2.23	80.0	± 9.6 %
10494- AAA	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.32			2.25		
		Υ	5.29	75.06	19.58		80.0	
		Z	4.18	71.25	17.73		80.0	
10495-	LTE-TDD (SC-FDMA, 50% RB, 20 MHz,	X	3.92	69.34	17.70	2.23	80.0	± 9.6 %
AAA	16-QAM, UL Subframe=2,3,4,7,8,9)			70.19	40.00		80.0	
		Y	4.53		18.09	<del></del>	80.0	_
		Z	4.04	68.27	16.95	0.00		± 9.6 %
10496- AAA	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.98	69.05	17.60	2.23	80.0	± 9.0 %
,,,,,	01 00 001 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0	Y	4.58	69.81	17.97		80.0	
		Z	4.12	68.07	16.91		80.0	
40407	LTE-TDD (SC-FDMA, 100% RB, 1.4	$\frac{1}{x}$	1.72	64.88	11.75	2.23	80.0	± 9.6 %
10497- AAA	MHz, QPSK, UL Subframe=2,3,4,7,8,9)							
		Υ	3.58	73 <u>.16</u>	17.12		80.0	
		Z	2.20	66.42	13.58		80.0	·
10498- AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	Х	1.30	60.00	8.13	2.23	80.0	± 9.6 %
	Subirariie=2,3,4,7,0,3/	Ý	2.81	67.13	13.70		80.0	
		Z	1.98	62.85	11.00		80.0	
					7.98	2.23	80.0	± 9.6 %
10499- AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.32	60.00		2.23		1 0.0 %
		Υ	2.75	66.54	13.31		80.0	
		Z	1.95	62.46	10.68		80.0	
10500- AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	Х	3.82	75.04	19.03	2.23	80.0	± 9.6 %
7001	<u> </u>	Υ	4.55	75.62	19.66		80.0	
		Z	3.32	70.66	17.20		80.0	
10501-	LTE-TDD (SC-FDMA, 100% RB, 3 MHz,	X	3.45	70.22	16.55	2.23	80.08	± 9.6 %
AAA	16-QAM, UL Subframe=2,3,4,7,8,9)	Y	4.10	71.10	17.69		80.0	
					15.99		80.0	_
		Z	3.41	68.23		2.22	80.0	± 9.6 %
10502- AAA	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.48	69.95	16.36	2.23		19.0 %
700		Y	4.15	70.89	17.57		80.0	
		Z	3.47	68.14	15.91		80.0	
10503-	LTE-TDD (SC-FDMA, 100% RB, 5 MHz,	X	3.83	74.06	19.24	2.23	80.0	± 9.6 %
AAA	QPSK, UL Subframe=2,3,4,7,8,9)	+	4.00	75.44	40.00	-	90.0	
		Y	4.68	75.11	19.69	<u> </u>	80.0	1
		Z	3.58	70.77	17.54	0.00	80.0	1000
10504- AAA	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.59	69.99	17.46	2.23	80.0	± 9.6 %
		Υ	4.16	70.53	18.00		80.0	
		Z	3.60	68.21	16.61		80.0	
10505-	LTE-TDD (SC-FDMA, 100% RB, 5 MHz,	X	3.66	69.75	17.36	2.23	80.0	± 9.6 %
AAA	64-QAM, UL Subframe=2,3,4,7,8,9)	Υ	4.23	70.25	17.91		80.0	1
					16.59		80.0	1
		Z	3.70	68.11		2.02		± 9.6 %
10506- AAA	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.28	73.52	19.12	2.23	80.0	1 9.0 %
		Υ	5.24	74.92	19.51		80.0	
		Z	4.15	71.12	17.66		80.0	
10507- AAA	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL	X	3.90	69.27	17.66	2.23	80.0	± 9.6 %
~~~	Subframe=2,3,4,7,8,9)							
	Juditatile=2,3,4,7,0,3/	Y	4.51	70.14	18.06		80.0	
		$\frac{1}{Z}$	4.02	68.21	16.91		80.0	1
l .		_	4.02	00.21	10.01			

10508- AAA	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.97	68.96	17.55	2.23	80.0	± 9.6 %
	Oubilain6=2,0,4,1,0,0/	Y	4.57	69.75	17.93		80.0	
	-	Z	4.11	68.00	16.87		80.0	
10509-	LTE-TDD (SC-FDMA, 100% RB, 15	X	4.54	71.87	18.48	2.23	80.0	± 9.6 %
AAA	MHz, QPSK, UL Subframe=2,3,4,7,8,9)					2,20		2 9.0 /0
	-	Y	5.35	73.05	18.77		80.0	
		Z	4.54	70.32	17.38	0.00	80.0	. 0 0 0/
10510- AAA	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.34	68.76	17.59	2,23	80.0	± 9.6 %
		Υ	4.97	69.73	17.95		80.0	
		Z	4.53	68.16	17.00		80.0	
10511- AAA	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.39	68.51	17.51	2.23	80.0	± 9.6 %
		Y	5.00	69.40	17.85		0.08	
	_	Z	4.59	67.95	16.96		80.0	
10512- AAA	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.78	73.48	18.98	2.23	80.0	±9.6%
		Y	5.80	75.09	19.41		80.0	
		Z	4.67	71.54	17.71		80.0	
10513- AAA	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL	X	4.24	69.00	17.69	2.23	80.0	± 9.6 %
	Subframe=2,3,4,7,8,9)	Y	4.89	70.17	18.11		80.0	
<del>.</del>		$\frac{1}{Z}$	4.41	68.40	17.07		80.0	
10514- AAA	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.26	68.58	17.56	2.23	80.0	± 9.6 %
	Submarile=2,5,4,7,6,9)	Y	4.87	69.63	17.95		80.0	
<del></del>	<del>-</del>	Z	4.44	68.04	16.99		80.0	
10515-	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2	X	1.03	64.84	16.18	0.00	150.0	± 9.6 %
AAA	Mbps, 99pc duty cycle)	Y	1.01	63.76	15.35		150.0	
		Z	0.97	62.74	14.37		150.0	
40546	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5	X	1.37	87.37	25.57	0.00	150.0	± 9.6 %
10516- AAA	Mbps, 99pc duty cycle)					0.00	150.0	
		Y	0.82	76.24	20.55		150.0	
		Z	0.54	67.46	15.73	0.00	150.0	± 9.6 %
10517- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle)	Х	0.93	68.34	17.75	0.00		± 9.0 %
		Y	0.89	66.40	16.42	-	150.0	_
		Z	0.81	64.28	14.78	6.64	150.0	
10518- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	X	4.48	67.19	16.57	0.00	150.0	± 9.6 %
		Y	4.6 <u>6</u>	66.80	16.35		150.0	
		Z	4.59	66.60	16.12		150.0	
10519- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle)	Х	4.64	67.36	16.66	0.00	150.0	± 9.6 %
		Υ	4.88	67.08	16.48		150.0	
		Z	4.7 <u>9</u>	66.86	16.25		150.0	
10520- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle)	Х	4.50	67.33	16.59	0.00	150.0	± 9.6 %
		Y	4.73	67.07	16.42		150.0	
		Z	4.64	66.83	16.17		150.0	
10521- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle)	Х	4.43	67.32	16.58	0.00	150.0	± 9.6 %
		Υ	4.66	67.08	16.41		150.0	
		Z	4.57	66.82	16.16		150.0	
10522- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle)	Х	4.49	67.45	16.68	0.00	150.0	± 9.6 %
		Y	4.71	67.07	16.44		150.0	
					16.22		150.0	

AAA	Mbps, 99pc duty cycle)	+ ·						
		Y	4.58	66.97	16.31		150.0	
		Z	4.50	66.74	16.07		150.0	
10524-	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle)	X	4.44	67.39	16.66	0.00	150.0	± 9.6 %
AAA	Mbps, 99pc duty cycle)	T Y	4.66	67.02	16.43		150.0	
		z	4.57	66.80	16.19		150.0	
		$\frac{1}{x}$		66.48	16.28	0.00	150.0	± 9.6 %
10525- AAA	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)		4.46			0.00	150.0	
		Y	4.62	66.06	16.02			
		Z	4.54	65.85	15.79	0.00	150.0	. 0.6.0/
10526- AAA	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	4.60	66.79	16.40	0.00	150.0	± 9.6 %
, , , ,		Ý	4.82	66.46	16.16		150.0	
		Z	4.72	66.22	15.93		150.0	
10527- AAA	IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle)	X	4.53	66.77	16.35	0.00	150.0	± 9.6 %
<del>^</del>	99pc daty cycle)	Y	4.74	66.44	16.12		150.0	
		Z	4.64	66.19	15.88		150.0	
40500	IEEE 802.11ac WiFi (20MHz, MCS3,	X	4.54	66.78	16.38	0.00	150.0	± 9.6 %
10528- AAA	99pc duty cycle)				16.15		150.0	
		Y	4.75	66.46			150.0	
		Z	4.66	66.21	15.91	0.00		± 9.6 %
10529- AAA	IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle)	X	4.54	66.78	16.38	0.00	150.0	± 9.6 %
		Y	4.75	66.46	16.15		150.0	
		Z	4.66	66.21	15.91		150.0	
10531-	IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle)	X	4.52	66.84	16.38	0.00	150.0	± 9.6 %
AAA	99pc daty cycle)	+ <sub>Y</sub> -	4.76	66.60	16.18		150.0	-
		Ż	4.66	66.32	15.93		150.0	
10532-	IEEE 802.11ac WiFi (20MHz, MCS7,	X	4.39	66.72	16.32	0.00	150.0	± 9.6 %
<u> </u>	99pc duty_cycle)		4.04	66.47	16.13		150.0	
		Y	4.61	66.47			150.0	
		Z	4.51	66.18	15.86	0.00	150.0	± 9.6 %
10533- AAA	IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle)	X	4.55	66.87	16.39	0.00		19.0%
		Υ	4.77	66.48	16.13		150.0	
		Z	4.67	66.24	15.89		150.0	
10534-	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	Х	5.09	66.73	16.38	0.00	150.0	± 9.6 %
AAA	Jupo daty Gyoro)	Y	5.26	66.58	16.18		150.0	
		Z	5.19	66.36	15.98		150.0	
10535-	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	5.14	66.89	16.46	0.00	150.0	± 9.6 %
AAA		Y	5.33	66.72	16.24		150.0	
		Z	5.25	66.50	16.04		150.0	
10536-	IEEE 802.11ac WiFi (40MHz, MCS2,	X	5.03	66.89	16.44	0.00	150.0	± 9.6 %
AAA	99pc duty cycle)	Y	5.20	66.71	16.22		150.0	1
	-	Z	5.12	66.47	16.01	†	150.0	
40505	JEEE 000 444 - 1885: 740441 - 84000	X	5.08	66.84	16.42	0.00	150.0	± 9.6 %
10537- AAA	IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)					0.00	150.0	2 3.3 70
		Y	5.27	66.68	16.21	-		
10538-	IEEE 802.11ac WiFi (40MHz, MCS4,	Z	5.1 <u>8</u> 5.15	66.44 66.81	16.00 16.44	0.00	150.0 150.0	± 9.6 %
AAA	99pc duty cycle)					ļ		<del> -</del>
-	<u> </u>	Υ	5.37	66.74	16.28		150.0	<u></u>
		Z	5.28	66.49	16.06		150.0	
					16.45	0.00	150.0	± 9.6 %
10540-	IEEE 802.11ac WiFi (40MHz, MCS6,	X	5.09	66.80	10.43	0.00		20:070
10540- AAA	IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)	X	5.09	66.69	16.27	0.00	150.0	

10541-	IEEE 802.11ac WiFi (40MHz, MCS7,	X	5.06	66.68	16.38	0.00	150.0	± 9.6 %
AAA	99pc duty cycle)	^	5.00	00.00	10.50	0.00	130.0	2 3.0 70
7001	Sopo daty syste)	Y	5.26	66.60	16.22		150.0	
	_	Z	5.18	66.36	16.00		150.0	
10542-	IEEE 802.11ac WiFi (40MHz, MCS8,	X	5.22	66.77	16.43	0.00	150.0	± 9.6 %
AAA	99pc duty cycle)							
		Υ	5.41	66.64	16.25		150.0	
		Z	5.33	66.43	16.05		150.0	
10543- AAA	IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)	X	5.28	66.79	16.47	0.00	150.0	± 9.6 %
		Ý	5.50	66.65	16.27		150.0	
		Z	5.41	66.46	16.08		150.0	
10544- AAA	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	Х	5.42	66.77	16.34	0.00	150.0	± 9.6 %
		Y	5.55	66.69	16.17		150.0	
		Z	5.48	66.48	15.98		150.0	
10545- AAA	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	X	5.61	67.23	16.53	0.00	150.0	± 9.6 %
		Y	5.75	67.07	16.30		150.0	
		Z	5.67	66.87	16.11		150.0	
10546- AAA	IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)	Х	5.46	66.92	16.38	0.00	150.0	± 9.6 %
		Υ	5.64	66.96	16.27		150.0	
		Z	5.56	66.72	16.06		150.0	
10547- AAA	IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)	Х	5.54	67.00	16.42	0.00	150.0	± 9.6 %
		Υ	5.73	67.04	16.29		150.0	
		Z.	5.64	66.77	16.07		150.0	
10548- AAA	IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)	X	5.73	67.79	16.78	0.00	150.0	± 9.6 %
		Υ	5.99	67.96	16.73		150.0	
		Z	5.87	67.64	16.48		150.0	
10550- AAA	IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)	Х	5.52	67.07	16.47	0.00	150.0	± 9.6 %
		Y	5.66	66.92	16.25		150.0	
		Z	5.58	66.70	16. <u>06</u>		150.0	
10551- AAA	IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)	X	5.47	66.93	16.36	0.00	150.0	± 9.6 %
		Υ	5.67	66.99	16.25		150.0	_
		Z	5.59	66.76	16.05		150.0	
10552- AAA	IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)	Х	5.43	66.87	16.34	0.00	150.0	± 9.6 %
		Y	5.58	66.77	16.15		150.0	
		Z	5.50	66.55	15.96		150.0	
10553- AAA	IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)	Х	5.49	66.84	16.35	0.00	150.0	± 9.6 %
<u> </u>		Y	5.67	66.82	16.21		150.0	
		Z	5.59	66.61	16.01		150.0	
10554- AAA	IEEE 1602.11ac WiFi (160MHz, MCS0, 99pc duty cycle)	X	5.84	67.09	16.40	0.00	150.0	± 9.6 %
		Υ	5.94	67.05	16.25		150.0	
		Z	5.88	66.85	16.07		150.0	
10555- AAA	IEEE 1602.11ac WiFi (160MHz, MCS1, 99pc duty cycle)	X	5.95	67.36	16.52	0.00	150.0	± 9.6 %
		Υ	6.0 <u>9</u>	67.37	16.39		150.0	
		Z	6.01	67.14	16.19		150.0	. 0 0 0/
10556- AAA	IEEE 1602.11ac WiFi (160MHz, MCS2, 99pc duty cycle)	X	5.98	67.45	16.56	0.00	150.0	± 9.6 %
-		Υ	6.10	67.39	16.39		150.0	
		Z	6.03	67.18	16.21		150.0	
10557- AAA	IEEE 1602.11ac WiFi (160MHz, MCS3, 99pc duty cycle)	Х	5.93	67.31	16.50	0.00	150.0	± 9.6 %
<del>^-</del>		Y	6.09	67.35	16.39		150.0	
		Z	6.01	67.12	16.19		150.0	

10558- AAA	IEEE 1602.11ac WiFi (160MHz, MCS4, 99pc duty cycle)	X	5.96	67.43	16.58	0.00	150.0	± 9.6 %
	3000 daily 0y010/	Y	6.14	67.53	16.50		150.0	
		Z	6.06	67.28	16.29		150.0	
10560-	IEEE 1602.11ac WiFi (160MHz, MCS6, 99pc duty cycle)	X	5.96	67.30	16.55	0.00	150.0	± 9.6 %
<u> </u>	99pc duty cycle)	Y	6.14	67.38	16.46		150.0	
		Z	6.06	67.14	16.26		150.0	
	THE LOOP AND THE MICE AND THE	X	5.90	67.30	16.59	0.00	150.0	± 9.6 %
10561- AAA	IEEE 1602.11ac WiFi (160MHz, MCS7, 99pc duty cycle)				16.47		150.0	
		Y	6.05	67.33			150.0	
		Z	5.97	67.09	16.27	0.00	150.0	± 9.6 %
10562- AAA	IEEE 1602.11ac WiFi (160MHz, MCS8, 99pc duty cycle)	Х	5.97	67.52	16.70	0.00		
		Y	6.20	67.78	16.70		150.0	
		Z	6.10	67.49	16.47		150.0	
10563- AAA	IEEE 1602.11ac WiFi (160MHz, MCS9, 99pc duty cycle)	X	6.05	67.43	16.61	0.00	150.0	± 9.6 %
70.00		Y	6.51	68.26	16.88		150.0	
	<del>-</del>	Z	6.42	68.01	16.67		150.0	
40504	IEEE 802.11g WiFi 2.4 GHz (DSSS-	X	4.79	67.15	16.65	0.46	150.0	±9.6 %
10564- AAA	OFDM, 9 Mbps, 99pc duty cycle)		4.99	66.89	16.50		150.0	
		Y	4.91	66.68	16.27		150.0	
		Z			16.27	0.46	150.0	± 9.6 %
10565- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 12 Mbps, 99pc duty cycle)	X	5.00	67.58		U.46		± 9.0 %
		Y	5.25	67 <u>.37</u>	16.83		150.0	
		Z	5.16	67.16	16.61		150.0	2 2 2 /
10566- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 18 Mbps, 99pc duty cycle)	Х	4.83	67.41	16.78	0.46	150.0	± 9.6 %
	Of Divi, 10 wispe, cope day	Υ	5.08	67.24	16.66		150.0	
		Z	4.99	67.00	16.41		150.0	
10567-	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 24 Mbps, 99pc duty cycle)	X	4.88	67.87	17.20	0.46	150.0	± 9.6 %
<u> </u>	OFDIM, 24 Mibbs, 99pc duty cycle)	Y	5.11	67.62	16.99		150.0	_
		Z	5.02	67.41	16.78		150.0	
10568-	IEEE 802.11g WiFi 2.4 GHz (DSSS-	X	4.73	67.14	16.52	0.46	150.0	± 9.6 %
AAA	OFDM, 36 Mbps, 99pc duty cycle)	\ \	4.00	66.97	16.41		150.0	
		Y	4.99				150.0	1
		Z	4.89	66.73	16.15	0.40		1069/
10569- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 48 Mbps, 99pc duty cycle)	Х	4.86	68.08	17.32	0.46	150.0	± 9.6 %
		Y	5.05	67.63	17.01		150.0	
		Z	4.97	67.46	16.82		150.0	
10570~ AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 54 Mbps, 99pc duty cycle)	Х	4.87	67.85	17.21	0.46	150.0	± 9.6 %
<u>`</u> ~~~	Or Divi, or mape, cope dad, eyers)	Υ	5.09	67.48	16.95		150.0	
		Ż	5.01	67.31	16.75		150.0	
10571-	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1	X	1.23	65.85	16.68	0.46	130.0	± 9.6 %
<u> </u>	Mbps, 90pc duty cycle)	Y	1.28	65.62	16.38	1	130.0	1
		- <u>r</u>	1.20	64.12	15.14	<del>                                     </del>	130.0	1
					17.14	0.46	130.0	± 9.6 %
10572- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	1.26	66.61		0.46		± ₹.0 /0
		Υ	1.30	66.27	16.76	-	130.0	
		Z	1.21	64.64	15.46	<u> </u>	130.0	1000
10573- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	Х	15.61	122.59	34.86	0.46	130.0	± 9.6 %
· · · · · ·		Y	7.32	105.62	29.57		130.0	
		Z	1.41	77.28	19.61		130.0	
10574-	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11	X	1.59	75.46	21.51	0.46	130.0	± 9.6 %
AAA	Mbps, 90pc duty cycle)	Y	1.56	73.46	20.23		130.0	_
		Z			17.90		130.0	
	T	1 Z	1.30	69.51	17.50	1	100.0	L

10575-	IEEE 802.11g WiFi 2.4 GHz (DSSS-	Х	4.57	66.90	16.65	0.46	130.0	± 9.6 %
AAA	OFDM, 6 Mbps, 90pc duty cycle)						100.0	
		Y	4.78	66.67	16.55		130.0	
		Z	4.70	66.43	16.27	0.40	130.0	. 0.0.0/
10576- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 9 Mbps, 90pc duty cycle)	X	4.60	67.11	16.74	0.46	130.0	± 9.6 %
		Y	4.81	66.83	16.61		130.0	
		Z	4.72	66.59	16.34		130.0	
10577- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 12 Mbps, 90pc duty cycle)	Х	4.78	67.36	16.89	0.46	130.0	± 9.6 %
700.	J. 2111, 12 1113 po, 10 po san, 1, 1, 1, 1, 1, 1, 1, 1, 1, 1, 1, 1, 1,	Y	5.04	67.16	16.78		130.0	
		Z	4.94	66.91	16.52		130.0	
10578- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 18 Mbps, 90pc duty cycle)	Х	4.68	67.55	17.03	0.46	130.0	± 9.6 %
	<u> </u>	Υ	4.93	67.32	16.88		130.0	
		Z	4.83	67.07	16.62		130.0	
10579- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 24 Mbps, 90pc duty cycle)	Х	4.43	66.68	16.24	0.46	130.0	± 9.6 %
7001	Of Bin, 2 i maps, sope daily system	Y	4.71	66.69	16.25		130.0	
		Ż	4.59	66.34	15.91		130.0	
10580- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 36 Mbps, 90pc duty cycle)	X	4.47	66.74	16.26	0.46	130.0	± 9.6 %
/V-V1	Or Divi, So wipps, Sopo dary cycle)	Y	4.75	66.68	16.26		130.0	
		Z	4.64	66.35	15.93		130.0	
10581-	IEEE 802.11g WiFi 2.4 GHz (DSSS-	X	4.59	67.62	16.99	0.46	130.0	± 9.6 %
AAA	OFDM, 48 Mbps, 90pc duty cycle)	Y	4.83	67.38	16.83		130.0	
			4.73	67.09	16.54		130.0	<del>-</del>
10582-	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 54 Mbps, 90pc duty cycle)	X	4.35	66.42	16.00	0.46	130.0	± 9.6 %
AAA	OF DIM, 54 IMBDS, 90pc duty cycle)	Y	4.66	66.46	16.06		130.0	
		Z	4.54	66.09	15.70		130.0	
10583-	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6	X	4.57	66.90	16.65	0.46	130.0	± 9.6 %
AAA	Mbps, 90pc duty cycle)	Y	1 70	66.67	16.55		130.0	
			4.78		16.33		130.0	<del>-</del>
	THE PART OF THE PA	Z	4.70	66.43 67.11	16.74	0.46	130.0	± 9.6 %
10584- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	Х	4.60			0.40		1 9.0 70
		Υ	4.8 <u>1</u>	66.83	16.61		130.0	
		Z	4.72	66.59	16.34		130.0	
10585- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	Х	4.78	67.36	16.89	0.46	130.0	± 9.6 %
		Υ	5.04	67.16	16.78		130.0	
		Z	4.94	66.91	16.52		130.0	
10586- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle)	Х	4.68	67.55	17.03	0.46	130.0	± 9.6 %
		Y	4.93	67.32	16.88		130.0	
		Z	4.83	67.07	16. <u>6</u> 2		130.0	1
10587- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)	Х	4.43	66.68	16.24	0.46	130.0	± 9.6 %
, , , , ,		Υ	4.71	66.69	16.25		130.0	
		Z	4.59	66.34	15.91	l	130.0	
10588- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)	X	4.47	66.74	16.26	0.46	130.0	± 9.6 %
		Y	4.75	66.68	16.26		130.0	
		Z	4.64	66.35	15.93		130.0	
10589- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)	X	4.59	67.62	16.99	0.46	130.0	± 9.6 %
700	impo, copo daty cycle/	Y	4.83	67.38	16.83		130.0	
		Ż	4.73	67.09	16.54		130.0	
10590-	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54	X	4.35	66.42	16.00	0.46	130.0	± 9.6 %
10590- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)				16.00 16.06	0.46	130.0	± 9.6 %

October 3, 2016

10591-	IEEE 802.11n (HT Mixed, 20MHz,	X	4.72	66.97	16.76	0.46	130.0	± 9.6 %
4AA	MCS0, 90pc duty cycle)	Y	4.93	66.73	16.63		130.0	
		Z	4.85	66.51	16.38		130.0	
	THE COOK IN THE THE CONTRACT	X	4.85	67.28	16.89	0.46	130.0	± 9.6 %
10592- NAA	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)					0.40		
		Y	5 <u>.1</u> 0	67.07	16.76		130.0	
		Z	5 <u>.01</u>	66.85	16.51		130.0	
10593- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle)	X	4.77	67.16	16.75	0.46	130.0	± 9.6 %
		Y	5.03	67.02	16.67		130.0	
		Z	4.93	66.76	16.39		130.0	
10594- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle)	X	4.83	67.35	16.92	0.46	130.0	± 9.6 %
		Y	5.08	67.17	16.80		130.0	
		Z	4.99	66.92	16.54		130.0	
10595-	IEEE 802.11n (HT Mixed, 20MHz,	X	4.79	67.31	16.82	0.46	130.0	± 9.6 %
AAA	MCS4, 90pc duty cycle)	Y	5.06	67.14	16.71		130.0	
			4.95	66.87	16.44		130.0	
		Z	4.93	67.29	16.82	0.46	130.0	± 9.6 %
10596- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle)	Х				— <del>-</del>	130.0	2 3.0 70
		Y	4.99	67.14	16.71			
		Z	4.89	66.86	16.43		130.0	. 0 0 0
10597- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle)	X	4.68	67.16	16.68	0.46 	130.0	± 9.6 %
, , , , ,		Y	4.95	67.07	16.62		130.0	
<del></del> .		Z	4.84	66.78	16.32		130.0	
10598-	IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle)	X	4.67	67.44	16.97	0.46	130.0	± 9.6 %
AAA	WOS1, sopo daty oyele)	Y	4.93	67.31	16.88		130.0	
		Z	4.82	67.03	16.60		130.0	
10599-	IEEE 802.11n (HT Mixed, 40MHz,	X	5.39	67.39	16.95	0.46	130.0	± 9.6 %
AAA	MCS0, 90pc duty cycle)	Y	5.60	67.32	16.82		130.0	_
			5.51	67.07	16.58		130.0	
10600-	IEEE 802.11n (HT Mixed, 40MHz,	Z X	5.51	67.80	17.12	0.46	130.0	± 9.6 %
AAA	MCS1, 90pc duty cycle)			07.04	17.04		130.0	
		Y	5.77	67.81			130.0	
		Z	5.65	67.49	16.76	0.40		. 0.6.9/
10601- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle)	X	5.41	67.56	17.02	0.46	130.0	± 9.6 %
,,,,,		Y	5.64	67.51	16.91		130.0	
		Z	5.54	67.24	16.65		130.0	
10602- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle)	X	5.54	67.73	17.02	0.46	130.0	± 9.6 %
, v v 1		Y	5.72	67.51	16.82		130.0	
	<del>                                     </del>	Z	5.62	67.22	16.56		130.0	
10603-	IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle)	X	5.62	68.07	17.33	0.46	130.0	± 9.6 %
AAA	ivicion, sope duty cycle)	Y	5.82	67.83	17.11		130.0	Î
		Z	5.72	67.58	16.87	1	130.0	
	JEEE 000 44- /UT 845 3-40840-		5.49	67.68	17.12	0.46	130.0	± 9.6 %
10604- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle)	X				0.40	130.0	
		Y	5.60	67.27	16.82	-		
		Z	5.51	67.03	16.58	0.10	130.0	1000
10605- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle)	X	5.51	67.70	17.12	0.46	130.0	± 9.6 %
- <del>*</del> ·		Y	5.70	67.55	16.96		130.0	
		Z	5.61	67.31	16.72		130.0	
10606-	IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle)	X	5.26	67.01	16.63	0.46	130.0	± 9.6 %
AAA	ivicor, sope duty cycle)	Y	5.49	67.08	16.60		130.0	
		Z	5.39	66.79	16.33		130.0	

10607-	IEEE 802.11ac WiFi (20MHz, MCS0,	X	4.58	66.35	16.43	0.46	130.0	± 9.6 %
AAA	90pc duty cycle)							
		Y	4.76	66.03	16.25		130.0	
		Z	4.68	65.79	15.98		130.0	
10608- AAA	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	4.73	66.71	16.58	0.46	130.0	± 9.6 %
		Y	4.98	66.46	16.42		130.0	
		Z	4.87	66.20	16.15		130.0	
10609- AAA	IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle)	X	4.62	66.54	16.40	0.46	130.0	± 9.6 %
		Y	4.87	66.34	16.28		130.0	
		Z	4.76	66.05	15.99		130.0	
10610- AAA	IEEE 802.11ac WiFi (20MHz, MC\$3, 90pc duty cycle)	X	4.68	66.72	16.58	0.46	130.0	± 9.6 %
		Y	4.92	66.49	16.43		130.0	
		Z	4.81	66.21	16.15		130.0	_
10611- AAA	IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle)	X	4.59	66.51	16.42	0.46	130.0	± 9.6 %
		Υ	4.84	66.32	16.29		130.0	
		Z	4.73	66.02	16.00		130.0	
10612- AAA	IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle)	Х	4.59	66.66	16.46	0.46	130.0	± 9.6 %
		Υ	4.85	66.48	16.33		130.0	
	_	Z	4.74	66.16	16.03		130.0	
10613- AAA	IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle)	X	4.58	66.47	16.30	0.46	130.0	± 9.6 %
		Υ	4.87	66.40	16.24		130.0	
		Z	4.75	66.06	15.92		130.0	
10614- AAA	IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle)	Х	4.55	66.74	16.59	0.46	130.0	± 9.6 %
		Y	4.80	66.57	16.46		130.0	
		Z	4.69	66.26	16.16		130.0	
10615- AAA	IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle)	X	4.58	66.31	16.16	0.46	130.0	± 9.6 %
7001	oopo aatij oyoloj	Y	4.84	66.15	16.08		130.0	
	-	Z	4.73	65.83	15.77		130.0	
10616- AAA	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	5.21	66.65	16.56	0.46	130.0	± 9.6 %
7001	3555 331, 35515,	Y	5.41	66.58	16.44		130.0	
		Z	5.33	66.33	16.20		130.0	
10617- AAA	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	Х	5.28	66.84	16.63	0.46	130.0	± 9.6 %
AAA	Sopo daty Systey	Y	5.47	66.68	16.45		130.0	
		Z	5.38	66.45	16.22		130.0	
10618- AAA	IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle)	X	5.18	66.90	16.68	0.46	130.0	± 9.6 %
7001		Y	5.37	66.76	16.51		130.0	
		Z	5.28	66.49	16.27		130.0	
10619- AAA	IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle)	Х	5.18	66.65	16.49	0.46	130.0	± 9.6 %
		Y	5.39	66.59	16.37		130.0	
		Z	5.30	66.32	16.11		130.0	
10620- AAA	IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle)	X	5.26	66.66	16.54	0.46	130.0	± 9.6 %
		Y	5.51	66.68	16.46		130.0	
		Z	5.40	66.39	16.19		130.0	
10621- AAA	IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle)	X	5.27	66.82	16.75	0.46	130.0	± 9.6 %
		Y	5.48	66.74	16.60		130.0	
		Z	5.39	66.50	16.37		130.0	
10622-	IEEE 802.11ac WiFi (40MHz, MCS6,	X	5.27	66.93	16.80	0.46	130.0	± 9.6 %
						l		
10622- AAA	90pc duty cycle)	Y	5.48	66.86	16.65		130.0	

10623- AAA	IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle)	X	5.14	66.42	16.40	0.46	130.0	± 9.6 %
	sope duty cycle)	Υ	5.37	66.46	16.34		130.0	
		Z	5.27	66.17	16.07		130.0	
10624-	IEEE 802.11ac WiFi (40MHz, MCS8,	X	5.34	66.68	16.59	0.46	130.0	± 9.6 %
<u> </u>	90pc duty cycle)	Y	5.56	66.62	16.48		130.0	
		Z	5.47	66.37	16.24		130.0	
	1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	X	5.51	67.05	16.84	0.46	130.0	± 9.6 %
10625- AAA	IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle)						130.0	
		Υ	5.94	67.60	17.02			
		Z	5.85	67.36	16.78	0.46	130.0 130.0	± 9.6 %
10626- AAA	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	Х	5.53	66.66	16.50	0.46		
		Υ	5.68	66.62	16.38		130.0	
		Z	5.60	66.40	16.16		130.0	
10627- AAA	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	X	5.78	67.30	16.79	0.46	130.0	± 9.6 %
/VV\		Y	5.92	67.14	16.59		130.0	
		Z	5.84	66.92	16.37		130.0	
10628-	IEEE 802.11ac WiFi (80MHz, MCS2,	X	5.53	66.65	16.39	0.46	130.0	± 9.6 %
AAA	90pc duty cycle)	Υ	5.74	66.79	16.36		130.0	
		Z	5.65	66.51	16.11		130.0	
10629-	IEEE 802.11ac WiFi (80MHz, MCS3,	X	5.63	66.79	16.45	0.46	130.0	± 9.6 %
AAA	90pc duty cycle)	Y	5.82	66.85	16.38		130.0	
			5.74	66.60	16.14		130.0	
		Z		67.97	17.05	0.46	130.0	± 9.6 %
10630- AAA	IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle)	Х	5.95			0.40		2 9.0 %
		Y	6.32	68.49	17.20		130.0	
		Z	6.17	68.05	16.86		130.0	
10631- AAA	IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle)	X	5.89	67.93	17.23	0.46	130.0	± 9.6 %
,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,		Y	6.21	68.27	17.26		130.0	
		Z	6.09	67.93	17.00		130.0	
10632- AAA	IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle)	X	5.77	67.44	17.00	0.46	130.0	± 9.6 %
AAA	gope daily cycle)	Υ	5.90	67.22	16.76		130.0	
		Ż	5.82	67.00	16.55		130.0	
10633-	IEEE 802.11ac WiFi (80MHz, MCS7,	X	5.60	66.87	16.54	0.46	130.0	± 9.6 %
AAA	90pc duty cycle)	Y	5.83	67.02	16.49		130.0	
		Z	5.72	66.69	16.23		130.0	
10634- AAA	IEEE 802.11ac WiFi (80MHz, MCS8,	X	5.59	66.92	16.62	0.46	130.0	± 9.6 %
	90pc duty cycle)	Y	5.81	67.01	16.55		130.0	
		Z	5.71	66.73	16.31		130.0	
10635- AAA	IEEE 802.11ac WiFi (80MHz, MCS9,	X	5.44	66.12	15.93	0.46	130.0	± 9.6 %
	90pc duty cycle)	Y	5.70	66.39	15.99		130.0	
		$\frac{1}{Z}$	5.70	66.05	15.69		130.0	-
10636-	IEEE 1602.11ac WiFi (160MHz, MCS0,	X	5.96	67.00	16.57	0.46	130.0	± 9.6 %
AAA	90pc duty cycle)	Υ	6.08	67.01	16.47		130.0	
		Z	6.01	66.78	16.25		130.0	<u> </u>
10637- AAA	IEEE 1602.11ac WiFi (160MHz, MCS1, 90pc duty cycle)	X	6.10	67.36	16.74	0.46	130.0	± 9.6 %
	oopo daty oyoloj	Y	6.25	67.39	16.63		130.0	
		Z	6.17	67.14	16.41		130.0	
10638-	IEEE 1602.11ac WiFi (160MHz, MCS2,	X	6.11	67.36	16.71	0.46	130.0	± 9.6 %
AAA	90pc duty cycle)	Y	6.25	67.36	16.60		130.0	
		Z	6.23	67.12	16.38	+	130.0	+

	<del>-</del>						1000	0.00
10639- AAA	IEEE 1602.11ac WiFi (160MHz, MCS3, 90pc duty cycle)	×	6.07	67.26	16.71	0.46	130.0	± 9.6 %
	0000000	Y	6.25	67.37	16.65		130.0	
		Z	6.16	67.11	16.42		130.0	
10640- AAA	IEEE 1602.11ac WiFi (160MHz, MCS4, 90pc duty cycle)	X	6.05	67.22	16.62	0.46	130.0	± 9.6 %
		Y	6.27	67.44	16.63		130.0	
	-	Ż	6.17	67.12	16.37		130.0	
10641- AAA	IEEE 1602.11ac WiFi (160MHz, MCS5, 90pc duty cycle)	X	6.13	67.23	16.65	0.46	130.0	± 9.6 %
7001		Y	6.27	67.20	16.53		130.0	
	-	Z	6.19	66.96	16.31		130.0	
10642- AAA	IEEE 1602.11ac WiFi (160MHz, MCS6, 90pc duty cycle)	X	6.16	67.45	16.94	0.46	130.0	± 9.6 %
		Y	6.34	67.53	16.85		130.0	
		Z	6.25	67.29	16.64		130.0	
10643- AAA	IEEE 1602.11ac WiFi (160MHz, MCS7, 90pc duty cycle)	Х	6.00	67.14	16.67	0.46	130.0	± 9.6 %
		Y	6.17	67.21	16.60		130.0	
		Z	6.08	66.93	16.36		130.0	
10644- AAA	IEEE 1602.11ac WiFi (160MHz, MCS8, 90pc duty cycle)	Х	6.08	67.39	16.82	0.46	130.0	± 9.6 %
		Υ	6.38	67.85	16.95		130.0	
		Z	6.26	67.49	16.66		130.0	
10645- AAA	IEEE 1602.11ac WiFi (160MHz, MCS9, 90pc duty cycle)	X	6.23	67.50	16.83	0.46	130.0	± 9.6 %
		Y	6.74	68.44	17.18		130.0	
		Z	6.68	68.29	17.00		130.0	_
10646- AAB	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)	Х	13.71	101.95	34.43	9.30	60.0	± 9.6 %
		Υ	31.42	116.20	38.46		60.0	
		Z	15.59	99.47	32.52		60.0	
10647- AAA	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7)	Х	12.18	100.02	33.95	9.30	60.0	± 9.6 %
		Y	30.06	116.00	38.55		60.0	
		Z	14.66	98.82	32.42		60.0	
10648- AAA_	CDMA2000 (1x Advanced)	X	0.74	65.73	11.50	0.00	150.0	± 9.6 %
		Y	0.86	65.73	12.88		150.0	
		Ż	0.73	63.45	11.13		150.0	

<sup>&</sup>lt;sup>E</sup> Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.