

## Appendix 2 Photodocumentation

**Description:** 19" cabinet  
front view with open door

Medizintechnik/Nach-  
richtentechnik/EMV

Department: EMC

Test report reference:  
M/EMV-05/141

Page: 1 of 36

Date: 31.05.2005

checked by: 4



## Appendix 2 Photodocumentation

Description: 19" cabinet front detail view #1

Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:  
M/EMV-05/141

Page: 2 of 36

Date: 31.05.2005

checked by: M





## Appendix 2 Photodocumentation

Description: 19" cabinet front detail view #2

Medizintechnik/Nach-  
richtentechnik/EMV


Department: EMC

Test report reference:  
M/EMV-05/141

Page: 3 of 36

Date: 31.05.2005

checked by: h

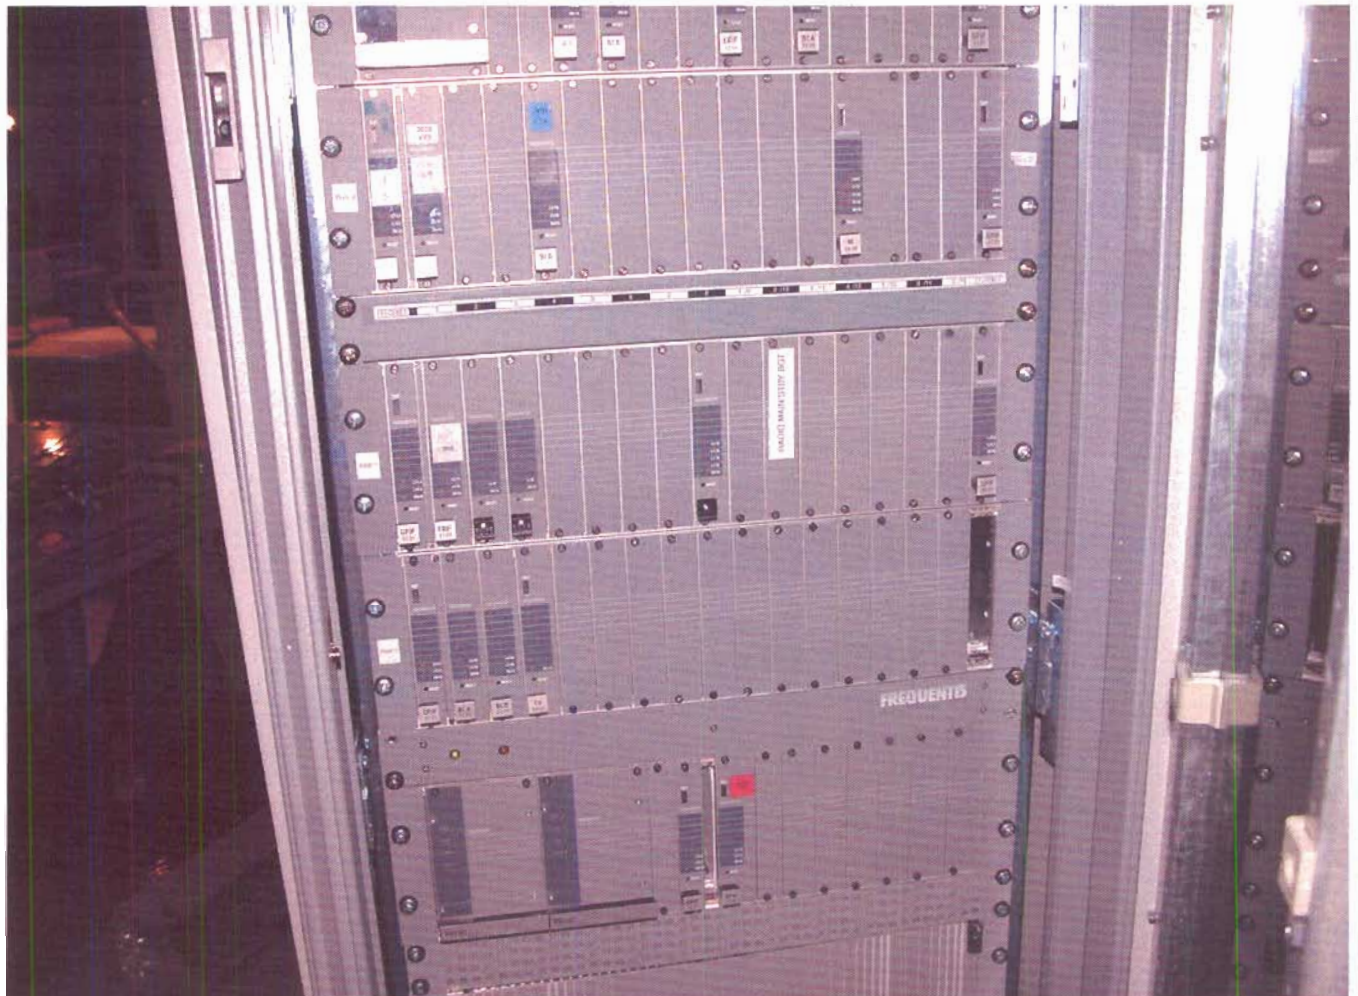

## Appendix 2 Photodocumentation

**Description:** 19" cabinet front detail view #3;  
the two power supplies at the bottom are not  
part of the EUT

Medizintechnik/Nach-  
richtentechnik/EMV


Department: EMC

Test report reference:  
M/EMV-05/141

Page: 4 of 36

Date: 31.05.2005

checked by: M

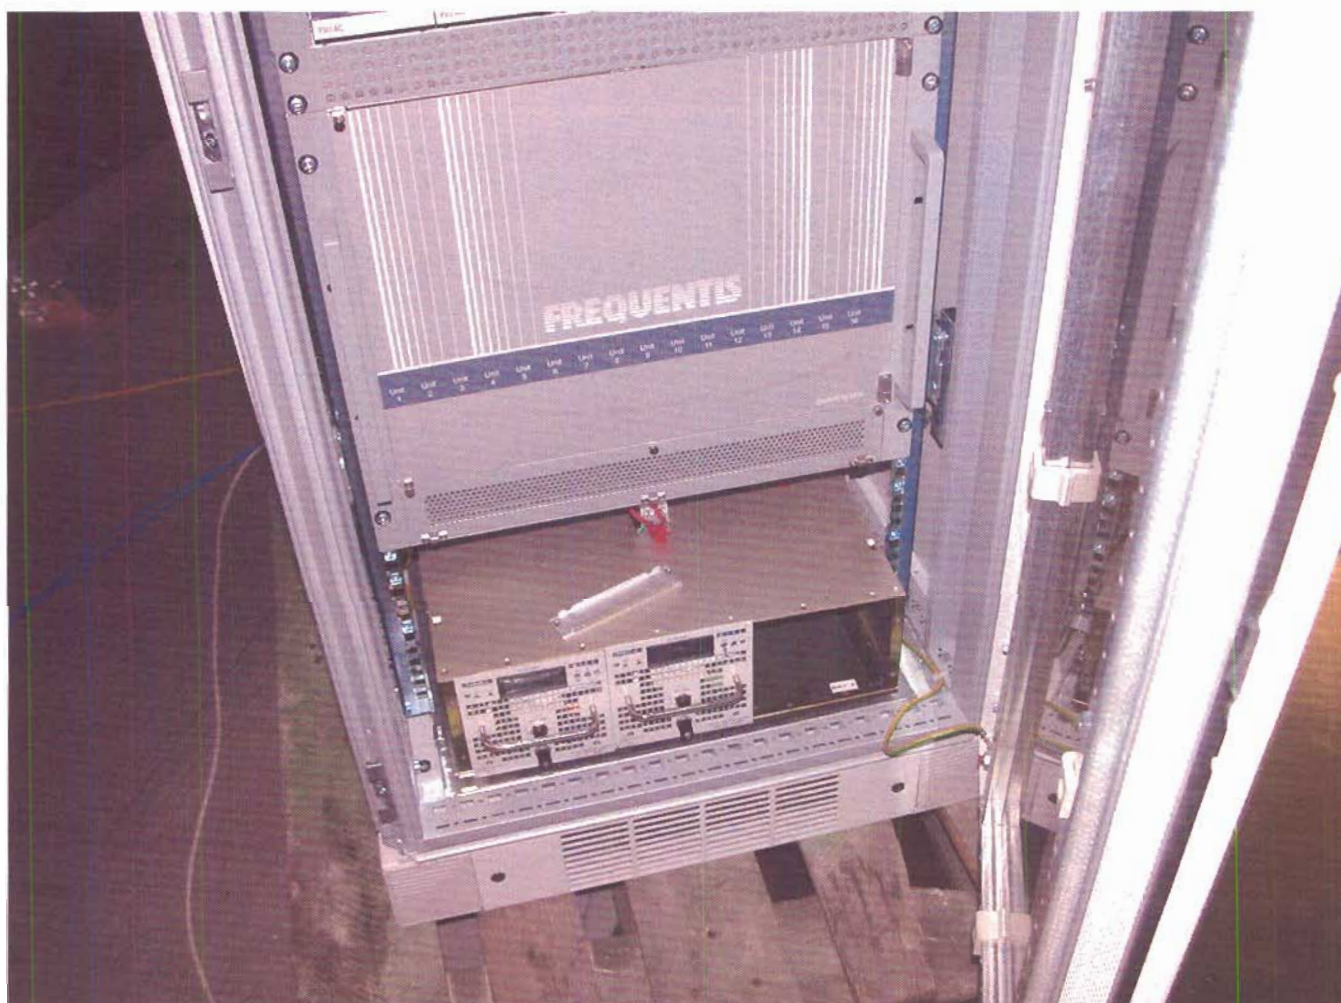



## Appendix 2 Photodocumentation

**Description:** 19" cabinet  
backside view with open door

Medizintechnik/Nach-  
richtentechnik/EMV


Department: EMC

Test report reference:  
M/EMV-05/141

Page: 5 of 36

Date: 31.05.2005

checked by: *M*

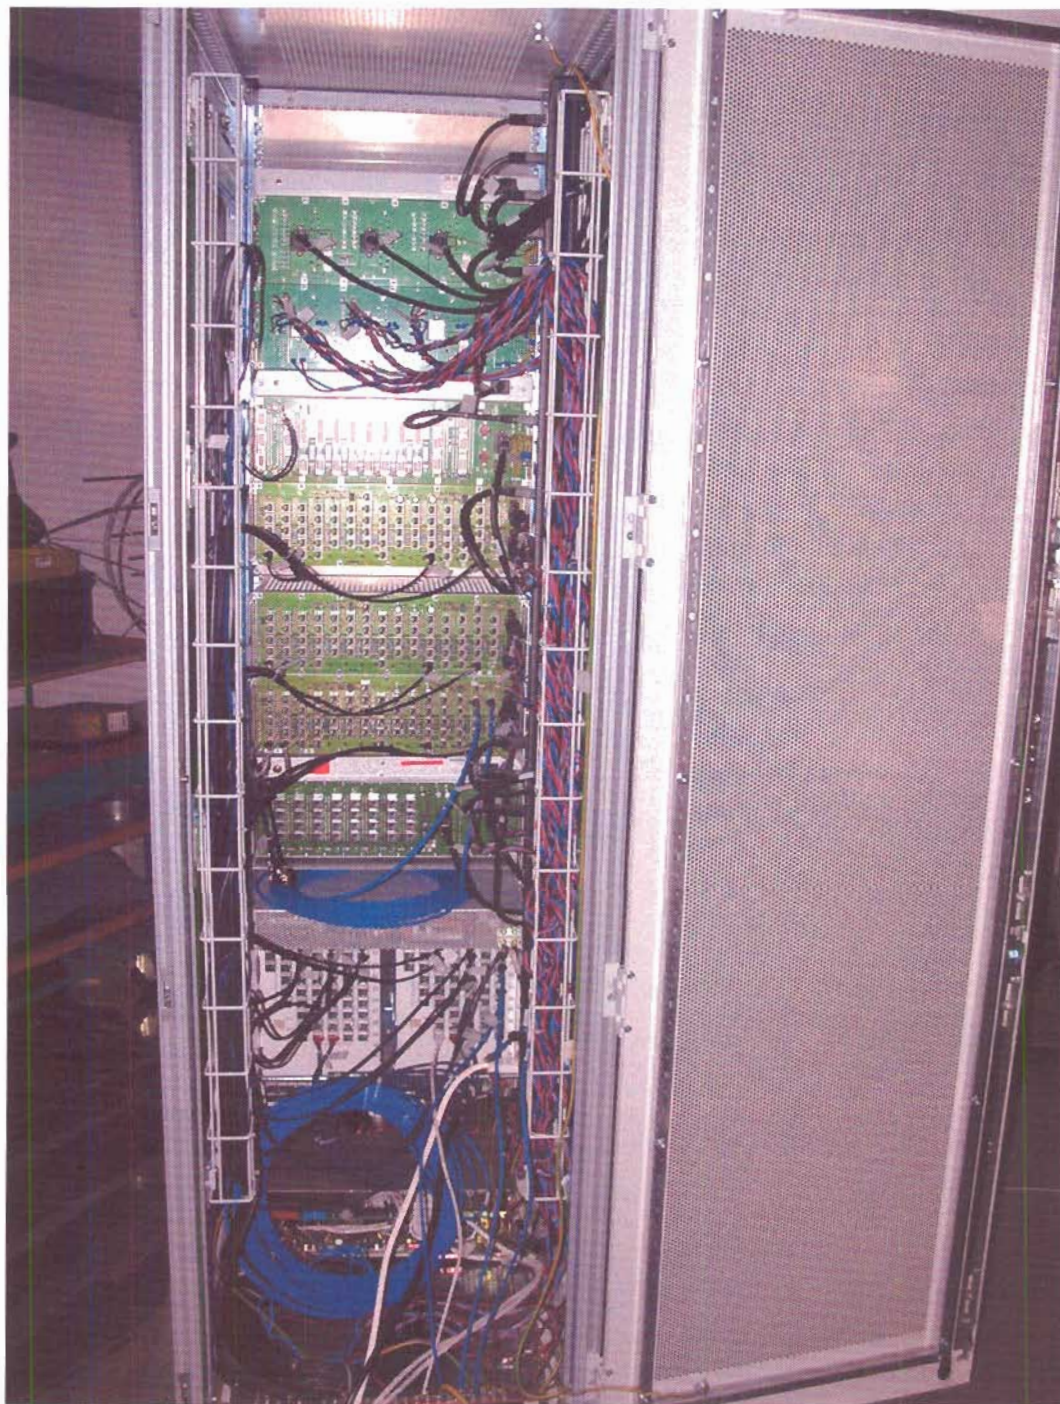


Medizintechnik/Nach-  
richtentechnik/EMV

Department: EMC

Test report reference:  
M/EMV-05/141

Page: 21 of 36

Date: 31.05.2005

checked by: 

## Appendix 2 Photodocumentation

**Description:** Operator positions EPOSA  
front view





## Appendix 2 Photodocumentation

**Description:** Operator positions EPOSA  
backside view

Medizintechnik/Nach-  
richtentechnik/EMV


Department: EMC

Test report reference:  
M/EMV-05/141

Page: 22 of 36

Date: 31.05.2005

checked by: *M*

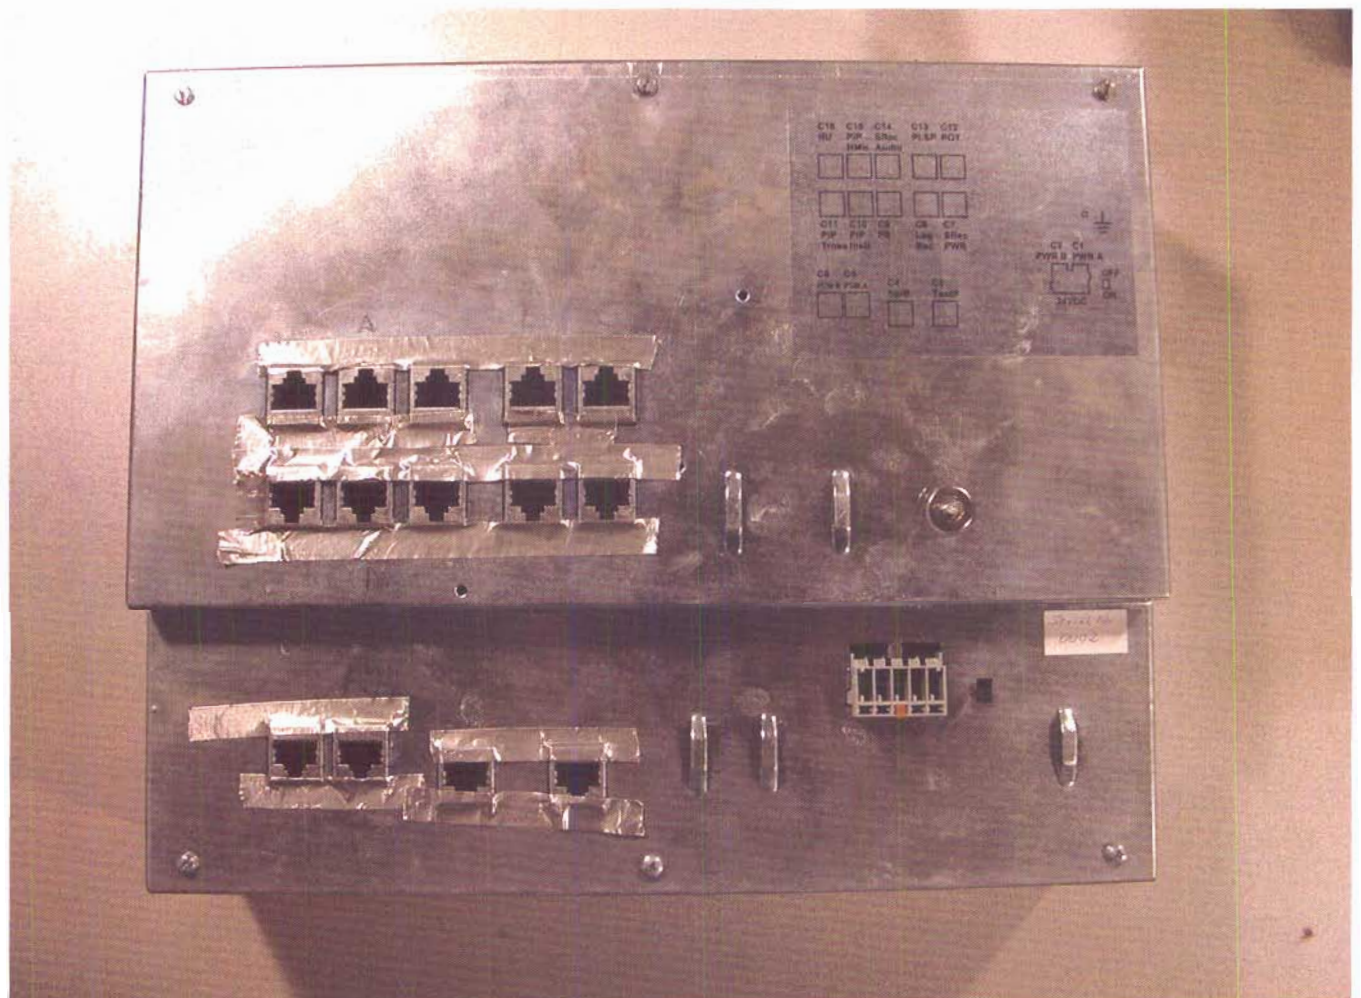

## Appendix 2 Photodocumentation

**Description:** Operator position C-POS 01  
front view

Medizintechnik/Nach-  
richtentechnik/EMV

Department: EMC

Test report reference:  
M/EMV-05/141

Page: 24 of 36

Date: 31.05.2005

checked by: 





## Appendix 2 Photodocumentation

**Description:** Operator position C-POS 01  
backside view

Medizintechnik/Nach-  
richtentechnik/EMV

Department: EMC

Test report reference:  
M/EMV-05/141

Page 25 of 36

Date: 31.05.2005

checked by: M

