

Appendix 2 Photodocumentation

Description: 19" cabinet backside detail view #1

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference
M/EMV-05/141

Page: 6 of 36

Date: 31.05.2005

checked by: M

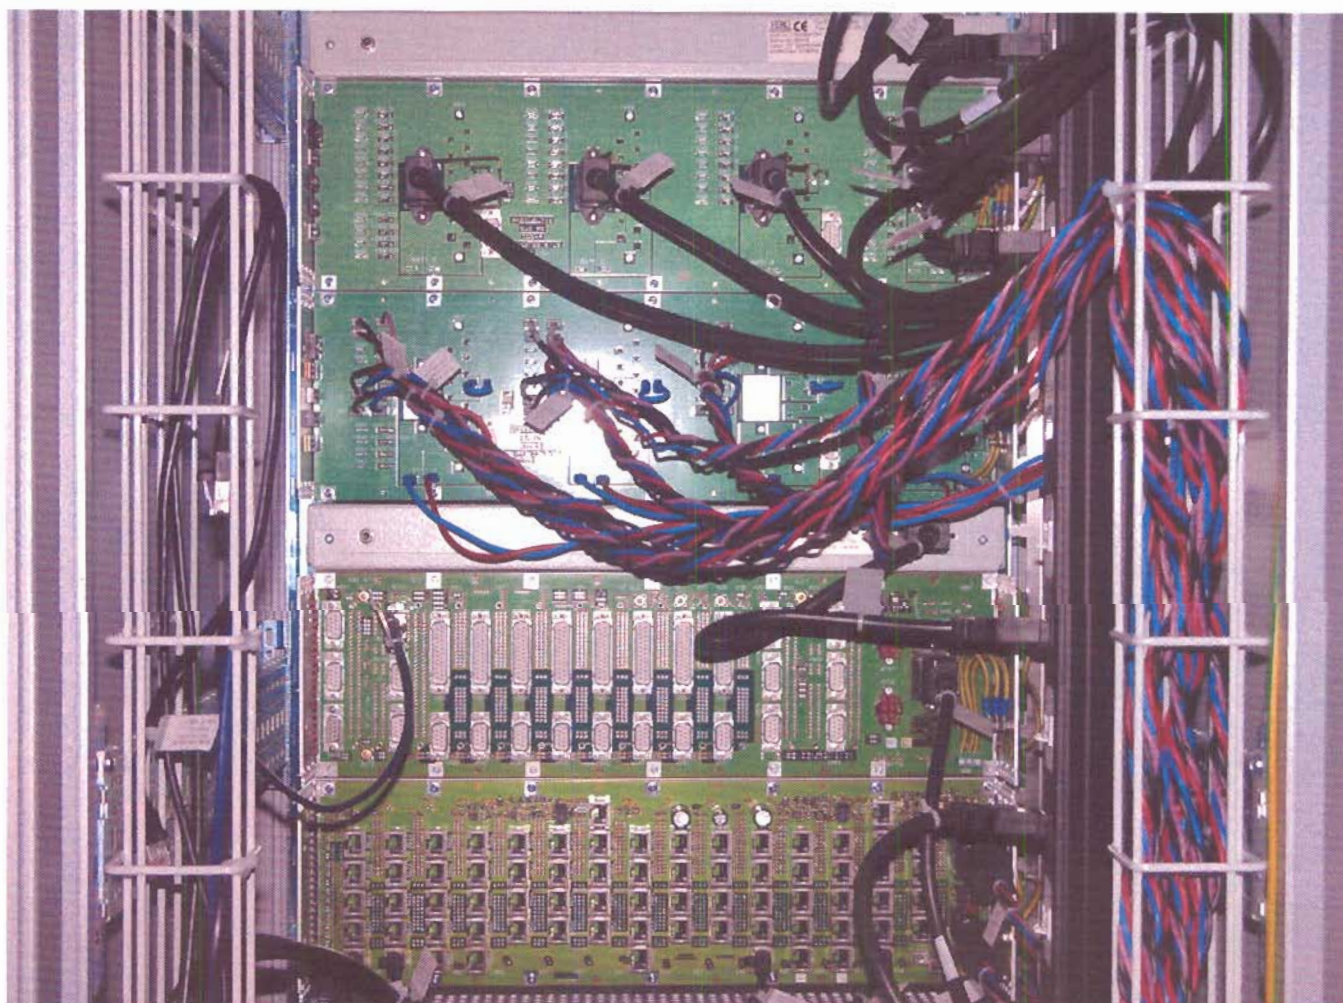

Appendix 2 Photodocumentation

Description: 19" cabinet backside detail view #2

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 7 of 36

Date: 31.05.2005

checked by: M

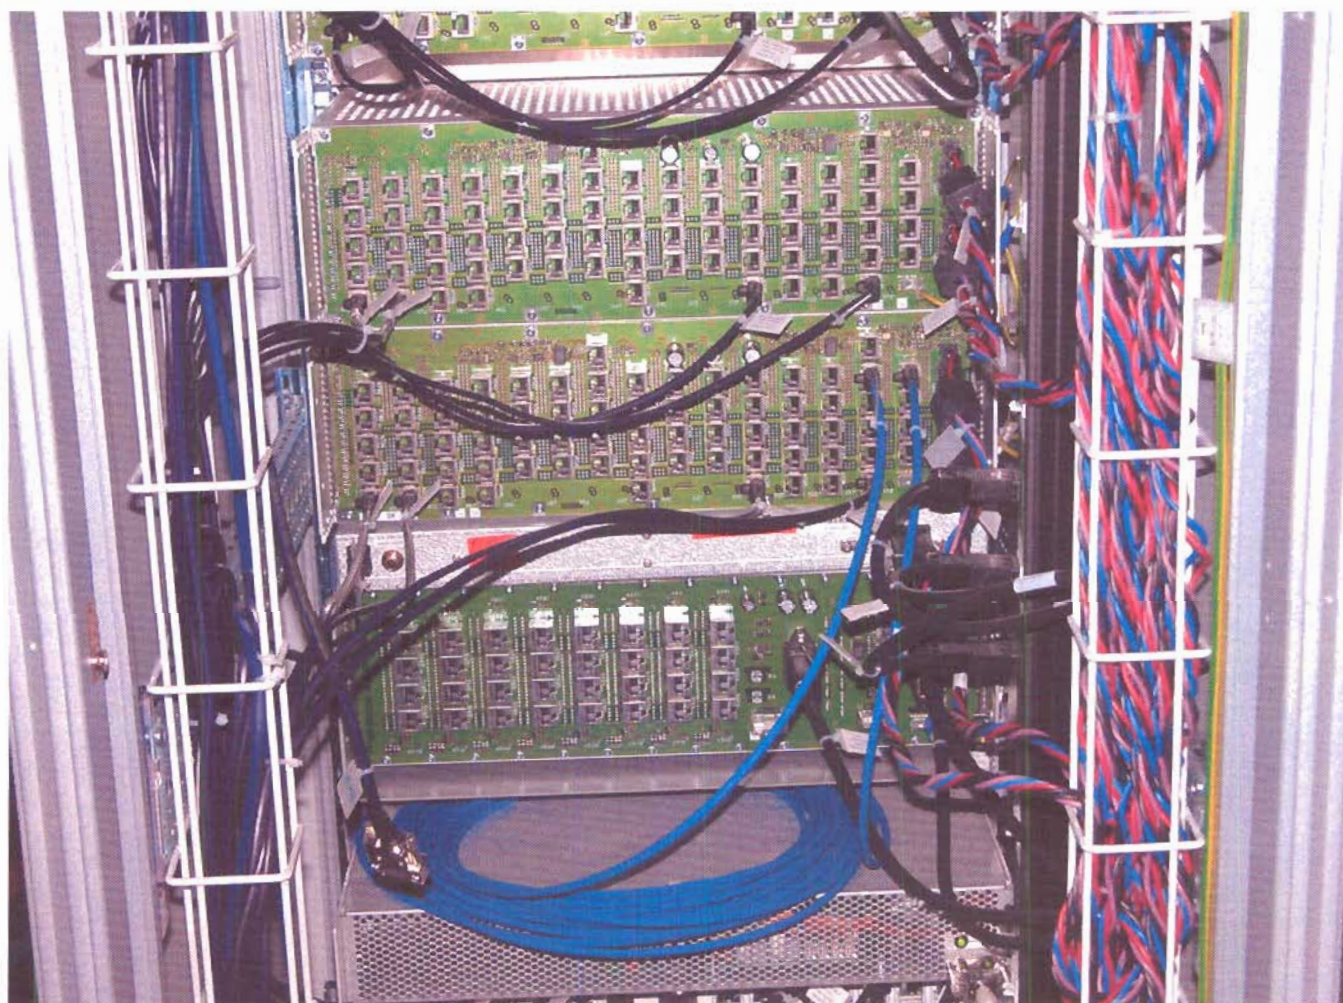

Appendix 2 Photodocumentation

Description: 19" cabinet backside detail view #3

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 8 of 36

Date: 31.05.2005

checked by: M

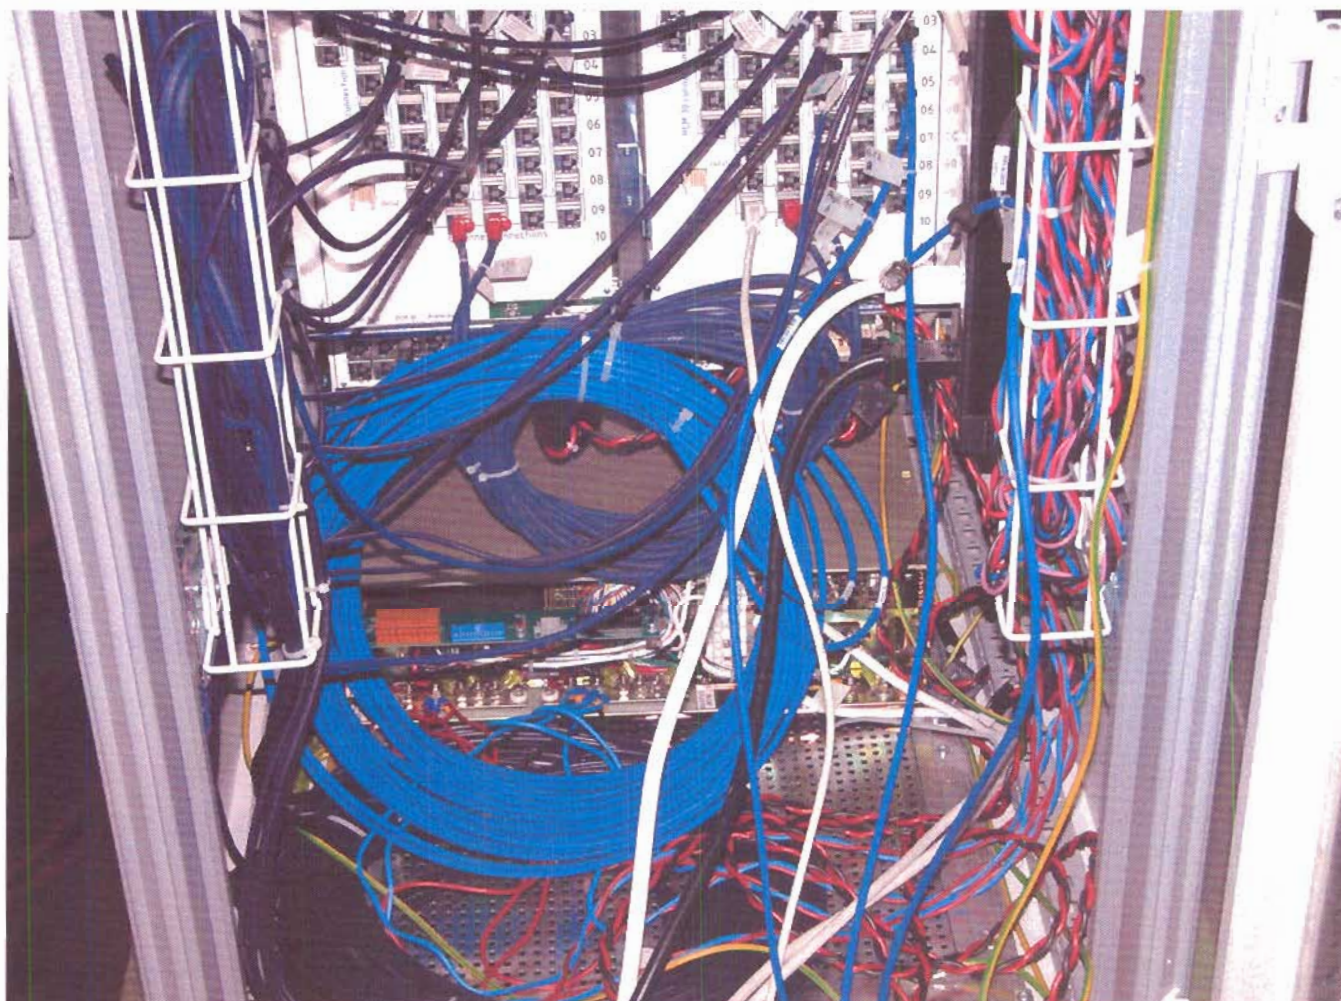

Appendix 2 Photodocumentation

Description: Interface BCA 03.00 view #1


Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 9 of 36

Date: 31.05.2005

checked by: 

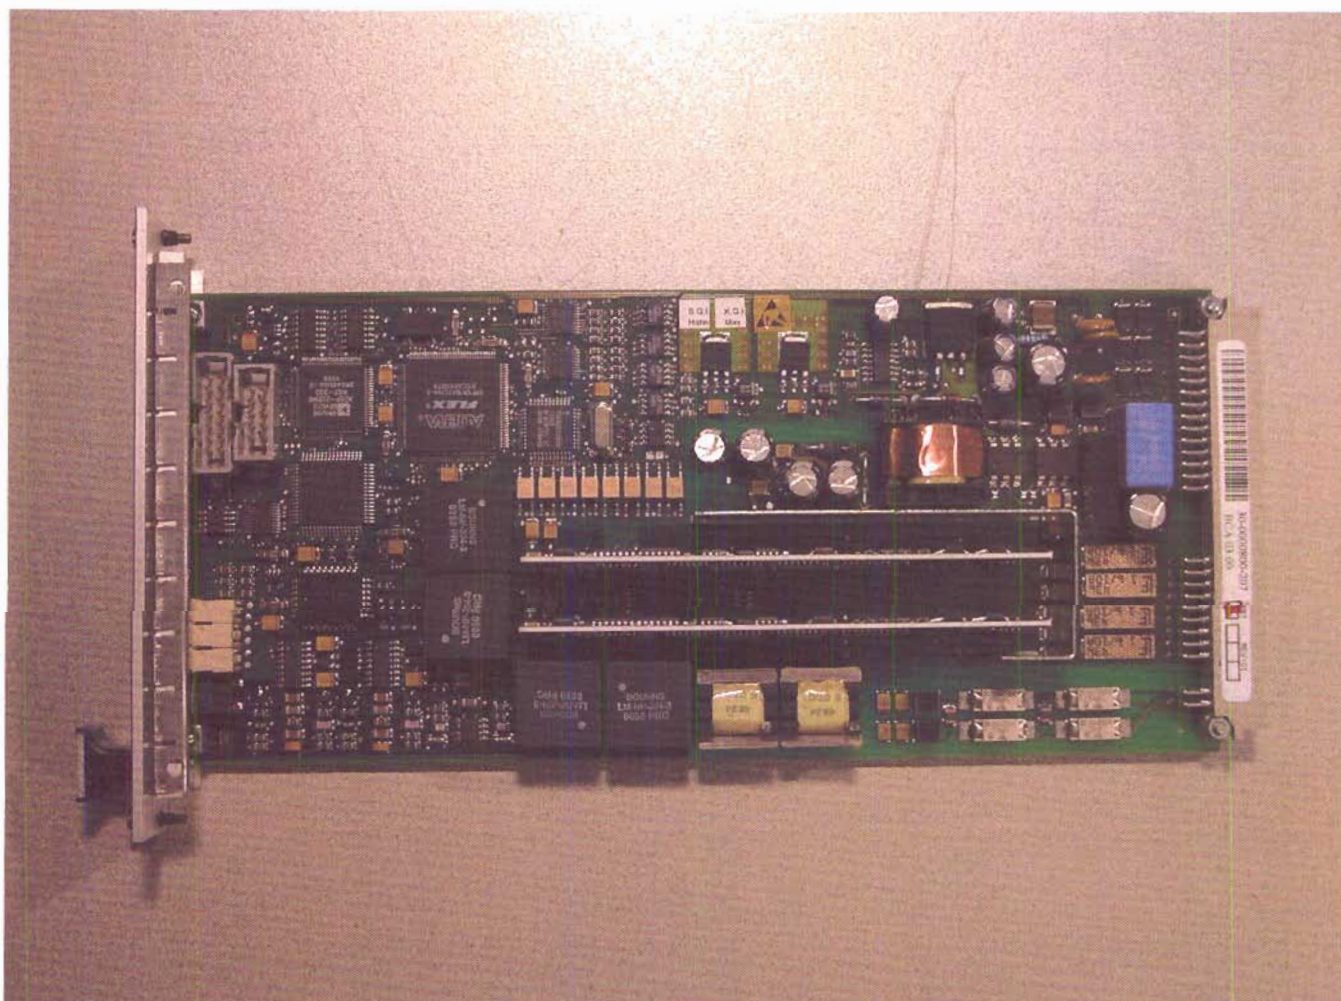

Appendix 2 Photodocumentation

Description: Interface BCA 03.00 view #2

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 10 of 36

Date: 31.05.2005

checked by: M

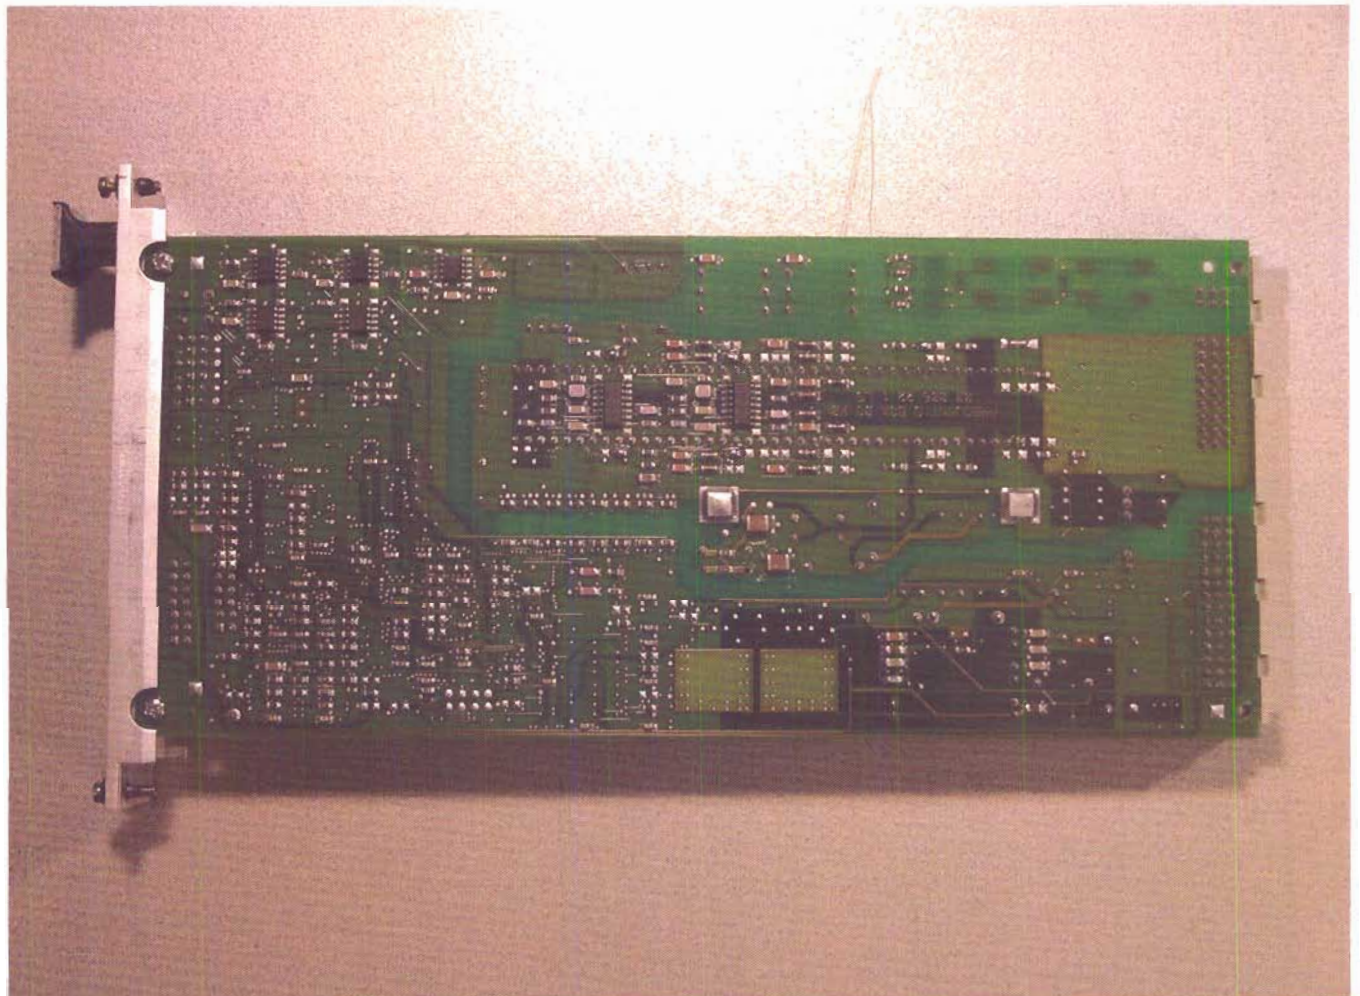

Appendix 2 Photodocumentation

Description: Interface BCB 03.00 view #1

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 11 of 36

Date: 31.05.2005

checked by: *M*

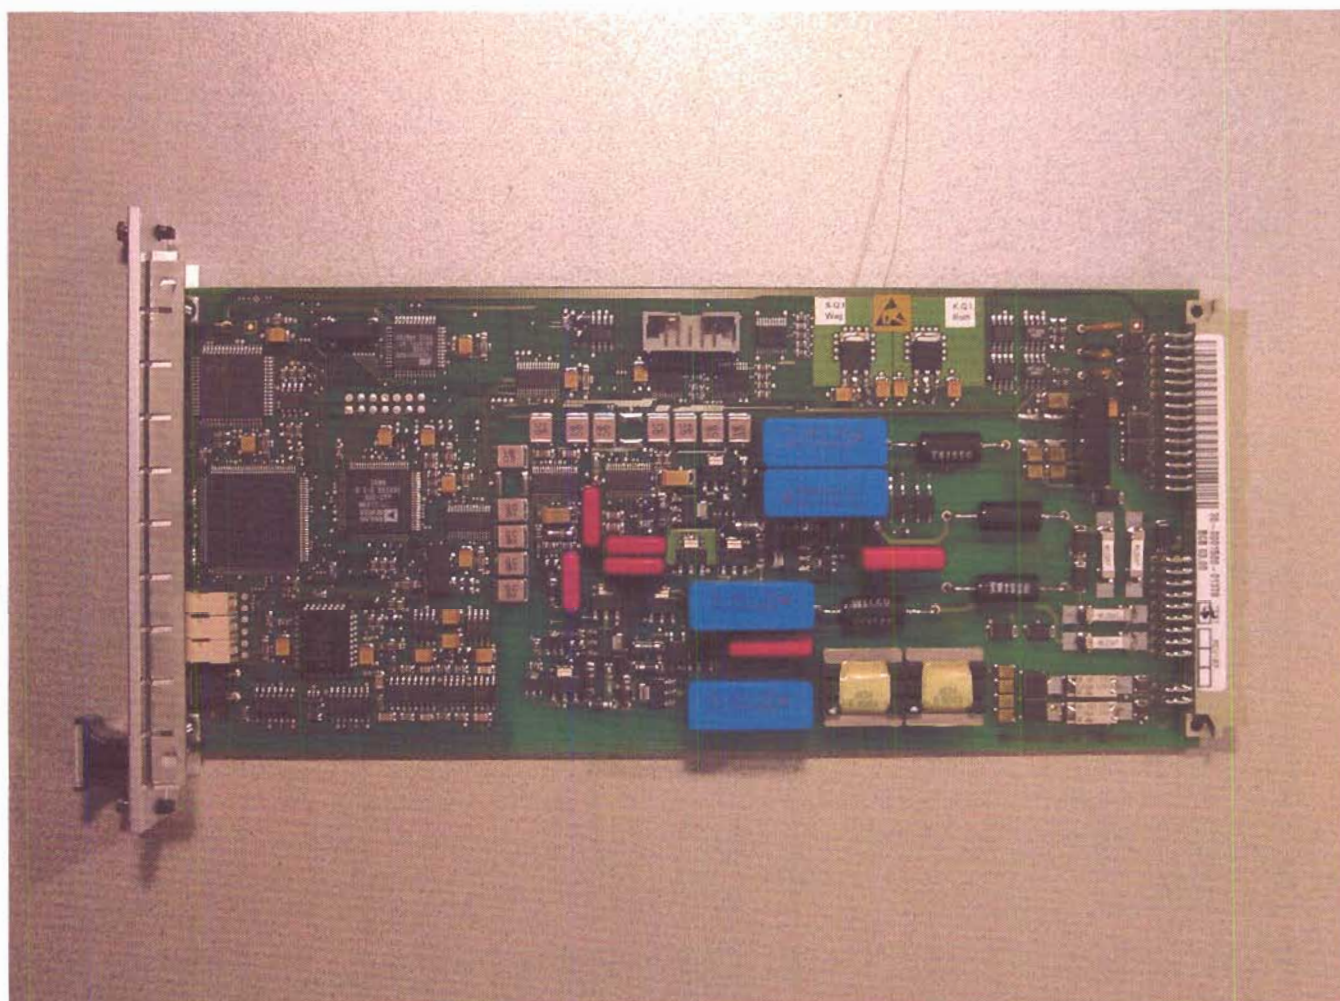

Appendix 2 Photodocumentation

Description: Interface BCB 03.00 view #2

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page 12 of 36

Date: 31.05.2005

checked by M

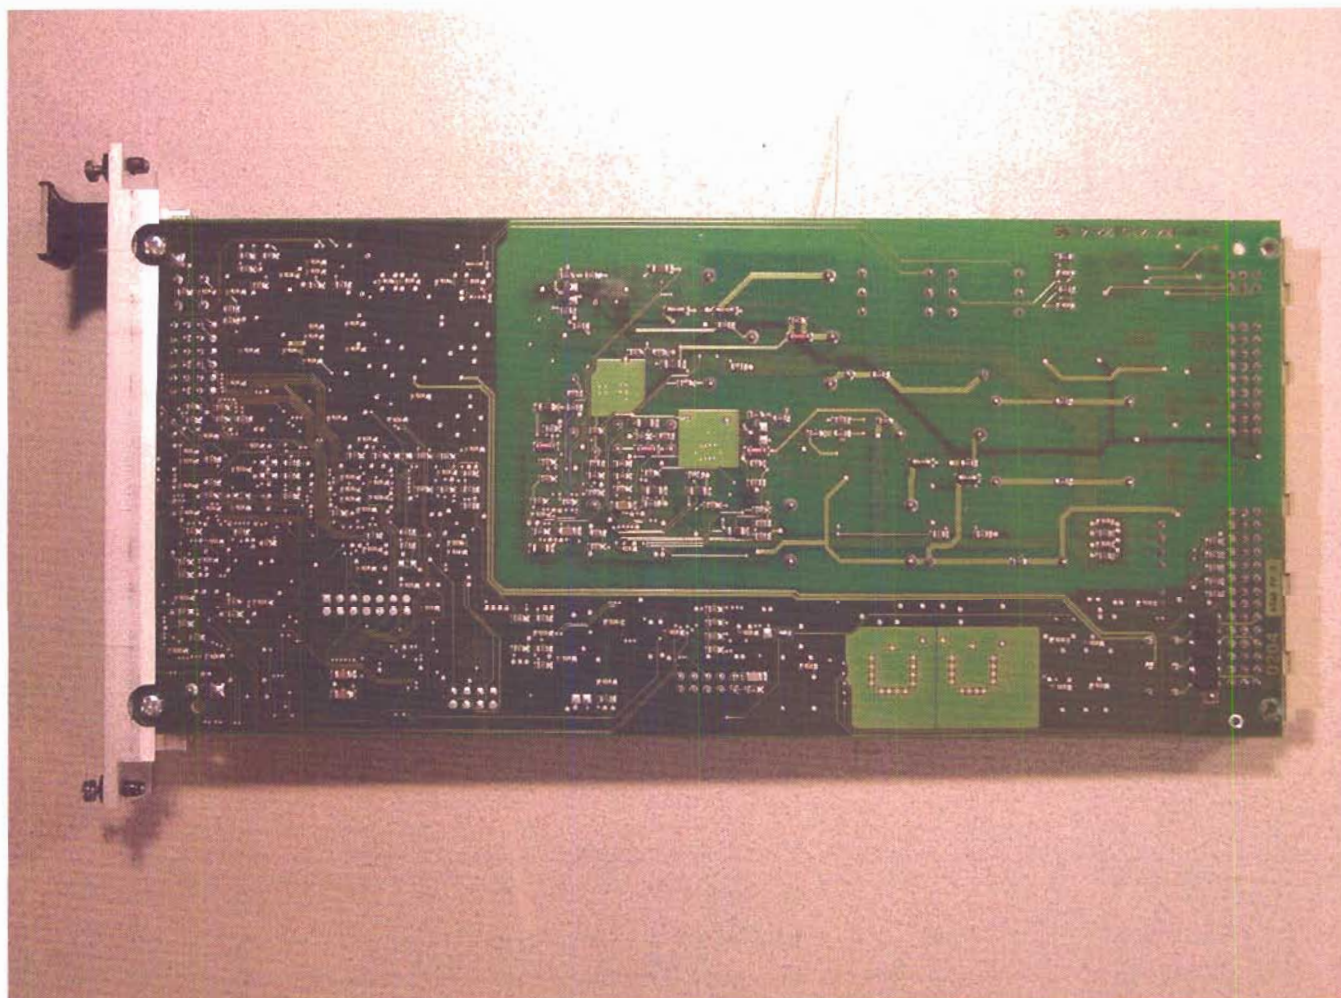

Appendix 2 Photodocumentation

Description: Interface ERIF 03.00 view #1

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 13 of 36

Date: 31.05.2005

checked by: M

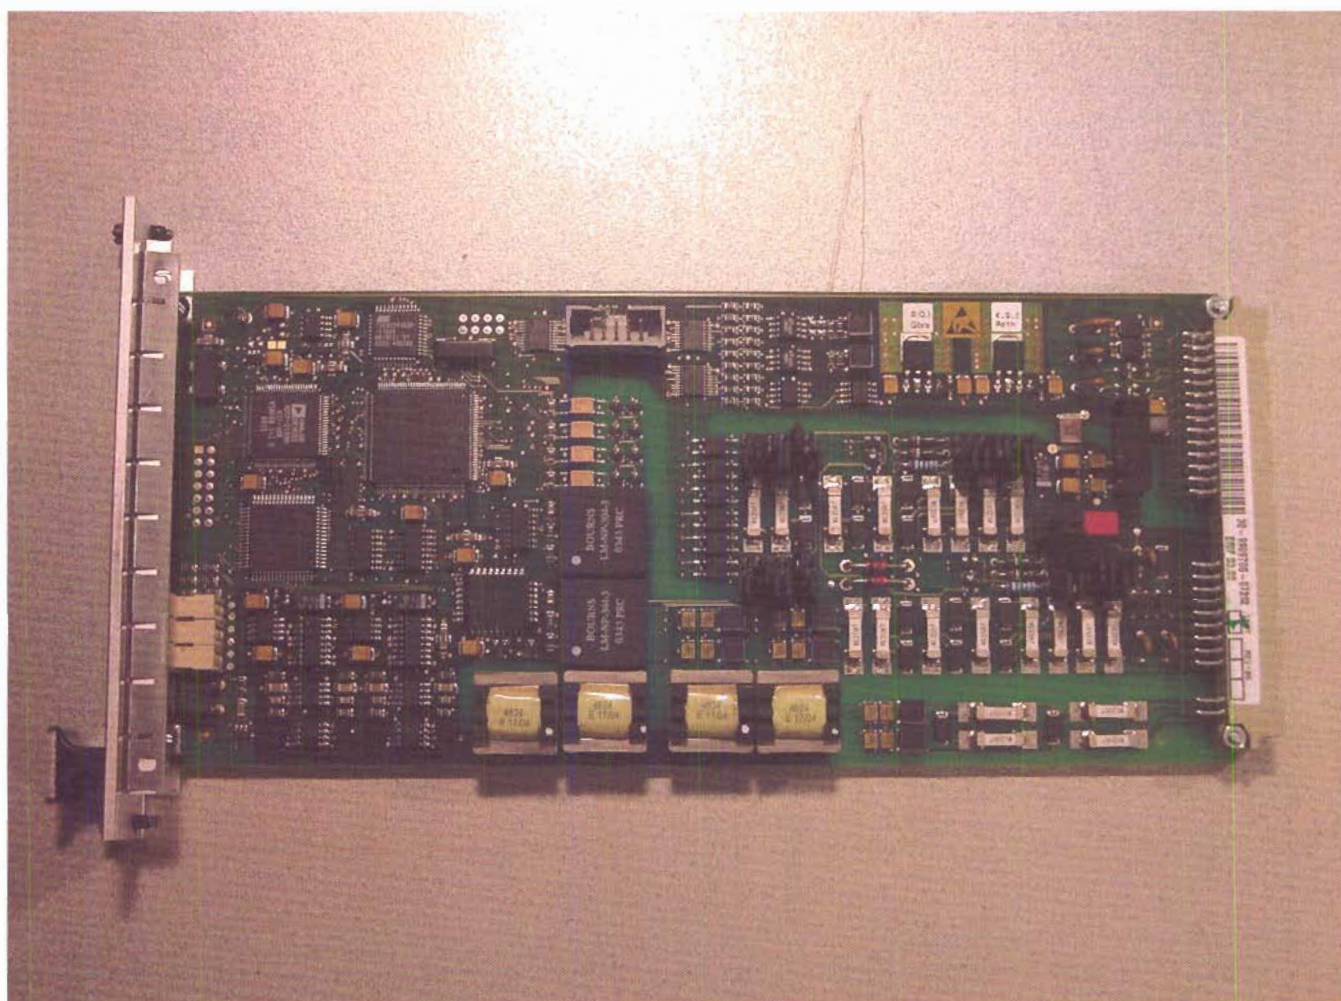

Appendix 2 Photodocumentation

Description: Interface ERIF 03.00 view #2

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 14 of 36

Date: 31.05.2005

checked by: 

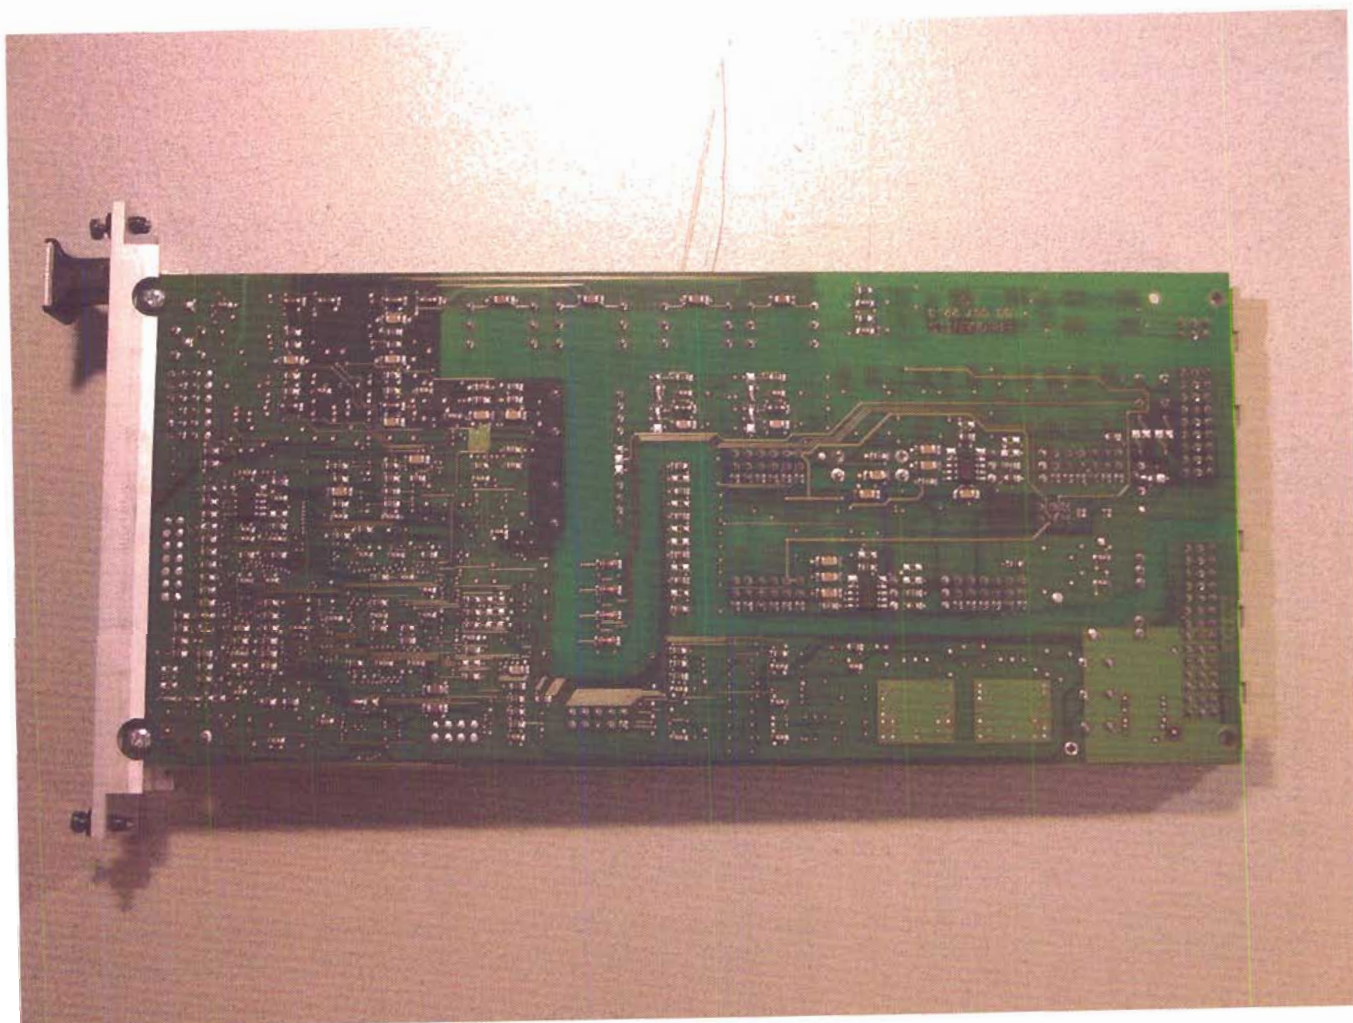

Appendix 2 Photodocumentation

Description: Interface GPIF 03.01 view #1

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 15 of 36

Date: 31.05.2005

checked by: M

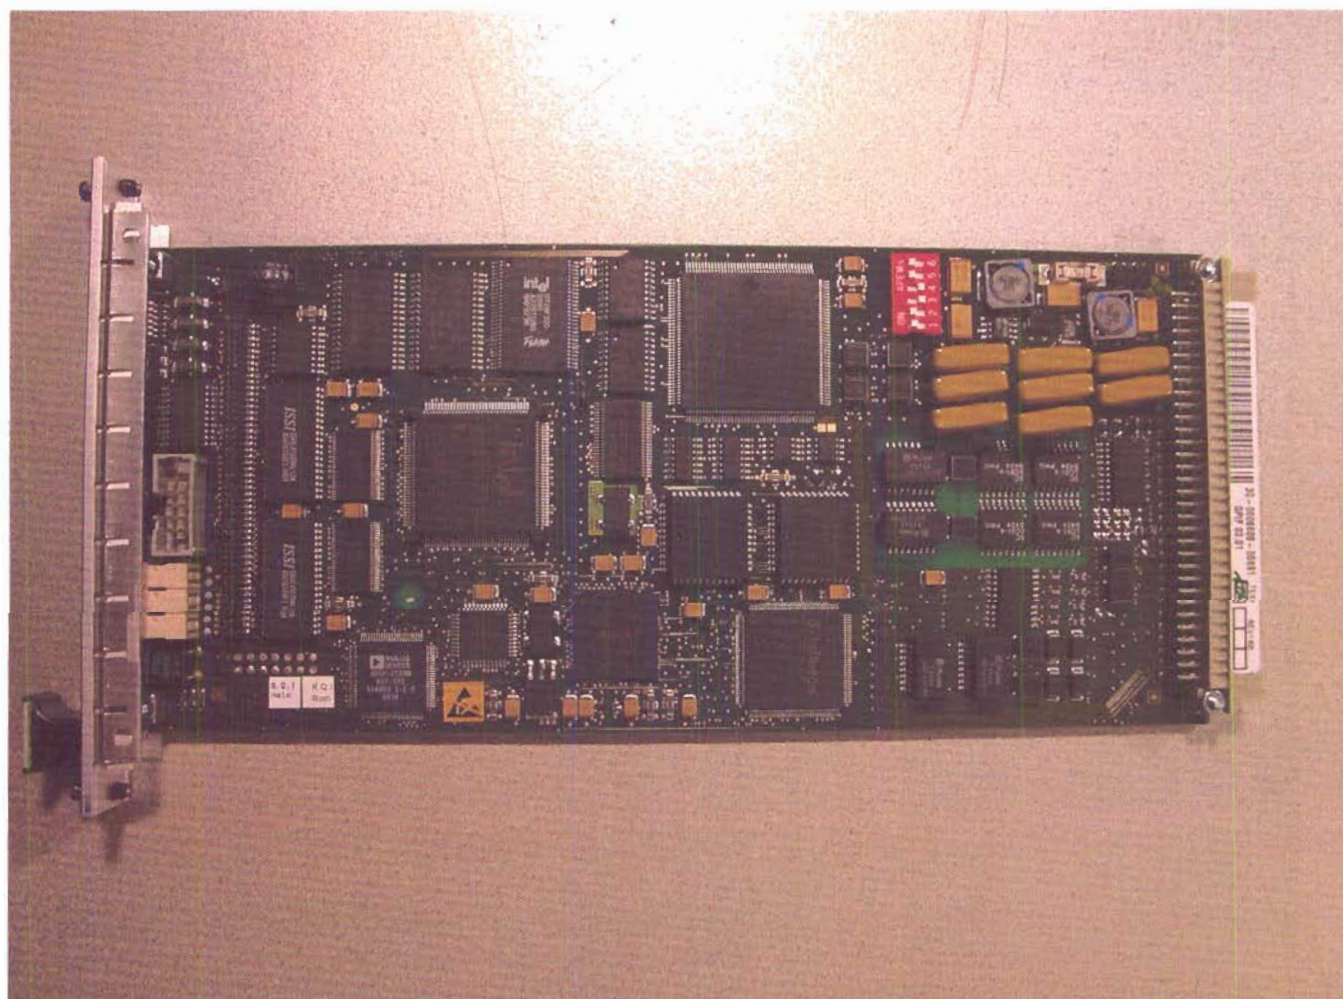

Appendix 2 Photodocumentation

Description: Interface GPIF 03.01 view #2

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 16 of 36

Date: 31.05.2005

checked by: 

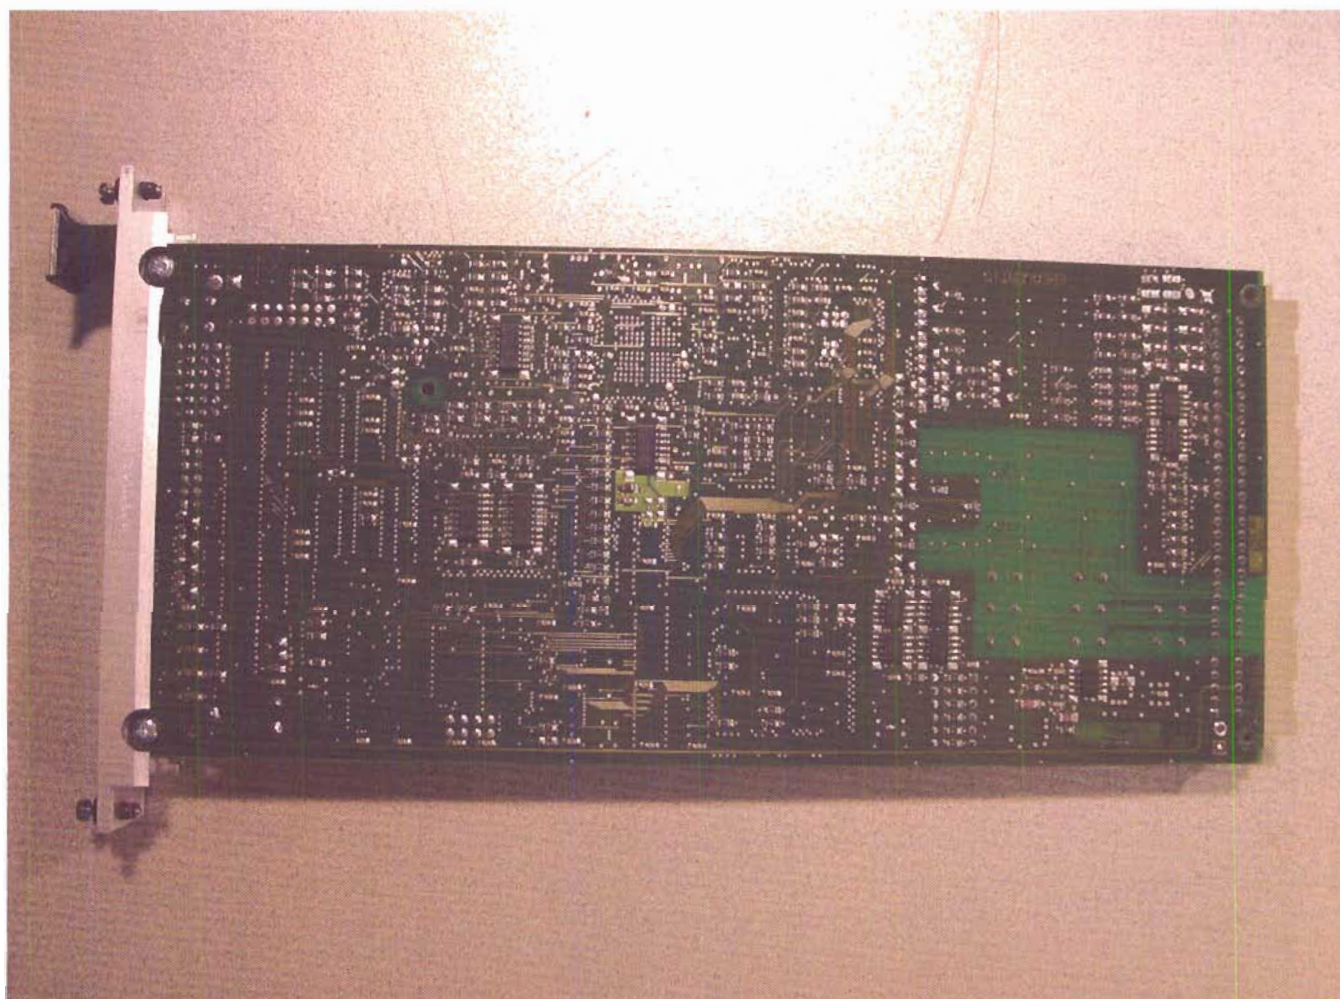

Appendix 2 Photodocumentation

Description: Interface LB 03.00 view #1

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference
M/EMV-05/141

Page: 17 of 36

Date: 31.05.2005

checked by: *M*

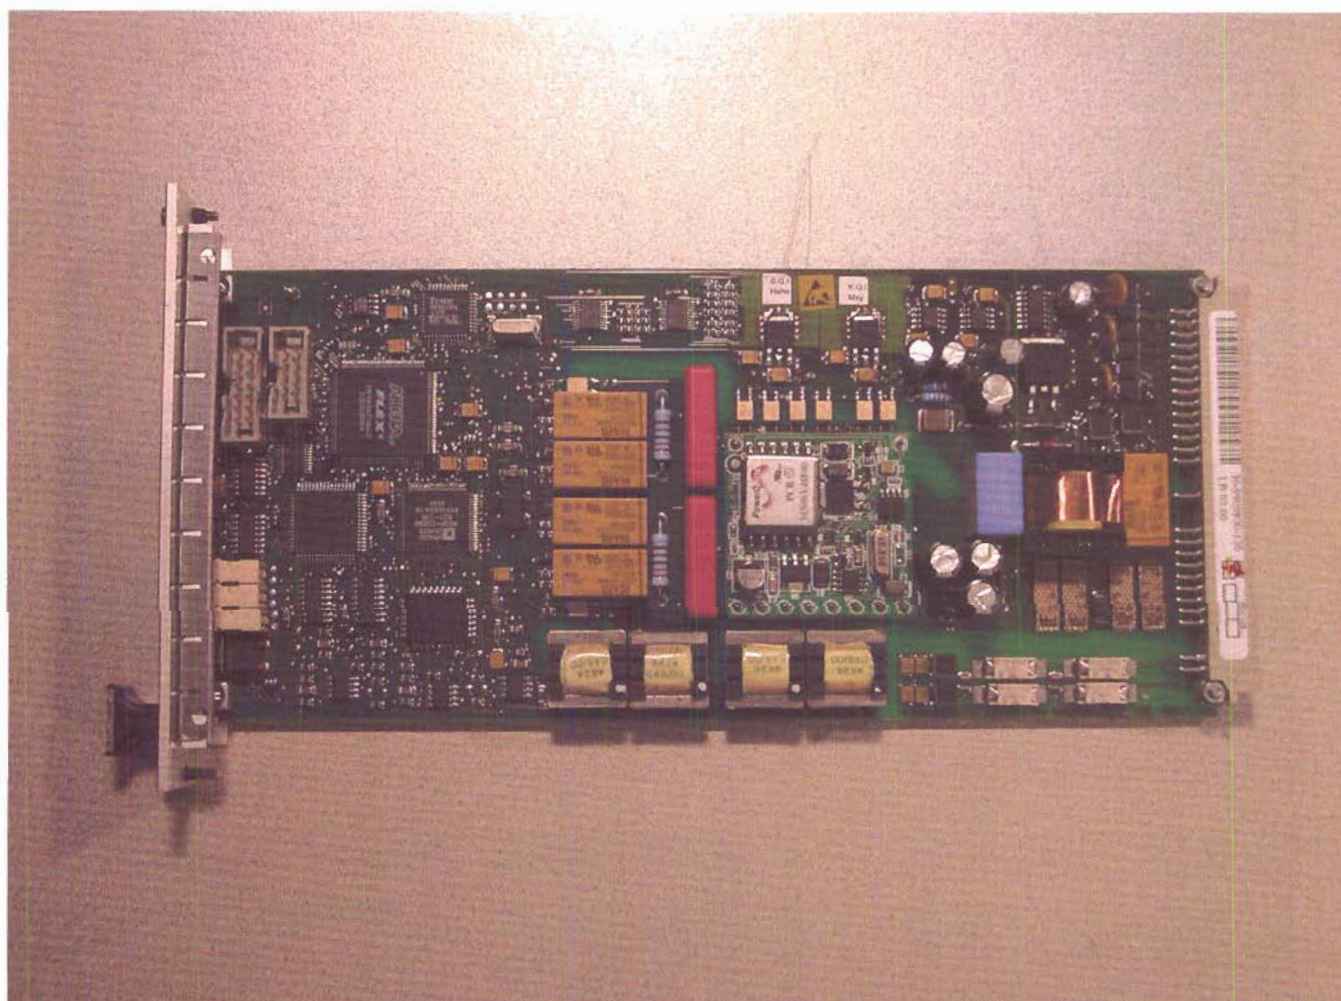

Appendix 2 Photodocumentation

Description: Interface LB 03.00 view #2

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 18 of 36

Date: 31.05.2005

checked by: M

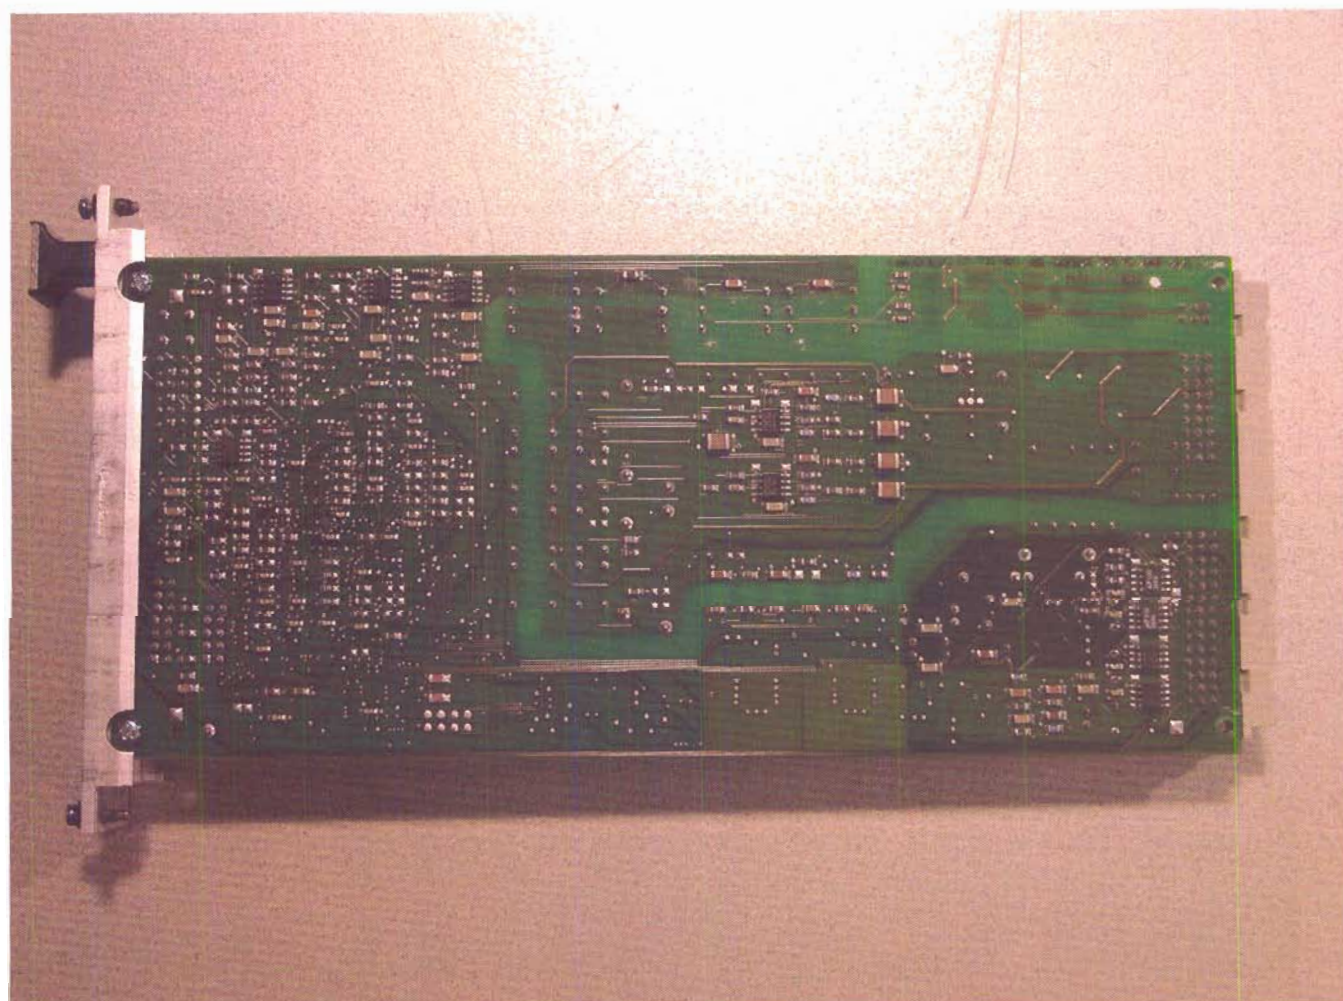

Appendix 2 Photodocumentation

Description: Interface T0 03.00 view #1

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 19 of 36

Date: 31.05.2005

checked by: M

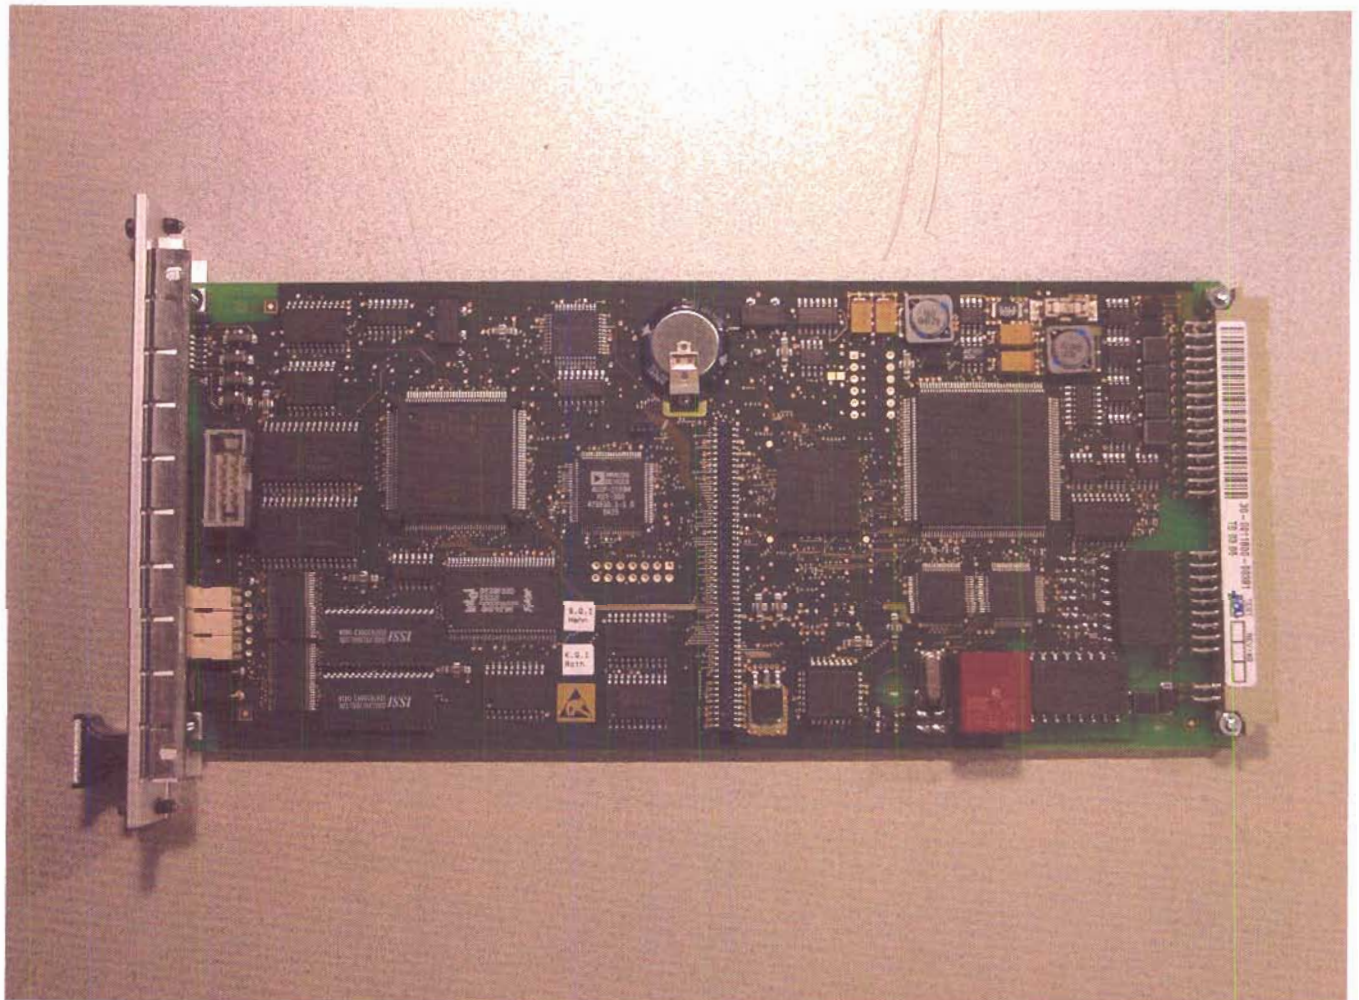

Appendix 2 Photodocumentation

Description: Interface T0 03.00 view #2

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 20 of 36

Date: 31.05.2005

checked by: M

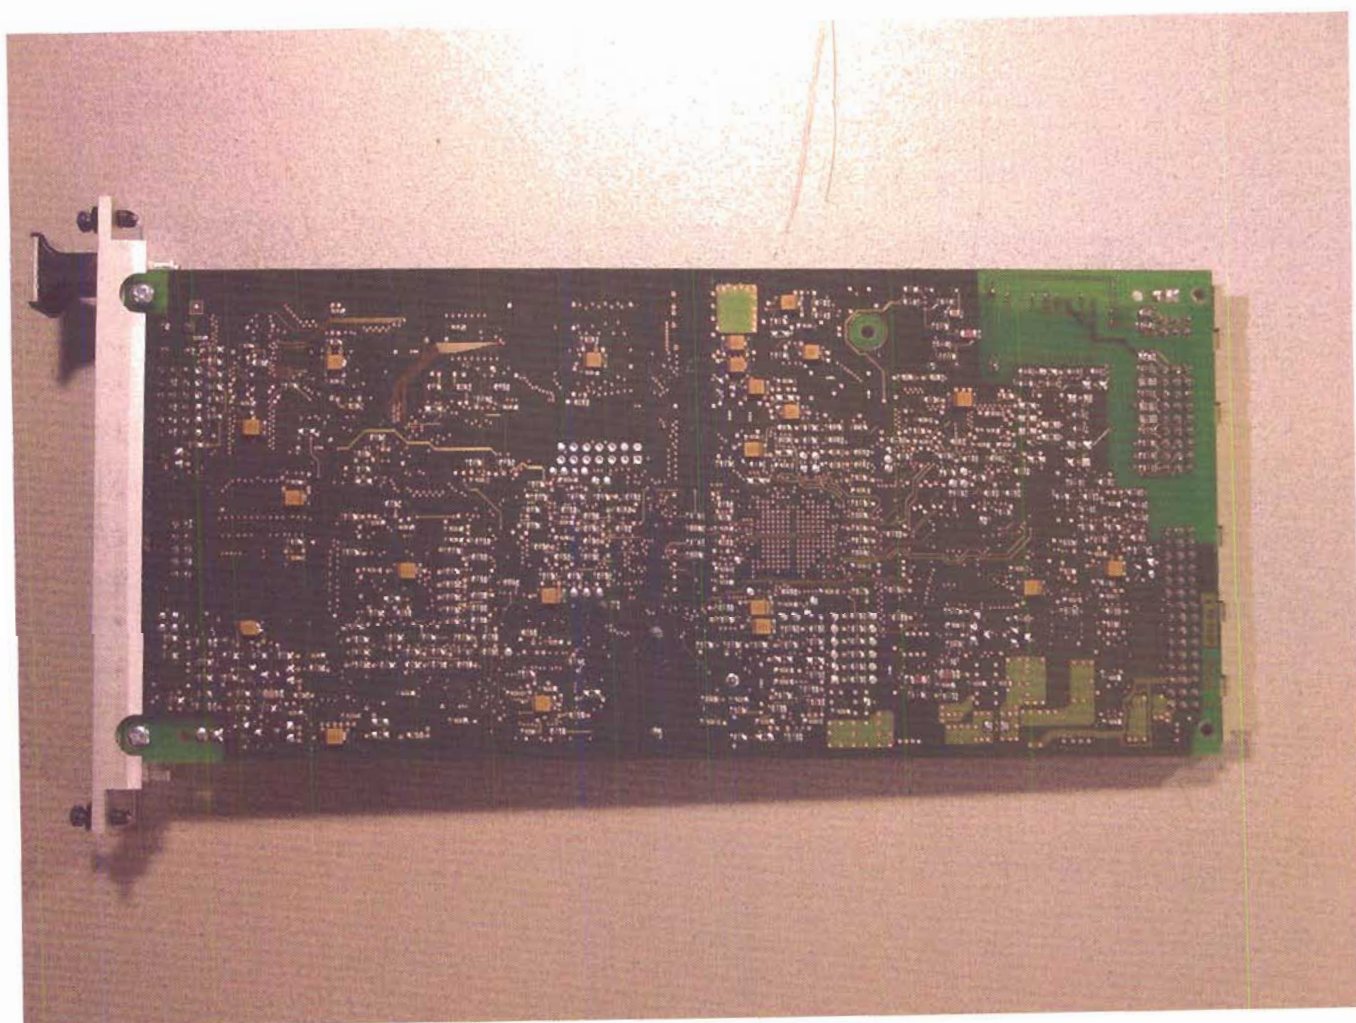

Appendix 2 Photodocumentation

Description: Operator positions EPOSA
open view


Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/141

Page: 23 of 36

Date: 31.05.2005

checked by: 

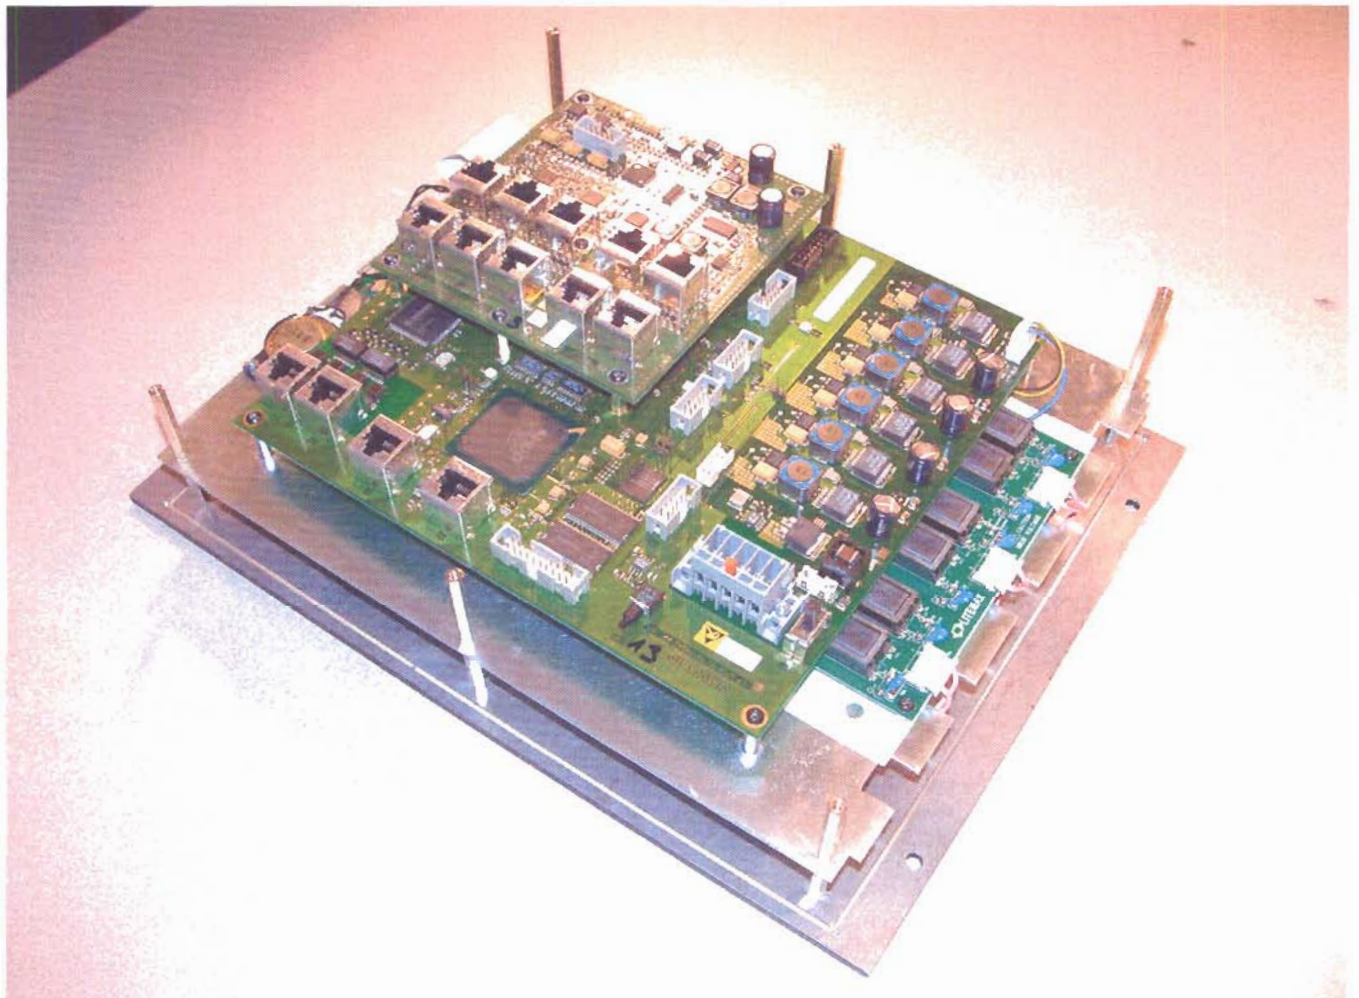

Appendix 2 Photodocumentation

Description: Operator position C-POS 01
open view

