


Date: Monday, January 02, 2006


SmartStep™ – V2.1.1-A2

Internal Photograph:

The Bluetooth Module front panel:

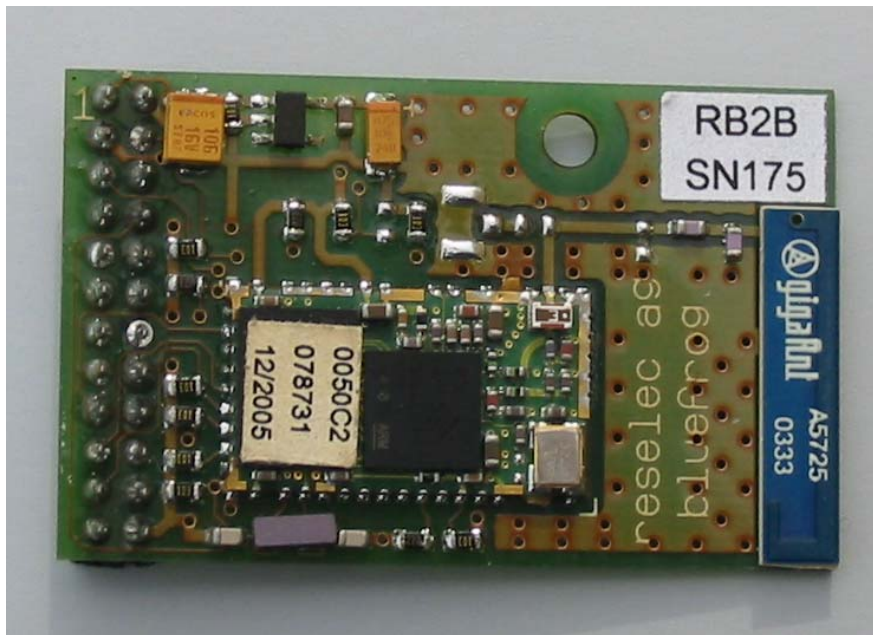

The Bluetooth Module rear panel:

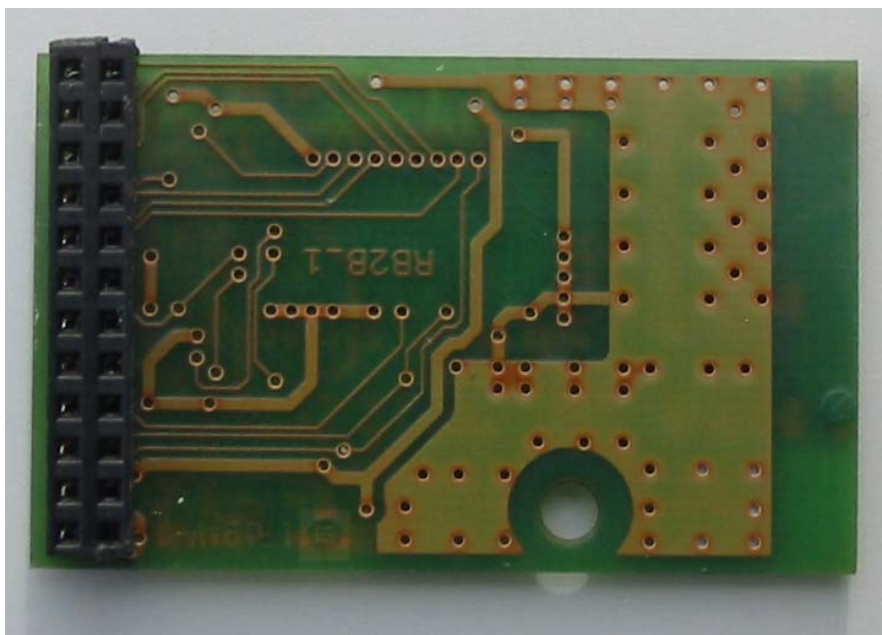


ANDANTE - MEDICAL DEVICES LTD.

P.O.Box 3023 Omer Industrial Park 84965, Building 8b


TEL: +972-8-6900027, FAX: +972-8-6900319

andante@actcom.co.il

SmartStep Main Bord Back Panel:

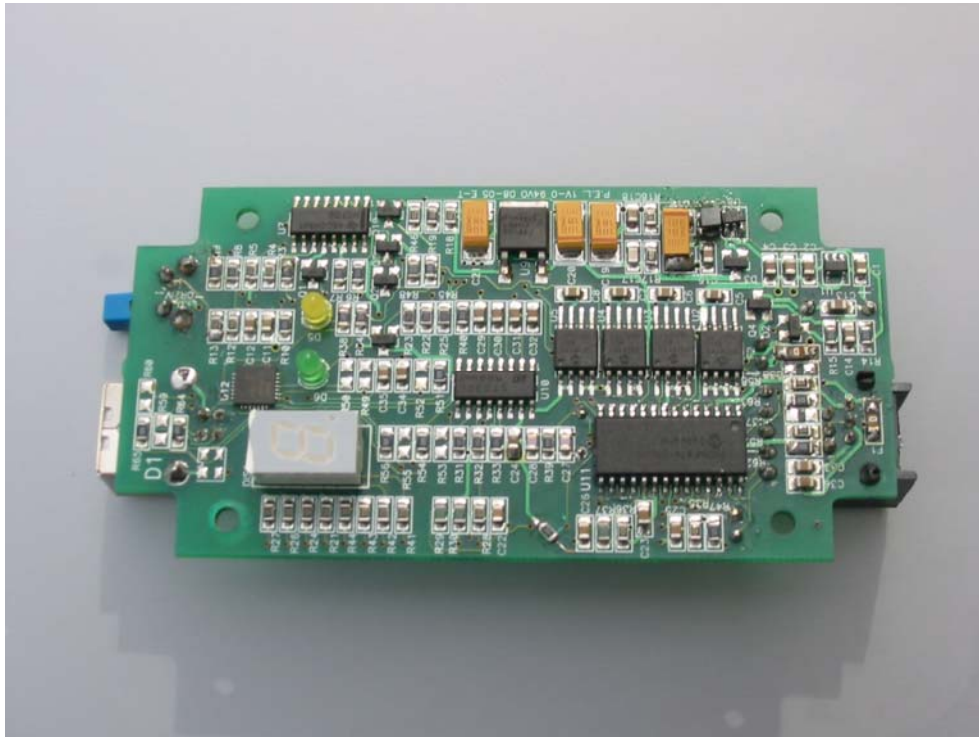

SmartStep Main Bord Front Panel:

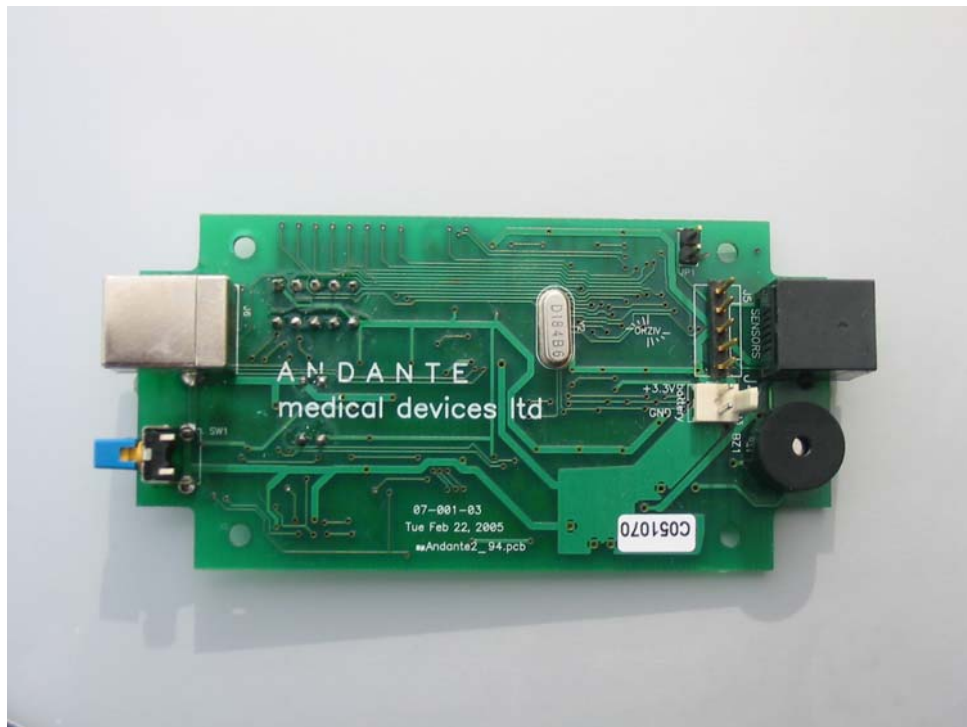

ANDANTE - MEDICAL DEVICES LTD.

P.O.Box 3023 Omer Industrial Park 84965, Building 8b

TEL: +972-8-6900027, FAX: +972-8-6900319

andante@actcom.co.il

SmartStep – Bluetooth module & Main Board:




ANDANTE - MEDICAL DEVICES LTD.

P.O.Box 3023 Omer Industrial Park 84965, Building 8b


TEL: +972-8-6900027, FAX: +972-8-6900319

andante@actcom.co.il

The following image shows the control unit connected to the mechanical connection of the control box:

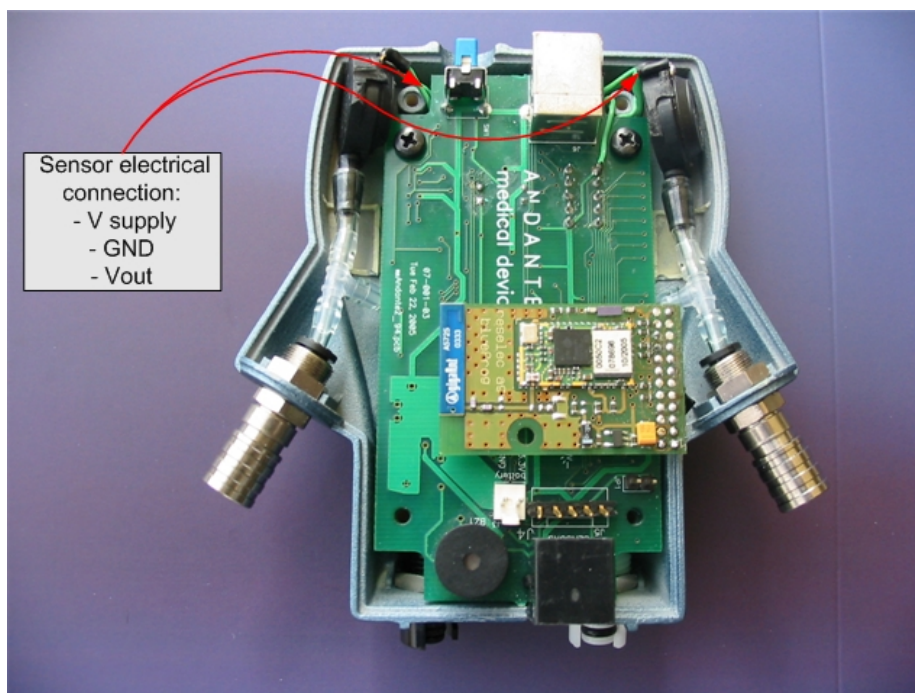

The following image shows the control unit and the Bluetooth from the rear side:

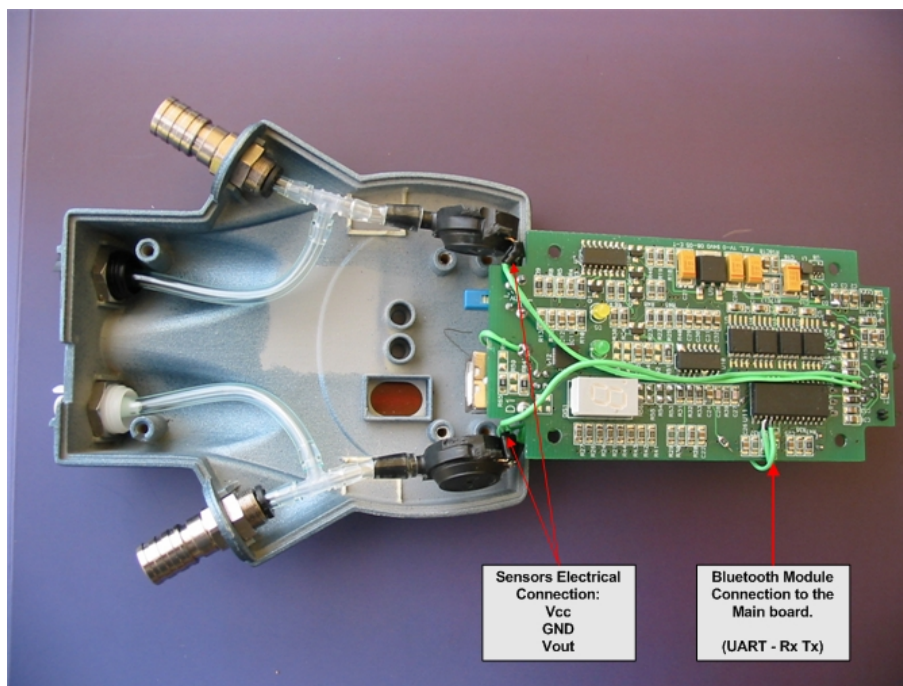

ANDANTE - MEDICAL DEVICES LTD.

P.O.Box 3023 Omer Industrial Park 84965, Building 8b

TEL: +972-8-6900027, FAX: +972-8-6900319

andante@actcom.co.il