



This is previous page plot (zoom in)

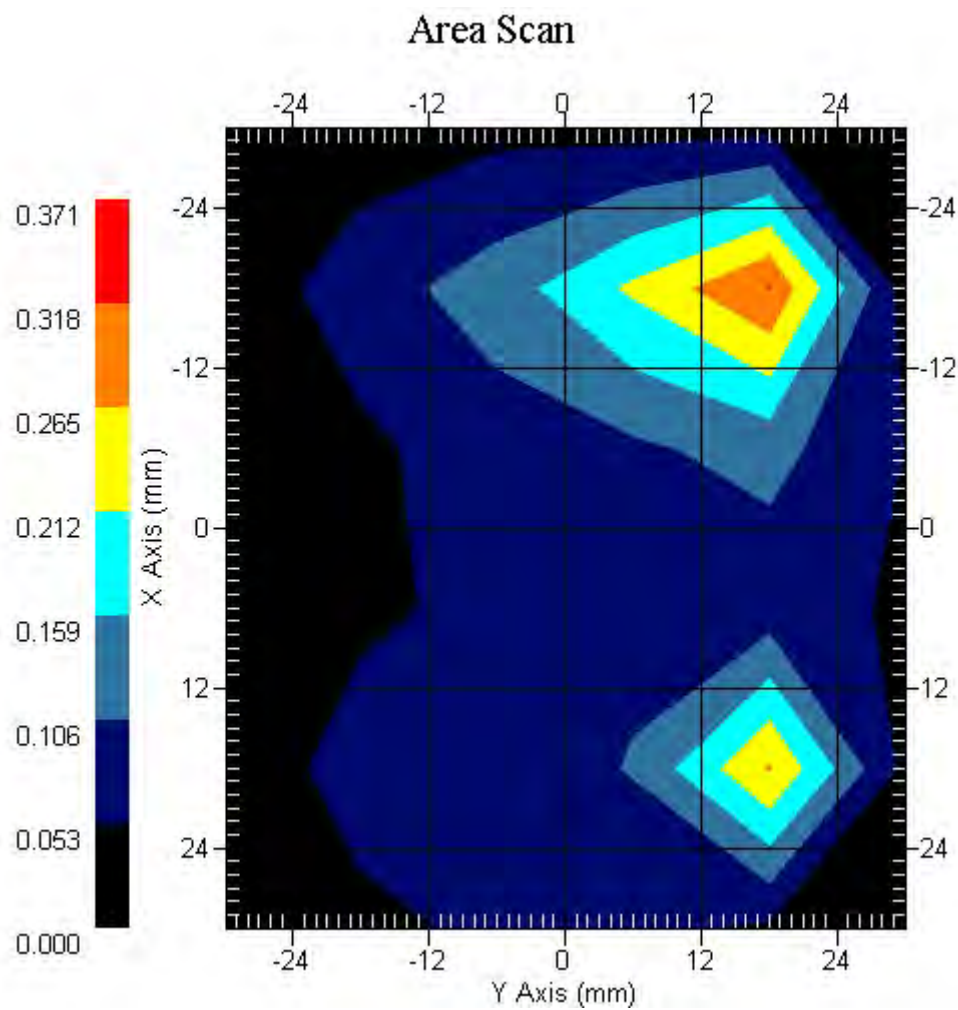

## Measurement Data


Crest Factor : 1  
 Tissue Temp. : 20.90 °C  
 Ambient Temp. : 21.60 °C  
 Area Scan : 6x6x1 : Measurement x=12mm, y=12mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm  
 Power Drift-Start : 0.043 W/kg  
 Power Drift-Finish: 0.042 W/kg  
 Power Drift (%) : -2.334

DUT Position : 15° Tilt  
 Channel : 1014

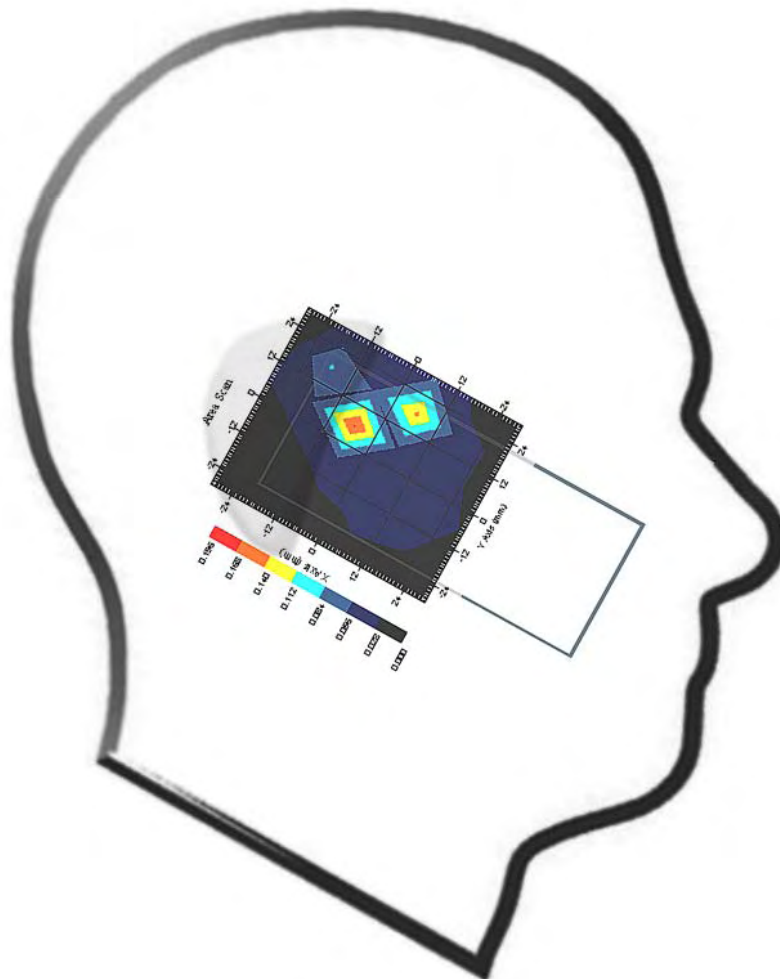

1 gram SAR value : 0.117 W/kg  
 10 gram SAR value : 0.056 W/kg  
 Area Scan Peak SAR : 0.169 W/kg  
 Zoom Scan Peak SAR : 0.330 W/kg


This is previous page plot (zoom in)

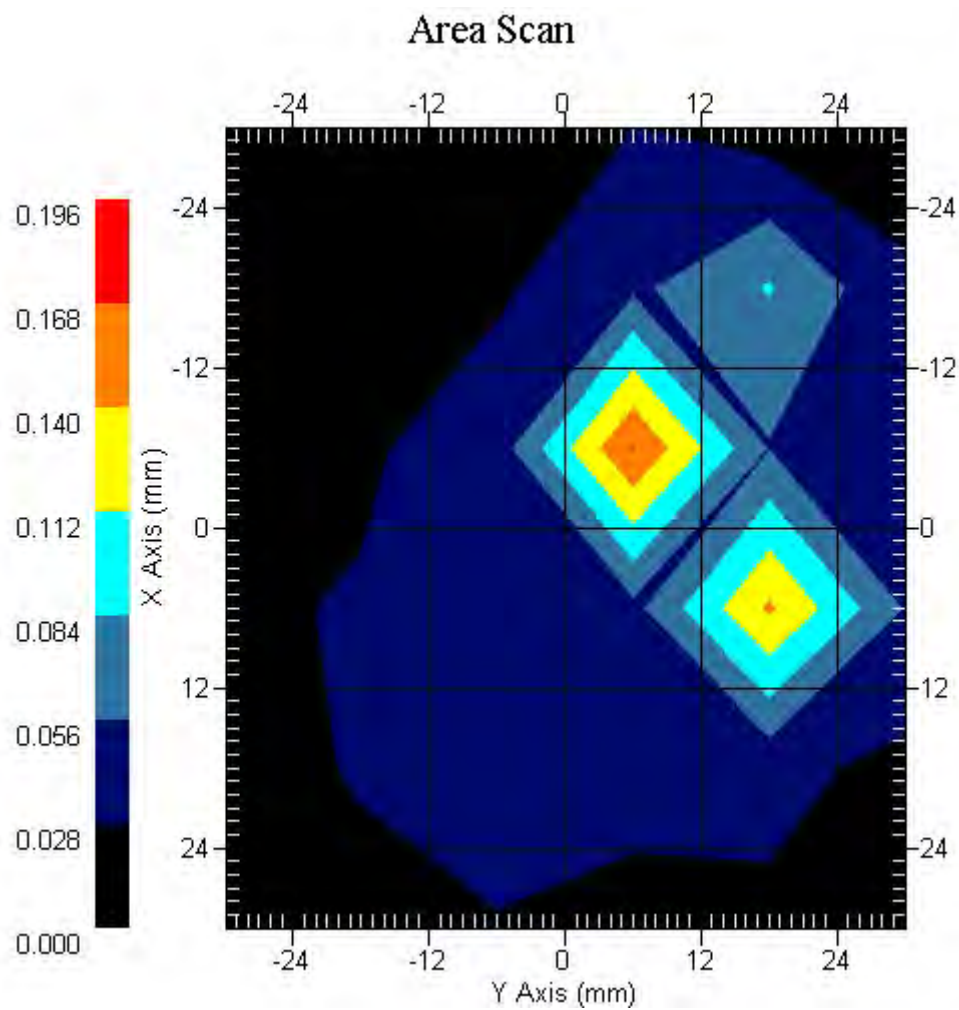

## Measurement Data


Crest Factor : 1  
 Tissue Temp. : 20.90 °C  
 Ambient Temp. : 21.60 °C  
 Area Scan : 6x6x1 : Measurement x=12mm, y=12mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm  
 Power Drift-Start : 0.059 W/kg  
 Power Drift-Finish: 0.058 W/kg  
 Power Drift (%) : -1.648

DUT Position : 15° Tilt  
 Channel : 380

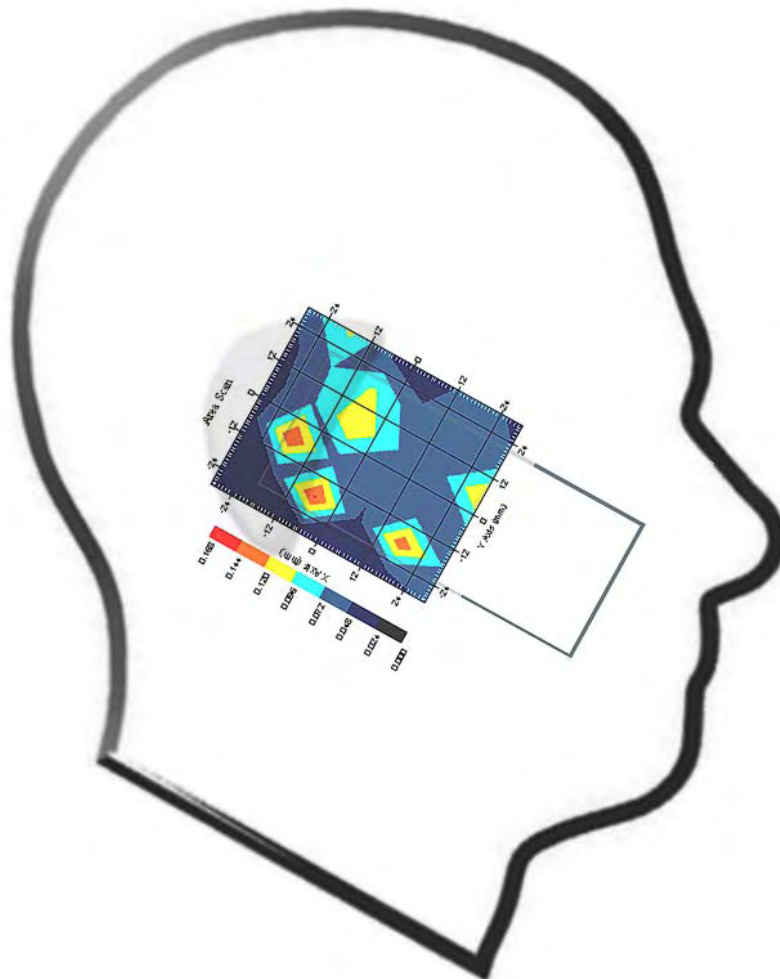

1 gram SAR value : 0.113 W/kg  
 10 gram SAR value : 0.060 W/kg  
 Area Scan Peak SAR : 0.147 W/kg  
 Zoom Scan Peak SAR : 0.340 W/kg


This is previous page plot (zoom in)

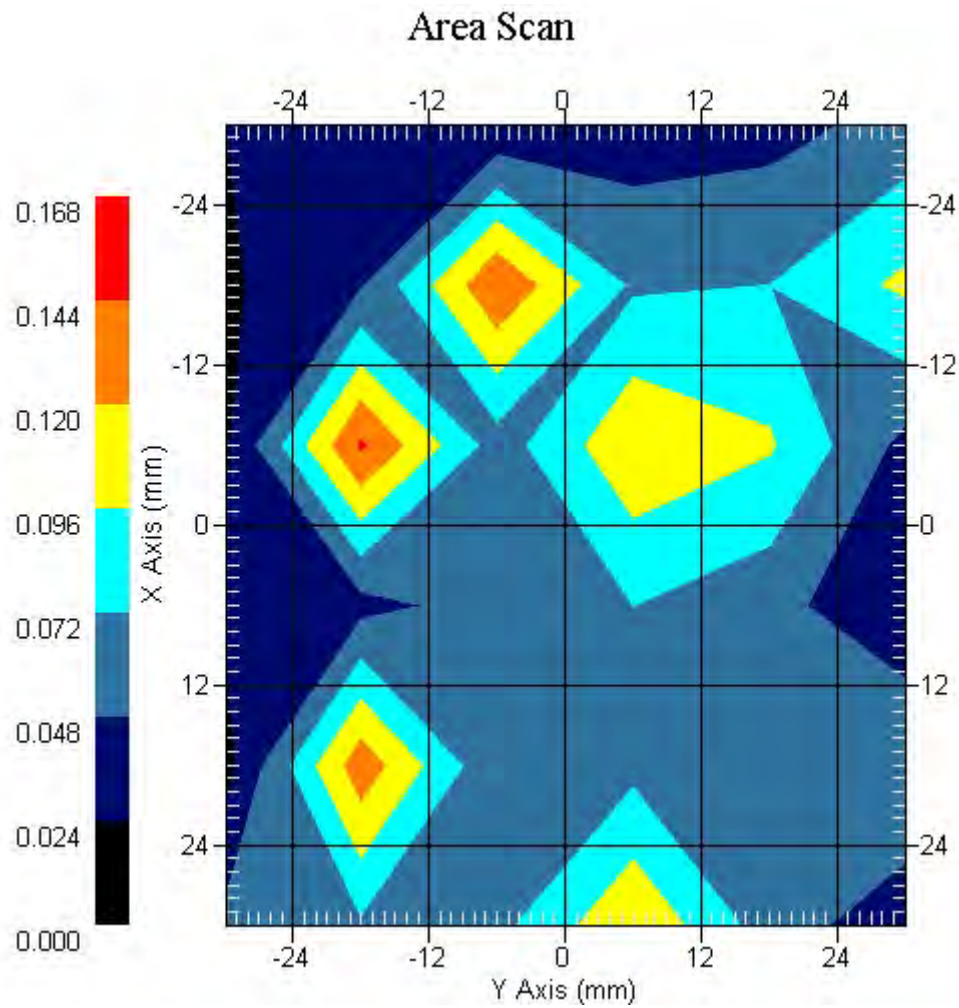

## Measurement Data

Crest Factor : 1  
 Tissue Temp. : 20.90 °C  
 Ambient Temp. : 21.60 °C  
 Area Scan : 6x6x1 : Measurement x=12mm, y=12mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm  
 Power Drift-Start : 0.054 W/kg  
 Power Drift-Finish: 0.055 W/kg  
 Power Drift (%) : 1.869


DUT Position : 15° Tilt  
 Channel : 773

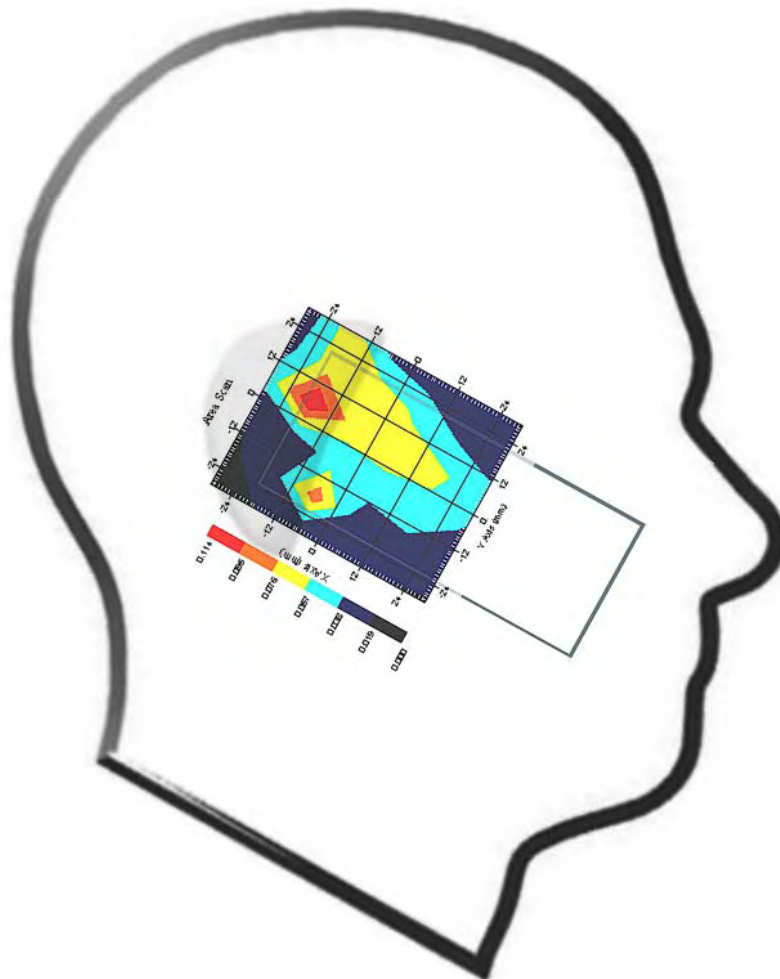

1 gram SAR value : 0.078 W/kg  
 10 gram SAR value : 0.044 W/kg  
 Area Scan Peak SAR : 0.113 W/kg  
 Zoom Scan Peak SAR : 0.150 W/kg




This is previous page plot (zoom in)

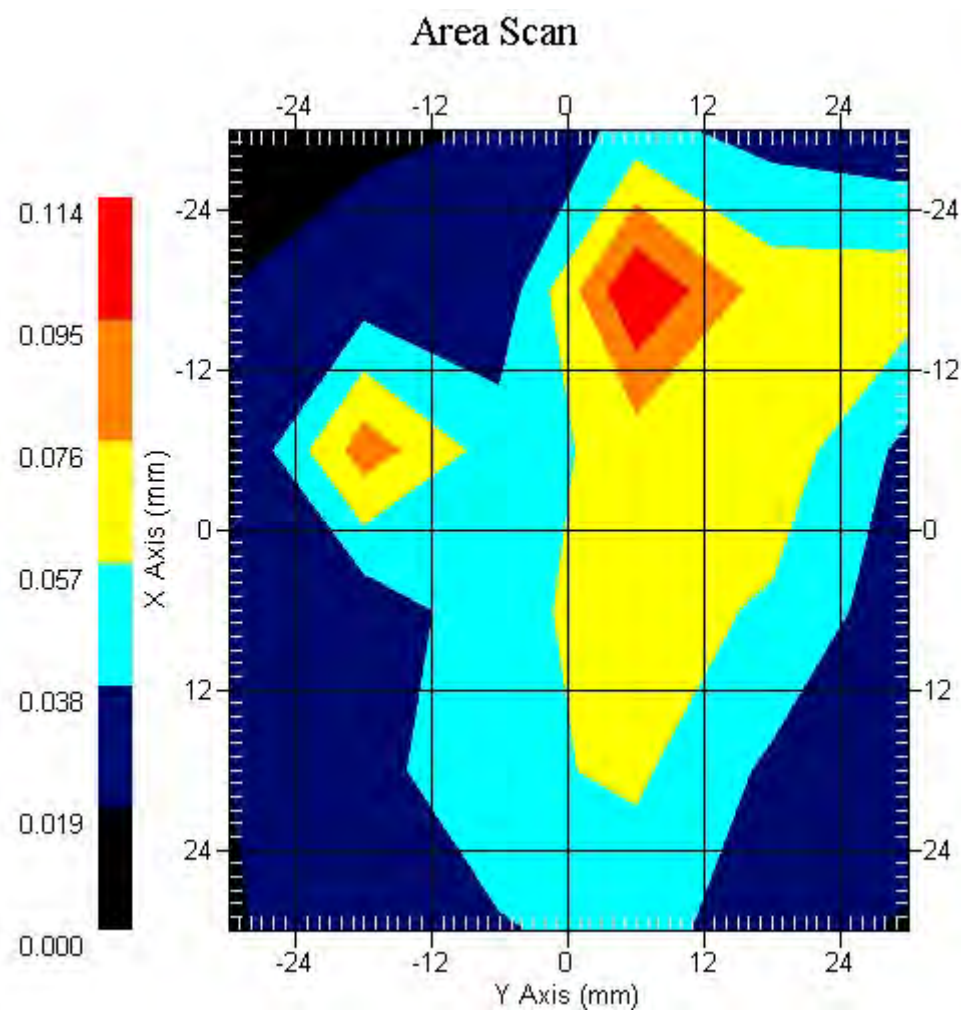

## Measurement Data

Crest Factor : 1  
 Tissue Temp. : 20.90 °C  
 Ambient Temp. : 21.60 °C  
 Area Scan : 6x6x1 : Measurement x=12mm, y=12mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm  
 Power Drift-Start : 0.034 W/kg  
 Power Drift-Finish: 0.034 W/kg  
 Power Drift (%) : -2.770


DUT Position : Touch  
 Channel : 1014

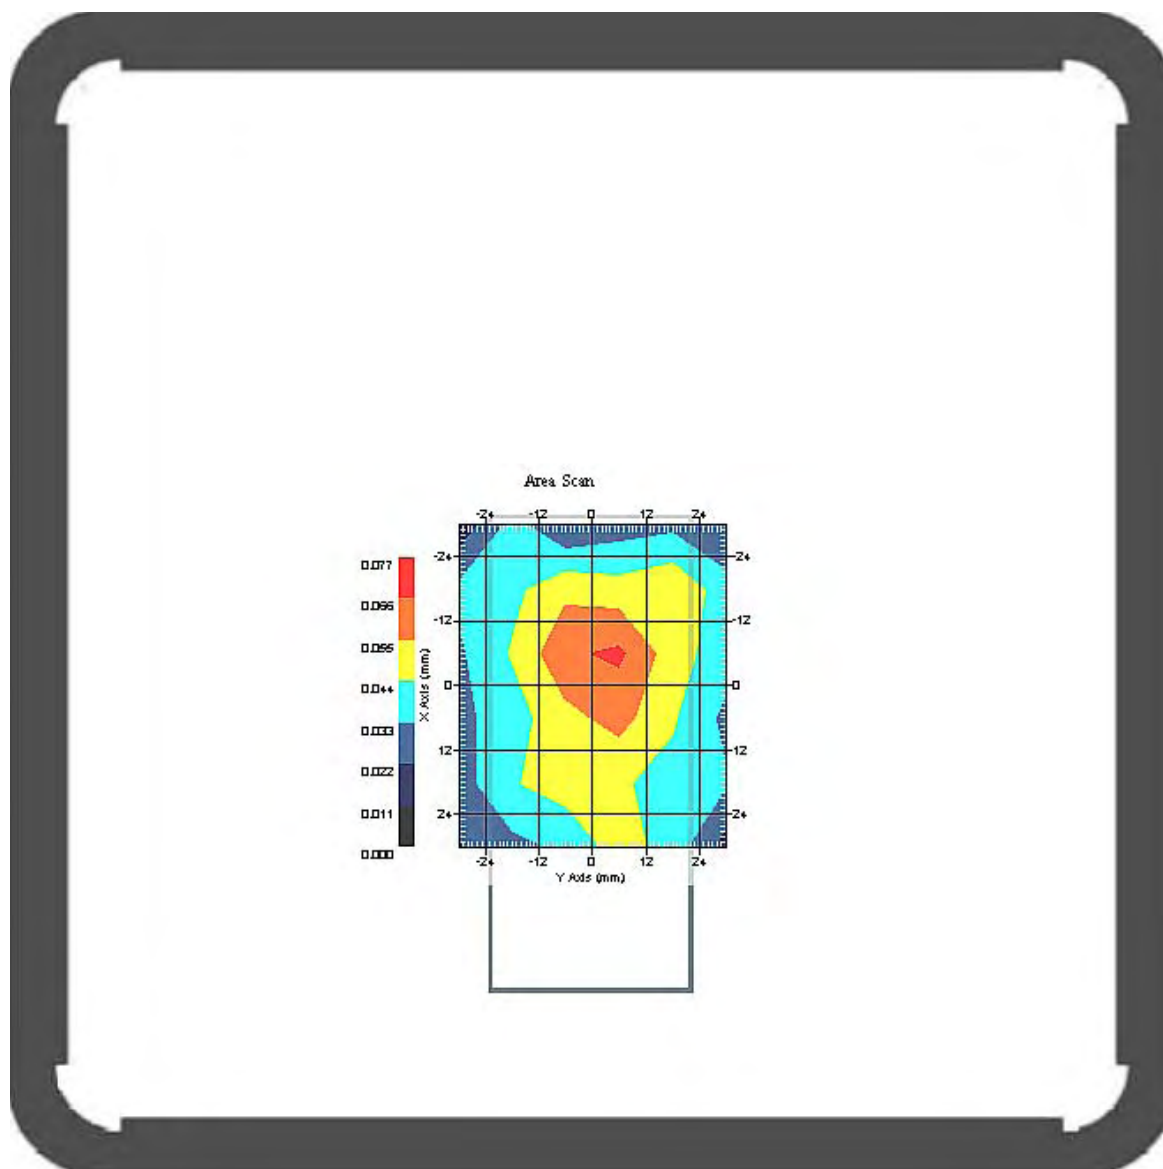

1 gram SAR value : 0.065 W/kg  
 10 gram SAR value : 0.048 W/kg  
 Area Scan Peak SAR : 0.068 W/kg  
 Zoom Scan Peak SAR : 0.290 W/kg




This is previous page plot (zoom in)

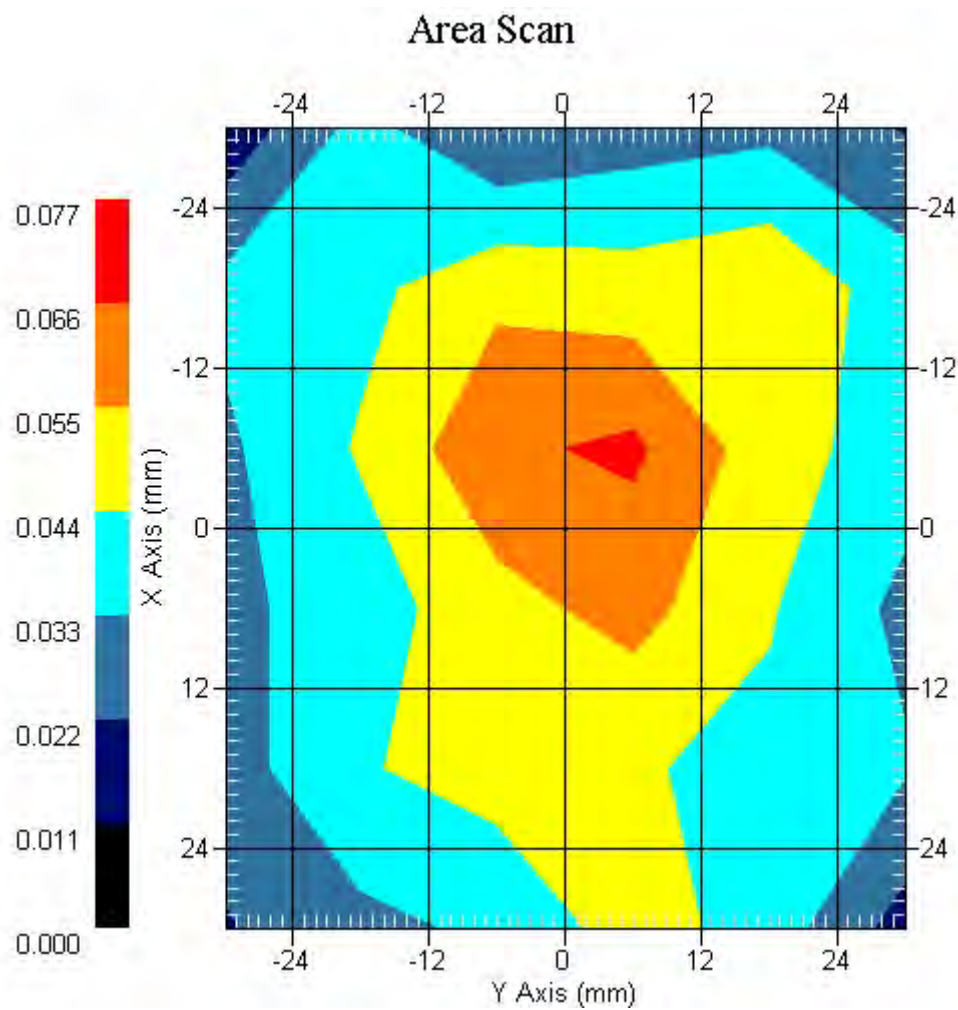

## Measurement Data


Crest Factor : 1  
 Tissue Temp. : 20.90 °C  
 Ambient Temp. : 21.60 °C  
 Area Scan : 6x6x1 : Measurement x=12mm, y=12mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm  
 Power Drift-Start : 0.047 W/kg  
 Power Drift-Finish: 0.046 W/kg  
 Power Drift (%) : -2.061

DUT Position : Touch  
 Channel : 380

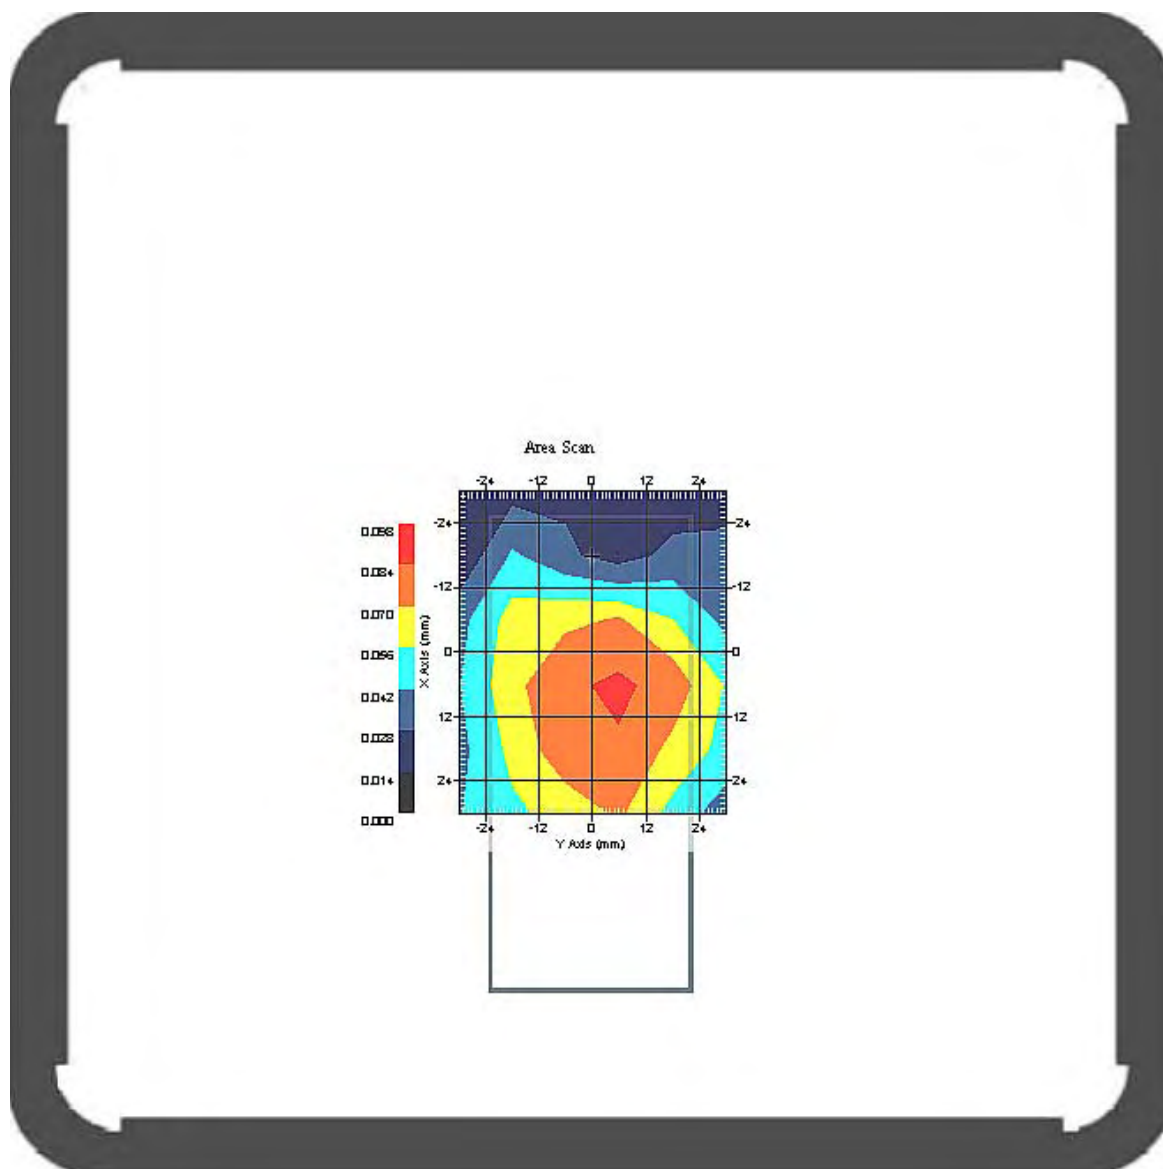

1 gram SAR value : 0.096 W/kg  
 10 gram SAR value : 0.049 W/kg  
 Area Scan Peak SAR : 0.087 W/kg  
 Zoom Scan Peak SAR : 0.170 W/kg


This is previous page plot (zoom in)

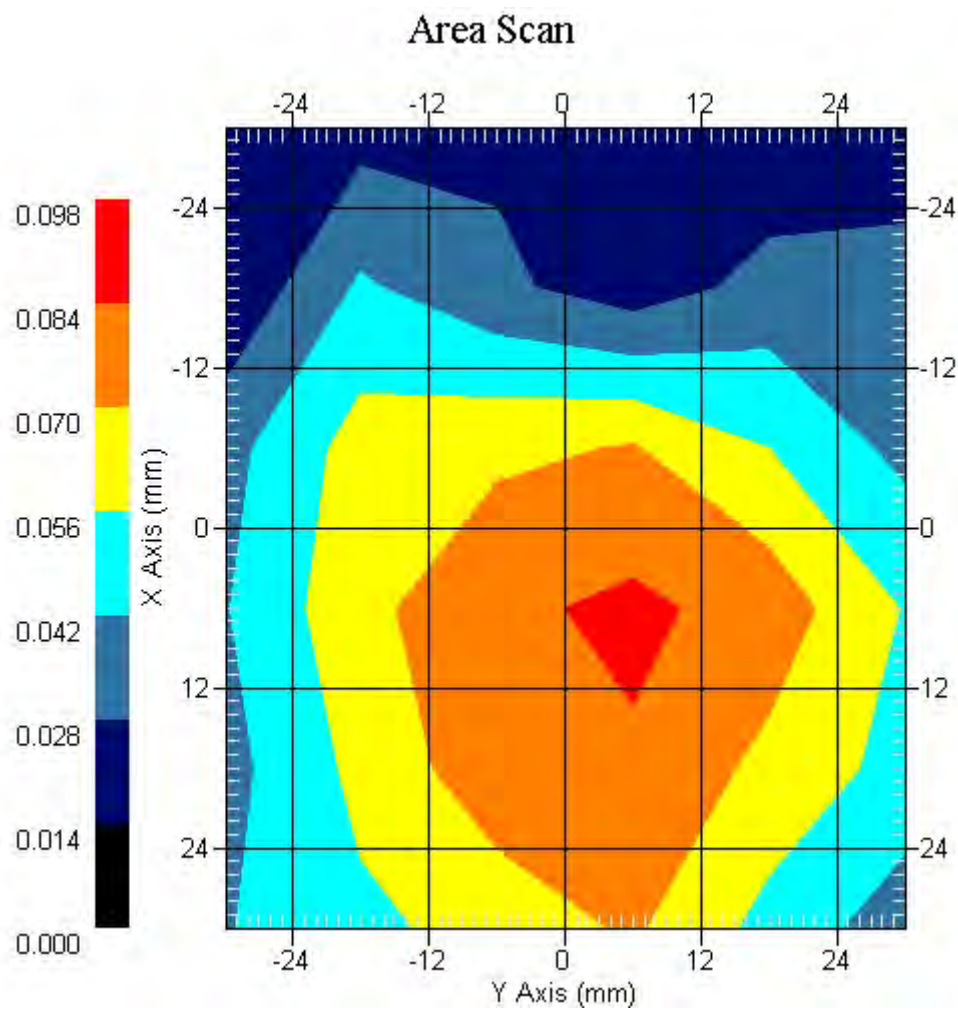

## Measurement Data


Crest Factor : 1  
 Tissue Temp. : 20.90 °C  
 Ambient Temp. : 21.60 °C  
 Area Scan : 6x6x1 : Measurement x=12mm, y=12mm, z=4mm  
 Zoom Scan : 7x7x7 : Measurement x=5mm, y=5mm, z=5mm  
 Power Drift-Start : 0.035 W/kg  
 Power Drift-Finish: 0.035 W/kg  
 Power Drift (%) : 2.560

DUT Position : Touch  
 Channel : 773

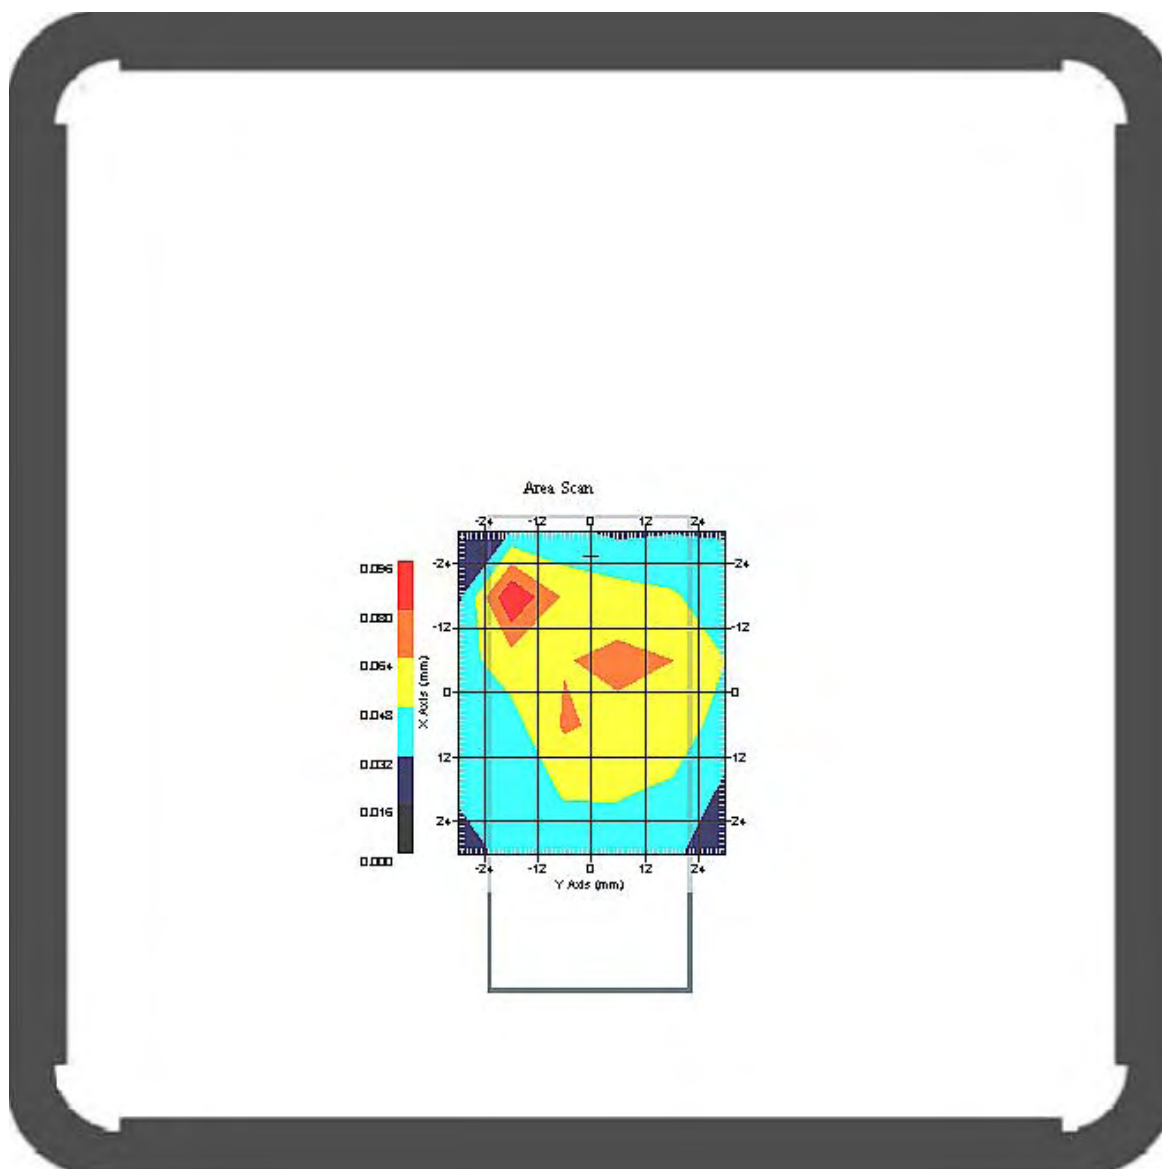


1 gram SAR value : 0.052 W/kg  
 10 gram SAR value : 0.044 W/kg  
 Area Scan Peak SAR : 0.096 W/kg  
 Zoom Scan Peak SAR : 0.160 W/kg

This is previous page plot (zoom in)

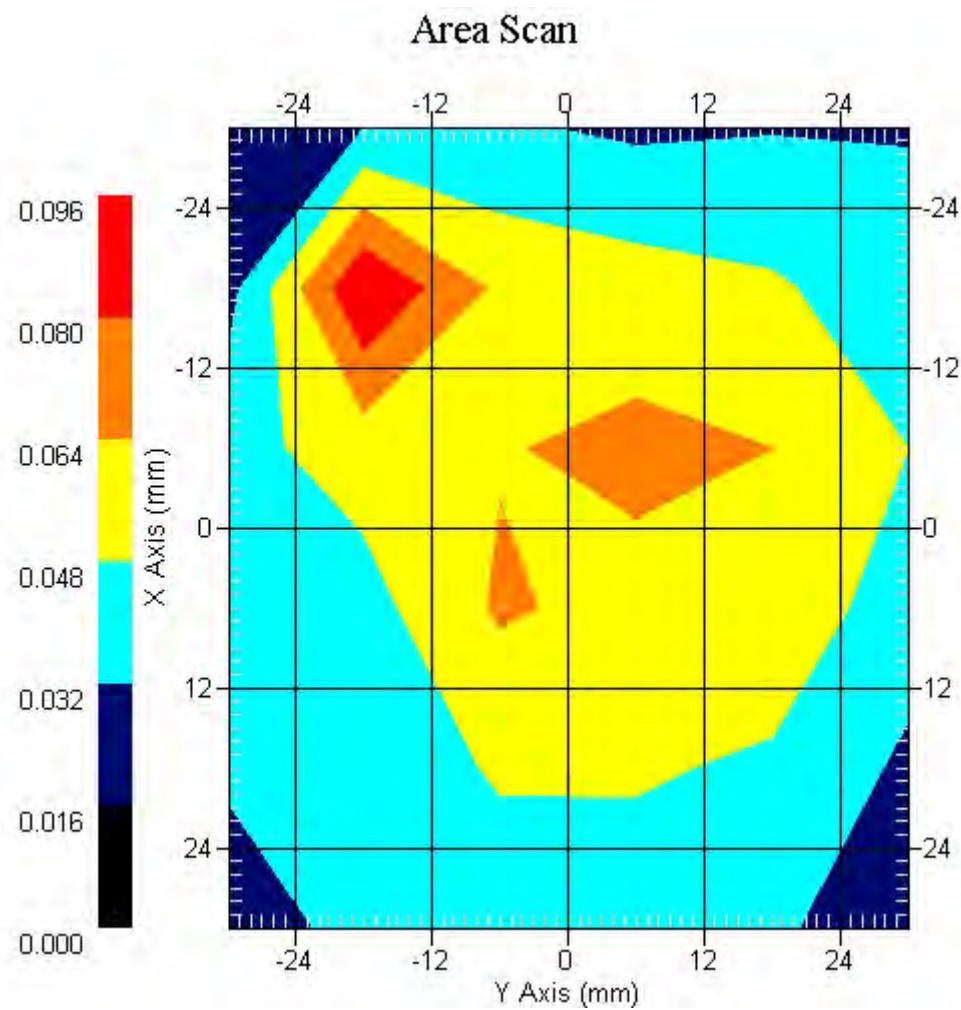

## EUT 835MHz SAR test Z-Axis plot


### CDMA2000 (800MHz), Left Cheek, Channel 773

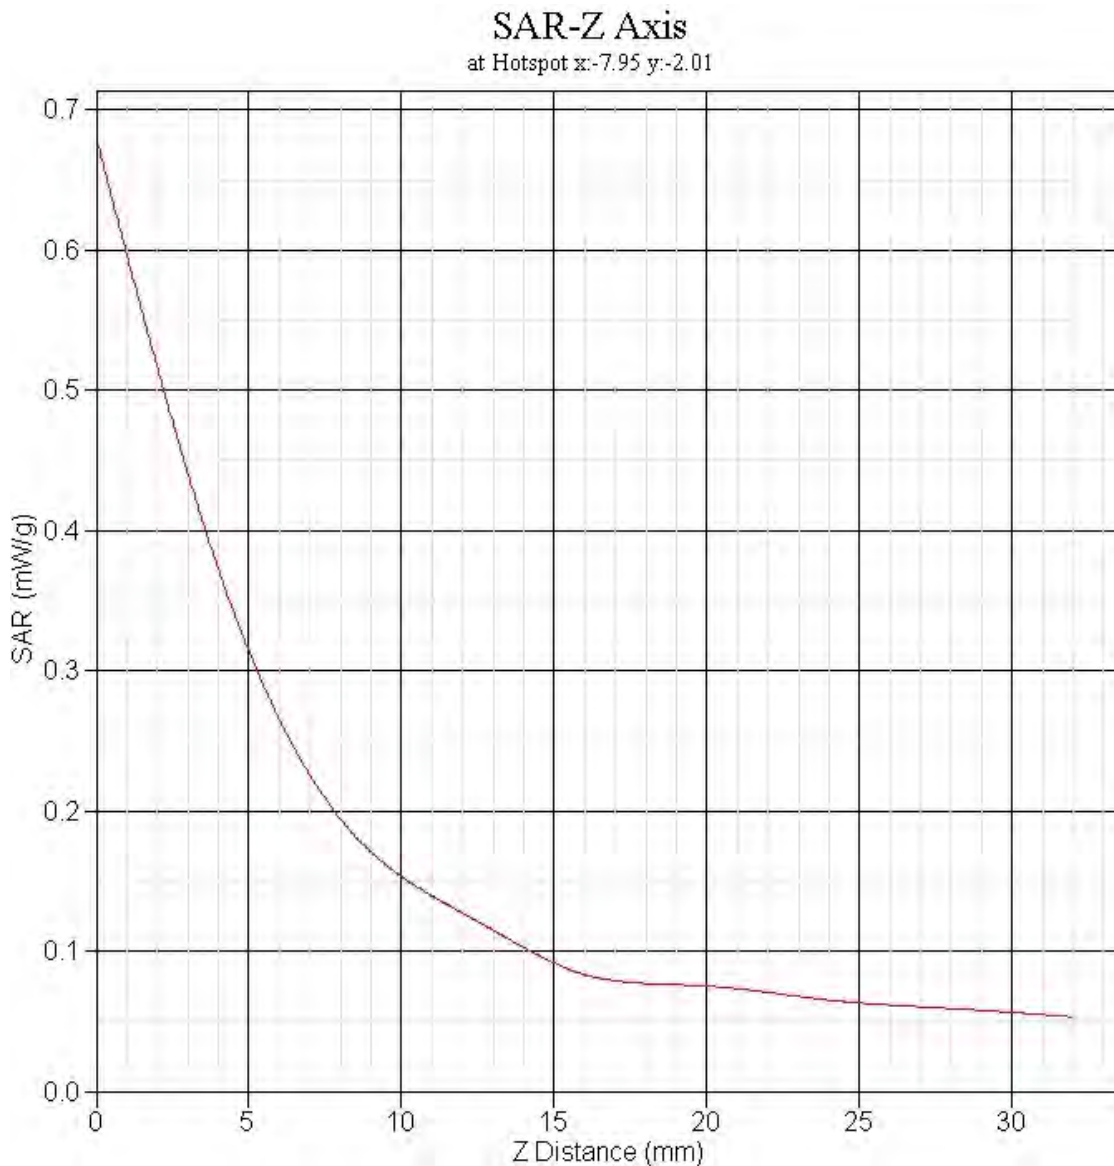



## Test Setup & EUT Photographs


**Right Head (EUT Cheek)**

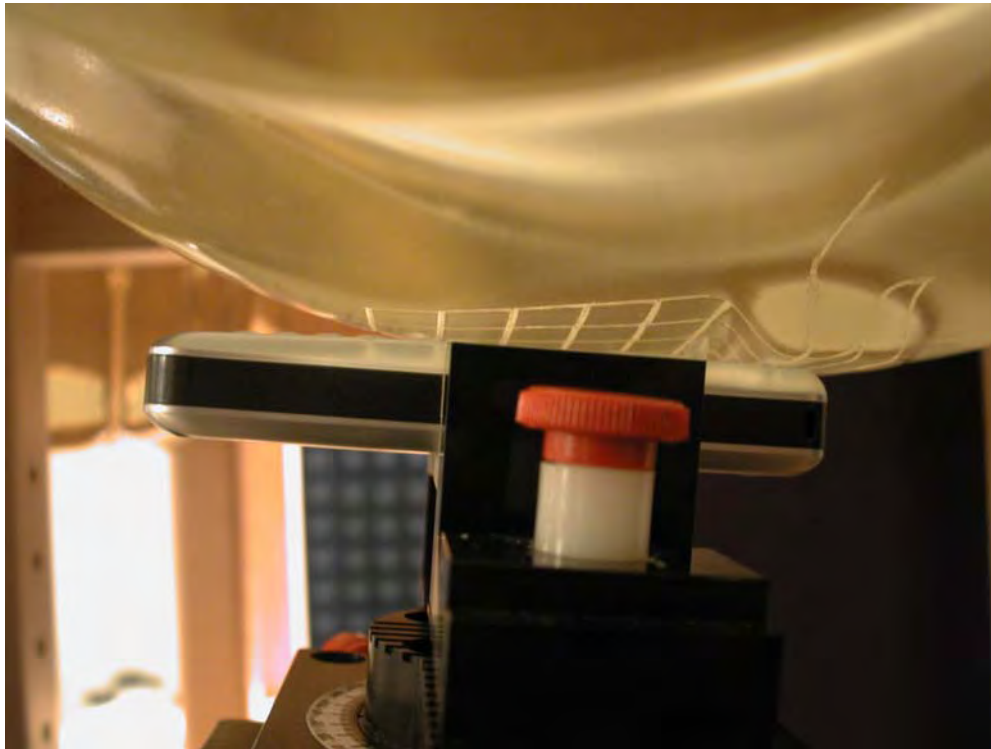

**Left Head (EUT Cheek)**




**Right Head (EUT Tilted)**

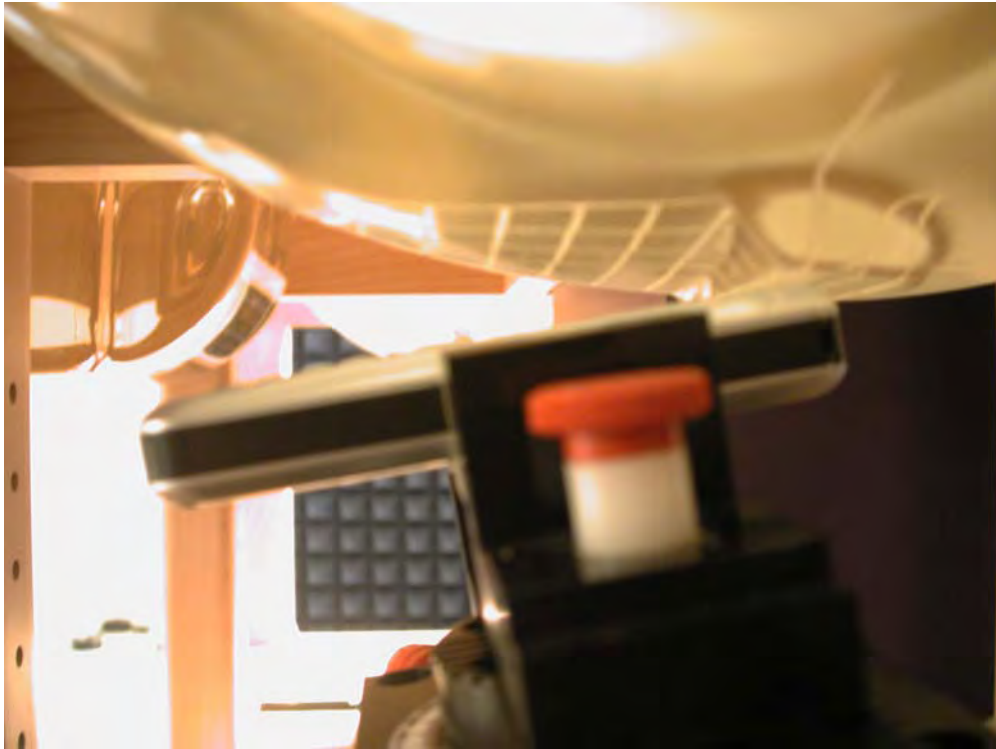

**Left Head (EUT Tilted)**

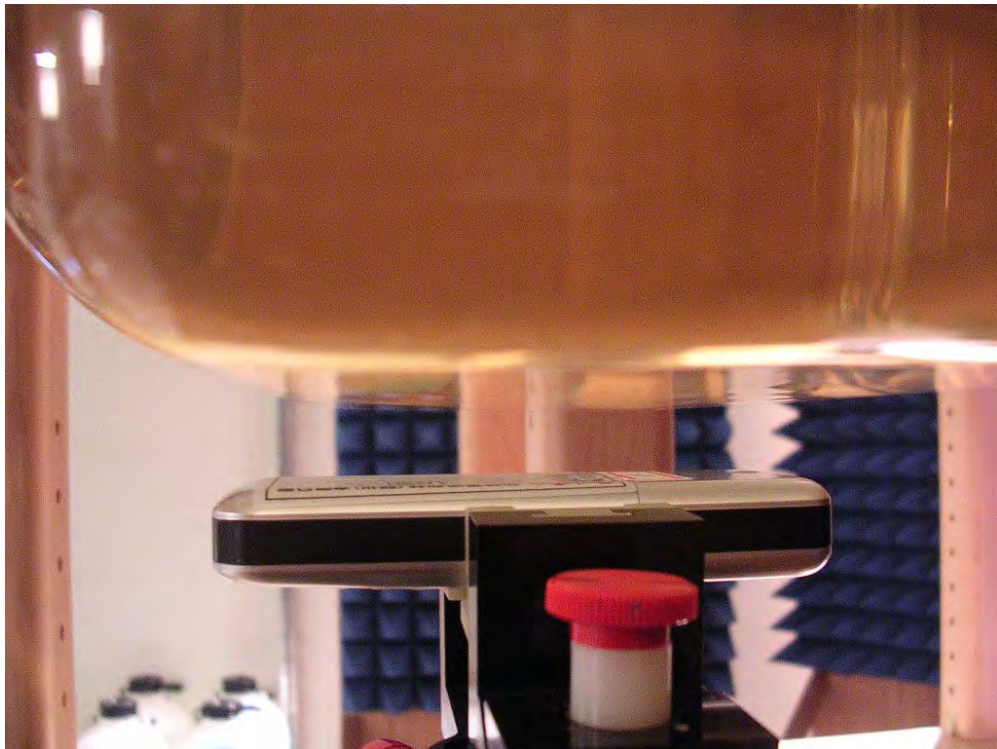

**Body-worn (Separation distance: 15mm)**

**Note: The positions used in the measurements were according to IEEE 1528-2003.**



**EUT Photographs****EUT Front****EUT Back**

## NCL CALIBRATION LABORATORIES

Calibration File No.: CP-630

Client: QUIETEK

# CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories

Model No.: ALS-E-020

Serial No.: 264

HEAD Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: QUIB-Probe-Cal-5210

Calibrated: 21<sup>st</sup> March 2006

Released on: 21<sup>st</sup> March 2006

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 264.

## References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

## Conditions

Probe 264 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

-----  
Stuart Nicol

  
-----  
Yi Pan



## Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	264
Frequency:	835 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

## **Sensitivity in Head Tissue**

**Frequency:** 835 MHz

**Epsilon:** 41.5 (+/-5%)      **Sigma:** 0.90 S/m (+/-5%)

### **ConvF**

**Channel X:** 6.3

**Channel Y:** 6.3

**Channel Z:** 6.3

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


## **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

## **Spatial Resolution:**



The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## Receiving Pattern 835 MHz (Air)

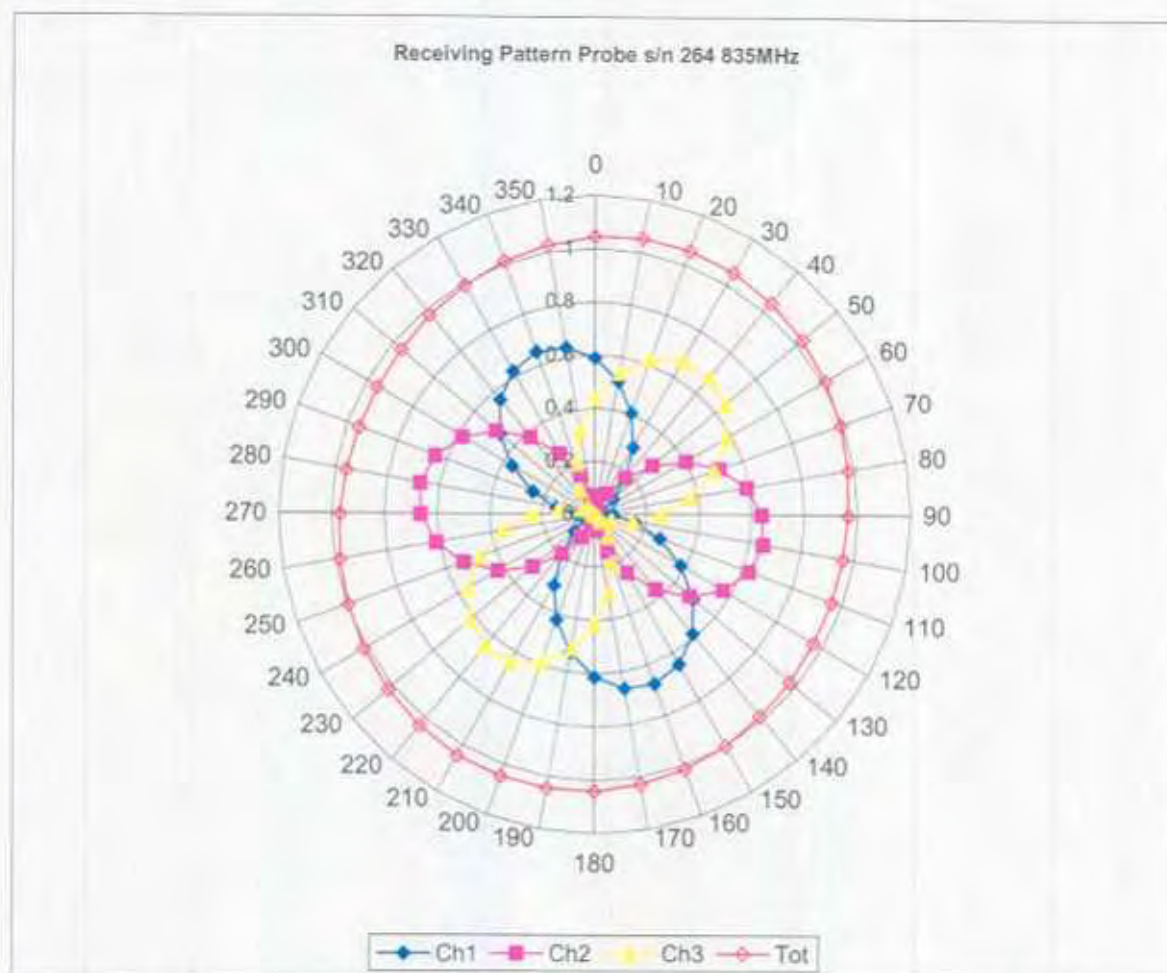




## Isotropy Error 835 MHz (Air)

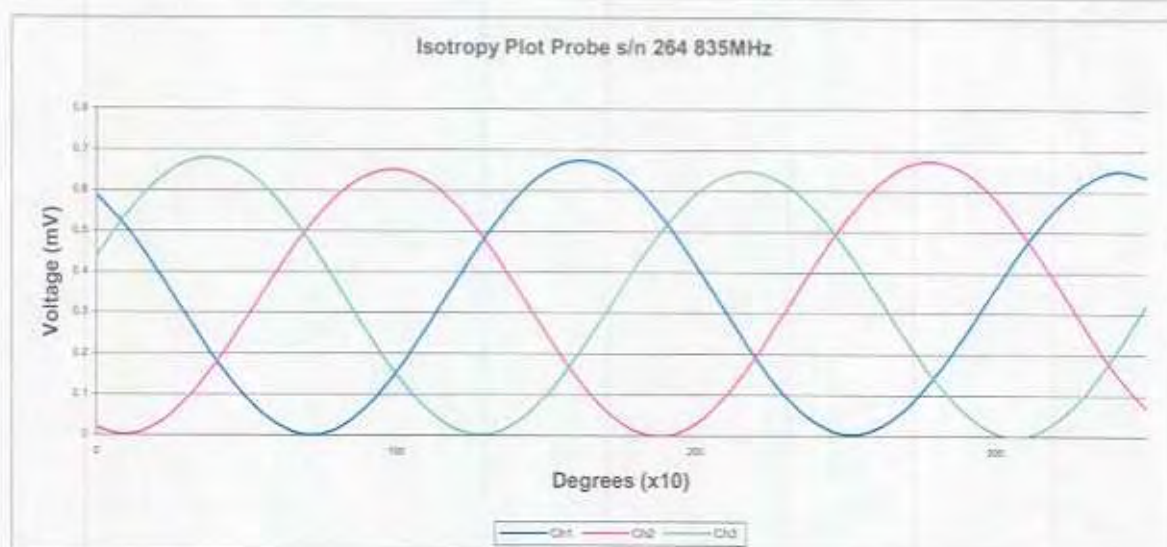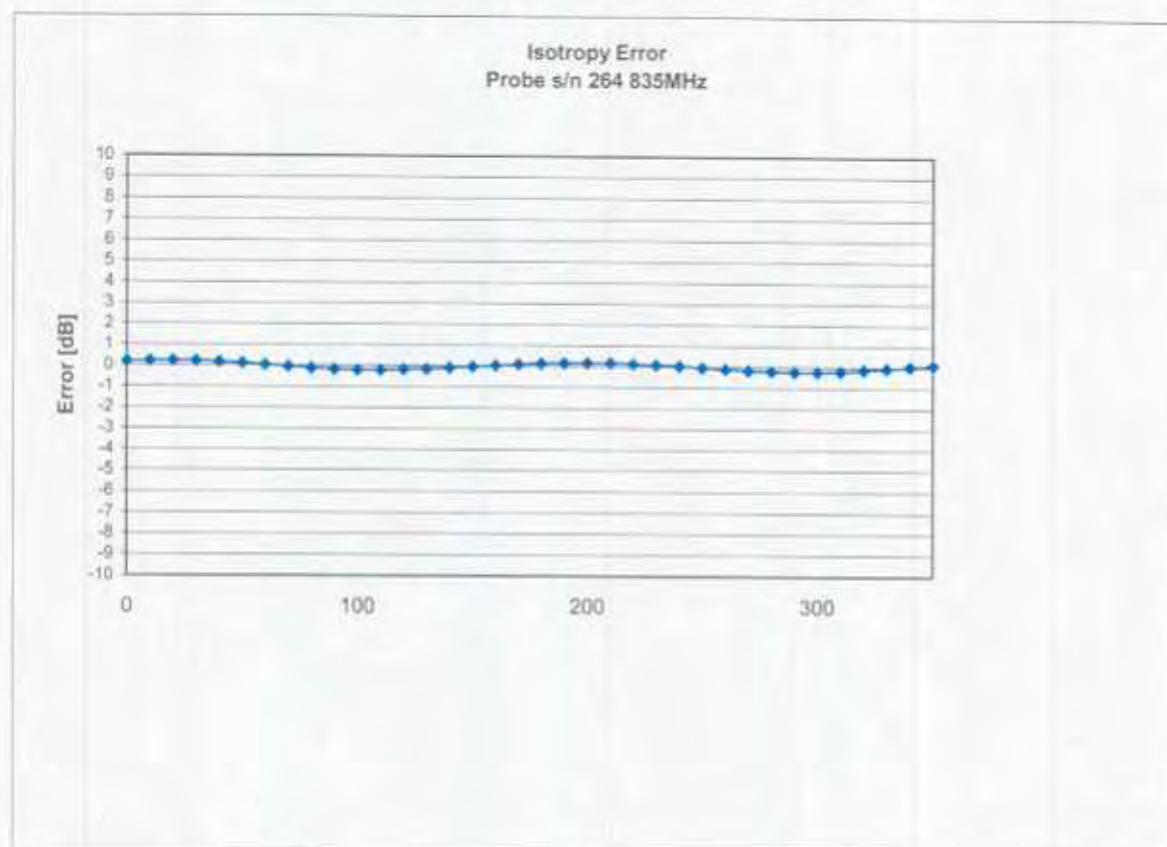


Isotropy Tissue:

0.10 dB

## Dynamic Range

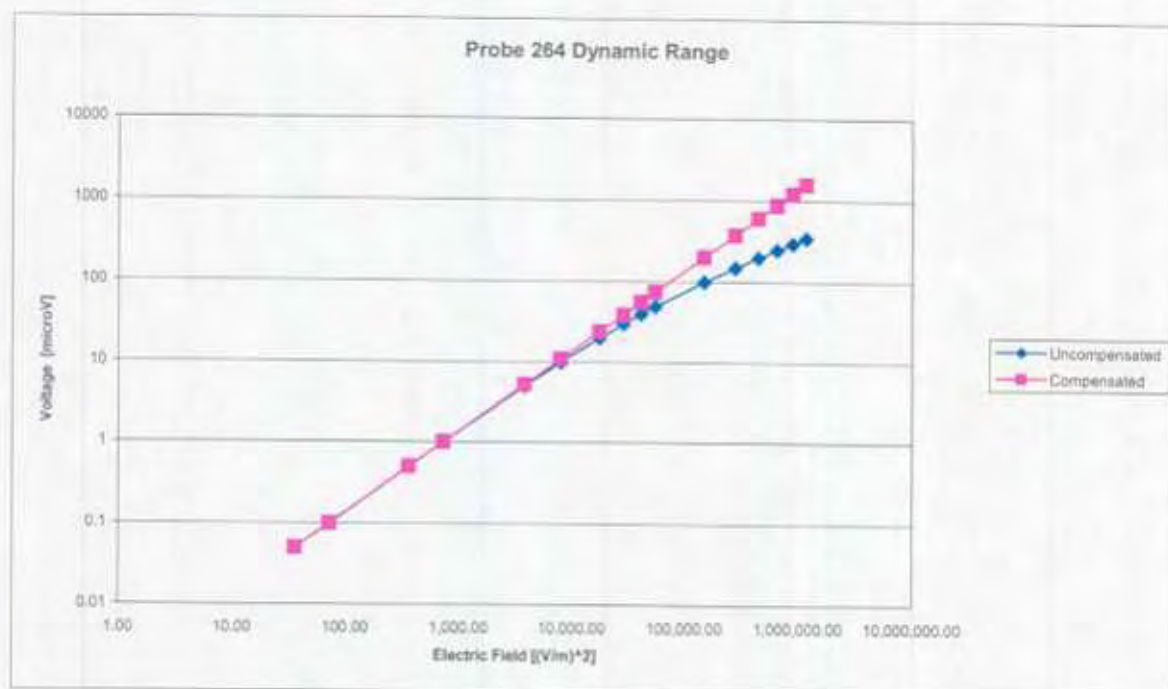

## Video Bandwidth

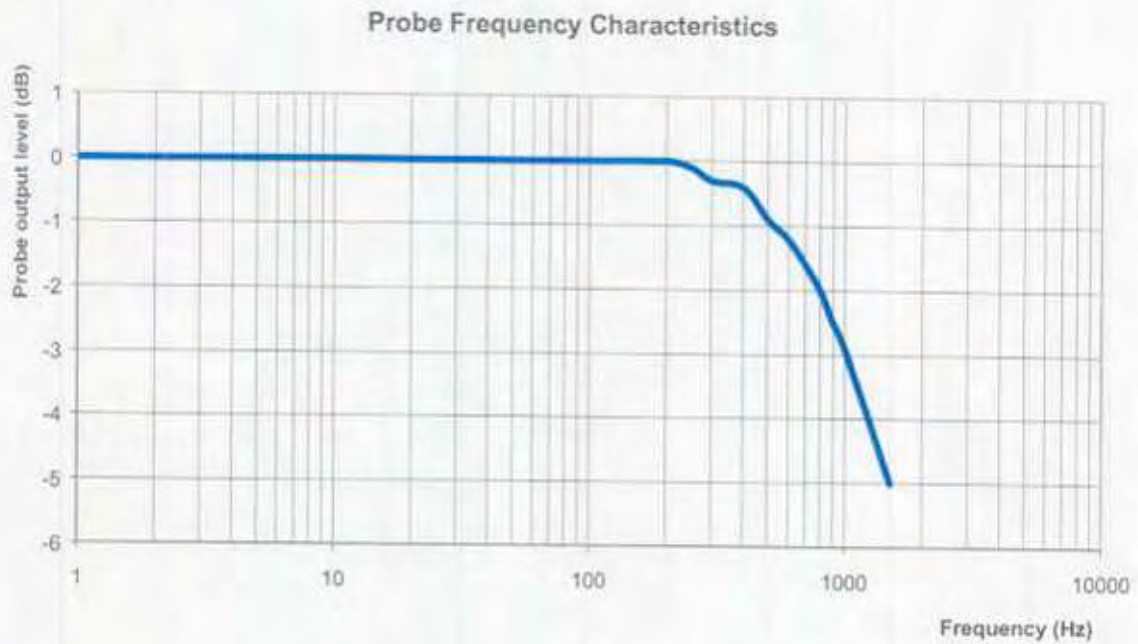

Video Bandwidth at 500 Hz	1 dB
Video Bandwidth at 1000 Hz	3 dB



## Conversion Factor Uncertainty Assessment

Frequency: 835MHz

Epsilon: 41.5 (+/-5%)

Sigma: 0.90 S/m (+/-5%)

### ConvF

Channel X: 6.3 7%(K=2)

Channel Y: 6.3 7%(K=2)

Channel Z: 6.3 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

### Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-637

Client: QUIETEK

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 835 MHz

Manufacturer: APREL Laboratories

Model No.: ALS-E-020

Serial No.: 264

BODY Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: QUIB-Probe-Cal-5210

Calibrated: 21<sup>st</sup> March 2006  
Released on: 21<sup>st</sup> March 2006

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab  
TEL: (613) 820-4988  
FAX: (613) 820-4161



## Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 264.

## References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

## Conditions


Probe 264 was a new probe taken from stock prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

-----  
Stuart Nicol

  
-----  
Yi Pan

## Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	264
Frequency:	835 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

Channel X:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Y:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Channel Z:	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
Diode Compression Point:	95 mV

## **Sensitivity in Body Tissue**

**Frequency:**

835 MHz

**Epsilon:** 55.2 (+/-5%)

**Sigma:** 0.97 S/m (+/-5%)

**ConvF**

**Channel X:** 6.8

**Channel Y:** 6.8

**Channel Z:** 6.8

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

## **Boundary Effect:**


Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

## **Spatial Resolution:**



The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.



## Receiving Pattern 835 MHz (Air)

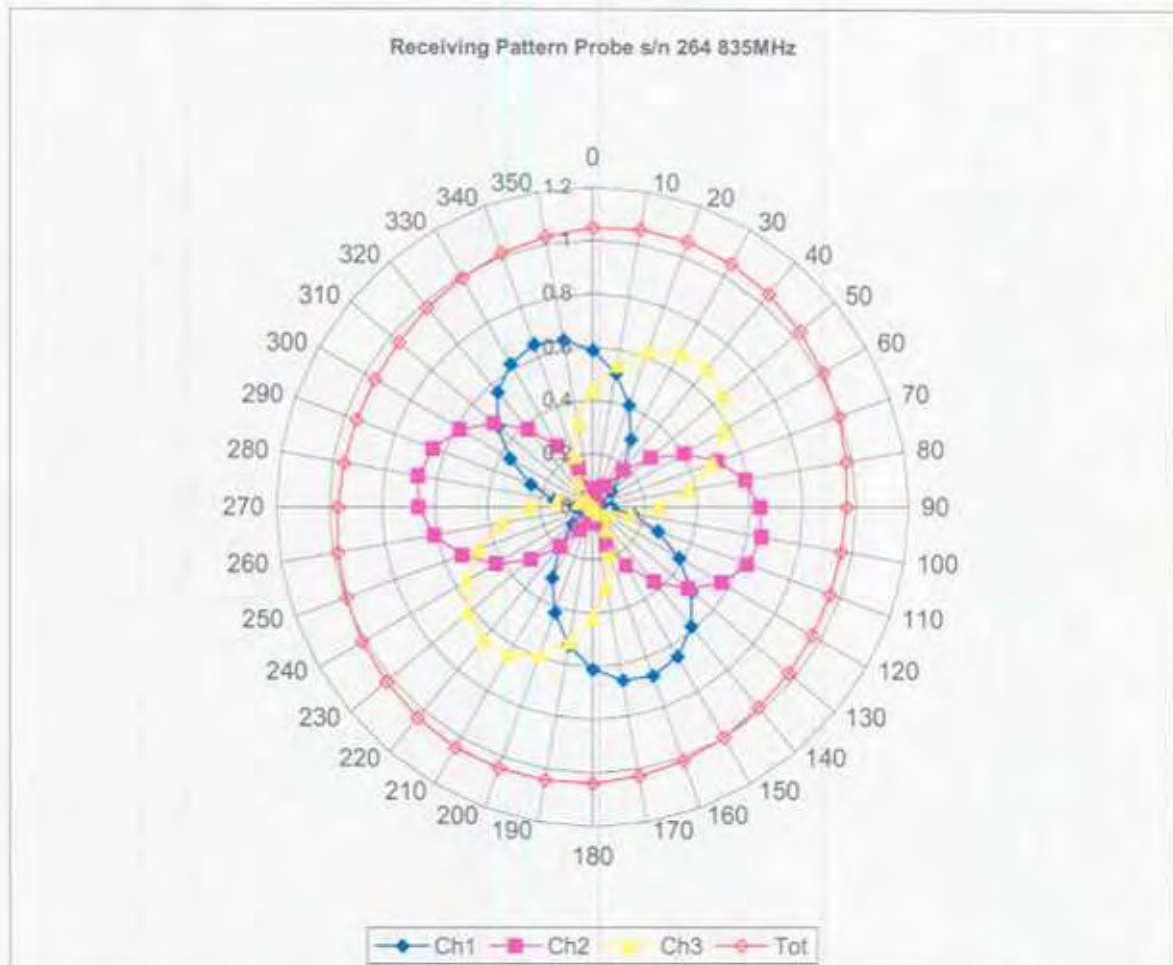


## Isotropy Error 835 MHz (Air)

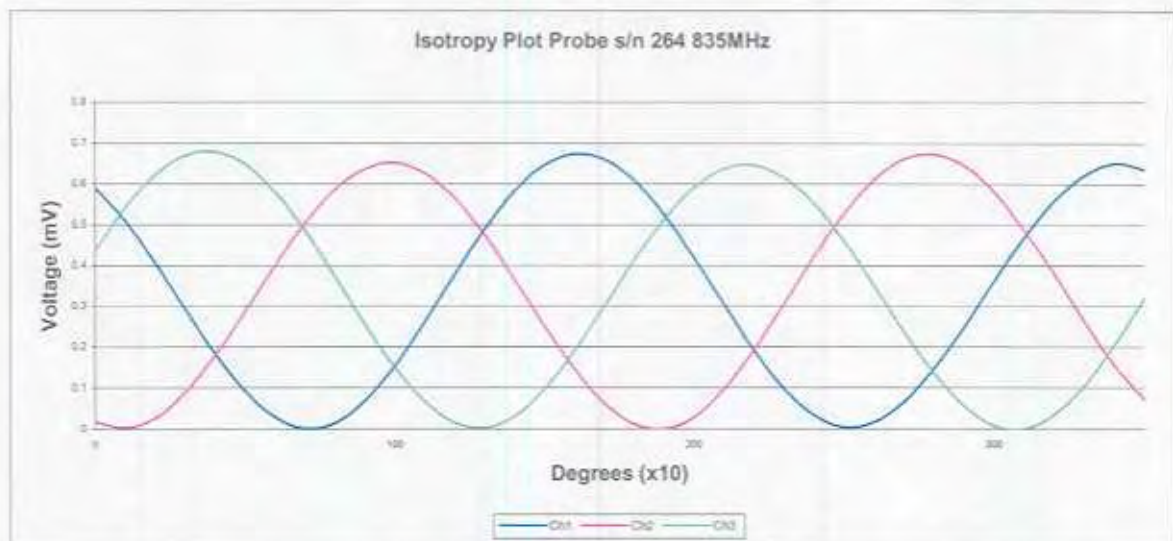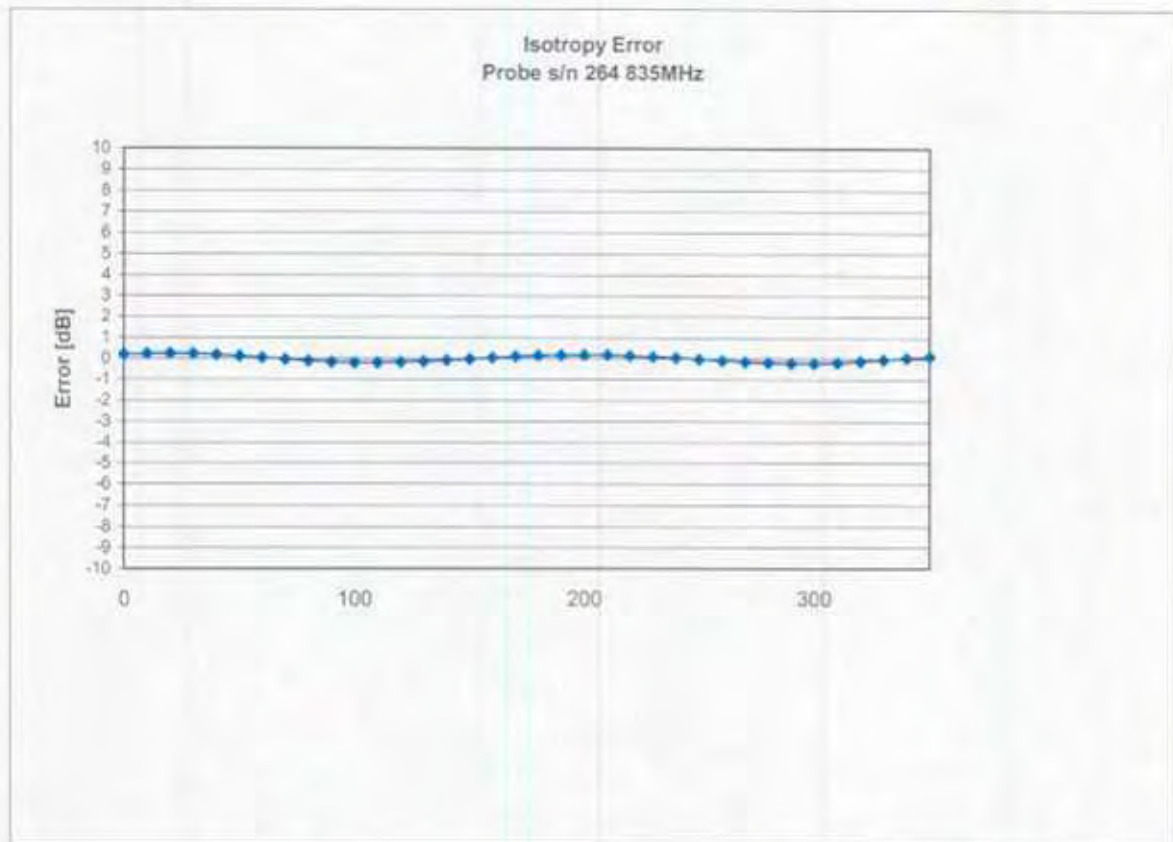

Isotropy in Tissue:


0.10 dB

## Dynamic Range

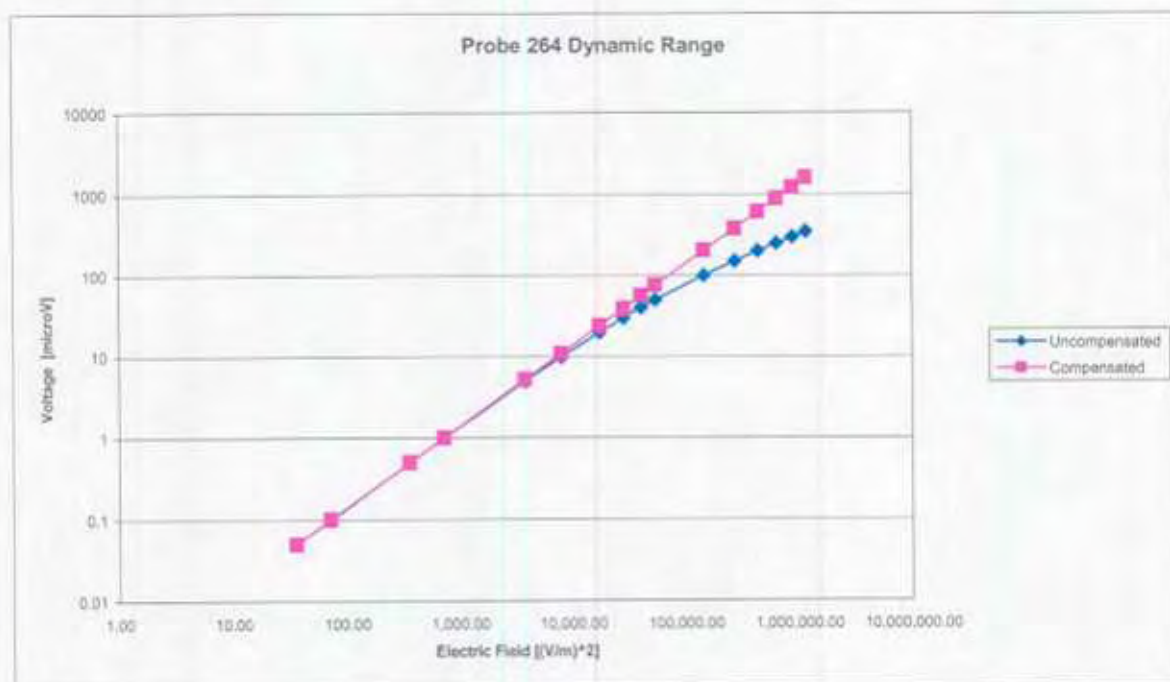



## Video Bandwidth

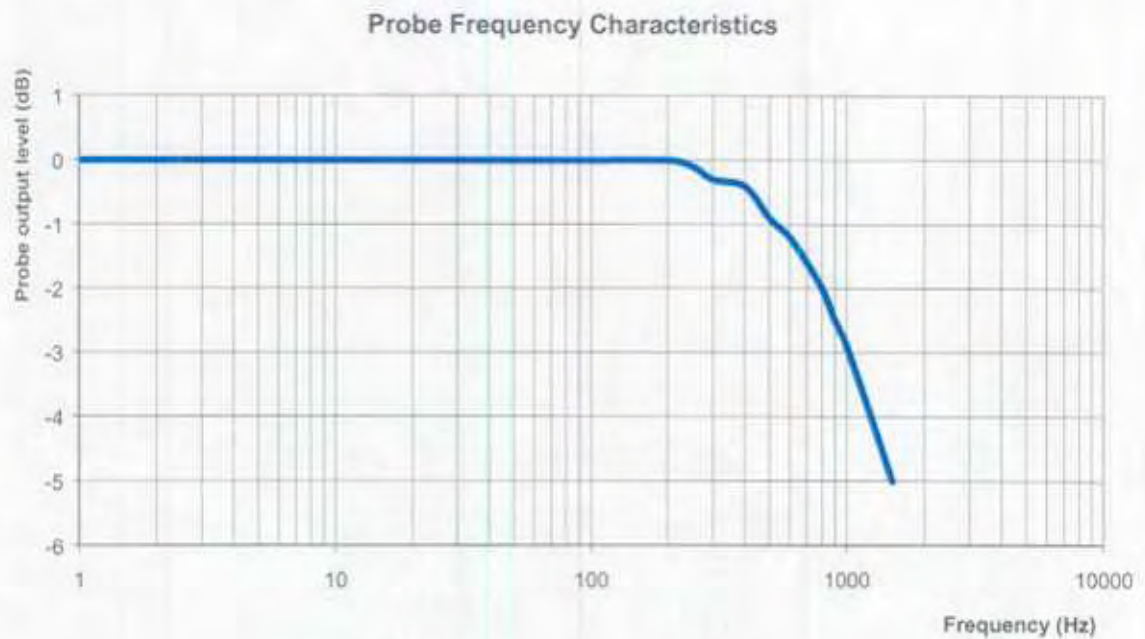

Video Bandwidth at 500 Hz	1 dB
Video Bandwidth at 1000 Hz	3 dB

## Conversion Factor Uncertainty Assessment

Frequency:	835MHz
Epsilon: 55.2 (+/-5%)	Sigma: 0.97 S/m (+/-5%)
ConvF	
Channel X: 6.8	7%(K=2)
Channel Y: 6.8	7%(K=2)
Channel Z: 6.8	7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

### Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List.



## NCL CALIBRATION LABORATORIES

Calibration File No: DC-405-1  
Project Number: QTKB-Dipole Cal-5226

# CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Quietek Validation Dipole

Manufacturer: APREL Laboratories

Part number: ALS-D-835-S-2

Frequency: 835 MHz

Serial No: QTK-315

Customer: Quietek

Calibrated: 15 June 2006  
Released on: 15 June 2006

Released By: \_\_\_\_\_

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4162

## Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions


**Length:** 165.0 mm  
**Height:** 90.0 mm

### Electrical Specification

**SWR:** 1.05 U  
**Return Loss:** -31.5 dB  
**Impedance:** 47.6  $\Omega$

### System Validation Results

Frequency	1 Gram	10 Gram	Peak
835 MHz	9.33	6.42	15.0

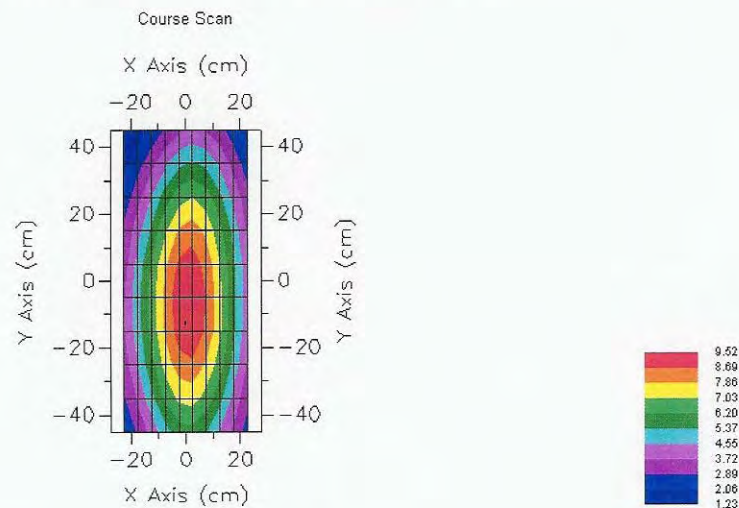

## Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole QTK-315. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the IEEE/APREL mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with QTK E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

## References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

## Conditions

Dipole QTK-315 was received for calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 20 °C +/- 0.5°C

## Dipole Calibration Results

### Mechanical Verification

IEEE Length	IEEE Height	Measured Length	Measured Height
161.0 mm	89.8 mm	165.0 mm	90.0 mm

### Tissue Validation

Head Tissue 835 MHz	Measured
Dielectric constant, $\epsilon_r$	42.54
Conductivity, $\sigma$ [S/m]	0.91





**Electrical Calibration**


Test	Result
S11 R/L	-31.5 dB
SWR	1.06 U
Impedance	47.6 $\Omega$

The Following Graphs are the results as displayed on the Vector Network Analyzer.

**S11 Parameter Return Loss**

S22 REVERSE REFLECTION

LOG MAGNITUDE REF=-20.000 dB 5.000 dB/DIV

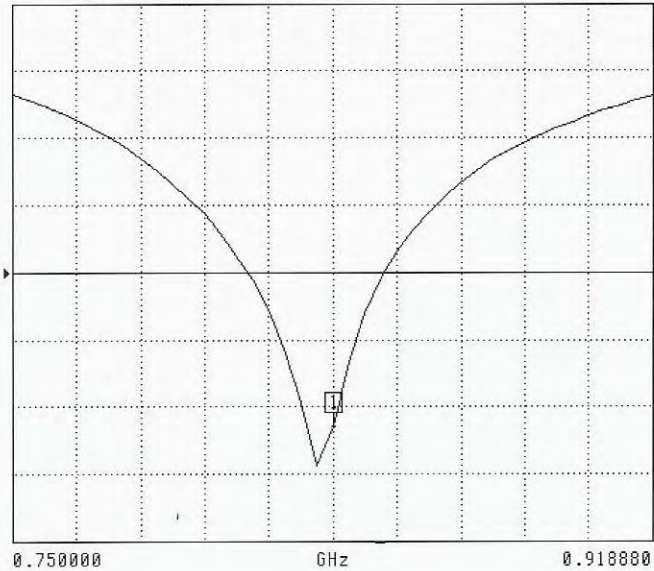

CH 4 - S22  
REFERENCE PLANE  
0.0000 mm

MARKER 1  
0.834440 GHz  
-31.489 dB

MARKER TO MAX  
MARKER TO MIN


MARKER READOUT  
FUNCTIONS

*[Signature]*

*[Signature]*

SWR

S22 REVERSE REFLECTION

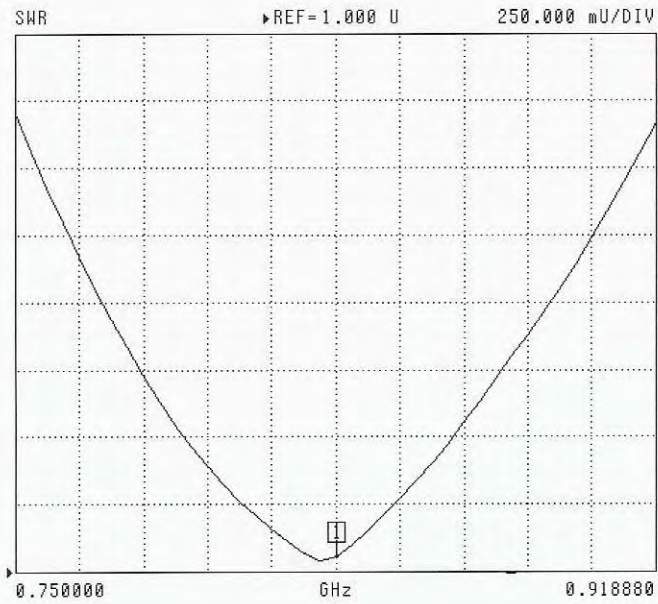

CH 4 - S22  
REFERENCE PLANE  
0.0000 mm

▶ MARKER 1  
0.834440 GHz  
1.055 U

MARKER TO MAX  
MARKER TO MIN


MARKER READOUT  
FUNCTIONS

*[Signature]*

*[Signature]*

## Smith Chart Dipole Impedance

S22 REVERSE REFLECTION  
IMPEDANCE

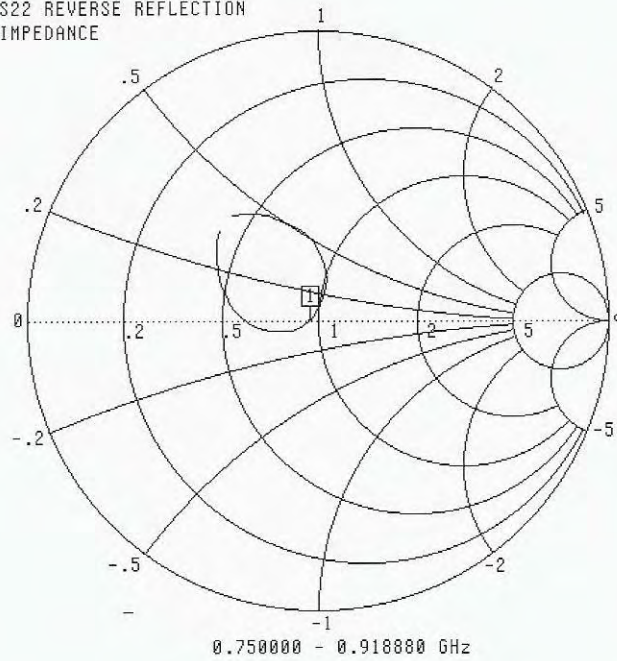

CH 4 - S22  
REFERENCE PLANE  
0.0000 mm


▶ MARKER 1  
0.834440 GHz  
47.585  $\Omega$   
34.845  $j\Omega$

MARKER TO MAX  
MARKER TO MIN

MARKER READOUT  
FUNCTIONS

System Validation Results Using the Electrically Calibrated Dipole

Head Tissue Frequency	1 Gram	10 Gram	Peak Above Feed Point
835 MHz	9.33	6.42	15.0

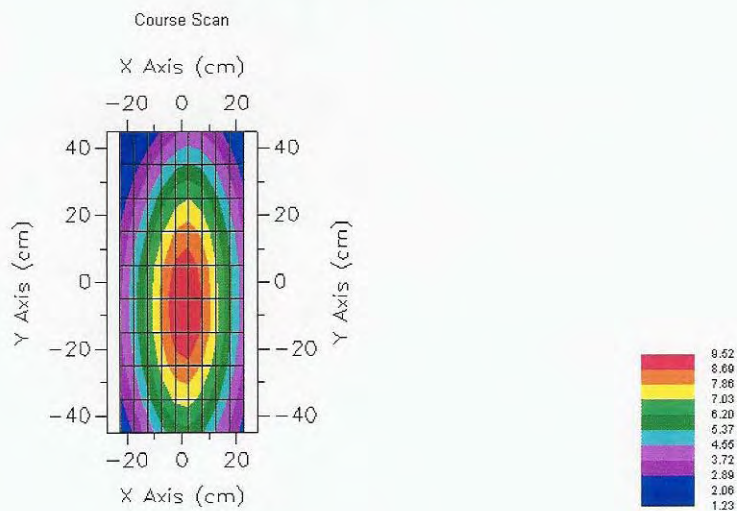



## Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List

