

Attachment A

Type / Model Name : Infinity M300

Product Description : Wireless patient monitor

Applicant : Draeger Medical Systems Inc.

Address : 6 Tech drive

ANDOVER, MA 01810

Manufacturer : Draeger Medical Systems Inc.

Address : 3135 Quarry Road

TELFORD, PA 18969-1042

Licence holder : Draeger Medical Systems Inc.

Address : 3135 Quarry Road

TELFORD, PA 18969-1042

according to

Test Report No. : T40046-05-00HS to T40046-05-06HS	18. January 2016 <hr/> Date of issue
---	---



Deutsche
Akkreditierungsstelle
D-PL-12030-01-01
D-PL-12030-01-02

The test report merely corresponds to the test sample.
It is not permitted to copy extracts of these test results
without the written permission of the test laboratory.

Contents

1	<u>Photo documentation of the EUT</u>	3
1.1	External views:	3
1.2	Internal views:	6
1.3	Antenna structure:	9
1.4	Cables:	10
1.5	Power supply and charger:	11
1.6	Control PCB used for testing only:	14

1 Photo documentation of the EUT

1.1 External views:


Front view





Rear view






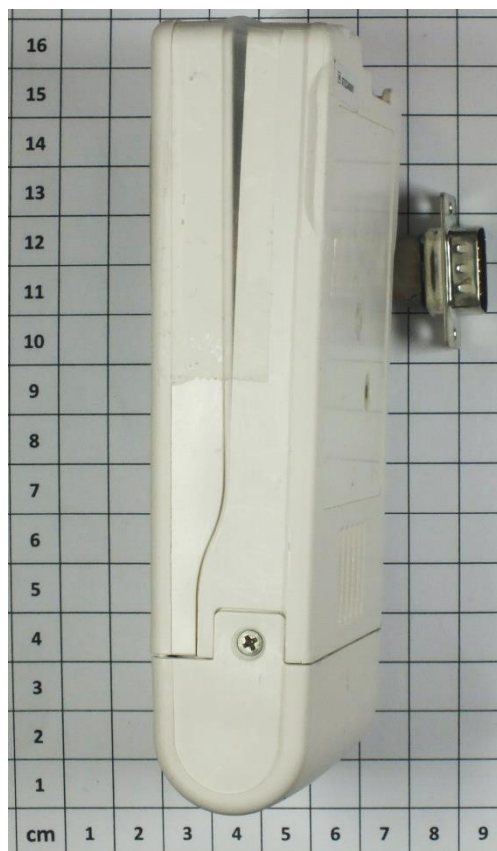




1.2 Internal views:

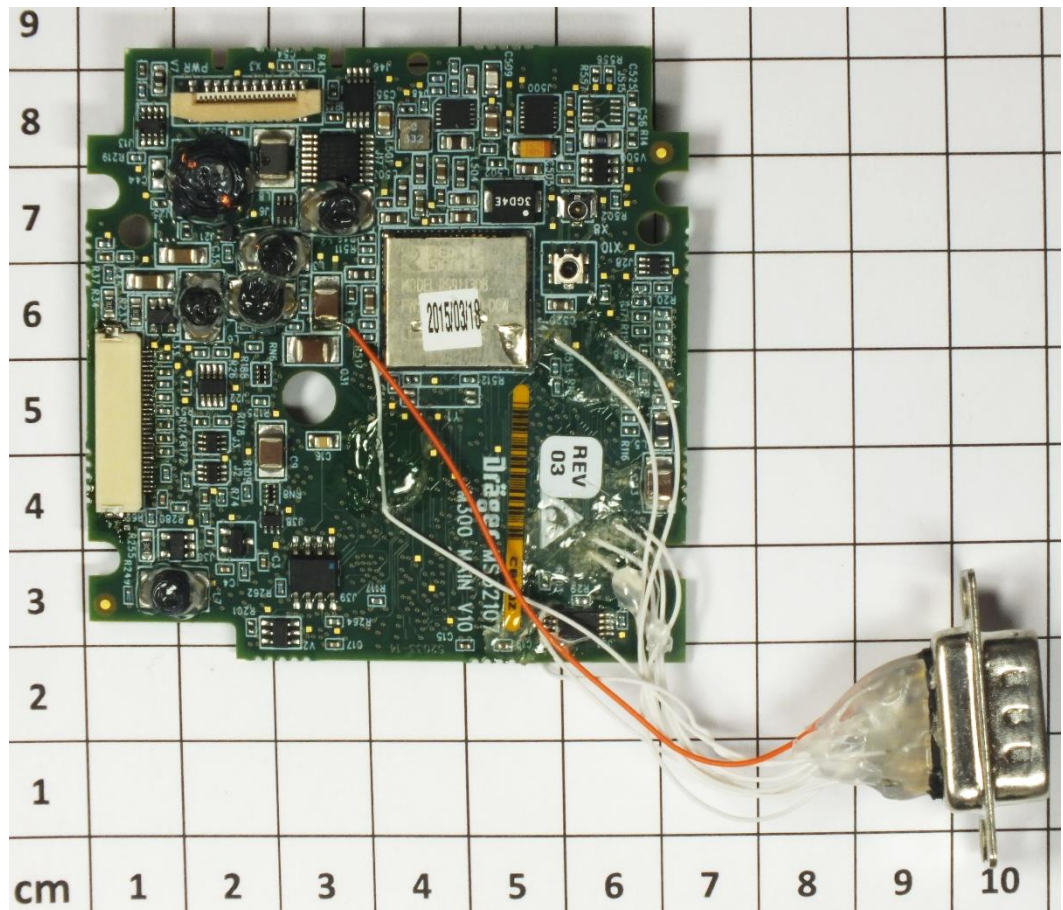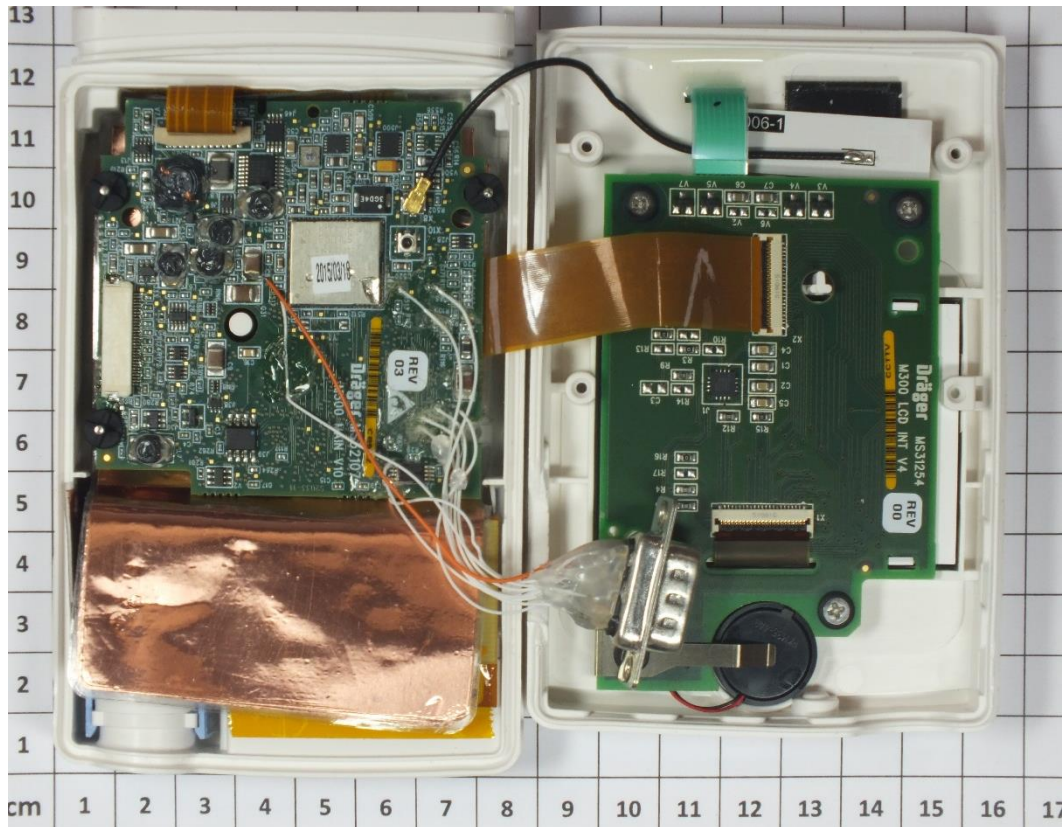

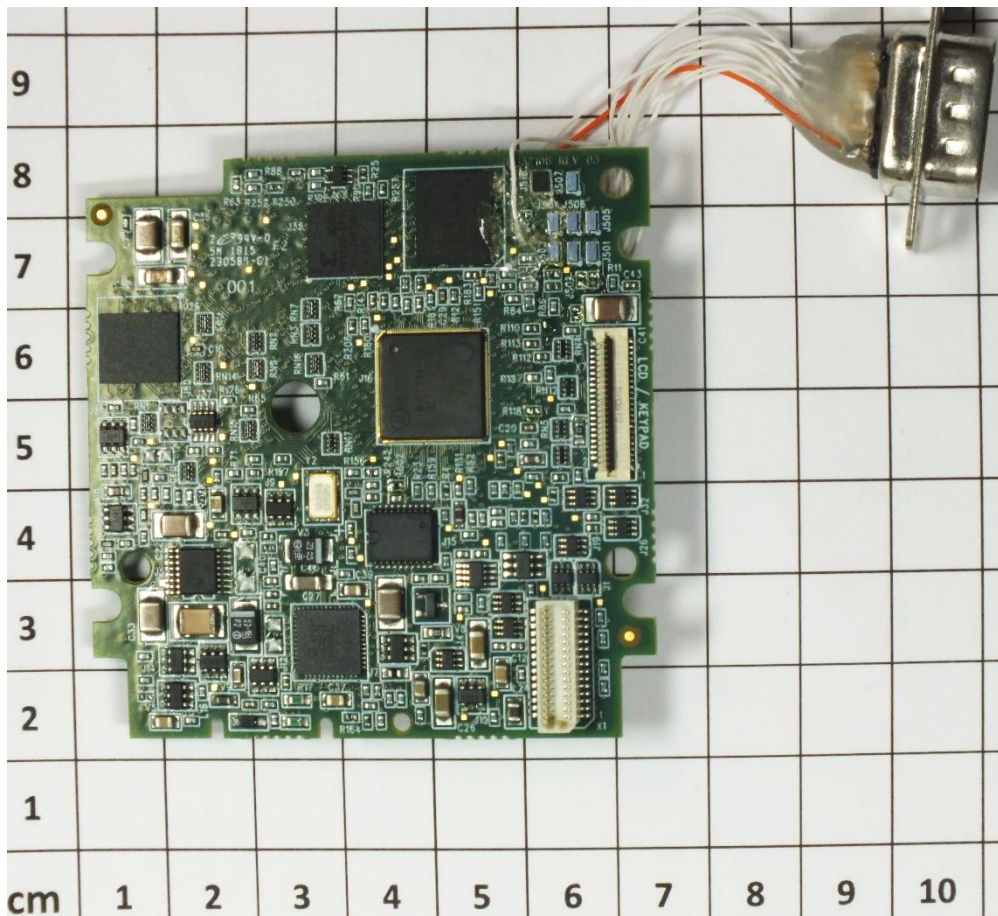

WLAN Module prepared for testing

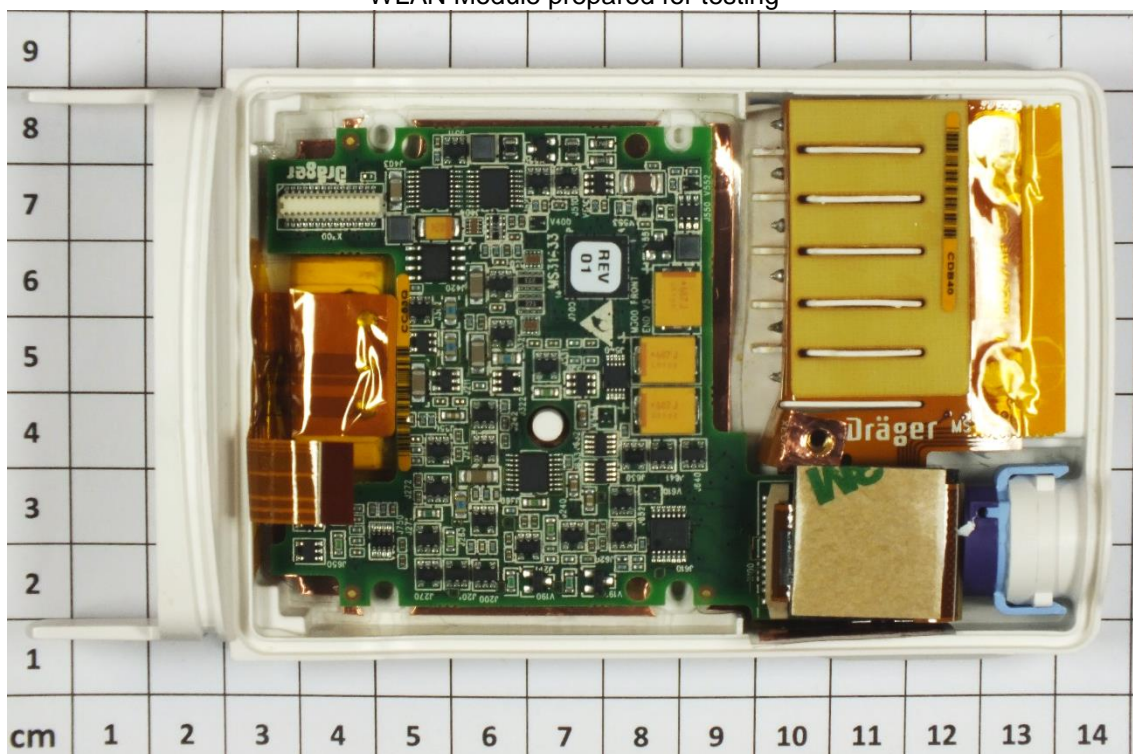

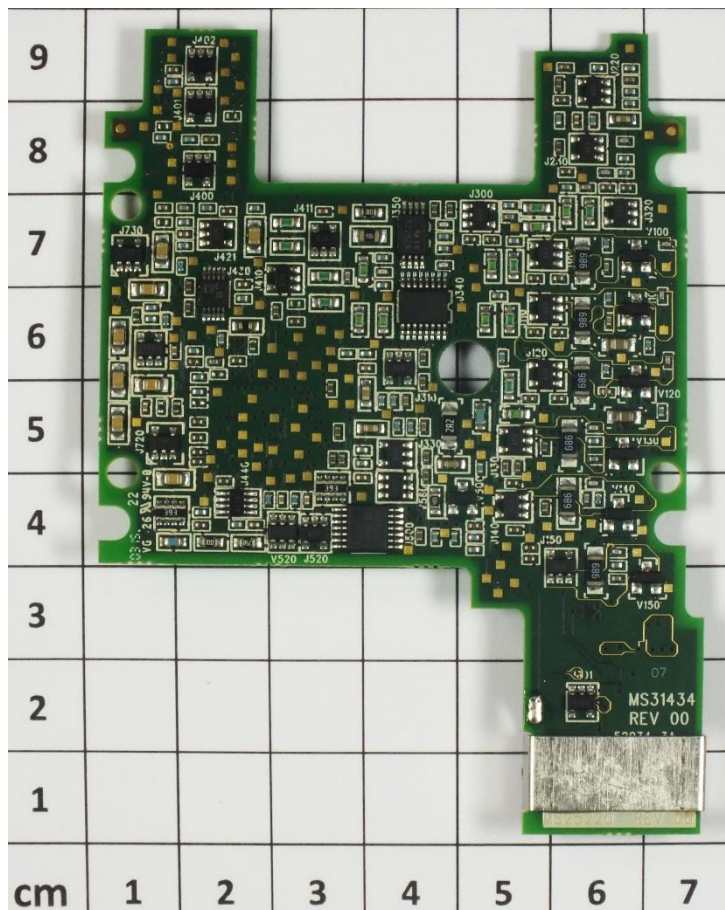
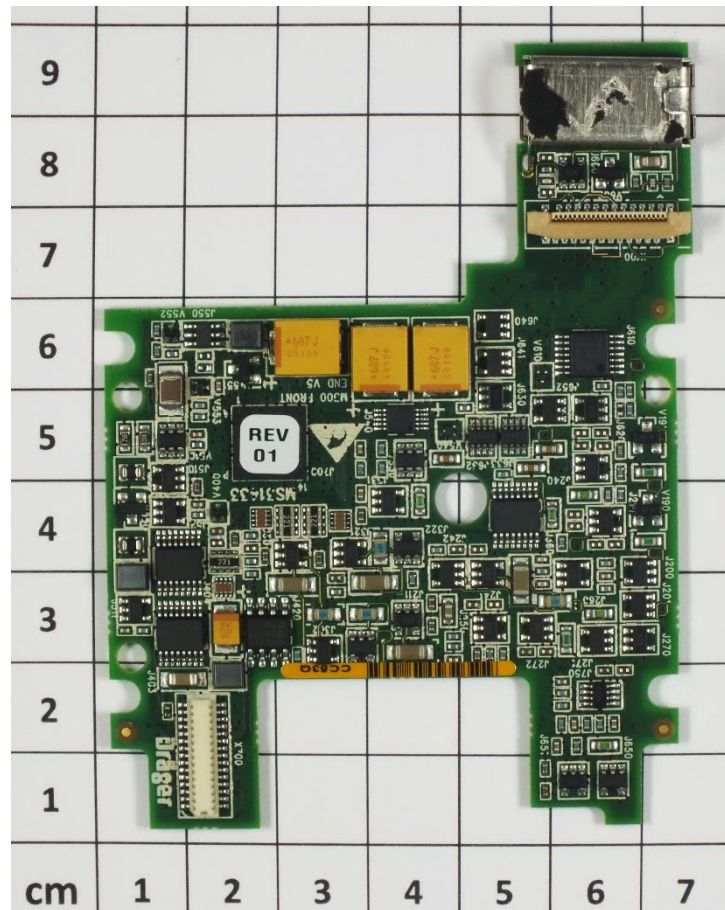





1.3 Antenna structure:



1.4 Cables:

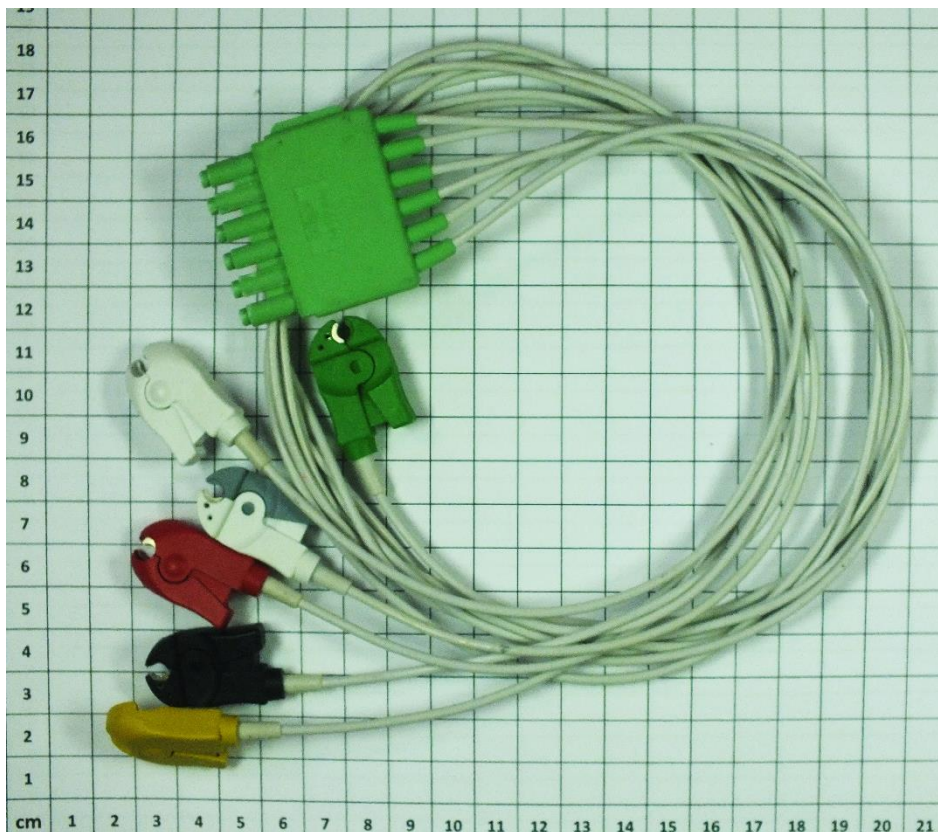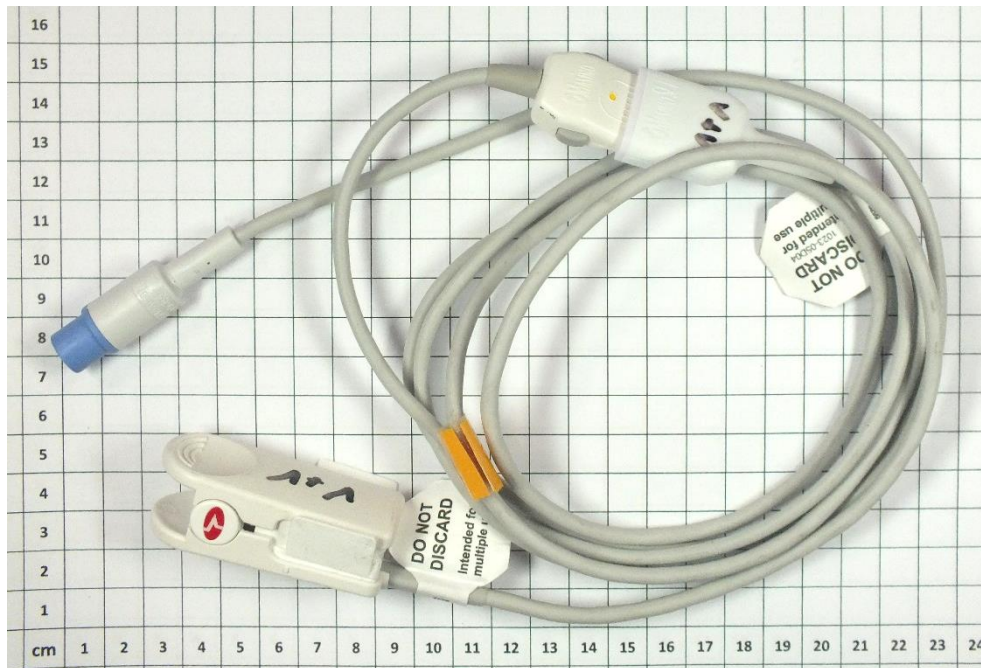

1.5 Power supply and charger:

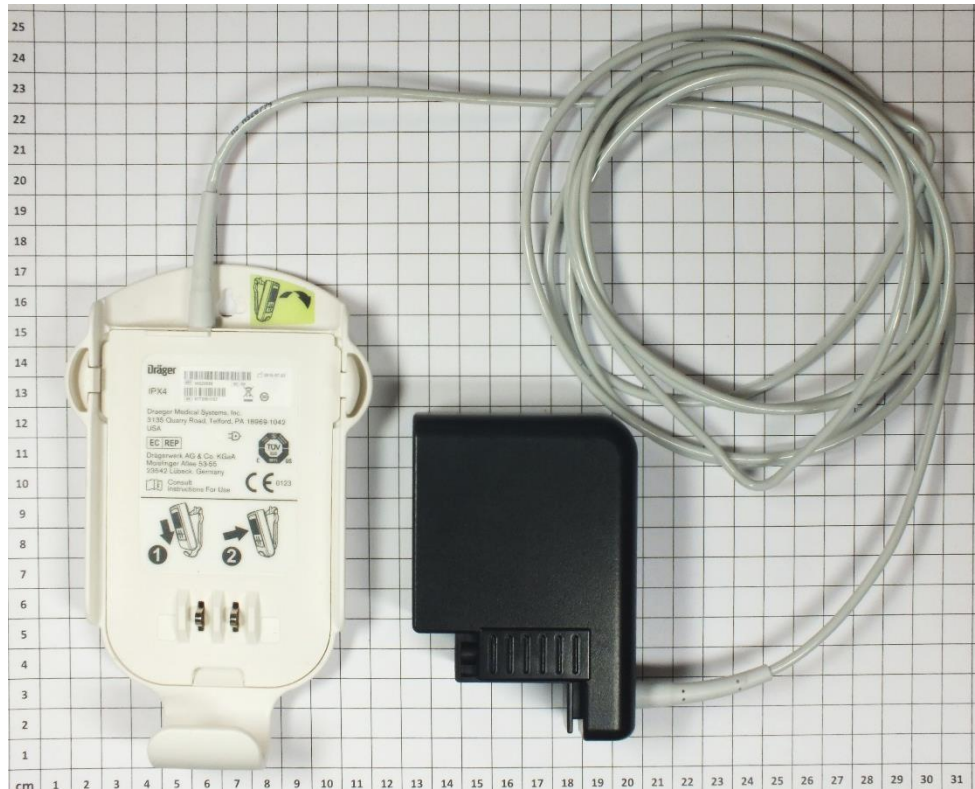





1.6 Control PCB used for testing only:

