

**ANNEX 2 TO TEST REPORT # EMCC-910036IEAB, 2011-06-16**

**PHOTOGRAPHS OF EQUIPMENT UNDER TEST (EUT)**

**EQUIPMENT UNDER TEST:**

Trade Name:	RFID Reader Module M21
Type Designation(s):	MP02001 / Rev. 17 (M21) with antenna: MK07491
Serial Number:	02171789 (RFID Reader M21), ASBE-0027 Antenna
Equipment Class:	Low Power Transceiver
Manufacturer:	Dräger Medical GmbH
Address:	Moislinger Allee 53-55 23558 Lübeck Germany
Phone:	+49 451 882-0
Fax:	+49 451 882-2080

**RELEVANT STANDARD(S):** 47 CFR 15.225, RSS-210 Issue 8,  
limited tests performed, only


**MEASUREMENT PROCEDURE:**

☒ RSS-Gen Issue 3      ☒ ANSI C63.4-2003      ☐ Other

## RFID Reader Module MP02001 (M21) and antennas



EUT: MP02001 / Rev. 17 (top view)

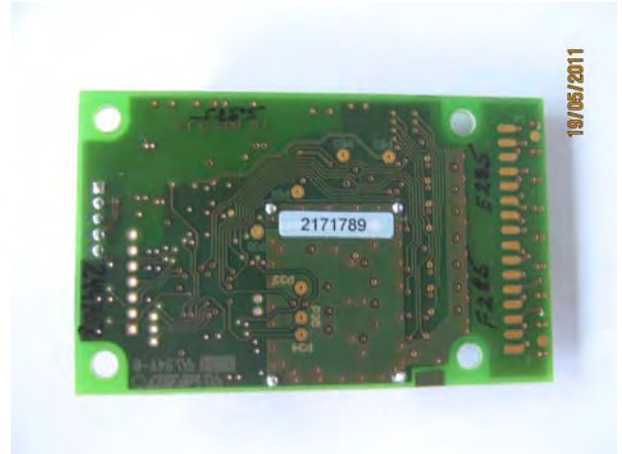


EUT: MP02001 / Rev. 17 (rear view)



EUT: MP02001 / Rev. 17 (label)



Antenna: MK07491(top view)

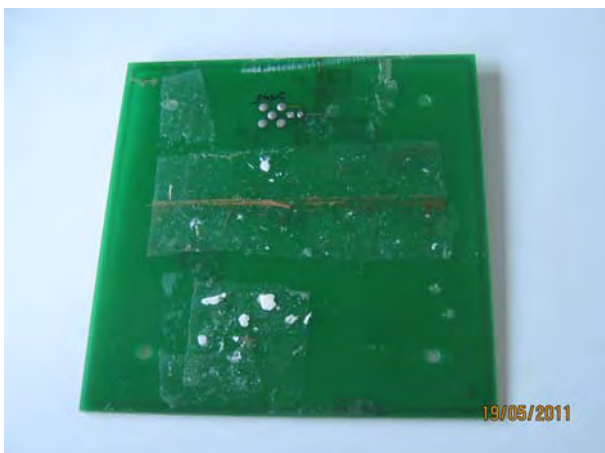
Antenna: FEIG antenna 100 mm \* 100 mm SN 1020307  
(used for Carrier Frequency Stability test only)