



**Label #5683**  
**Right Side Label**



**MODEL#: 60-3020**  
**IC: 7865A-603020**  
**FCC ID: WKO-603020**

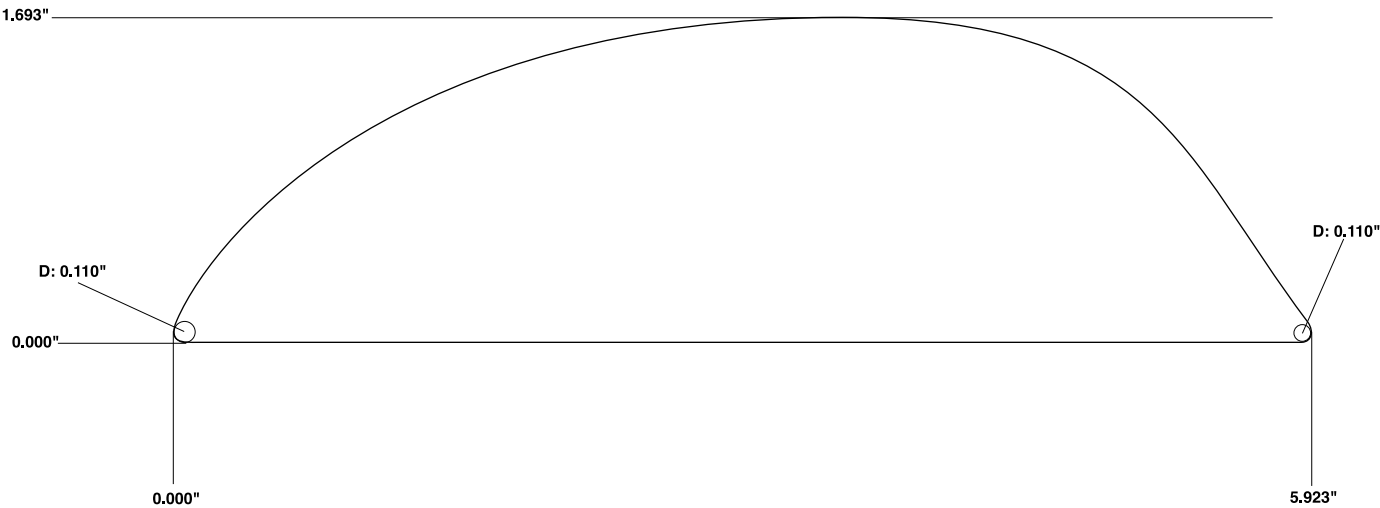

**Read manual  
before use**

**CAUTIONS:**

- Prior to catheter use, confirm position with x-ray
- Federal (USA) law restricts this device to sale by or on the order of a physician

**VIASYS MedSystems**, Wheeling, IL 60090 U.S.A.  
1(800)323-6305 1(847)403-3400