



The Testcenter facility 'Dosimetric Test Lab' within IMST GmbH is accredited by the German National 'Deutsche Akkreditierungsstelle GmbH (DAkkS)' for testing according to the scope as listed in the accreditation certificate: D-PL-12139-01-00.

Appendix for the Report

Dosimetric Assessment of the Prodigi Tablet PGI-100 from HumanWare

(FCC ID: 0019188978PGITAB)

(IC: 8670A-PGITAB)

According to the FCC Requirements

May 20, 2014

IMST GmbH

Carl-Friedrich-Gauß-Str. 2 - 4 D-47475 Kamp-Lintfort

Customer

HumanWare 445, Rue Du Parc-Industriel Longueuil, (Quebec) Canada J4H 3V7

The test results only relate to the items tested.

This report shall not be reproduced except in full without the written approval of the testing laboratory.

Dasy_Report_FCC_DECT_1900_1.1.doc/28.11.2013/AvB

Subject of Investigation



Fig.1: Picture of the device under test.

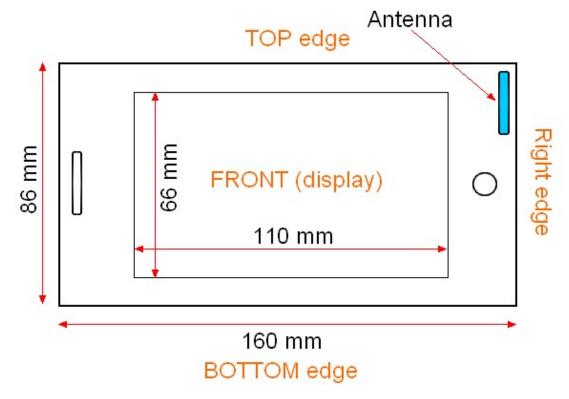


Fig. 2: Antenna location and separation distances.

7.9 Pictures of the Device under Test

Fig. 8 - 9 show the device under test.





Fig. 8: Front and back view of HumanWare Prodigi Tablet PGI-100.

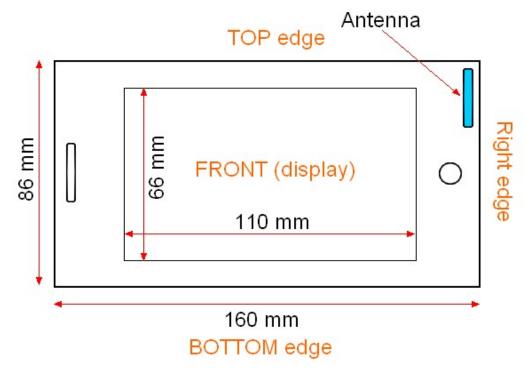


Fig. 9: Antenna location and separation distances.

7.10 Test Positions for the Device under Test

Fig. 10 - 14 show the test positions for the SAR measurements.

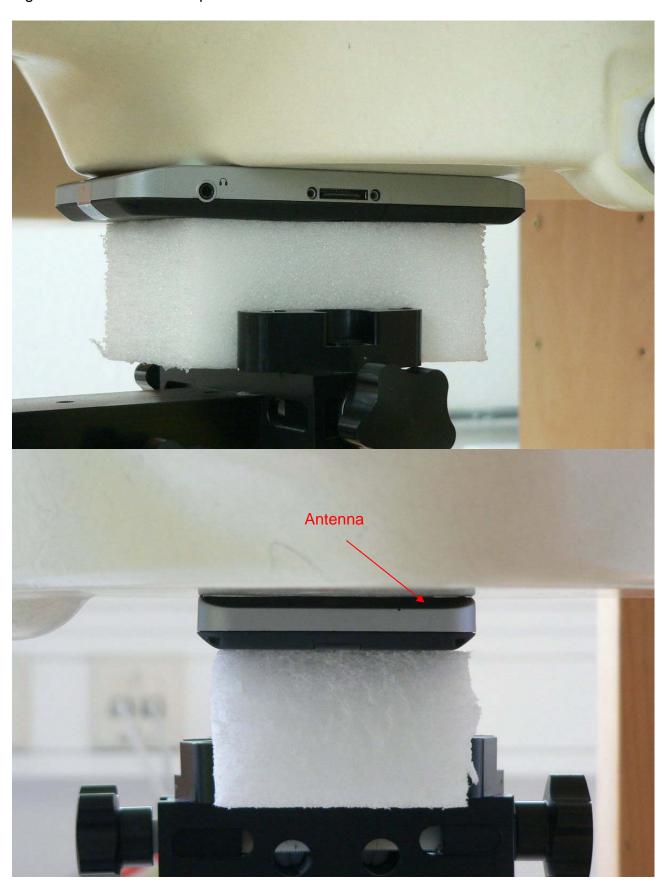


Fig. 10: Body supported configuration, position 1, front side toward the phantom, gap = 0 mm.



Fig. 11: Body supported configuration, position 2, back side toward the phantom, gap = 0 mm.



Fig. 12: Body supported configuration, position 3, top edge toward the phantom, gap = 0 mm.



Fig. 13: Body supported configuration, position 4, right edge toward the phantom, gap = 0 mm.

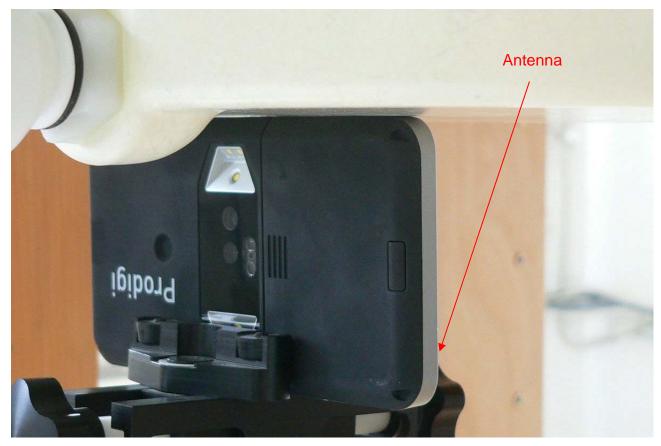


Fig. 14: Body supported configuration, position 5, bottom edge toward the phantom, gap = 0 mm.