

Report No.: RZA1103-0427SAR01R1



OET 65 TEST REPORT

Product Name Digital Portable Radio

Model PD702 U(2)/PD705 U(2)/ PD706 U(2)/ PD708 U(2)

FCC ID YAMPD70XU2

Client Hytera Communications Corporation Ltd.

TA Technology (Shanghai) Co., Ltd. 报告专用章

GENERAL SUMMARY

Product Name	Digital Portable Radio	Model	PD702 U(2)/PD705 U(2)/ PD706 U(2)/ PD708 U(2)	
FCC ID	YAMPD70XU2	Report No.	RZA1103-0427SAR	
Client	Hytera Communications (Corporation Ltd.		
Manufacturer	Hytera Communications (Corporation Ltd.		
Reference Standard(s)	IEEE Std C95.1, 1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 KHz to 300 GHz. IEEE Std 1528™-2003: IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques. SUPPLEMENT C Edition 01-01 to OET BULLETIN 65 Edition 97-01 June 2001 including DA 02-1438 June 19, 2002: Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields Additional Information for Evaluation Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions.			
Conclusion	This portable wireless equipment has been measured in all cases requested by the relevant standards. Test results in Chapter 7 of this test report are below limits specified in the relevant standards. General Judgment: Pass (Stamp) Date of issue: April 18 th , 2011			
Comment	The test result only response	onds to the mea	asured sample.	

Approved by Mo 135 1

Revised by

Performe

Li Siyuan

Yang Weizhong

Ling Minbao

TABLE OF CONTENT

1. Ge	eneral Information	4
1.1.	Notes of the Test Report	4
1.2.	Testing Laboratory	4
1.3.	Applicant Information	5
1.4.	Manufacturer Information	5
1.5.	Information of EUT	6
1.6.	The Maximum SAR _{1g} Values and Power of each tested Mode	6
1.7.	Test Date	6
2. Op	perational Conditions during Test	7
3. SA	AR Measurements System Configuration	8
3.1.	SAR Measurement Set-up	8
3.2.	DASY4 E-field Probe System	9
3.2	2.1. EX3DV4 Probe Specification	9
3.2	2.2. E-field Probe Calibration	10
3.3.	Other Test Equipment	10
3.3	3.1. Device Holder for Transmitters	10
3.3	3.2. Phantom	11
3.4.	Scanning Procedure	11
3.5.	Data Storage and Evaluation	13
3.5	5.1. Data Storage	13
3.5	5.2. Data Evaluation by SEMCAD	13
3.6.	System Check	16
3.7.	Equivalent Tissues	17
4. La	boratory Environment	17
5. Ch	narcteristics of the Test	18
5.1.	Applicable Limit Regulations	18
5.2.	Applicable Measurement Standards	18
6. Cc	onducted Output Power Measurement	19
6.1.	Conducted Power Results	19
7. Te	st Results	20
7.1.	Dielectric Performance	20
7.2.	System Check Results	20
7.3.	Summary of Measurement Results	21
8. Me	easurement Uncertainty	23
9. Ma	ain Test Instruments	24
ANNEX	X A: Test Layout	25
ANNEX	X B: System Check Results	26
ANNEX	X C: Graph Results	28
ANNE	X D: Probe Calibration Certificate	41
ANNE	X E: D450V3 Dipole Calibration Certificate	52
	X F: DAE4 Calibration Certificate	
ANNE	X G: The EUT Appearances and Test Configuration	66

Report No. RZA1103-0427SAR

Page 4 of 67

1. General Information

1.1. Notes of the Test Report

TA Technology (Shanghai) Co., Ltd. guarantees the reliability of the data presented in this test report, which is the results of measurements and tests performed for the items under test on the date and under the conditions stated in this test report and is based on the knowledge and technical facilities available at TA Technology (Shanghai) Co., Ltd. at the time of execution of the test.

TA Technology (Shanghai) Co., Ltd. is liable to the client for the maintenance by its personnel of the confidentiality of all information related to the items under test and the results of the test. This report only refers to the item that has undergone the test.

This report standalone dose not constitute or imply by its own an approval of the product by the certification Bodies or competent Authorities. This report cannot be used partially or in full for publicity and/or promotional purposes without previous written approval of **TA Technology (Shanghai) Co., Ltd.** and the Accreditation Bodies, if it applies.

If the electrical report is inconsistent with the printed one, it should be subject to the latter.

1.2. Testing Laboratory

Company: TA Technology (Shanghai) Co., Ltd.

Address: No.145, Jintang Rd, Tangzhen Industry Park, Pudong Shanghai, China

City: Shanghai

Post code: 201201

Country: P. R. China

Contact: Yang Weizhong

Telephone: +86-021-50791141/2/3

Fax: +86-021-50791141/2/3-8000 Website: http://www.ta-shanghai.com

E-mail: yangweizhong@ta-shanghai.com

Report No. RZA1103-0427SAR

Page 5 of 67

1.3. Applicant Information

Company: Hytera Communications Corporation Ltd.

Address: HYT Tower, Hi-Tech Industrial Park North, Nanshan District, Shenzhen China. 518057

City: Shenzhen

Postal Code: /

Country: P. R. China

Telephone: /

Fax: /

1.4. Manufacturer Information

Company: Hytera Communications Corporation Ltd.

Address: HYT Tower, Hi-Tech Industrial Park North, Nanshan District, Shenzhen China. 518057

City: Shenzhen

Postal Code: /

Country: P. R. China

Telephone: /

Fax: /

1.5. Information of EUT

General Information

Device Type:	Portable Device	
Exposure Category:	Controlled Environment /Occupational	
Product Name:	Digital Portable Radio	
S/N:		
Hardware Version:		
Software Version:		
Antenna Type:	External Antenna	
Device Operating Configurations:		
Operating Mode(s):	450.5 MHz –519.5 MHz	
Test Modulation:	FM (Analog), 4FSK(digital)	
Operating Frequency Range(s):	450.5 MHz ~ 519.5 MHz(UHF)	
Test Frequency:	450.5 MHz – 467.5MHz – 485MHz – 502.5MHz – 519.5MHz	

Equipment Under Test (EUT) is Digital Portable Radio. SAR is tested for 450.5 - 519.5 MHz only. The EUT has one external antenna that is used for Tx/Rx.

The sample undergoing test was selected by the Client.

Components list please refer to documents of the manufacturer.

1.6. The Maximum SAR_{1g} Values and Power of each tested Mode

Configuration

Mode	Channel/f(MHz)	Position	SAR _{1g} (W/kg)
UHF	485	Body-Worn for 12.5 KHz	5.978

Maximum Power

Mode	Max Conducted Power (dBm)
Analog 12.5K UHF	36.95
Digital 12.5K UHF	35.99

1.7. Test Date

The test is performed from April 7, 2011 to April 8, 2011.

Report No. RZA1103-0427SAR

Page 7 of 67

2. Operational Conditions during Test

The spatial peak SAR values were assessed for UHF (450.5 MHz, 467.5 MHz, 485MHz, 502.5MHz and 519.5MHz) systems. Battery and accessories shall be specified by the manufacturer. The EUT battery must be fully charged and checked periodically during the test to ascertain uniform power output.

3. SAR Measurements System Configuration

3.1. SAR Measurement Set-up

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- A unit to operate the optical surface detector which is connected to the EOC.
- The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DASY4 measurement server.
- The DASY4 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2003
- DASY4 software and SEMCAD data evaluation software.
- Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles allowing to validate the proper functioning of the system.

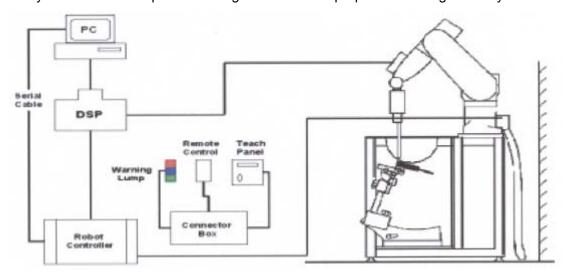


Figure 1. SAR Lab Test Measurement Set-up

3.2. DASY4 E-field Probe System

The SAR measurements were conducted with the dosimetric probe EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation.

3.2.1. EX3DV4 Probe Specification

Construction Symmetrical design with triangular core

Built-in shielding against static charges PEEK enclosure material (resistant to

organic solvents, e.g., DGBE)

Calibration ISO/IEC 17025 calibration service available

Frequency 10 MHz to > 6 GHz

Linearity: ± 0.2 dB (30 MHz to 6 GHz)

Directivity \pm 0.3 dB in HSL (rotation around probe

axis) ± 0.5 dB in tissue material (rotation

normal to probe axis)

Dynamic Range 10 μ W/g to > 100 mW/g Linearity:

 \pm 0.2dB (noise: typically < 1 μ W/g)

Dimensions Overall length: 330 mm (Tip: 20 mm)

Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole

centers: 1 mm

Application High precision dosimetric

measurements in any exposure

scenario (e.g., very strong gradient

fields).

Only probe which enables compliance testing for frequencies up to 6 GHz

with precision of better 30%.



Figure 2.EX3DV4 E-field Probe



Figure 3. EX3DV4 E-field probe

Report No. RZA1103-0427SAR

3.2.2. E-field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy was evaluated and found to be better than \pm 0.25dB. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies bellow 1 GHz, and in a wave guide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where: $\Delta t = \text{Exposure time (30 seconds)}$,

C = Heat capacity of tissue (brain or muscle),

 ΔT = Temperature increase due to RF exposure.

Or

$$SAR = \frac{|E|^2 \sigma}{\rho}$$

Where:

 σ = Simulated tissue conductivity,

 ρ = Tissue density (kg/m3).

3.3. Other Test Equipment

3.3.1. Device Holder for Transmitters

The DASY device holder is designed to cope with the die rent positions given in the standard.

It has two scales for device rotation (with respect to the body axis) and device inclination (with

respect to the line between the ear reference points). The rotation centers for both scales is the

ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder is constructed of low-loss POM material. The amount of dielectric material



Page 10 of 67

Figure 4.Device Holder

has been reduced in the closest vicinity of the device, since measurements have suggested that the inference of the clamp on the test results could thus be lowered.

3.3.2. **Phantom**

The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (Oval Flat) phantom defined in IEEE 1528-2003, CENELEC 50361 and IEC 62209. It enables the dosimetric evaluation of wireless portable device usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points with the robot.

Shell Thickness 2 ± 0.2 mm Filling Volume Approx. 30 liters Dimensions 190×600×400 mm (H×L×W)



Figure 5.ELI4 Phantom

3.4. Scanning Procedure

The DASY4 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

- The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. ± 5 %.
- The "surface check" measurement tests the optical surface detection system of the DASY4 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above ± 0.1mm). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within ± 30°.)

Report No. RZA1103-0427SAR

Page 12 of 67

Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values before running a detailed measurement around the hot spot.Before starting the area scan a grid spacing of 15 mm x 15 mm is set. During the scan the distance of the probe to the phantom remains unchanged.

After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

Zoom Scan

Zoom Scans are used to estimate the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default Zoom Scan is done by 7x7x7 points within a cube whose base is centered around the maxima found in the preceding area scan.

Spatial Peak Detection

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY4 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard s method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard s method for extrapolation. For a grid using 7x7x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1g and 10g cubes.

 A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube 7x7x7 scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

3.5. Data Storage and Evaluation

3.5.1. Data Storage

The DASY4 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DA4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm²], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

3.5.2. Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	SensitivityConversion factorDiode compression point	Normi, a_{i0} , a_{i1} , a_{i2} ConvF _i Dcp _i
Device parameters:	- Frequency - Crest factor	f cf
Media parameters:	- Conductivity - Density	σ ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot c f/d c p_i$$

With V_i = compensated signal of channel i (i = x, y, z)

 U_i = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes: $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes: $H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1} f + a_{i2} f^2) / f$

With V_i = compensated signal of channel i (i = x, y, z)

Norm_i = sensor sensitivity of channel i (i = x, y, z)

[mV/(V/m)²] for E-field Probes

ConvF = sensitivity enhancement in solution

a_{ij} = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 E_i = electric field strength of channel i in V/m

 H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot}^2 \cdot \sigma) / (\rho \cdot 1000)$$

Report No. RZA1103-0427SAR

Page 15 of 67

with **SAR** = local specific absorption rate in mW/g

 $\boldsymbol{E_{tot}}$ = total field strength in V/m

 σ = conductivity in [mho/m] or [Siemens/m]

 ρ = equivalent tissue density in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{\text{pwe}} = E_{\text{tot}}^2 / 3770$$
 or $P_{\text{pwe}} = H_{\text{tot}}^2 \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm²

 $\boldsymbol{E_{tot}}$ = total electric field strength in V/m

H_{tot} = total magnetic field strength in A/m

3.6. System Check

The manufacturer calibrates the probes annually. Dielectric parameters of the tissue simulants were measured every day using the dielectric probe kit and the network analyser. A system check measurement was made following the determination of the dielectric parameters of the simulant, using the dipole validation kit. A power level of 398 mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom. The system check results (dielectric parameters and SAR values) are given in the table 7 and table 8.

System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system (±10 %).

System check is performed regularly on all frequency bands where tests are performed with the DASY4 system.

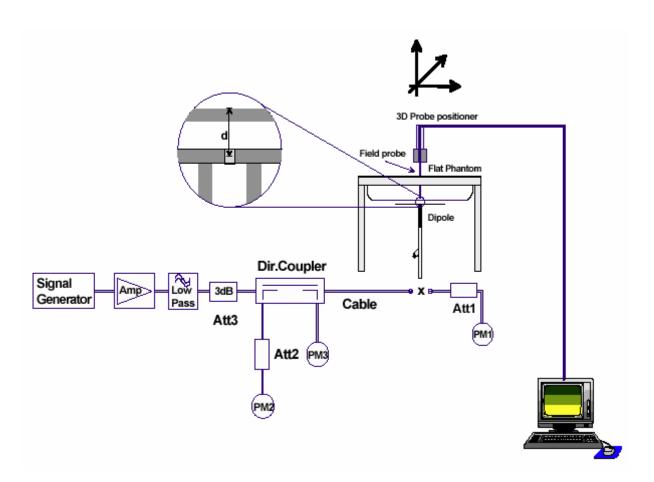


Figure 6. System Check Set-up

3.7. Equivalent Tissues

The liquid is consisted of water, sugar, salt, Preventol and Cellulose. The liquid has previously been proven to be suited for worst-case. The Table 1 and Table 2 show the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the OET 65.

Table 1: Composition of the Head Tissue Equivalent Matter

MIXTURE%	FREQUENCY(Brain) 450MHz		
Water	38.56		
Sugar	56.32		
Salt	3.95		
Preventol	0.10		
Cellulose	1.07		
Dielectric Parameters	5-450MU42 50 07		
Target Value	f=450MHz ε=43.5 σ=0.87		

Table 2: Composition of the Body Tissue Equivalent Matter

MIXTURE%	FREQUENCY(Body) 450MHz	
Water	51.16	
Sugar	46.78	
Salt	1.49	
Preventol	0.10	
Cellulose	0.47	
Dielectric Parameters	5-450MU50.70.04	
Target Value	f=450MHz ε=56.7 σ =0.94	

4. Laboratory Environment

Table 3: The Ambient Conditions during Test

Table 3. The Ambient Conditions during Test				
Temperature	Min. = 20°C, Max. = 25 °C			
Relative humidity	Min. = 30%, Max. = 70%			
Ground system resistance	< 0.5 Ω			
Ambient noise is checked and found very low and in compliance with requirement of standards.				
Reflection of surrounding objects is minimi	Reflection of surrounding objects is minimized and in compliance with requirement of standards.			

5. Charcteristics of the Test

5.1. Applicable Limit Regulations

IEEE Std C95.1, 1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 KHz to 300 GHz.

5.2. Applicable Measurement Standards

IEEE Std 1528™-2003: IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques.

SUPPLEMENT C Edition 01-01 to OET BULLETIN 65 Edition 97-01 June 2001 including DA 02-1438 June 19, 2002: Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields Additional Information for Evaluation Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions.

6. Conducted Output Power Measurement

6.1. Conducted Power Results

Table 4: Conducted Power Measurement Results

Analog 12.5K UHF	Conducted Power				
Alialog 12.5K OHF	450.5 MHz	467.5MHz	485MHz	502.5MHz	519.5MHz
Test Result (dBm)	36.05	35.93	36.95	36.06	36.06
Digital 12 EK IIUE	Conducted Power				
Digital 12.5K UHF	450.5 MHz	467.5MHz	485MHz	502.5MHz	519.5MHz
Test Result (dBm)	35.92	35.86	35.91	35.99	35.99

7. Test Results

7.1. Dielectric Performance

Table 5: Dielectric Performance of Head Tissue Simulating Liquid

Eroguenev	Description	Dielectric Par	Temp	
Frequency		ε _r	σ(s/m)	C
	Target value	43.50	0.87	,
450MHz	±5% window	41.33 — 45.68	0.83 — 0.91	1
(head)	Measurement value 2011-4-7	44.75	0.88	21.6

Table 6: Dielectric Performance of Body Tissue Simulating Liquid

Eroguepov	Description	Dielectric Par	Temp	
Frequency		ε _r	σ(s/m)	${\mathfrak C}$
	Target value	56.70	0.94	,
450MHz	±5% window	53.87 — 59.54	0.89 — 0.99	,
(body)	Measurement value 2011-4-8	57.02	0.94	21.5

7.2. System Check Results

Table 7: System Check for Head Tissue Simulating Liquid

Frequency	Description	SAR(W/kg)		Diele Paran	Temp	
		10g	1g	ε _r	σ(s/m)	$^{\circ}$
	Recommended value	1.25	1.87	44.2	0.86	,
450MHz	±10% window	1.13—1.38	1.68 — 2.06	44.2		/
450MH2	Measurement value	1.31	2.00	44.75		21.6
	2011-4-7	1.51	2.00	44.73		21.0

Note: 1. The graph results see ANNEX B.

2. Recommended Values used derive from the calibration certificate and 398 mW is used as feeding power to the calibrated dipole.

Table 8: System Check for Body Tissue Simulating Liquid

Frequency	Description	SAR(V	Diele Paran	Temp		
		10g	1g	ε _r	σ(s/m)	$^{\circ}\mathbb{C}$
	Recommended value	1.18	1.77	54.1	0.90	1
450MHz	±10% window	1.06—1.30	1.59 — 1.95	54.1		/
450141712	Measurement value	1.17	1.78	57.02	0.94	21.5
	2011-4-8	1.17	1.76	57.02	0.94	21.5

Note: 1. The graph results see ANNEX B.

2. Recommended Values used derive from the calibration certificate and 398 mW is used as feeding power to the calibrated dipole.

7.3. Summary of Measurement Results

7.3.1. UHF

Table 9: SAR Values (UHF)

Limits		1 g Avera	ge (W/kg)	Power Drift (dB)						
		8	.0	± 0.21	Graph					
-	£/8411_\	Duty	Cycle	Davier Drift (dD)	Results					
Frequency	f(MHz)	100% 50%		Power Drift (dB)						
The EUT display towards phantom for 12.5 KHz (Face Held)										
519.5 MHz	519.5 MHz	4.280	2.140	-0.159	Figure 9					
502.5 MHz	502.5 MHz	5.990	2.995	-0.126	Figure 10					
485 MHz	485 MHz	6.210	3.105	-0.189	Figure 11					
467.5 MHz	467.5 MHz	4.730	2.365	-0.066	Figure 12					
450.5 MHz	450.5 MHz	5.150	2.575	-0.075	Figure 13					
The EU	T display towards	ground with	belt clip for	12.5 KHz (Body-Wo	rn)					
519.5 MHz	519.5 MHz	11.300	5.650	-0.083	Figure 14					
502.5 MHz	502.5 MHz	11.500	5.750	-0.084	Figure 15					
485 MHz	485 MHz	11.800	5.900	-0.057	Figure 16					
467.5 MHz	467.5 MHz	11.100	5.550	-0.136	Figure 17					
450.5 MHz	450.5 MHz	11.000 5.500		-0.022	Figure 18					
The EUT display towards ground with Digital Channel (Body-Worn)										
485 MHz	485 MHz	5.400	2.700	0.066	Figure 19					
The EU	T display towards	ground with	Speaker-Mic	rophone (Body-Wo	rn)					
485 MHz	485 MHz	11.200	5.600	-0.022	Figure 20					

Table 10: SAR Values are scaled for the power drift

Limits		1 g Average (W/kg) 8.0		Power Drift (dB) ± 0.21	+ Power Drift	SAR 1g (W/kg) (include + power drift)	
Frequency	f(MHz)	Duty Cycle		Power	10^(dB/10)	Duty Cycle	
rrequency	I(IVITIZ)	100%	50%	Drift(dB)		100%	50%
	The EUT displa	ay towards	s phantor	n for 12.5 KH	lz (Face Held)	
519.5 MHz	519.5 MHz	4.280	2.140	0.159	1.037	4.440	2.220
502.5 MHz	502.5 MHz	5.990	2.995	0.126	1.029	6.166	3.083
485 MHz	485 MHz	6.210	3.105	0.189	1.044	6.486	3.243
467.5 MHz	467.5 MHz	4.730	2.365	0.066	1.015	4.802	2.401
450.5 MHz	450.5 MHz	5.150	2.575	0.075	1.017	5.240	2.620
The	EUT display towa	ards groui	nd with be	elt clip for 12	2.5 KHz (Body	-Worn)	
519.5 MHz	519.5 MHz	11.300	5.650	0.083	1.019	11.518	5.759
502.5 MHz	502.5 MHz	11.500	5.750	0.084	1.020	11.725	5.862
485 MHz	485 MHz	11.800	5.900	0.057	1.013	11.956	5.978
467.5 MHz	467.5 MHz	11.100	5.550	0.136	1.032	11.453	5.727
450.5 MHz	450.5 MHz	11.000	5.500	0.022	1.005	11.056	5.528
7	he EUT display to	owards gr	ound with	Digital Cha	nnel (Body-W	orn)	
485 MHz	485 MHz	5.400	2.700	0.066	1.015	5.483	2.741
The	EUT display towa	ards groui	nd with S _l	oeaker-Micro	phone (Body	/-Worn)	
485 MHz	485 MHz	11.200	5.600	0.022	1.005	11.257	5.628

Note: 1. The value with blue color is the maximum SAR Value of each test band.

^{2.} The Exposure category about EUT: controlled environment / Occupational, so the SAR limit is 8.0 W/kg averaged over any 1 gram of tissue.

Report No. RZA1103-0427SAR

Page 23 of 67

8. Measurement Uncertainty

No.	source	Туре	Uncertaint y Value (%)	Probabilit y Distributio	k	Ci	Standard ncertaint y $u_i(\%)$	Degree of freedom		
1	System repetivity	Α	0.5	n N	1	1	0.5	V _{eff} or v_i		
			surement syst					-		
2	-probe calibration	В	5.9	N	1	1	5.9	∞		
3	-axial isotropy of the probe	В	4.7	R	$\sqrt{3}$	$\sqrt{0.5}$	1.9	80		
4	- Hemispherical isotropy of the probe	В	9.4	R	$\sqrt{3}$	$\sqrt{0.5}$	3.9	8		
6	-boundary effect	В	1.9	R	$\sqrt{3}$	1	1.1	∞		
7	-probe linearity	В	4.7	R	$\sqrt{3}$	1	2.7	8		
8	- System detection limits	В	1.0	R	$\sqrt{3}$	1	0.6	∞		
9	-readout Electronics	В	1.0	N	1	1	1.0	∞		
10	-response time	В	0	R	$\sqrt{3}$	1	0	8		
11	-integration time	В	4.32	R	$\sqrt{3}$	1	2.5	∞		
12	-noise	В	0	R	$\sqrt{3}$	1	0	∞		
13	-RF Ambient Conditions	В	3	R	$\sqrt{3}$	1	1.73	∞		
14	-Probe Positioner Mechanical Tolerance	В	0.4	R	$\sqrt{3}$	1	0.2	∞		
15	-Probe Positioning with respect to Phantom Shell	В	2.9	R	$\sqrt{3}$	1	1.7	∞		
16	-Extrapolation, interpolation and Integration Algorithms for Max. SAR Evaluation	В	3.9	R	$\sqrt{3}$	1	2.3	8		
	Test sample Related									
17	-Test Sample Positioning	Α	2.9	N	1	1	4.92	71		
18	-Device Holder Uncertainty	Α	4.1	N	1	1	4.1	5		
19	-Output Power Variation - SAR drift measurement	В	5.0	R	$\sqrt{3}$	1	2.9	∞		
		Phy	sical paramet	ter		 				
20	-phantom	В	4.0	R	$\sqrt{3}$	1	2.3	∞		

Report No. RZA1103-0427SAR

Page 24 of 67

21	-liquid conductivity (deviation from target)	В	5.0	R	$\sqrt{3}$	0.64	1.8	∞
22	-liquid conductivity (measurement uncertainty)	В	0.77	N	1	0.64	0.493	9
23	-liquid permittivity (deviation from target)	В	5.0	R	$\sqrt{3}$	0.6	1.7	8
24	-liquid permittivity (measurement uncertainty)	В	0.29	N	1	0.6	0.174	9
Combined standard uncertainty		$u_c' = \sqrt{\sum_{i=1}^{21} c_i^2 u_i^2}$					11.36	
Expanded uncertainty (confidence interval of 95 %)		$u_e = 2u_c$		N k=2		22.72	_	

9. Main Test Instruments

Table 11: List of Main Instruments

No.	Name	Туре	Serial Number	Calibration Date	Valid Period
01	Network analyzer	Agilent 8753E	US37390326	September 13, 2010	One year
02	Dielectric Probe Kit	Agilent 85070E	US44020115	No Calibration Requested	
03	Power meter	Agilent E4417A	GB41291714	March 12, 2011	One year
04	Power sensor	Agilent N8481H	MY50350004	September 26, 2010	One year
05	Signal Generator	HP 8341B	2730A00804	September 13, 2010	One year
06	Amplifier	IXA-020	0401	No Calibration Requested	
07	E-field Probe	EX3DV4	3677	November 24, 2010	One year
08	DAE	DAE4	871	November 18, 2010	One year
09	Validation Kit 450MHz	D450V3	1065	November 9, 2010	Two years

*****END OF REPORT BODY*****

ANNEX A: Test Layout



Picture 1: Specific Absorption Rate Test Layout



Picture 2: Liquid depth in the Flat Phantom (450 MHz, 15.4cm depth)

ANNEX B: System Check Results

System Performance Check at 450 MHz Head

DUT: Dipole450 MHz; Type: D450V3; Serial: 1065

Date/Time: 4/7/2011 5:26:21 PM

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 450 MHz; σ = 0.88 mho/m; ε_r = 44.75; ρ = 1000 kg/m³

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.6 ℃

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.04, 10.04, 10.04) Calibrated: 11/24/2010;

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

d=15mm, Pin=398mW/Area Scan (41x131x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 2.15 mW/g

d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 52.2 V/m; Power Drift = -0.033 dB

Peak SAR (extrapolated) = 3.29 W/kg

SAR(1 g) = 2.00 mW/g; SAR(10 g) = 1.31 mW/g Maximum value of SAR (measured) = 2.15 mW/g

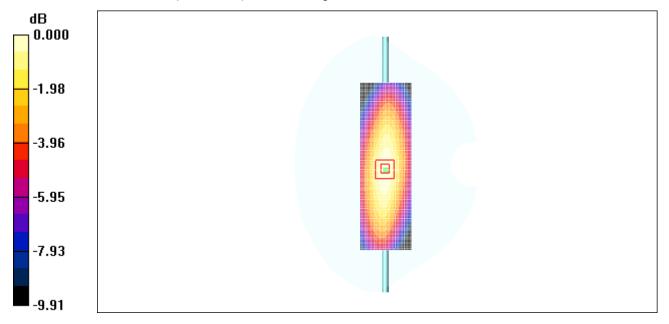

0 dB = 2.15 mW/g

Figure 7 System Performance Check 450MHz 398mW

System Performance Check at 450 MHz Body

DUT: Dipole450 MHz; Type: D450V3; Serial: 1065

Date/Time: 4/8/2011 9:00:21 AM

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 450 MHz; σ = 0.94 mho/m; ε_r = 57.02; ρ = 1000 kg/m³

Ambient Temperature: 22.3 °C Liquid Temperature: 21.5 °C

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62) Calibrated: 11/24/2010;

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

d=15mm, Pin=398mW/Area Scan (61x221x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 1.9 mW/g

d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 44.7 V/m; Power Drift = -0.014 dB

Peak SAR (extrapolated) = 2.64 W/kg

SAR(1 g) = 1.78 mW/g; SAR(10 g) = 1.17 mW/g Maximum value of SAR (measured) = 1.89 mW/g

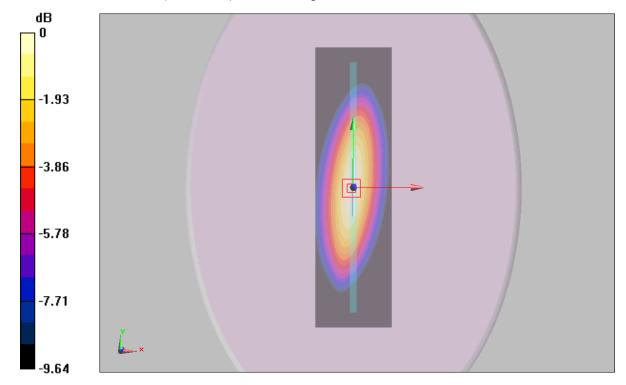

0 dB = 1.89 mW/g

Figure 8 System Performance Check 450MHz 398mW

ANNEX C: Graph Results

Face Held, Front towards Phantom for 12.5 KHz 519.5 MHz

Date/Time: 4/7/2011 9:41:08 PM

Communication System: PTT 450; Frequency: 519.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 519.5 MHz; $\sigma = 0.91 \text{ mho/m}$; $\varepsilon_r = 43.3$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 °C Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.04, 10.04, 10.04); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Phantom 519.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 4.55 mW/g

towards Phantom 519.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 69.7 V/m; Power Drift = -0.159 dB

Peak SAR (extrapolated) = 5.41 W/kg

SAR(1 g) = 4.28 mW/g; SAR(10 g) = 3.25 mW/gMaximum value of SAR (measured) = 4.48 mW/g

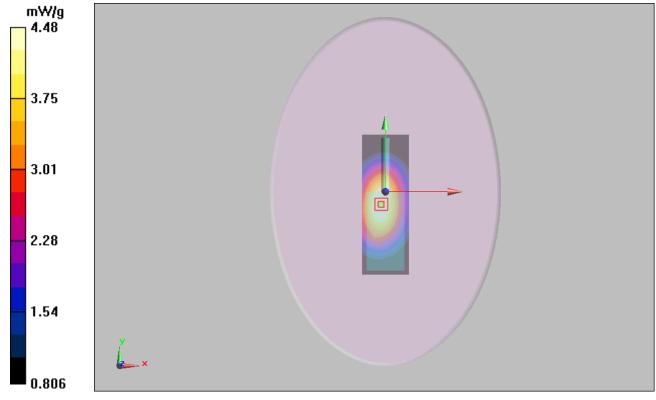


Figure 9 Face Held, Front towards Phantom for 12.5 KHz 519.5 MHz

Face Held, Front towards Phantom for 12.5 KHz 502.5 MHz

Date/Time: 4/7/2011 9:24:21 PM

Communication System: PTT 450; Frequency: 502.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 502.5 MHz; $\sigma = 0.91 \text{ mho/m}$; $\varepsilon_r = 43.6$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 °C Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.04, 10.04, 10.04); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Phantom 502.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 6.31 mW/g

towards Phantom 502.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 82.8 V/m; Power Drift = -0.126 dB

Peak SAR (extrapolated) = 7.63 W/kg

SAR(1 g) = 5.99 mW/g; SAR(10 g) = 4.49 mW/gMaximum value of SAR (measured) = 6.25 mW/g

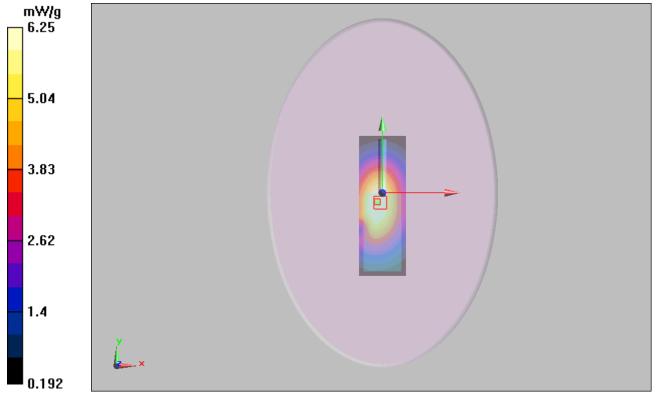


Figure 10 Face Held, Front towards Phantom for 12.5 KHz 502.5 MHz

Face Held, Front towards Phantom for 12.5 KHz 485 MHz

Date/Time: 4/7/2011 9:07:31 PM

Communication System: PTT 450; Frequency: 485 MHz; Duty Cycle: 1:1

Medium parameters used: f = 485 MHz; $\sigma = 0.909 \text{ mho/m}$; $\varepsilon_r = 44$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.04, 10.04, 10.04); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Phantom 485 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 6.48 mW/g

towards Phantom 485 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 83.6 V/m; Power Drift = -0.189 dB

Peak SAR (extrapolated) = 8.12 W/kg

SAR(1 g) = 6.21 mW/g; SAR(10 g) = 4.42 mW/gMaximum value of SAR (measured) = 6.34 mW/g

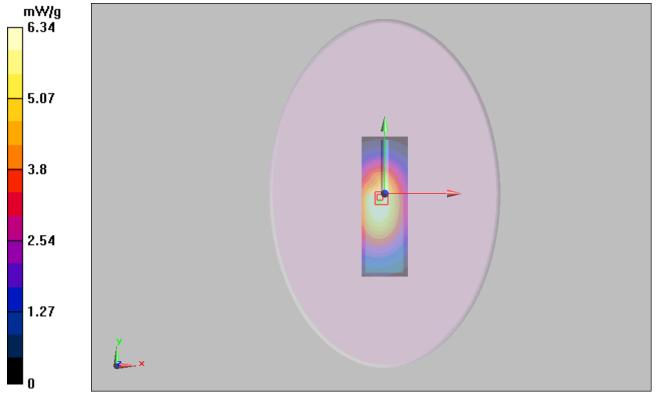


Figure 11 Face Held, Front towards Phantom for 12.5 KHz 485 MHz

Face Held, Front towards Phantom for 12.5 KHz 467.5 MHz

Date/Time: 4/7/2011 9:58:23 PM

Communication System: PTT 450; Frequency: 467.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 467.5 MHz; $\sigma = 0.893 \text{ mho/m}$; $\epsilon_r = 44.4$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 °C Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.04, 10.04, 10.04); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Phantom 467.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 5.01 mW/g

towards Phantom 467.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 74.7 V/m; Power Drift = -0.066 dB

Peak SAR (extrapolated) = 5.95 W/kg

SAR(1 g) = 4.73 mW/g; SAR(10 g) = 3.61 mW/g Maximum value of SAR (measured) = 4.96 mW/g

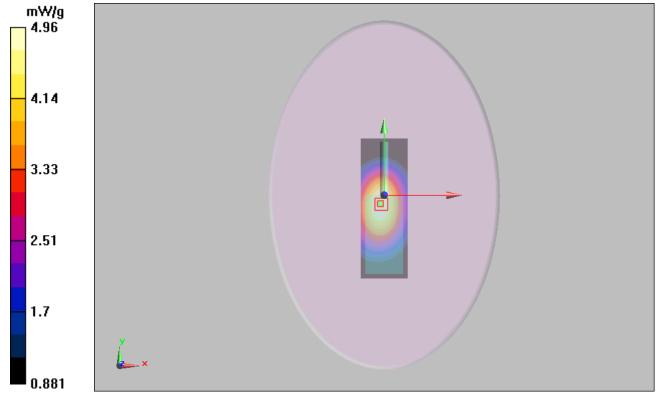


Figure 12 Face Held, Front towards Phantom for 12.5 KHz 467.5 MHz

Face Held, Front towards Phantom for 12.5 KHz 450.5 MHz

Date/Time: 4/7/2011 8:34:10 PM

Communication System: PTT 450; Frequency: 450.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 450.5 MHz; $\sigma = 0.88 \text{ mho/m}$; $\epsilon_r = 44.7$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 °C Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.04, 10.04, 10.04); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Phantom 450.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 5.64 mW/g

towards Phantom 450.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 81.1 V/m; Power Drift = -0.075 dB

Peak SAR (extrapolated) = 6.42 W/kg

SAR(1 g) = 5.15 mW/g; SAR(10 g) = 3.98 mW/gMaximum value of SAR (measured) = 5.39 mW/g

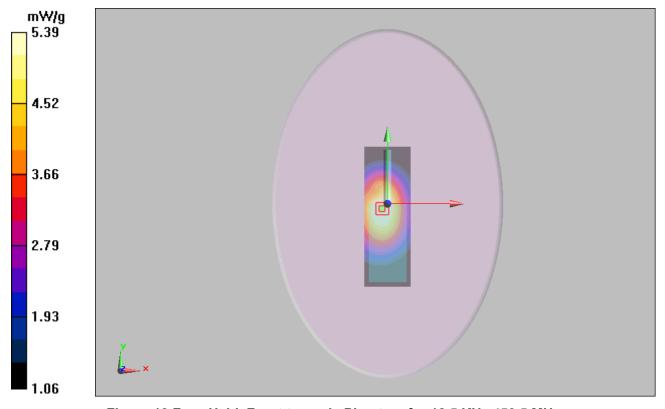


Figure 13 Face Held, Front towards Phantom for 12.5 KHz 450.5 MHz

Body-Worn, Back towards Ground for 12.5 KHz 519.5 MHz

Date/Time: 4/8/2011 5:13:13 PM

Communication System: PTT 450; Frequency: 519.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 519.5 MHz; $\sigma = 0.99 \text{ mho/m}$; $\varepsilon_r = 55.8$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 °C Liquid Temperature: 21.5 °C

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 519.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 12.3 mW/g

towards Ground 519.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 111.7 V/m; Power Drift = -0.083 dB

Peak SAR (extrapolated) = 15.3 W/kg

SAR(1 g) = 11.3 mW/g; SAR(10 g) = 8.01 mW/gMaximum value of SAR (measured) = 11.9 mW/g

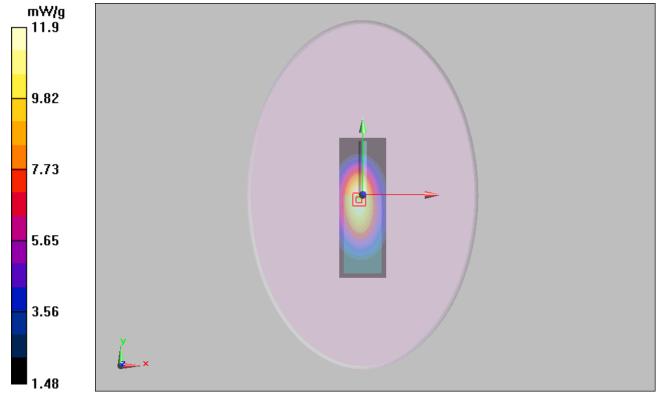


Figure 14 Body-Worn, Back towards Ground for 12.5 KHz 519.5 MHz

Body-Worn, Back towards Ground for 12.5 KHz 502.5 MHz

Date/Time: 4/8/2011 6:56:18 PM

Communication System: PTT 450; Frequency: 502.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 502.5 MHz; $\sigma = 0.99 \text{ mho/m}$; $\epsilon_r = 56$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 502.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 12.3 mW/g

towards Ground 502.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 114.2 V/m; Power Drift = -0.084 dB

Peak SAR (extrapolated) = 15.5 W/kg

SAR(1 g) = 11.5 mW/g; SAR(10 g) = 8.25 mW/g Maximum value of SAR (measured) = 12.2 mW/g

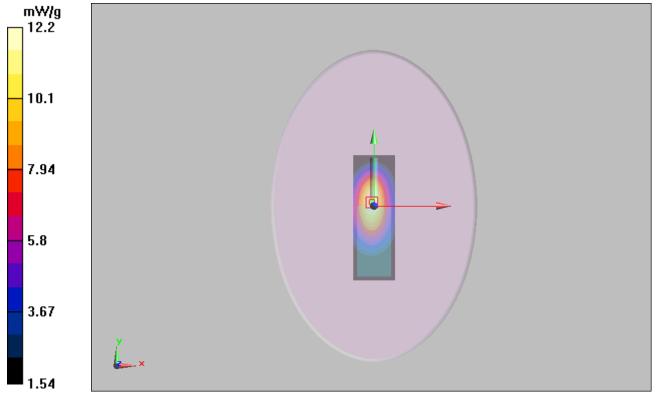


Figure 15 Body-Worn, Back towards Ground for 12.5 KHz 502.5 MHz

Body-Worn, Back towards Ground for 12.5 KHz 485 MHz

Date/Time: 4/8/2011 6:21:43 PM

Communication System: PTT 450; Frequency: 485 MHz; Duty Cycle: 1:1

Medium parameters used: f = 485 MHz; σ = 0.971 mho/m; ε_r = 56.2; ρ = 1000 kg/m³

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 485 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 12.4 mW/g

towards Ground 485 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,


dz=5mm

Reference Value = 111.2 V/m; Power Drift = -0.057 dB

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 11.8 mW/g; SAR(10 g) = 8.38 mW/g

Maximum value of SAR (measured) = 12.6 mW/g

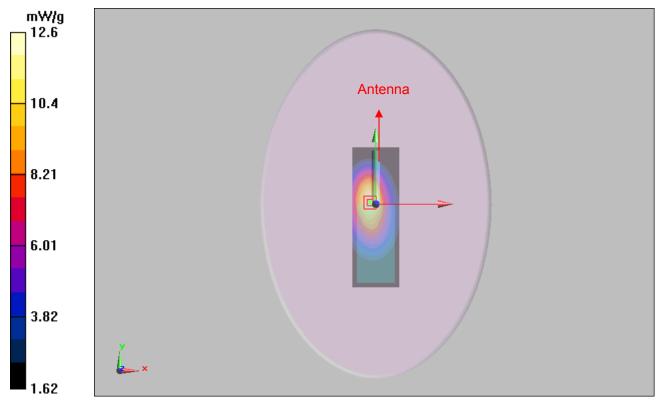

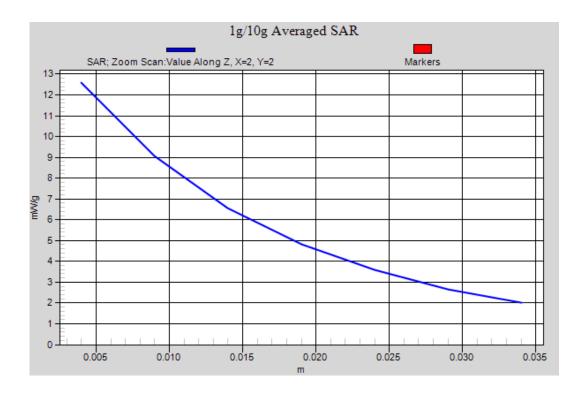


Figure 16 Body-Worn, Back towards Ground for 12.5 KHz 485 MHz

Body-Worn, Back towards Ground for 12.5 KHz 467.5 MHz

Date/Time: 4/8/2011 5:54:02 PM

Communication System: PTT 450; Frequency: 467.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 467.5 MHz; $\sigma = 0.956 \text{ mho/m}$; $\epsilon_r = 56.7$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 467.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 11.8 mW/g

towards Ground 467.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 109.2 V/m; Power Drift = -0.136 dB

Peak SAR (extrapolated) = 15.1 W/kg

SAR(1 g) = 11.1 mW/g; SAR(10 g) = 7.9 mW/g

Maximum value of SAR (measured) = 11.8 mW/g

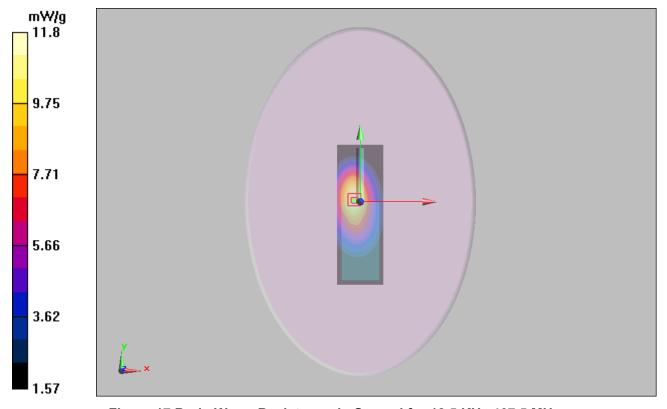


Figure 17 Body-Worn, Back towards Ground for 12.5 KHz 467.5 MHz

Body-Worn, Back towards Ground for 12.5 KHz 450.5 MHz

Date/Time: 4/8/2011 5:31:26 PM

Communication System: PTT 450; Frequency: 450.5 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 450.5 MHz; $\sigma = 0.945 \text{ mho/m}$; $\epsilon_r = 57$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 450.5 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 11.8 mW/g

towards Ground 450.5 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 111.1 V/m; Power Drift = -0.022 dB

Peak SAR (extrapolated) = 14.9 W/kg

SAR(1 g) = 11 mW/g; SAR(10 g) = 7.86 mW/g

Maximum value of SAR (measured) = 11.6 mW/g

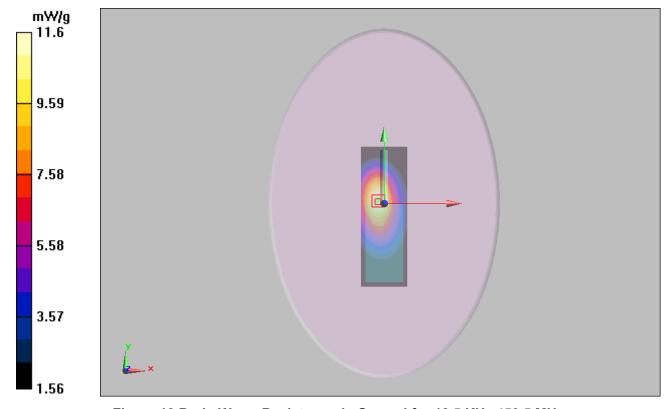


Figure 18 Body-Worn, Back towards Ground for 12.5 KHz 450.5 MHz

Body-Worn, Back towards Ground with Digital for 12.5 KHz 485 MHz

Date/Time: 4/8/2011 8:09:18 PM

Communication System: PTT 450; Frequency: 485 MHz; Duty Cycle: 1:1

Medium parameters used: f = 485 MHz; σ = 0.971 mho/m; ε_r = 56.2; ρ = 1000 kg/m³

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 485 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 5.92 mW/g

towards Ground 485 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,

dz=5mm

Reference Value = 76.3 V/m; Power Drift = 0.066 dB

Peak SAR (extrapolated) = 7.91 W/kg

SAR(1 g) = 5.4 mW/g; SAR(10 g) = 3.87 mW/g

Maximum value of SAR (measured) = 5.75 mW/g

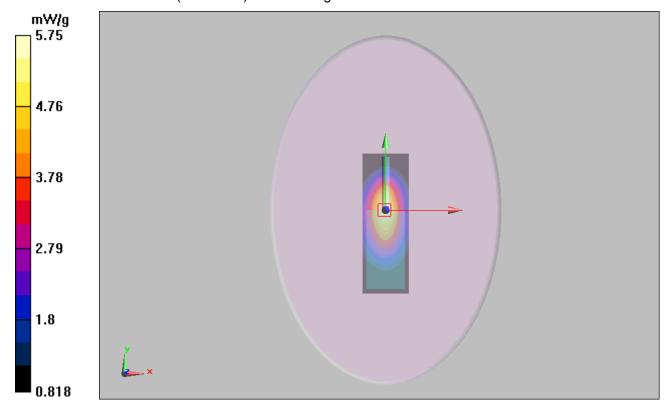


Figure 19 Body-Worn, Back towards Ground with Digital for 12.5 KHz 485 MHz

Body-Worn, Back towards Ground with Speaker-Microphone for 12.5 KHz 485 MHz

Date/Time: 4/8/2011 7:50:03 PM

Communication System: PTT 450; Frequency: 485 MHz; Duty Cycle: 1:1

Medium parameters used: f = 485 MHz; σ = 0.971 mho/m; ε_r = 56.2; ρ = 1000 kg/m³

Ambient Temperature: 22.3 ℃ Liquid Temperature: 21.5 ℃

Phantom section: Flat Section

DASY4 Configuration:

Probe: EX3DV4 - SN3677; ConvF(10.62, 10.62, 10.62); Calibrated: 11/24/2010

Electronics: DAE4 Sn871; Calibrated: 11/18/2010

Phantom: ELI 4.0; Type: QDOVA001BA;

Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

towards Ground 485 MHz/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 12.2 mW/g

towards Ground 485 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,

dz=5mm

Reference Value = 111.3 V/m; Power Drift = -0.022 dB

Peak SAR (extrapolated) = 15.4 W/kg

SAR(1 g) = 11.2 mW/g; SAR(10 g) = 7.93 mW/g

Maximum value of SAR (measured) = 12 mW/g

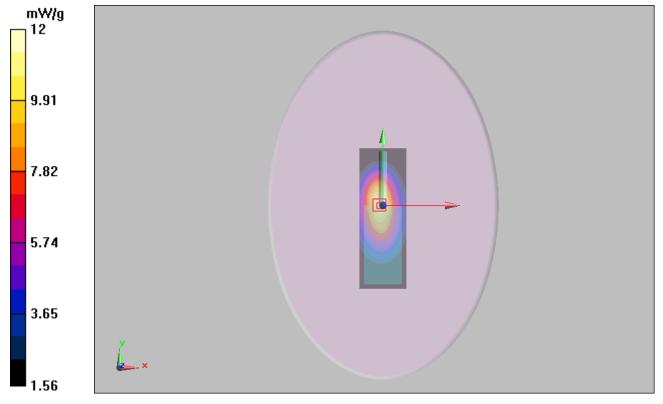


Figure 20 Body-Worn, Back towards Ground with Speaker-Microphone for 12.5 KHz 485 MHz

ANNEX D: Probe Calibration Certificate

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Calibration procedure(s) QA CAL-01.v6, QA CAL-14.v3, QA CAL-23.v3 and QA CAL-25.v2 Calibration procedure for dosimetric E-field probes Calibration date: November 24, 2010 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Def Cal Date (Certificate No.) Scheduled Calibration Primary Standards Cal Date (Certificate No.) Scheduled Calibration Prower meter E44196 GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Apr-11 Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator Reference 30 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5059 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5058 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator Reference 30 dB Attenu	lient TA-SH (Auder)	Certi	ficate No: EX3-3677_Nov10
Calibration procedure(s) QA CAL-01.v6, QA CAL-14.v3, QA CAL-23.v3 and QA CAL-25.v2 Calibration procedure for dosimetric E-field probes Calibration date: November 24, 2010 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Def Cal Date (Certificate No.) Scheduled Calibration Primary Standards Cal Date (Certificate No.) Scheduled Calibration Prower meter E44198 GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Apr-11 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference 20 dB Attenuator SN: S5058 (3c) 30-Mar-10 (No. 217-01161) Mar-11 Reference 30 dB Attenuator SN: S5058 (3c) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5059 (3c) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5059 (3c) 30-Mar-10 (No. 217-01160) Mar-11 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3012_Dec09) Dec-10 DAE4 Secondary Standards ID # Check Date (in house) Scheduled Check RE generator HP 8648C US3842U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Name Function Signature Technical Manager	CALIBRATION	CERTIFICAT		
Calibration procedure for dosimetric E-field probes Calibration date: November 24, 2010 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Prower meter E4412A My41495277 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A My41495277 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01161) Mar-11 Reference 20 dB Attenuator SN: S5058 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference Probe E530V2 SN: 3013 30-Dec-09 (No. E53-3013_Dec09) Dec-10 Apr-11 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Name Function Signature Calibrated by: Katja Pokovic Technical Manager	Object	EX3DV4 - SN:3	677	
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Prower meter E44198 GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY41495277 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY41498067 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference 30 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference 30 dB Attenuator SN: S5080 (20b) 30-Mar-10 (No. 217-01160) Mar-11 Reference Probe E830V2 SN: 3013 30-Dec-09 (No. E83-3013_Dec09) Dec-10 DAE4 SN: 860 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8448C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Name Function Signature Calibrated by:	Calibration procedure(s)			
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards D #	Calibration date:	November 24, 2	2010	
Power meter E44198 GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY41495277 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY41498067 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference 30 dB Attenuator SN: S5129 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. E53-3013_Dec09) Dec-10 DAE4 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Secondary Standards ID ≠ Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Name Function Signature Calibrated by: Katja Pokovic Technical Manager	All calibrations have been condi	ucted in the closed laborat		
Power meter E44198 GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Apr-10 (No. 217-01136) Apr-11 Apr-11 Apr-10 (No. 217-01136) Apr-11 Apr-11 Apr-10 (No. 217-01136) Apr-10 (No. 217-01136) Apr-10 (No. 217-01136) Apr-11 Apr-10 (No. 217-01136) Apr-10	Primary Standards	line	Cal Date (Certificate No.)	School yed Calibration
Power sensor E4412A MY41495277 1-Apr-10 (No. 217-01136) Apr-11 Apr-10 (No. 217-01136) Mar-11 Apr-10 (No. 217-01136) Mar-11 Apr-10 (No. 217-01136) Mar-11 Apr-10 (No. 217-01136) Mar-11 Apr-11 Apr-10 (No. 217-01136) Mar-11 Apr-11 Apr-10 (No. 217-01136) Mar-11 Apr-11 Apr-11 Apr-10 (No. 217-01136) Mar-11 Apr-11 Apr-11 Apr-10 (No. 217-01136) Mar-11 Apr-11 Apr-11 Apr-11 Apr-11 Apr-11 Apr-11 Apr-11 Apr-11 (No. 217-01136) Mar-11 Apr-11	ALERGA TO A CONTROL OF THE STATE OF THE STAT	17.00		
Power sensor E4412A MY41498087 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference 30 dB Attenuator SN: S5129 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 DAE4 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Reference Probe ES30V2 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Reference Probe ES30V2 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Reference Probe ES30V2 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Reference Probe ES30V2 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Reference Probe ES30V2 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Reference Probe ES30V2 SN: 660 20-Apr-10 (No. 217-01160) Apr-11 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 Reference Probe ES30V2 SN: 3013 30-De				
Seference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11	ower sensor E4412A	MY41498087		10/20/06/06
Seference 20 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11	Reference 3 dB Attenuator	SN: S5054 (3c)		DW 1980 I
Seference Probe ES3DV2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10	eference 20 dB Attenuator	SN: S5086 (20b)		Mar-11
SN: 860 20-Apr-10 (No. DAE4-860_Apr-10) Apr-11	Reference 30 dB Attenuator	SN: S5129 (30b)	30-Mar-10 (No. 217-01160)	Mar-11
Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Name Function Signature Calibrated by: Katja Pokovic Technical Manager	Reference Probe ES3DV2	SN: 3013	30-Dec-09 (No. ES3-3013_Dec05) Dec-10
RF generator HP 8649C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Name Function Signature Calibrated by: Retyonal Pokovic Function Function Signature	DAE4	SN: 660	20-Apr-10 (No. DAE4-660_Apr10	Apr-11
RF generator HP 8648C US3642U01700 4-Aug-98 (in house check Oct-09) In house check: Oct-11 US37390585 18-Oct-01 (in house check Oct-10) In house check: Oct-11 I	Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Name Function Signature Calibrated by: Technical Manager		US3642U01700	The state of the s	In house check: Oct-11
Calibrated by: Katja Pokovic Technical Manager	Network Analyzer HP 8753E	US37390585	그 사이지 살아왔다면 하다 하다. 얼마나 이 그리지 않아 살아왔다면서	
Calibrated by: Katja Pokovic Technical Manager		Name	Function	Signature.
Approved by: Niels Kuster Quality Manager	Calibrated by:	Katja Pokovic	Technical Manager	1910
Approved by: Niets Kuster Quality Manager				1 The said
/ \ / \	Approved by:	Niels Kuster	Quality Manager	1/16:5
Issued: November 25.				

Certificate No: EX3-3677_Nov10

Page 1 of 11

Report No. RZA1103-0427SAR

Page 42 of 67

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdiens

C Service suisse d'étalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z

tissue simulating liquid sensitivity in free space sensitivity in TSL / NORMx,y,z diode compression point

ConvF DCP CF

crest factor (1/duty_cycle) of the RF signal modulation dependent linearization parameters

A, B, C Polarization φ

Polarization φ Polarization 9 $\boldsymbol{\phi}$ rotation around probe axis

3 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- EC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
 power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
 maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

November 24, 2010

Probe EX3DV4

SN:3677

Manufactured:

Last calibrated:

Recalibrated:

September 9, 2008

September 23, 2009

November 24, 2010

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

November 24, 2010

DASY/EASY - Parameters of Probe: EX3DV4 SN:3677

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	0.41	0.47	0.39	± 10.1%
DCP (mV) ⁸	96.8	98.9	98.8	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dBuV	С	VR mV	Unc ^E (k=2)
10000	cw	0.00	х	0.00	0.00	1.00	143.2	± 2.4 %
			Υ	0.00	0.00	1.00	140.9	
			Z	0.00	0.00	1.00	135.8	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

⁶ The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^b Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

November 24, 2010

DASY/EASY - Parameters of Probe: EX3DV4 SN:3677

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] ^C	Permittivity	Conductivity	ConvF X C	ConvF Y	ConvF Z	Alpha	Depth Unc (k=2)
450	±50/±100	43.5 ± 5%	$0.87 \pm 5\%$	10.04	10.04	10.04	0.09	1.00 ± 13.3%
835	±50/±100	41.5 ± 5%	$0.90 \pm 5\%$	9.50	9.50	9.50	0.72	0.64 ± 11.0%
1750	±50/±100	40.1 ± 5%	$1.37\pm5\%$	8.22	8.22	8.22	0.72	0.59 ± 11.0%
1900	±50/±100	$40.0 \pm 5\%$	$1.40\pm5\%$	7.94	7.94	7.94	0.81	0,57 ± 11.0%
2450	±50/±100	39.2 ± 5%	1.80 ± 5%	7.32	7.32	7.32	0.47	0.75 ± 11.0%

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

November 24, 2010

DASY/EASY - Parameters of Probe: EX3DV4 SN:3677

Calibration Parameter Determined in Body Tissue Simulating Media


Validity [MHz] ^c	Permittivity	Conductivity	ConvF X	ConvF Y	ConvF Z	Alpha	Depth Unc (k=2)
±50/±100	56.7 ± 5%	0.94 ± 5%	10.62	10.62	10.62	0.02	1.00 ± 13.3%
±50/±100	$55.5\pm5\%$	0.96 ± 5%	10.14	10.14	10.14	0.59	0.72 ± 11.0%
±50/±100	55.2 ± 5%	$0.97 \pm 5\%$	10.33	10.33	10.33	0.20	2.06 ± 11.0%
±50/±100	$54.0 \pm 5\%$	1.30 ± 5%	8.47	8.47	8.47	0.99	0.53 ± 11.0%
±50/±100	53.4 ± 5%	1.49 ± 5%	8.02	8.02	8.02	0.63	0.67 ± 11.0%
±50/±100	$53.3 \pm 5\%$	1.52 ± 5%	7.77	7.77	7.77	0.69	0.67 ± 11.0%
±50/±100	$53.2\pm5\%$	1.62 ± 5%	8.04	8.04	8.04	0.16	1.44 ± 11.0%
±50/±100	52.7 ± 5%	1.95 ± 5%	7.46	7.46	7.46	0.99	0.49 ± 11.0%
±50/±100	51.3 ± 5%	3.31 ± 5%	6.61	6.61	6.61	0.28	1.40 ± 13.1%
	±50/±100 ±50/±100 ±50/±100 ±50/±100 ±50/±100 ±50/±100 ±50/±100 ±50/±100	± 50 /± 100 56.7 ± 5% ± 50 /± 100 55.5 ± 5% ± 50 /± 100 55.2 ± 5% ± 50 /± 100 54.0 ± 5% ± 50 /± 100 53.4 ± 5% ± 50 /± 100 53.3 ± 5% ± 50 /± 100 53.2 ± 5% ± 50 /± 100 52.7 ± 5%	±50/±100 56.7±5% 0.94±5% ±50/±100 55.5±5% 0.96±5% ±50/±100 55.2±5% 0.97±5% ±50/±100 54.0±5% 1.30±5% ±50/±100 53.4±5% 1.49±5% ±50/±100 53.3±5% 1.52±5% ±50/±100 53.2±5% 1.62±5% ±50/±100 52.7±5% 1.95±5%	\$\pmodel{\pmodel} \pmodel{\pmodel} \pmod	±50/±100 56.7±5% 0.94±5% 10.62 10.62 ±50/±100 55.5±5% 0.96±5% 10.14 10.14 ±50/±100 55.2±5% 0.97±5% 10.33 10.33 ±50/±100 54.0±5% 1.30±5% 8.47 8.47 ±50/±100 53.4±5% 1.49±5% 8.02 8.02 ±50/±100 53.3±5% 1.52±5% 7.77 7.77 ±50/±100 53.2±5% 1.62±5% 8.04 8.04 ±50/±100 52.7±5% 1.95±5% 7.46 7.46	\$\pmodel{\pmodel} \pmodel{\pmodel} \pmod	$ \begin{array}{cccccccccccccccccccccccccccccccccccc$

The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

November 24, 2010

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

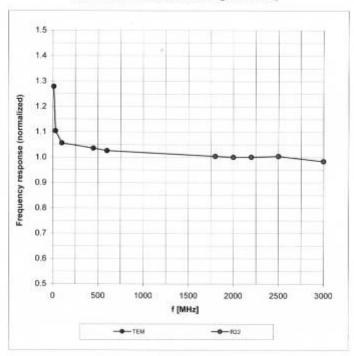



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

November 24, 2010


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$





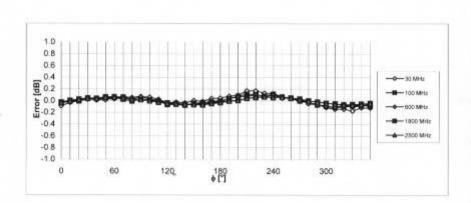


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

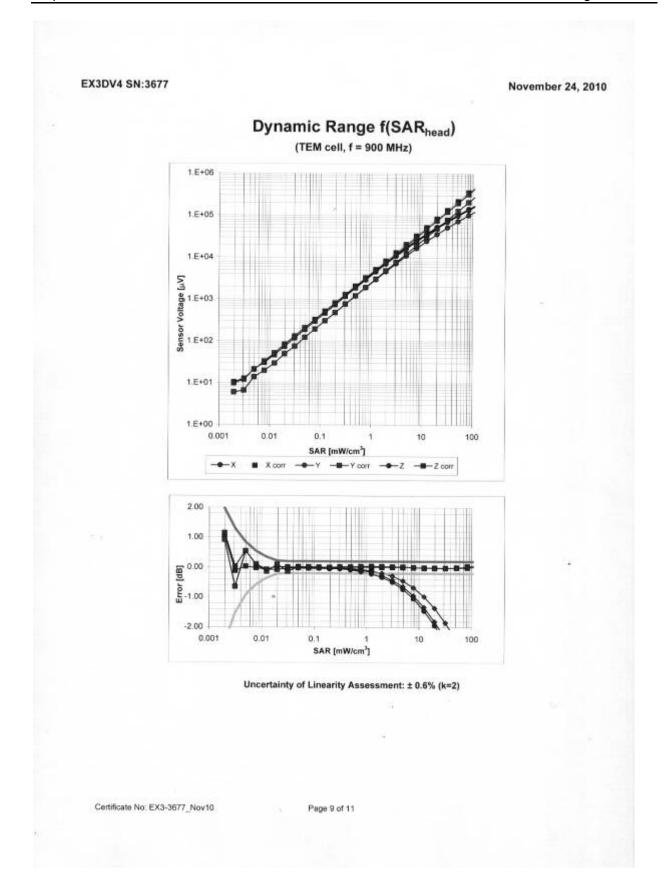




November 24, 2010


Conversion Factor Assessment





Deviation from Isotropy in HSL

Error (φ, θ), f = 900 MHz

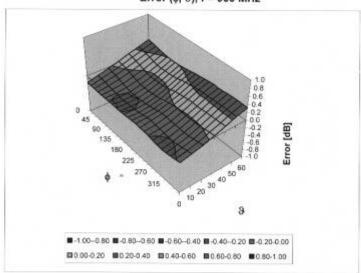

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Report No. RZA1103-0427SAR

Page 51 of 67

EX3DV4 SN:3677

November 24, 2010

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

ANNEX E: D450V3 Dipole Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

CALIBRATION	CERTIFICATE		
Object	D450V3 - SN: 10	065	
Calibration procedure(s)	QA CAL-15.v5 Calibration Proce	edure for dipole validation kits below	w 800 MHz
Calibration date:	November 09, 20	010	
This calibration certificate doo The measurements and the u	ncertainties with confidence p	probability are given on the following pages and	are part of the certificate.
The measurements and the u All calibrations have been cor Calibration Equipment used (nducted in the closed laborato	ry facility: environment temperature $(22\pm3)^{\circ}$ C a	and humidity < 70%.
The measurements and the u NI calibrations have been cor Calibration Equipment used (I Primary Standards	nducted in the closed laborato M&TE critical for calibration) ID #	ry facility: environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.)	and humidity < 70%. Scheduled Calibration
The measurements and the uniform that th	M&TE critical for calibration) ID # GB41293874	ry facility: environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030)	Scheduled Calibration Apr-11
The measurements and the unit calibrations have been concalibration Equipment used (I Primary Standards Power meter E4419B Power sensor E4412A	M&TE critical for calibration) ID # GB41293874 MY41495277	ry facility: environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030)	Scheduled Calibration Apr-11 Apr-11
The measurements and the unit calibrations have been concalibration Equipment used (I Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	M&TE critical for calibration) ID # GB41293874 MY41496277 MY41498087	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030)	Scheduled Calibration Apr-11 Apr-11 Apr-11
The measurements and the under the control of the c	M&TE critical for calibration) ID # GB41293874 MY41496277 MY41498087 SN: S5054 (3c)	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11
The measurements and the unal calibration Equipment used (I Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11
The measurements and the under the conformation Equipment used (I Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Type-N mismatch combination	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) n SN: 5047.2 / 06327	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01029)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11 Mar-11
The measurements and the u	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) n SN: 5047.2 / 06327	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11
The measurements and the unit calibrations have been concerned to the conc	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) n SN: 5047.2 / 06327 SN: 654	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01029) 03-Jul-10 (No. ET3-1507_Jul10)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11 Mar-11 Jul-11
The measurements and the unit of the measurements and the unit of the measurements and the unit of the measurement used (I) Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 (LFDAE4 Secondary Standards RF generator HP 8648C	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) n SN: 5047.2 / 06327 SN: 1507 SN: 654 ID # US3642U01700	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01029) 03-Jul-10 (No. ET3-1507_Jul10) 04-May-10 (No. DAE4-654_May10) Check Date (in house) 04-Aug-99 (in house check Oct-10)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11 Mar-11 Jul-11 May-11
The measurements and the unit calibrations have been concalibration Equipment used (I) Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 (LF	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) n SN: 5047.2 / 06327 SN: 654	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01029) 03-Jul-10 (No. ET3-1507_Jul10) 04-May-10 (No. DAE4-654_May10) Check Date (in house)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11 Mar-11 Jul-11 May-11 Scheduled Check
The measurements and the unit calibrations have been concerned by the calibration of the concerned by the calibration of the ca	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5096 (20b) SN: 5047.2 / 06327 SN: 654 ID # US3642U01700 US37390585 S4206 Name	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01029) 03-Jul-10 (No. ET3-1507_Jul10) 04-May-10 (No. DAE4-654_May10) Check Date (in house) 04-Aug-99 (in house check Oct-10) 18-Oct-01 (in house check Oct-10)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11 Mar-11 Jul-11 May-11 Scheduled Check In house check: Oct-11
The measurements and the unit of the measurements and the unit of the measurements and the unit of the measurement used (I) Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ET3DV6 (LFDAE4 Secondary Standards RF generator HP 8648C	M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) n SN: 5047.2 / 06327 SN: 1507 SN: 654 ID # US3642U01700 US37390585 S4206	Cal Date (Calibrated by, Certificate No.) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 1-Apr-10 (No. 217-01030) 31-Mar-10 (No. 217-01026) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01028) 31-Mar-10 (No. 217-01029) 03-Jul-10 (No. ET3-1507_Jul10) 04-May-10 (No. DAE4-654_May10) Check Date (in house) 04-Aug-99 (in house check Oct-10) 18-Oct-01 (in house check Oct-10)	Scheduled Calibration Apr-11 Apr-11 Apr-11 Mar-11 Mar-11 Mar-11 Jul-11 May-11 Scheduled Check In house check: Oct-11 In house check: Oct-11

Certificate No: D450V3-1065_Nov10

Page 1 of 9

Report No. RZA1103-0427SAR

Page 53 of 67

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kallbrierdienst Service suisse d'étalonnage

C Service suisse d etaionnage
Service suisse d etaionnage
Service suisse d etaionnage
Service suisse d etaionnage

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms eriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D450V3-1065_Nov10

Report No. RZA1103-0427SAR

Page 54 of 67

Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY5	V5.2
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Area Scan Resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters The following parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	-0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	44.2 ± 6 %	0.86 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	398 mW input power	1.87 mW / g
SAR normalized	normalized to 1W	4.70 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	4.76 mW / g ± 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	398 mW input power	1.25 mW / g
SAR normalized	normalized to 1W	3.14 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	3.17 mW / g ± 17.6 % (k=2)

Report No. RZA1103-0427SAR

Page 55 of 67

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.1 ± 6 %	0.90 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	398 mW input power	1.77 mW / g
SAR normalized	normalized to 1W	4.37 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	4.51 mW / g ± 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	398 mW input power	1.18 mW / g
SAR normalized	normalized to 1W	2.94 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	3.03 mW / g ± 17.6 % (k=2)

Certificate No: D450V3-1065_Nov10

Report No. RZA1103-0427SAR

Page 56 of 67

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	59.2 Ω - 4.9 jΩ	
Return Loss	- 20.5 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	56.5 Ω - 7.9 jΩ
Return Loss	- 20.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.354 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 16, 2010

Certificate No: D450V3-1065_Nov10

DASY5 Validation Report for Head TSL

Date/Time: 09.11.2010 10:36:58

Test Laboratory: The name of your organization

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1065

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium: HSL450

Medium parameters used: f = 450 MHz; $\sigma = 0.86 \text{ mho/m}$; $\varepsilon_r = 44.2$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ET3DV6 SN1507 (LF); ConvF(6.66, 6.66, 6.66); Calibrated: 03.07.2010
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 04.05.2010
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1003
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Pin=398mW /d=15mm /Area Scan (41x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.99 mW/g


Pin=398mW /d=15mm /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 50.3 V/m; Power Drift = -0.00664 dB

Peak SAR (extrapolated) = 2.81 W/kg


SAR(1 g) = 1.87 mW/g; SAR(10 g) = 1.25 mW/g

Maximum value of SAR (measured) = 2.01 mW/g

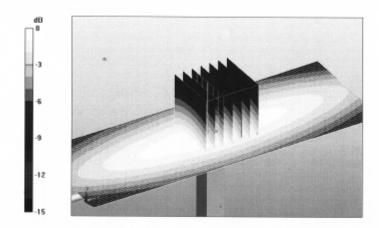

0 dB = 2.01 mW/g



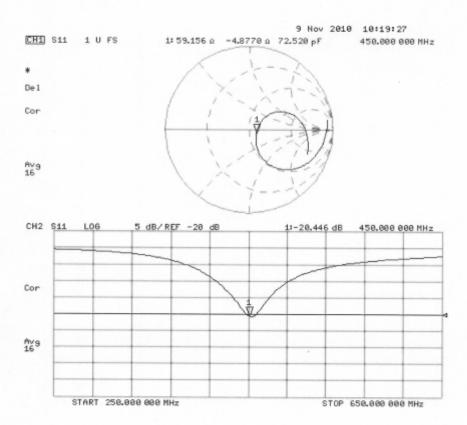

DASY5 Validation Report for Body TSL

Date/Time: 09.11.2010 13:52:55

Test Laboratory: The name of your organization

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1065

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium: MSL450

Medium parameters used: f = 450 MHz; $\sigma = 0.9 \text{ mho/m}$; $\varepsilon_f = 54.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ET3DV6 SN1507 (LF); ConvF(7.11, 7.11, 7.11); Calibrated: 03.07.2010
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 04.05.2010
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1003
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Pin=398mW /d=15mm /Area Scan (61x201x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 1.89 mW/g


Pin=398mW /d=15mm, /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 47.4 V/m; Power Drift = -0.016 dB

Peak SAR (extrapolated) = 2.7 W/kg


SAR(1 g) = 1.77 mW/g; SAR(10 g) = 1.18 mW/g

Maximum value of SAR (measured) = 1.89 mW/g

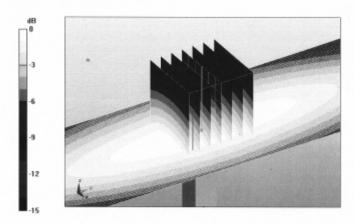

0 dB = 1.89 mW/g

Impedance Measurement Plot for Body TSL

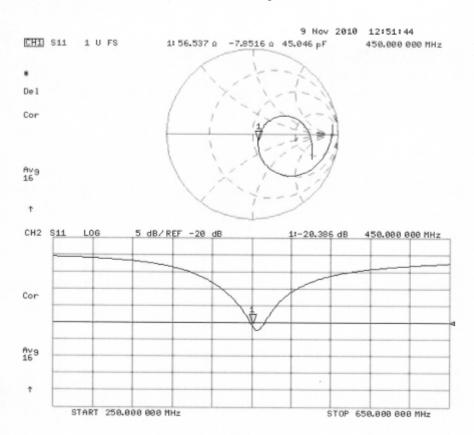

ANNEX F: DAE4 Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

lent TA - SH (Aude	n)	Cert	Ifficate No: DAE4-871_Nov10
CALIBRATION C	ERTIFICATE		
Object	DAE4 - SD 000 D	04 BJ - SN: 871	
Calibration procedure(s)	QA CAL-06.v22 Calibration process	dure for the data acquisiti	on electronics (DAE)
Calibration date:	November 18, 20	10	
			nysical units of measurements (SI). pages and are part of the certificate.
All calibrations have been conduc	ated in the closed laboratory	facility: environment temperature	(22 ± 3)*C and humidity < 70%.
Calibration Equipment used (M&T	E critical for calibration)		
Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	28-Sep-10 (No:10376)	Sep-11
Secondary Standards Calibrator Box V1.1	ID # SE UMS 006 AB 1004	Oneck Date (in house) 07-Jun-10 (in house check)	Scheduled Check In house check: Jun-11
Secretary Section 7-11.1	32 313 33 13	and the standard of standard	
	Name	Function	Signature
Calibrated by:	Andrea Gunti	Technician	Sud
Approved by:	Fin Bomholt	R&D Director	W. Blum
			Issued: November 18, 2010
This calibration certificate shall no	t be reproduced except in f	ull without written approval of the	aboratory.

Certificate No: DAE4-871_Nov10

Page 1 of 5

Report No. RZA1103-0427SAR

Page 62 of 67

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Report No. RZA1103-0427SAR

Page 63 of 67

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: $1LSB = 6.1\mu V$, full ra Low Range: 1LSB = 61n V, full ra

full range = -100...+300 mV full range = -1......+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.757 ± 0.1% (k=2)	404.740 ± 0.1% (k=2)	405.181 ± 0.1% (k=2)
Low Range	3.98219 ± 0.7% (k=2)	3.93489 ± 0.7% (k=2)	3.96831 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	90.0 ° ± 1 °
Connector Angle to be used in DAS1 system	90.0 II

Certificate No: DAE4-871_Nov10

Page 3 of 5

Appendix

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	200001.2	-1.56	-0.00
Channel X + Input	20000.71	0.71	0.00
Channel X - Input	-19997.87	1.63	-0.01
Channel Y + Input	199994.3	1.99	0.00
Channel Y + Input	19998.92	-1.08	-0.01
Channel Y - Input	-20000.26	-0.76	0.00
Channel Z + Input	200009.2	-1,04	-0.00
Channel Z + Input	19998.70	-1.10	-0.01
Channel Z - Input	-20000.16	-0.76	0.00

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2000.1	0.16	0.01
Channel X + Input	199.58	-0.52	-0.26
Channel X - Input	-200.79	-0.89	0.45
Channel Y + Input	1999.9	-0.03	-0.00
Channel Y + Input	199.45	-0.55	-0.27
Channel Y - Input	-200.31	-0.41	0.21
Channel Z + Input	2000.1	0.33	0.02
Channel Z + Input	199.13	-0.77	-0.38
Channel Z - Input	-201.47	-1.37	0.69

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	14.25	12.86
	- 200	-12.68	-14.21
Channel Y	200	-10.04	-10.39
	- 200	9.20	9.17
Channel Z	200	-0.85	-1.40
	- 200	-0.34	-0.31

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (µV)	Channel Z (μV)
Channel X	200	-	2.85	0.69
Channel Y	200	2.41		2.73
Channel Z	200	2.54	0.73	2

Certificate No: DAE4-871_Nov10

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec: Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15920	15517
Channel Y	. 16171	16732
Channel Z	15803	16474

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MO

iiput rowaz	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.03	-2.35	0.86	0.43
Channel Y	-0.50	-1.49	-0.49	0.38
Channel Z	-0.92	-2.21	0.14	0.44

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	


9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9


ANNEX G: The EUT Appearances and Test Configuration




Picture 3: Constituents of the sample

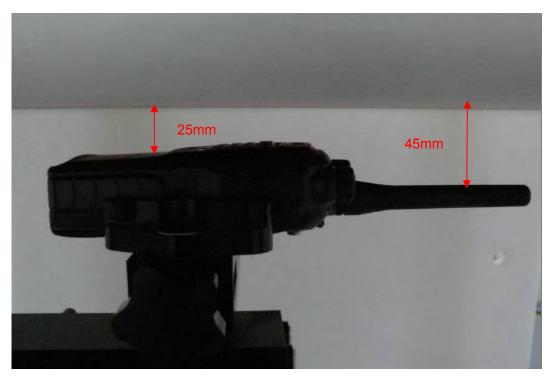

Picture 4: Face-held, The EUT display towards phantom, the distance from EUT Antenna to the bottom of the Phantom is 45mm

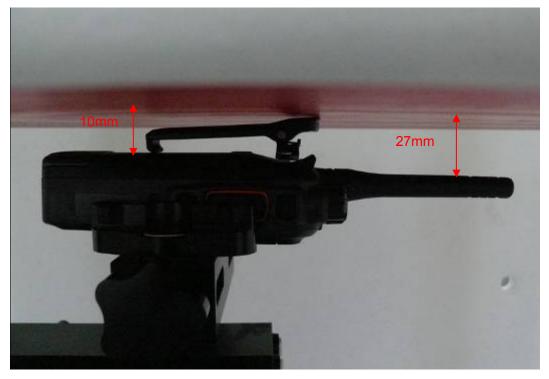

Picture 5: Body-worn, The EUT display towards ground, Belt clip attach the Phantom, the distance from EUT Antenna to the bottom of the Phantom is 27mm

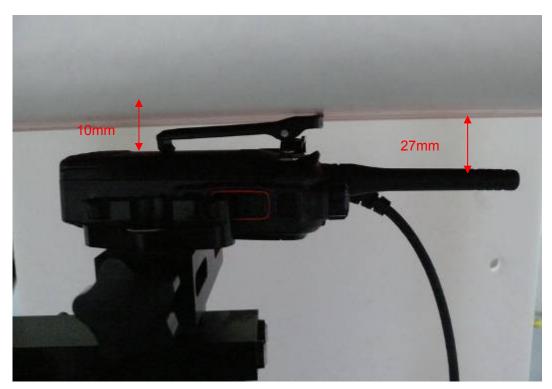

Picture 6: Body-worn, The EUT display towards ground with Speaker-Microphone, Belt clip attach the Phantom, the distance from EUT Antenna to the bottom of the Phantom is 27mm