Report No.: SZEM190101023709

Appendix I


Photographs

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details




Report No.: SZEM190101023709

1. SAR measurement System

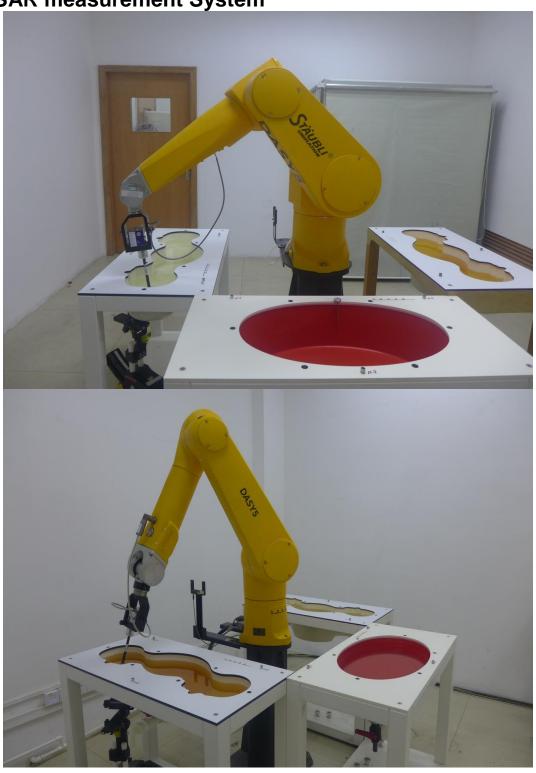

Report No.: SZEM190101023709

2. Photographs of Tissue Simulate Liquid

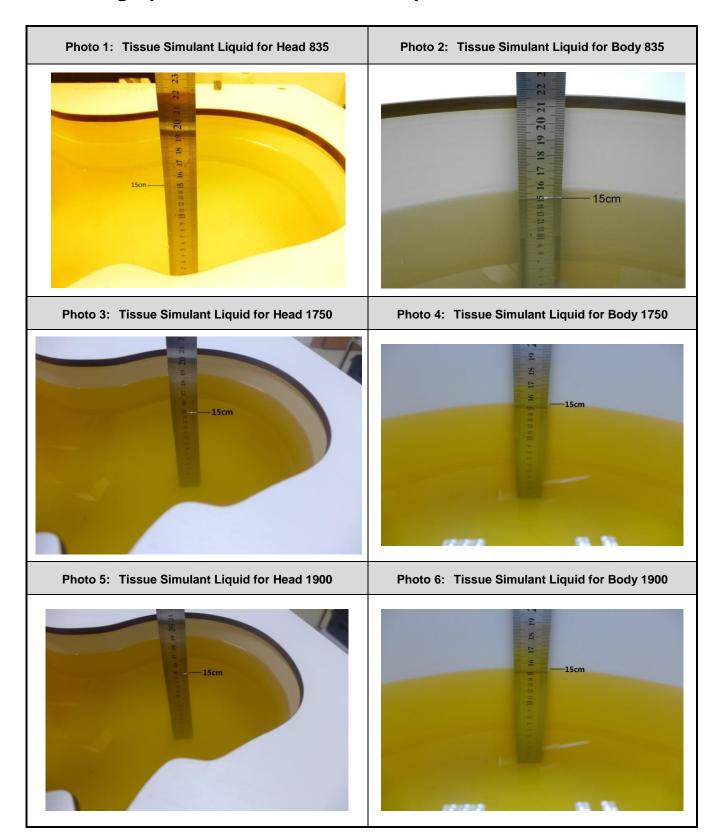



Report No.: SZEM190101023709

Photo 7: Tissue Simulant Liquid for Head 2300 Photo 8: Tissue Simulant Liquid for Body 2300 Photo 9: Tissue Simulant Liquid for Head 2450 Photo 10: Tissue Simulant Liquid for Body 2450 Photo 11: Tissue Simulant Liquid for Head 2600 Photo 12: Tissue Simulant Liquid for Body 2600



Report No.: SZEM190101023709

Photo 14: Left tilted 15 degree

3. Photographs of EUT test position

Photo 13: Left touch cheek

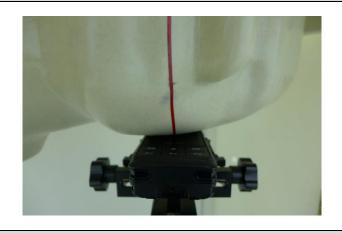


Photo 15: Right touch cheek

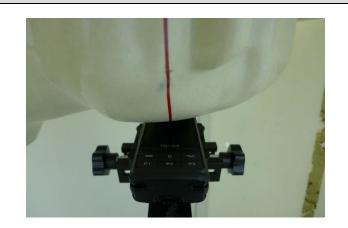


Photo 16: Right tilted 15 degree

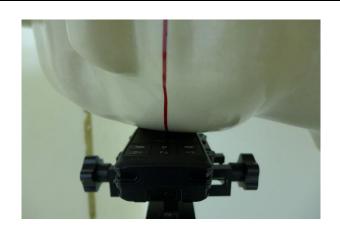


Photo 17: Front side 15mm

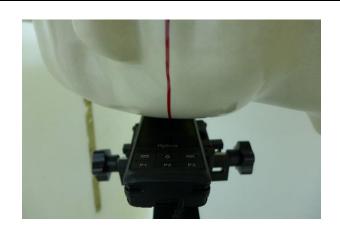


Photo 18: Back side 15mm







Report No.: SZEM190101023709

Photo 19: Front side 10mm



Photo 20: Back side 10mm



Photo 21: Left side 10mm



Photo 22: Right side 10mm



Photo 23: Top side 10mm



Photo 24: Bottom side 10mm





Report No.: SZEM190101023709

Photo 25: Back splint 0mm	NA
	NA



Report No.: SZEM190101023709

4. EUT Constructional Details

