




# **Appendix I**







## **Photographs**


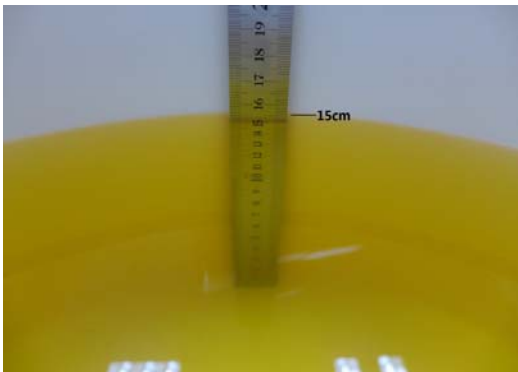

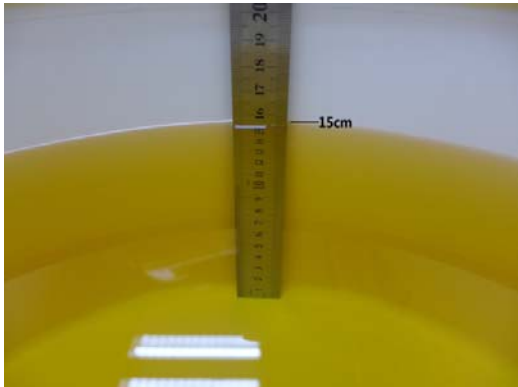

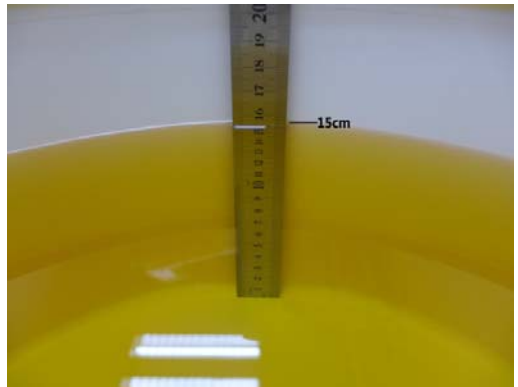
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System

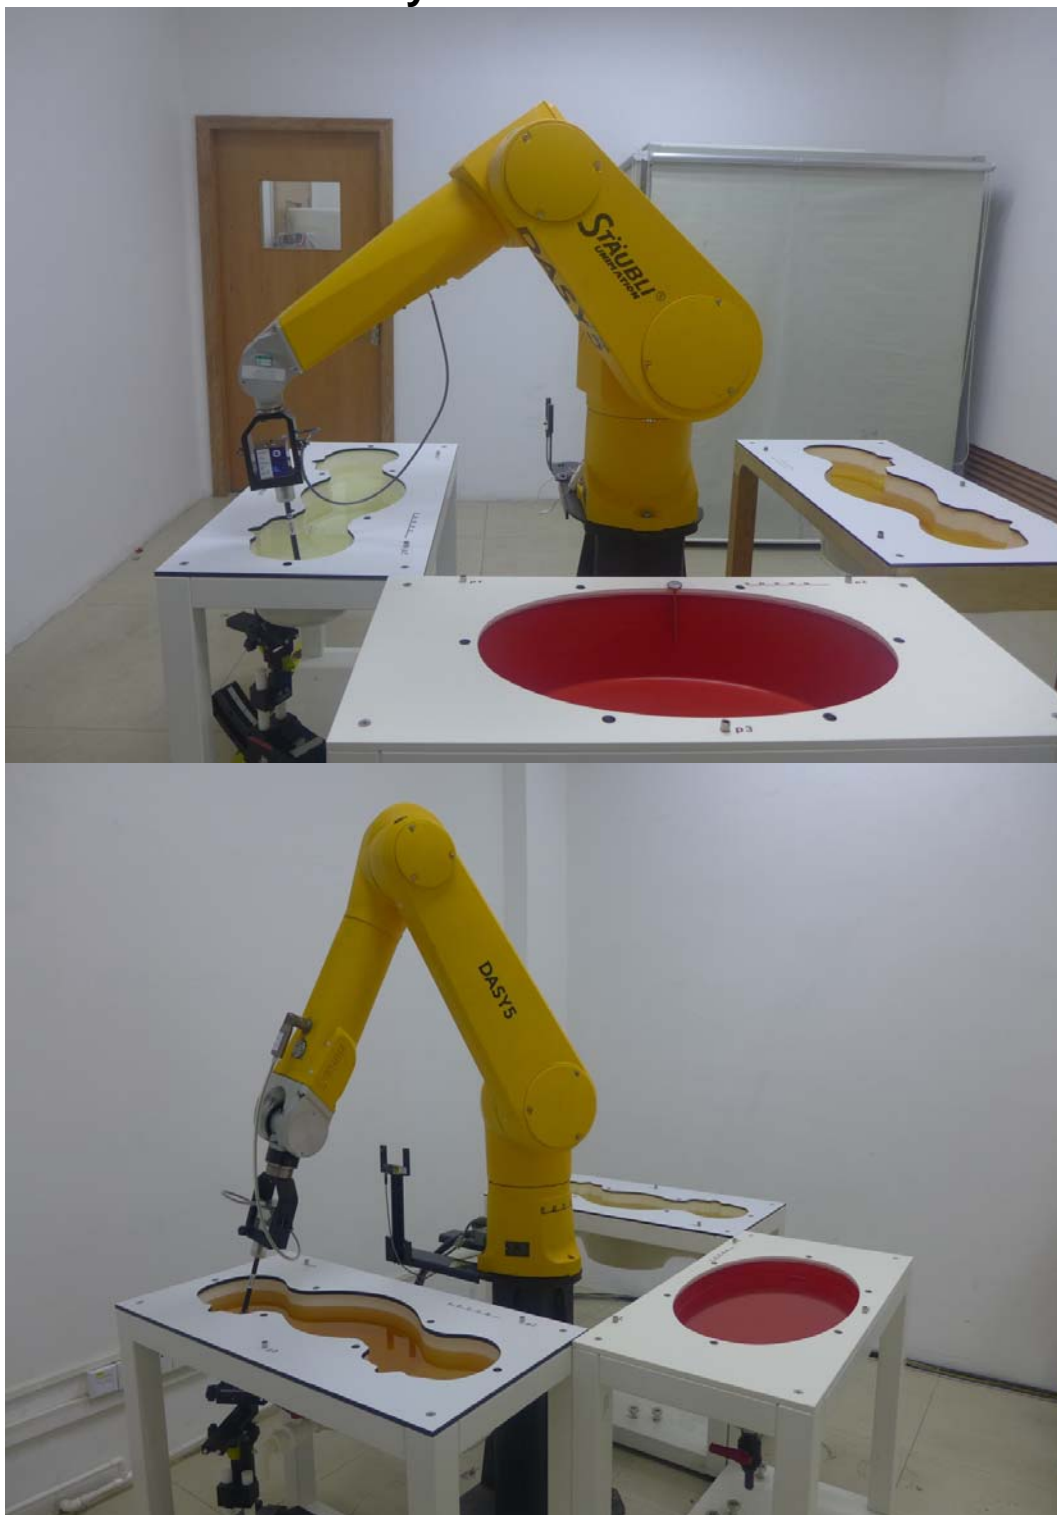



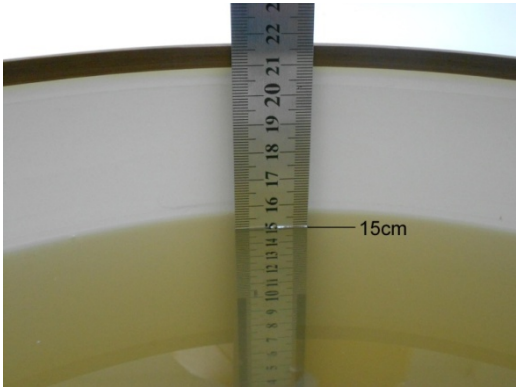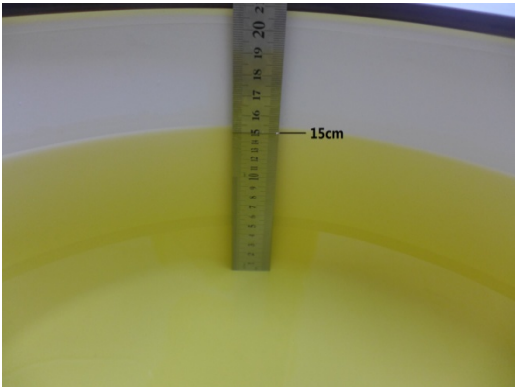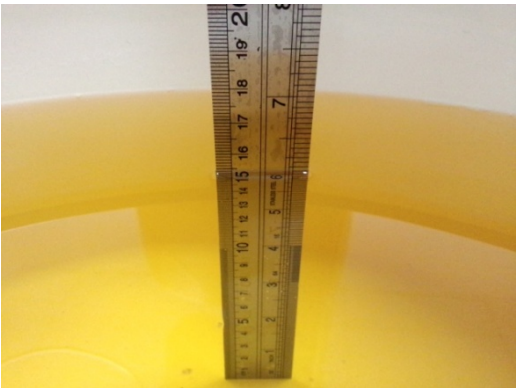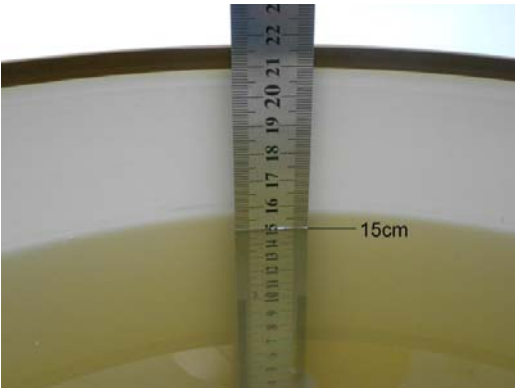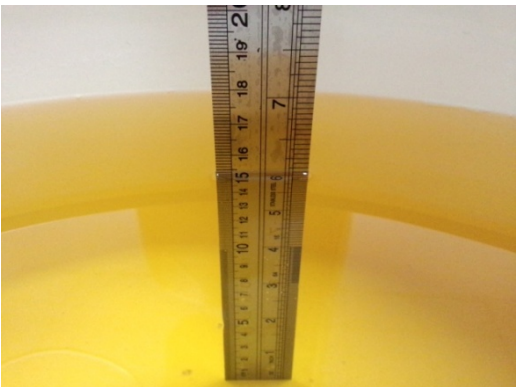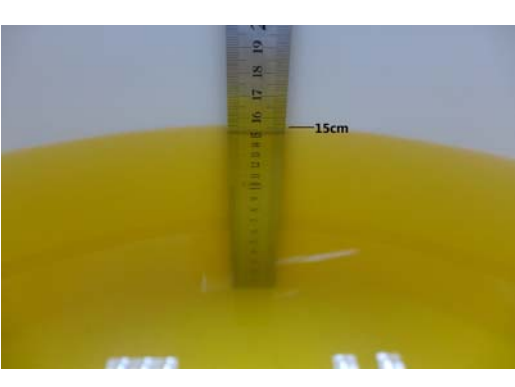

## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Body 750</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Body 835</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 1750</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Body 1750</b></p>
	




<p><b>Photo 7: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 8: Tissue Simulant Liquid for Body 1900</b></p>
	
<p><b>Photo 9: Tissue Simulant Liquid for Head 2450</b></p>	<p><b>Photo 10: Tissue Simulant Liquid for Body 2450</b></p>
	
<p><b>Photo 11: Tissue Simulant Liquid for Head 2600</b></p>	<p><b>Photo 12: Tissue Simulant Liquid for Body 2600</b></p>
	

### 3. Photographs of EUT test position

Photo 13: Front side 10mm	Photo 14: Front side 15mm
	
Photo 15: Back side 15mm	Photo 16: Back splint 0mm
	



## 4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
	
Photo 19: Back View	NA
	<p>NA</p>