# FCC SAR TEST REPORT

No. 130601

for

Shenzhen Contel Electronics Technology Co., Ltd

10 Inch Tablet

Model Name: TAB-1040, TAB-1040G, TPC-1040M, TAB-1040\_G,

**TAB-1040E** 

**FCC ID: YAPTAB1040** 

Issued Date: 2013-06-18

#### Note:

The test results in this test report relate only to the devices specified in this report. This report shall not be reproduced except in full without the written approval of GCCT. **Test Laboratory:** 

GCCT, Guangdong Telecommunications Terminal Products Quality Supervision and Testing Center Technology Road, High-tech Zone, He Yuan City, Guang Dong Province, PR China 517001 Tel:+86(0)762-3607139, Fax:+86(0)762-3603336 Email: ncctmail@126.com. www.ncct.org.cn

# **GCCT**

# **TABLE OF CONTENTS**

1.	Gen	eral Information	4
	1.1	Testing Laboratory	4
	1.2	Application Information	
	1.3	Manufacturer Information	
	1.4	EUT Information	5
2.	<b>EUT</b>	Operational Conditions During Test	6
	2.1	General Description of Test Procedures	6
3.	SAR	Measurements System Configuration	7
	3.1	Measurement System Diagram	
	3.2	System Components	8
	3.3	Equivalent Tissues	11
4.	Eval	uation Procedures	12
	4.1	Data Evaluation	12
		SAR Evaluation Procedures	
	4.3	Spatial Peak SAR Evaluation	14
5.	Test	Laboratory Environment	16
6.		ducted Output Power Measurement	
7.		Measurement Results	_
		Liquid Measurement Results	
	7.2	System Performance Check	18
	7.3	Measurement Results	20
8.		surement Uncertainty	
9.		Photos and Test Positions	
		pment List & Calibration Status	
		chments	
		E 1 System Performance Check Plots	
		E 2 SAR Test Plots	
ΑN	NEX	E 3 Probe calibration report	36
		E 4 Dipole calibration report	
ΑN	NEX	E 5 DAE calibration report	57



# **GENERAL SUMMARY**

Product Name	10 Inch Tablet
Model Name	TAB-1040, TAB-1040G, TPC-1040M, TAB-1040_G, TAB-1040E
Applicant	Shenzhen Contel Electronics Technology Co., Ltd
Manufacturer	Dongguan Contel Cloud Terminal System Co., Ltd
Test laboratory	GCCT, Guangdong Telecommunications Terminal Products Quality Supervision and Testing Center
Reference Standards	OET Bulletin 65 (Edition 97-01) and Supplement C (Edition 01-01): Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits IEEE Std C95.1, 1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz IEEE 1528-2003: Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques FCC KDB 447498 D01 v05r01: Mobile and Portable Devices RF Exposure Procedures and Equipment Authorization Policies FCC KDB 865664 D01 v01r01: SAR Measurement Requirements for 100 MHz to 6 GHz FCC KDB 616217 D04 v01r01: SAR Evaluation Considerations for Laptop, Notebook, Netbook and Tablet Computers FCC KDB 248227 D01 v01r02: SAR measurement Procedures for 802.11a/b/g Transmitters IEC 62209-1: 2006: Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures, Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz) IEC 62209-2: 2010: Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices - Human models, instrumentation, and procedures, Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)
Test Conclusion	This portable wireless equipment has been measured in all cases requested by the relevant standards. Test results in Chapter 7 of this test report are below limits specified in the relevant standards.  General Judgment: Pass  Date of issue:2013.06.18
Comment:	The test results in this report apply only to the tested sample of the stated device/equipment.

Approved by:	Reviewed by:	Tested by:
luo jian	Dong Xraubo	A Unglang
Deputy Manager	Deputy Manager	Test Engineer



# 1. General Information

# 1.1 Testing Laboratory

Company	GCCT, Guangdong Telecommunications Terminal Products  Quality Supervision and Testing Center
Address	Technology Road, High-tech Zone, He Yuan City, Guang Dong Province, PR China
Country	P. R. China
Contact	Dong Xiaobo
Telephone	+86-762-3607139
Fax	+86-762-3603336
E-mail	dongxiaobo126@126.com
Website	http://www.ncct.org.cn

# 1.2 Application Information

Company	Shenzhen Contel Electronics Technology Co., Ltd
Address	3/F, R2-A, High-tech Industrial Park, Nanshan District, Shenzhen, China
Contact	
Email	1
Telephone	1
Fax	1

# 1.3 Manufacturer Information

Company	Dongguan Contel Cloud Terminal System Co., Ltd
Address	Waijing Industrial Park, Gaolong road, Gaobu Town, Dongguan, GuangDong
Contact	
Email	1
Telephone	1
Fax	1



# 1.4 EUT Information

Product Name	10 Inch Tablet				
Exposure Category	Uncontrolled Environment / General Population				
Model Number	TAB-1040, TAB-1040G, TPC-1040M, TAB-1040_G, TAB-1040E				
Device Type	Portable Device				
Hardware version	TVE102S_V1.2				
Software version	Update_jellybean_tve102s_v2_101inch_rk903_volume_flash _gt9xx_tab1040_r2493				
Supporting modes	WIFI 802.11b (tested) WIFI 802.11g WIFI 802.11n Bluetooth				
	Mode	1g SAR(W/Kg)			
Max. SAR (1g):	WIFI 802.11b 1.33				
Antenna Type	na Type Internal Antenna				
Accessories	Charger:  Molel:BSC15-050210-UD, Input: 100-240v, 1.0A  Output: 5v, 2.5A				
Comment	The diagonal dimension of The above EUT's information	the table is 25.4 cm. on was declared by manufacture.			



### 2. EUT Operational Conditions During Test

## 2.1 General Description of Test Procedures

A communication link is set up with a System Simulator (SS) by air link. The Absolute Radio Frequency Channel Number (ARFCN) is allocated to 1, 6 and 11 in the case of WIFI. When we test, the EUT battery must be fully charged and checked periodically during the test to ascertain uniform power output.

For the 802.11b/g SAR tests, a communication link is set up with the test mode software for WIFI mode test. The Absolute Radio Frequency Channel Number (ARFCN) is allocated to 1, 6 and 11 respectively in the case of 2450 MHz. During the test, at the each test frequency channel, the EUT is operated at the RF continuous emission mode. Each channel should be tested at the lowest data rate.

802.11b/g operating modes are tested independently according to the service requirements in each frequency band. 802.11b/g modes are tested on channels1,6,11; however, if output power reduction is necessary for channels 1 and /or 11 to meet restricted band requirements the highest output channels closest to each of these channels must be tested instead.


SAR is not required for 802.11g/n channels when the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels.



### 3. SAR Measurements System Configuration

These measurements were performed with the automated near-field scanning system DASY5 from SPEAG. The system is based on a high precision robot, which positions the probes with a positional repeatability of better than ± 0.02 mm. Special E-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit. The SAR measurements were conducted with the dosimetric probe manufactured by SPEAG, designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure described in with accuracy of better than ±10%. The spherical isotropy was evaluated and found to be better than ±0.3 dB. The phantom used was the SAM Twin Phantom and ELI4 Phantom as described in IEC 62209-1, FCC OET 065 supplement C, IEEE1528 and EN 62209-1.

#### 3.1 Measurement System Diagram

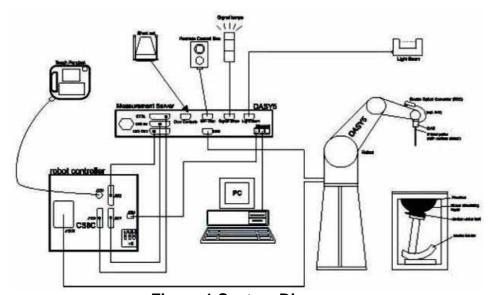

**Figure 1 System Diagram** 

#### The DASY5 system consists of the following items:

- 1. A standard high precision 6-axis robot (TX90XL) with St¨aubli CS8c robot controllers.
- 2. DASY5 Measurement Server.
- 3. Data Acquisition Electronics.
- 4. A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- 5. Light Beam Unit.

# **GCCT**

- 6. The SAM phantom enabling testing left-hand right-hand and the ELI4 phantom for body usage.
- 7. The Position device for handheld EUT.
- 8. Tissue simulating liquid mixed according to the given recipes.
- 9. System validation dipoles to validate the proper functioning of the system.
- 10. A computer operating Windows XP.

#### 3.2 System Components

The mobile phone under test operating at the maximum power level is placed in the phone holder, under the phantom, which is filled with head simulating liquid. The E-Field probe measures the electric field inside the phantom. The DASY5 software computes the results to give a SAR value in a 1g or 10 g mass.

#### 3.2.1 TX90XL

The TX90XL robot has six axes. The six axes are controlled by the St aubli CS8c robot controllers. It offers the features important for our application:

- High precision (repeatability 0.02mm)
- High reliability (industrial design)
- Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- Jerk-free straight movements (brushless synchrony motors; no stepper motors)
- Low ELF

#### 3.2.2 DASY5 Measurement Server

The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz Intel ULV Celeron, 128MB chip disk and 128MB RAM. The necessary circuits for communication with either the DAE4 electronics box as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.



Figure 2 TX90XL



Figure 3 Measurement Server



#### 3.2.3 **Probe**

For the measurements the specific dosimetric E-Field Probe ES3DV3 and EX3DV4 with following specifications is used.

Frequency: 10 MHz to 3 GHz; Linearity: ± 0.2 dB

Directivity: ± 0.3 dB in HSL (rotation around probe axis)

± 0.5 dB in tissue material (rotation normal to probe axis)

Dynamic Range: 10  $\mu$ W/g to > 100 mW/g; Linearity:  $\pm$  0.2 dB

Tip Diameter: 5 mm; Distance between probe tip and sensor center: 2.5 mm

Probe linearity: ±0.3 dB

Calibration range: 835 to 2500 MHz for head & body simulating liquid

#### 3.2.4 Device holder

The DASY device holder is designed to cope with the different positions given in the standard.

It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales are the ear reference point (ERP). Thus the device needs no repositioning when changing the angles. The DASY device holder is constructed of low-loss POM material having the following dielectric parameters: relative permittivity =3 and loss tangent =0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Figure 4 Probe



Figure 5 Device Holder

#### 3.2.5 Phantom

The SAM Twin Phantom and the ELI4 Phantom are constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is in compliance with the specification set in IEEE P1528 and CENELEC EN62209-1. The SAM Twin phantom



enables the dosimetric evaluation of left and right hand phone usage and the ELI4 phantom enables the dosimetric evaluation of body mounted usage. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot.

Shell thickness: 2 mm +/-0.2 mm Filling Volume: Approx. 25 liters

Dimensions (H x L x W): 850 x 1000 x 500 mm





Figure 6 SAM Twin Phantom and ELI Phantom

#### 3.2.6 Data Acquisition Electronics

DAE4 consist of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder with a control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information, as well as an optical uplink for commands and the clock. The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

Input impedance: 200MOhm, symmetrical and floating.

Common mode rejection: > 80 dB.

#### 3.2.7 Validation dipoles

SPEAG has a full range of dipoles corresponding to the frequencies defines by the standards: 835, 900, 1800, 1900, 2000, 2450MHz



Maximum input Power: 100W

Connectors: SMA

Dimensions: (depends on the dipole frequency)





Figure 7 DAE4

Figure 8 Validation Dipoles

### 3.3 Equivalent Tissues

The relative permittivity and conductivity of the tissue material should be within ±5% of the values given in the table below recommended by the FCC OET 65 supplement C.

Target Frequency	Head		Вос	dy
(MHz)	٤r	σ (S/m)	εr	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800-2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

(  $\varepsilon r = relative permittivity, \sigma = conductivity and \rho = 1000 kg/m<sup>3</sup>)$ 



#### 4. Evaluation Procedures

#### 4.1 Data Evaluation

The DASY5 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters: - Sensitivity Normi, aio, ai1, ai2

- Conversion factor ConvFi

- Diode compression point dcpi

Device parameters: - Frequency f

- Crest factor cf

Media parameters: - Conductivity σ

- Density ρ

These parameters must be set correctly in the software. They can be found in the component documents or be imported into the software from the configuration files issued for the DASY5 components. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_{i} = U_{i} + U_{i}^{2} \bullet \frac{cf}{dcpi}$$

with Vi = Compensated signal of channel i (i = x, y, z)

Ui = Input signal of channel i (i = x, y, z)

cf = Crest factor of exciting field (DASY5 parameter)

dcpi = Diode compression point (DASY5 parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes: 
$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

# **GCCT**

H-field probes:  $H_i = \sqrt{V_i \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}}$ 

With Vi = Compensated signal of channel i (i = x, y, z)

Normi = Sensor sensitivity of channel i (i = x, y, z)

ConvF= Sensitivity enhancement in solution

aij = Sensor sensitivity factors for H-field probes

f = Carrier frequency (GHz)

Ei = Electric field strength of channel i in V/m

Hi = Magnetic field strength of channel i in A/m

The RSS value of the field components give the total field strength:

$$E_{\text{tot}} = \sqrt{E_{\text{x}}^2 + E_{\text{y}}^2 + E_{\text{z}}^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{\text{tot}}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

With SAR = local specific absorption rate in mW/g

 $E_{tot}$  = total field strength in V/m

σ= conductivity in [mho/m] or [Siemens/m]

ρ= equivalent tissue density in g/cm<sup>3</sup>

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field as a free space field.

$$P_{\text{pwe}} = \frac{E_{\text{tot}}^2}{3770} \quad \text{Or} \quad P_{\text{pwe}} = H_{\text{tot}}^2 \cdot 37.7$$

With Ppwe = Equivalent power density of a plane wave in mW/cm<sup>2</sup>

E<sub>tot</sub> = total electric field strength in V/m

H<sub>tot</sub> = total magnetic field strength in A/m

#### 4.2 SAR Evaluation Procedures

The procedure for assessing the peak spatial-average SAR value consists of the following steps:

#### Power Reference Measurement

The reference and drift jobs are useful jobs for monitoring the power drift of the device under test in the batch process. Both jobs measure the field at a specified reference position, at a selectable distance from the phantom surface. The reference position can be either the selected section's grid reference point or a



user point in this section. The reference job projects the selected point onto the phantom surface, orients the probe perpendicularly to the surface, and approaches the surface using the selected detection method.

#### Area Scan

The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines implemented in DASY5 software can find the maximum locations even in relatively coarse grids. The scan area is defined by an editable grid. This grid is anchored at the grid reference point of the selected section in the phantom. When the area scan's property sheet is brought-up, grid was at to 15 mm by 15 mm and can be edited by a user.

#### Zoom Scan

Zoom scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default zoom scan measures 7 x 7 x 7 points within a cube whose base faces are centered around the maximum found in a preceding area scan job within the same procedure. If the preceding Area Scan job indicates more then one maximum, the number of Zoom Scans has to be enlarged accordingly (The default number inserted is 1).

#### Power Drift Measurement

The drift job measures the field at the same location as the most recent reference job within the same procedure, and with the same settings. The drift measurement gives the field difference in dB from the reading conducted within the last reference measurement. Several drift measurements are possible for one reference measurement. This allows a user to monitor the power drift of the device under test within a batch process. In the properties of the Drift job, the user can specify a limit for the drift and have DASY5 software stop the measurements if this limit is exceeded.

### 4.3 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEC62209-1 standard. It can be conducted for 1 g and 10 g. The DASY5 system allows evaluations that combine measured data and robot positions, such as:

maximum search

extrapolation



#### boundary correction

#### Peak search for averaged SAR

During a maximum search, global and local maximum searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

#### **Extrapolation**

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Cube Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 7x7x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1 g and 10 g cubes.

#### **Boundary effect**

For measurements in the immediate vicinity of a phantom surface, the field coupling effects between the probe and the boundary influence the probe characteristics. Boundary effect errors of different dosimetric probe types have been analyzed by measurements and using a numerical probe model. As expected, both methods showed an enhanced sensitivity in the immediate vicinity of the boundary. The effect strongly depends on the probe dimensions and disappears with increasing distance from the boundary. The sensitivity can be approximately given as:

$$S \approx S_o + S_b \exp(-\frac{z}{a})\cos(\pi \frac{z}{\lambda})$$

Since the decay of the boundary effect dominates for small probes (a $<<\lambda$ ), the cos-term can be omitted. Factors Sb (parameter Alpha in the DASY5 software) and a (parameter Delta in the DASY5 software) are assessed during probe calibration and used for numerical compensation of the boundary effect. Several simulations and measurements have confirmed that the compensation is valid for different field and



boundary configurations.

This simple compensation procedure can largely reduce the probe uncertainty near boundaries. It works well as long as:

the boundary curvature is small

the probe axis is angled less than 30° to the boundary normal

the distance between probe and boundary is larger than 25% of the probe diameter

the probe is symmetric (all sensors have the same offset from the probe tip) Since all of these requirements are fulfilled in a DASY5 system, the correction of the probe boundary effect in the vicinity of the phantom surface is performed in a fully automated manner via the measurement data extraction during post processing.

# 5. Test Laboratory Environment

Temperature	Min. = 20°C, Max. = 25 °C
Relative humidity	Min. = 30%, Max. = 70%
Ground system resistance	< 0.5 Ω

Ambient noise is checked and found very low and in compliance with requirement of standards. Reflection of surrounding objects is minimized and in compliance with requirement of standards.



# **6. Conducted Output Power Measurement**

The following procedures had been used to prepare the EUT for the SAR test.

WIFI (802.11b/g/n)

		Power (dBm)						
	802.11b	802.11g	802.11n(H20)					
Lowest	16.38	15.33	14.01					
Middle	16.31	15.18	13.89					
Highest	16.12	14.91	13.72					
Tune-up limit	17	16	15					



#### 7. SAR Measurement Results

#### 7.1 Liquid Measurement Results

The simulating liquids should be checked at the beginning of a series of SAR measurements to determine of the dielectric parameters are within the tolerances of the specified target values.

Freq. [MHz]	Date	Liquid Type	Liquid Temp. [°C]	Ambient Temp. [°C]	Relative Humidity	Para.	Target Value	Measured Value	Deviation [%]	Limit [%]
2450	June	Body	21.5	21	<b>56</b> 0/	εr	52.7	50.71	-3.78	±5
2430	18, 2013	Бойу	21.5	21	56%	σ	1.95	2.02	3.59	±5

### 7.2 System Performance Check

#### **System Performance Check Measurement conditions**

- The measurements were performed in the flat section of the SAM twin phantom filled with head and body simulating liquid of the following parameters.
- The DASY5 system with an E-field probe was used for the measurements.
- The dipole was mounted on the small tripod so that the dipole feed point was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15 mm (below 1 GHz) and 10 mm (above 1 GHz) from dipole center to the simulating liquid surface.
- The coarse grid with a grid spacing of 10mm was aligned with the dipole.
- Special 5x5x7 fine cube was chosen for cube integration (dx= 8 mm, dy= 8 mm, dz= 5 mm).
- Distance between probe sensors and phantom surface was set to 2.5 mm.



# The depth of Liquid must above 15cm



# **System Performance Check Results**

Freq. [MHz]	Date	Liquid Type	Liquid Temp. [°C]	Amb. Temp . [°C]	Input Power (mW)	Measured SAR_1g (W/Kg)	250mW Target SAR_1g (W/Kg)	Dev. [%]	Limit [%]
2450	June 18, 2013	Body	21.5	21	250	14.1	13.0	8.46	±10



#### 7.3 Measurement Results

Band	Test configuration		Mode	Ch#.	Freq. [MHz]	Powe	r (dBm)	1g SAR (	Power Drift	
Band						Tune-up limit	Measured	Measured	Scaled	(dB)
	Body	Back	802.11 b	11	2462	17	16.38	0.969	1.12	0.15
	Body	Back	802.11 b	6	2437	17	16.38	1.05	1.21	-0.14
WIFI	Body	Back	802.11 b	1	2412	17	16.38	1.15	1.33	0.14
	Body	Back	802.11 b	1	2412	17	16.38	1.14	1.32	-0.07
	Body	Bottom	802.11 b	1	2412	17	16.38	0.348	0.402	-0.12

Note: 1) The body SAR was tested with separation distance 0mm.

- 2) SAR is not required for 802.11g/n channels because the maximum average output power is less than 0.25dB higher than that measured on the corresponding 802.11b channels.
- 3) According to KDB 447498 section 4.3.1, the 1-g SAR test exclusion thresholds at test separation distances≤ 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)]  $\cdot [\sqrt{f(GHz)}] \le 3.0$ .

WIFI maximum tune-up limit power is 17dBm=50.12mW. So SAR measurements are not required when the distance between the antenna and tablet edge further than 26.15mm. Hence, body SAR for top, right and left configuration measurements was not required because the bottom, right and left side of the EUT with WIFI antenna further than 26.15 mm from these surfaces.

4) Blue entries represent repeated test.



### **Measurement variability consideration**

According to KDB 865664 D01v01r01 section 2.8.1, repeated measurements are required following the procedures as below:

- 1) Repeated measurement is not required when the original highest measured SAR is < 0.80 W/kg; steps 2) through 4) do not apply.
- 2) When the original highest measured SAR is ≥ 0.80 W/kg, repeat that measurement once.
- 3) Perform a second repeated measurement only if the ratio of largest to smallest SAR for the original and first repeated measurements is > 1.20 or when the original or repeated measurement is ≥ 1.45 W/kg (~ 10% from the 1-g SAR limit).
- 4) Perform a third repeated measurement only if the original, first or second repeated measurement is  $\geq$  1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20.


	Test configuration		Mode	Ch#.	Freq. (MHz)	Measured SAR (W/Kg)				
Band						Original	1 <sup>st</sup> Repeated		2 <sup>nd</sup> Repeated	
							Value	Ratio	Value	Ratio
WIFI	Body	Back	802.11 b	1	2412	1.15	1.14	1.01	NA	NA



#### **SAR** consideration for Bluetooth:

The EUT also support Bluetooth function, the output power of Bluetooth and the antenna layout are as follow:

This picture is look from the back of the MID

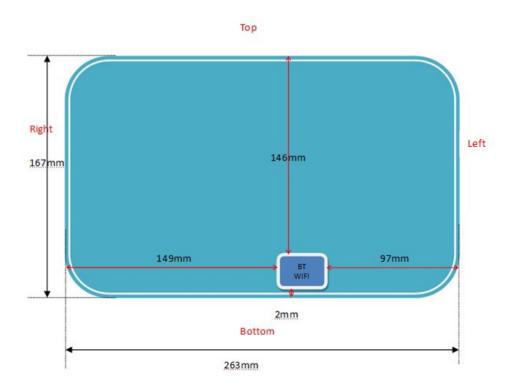

#### Bluetooth:

	Conducted power (dBm)					
	GFSK	Pi/4DQPSK	8QPSK			
Lowest	-2.17	-2.80	-2.84			
Middle	-2.03	-2.54	-2.49			
Highest	-1.56	-2.78	-2.64			
Tune-up limit	-1	-1	-1			

According to KDB 447498 section 4.3.1, the 1-g SAR test exclusion thresholds at test separation distances≤ 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)]  $\cdot [\sqrt{f(GHz)}] \le 3.0$ .

1) Bluetooth maximum tune-up limit power is -1dBm=0.80mW.



For the body SAR, use 5mm as the conservative minimum test separation distance, [(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)]  $\cdot [\sqrt{f(GHz)}] = 0.25 \le 3.0$ .

So Bluetooth standalone SAR measurements are not required.

2) According to KDB 447498 section 4.3.2.2, when standalone SAR test exclusion applies, the standalone SAR must be estimated according to following formula: (max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)]·[ $\sqrt{f(GHz)/x}$ ] W/kg for test separation distances  $\leq$  50 mm; where x = 7.5 for 1-g SAR.

So the estimated Bluetooth SAR is 0.033 W/kg.




# 8. Measurement Uncertainty

Uncertainty Component	Sec.	Tol (+-%)	Prob. Dist.	Div.	Ci (1g)	Ci (10g)	1g Ui (+-%)	10g Ui (+-%)	Vi
Measurement System									
Probe calibration	E.2.1	6.55	N	1.0	1.0	1.0	6.55	6.55	∞
Axial Isotropy	E.2.2	0.5	R	$\sqrt{3}$	1.0	1.0	0.29	0.29	8
Hemispherical Isotropy	E.2.2	2.6	R	$\sqrt{3}$	1.0	1.0	1.5	1.5	8
Boundary effect	E.2.3	0.8	R	$\sqrt{3}$	1.0	1.0	0.46	0.46	∞
Linearity	E.2.4	0.6	R	$\sqrt{3}$	1.0	1.0	0.35	0.35	∞
System detection limits	E.2.5	0.25	R	$\sqrt{3}$	1.0	1.0	0.14	0.14	8
Readout Electronics	E.2.6	0.35	N	1	1.0	1.0	0.35	0.35	∞
Reponse Time	E.2.7	0	R	$\sqrt{3}$	1.0	1.0	0	0	8
Integration Time	E.2.8	2.6	R	$\sqrt{3}$	1.0	1.0	1.5	1.5	∞
RF ambient Conditions-Noise	E.6.1	0	R	$\sqrt{3}$	1.0	1.0	0	0	∞
RF ambient Conditions-Reflections	E.6.1	3.0	R	$\sqrt{3}$	1.0	1.0	1.7	1.7	∞
Probe positioner Mechanical Tolerance	E.6.2	1.5	R	$\sqrt{3}$	1.0	1.0	0.87	0.87	∞
Probe positioning with respect to Phantom Shell	E.6.3	2.9	R	$\sqrt{3}$	1.0	1.0	1.67	1.67	∞
Extrapolation, interpolation and integration Algoritms for Max. SAR	E.5	1.0	R	$\sqrt{3}$	1.0	1.0	0.58	0.58	∞
Test sample Related		<u> </u>		ı	l		l .		
Test Sample Positioning	E.4.2	4.6	N	1.0	1.0	1.0	4.6	4.6	N-1
Device Holder Uncertainty	E.4.1	5.2	N	1.0	1.0	1.0	5.2	5.2	N-1
Output Power Variation - SAR drift measurement	6.6.2	5	R	$\sqrt{3}$	1.0	1.0	2.89	2.89	∞
Phantom and Tissue Parameters									
Phantom Uncertainty (Shape and thickness tolerances)	E.3.1	4.0	R	$\sqrt{3}$	1.0	1.0	2.31	2.31	∞
Liquid conductivity - deviation from target value	E.3.2	5.0	R	$\sqrt{3}$	0.64	0.43	1.85	1.24	∞
Liquid conductivity - measurement uncertainty	E.3.3	2.5	N	1.0	0.64	0.43	1.60	1.08	М
Liquid permitivity - deviation from target value	E.3.2	5.0	R	$\sqrt{3}$	0.6	0.49	1.73	1.42	∞
Liquid permitivity - measurement uncertainty	E.3.3	2.5	N	1.0	0.6	0.49	1.5	1.23	М
Combined Standard Uncertainty			RSS	l	I	l	11.3	11.0	
Expanded Uncertainty (95% Confidence interval)			K				23	22	



# 9. EUT Photos and Test Positions

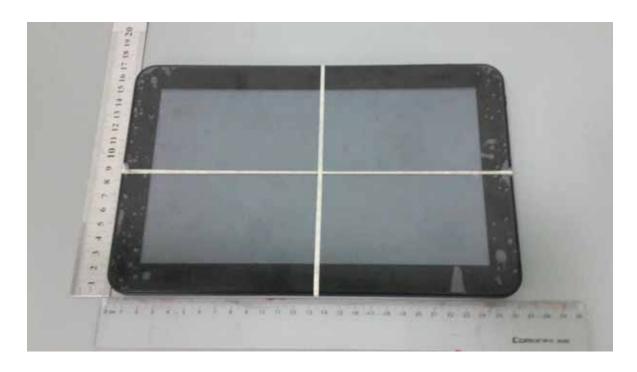

10" Tablet




10" Tablet

# **GCCT**

#### **Test Position:**



**Back side Position (0mm)** 

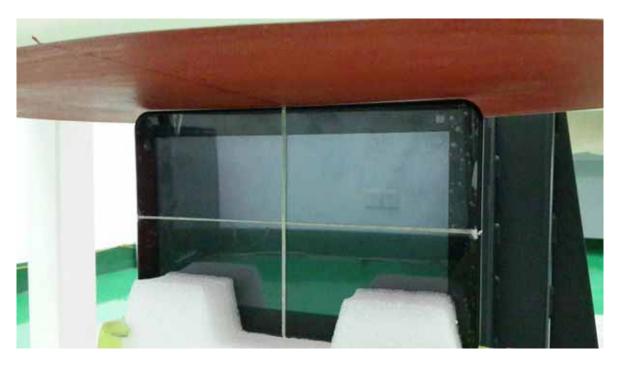

**Bottom side Position (0mm)** 



# 10. Equipment List & Calibration Status

Name of Equipment	Manufacturer	Type/Model	Serial Number	Last Cal. Date	Calibration Due
PC	HP	d7900eC	CZC9312JJ4	N/A	N/A
E-field Probe	SPEAG	ES3DV3	SN 3221	2012-9-27	2013-9-26
DAE	SPEAG	DAE4-SD 000 D04 BJ	SN 893	2012-9-27	2013-9-26
Device Holder	Stäubli	N/A	N/A	N/A	N/A
SAM Phantom	SPEAG	SAM Twin Phantom	TP-1545/TP-1548	N/A	N/A
6 Axis Robot	Stäubli	Robot TX90XL	F09/5B9UA1/A/01	N/A	N/A
DIPOLE 2450MHz	SPEAG	D2450V2	815	2012-9-26	2013-9-25
Wireless Communication Test Set	Anritsu	MT8820C	6201060976	2012-8-27	2013-8-26
Signal Generator	Agilent	5183A	MY49060563	2012-8-27	2013-8-26
Power Meter	Agilent	E4419B	MY45104719	2012-8-27	2013-8-26
Power Sensor	Agilent	N8481H	MY48100148	2012-8-27	2013-8-26
Directional couplers	Agilent	778D	MY48220223	N/A	N/A
Power amplifier	mini-circuits	ZHL-42W	QA0940002	N/A	N/A
Power supply	Topward	3303d	796708	2012-8-27	2013-8-26
Network Analyzer	Agilent	E5071C	MY46108263	2012-8-27	2013-8-26
Liquid Calibration Kit	Agilent	85070E	N/A	N/A	N/A



# 11. Attachments

Exhibit	Content			
1	System Performance Check Plots			
2	SAR Test Plots			
3	Probe calibration report			
4	Dipole calibration report			
5	DAE calibration report			



#### **ANNEXE 1 System Performance Check Plots**

Test Laboratory: GCCT Test Date: June.18, 2013

#### System 2450 MHz dipole

**DUT: Dipole 2450 MHz D2450V2; Type: D2450V2** 

Communication System: CW; Communication System Band: D2450 (2450.0 MHz);

Frequency: 2450 MHz; Communication System PAR: 0 dB

Medium parameters used: f = 2450 MHz;  $\sigma = 2.02 \text{ mho/m}$ ;  $\varepsilon_r = 50.71$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY5 Configuration:

Probe: ES3DV3 - SN3221; ConvF(4.31, 4.31, 4.31); Calibrated: 9/27/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn893; Calibrated: 9/27/2012

Phantom: SAM 1 with CRP v4.0; Type: QD000P40CC; Serial: TP:1586

 Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

**2450 Body/System check/Area Scan (31x71x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm

Reference Value = 87.861 V/m; Power Drift = -0.03 dB

Maximum value of SAR (interpolated) = 16.3 W/kg

2450 Body/System check/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 87.861 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 29.252 mW/g

SAR(1 g) = 14.1 mW/g; SAR(10 g) = 6.56 mW/g

Maximum value of SAR (measured) = 16.0 W/kg

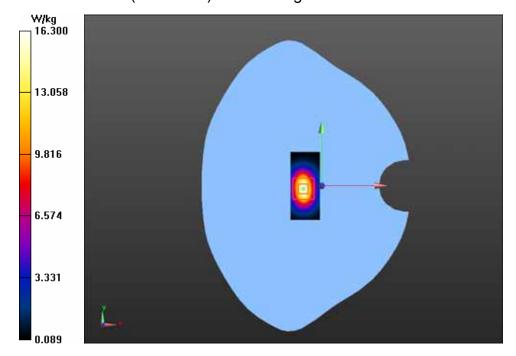



#### **ANNEXE 2 SAR Test Plots**

Test Laboratory: GCCT Test Date: June.18, 2013

WIFI 802.11b back side/High DUT: Contel; Type: TAB-1040

Communication System: 802.11b WiFi 2.4 GHz; Communication System Band: 2450;

Frequency: 2462 MHz; Communication System PAR: 0 dB

Medium parameters used (interpolated): f = 2462 MHz;  $\sigma = 2.048$  mho/m;  $\epsilon_r = 50.622$ ;

 $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### **DASY5** Configuration:

Probe: ES3DV3 - SN3221; ConvF(4.31, 4.31, 4.31); Calibrated: 9/27/2012;

• Sensor-Surface: 4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn893; Calibrated: 9/27/2012

Phantom: ELI v4.0; Type: QD OVA 001 BB; Serial: TP:1069

 Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

WIFI 802.11b back side/High/Area Scan (121x181x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 4.530 V/m; Power Drift = 0.15 dB

Maximum value of SAR (interpolated) = 1.05 W/kg

WIFI 802.11b back side/High/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.530 V/m; Power Drift = 0.15 dB

Peak SAR (extrapolated) = 2.002 mW/g

SAR(1 g) = 0.969 mW/g; SAR(10 g) = 0.500 mW/g

Maximum value of SAR (measured) = 1.05 W/kg

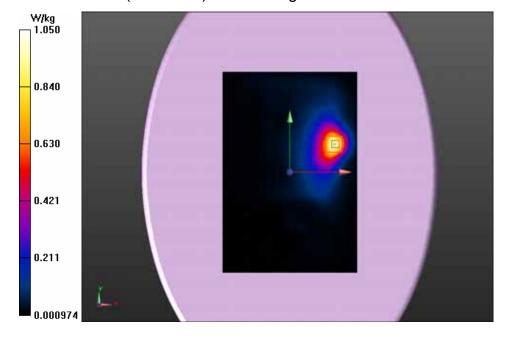



WIFI 802.11b back side/Mid DUT: Contel; Type: TAB-1040

Communication System: 802.11b WiFi 2.4 GHz; Communication System Band: 2450;

Frequency: 2437 MHz; Communication System PAR: 0 dB

Medium parameters used (interpolated): f = 2437 MHz;  $\sigma = 2.013$  mho/m;  $\varepsilon_r = 50.739$ ;

 $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### **DASY5** Configuration:

Probe: ES3DV3 - SN3221; ConvF(4.31, 4.31, 4.31); Calibrated: 9/27/2012;

• Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn893; Calibrated: 9/27/2012

Phantom: ELI v4.0; Type: QD OVA 001 BB; Serial: TP:1069

 Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

WIFI 802.11b back side/Mid/Area Scan (121x181x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 4.392 V/m; Power Drift = -0.14 dB

Maximum value of SAR (interpolated) = 1.16 W/kg

WIFI 802.11b back side/Mid/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.392 V/m; Power Drift = -0.14 dB

Peak SAR (extrapolated) = 2.142 mW/g

SAR(1 g) = 1.05 mW/g; SAR(10 g) = 0.545 mW/g

Maximum value of SAR (measured) = 1.13 W/kg

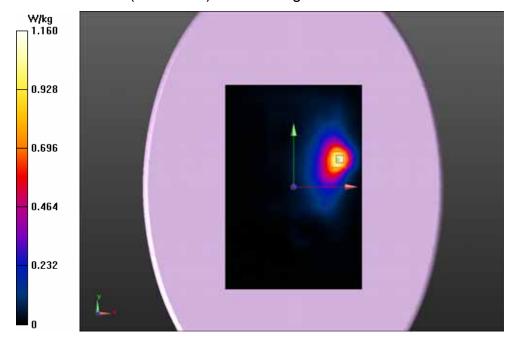



WIFI 802.11b back side/Low DUT: Contel; Type: TAB-1040

Communication System: 802.11b WiFi 2.4 GHz; Communication System Band: 2450;

Frequency: 2412 MHz; Communication System PAR: 0 dB

Medium parameters used (interpolated): f = 2412 MHz;  $\sigma = 1.968$  mho/m;  $\varepsilon_r = 50.861$ ;

 $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### **DASY5** Configuration:

Probe: ES3DV3 - SN3221; ConvF(4.31, 4.31, 4.31); Calibrated: 9/27/2012;

• Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn893; Calibrated: 9/27/2012

Phantom: ELI v4.0; Type: QD OVA 001 BB; Serial: TP:1069

 Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

WIFI 802.11b back side/Low/Area Scan (121x181x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 3.531 V/m; Power Drift = 0.14 dB

Maximum value of SAR (interpolated) = 1.25 W/kg

WIFI 802.11b back side/Low/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.531 V/m; Power Drift = 0.14 dB


Peak SAR (extrapolated) = 2.338 mW/g

SAR(1 g) = 1.15 mW/g; SAR(10 g) = 0.595 mW/g

Maximum value of SAR (measured) = 1.25 W/kg

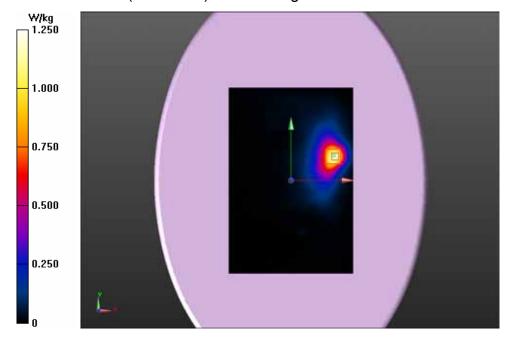



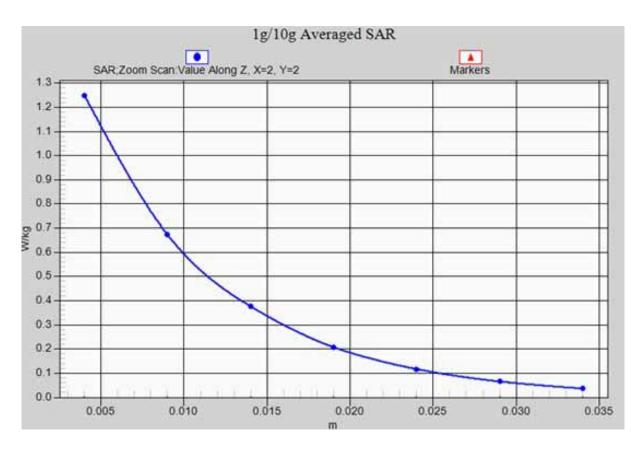

WIFI 802.11b back side/Low\_ z-axis scan



WIFI 802.11b back side/Low DUT: Contel; Type: TAB-1040

Communication System: 802.11b WiFi 2.4 GHz; Communication System Band: 2450;

Frequency: 2412 MHz; Communication System PAR: 0 dB

Medium parameters used (interpolated): f = 2412 MHz;  $\sigma = 1.968$  mho/m;  $\epsilon_r = 50.861$ ;

 $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY5 Configuration:

Probe: ES3DV3 - SN3221; ConvF(4.31, 4.31, 4.31); Calibrated: 9/27/2012;

• Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn893: Calibrated: 9/27/2012

Phantom: ELI v4.0; Type: QD OVA 001 BB; Serial: TP:1069

 Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

WIFI 802.11b back side/Low 2/Area Scan (121x181x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 3.875 V/m; Power Drift = -0.07 dB

Maximum value of SAR (interpolated) = 1.26 W/kg

WIFI 802.11b back side/Low 2/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.875 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 2.325 mW/g

SAR(1 g) = 1.14 mW/g; SAR(10 g) = 0.593 mW/g

Maximum value of SAR (measured) = 1.25 W/kg

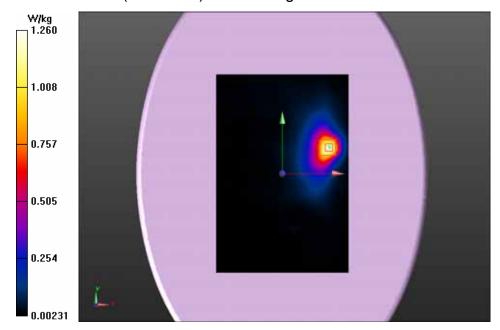



WIFI802.11b/Bottom side-Low DUT: Contel; Type: TAB-1040

Communication System: 802.11b WiFi 2.4 GHz; Communication System Band: 2450;

Frequency: 2412 MHz; Communication System PAR: 0 dB

Medium parameters used (interpolated): f = 2412 MHz;  $\sigma = 1.968$  mho/m;  $\varepsilon_r = 50.861$ ;

 $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### **DASY5** Configuration:

Probe: ES3DV3 - SN3221; ConvF(4.31, 4.31, 4.31); Calibrated: 9/27/2012;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn893; Calibrated: 9/27/2012

Phantom: ELI v4.0; Type: QD OVA 001 BB; Serial: TP:1069

 Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

WIFI802.11b/Bottom side-Low/Area Scan (21x181x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 10.077 V/m; Power Drift = -0.12 dB

Maximum value of SAR (interpolated) = 0.390 W/kg

WIFI802.11b/Bottom side-Low/Zoom Scan (5x5x7)/Cube 0: Measurement grid:


dx=8mm, dy=8mm, dz=5mm

Reference Value = 10.077 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 0.807 mW/g

SAR(1 g) = 0.348 mW/g; SAR(10 g) = 0.170 mW/g

Maximum value of SAR (measured) = 0.389 W/kg

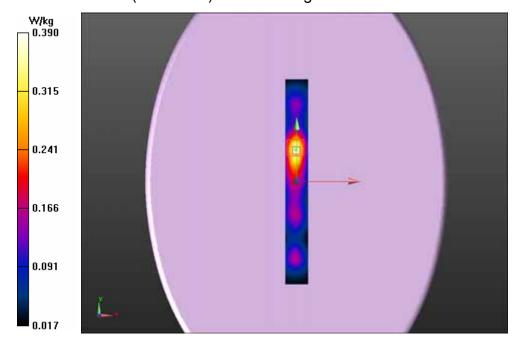

# **GCCT**

# **ANNEXE 3 Probe calibration report**

## GCCT

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

GCCT (Auden)

Certificate No: ES3-3221\_Sep12

S

Accreditation No.: SCS 108

### CALIBRATION CERTIFICATE

Object

ES3DV3 - SN:3221

Calibration procedure(s)

QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4 Calibration procedure for dosimetric E-field probes

Calibration date:

September 27, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4412A	MY41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: S5054 (3c)	27-Mar-12 (No. 217-01531)	Apr-13
Reference 20 dB Attenuator	SN: S5086 (20b)	27-Mar-12 (No. 217-01529)	Apr-13
Reference 30 dB Attenuator	SN: S5129 (30b)	27-Mar-12 (No. 217-01532)	Apr-13
Reference Probe ES3DV2	SN: 3013	29-Dec-11 (No. ES3-3013_Dec11)	Dec-12
DAE4	SN: 660	20-Jun-12 (No. DAE4-660_Jun12)	Jun-13
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-11)	In house check: Apr-13
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

Function Calibrated by: Jeton Kastrati Laboratory Technician Katja Pokovic Technical Manager Approved by:

Issued October 1, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory



#### Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z

CF

tissue simulating liquid sensitivity in free space

ConvF DCP sensitivity in TSL / NORMx,y,z diode compression point

crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

A, B, C Polarization φ

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
  power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
  maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
  exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

No.130601 Page 39 of 62



ES3DV3 - SN:3221

September 27, 2012

# Probe ES3DV3

SN:3221

Manufactured:

September 1, 2009

Repaired:

September 11, 2012

Calibrated:

September 27, 2012

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)



ES3DV3- SN:3221

September 27, 2012

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3221

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) <sup>2</sup> ) <sup>A</sup>	1.11	1.38	1.06	± 10.1 %
DCP (mV) <sup>B</sup>	103.6	100.4	103.1	

#### **Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dB	C dB	WR mV	Unc <sup>E</sup> (k=2)
0	CW	0.00	X	0.00	0.00	1.00	144.5	±3.5 %
			Y	0.00	0.00	1.00	122.0	
			Z	0.00	0.00	1.00	143.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>^</sup> The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the



ES3DV3-SN:3221

September 27, 2012

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3221

#### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	41.5	0.90	6.20	6.20	6.20	0.25	2.17	± 12.0 %
900	41.5	0.97	6.17	6.17	6.17	0.27	1.99	± 12.0 %
1750	40.1	1.37	5.60	5.60	5.60	0.80	1.16	± 12.0 %
1900	40.0	1.40	5.39	5.39	5.39	0.62	1.40	± 12.0 %
2000	40.0	1.40	5.34	5.34	5.34	0.76	1.22	± 12.0 %
2450	39.2	1.80	4.68	4.68	4.68	0.80	1.24	± 12.0 %

 $<sup>^{\</sup>rm C}$  Frequency validity of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to  $\pm$  50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.  $^{\rm T}$  At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



ES3DV3-SN:3221

September 27, 2012

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3221

#### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	55.2	0.97	6.23	6.23	6.23	0.37	1.80	± 12.0 %
900	55.0	1.05	6.17	6.17	6.17	0.80	1.16	± 12.0 %
1750	53.4	1.49	5.17	5.17	5.17	0.59	1.46	± 12.0 %
1900	53.3	1.52	4.87	4.87	4.87	0.46	1.73	± 12.0 %
2000	53.3	1.52	4.89	4.89	4.89	0.64	1.49	± 12.0 %
2450	52.7	1.95	4.31	4.31	4.31	0.68	1.16	± 12.0 9


<sup>&</sup>lt;sup>c</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>c</sup> At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to

<sup>\*</sup> At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

ES3DV3-SN:3221 September 27, 2012


## Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

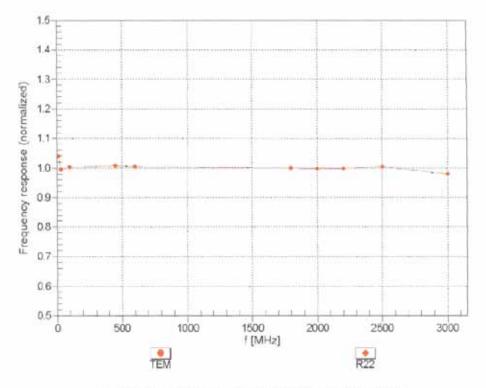


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

ES3DV3- SN:3221 September 27, 2012

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

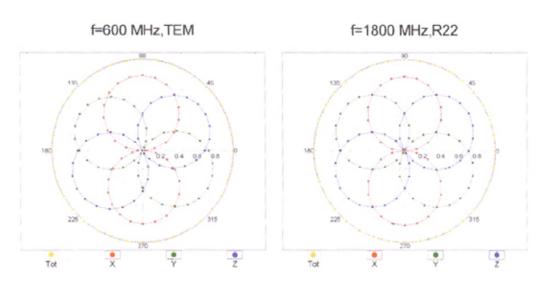


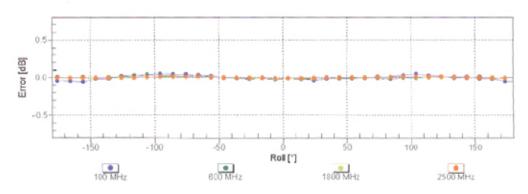


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

ES3DV3- SN:3221 September 27, 2012

### Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

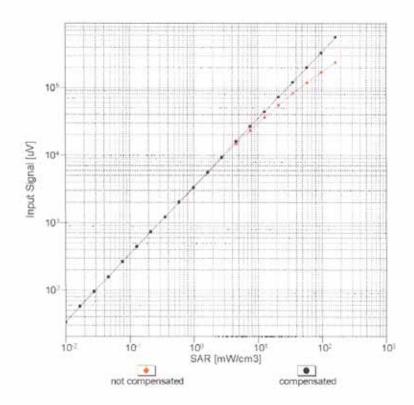


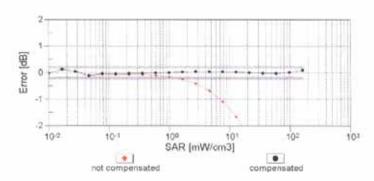


Uncertainty of Linearity Assessment: ± 0.6% (k=2)






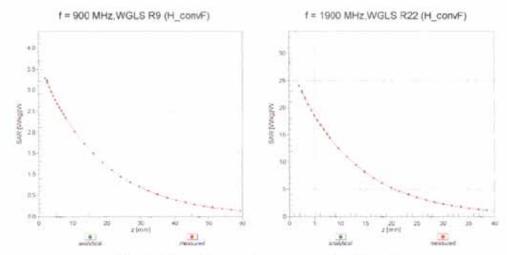

### Deviation from Isotropy in Liquid Error (\( \phi, \( \Pri \)), f = 900 MHz

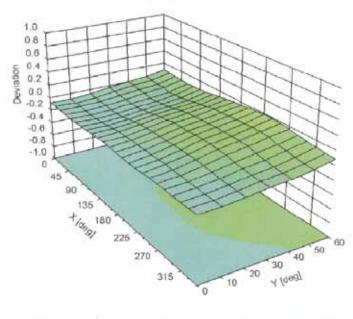





ES3DV3-SN:3221

September 27, 2012

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3221

#### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	34
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

## **GCCT**

## **ANNEXE 4 Dipole calibration report**

## **GCCT**

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

GCCT (Auden)

Certificate No: D2450V2-815\_Sep12

Accreditation No.: SCS 108

CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 815

Calibration procedure(s)

QA CAL-05.v8

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

September 26, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	
Power meter EPM-442A	GB37480704	05-Oct-11 (No. 217-01451)	Oct-12	
Power sensor HP 8481A	US37292783	05-Oct-11 (No. 217-01451)	Oct-12	
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13	
Type-N mismatch combination	SN: 5047.2 / 06327	27-Mar-12 (No. 217-01533)	Apr-13	
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12	
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13	
Secondary Standards	10.#	Check Date (in house)	Scheduled Check	
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13	
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13	
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12	

Calibrated by:

Israe El-Naouq

Function Laboratory Technician Signature

Approved by:

Katja Pokovic

Technical Manager

Issued: September 26, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



#### Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdien
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.4 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.2 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.24 mW/g
SAR for nominal Head TSL parameters	normalized to 1W	24.9 mW /g ± 16.5 % (k=2)

#### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.0 ± 6 %	2.01 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	50.9 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.06 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.9 mW / g ± 16.5 % (k=2)



#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.4 Ω + 3.0 jΩ
Return Loss	- 29.7 dB

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$48.7 \Omega + 4.7 j\Omega$
Return Loss	- 26.1 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.158 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 23, 2007



#### DASY5 Validation Report for Head TSL

Date: 26.09.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 815

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 1.84 \text{ mho/m}$ ;  $\varepsilon_r = 39.9$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard; DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2011;

· Sensor-Surface: 3mm (Mechanical Surface Detection)


· Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

#### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 99.653 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 27.468 mW/g SAR(1 g) = 13.4 mW/g; SAR(10 g) = 6.24 mW/g Maximum value of SAR (measured) = 16.9 W/kg

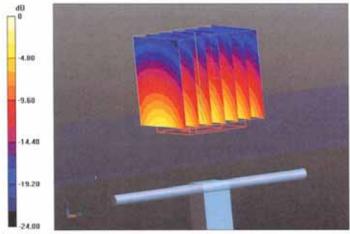

0 dB = 16.9 W/kg = 24.56 dB W/kg



#### Impedance Measurement Plot for Head TSL

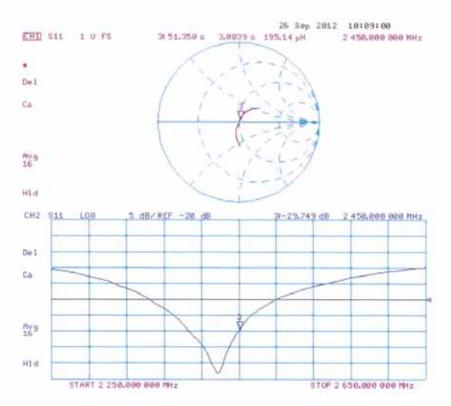



#### **DASY5 Validation Report for Body TSL**

Date: 26.09.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 815

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 2.01 \text{ mho/m}$ ;  $\varepsilon_r = 51$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.26, 4.26, 4.26); Calibrated: 30.12.2011;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 27.06.2012

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

#### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.205 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.024 mW/g

SAR(1 g) = 13 mW/g; SAR(10 g) = 6.06 mW/g


Maximum value of SAR (measured) = 17.0 W/kg

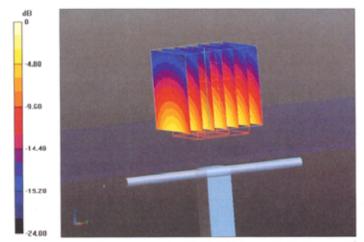

0 dB = 17.0 W/kg = 24.61 dB W/kg



#### Impedance Measurement Plot for Body TSL

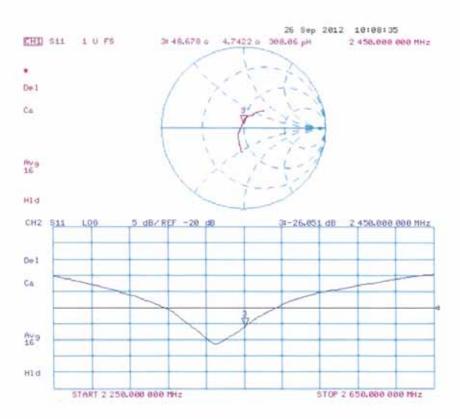

# **GCCT**

# **ANNEXE 5 DAE calibration report**



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

CALIBRATION C	EKTIFICATE		
Object	DAE4 - SD 000 D	04 BJ - SN: 893	
Calibration procedure(s)	QA CAL-06.v25 Calibration proced	lure for the data acquisition of	electronics (DAE)
Calibration date:	September 27, 20	12	
		nal standards, which realize the physic shability are given on the following page	
The measurements and the unce	ertainties with confidence proceed in the closed laboratory TE critical for calibration)	obability are given on the following page facility: environment temperature (22	es and are part of the certificate.  ± 3)°C and humidity < 70%.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence proceed in the closed laboratory TE critical for calibration)  ID #	chability are given on the following page facility: environment temperature (22: Cal Date (Certificate No.)	es and are part of the certificate.  ± 3)°C and humidity < 70%.  Scheduled Calibration
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence proceed in the closed laboratory TE critical for calibration)	obability are given on the following page facility: environment temperature (22:	es and are part of the certificate.  ± 3)°C and humidity < 70%.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	ertainties with confidence proceed in the closed laboratory TE critical for calibration)  ID #  SN: 0810278  ID #	chability are given on the following page facility: environment temperature (22:  Cal Date (Certificate No.) 28-Sep-11 (No:11460)  Check Date (in house)	es and are part of the certificate.  ± 3)°C and humidity < 70%.  Scheduled Calibration  Sep-12  Scheduled Check
The measurements and the unce	ertainties with confidence proceed in the closed laboratory TE critical for calibration)  ID #  SN: 0810278  ID #	chability are given on the following page facility: environment temperature (22: Cal Date (Certificate No.) 28-Sep-11 (No:11450)	es and are part of the certificate.  ± 3)°C and humidity < 70%.  Scheduled Calibration  Sep-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	ertainties with confidence proceed in the closed laboratory TE critical for calibration)  (D#  SN: 0810278  ID#  SE UWS 053 AA 1001	chability are given on the following page facility: environment temperature (22 :  Cal Date (Certificate No.)  28-Sep-11 (No:11450)  Check Date (in house)  05-Jan-12 (in house check)	es and are part of the certificate.  £ 3)°C and humidity < 70%.  Scheduled Calibration  Sep-12  Scheduled Check  In house check: Jan-13
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V2.1	ertainties with confidence proceed in the closed laboratory TE critical for calibration)  (D#  SN: 0810278  ID#  SE UWS 053 AA 1001	chability are given on the following page facility: environment temperature (22 :  Cal Date (Certificate No.) 28-Sep-11 (No:11450) Check Date (in house) 05-Jan-12 (in house check)	es and are part of the certificate.  ± 3)°C and humidity < 70%.  Scheduled Calibration  Sep-12  Scheduled Check
The measurements and the unco All calibrations have been condu Calibration Equipment used (M& Primary Standards Keilthley Multimeter Type 2001 Secondary Standards	ertainties with confidence proceed in the closed laboratory TE critical for calibration)  (D#  SN: 0810278  ID#  SE UWS 053 AA 1001	chability are given on the following page facility: environment temperature (22 :  Cal Date (Certificate No.)  28-Sep-11 (No:11450)  Check Date (in house)  05-Jan-12 (in house check)	es and are part of the certificate.  £ 3)°C and humidity < 70%.  Scheduled Calibration  Sep-12  Scheduled Check  In house check: Jan-13

Certificate No: DAE4-893\_Sep12 Page 1 of 5

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.



## DC Voltage Measurement A/D - Converter Resolution nominal

 $\begin{array}{lll} \mbox{High Range:} & \mbox{1LSB} = & \mbox{6.1} \mu\mbox{V} \,, & \mbox{full range} = & \mbox{-100...+300 mV} \\ \mbox{Low Range:} & \mbox{1LSB} = & \mbox{61nV} \,, & \mbox{full range} = & \mbox{-1......+3mV} \end{array}$ 

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	Х	Y	Z
High Range	406.225 ± 0.1% (k=2)	406.084 ± 0.1% (k=2)	405.117 ± 0.1% (k=2)
Low Range	4.01000 ± 0.7% (k=2)	4.02161 ± 0.7% (k=2)	3.98512 ± 0.7% (k=2)

#### Connector Angle

Connector Angle to be used in DASY system 174.5 *± 1 *	Connector Angle to be used in DASY system	174.5°±1°
--	---	-----------



#### Appendix

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	199995.97	-2.11	-0.00
Channel X + Input	20003.49	2.31	0.01
Channel X - Input	-19996.34	3.89	-0.02
Channel Y + Input	199996.46	-1.92	-0.00
Channel Y + Input	19999.56	-1.41	-0.01
Channel Y - Input	-20000.29	0.07	-0.00
Channel Z + Input	199997.57	-0.73	-0.00
Channel Z + Input	19998.79	-2.14	-0.01
Channel Z - Input	-20001.40	-1.01	0.01

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2003.38	2.07	0.10
Channel X + Input	202.34	0.57	0.28
Channel X - Input	-197.99	0.01	-0.01
Channel Y + Input	2002.03	0.81	0.04
Channel Y + Input	200.97	-0.69	-0.34
Channel Y - Input	-198.23	0.01	-0.01
Channel Z + Input	2002.07	0.82	0.04
Channel Z + Input	201.75	0.14	0.07
Channel Z - Input	-200.05	-1.79	0.90

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	17.36	15.93
	- 200	-15.52	-16.86
Channel Y	200	7.39	6.92
	- 200	-8.23	-8.65
Channel Z	200	5.62	5.64
	- 200	-8.03	-8.06

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	3.18	-3.22
Channel Y	200	8.71	-	3.65
Channel Z	200	9.66	6.68	-



#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16472	14639
Channel Y	16065	13652
Channel Z	15699	15904

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input  $10M\Omega$ 

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.78	-1.09	2.36	0.66
Channel Y	-0.06	-2.31	2.02	0.70
Channel Z	-0.52	-2.78	1.43	0.74

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9