

Review & approval

Name Reviewer	Function Reviewer	Review date	Signature
Olaf Weiner	CEO/GM <i>Medimetrics</i>		
Jeff Shimizu	CTO/Director R&D <i>Medimetrics</i>		

Name Approver	Function Approver	Approval date	Signature
Ventzeslav Iordanov	Director QA&RA <i>Medimetrics</i>		

Name Author	Function Author
Ventzeslav Iordanov	Director QA&RA <i>Medimetrics</i>

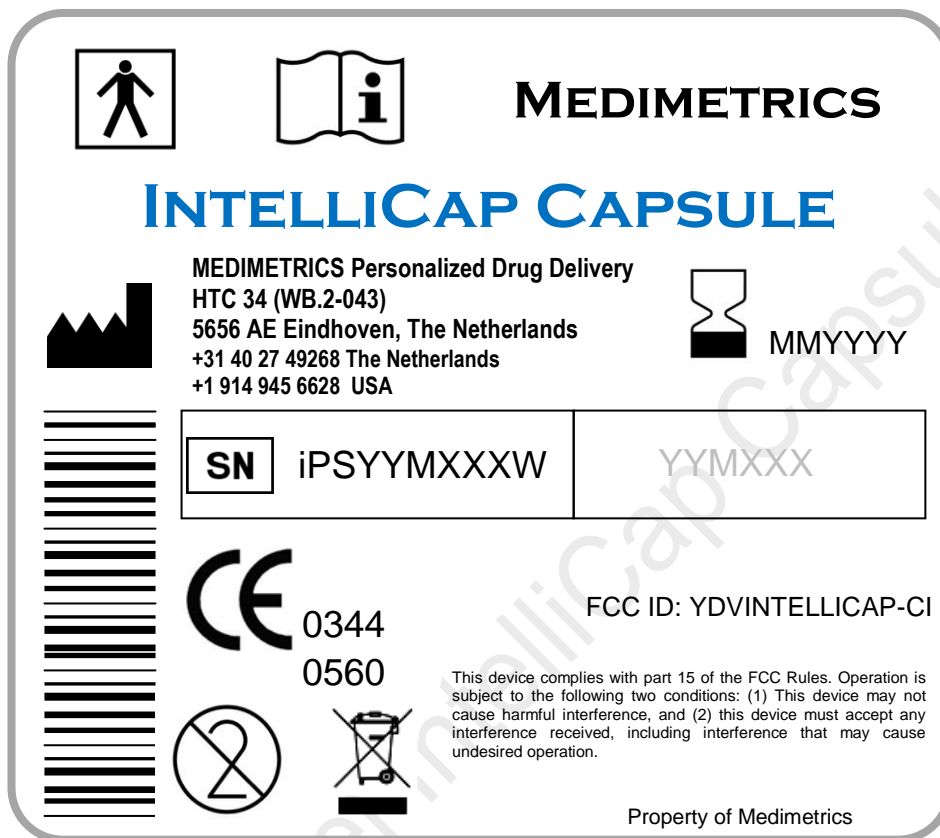
Printed copies are uncontrolled unless authenticated

16 **Table of Contents**


17	1.	Concept Label.....	3
18	2.	Annexes.....	4
19	3.	Document history	4
20			
21			

Printed copies are uncontrolled unless authenticated

1. Concept Label

Manual label IntelliCap container carrier:**Note:**

The IntelliCap serial number is formed by two numbers: the one on the electronic body + the one on the medicine reservoir ring. Since the electronic body will directly be placed in the container carrier it is proposed the container is labeled directly with the number on the electronic body. The medicine ring number is additionally added (e.g. by hand writing) when the reservoir attached. Detailed information on the numbering can be found in Annex 1.

Container label in real size:

Printed copies are uncontrolled unless authenticated

2. Annexes

Annex #	Document title	Document ID
1	Annex IntelliCap capsule label - laser engraving	iPS-100213

3. Document history

Version	Date	Author	Description of changes	CR
0.1	2011-04-28	Ventzeslav Iordanov	Proposed draft	N/A

END OF DOCUMENT

Printed copies are uncontrolled unless authenticated