


Appendix D





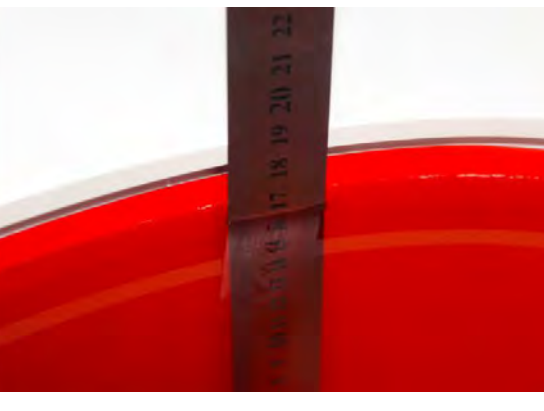

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details


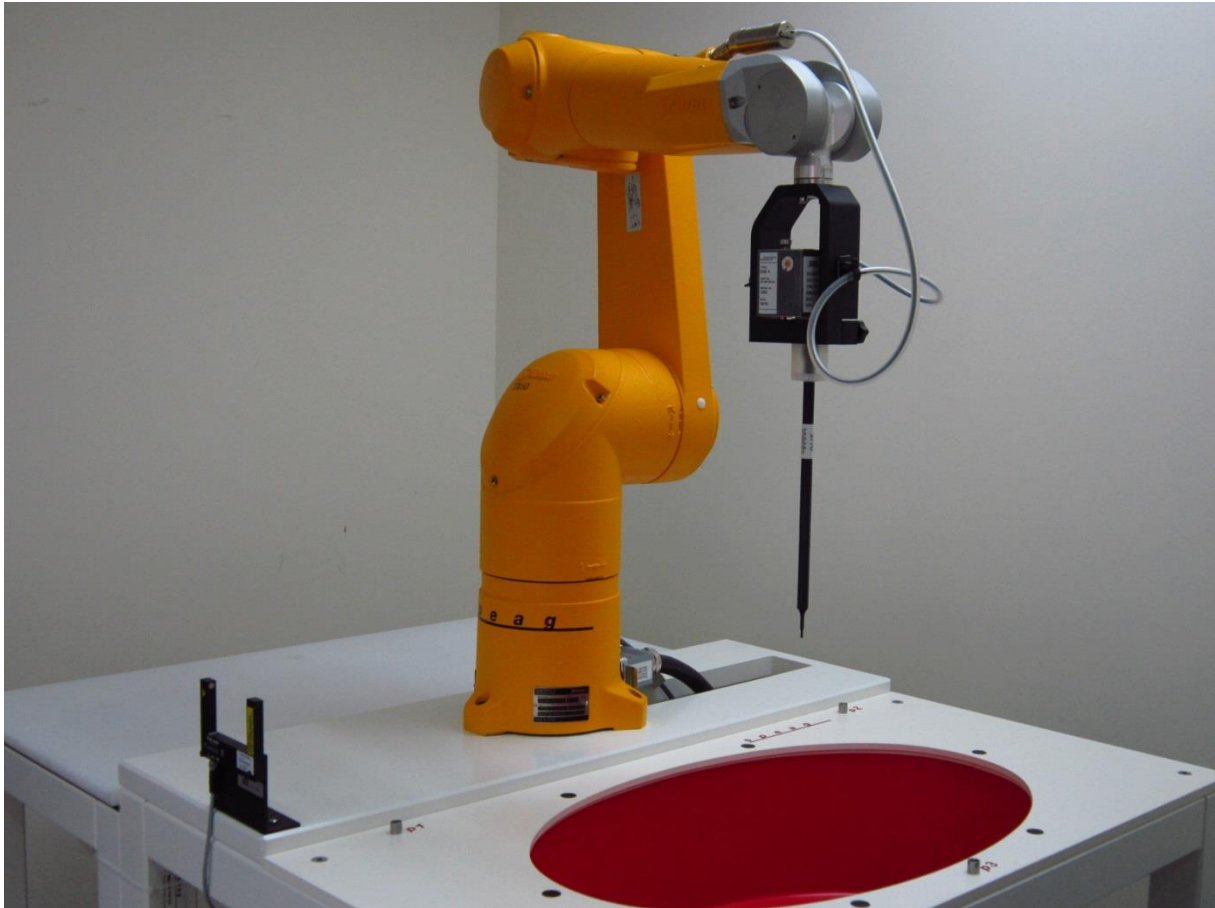



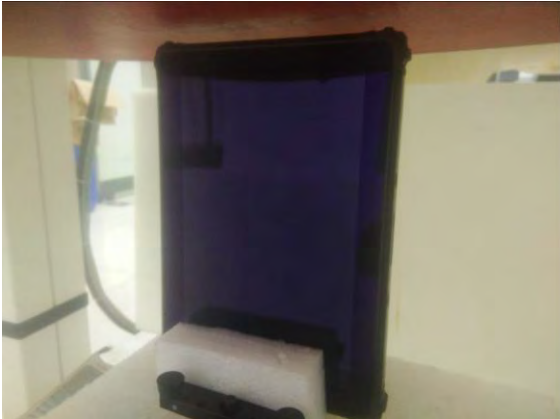
1. SAR measurement System

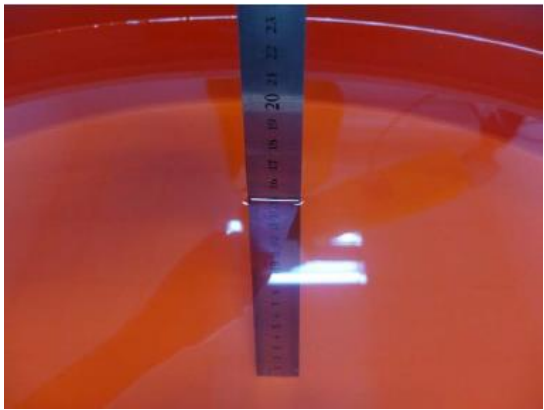

2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Body 750</p>	<p>Photo 2: Tissue Simulant Liquid for Body 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Body 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Body 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Body 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Body 5G</p>
	

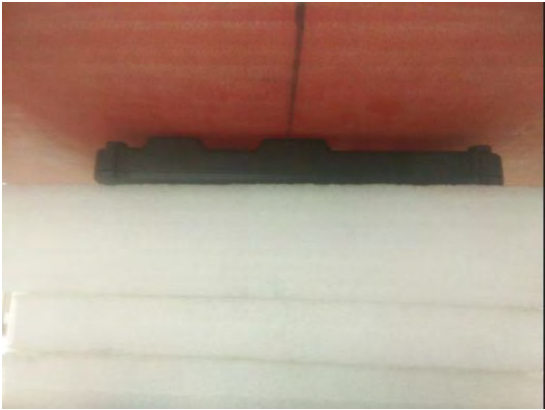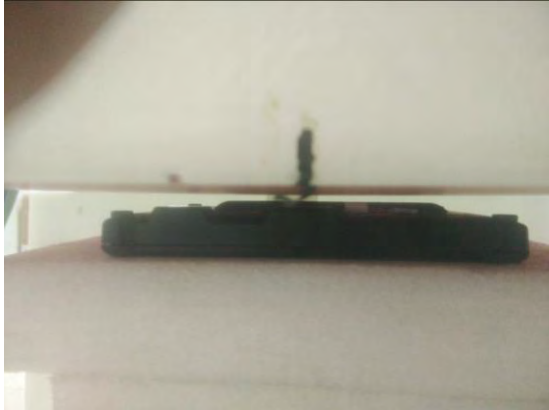3. Photographs of EUT test position

<p>Photo 7: Bottom Face 0mm</p>	<p>Photo 8: Bottom Face 10mm</p>
	
<p>Photo 9: Edge1 0mm</p>	<p>Photo 10: Edge3 0mm</p>
	
<p>Photo 11: Edge2 0mm</p>	<p>Photo 12: Edge2 10mm</p>
	

4. EUT Constructional Details

<div>Photo 13: Front View</div> 	<div>Photo 14: Back View</div> 
<div>Photo 15: Back View</div> 	