

Label location



Label with **FCC ID: ZBE-CR-SCANNER** will be located at the rear side panel.

The statement according to FCC part 15 §15.19(a)(3) is placed in Technical Specification Guide, page 16 (Application exhibit User_manual_21161).

4

3

2

1

D

C

B

A

1.6 in
40.6

1.2 in
30.5

Scanner FCC ID: ZBE-GR-SCANNER
Manufacturer: Carestream Health, Inc.
This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference,
and
(2) this device must accept any interference
received, including interference that may cause
undesired operation.
XXXXXX.A

1.5 radius
4 places

ARTWORK FOR XXXXXX REV. A

DIELINE FOR XXXXXX REV. A

REVISION RECORD

REV	ECO	DATE	DESCRIPTION	DESIGNER
A	XXX	2011-03-03	RELEASE TO PRODUCTION. NEW LABEL	MICHAEL MAROU


MATERIALS:

1. MATERIAL: GENERAL ELECTRIC LEXAN 8010, 0.254mm
HIGH GLOSS, POLYCARBONATE WITH 3M 468MP ADHESIVE OR
3M #9505 ADHESIVE.

2. LABEL TO BE MADE PER ELECTRONIC ARTWORK SUPPLIED BY
CARESTREAM HEALTH INC.

3. OVERLAY MATERIAL MUST MEET THE REQUIREMENTS OF
UL STANDARD 969 (MARKING AND LABELING SYSTEMS [PGDQ2]).

4. SUPPLIER ARTWORK TO BE APPROVED BY CUSTOMER PRIOR TO PRINTING.

5. INSPECTION REQUIREMENTS, IF SHOWN ON DRAWING:
A.  INDICATES PRIMARY INSPECTION DIMENSION.
B. GEOMETRIC TOLERANCES ARE PRIMARY INSPECTION ATTRIBUTES.
C. REFERENCE DIMENSIONS ARE ENCLOSED IN PARENTHESES (). DO NOT
INSPECT REFERENCE DIMENSIONS.

SUPPLIER REQUIREMENTS:

1. SUPPLIER MUST USE UL RECOGNIZED PRINTING PROCESS PER
UL STANDARD 969 (MARKING AND LABELING SYSTEMS [PGDQ2]).

2. UL RECOGNIZED SUPPLIERS MUST INDICATE COMPLIANCE TO
UL STANDARD 969 BY MARKING THE SMALLEST LOT SIZE WITH
THE FOLLOWING:
A. UL FILE NUMBER
B. SUPPLIER'S NAME AND/OR TRADEMARK
C. CARESTREAM HEALTH INC. PART NUMBER AND REVISION
D. DATE OF PRODUCTION.

PMS White
 PMS Black
 DIE LINE

MM (INCH)
25.4 MM = 1 INCH

TOLERANCES EXCEPT AS NOTED

MM	INCHES
0 ± 1	.0 ±
.0 ± 0.5	.00 ±
.00 ± 0.26	.000±
ANGLES ± 0.5	
MATERIAL SEE NOTES	
FINISH SEE NOTES	


CARESTREAM HEALTH, INC.
OAKDALE, MN

THIS IS AN UNPUBLISHED WORK THAT IS CARESTREAM HEALTH, INCORPORATED. RESTRICTED INFORMATION. DISCLOSURE, USE OR
REPRODUCTION WITHOUT THE WRITTEN AUTHORIZATION OF CARESTREAM HEALTH, INCORPORATED IS PROHIBITED. IF PUBLICATION
OCCURS, THE FOLLOWING NOTICE APPLIES: COPYRIGHT (c) 2011, CARESTREAM HEALTH, INCORPORATED. ALL RIGHTS RESERVED.

TITLE LABEL- FCC STATEMENT

MODEL CS7600	DRFT MICHAEL MAROU	DATE 2011-03-03
ENG		DATE 2011-03-03
FSCM NO.	SIZE C	DRAWING NO. XXXXXX
THIRD ANGLE PROJECTION		REV A
INTERPRET PER ASME Y14.5M-1994		DO NOT SCALE DRAWING
SHT 1		OF 1

DRAWING NO.
XXXXXX

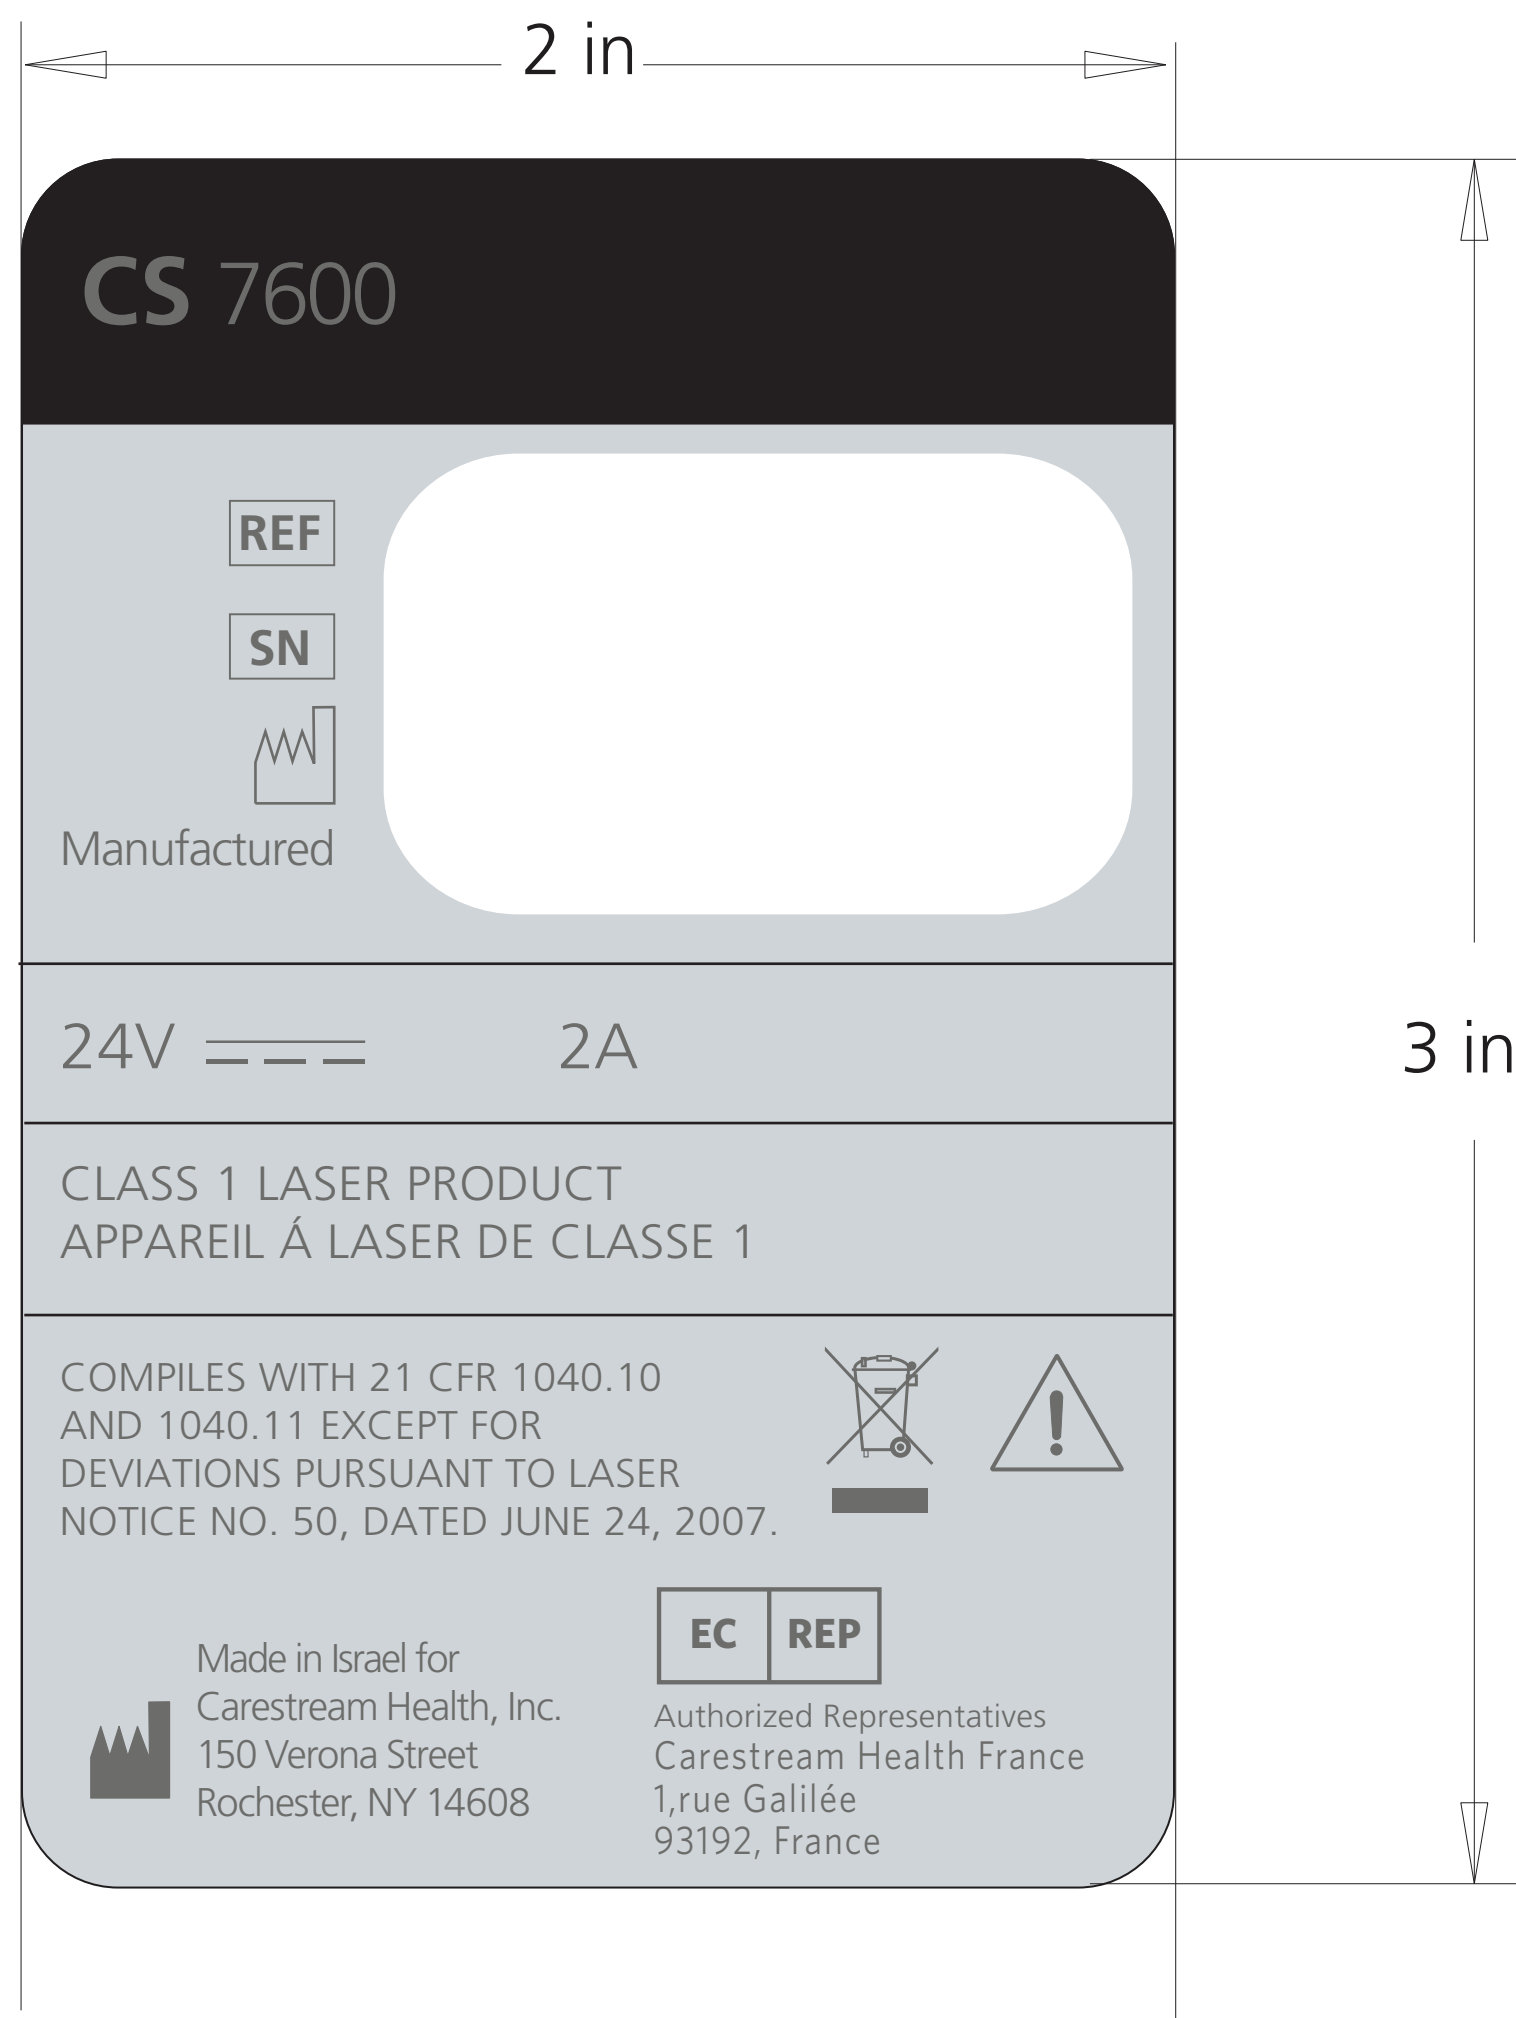

LABEL AT 300% SCALE



LABEL AT 100% SCALE

NOTES:

- 1) MATERIAL, .010" THICK POLYCARBONATE, MATTE FINISH, WITH 3M 467 PRESSURE SENSITIVE ADHESIVE, FARSIDE.
- 2) PARTS SHALL BE SUPPLIED DIE-CUT TO SHAPE WITH PEEL-OFF LINER.
- 3) COLORS: BACKGROUND TO BE SILVER LINING (PANTONE 428), TEXT AND SYMBOLS TO BE ECLIPSE EXCEPT WHERE INDICATED.
- 4) SHALL MEET THE DURABILITY REQUIREMENTS OF UL 60950-1.
- 5) PLACE WRITE-ON OVERLAMINATE OVER ENTIRE SURFACE.
- 6) LABEL TO BE SERIALIZED STARTING WITH 0101 AND RUNNING SEQUENTIALLY,VENDOR TO TRACK NUMBERS.
- 7) SEE PACKAGING GROUP FOR ARTWORK.

NO. XXXXXXX SHEET 1 NEXT SHEET 0		
CHG. NO. DATE REL	REVISIONS	DR BY APPS.
REV A 01/1111	INITIAL RELEASE	DR
UNLESS OTHERWISE SPECIFIED LINEAR TOLERANCE ± 1.6 ANGULAR TOLERANCE $\pm \text{---}$ DIMENSIONS ARE IN MILLIMETERS		MD
CARESTREAM HEALTH, INC. ROCHESTER, NY 14608		
DR. MAROU	DATE 02-14-11	CK
DFTG. KAB	DES. ENG.	MFG. ENG.
NAME LABEL-DATA PLATE, CS 7600 WIRED USB		
SCALE 1X SIZE		DWG SIZE A
NO. XXXXXXX SHEET 1 NEXT SHEET 0		