



Test Setup Photos  
CSA Medical

©2008 Washington Laboratories, Ltd

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE









Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE







# Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE





Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE







Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE





Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE







Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE







Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE





Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE







Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE





Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE







Test Setup Photos  
CSA Medical

©2008 Washington Laboratories, Ltd

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE






# Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE

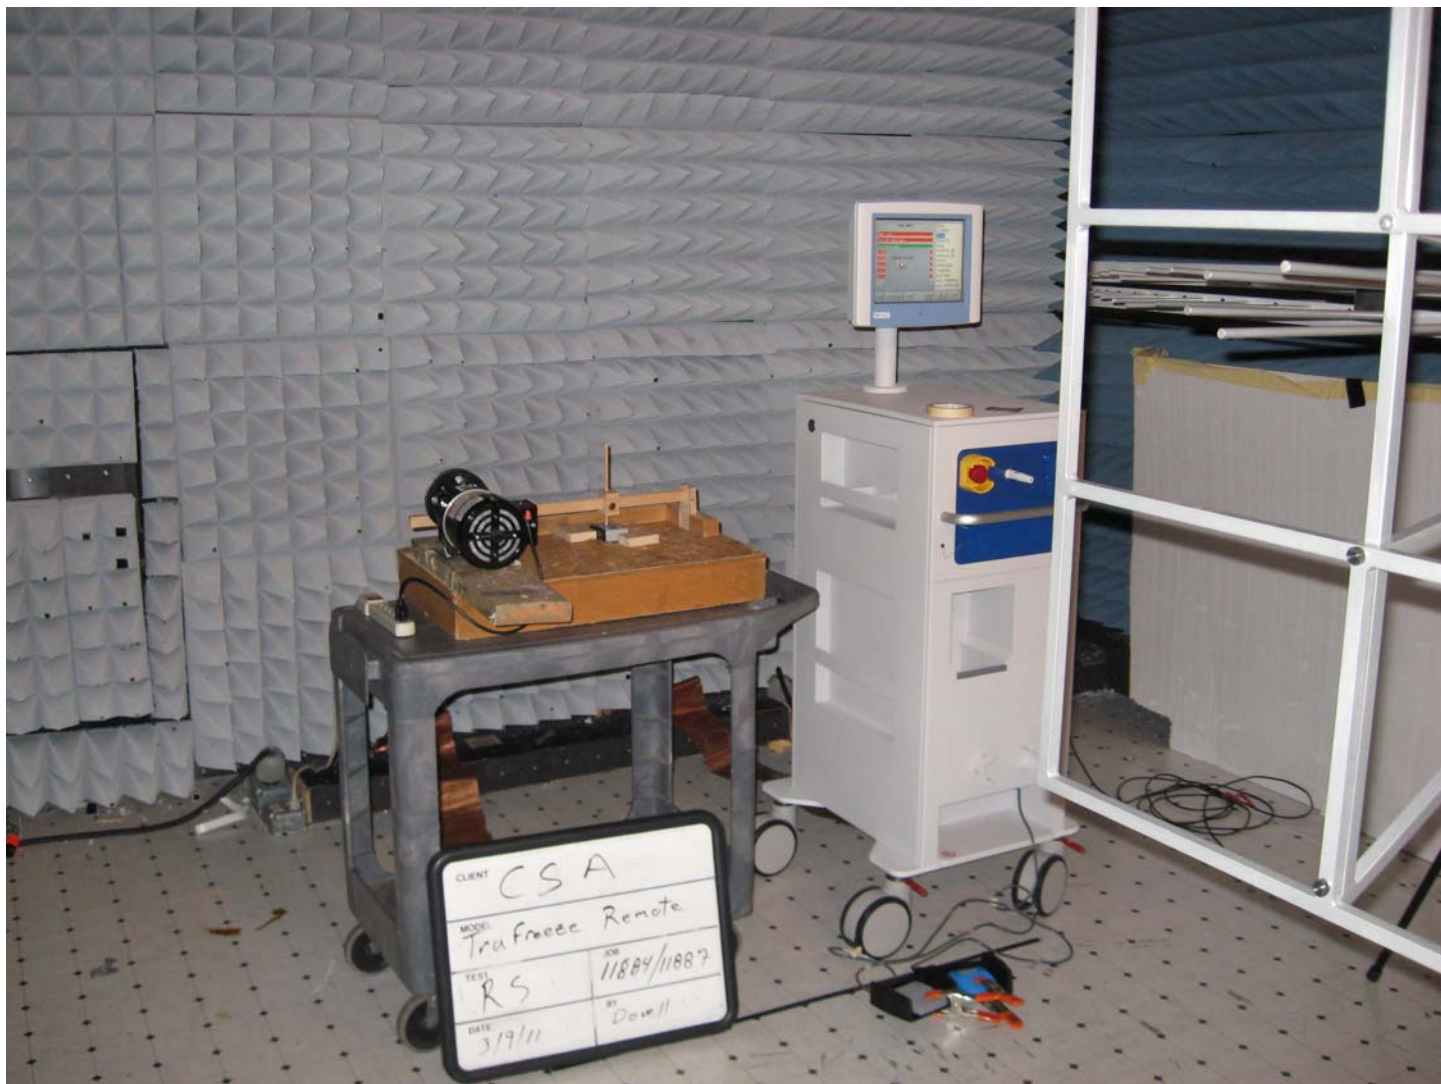





# Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE





# Test Setup Photos

©2008 Washington Laboratories, Ltd

CSA Medical

FCC ID: ZC3-TRUEFREEZE and IC: 9573A-TRUEFREEZE

