


TiO₂ pad: one saline injection, and the recovery

scope_20260829_110950-saline-injection&recovery.csv, one continuous 1 kHz record. Thin trace raw, thick trace smoothed over 101 ms (which nulls the 50 Hz mains pickup on the droplet).


1 — one injection

baseline 1.5523 V, and it comes all the way back

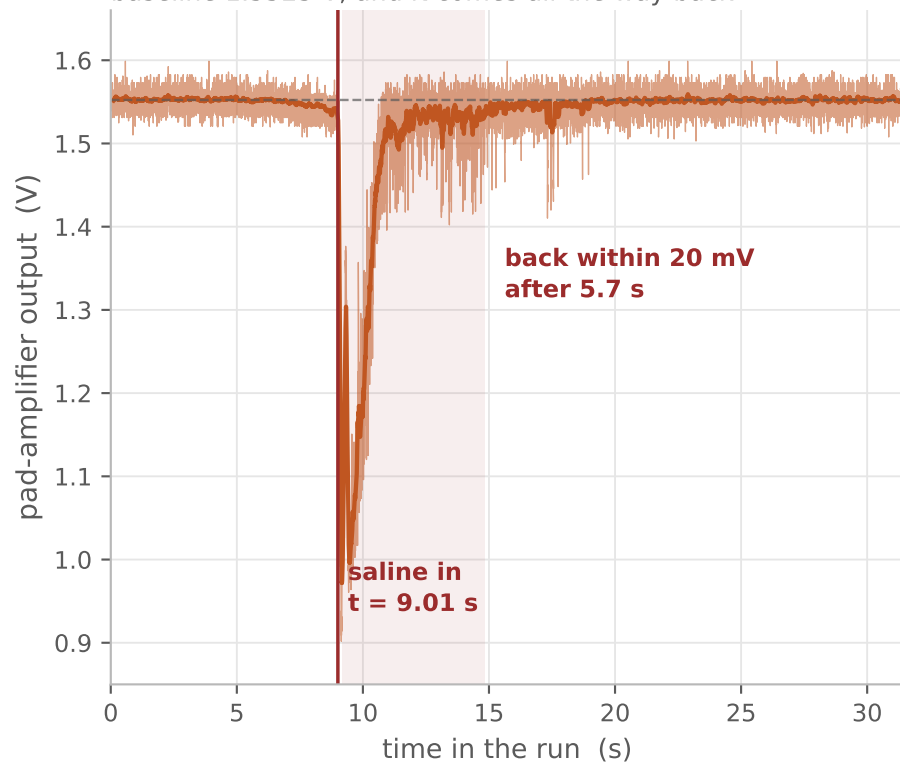

2 — the edge

fast in, and far past the linear range

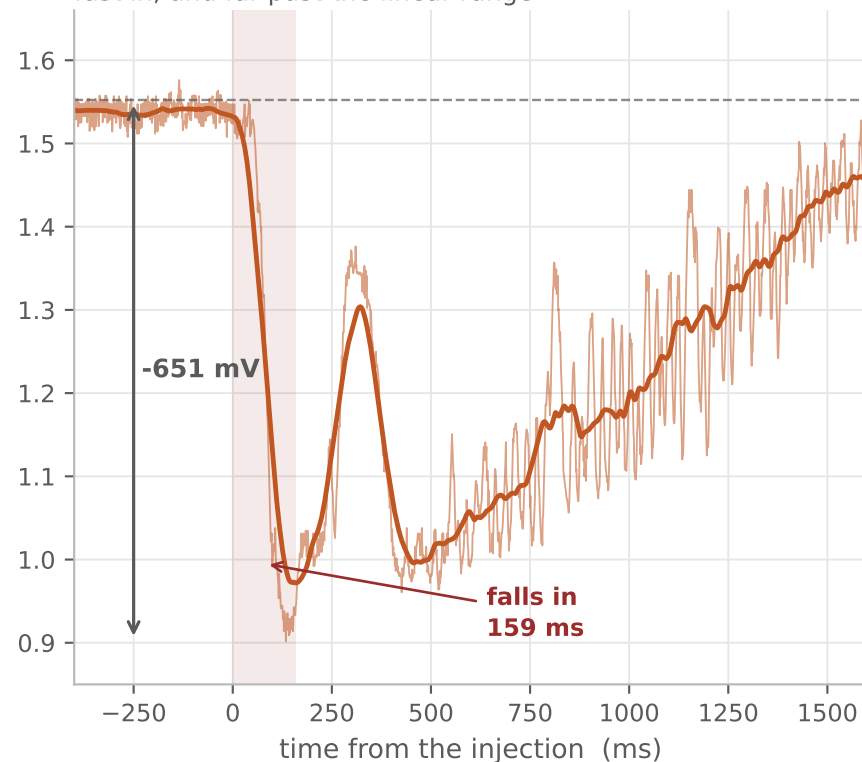

3 — the recovery

the whole rising edge, all the way back

