



DHT22 Humidity and Temperature




MQ Sensor




* RL is 1MOhm for MQ-131 and 4k7Ohm for the others

Voltage Regulator for +5V

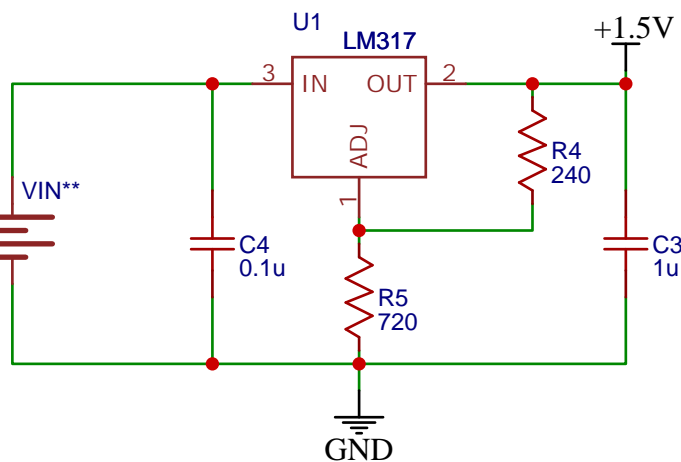


** The Input Voltage (Vin) should be 7~12V DC

Voltage Regulator for +1.5V

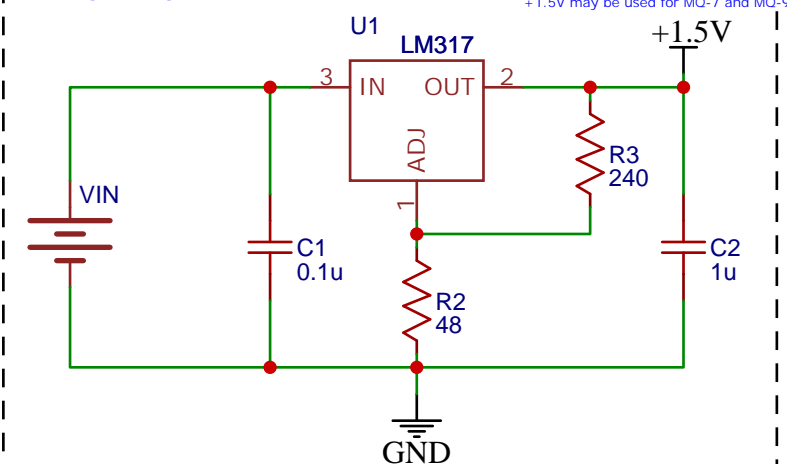

+1.5V may be used for MQ-7 and MQ-9

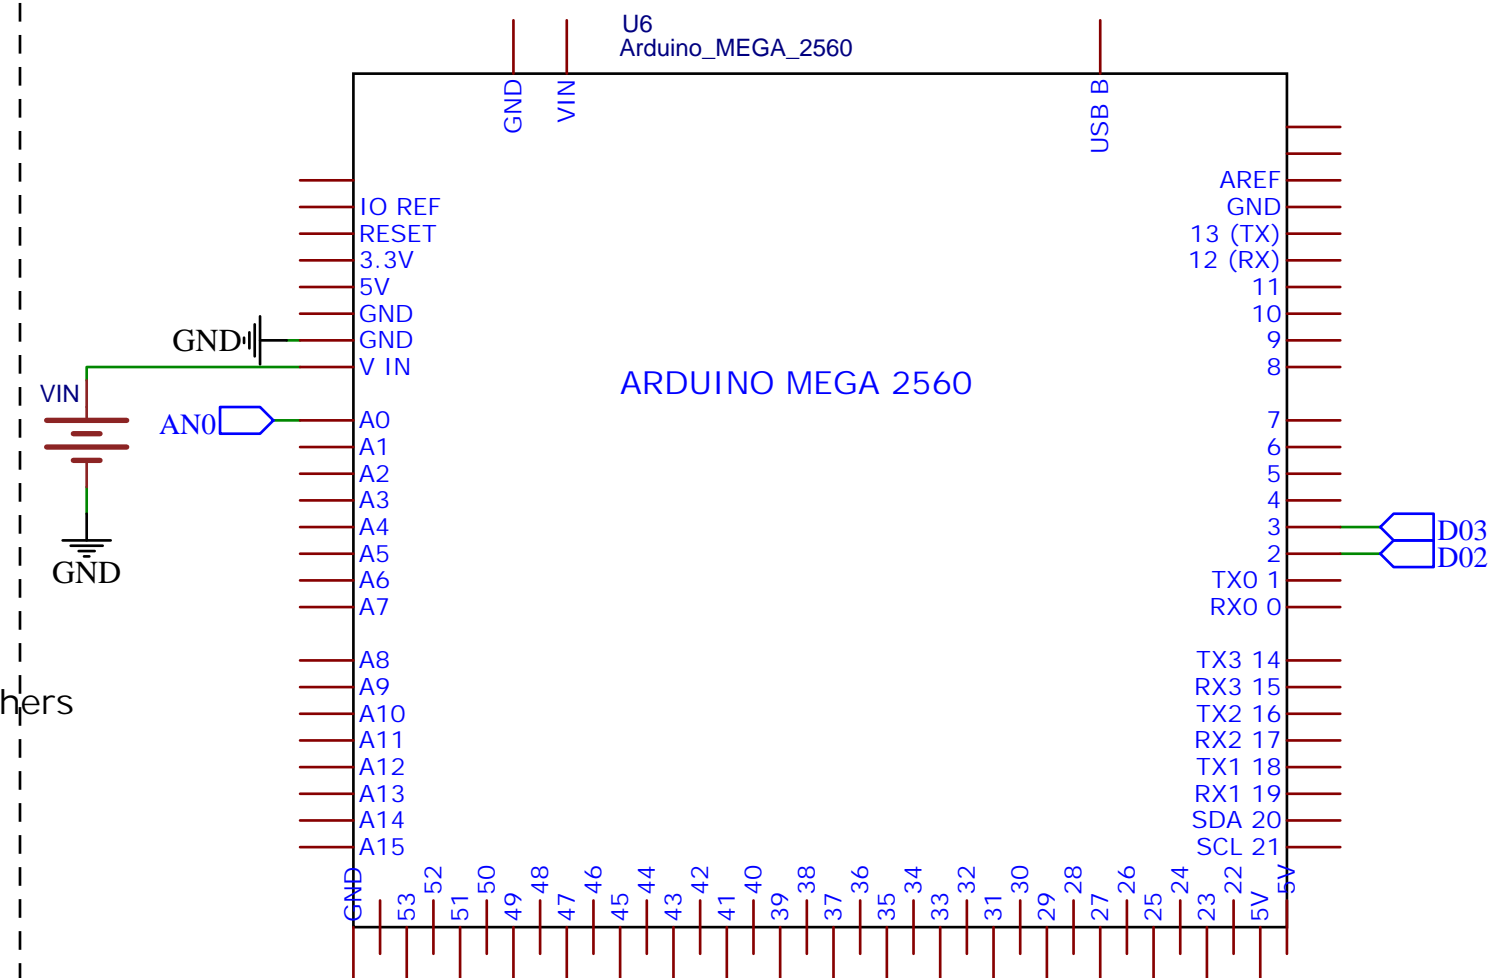

TITLE:

Circuit used for MQSensors Calibration

REV: 1.0



Company: Your Company

Sheet: 1/1

Date: 2021-06-23 Drawn By: Diego Ferreira