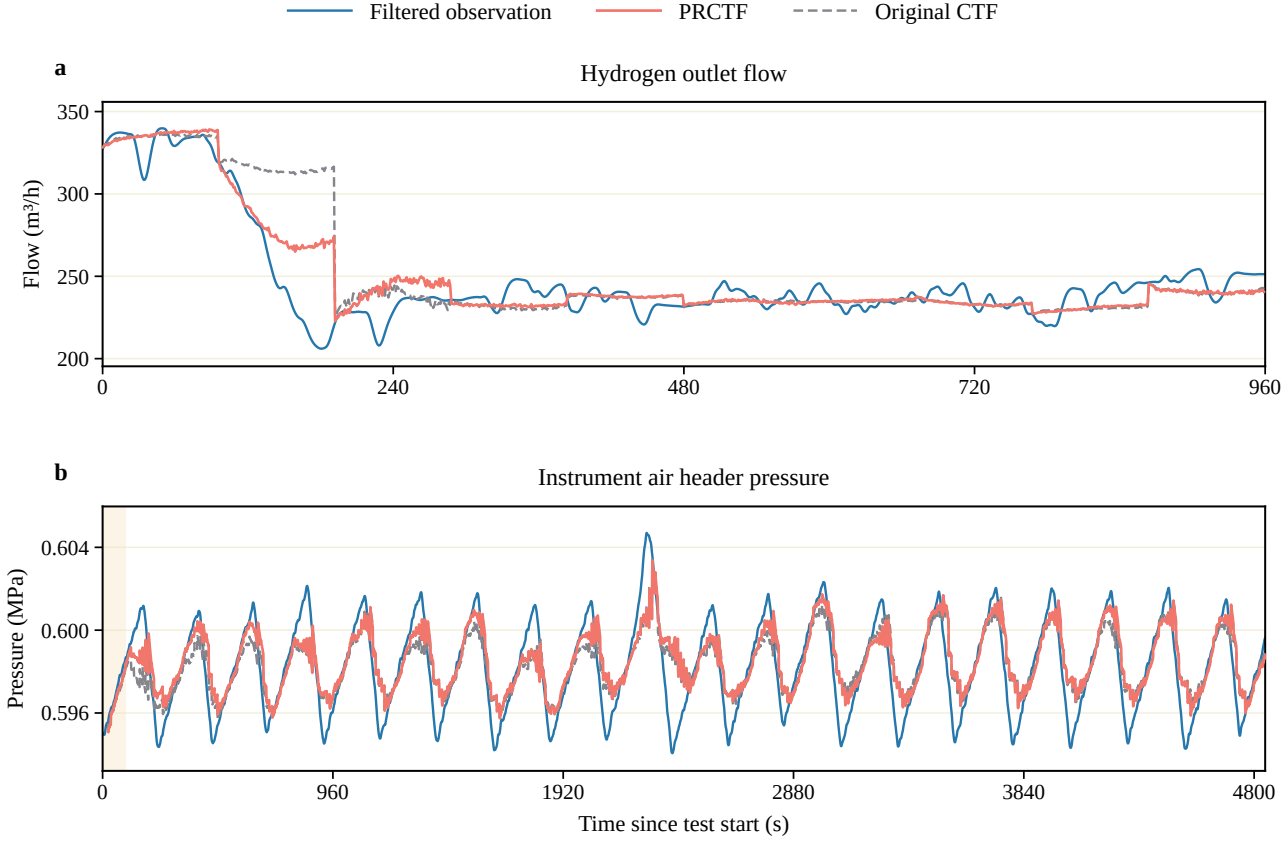

Filtered observation
PRCTF
Original CTF
a
Hydrogen outlet flow
Flow (m³/h)
350
300
250
200
0
240
480
720
960
b
Instrument air header pressure
Pressure (MPa)
0.604
0.600
0.596
0
960
1920
2880
3840
4800
Time since test start (s)