ALCOA

THERALIA
TARGETED THERAPEUTICS

Data Integrity Report

Experiment: Nuclease Activity of Staphylococcus aureus with different TTprobes

Date: 01.02.2022

By: Baris Ata Borsa

APPROVED by Frank J. Hernandez, 2026-03-31 19:44

ALCOA

Experimental Conditions

Recording Report (96-Well Plate Reader)

Experiment Overview:

- **Study Title:** Nuclease Activity of Staphylococcus aureus with different TTprobes
- **Experiment Date and time:** February 01, 2022 at 9:15AM.
- **Laboratory:** Microbiology Lab at 2E:686
- **Type of Lab:** BSL-2
- **Lab Technician:** Baris Ata Borsa
- **Plate Reader Model:** BioTek Cytation
- **Software:** Gen5
- **Protocol name:** Probe Protocol
- **Excitation Wavelength:** 485 nm
- **Emission Wavelength:** 528 nm
- **Measurement Type:** Fluorescence Intensity

Instrument Settings:

- **Gain:** 35
- **Measurement Time:** 100 ms
- **Temperature:** Room temperature
- **Shaking:** No

APPROVED by Frank J. Hernandez, 2026-03-31 19:44

Samples:

Sample 1: TSB
Sample 2: Micrococcal Nuclease (1U/µL)
Sample 3: Culture supernatant of *Staphylococcus aureus ATCC29213*
Sample 4: Culture supernatant of *Staphylococcus epidermidis ATCC35984*

Probes:

Probe 1: *TT Probe Original*
Probe 2: *TT Probe2*

ALCOA

Data acquisition:

Plate Layout (96-Well Format):

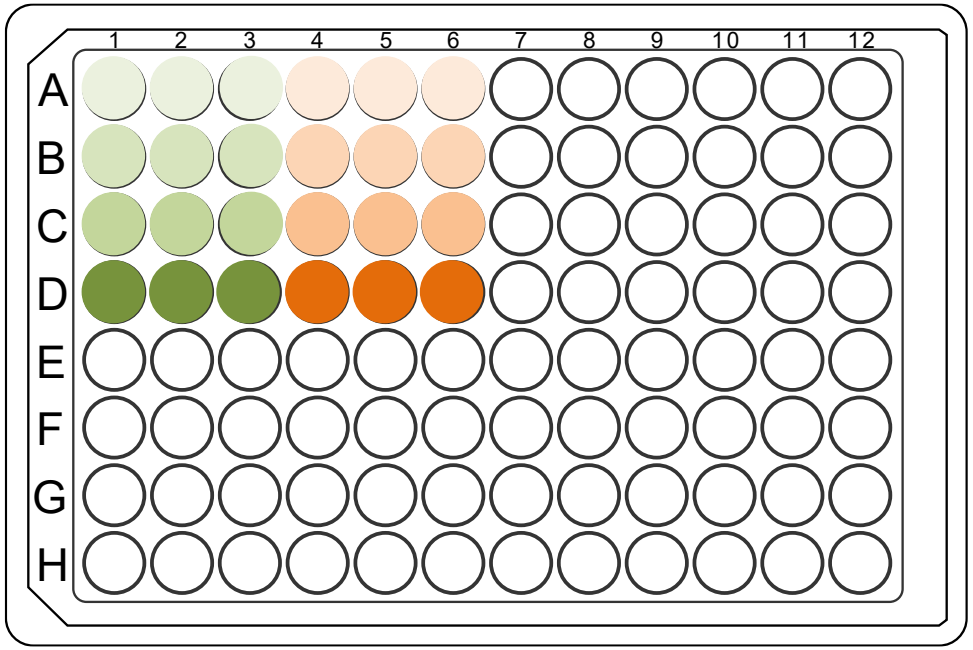

Raw Data

	1	2	3	4	5	6	7	8	9	10	11	12
A	150500	154500	150200	132400	138500	127800						
B	3182300	3222100	3189600	3053300	3145200	3153300						
C	2096600	2143400	2191400	1981200	2055000	2032000						
D	155600	157600	159000	130000	137800	141300						
E												
F												
G												
H												

Notes: Color codes of the samples

- TSB + TTprobe Original
- MN + TTprobe Original
- S.aureus + TTprobe Original
- S.Epidermidis + TTprobe Original
- TSB + Ttprobe2
- MN + TTprobe2
- S.aureus + TTprobe2
- S.epidermidis + TTprobe2

APPROVED by Frank J. Hernandez, 2026-03-31 19:44

ALCOA

Data& Analysis

Plate Layout (96-Well Format):

To ensure data robustness, I have computed the **mean** and **standard deviation** for the triplicate measurements in each sample. This provides insight into the variability of the fluorescence readings within each sample group.

Mean and Standard Deviation (SD) for Each Condition:

	TTprobe original		TTprobe 2	
Samples	**Mean**	**SD**	**Mean**	**SD**
TBS - Negative Control	151733	2401	132900	5367
MN - Positive Control	3198000	21188	3117267	55545
S. aureus	2143800	47401	2022733	37763
S. epidermidis	157400	1709	136367	5785

APPROVED by Frank J. Hernandez, 2026-03-31 19:44

ALCOA

Fluorescence Data- Plot of Results

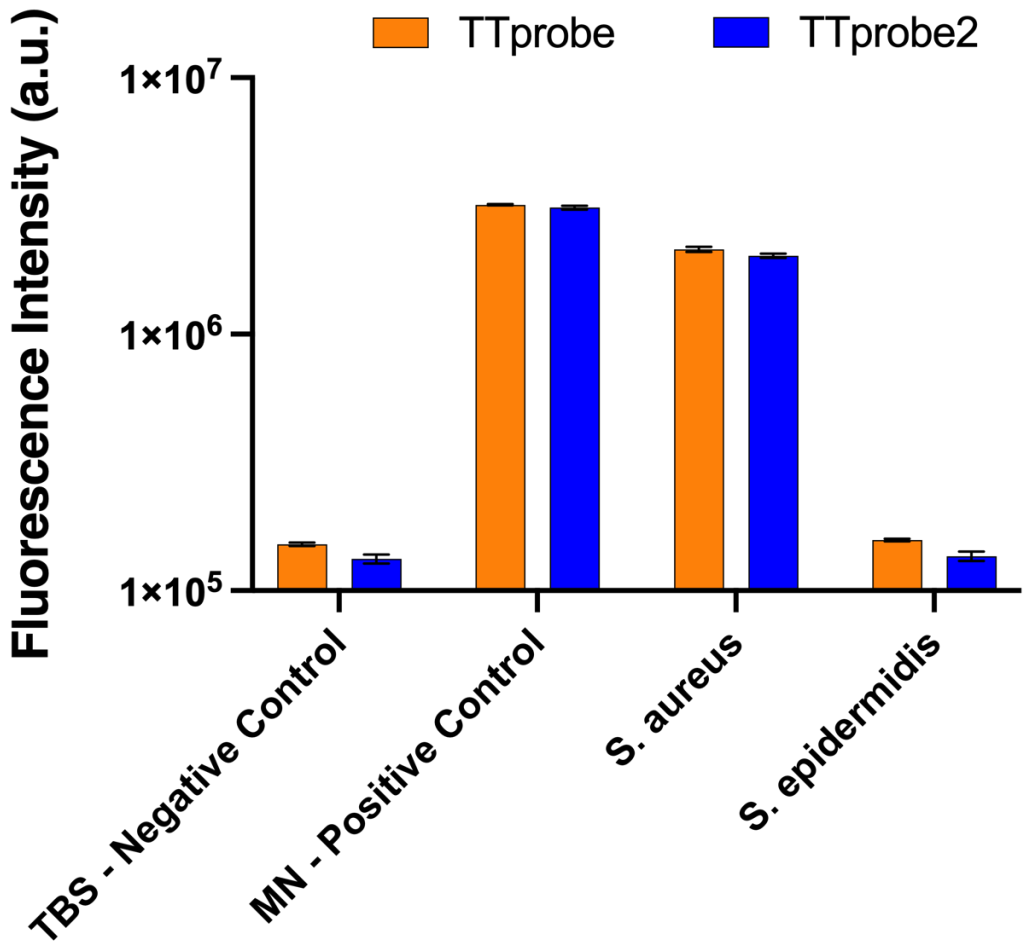

Date: 22/02/02
Signature

Researcher:
Baris Ata Borsa

Date: 22/02/02
Signature

Supervisor:

Date:
22/02/02
Signature

Principal Investig.
Frank J Hernandez

APPROVED by Frank J. Hernandez, 2026-03-31 19:44