09931045A

Description of Non-Environmental Templates



PerkinElmer, 710 Bridgeport Avenue,
Shelton, CT 06484-4794, U.S.A

Produced in the USA.

Template: Accelerants Chroms

ActiveX Plot– “ACTIVE1”


- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 TIC
- Frame Caption: “Total Ion Current”

ActiveX Plot– “ACTIVEX3”

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 Mass chromatogram: 43+57+71+85+99
- Frame Caption: “Alkanes: 43+57+71+85+99”

ActiveX Plot– “ACTIVEX5”

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 Mass chromatogram: 117+131+145+159
- Frame Caption: “Indanes: 117+131+145+159”

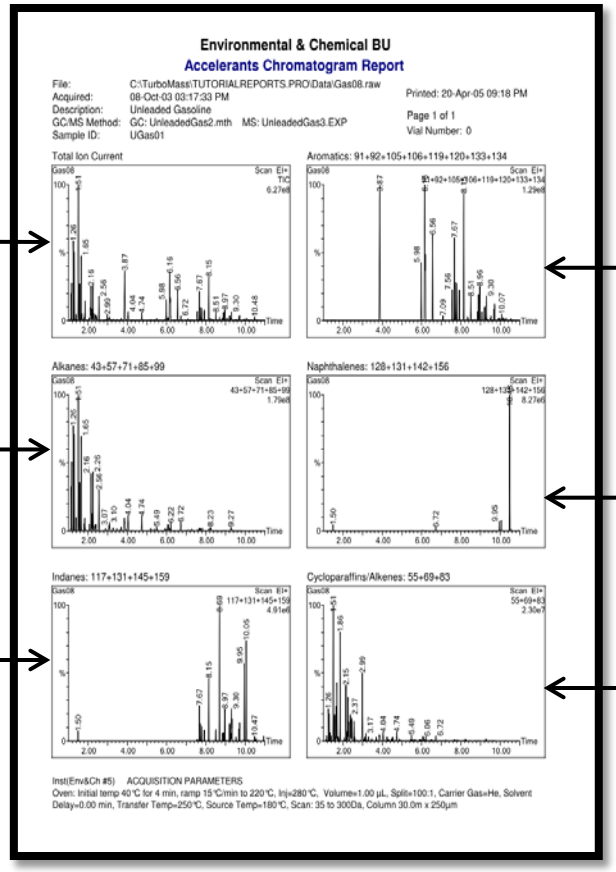

ActiveX Plot– “ACTIVEX2”

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 Mass chromatogram: 91+92+105+106+119+120+133+134
- Frame Caption: “Aromatics: 91+92+105+106+119+120+133+134”

ActiveX Plot– “ACTIVEX4”

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 Mass chromatogram: 128+131+142+156
- Frame Caption: “Naphthalenes: 128+131+142+156”

ActiveX Plot– “ACTIVEX6”

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 Mass chromatogram: 55+69+83
- Frame Caption: “Cycloparaffins/Alkenes: 55+69+83”

Template: Chromatogram


Environmental and Chemical BU

Chromatogram Plot

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix38.raw
Acquired: 02-Oct-03 12:46:13 PM
Description: Standard Text Mix, HCB Int. Std. 5.0 ppm
GC/MS Method: GC: StdMix6.mth MS: stdmix4.EXP
Sample ID: Std. Mix 5.1

Printed: 20-Apr-05 09:18 PM
Page 1 of 1

Vial Number: 13

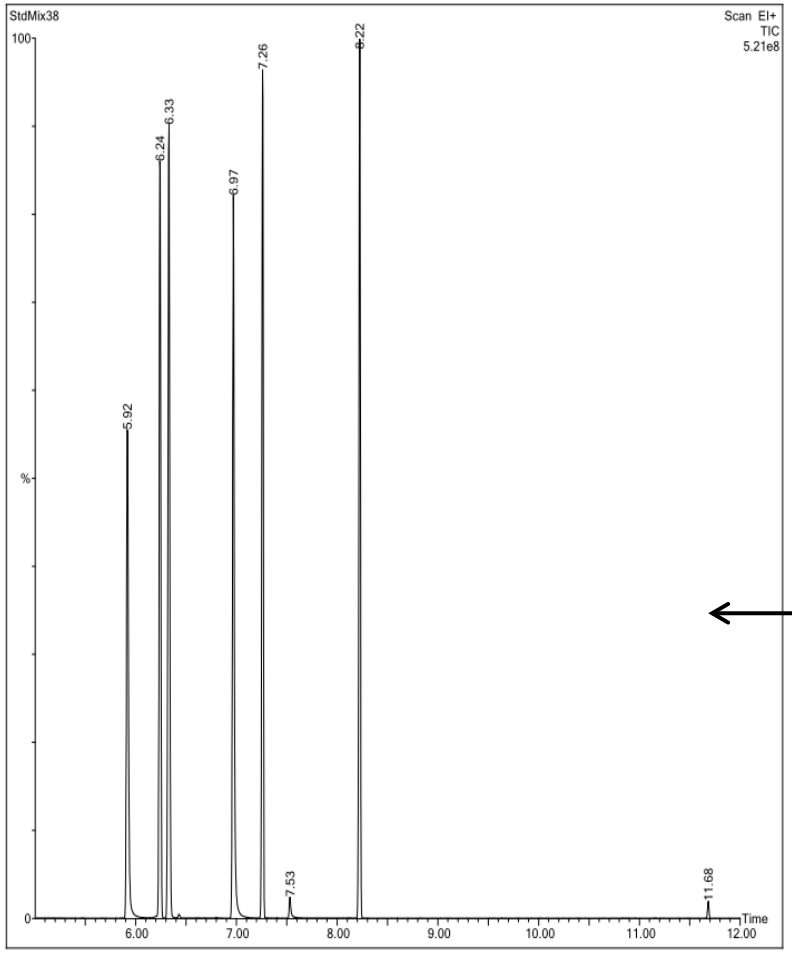


Inst(E&C BU #5) ACQUISITION PARAMETERS
Oven: Initial temp 45°C for 1 min, ramp 15°C/min to 205°C, hold 0.33 min, InjAauto=250°C, Volume=1.00 µL, Split=0:1, Carrier Gas=He, Solvent Delay=4.50 min, Transfer Temp=250°C, Source Temp=180°C, Scan: 45 to 300Da, Column 30.0m x 250µm

ActiveX Plot– "ActiveX1"

- Source: Project.Samples(Last). Chromatogram
- Data set to Function 1 TIC


Template: Chromatogram_Names

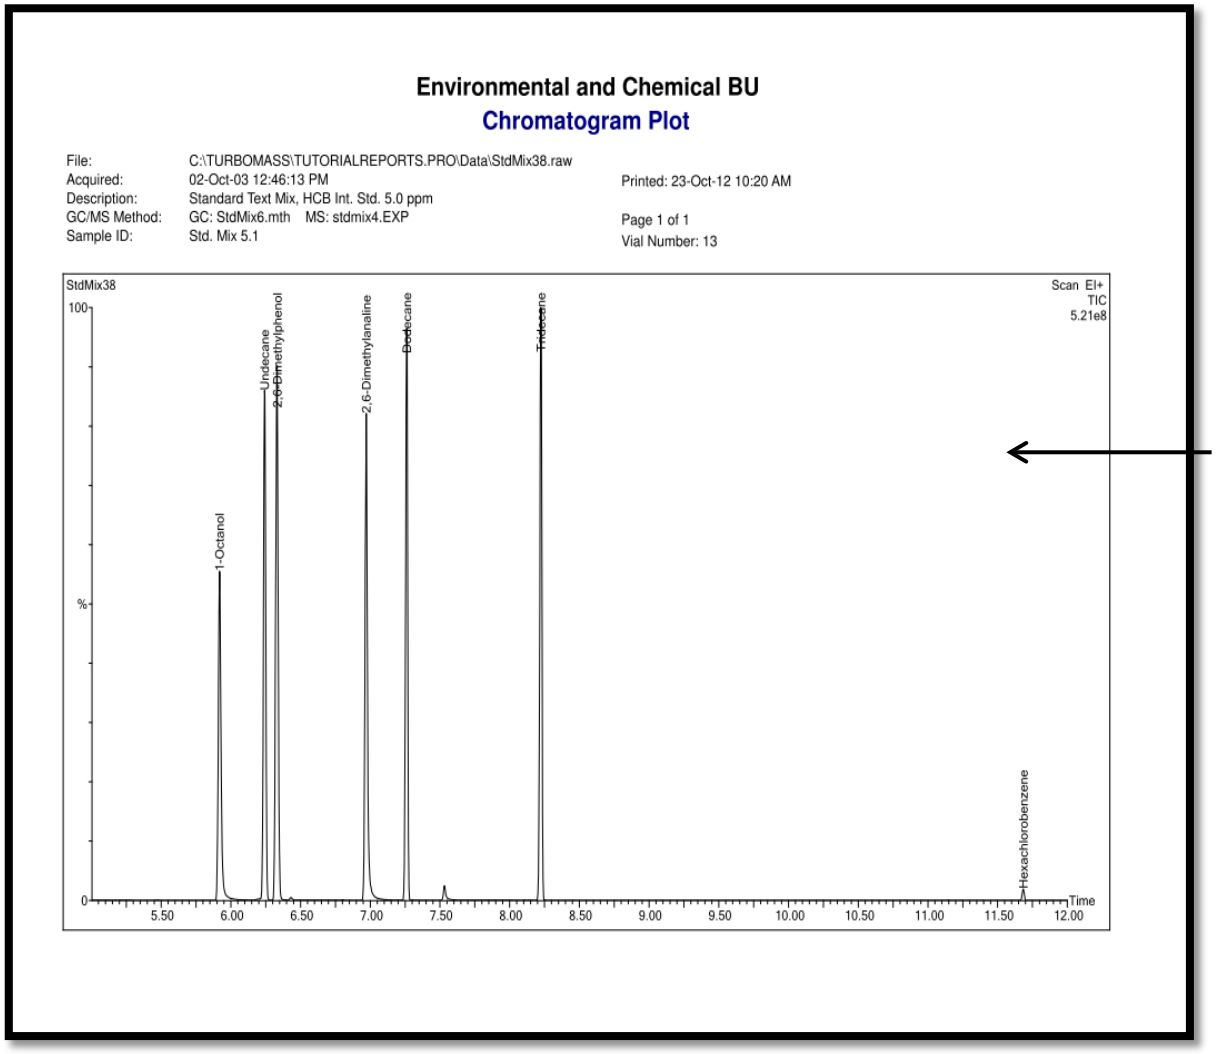

ActiveX Plot– "ActiveX1"

- Source: Project.Samples(Last). Chromatogram
- Data set to Function 1 TIC

Template: Chromatogram-Spectrum Peak Report

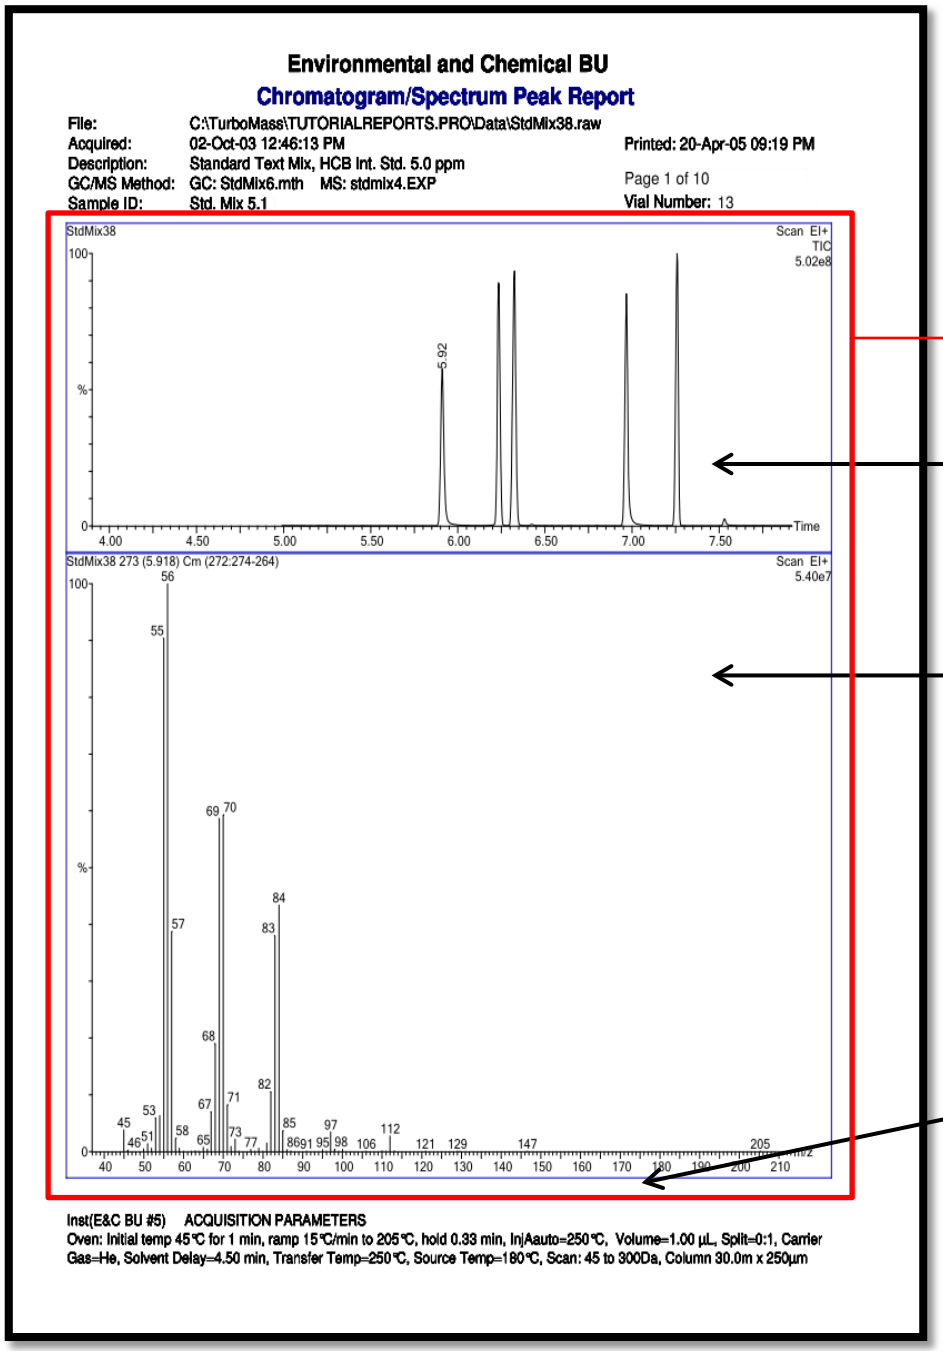

Environmental and Chemical BU

Chromatogram/Spectrum Peak Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix38.raw
Acquired: 02-Oct-03 12:46:13 PM
Printed: 20-Apr-05 09:19 PM
Description: Standard Text Mix, HCB Int. Std. 5.0 ppm
GC/MS Method: GC: StdMix6.mth MS: stdmix4.EXP
Page 1 of 10
Sample ID: Std. Mix 5.1
Vial Number: 13

StdMix38 Scan EI+ TIC 5.02e8

StdMix38 273 (5.918) Cm (272:274-264) Scan EI+ 5.40e7

Inst(E&C BU #5) ACQUISITION PARAMETERS
Oven: Initial temp 45°C for 1 min, ramp 15°C/min to 205°C, hold 0.33 min, InjAauto=250°C, Volume=1.00 µL, Split=0:1, Carrier Gas=He, Solvent Delay=4.50 min, Transfer Temp=250°C, Source Temp=180°C, Scan: 45 to 300Da, Column 30.0m x 250µm

Section – "Section1" with 2 ActiveX Plots

- Repeats based on QualitativePeaks()

ActiveX Plot– "ActiveX1" Chromatogram centered around peak of interest

- Source: Project.Samples(Last).QUalPeaks(Current).QualitativePlot
- Largest peak/baseline at zero/"Time" window 4 minutes

ActiveX Plot– "ActiveX2" mass spectrum at peak of interest

- Source: Project.Samples(Last).QualPeaks(Current).Spectrum
- Background subtracted/Full Scale (0%)


Page Break

Template: Default

Environmental & Chemical BU

Qualitative Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix54.raw
Acquired: 07-Oct-03 06:04:38 PM
Printed: 20-Apr-05 09:19 PM
Description: Unknown, HCB Int. Std.
GC/MS Method: GC: StdMix6.mth MS: stdmix4.EXP
Page 1 of 1
Sample ID: U44366c
Vial Number: 24

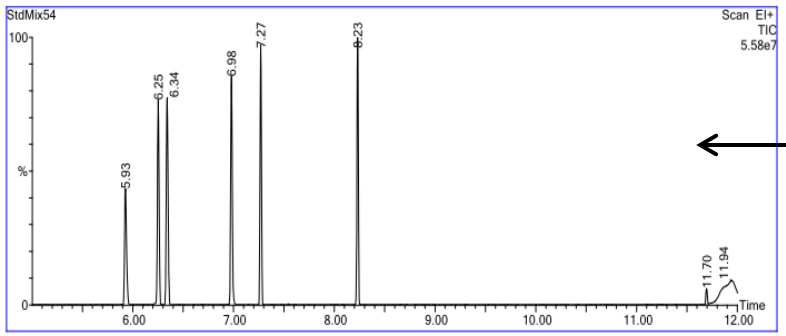

#	RT	Scan	Height	Area	Area %	Norm %	Name	ng/uL
1	5.928	276	24,192,158	561,012.9	11.326	62.99	1-Octanol	0.790
2	6.254	373	42,645,360	819,828.1	16.551	92.05	Undecane	0.726
3	6.342	399	43,043,964	880,686.6	17.780	98.89	2,6-Dimethylphenol	0.770
4	6.981	589	47,653,936	874,483.8	17.655	98.19	2,6-Dimethylanaline	0.792
5	7.270	675	54,236,284	853,243.6	17.226	95.80	Dodecane	0.765
6	7.543	756	174,849	2,204.4	0.045	0.25		
7	8.232	961	55,826,800	890,616.6	17.980	100.00	Tridecane	0.758
8	11.128	1822	84,500	2,308.9	0.047	0.26		
9	11.155	1830	79,453	1,790.6	0.036	0.20		
10	11.696	1991	3,299,444	53,775.3	1.086	6.04	Hexachlorobenzene	2.652

Inst(Env&Ch #5) ACQUISITION PARAMETERS
Oven: Initial temp 45°C for 1 min, ramp 15°C/min to 205°C, hold 0.33 min, InjAauto=250°C, Volume=1.00 µL, Split=0:1, Carrier Gas=He, Solvent Delay=4.50 min, Transfer Temp=250°C, Source Temp=180°C, Scan: 45 to 300Da, Column 30.0m x 250µm

Section – "Chromatogram Plot" containing ActiveX Plot

- Can be turned off in the Report Method
- Does not repeat

ActiveX Plot – "ActiveX1" TIC of sample

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 TIC


Section – "With Quant method" containing Table

- Can be turned off in the Report Method
- Does not repeat

Table – "Table1" Qualitative and quantitative results

- Expands on QualitativePeaks()
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "#"
  2. Text – "RT"
  3. Text – "Scan"
  4. Text – "Height"
  5. Text – "Area"
  6. Text – "Area %"
  7. Text – "Norm %"
  8. Text – "Name"
  9. Project.Samples(Last).Targets(First).ConcUnits
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).QualPeaks(Current).PeakNumber
  2. Project.Samples(Last).QualPeaks(Current).RetentionTime
  3. Project.Samples(Last).QualPeaks(Current).ScanNumber
  4. Project.Samples(Last).QualPeaks(Current).Height
  5. Project.Samples(Last).QualPeaks(Current).Area
  6. Project.Samples(Last).QualPeaks(Current).PercentArea
  7. Project.Samples(Last).QualPeaks(Current).PercentNorm
  8. Project.Samples(Last).QualPeaks(Current).Name
  9. Project.Samples(Last).QualPeaks(Current).Conc

Template: Default CSV

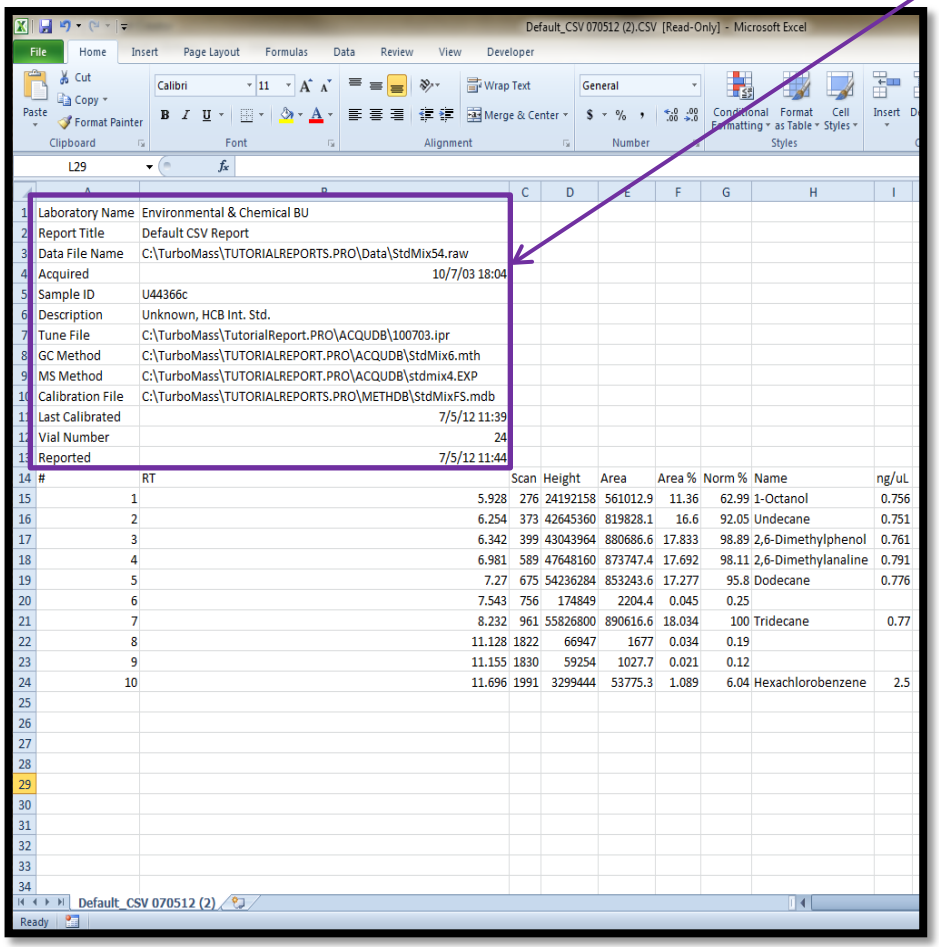


	A	B	C	D	E	F	G	H	I
1	Laboratory Name	Environmental & Chemical BU							
2	Report Title	Default CSV Report							
3	Data File Name	C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix54.raw							
4	Acquired	10/7/03 18:04							
5	Sample ID	U44366c							
6	Description	Unknown, HCB Int. Std.							
7	Tune File	C:\TurboMass\TutorialReport.PRO\ACQUDB\100703.ipr							
8	GC Method	C:\TurboMass\TUTORIALREPORT.PRO\ACQUDB\StdMix6.mth							
9	MS Method	C:\TurboMass\TUTORIALREPORT.PRO\ACQUDB\stdmix4.EXP							
10	Calibration File	C:\TurboMass\TUTORIALREPORTS.PRO\METHDB\StdMixFS.mdb							
11	Last Calibrated	7/5/12 11:39							
12	Vial Number	24							
13	Reported	7/5/12 11:44							
14	#	RT	Scan	Height	Area	Area %	Norm %	Name	ng/uL
15	1	5.928	276	24192158	561012.9	11.36	62.99	1-Octanol	0.756
16	2	6.254	373	42645360	819828.1	16.6	92.05	Undecane	0.751
17	3	6.342	399	43043964	880686.6	17.833	98.89	2,6-Dimethylphenol	0.761
18	4	6.981	589	47648160	873747.4	17.692	98.11	2,6-Dimethylanaline	0.791
19	5	7.27	675	54236284	853243.6	17.277	95.8	Dodecane	0.776
20	6	7.543	756	174849	2204.4	0.045	0.25		
21	7	8.232	961	55826800	890616.6	18.034	100	Tridecane	0.77
22	8	11.128	1822	66947	1677	0.034	0.19		
23	9	11.155	1830	59254	1027.7	0.021	0.12		
24	10	11.696	1991	3299444	53775.3	1.089	6.04	Hexachlorobenzene	2.5

Table – "Table1" Sample information

- Does not expand
- No filtering/sorting/grouping
- Data items for 1st column (by row number):
  1. Text – "Laboratory Name"
  2. Text – "Report Title"
  3. Text – "Data File Name"
  4. Text – "Acquired"
  5. Text – "Sample ID"
  6. Text – "Description"
  7. Text – "Tune File"
  8. Text – "GC Method"
  9. Text – "MS Method"
  10. Text – "Calibration File"
  11. Text – "Last Calibrated"
  12. Text – "Vial Number"
  13. Text – "Reported"
- Data items for 2nd Column (by row number):
  1. Project.Samples(Last).Data.LabName
  2. Text – "Default CSV Report"
  3. Project.Samples(Last).Data.Path
  4. Project.Samples(Last).Data.ModifyDateTime
  5. Project.Samples(Last).Data.SampleID
  6. Project.Samples(Last).Data.SamleDesc
  7. Project.Samples(Last).Instr.Path + Project.Samples(Last).Instr.Filename
  8. Project.Samples(Last).GCMethod.Fullname
  9. Project.Samples(Last).MSMethod.Fullname
  10. Project.Samples(Last).QuantMethod.Fullname
  11. Project.Samples(Last).QuantMethod.ModifyDateTime
  12. Project.Samples(Last).Data.VialNumber
  13. System – Miscellaneous – Date Time Report

(Continued to next page)

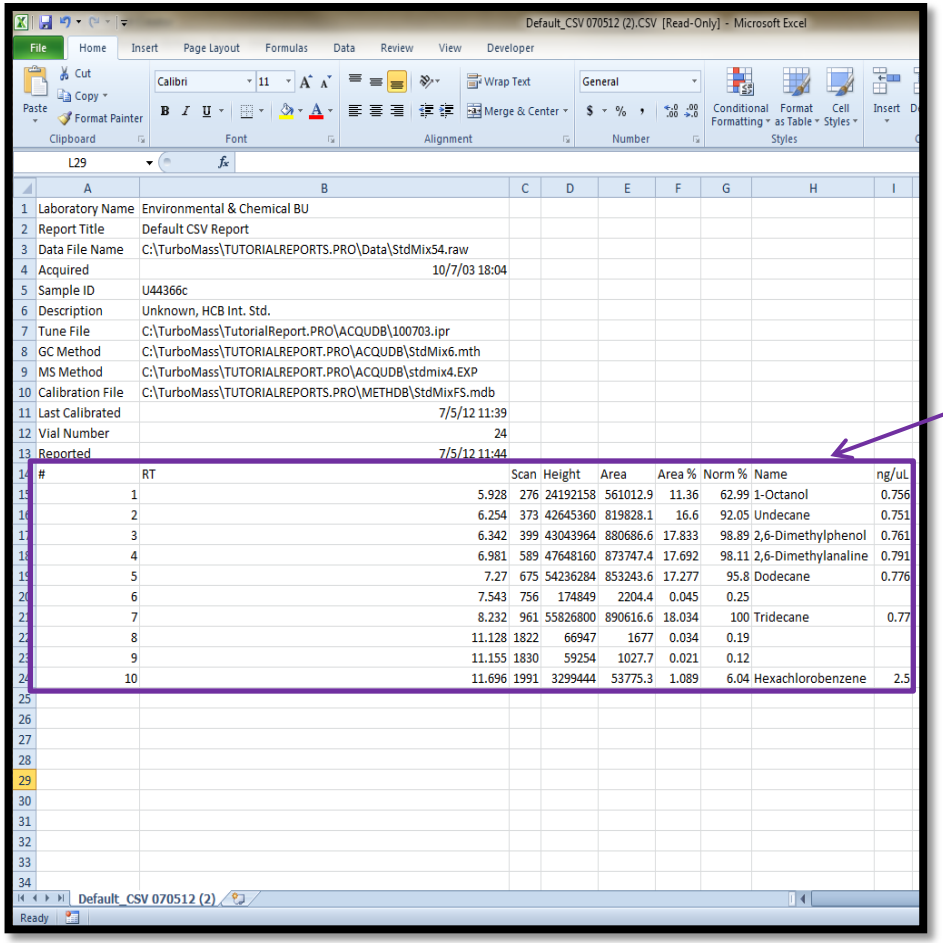


	A	B	C	D	E	F	G	H	I
1	Laboratory Name	Environmental & Chemical BU							
2	Report Title	Default CSV Report							
3	Data File Name	C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix54.raw							
4	Acquired	10/7/03 18:04							
5	Sample ID	U44366c							
6	Description	Unknown, HCB Int. Std.							
7	Tune File	C:\TurboMass\TutorialReport.PRO\ACQUDB\100703.ipr							
8	GC Method	C:\TurboMass\TUTORIALREPORT.PRO\ACQUDB\StdMix6.mth							
9	MS Method	C:\TurboMass\TUTORIALREPORT.PRO\ACQUDB\stdmix4.EXP							
10	Calibration File	C:\TurboMass\TUTORIALREPORTS.PRO\METHDB\StdMixFS.mdb							
11	Last Calibrated	7/5/12 11:39							
12	Vial Number	24							
13	Reported	7/5/12 11:44							
14	#	RT	Scan	Height	Area	Area %	Norm %	Name	ng/uL
15	1	5.928	276	24192158	561012.9	11.36	62.99	1-Octanol	0.756
16	2	6.254	373	42645360	819828.1	16.6	92.05	Undecane	0.751
17	3	6.342	399	43043964	880686.6	17.833	98.89	2,6-Dimethylphenol	0.761
18	4	6.981	589	47648160	873747.4	17.692	98.11	2,6-Dimethylanaline	0.791
19	5	7.27	675	54236284	853243.6	17.277	95.8	Dodecane	0.776
20	6	7.543	756	174849	2204.4	0.045	0.25		
21	7	8.232	961	55826800	890616.6	18.034	100	Tridecane	0.77
22	8	11.128	1822	66947	1677	0.034	0.19		
23	9	11.155	1830	59254	1027.7	0.021	0.12		
24	10	11.696	1991	3299444	53775.3	1.089	6.04	Hexachlorobenzene	2.5
25									
26									
27									
28									
29									
30									
31									
32									
33									
34									

Table – "Table2" Qualitative and quantitative results

- Expands base on QualitativePeaks()
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "#"
  2. Text – "RT"
  3. Text – "Scan"
  4. Text – "Height"
  5. Text – "Area"
  6. Text – "Area %"
  7. Text – "Norm %"
  8. Text – "Name"
  9. Project.Samples(Last).Targets(First).ConcUnits
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).QualPeaks(Current).PeakNumber
  2. Project.Samples(Last).QualPeaks(Current).RetentionTime
  3. Project.Samples(Last).QualPeaks(Current).ScanNumber
  4. Project.Samples(Last).QualPeaks(Current). Height
  5. Project.Samples(Last).QualPeaks(Current).Area
  6. Project.Samples(Last).QualPeaks(Current).PercentArea
  7. Project.Samples(Last).QualPeaks(Current).PercentNorm
  8. Project.Samples(Last).QualPeaks(Current).Name
  9. Project.Samples(Last).QualPeaks(Current).Conc

Template: Integration Summary Report 1-24, 1-48, 1-72, 1-96

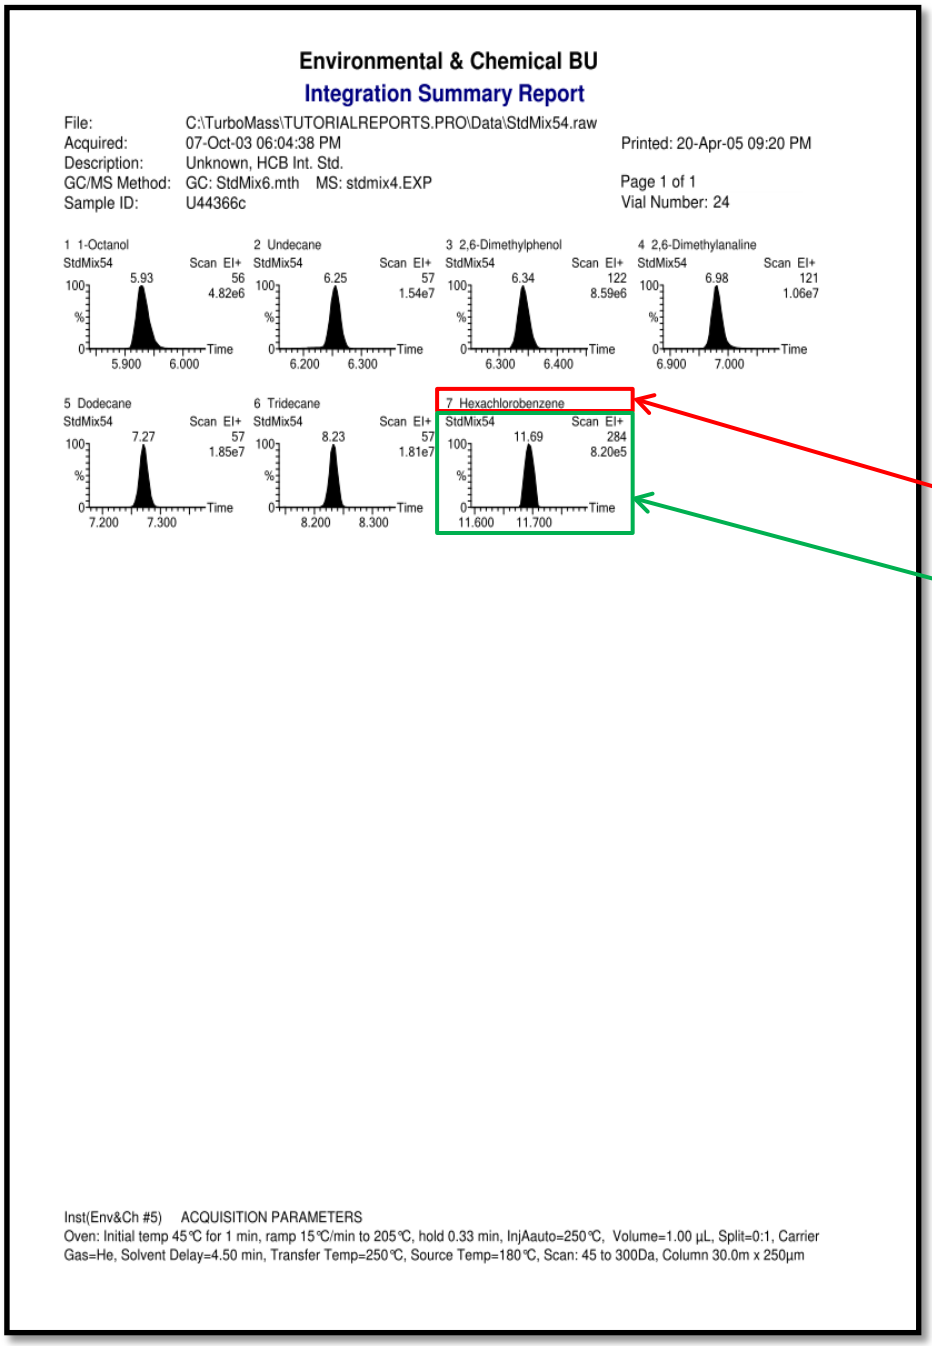

Environmental & Chemical BU

Integration Summary Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix54.raw
Acquired: 07-Oct-03 06:04:38 PM
Printed: 20-Apr-05 09:20 PM
Description: Unknown, HCB Int. Std.
GC/MS Method: GC: StdMix6.mth MS: stdmix4.EXP
Page 1 of 1
Sample ID: U44366c
Vial Number: 24

1 1-Octanol — StdMix54 — Scan EI+ 56 — 4.82e6 — 5.93
2 Undecane — StdMix54 — Scan EI+ 57 — 1.54e7 — 6.25
3 2,6-Dimethylphenol — StdMix54 — Scan EI+ 122 — 8.59e6 — 6.34
4 2,6-Dimethylanaline — StdMix54 — Scan EI+ 121 — 1.06e7 — 6.98
5 Dodecane — StdMix54 — Scan EI+ 57 — 1.85e7 — 7.27
6 Tridecane — StdMix54 — Scan EI+ 57 — 1.81e7 — 8.23
7 Hexachlorobenzene — StdMix54 — Scan EI+ 284 — 8.20e5 — 11.69

Inst(Env&Ch #5) ACQUISITION PARAMETERS
Oven: Initial temp 45℃ for 1 min, ramp 15℃/min to 205℃, hold 0.33 min, InjAauto=250℃, Volume=1.00 µL, Split=0:1, Carrier Gas=He, Solvent Delay=4.50 min, Transfer Temp=250℃, Source Temp=180℃, Scan: 45 to 300Da, Column 30.0m x 250µm

"1-24" is a 4x6 Matrix of ActiveX Plots

"1-48", "1-72", and "1-96" are identical to "1-24" however have two, three and four additional pages, respectively, of the 4x6 matrix template pages.


- Additional pages have the same header/footer

Individual Structure

- **Text Label**
  - Project.Samples(Last).Targets(#).CompoundNum
  - Project.Samples(Last). Targets(#).Name
- **ActiveX Plot – "ActiveX#"**
  - Project.Samples(Last).Targets(#).PeakPlot
  - Data: Target compound – Quantify trace

Note: Empty plots/text will not show up (as for compounds 8-24 in example at left)
Note: # is hard coded into template from 1-24 (-72, etc…)

Template: Ion Ratio Intg Summary

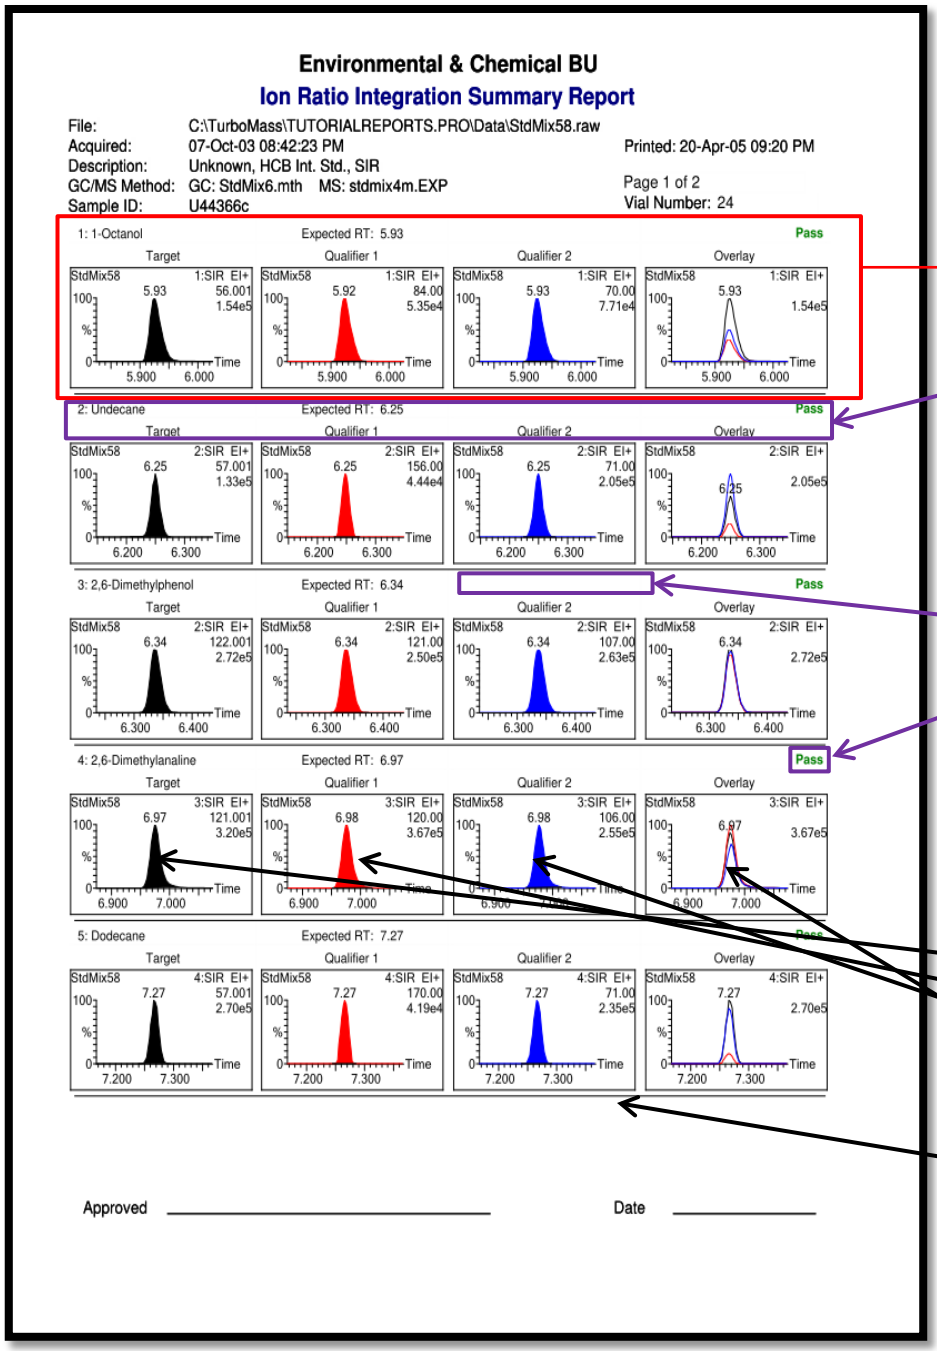

Section – "Section1" containing Table , 4 ActiveX Plots, and Horizontal Line

- Repeats based on: Target Compounds()

Table – "Table1"

- Does not expand
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Project.Samples(Last).Targets(Current).CompoundNum
     Project.Samples(Last).Targets(Current).Name
  2. Text – "Expected RT:" +
     Project.Samples(Last).Targets(Current).ExpectedTime
  3. EQUATION: "IonRatiosOverride"
  4. EQUATION: "CompoundPassFail"
- Data items for 2nd Row (by column number):
  1. Text – "Target"
  2. Text – "Qualifier 1"
  3. Text – "Qualifier 2"
  4. Text – "Overlay"

ActiveX Plots – "ActiveX1-4"

- Source: Project.Samples(Last).Targets(Current).PeakPlot
- Data (from left to right):
  1. Target compound – Quantify Trace
  2. Target compound – Qualifier Ion 1
  3. Target compound – Qualifier Ion 2
  4. Target compound – Overlay Quantify trace and Qualifier Ions

Horizontal Line

(Continued to next page)

Environmental & Chemical BU

Ion Ratio Integration Summary Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix58.raw
Acquired: 07-Oct-03 08:42:23 PM
Printed: 20-Apr-05 09:20 PM
Description: Unknown, HCB Int. Std., SIR
GC/MS Method: GC: StdMix6.mth MS: stdmix4m.EXP
Sample ID: U44366c
Page 1 of 2
Vial Number: 24

1: 1-Octanol — Expected RT: 5.93 — Pass

Target	Qualifier 1	Qualifier 2	Overlay
StdMix58 1:SIR EI+	StdMix58 1:SIR EI+	StdMix58 1:SIR EI+	StdMix58 1:SIR EI+
5.93 56.001 1.54e5	5.92 84.00 5.35e4	5.93 70.00 7.71e4	5.93 1.54e5

2: Undecane — Expected RT: 6.25 — Pass

Target	Qualifier 1	Qualifier 2	Overlay
StdMix58 2:SIR EI+	StdMix58 2:SIR EI+	StdMix58 2:SIR EI+	StdMix58 2:SIR EI+
6.25 57.001 1.33e5	6.25 156.00 4.44e4	6.25 71.00 2.05e5	6.25 2.05e5

3: 2,6-Dimethylphenol — Expected RT: 6.34 — Pass

Target	Qualifier 1	Qualifier 2	Overlay
StdMix58 2:SIR EI+	StdMix58 2:SIR EI+	StdMix58 2:SIR EI+	StdMix58 2:SIR EI+
6.34 122.001 2.72e5	6.34 121.00 2.50e5	6.34 107.00 2.63e5	6.34 2.72e5

4: 2,6-Dimethylanaline — Expected RT: 6.97 — Pass


Target	Qualifier 1	Qualifier 2	Overlay
StdMix58 3:SIR EI+	StdMix58 3:SIR EI+	StdMix58 3:SIR EI+	StdMix58 3:SIR EI+
6.97 121.001 3.20e5	6.98 120.00 3.67e5	6.98 106.00 2.55e5	6.97 3.67e5

5: Dodecane — Expected RT: 7.27 — Pass

Target	Qualifier 1	Qualifier 2	Overlay
StdMix58 4:SIR EI+	StdMix58 4:SIR EI+	StdMix58 4:SIR EI+	StdMix58 4:SIR EI+
7.27 57.001 2.70e5	7.27 170.00 4.19e4	7.27 71.00 2.35e5	7.27 2.70e5


Approved _____ Date _____

Equation – "IonRatiosOverride"

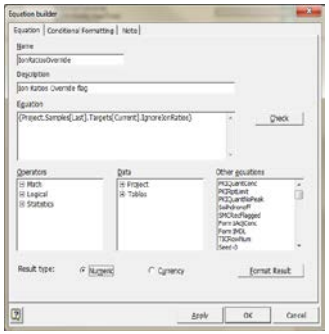




Equation – "CompoundPassFail"

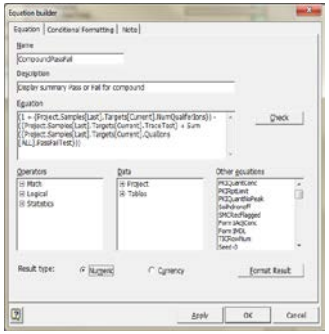



Template: LibSearch 3

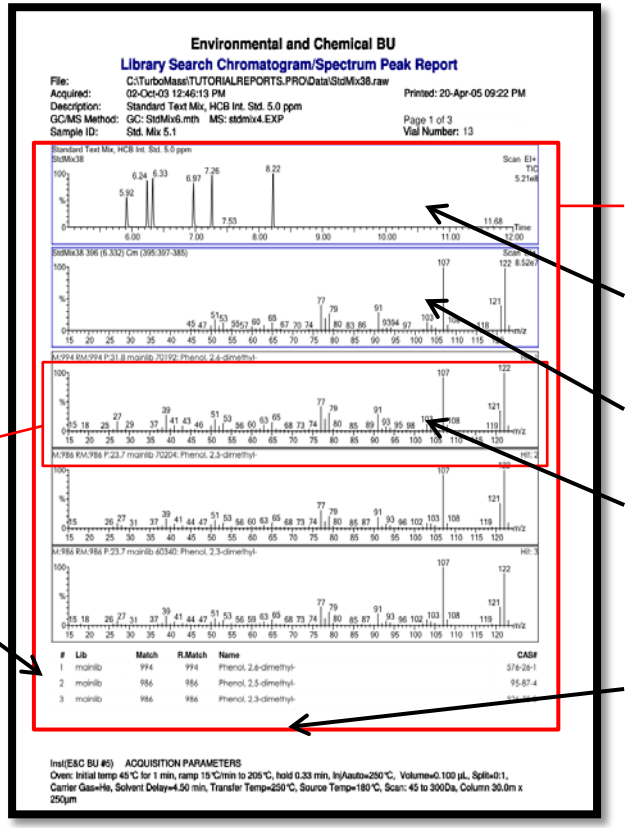

Section – "Section" containing 2 ActiveX Plots, Table, a sub-section and Page Break

- Repeats based on: QualitativePeaks()

ActiveX Plot – "ActiveX1" (Chromatogram showing entire data set)

- Source: Project.Samples(Last).Chromatogram
- Data: Function 1 TIC

ActiveX Plot – "ActiveX3" (Spectrum showing peak of interest)

- Source: Project.Samples(Last).QualPeaks(Current).Spectrum

ActiveX Plot – "ActiveX2" (Library Hit Spectra – recommended to use 3 only)

- Source: Project.Samples(Last).QualPeaks(Current).PlotHits(Current).Spectrum

Page Break

Section – "Section2" containing ActiveX Plot

- Repeats based on PlotHits()

Table – "Table1"

- Expands on TextHits()
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "#"
  2. Text – "Lib"
  3. Text – "Match"
  4. Text – "R.Match"
  5. Text – "Name"
  6. Text – ""CAS #
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).QualPeaks(Current).TextHits(Current).HitRank
  2. Project.Samples(Last).QualPeaks(Current).TextHits(Current).Library
  3. Project.Samples(Last). QualPeaks(Current).TextHits(Current).MatchFactor
  4. Project.Samples(Last).QualPeaks(Current).TextHits(Current).RevMatchFactor
  5. Project.Samples(Last).QualPeaks(Current).TextHits(Current).Name
  6. Project.Samples(Last).QualPeaks(Current).TextHits(Current).CAS

Template: LibSearch Text

Environmental & Chemical BU

Library Search Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\Gas08.raw
Acquired: 08-Oct-03 03:17:33 PM Printed: 20-Apr-05 09:23 PM
Description: Unleaded Gasoline
GC/MS Method: GC: UnleadedGas2.mth MS: UnleadedGas3.EXP Page 1 of 2
Sample ID: UGas01 Vial Number: 0

Pk #	RT	Hit	Compound Name	Match	R.Match	Prob.	CAS	Library
1	1.257	1	Butane, 2-methyl-	962	962	79.2	78-78-4	replib
		2	Butane, 2-methyl-	959	963	79.2	78-78-4	mainlib
		3	Butane, 2-methyl-	958	958	79.2	78-78-4	replib
		4	Pentane	911	911	16.0	109-66-0	replib
		5	Pentane	880	884	16.0	109-66-0	mainlib
2	1.304	1	Pentane	957	957	86.6	109-66-0	replib
		2	Pentane	956	956	86.6	109-66-0	replib
		3	Pentane	952	960	86.6	109-66-0	replib
		4	Pentane	943	947	86.6	109-66-0	mainlib
		5	Pentane	933	935	86.6	109-66-0	replib
3	1.514	1	Propane, 2-methoxy-2-methyl-	811	827	23.0	1634-04-4	mainlib
		2	Propane, 2-methoxy-2-methyl-	807	823	23.0	1634-04-4	replib
		3	2-Methyl-5-hexen-3-ol	804	819	17.6	32815-70-6	mainlib
		4	Propane, 2-methoxy-2-methyl-	794	811	23.0	1634-04-4	replib
		5	3-Pentanol, 2,4-dimethyl-	789	789	10.7	600-36-2	replib
4	1.654	1	Hexane	958	963	82.6	110-54-3	mainlib
		2	Hexane	949	949	82.6	110-54-3	replib
		3	Hexane	948	950	82.6	110-54-3	replib
		4	Pentane, 3-methyl-	868	868	7.1	96-14-0	replib
		5	Pentane, 3-methyl-	851	856	7.1	96-14-0	replib
5	2.160	1	Hexane, 2-methyl-	905	906	47.2	591-76-4	replib
		2	Hexane, 2-methyl-	900	900	47.2	591-76-4	replib
		3	Hexane, 2-methyl-	886	887	47.2	591-76-4	mainlib
		4	Hexane, 2,4-dimethyl-	854	854	9.5	589-43-5	mainlib
		5	Heptane, 3-methyl-	838	851	5.5	589-81-1	replib
6	2.257	1	Hexane, 3-methyl-	920	920	54.8	589-34-4	mainlib
		2	Hexane, 3-methyl-	910	919	54.8	589-34-4	replib
		3	Hexane, 3-methyl-	893	893	54.8	589-34-4	replib
		4	Heptane, 3,4-dimethyl-	890	890	15.2	922-28-1	replib
		5	Heptane, 3,4-dimethyl-	873	873	15.2	922-28-1	mainlib
7	3.871	1	Toluene	920	935	50.5	108-88-3	replib
		2	Toluene	900	914	50.5	108-88-3	replib

Inst(Env&Ch #5) ACQUISITION PARAMETERS
Oven: Initial temp 40℃ for 4 min, ramp 15℃/min to 220℃, Inj=280℃, Volume=1.00 µL, Split=100:1, Carrier Gas=He, Solvent Delay=0.00 min, Transfer Temp=250℃, Source Temp=180℃, Scan: 35 to 300Da, Column 30.0m x 250µm

Table – "Table1"

- Expands on QualitativePeaks() & TextHits().
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "Pk #"
  2. Text – "RT"
  3. Text – "Hit"
  4. Text – "Compound Name"
  5. Text – "Match"
  6. Text – "R.Match"
  7. Text – "Prob."
  8. Text – "CAS"
  9. Text – "Library"
- Data items for 2nd Row (by column number):
  1. EQUATION: "Show Peaknumber if Hit 1"
  2. EQUATION: "Show RT if Hit 1"
  3. Project.Samples(Last).QualPeaks(Current).TextHits(Current).HitRank
  4. Project.Samples(Last).QualPeaks(Current).TextHits(Current).Name
  5. Project.Samples(Last).QualPeaks(Current).TextHits(Current).MatchFactor
  6. Project.Samples(Last).QualPeaks(Current).TextHits(Current).RevMatchFactor
  7. Project.Samples(Last).QualPeaks(Current).TextHits(Current).Score
  8. Project.Samples(Last).QualPeaks(Current).TextHits(Current).CAS
  9. Project.Samples(Last).QualPeaks(Current).TextHits(Current).Library

(Continued to next page)

Environmental & Chemical BU


Library Search Report


File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\Gas08.raw
Acquired: 08-Oct-03 03:17:33 PM Printed: 20-Apr-05 09:23 PM
Description: Unleaded Gasoline
GC/MS Method: GC: UnleadedGas2.mth MS: UnleadedGas3.EXP Page 1 of 2
Sample ID: UGas01 Vial Number: 0

Pk #	RT	Hit	Compound Name	Match	R.Match	Prob.	CAS	Library
1	1.257	1	Butane, 2-methyl-	962	962	79.2	78-78-4	replib
		2	Butane, 2-methyl-	959	963	79.2	78-78-4	mainlib
		3	Butane, 2-methyl-	958	958	79.2	78-78-4	replib
		4	Pentane	911	911	16.0	109-66-0	replib
		5	Pentane	880	884	16.0	109-66-0	mainlib
2	1.304	1	Pentane	957	957	86.6	109-66-0	replib
		2	Pentane	956	956	86.6	109-66-0	replib
		3	Pentane	952	960	86.6	109-66-0	replib
		4	Pentane	943	947	86.6	109-66-0	mainlib
		5	Pentane	933	935	86.6	109-66-0	replib
3	1.514	1	Propane, 2-methoxy-2-methyl-	811	827	23.0	1634-04-4	mainlib
		2	Propane, 2-methoxy-2-methyl-	807	823	23.0	1634-04-4	replib
		3	2-Methyl-5-hexen-3-ol	804	819	17.6	32815-70-6	mainlib
		4	Propane, 2-methoxy-2-methyl-	794	811	23.0	1634-04-4	replib
		5	3-Pentanol, 2,4-dimethyl-	789	789	10.7	600-36-2	replib
4	1.654	1	Hexane	958	963	82.6	110-54-3	mainlib
		2	Hexane	949	949	82.6	110-54-3	replib
		3	Hexane	948	950	82.6	110-54-3	replib
		4	Pentane, 3-methyl-	868	868	7.1	96-14-0	replib
		5	Pentane, 3-methyl-	851	856	7.1	96-14-0	replib
5	2.160	1	Hexane, 2-methyl-	905	906	47.2	591-76-4	replib
		2	Hexane, 2-methyl-	900	900	47.2	591-76-4	replib
		3	Hexane, 2-methyl-	886	887	47.2	591-76-4	mainlib
		4	Hexane, 2,4-dimethyl-	854	854	9.5	589-43-5	mainlib
		5	Heptane, 3-methyl-	838	851	5.5	589-81-1	replib
6	2.257	1	Hexane, 3-methyl-	920	920	54.8	589-34-4	mainlib
		2	Hexane, 3-methyl-	910	919	54.8	589-34-4	replib
		3	Hexane, 3-methyl-	893	893	54.8	589-34-4	replib
		4	Heptane, 3,4-dimethyl-	890	890	15.2	922-28-1	replib
		5	Heptane, 3,4-dimethyl-	873	873	15.2	922-28-1	mainlib
7	3.871	1	Toluene	920	935	50.5	108-88-3	replib
		2	Toluene	900	914	50.5	108-88-3	replib

Inst(Env&Ch #5) ACQUISITION PARAMETERS
Oven: Initial temp 40℃ for 4 min, ramp 15℃/min to 220℃, Inj=280℃, Volume=1.00 µL, Split=100:1, Carrier Gas=He, Solvent Delay=0.00 min, Transfer Temp=250℃, Source Temp=180℃, Scan: 35 to 300Da, Column 30.0m x 250µm

Equation – "Show Peaknumber if Hit 1"

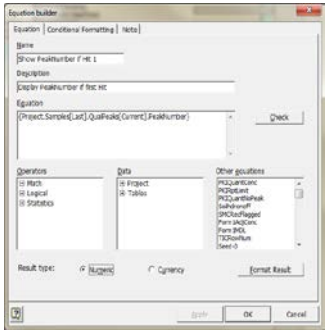


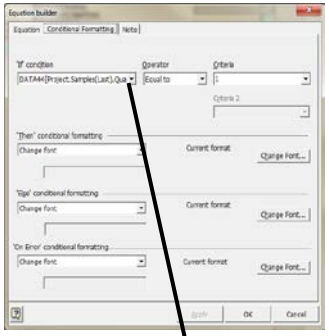

DATA44[Project.Samples(Last).QualPeaks(Current).TextHits(Current).HitRank]

Equation – "Show RT if Hit 1"



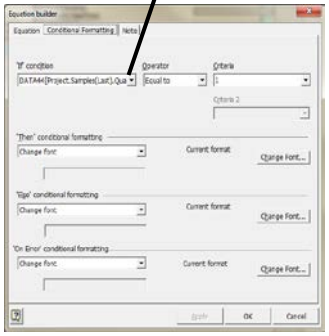

Template: Qualitative Report


Environmental & Chemical BU

Qualitative Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\Gas08.raw
Acquired: 08-Oct-03 03:17:33 PM
Description: Unleaded Gasoline
GC/MS Method: GC: UnleadedGas2.mth MS: UnleadedGas3.EXP
Sample ID: UGas01

Printed: 20-Apr-05 09:25 PM

Page 1 of 4
Vial Number: 0

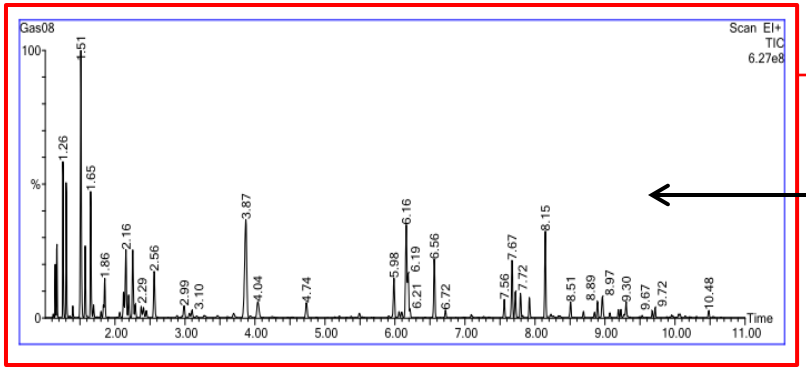

#	RT	Scan	Height	Area	Area %	Norm %
1	1.118	28	8,296,956	89,551.4	0.106	0.85
2	1.148	35	122,296,288	1,099,062.9	1.307	10.45
3	1.173	41	168,598,496	1,812,455.8	2.155	17.24
4	1.257	61	364,566,368	4,141,580.8	4.924	39.39
5	1.304	72	313,796,704	3,636,888.0	4.324	34.59
6	1.354	84	3,505,060	40,612.2	0.048	0.39
7	1.401	95	27,168,838	308,633.5	0.367	2.94
8	1.472	112	724,034	5,671.9	0.007	0.05
9	1.514	122	626,368,896	10,513,787.0	12.500	100.00
10	1.573	136	166,745,056	2,222,052.2	2.642	21.13
11	1.654	155	294,390,464	3,953,304.2	4.700	37.60
12	1.696	165	27,359,364	369,002.2	0.439	3.51
13	1.746	177	1,924,781	21,918.0	0.026	0.21
14	1.801	190	14,155,619	194,239.9	0.231	1.85
15	1.856	203	91,019,856	1,755,547.8	2.087	16.70
16	1.911	216	1,519,074	19,757.0	0.023	0.19
17	2.029	244	653,658	8,698.1	0.010	0.08
18	2.067	253	11,938,587	191,017.5	0.227	1.82
19	2.126	267	57,103,736	1,006,413.1	1.197	9.57
20	2.160	275	155,055,968	3,067,493.2	3.647	29.18

Inst(Env&Ch #5) ACQUISITION PARAMETERS
Oven: Initial temp 40°C for 4 min, ramp 15°C/min to 220°C, Inj=280°C, Volume=0.100 µL, Split=100:1, Carrier Gas=He, Solvent Delay=0.00 min, Transfer Temp=250°C, Source Temp=180°C, Scan: 35 to 300Da, Column 30.0m x 250µm

Section – "Chromatogram Plot" containing ActiveX Plot

- Can be turned off in the Report Method
- Does not repeat

ActiveX Plot – "ActiveX1"

- Source: Project.Samples(Last).Chromatogram
- Data set to Function 1 TIC

Table – "TABLE1"

- Expands on QualitativePeaks()
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "#"
  2. Text – "RT"
  3. Text – "Scan"
  4. Text – "Height"
  5. Text – "Area"
  6. Text – "Area %"
  7. Text – "Norm %"
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).QualPeaks(Current).PeakNumber
  2. Project.Samples(Last).QualPeaks(Current).RetentionTime
  3. Project.Samples(Last).QualPeaks(Current).ScanNumber
  4. Project.Samples(Last).QualPeaks(Current).Height
  5. Project.Samples(Last).QualPeaks(Current).Area
  6. Project.Samples(Last).QualPeaks(Current).PercentArea
  7. Project.Samples(Last).QualPeaks(Current).PercentNorm

Template: QualQuant Report


Environmental & Chemical BU

Qualitative/Quantitative Report

File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix54.raw
Acquired: 07-Oct-03 06:04:38 PM
Description: Unknown, HCB Int. Std.
GC/MS Method: GC: StdMix6.mth MS: stdmix4.EXP
Sample ID: U44366c

Printed: 20-Apr-05 09:25 PM

Page 1 of 1
Vial Number: 24

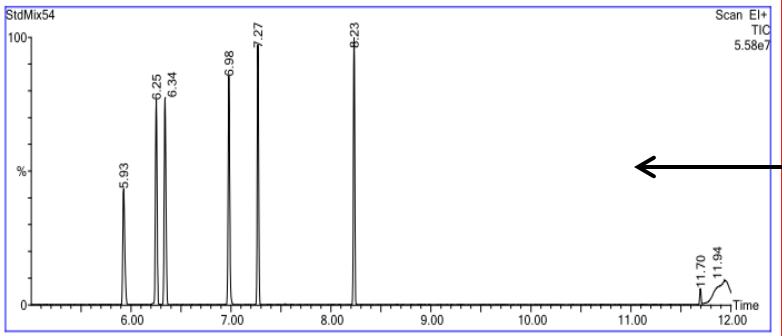

#	RT	Scan	Height	Area	Area %	Norm %	Name	ng/uL
1	5.928	276	24,192,158	561,012.9	11.360	62.99	1-Octanol	0.790
2	6.254	373	42,645,360	819,828.1	16.600	92.05	Undecane	0.726
3	6.342	399	43,043,964	880,686.6	17.833	98.89	2,6-Dimethylphenol	0.770
4	6.981	589	47,648,160	873,747.4	17.692	98.11	2,6-Dimethylanaline	0.792
5	7.270	675	54,236,284	853,243.6	17.277	95.80	Dodecane	0.765
6	7.543	756	174,849	2,204.4	0.045	0.25		
7	8.232	961	55,826,800	890,616.6	18.034	100.00	Tridecane	0.758
8	11.101	1814	57,793	784.2	0.016	0.09		
9	11.128	1822	66,947	1,677.0	0.034	0.19		
10	11.155	1830	59,254	1,027.7	0.021	0.12		
11	11.696	1991	3,299,444	53,775.3	1.089	6.04	Hexachlorobenzene	2.652

Inst(Env&Ch #5) ACQUISITION PARAMETERS
Oven: Initial temp 45℃ for 1 min, ramp 15℃/min to 205℃, hold 0.33 min, InjAauto=250℃, Volume=1.00 µL, Split=0:1, Carrier Gas=He, Solvent Delay=4.50 min, Transfer Temp=250℃, Source Temp=180℃, Scan: 45 to 300Da, Column 30.0m x 250µm

Section – "Chromatogram Plot" containing ActiveX Plot

- Can be turned off in the Report Method
- Does not repeat


ActiveX Plot – "ActiveX1"

- Source: Project.Samples(Last).Chromatogram
- ActiveX Plot Data set to Function 1 TIC

Table – "Table1"

- Expands on QualitativePeaks()
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "#"
  2. Text – "RT"
  3. Text – "Scan"
  4. Text – "Height"
  5. Text – "Area"
  6. Text – "Area %"
  7. Text – "Norm %"
  8. Text – "Name"
  9. Project.Samples(Last).Targets(First).ConcUnits
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).QualPeaks(Current).PeakNumber
  2. Project.Samples(Last).QualPeaks(Current).RetentionTime
  3. Project.Samples(Last).QualPeaks(Current).ScanNumber
  4. Project.Samples(Last).QualPeaks(Current).Height
  5. Project.Samples(Last).QualPeaks(Current).Area
  6. Project.Samples(Last).QualPeaks(Current).PercentArea
  7. Project.Samples(Last).QualPeaks(Current).PercentNorm
  8. Project.Samples(Last).QualPeaks(Current).Name
  9. Project.Samples(Last).QualPeaks(Current).Conc

Template: Quant Report Table

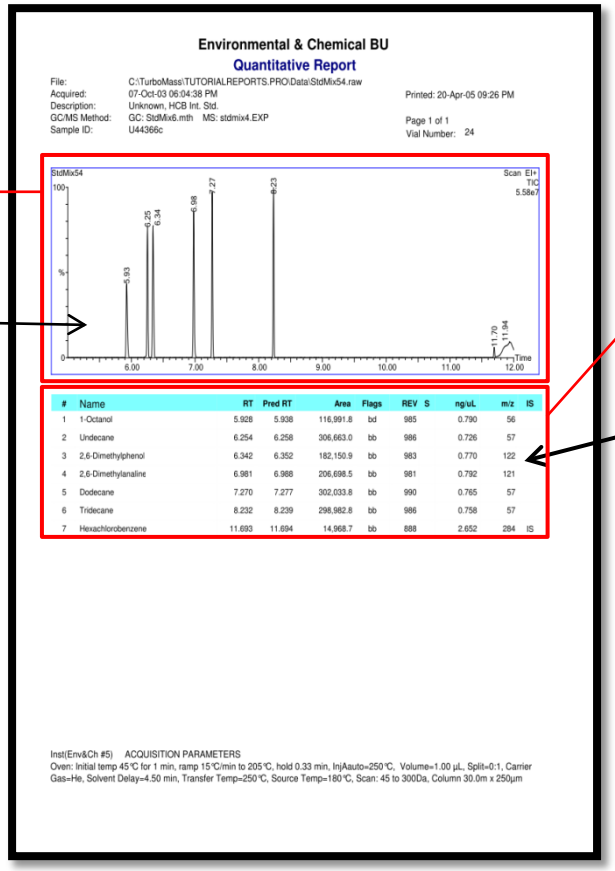

Section – "Chromatogram Plot" containing ActiveX Plot

- Can be turned off in the Report Method
- Does not repeat

ActiveX Plot – "ActiveX1"

- Source: Project.Samples(Last).Chromatogram
- ActiveX Plot Data set to Function 1 TIC


Section – "Table" containing Table

- Repeats based on Samples()

Table – "Table1"


- Expands on Target Compounds()
- No filtering/sorting/grouping
- Data items for 1st Row (by column number):
  1. Text – "#"
  2. Text – "Name"
  3. Text – "RT"
  4. Text – "Pred RT"
  5. Text – "Area"
  6. Text – "Flags"
  7. Text – "REV"
  8. Text – "S"
  9. Project.Samples(Last).Targets(Current).ConcUnits
  10. Text – "m/z"
  11. Text – "IS"
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).Targets(Current).CompoundNum
  2. Project.Samples(Last).Targets(Current).Name
  3. Project.Samples(Last).Targets(Current).ActualTime
  4. Project.Samples(Last).Targets(Current).ExpectedTime
  5. Project.Samples(Last).Targets(Current).Area
  6. Project.Samples(Last).Targets(Current).PeakIntFlag
  7. Project.Samples(Last).Targets(Current).ReverseFitScore
  8. EQUATION: "TargetSaturated"
  9. Project.Samples(Last).Targets(Current).Conc
  10. Project.Samples(Last).Targets(Current).QuantifyTrace
  11. EQUATION: "InternalStandardFlag"


Equation – "TargetSaturated"

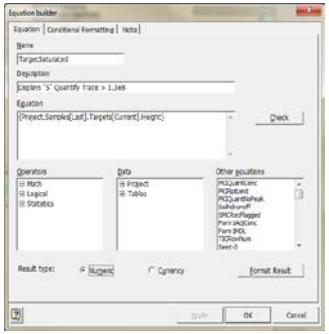




Equation – "InternalStandardFlag"

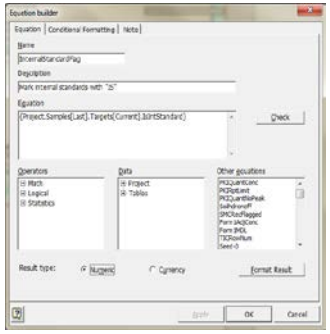

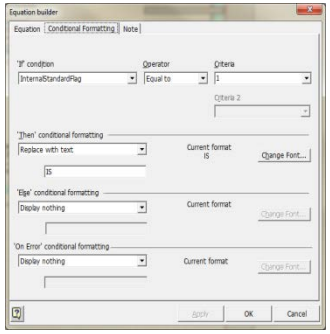

Template: Quantitation Report

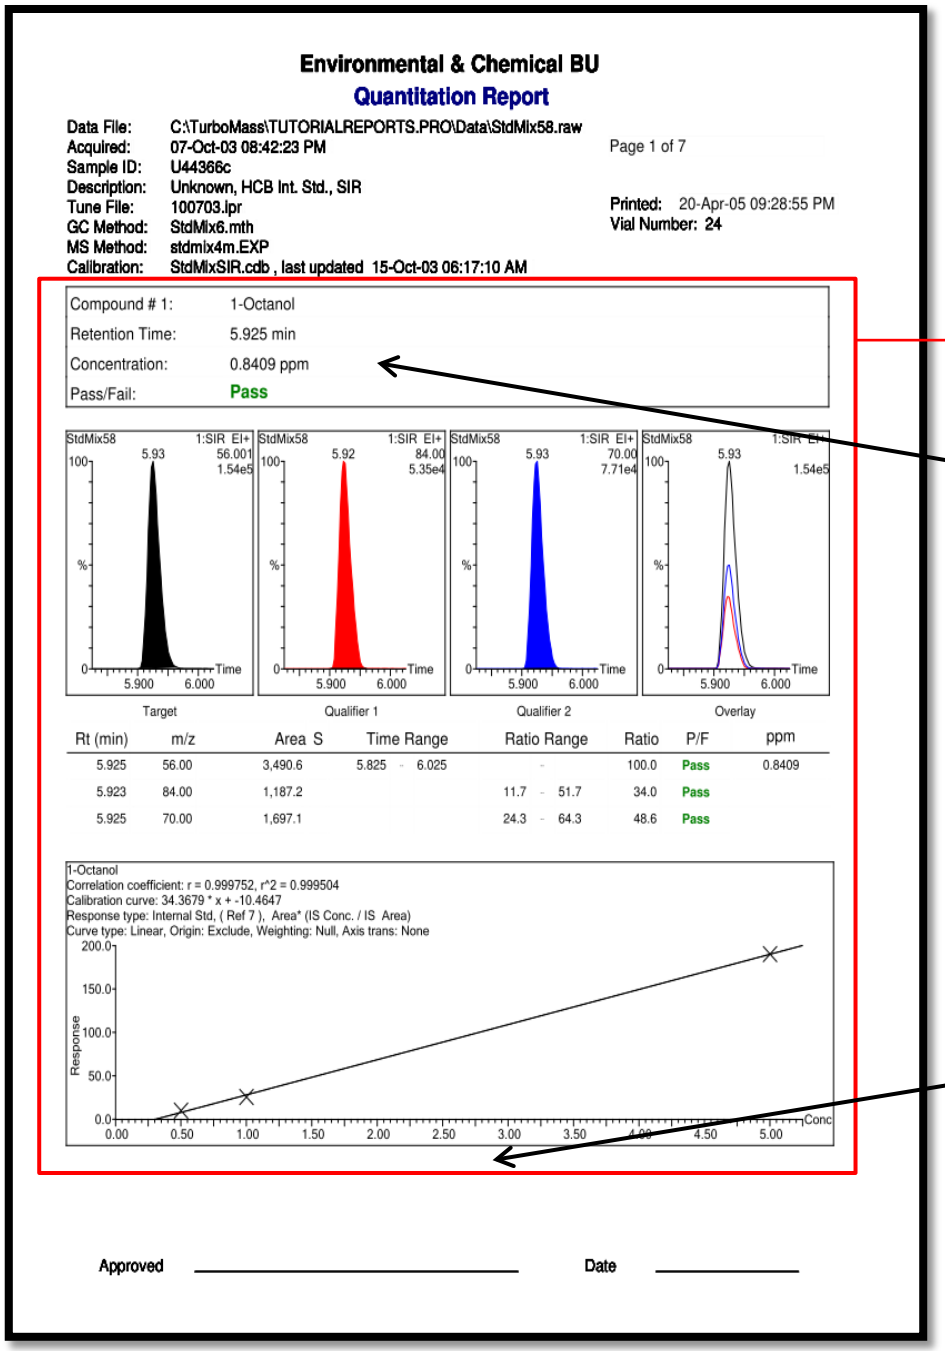

Environmental & Chemical BU

Quantitation Report

Data File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix58.raw
Acquired: 07-Oct-03 08:42:23 PM
Sample ID: U44366c
Description: Unknown, HCB Int. Std., SIR
Tune File: 100703.lpr
GC Method: StdMix6.mth
MS Method: stdmix4m.EXP
Calibration: StdMixSIR.cdb , last updated 15-Oct-03 06:17:10 AM

Page 1 of 7

Printed: 20-Apr-05 09:28:55 PM
Vial Number: 24

Compound # 1: 1-Octanol
Retention Time: 5.925 min
Concentration: 0.8409 ppm
Pass/Fail: Pass

Rt (min)	m/z	Area S	Time Range	Ratio Range	Ratio	P/F	ppm
5.925	56.00	3,490.6	5.825 - 6.025	-	100.0	Pass	0.8409
5.923	84.00	1,187.2		11.7 - 51.7	34.0	Pass	
5.925	70.00	1,697.1		24.3 - 64.3	48.6	Pass	

Approved _____ Date _____

Section – "Section1" containing 5 ActiveX Plots, Equation, 3 tables, and Page Break

- Repeat section based on Target Compounds()
- No sorting/filtering


Table – "Table2" (Top table – general description of target compound)

- Does not expand
- Data items for 1st Column (by row number):
  1. Text - "Compound #" + Project.Samples(Last).Targets(Current).CompoundNum
  2. Text – "Retention Time:"
  3. Text – "Concentration:"
  4. Text – "Pass/Fail:"

- Data items for 2nd Column (by row number):
  1. Project.Samples(Last).Targets(Current).Name
  2. Project.Samples(Last).Targets(Current).ActualTime + Text
  3. Project.Samples(Last).Targets(Current).Conc + Project.Samples(Last).Targets(Current).ConcUnits
  4. EQUATION: "CompoundPassFail"

Page Break

(Continued to next page)

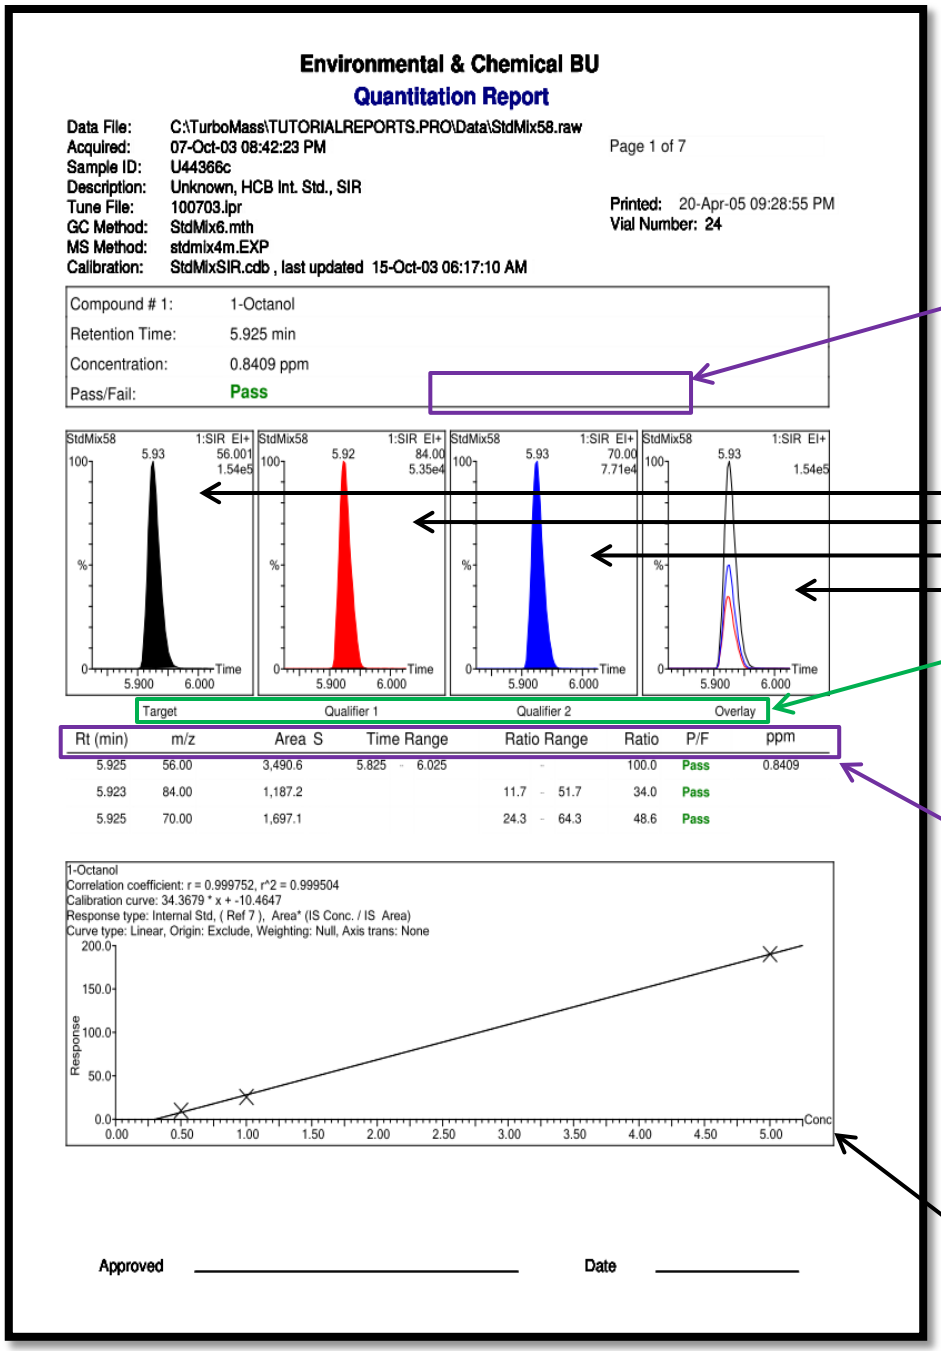

Equation – "IonRatiosOverride"

ActiveX Plots – "ActiveX1-4"

- Source: Project.Samples(Last).Targets(Current).PeakPlot
- Data:
  1. Target compound – Quantify Trace
  2. Target compound – Qualifier Ion 1
  3. Target compound – Qualifier Ion 2
  4. Target compound – Overlay Quantify trace and Qualifier Ions

Text (floating)


- Text – "Target"
- Text – " Qualifier 1"
- Text – "Qualifier 2"
- Text – "Overlay"

Table – "Table1" (Header row of main table)

- Does not expand
- Data items for 1st Row (by column number):
  1. Text – "RT (min)"
  2. Text – "m/z"
  3. Text – "Area"
  4. Text – "S"
  5. Text – "Time Range"
  6. Text – "Ratio Range"
  7. Text – "Ratio"
  8. Text – "P/F"
  9. Project.Samples(Last).Targets(Current).ConcUnits

ActiveX Plot – "ActiveX3" (Calibration curve)

- Source: Project.Samples(Last).Targets(Current).CalibCurve

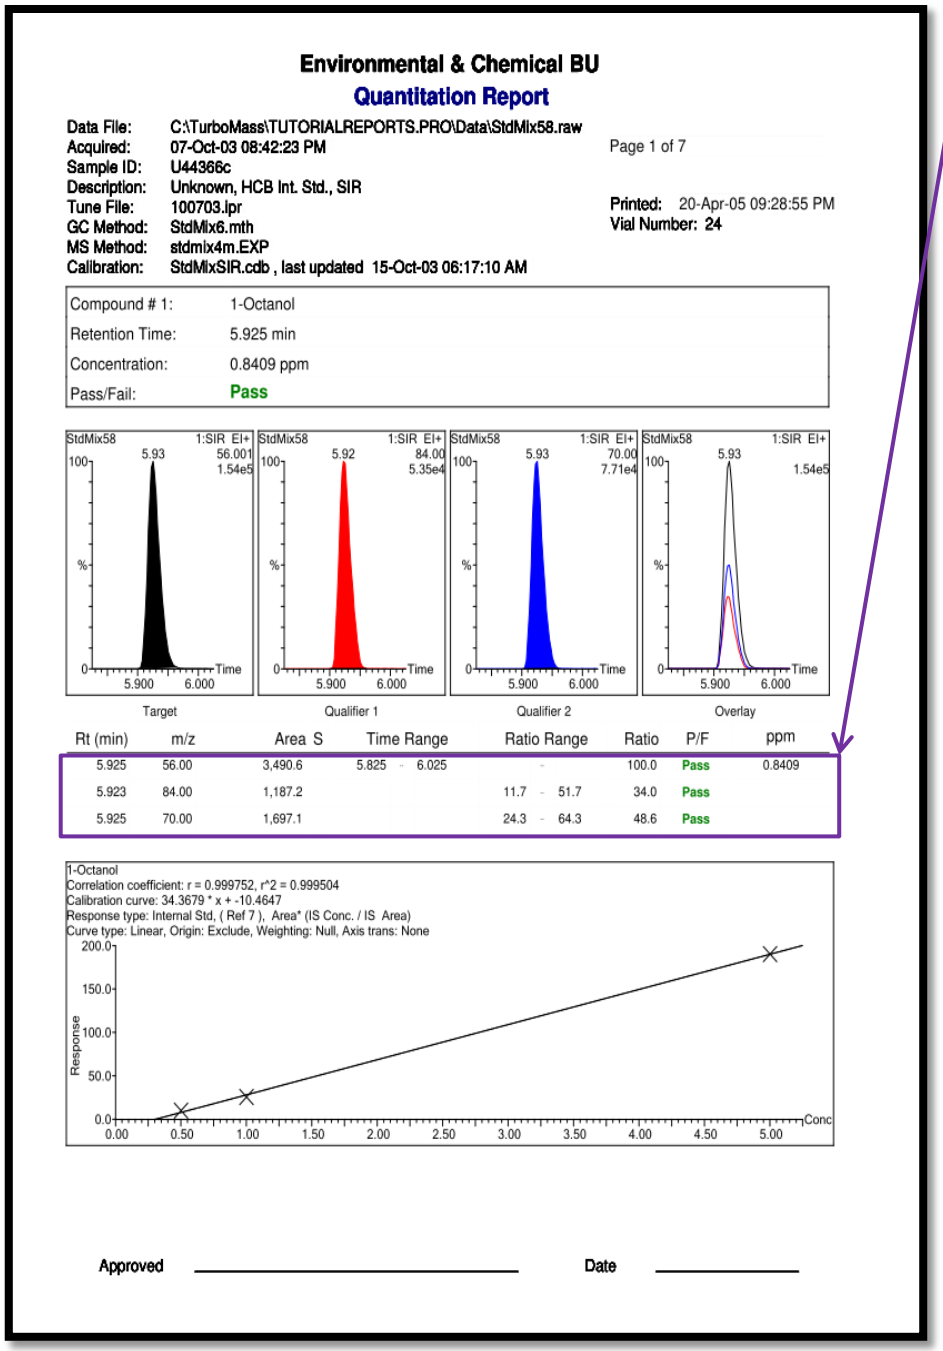

Environmental & Chemical BU

Quantitation Report

Data File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix58.raw
Acquired: 07-Oct-03 08:42:23 PM
Sample ID: U44366c
Description: Unknown, HCB Int. Std., SIR
Tune File: 100703.lpr
GC Method: StdMix6.mth
MS Method: stdmix4m.EXP
Calibration: StdMixSIR.cdb , last updated 15-Oct-03 06:17:10 AM

Page 1 of 7

Printed: 20-Apr-05 09:28:55 PM
Vial Number: 24

Compound # 1:	1-Octanol
Retention Time:	5.925 min
Concentration:	0.8409 ppm
Pass/Fail:	Pass

Target | Qualifier 1 | Qualifier 2 | Overlay

Rt (min)	m/z	Area S	Time Range	Ratio Range	Ratio	P/F	ppm
5.925	56.00	3,490.6	5.825 - 6.025	-	100.0	Pass	0.8409
5.923	84.00	1,187.2		11.7 - 51.7	34.0	Pass	
5.925	70.00	1,697.1		24.3 - 64.3	48.6	Pass	

1-Octanol
Correlation coefficient: r = 0.999752, r^2 = 0.999504
Calibration curve: 34.3679 * x + -10.4647
Response type: Internal Std, (Ref 7), Area* (IS Conc. / IS Area)
Curve type: Linear, Origin: Exclude, Weighting: Null, Axis trans: None

Response | Conc

Approved _____ Date _____

Table – "Table4" (Body rows of main table)

- Expands on QualIons()
- Data items for 1st Row (by column number):
  1. Project.Samples(Last).Targets(Current).ActualTime
  2. Project.Samples(Last).Targets(Current).QuantifyTrace
  3. Project.Samples(Last).Targets(Current).Area
  4. EQUATION: "TargetSaturated"
  5. EQUATION: "LowRTLimit"
  6. Text – "-"
  7. EQUATION: "HighRTLimit"
  8. Project.Samples(Last).Targets(Current).TraceLowLimit
  9. Text – "-"
  10. Project.Samples(Last).Targets(Current).TraceHighLimit
  11. Project.Samples(Last).Targets(Current).TraceRatio
  12. EQUATION: "PassFailTarget1"
  13. Project.Samples(Last).Targets(Current).Conc
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).Targets(Current).QualIons(Current).ActualRetentionTime
  2. Project.Samples(Last).Targets(Current).QualIons(Current).Mass
  3. Project.Samples(Last).Targets(Current).QualIons(Current).Area
  4. EQUATION: "QualifierSaturated"
  5. Empty
  6. Empty
  7. Empty
  8. Project.Samples(Last). Targets(Current).QualIons(Current).LowLimit
  9. Text – "
  10. Project.Samples(Last). Targets(Current).QualIons(Current).HighLimit
  11. Project.Samples(Last). Targets(Current).QualIons(Current).Ratio
  12. EQUATION: "PassFail"
  13. Empty

(Continued to next page)

Environmental & Chemical BU


Quantitation Report

Data File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix58.raw
Acquired: 07-Oct-03 08:42:23 PM
Sample ID: U44366c
Description: Unknown, HCB Int. Std., SIR
Tune File: 100703.lpr
GC Method: StdMix6.mth
MS Method: stdmix4m.EXP
Calibration: StdMixSIR.cdb , last updated 15-Oct-03 06:17:10 AM

Page 1 of 7


Printed: 20-Apr-05 09:28:55 PM
Vial Number: 24

Compound # 1: 1-Octanol
Retention Time: 5.925 min
Concentration: 0.8409 ppm
Pass/Fail: Pass

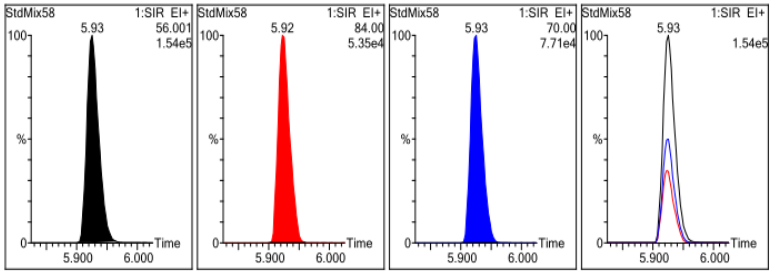


Target | Qualifier 1 | Qualifier 2 | Overlay


Rt (min)	m/z	Area S	Time Range	Ratio Range	Ratio	P/F	ppm
5.925	56.00	3,490.6	5.825 - 6.025		100.0	Pass	0.8409
5.923	84.00	1,187.2		11.7 - 51.7	34.0	Pass	
5.925	70.00	1,697.1		24.3 - 64.3	48.6	Pass	

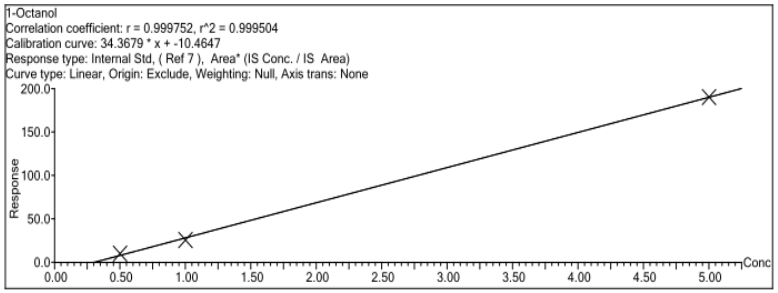


Approved _____ Date _____

Equation – "CompoundPassFail"

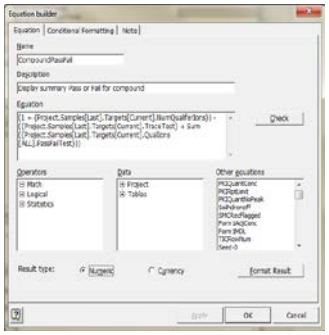

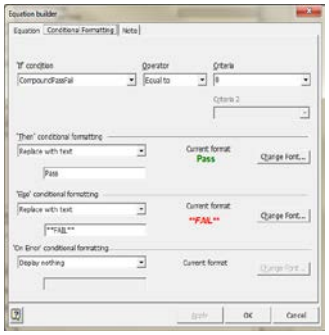


Equation – "IonRatiosOverride"

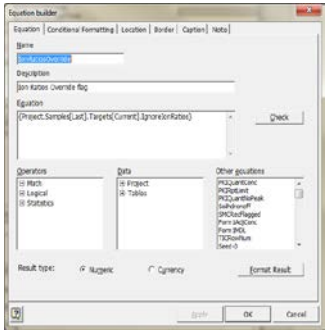



Equation – "TargetSaturated"

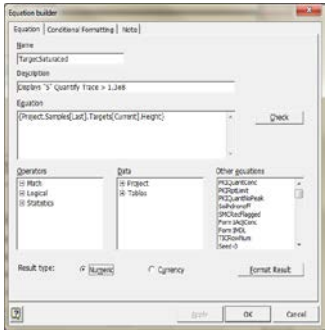



(Continued to next page)


Environmental & Chemical BU

Quantitation Report


Data File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix58.raw
Acquired: 07-Oct-03 08:42:23 PM
Sample ID: U44366c
Description: Unknown, HCB Int. Std., SIR
Tune File: 100703.lpr
GC Method: StdMix6.mth
MS Method: stdmix4m.EXP
Calibration: StdMixSIR.cdb , last updated 15-Oct-03 06:17:10 AM

Printed: 20-Apr-05 09:28:55 PM
Vial Number: 24

Compound # 1:	1-Octanol
Retention Time:	5.925 min
Concentration:	0.8409 ppm
Pass/Fail:	Pass

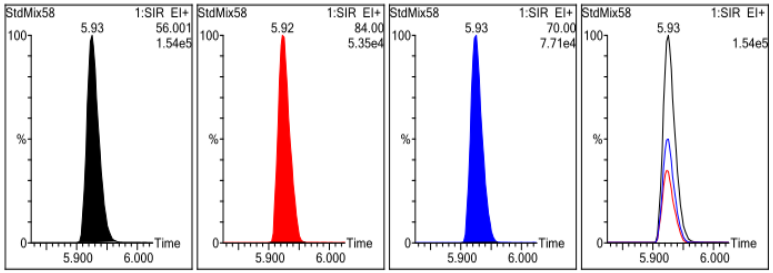


Rt (min)	m/z	Area S	Time Range	Ratio Range	Ratio	P/F	ppm
5.925	56.00	3,490.6	5.825 - 6.025	-	100.0	Pass	0.8409
5.923	84.00	1,187.2		11.7 - 51.7	34.0	Pass	
5.925	70.00	1,697.1		24.3 - 64.3	48.6	Pass	

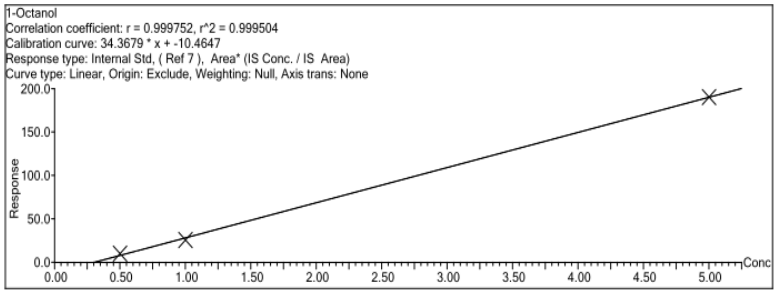


Approved _____ Date _____

Equation – "LowRTLimit"

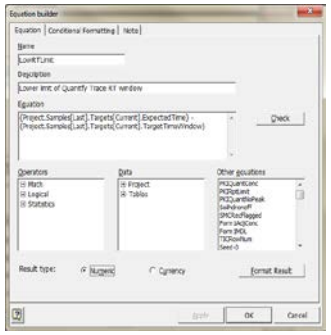





Equation – "HighRTLimit"

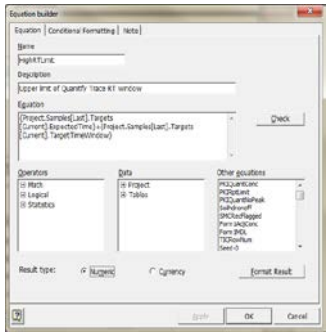



Equation – "PassFailTarget1"

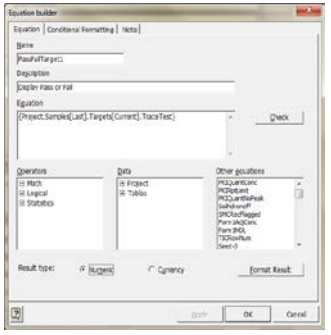

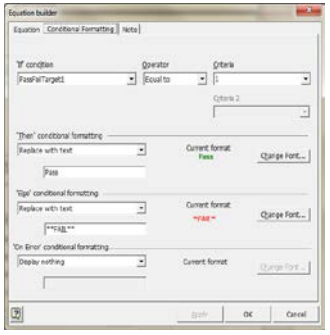

(Continued to next page)


Environmental & Chemical BU

Quantitation Report

Data File: C:\TurboMass\TUTORIALREPORTS.PRO\Data\StdMix58.raw
Acquired: 07-Oct-03 08:42:23 PM
Sample ID: U44366c
Description: Unknown, HCB Int. Std., SIR
Tune File: 100703.lpr
GC Method: StdMix6.mth
MS Method: stdmix4m.EXP
Calibration: StdMixSIR.cdb , last updated 15-Oct-03 06:17:10 AM


Printed: 20-Apr-05 09:28:55 PM
Vial Number: 24

Compound # 1:	1-Octanol
Retention Time:	5.925 min
Concentration:	0.8409 ppm
Pass/Fail:	Pass

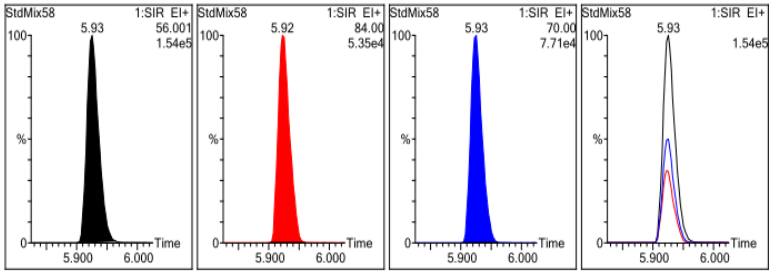


Target | Qualifier 1 | Qualifier 2 | Overlay


Rt (min)	m/z	Area S	Time Range	Ratio Range	Ratio	P/F	ppm
5.925	56.00	3,490.6	5.825 - 6.025	-	100.0	Pass	0.8409
5.923	84.00	1,187.2		11.7 - 51.7	34.0	Pass	
5.925	70.00	1,697.1		24.3 - 64.3	48.6	Pass	

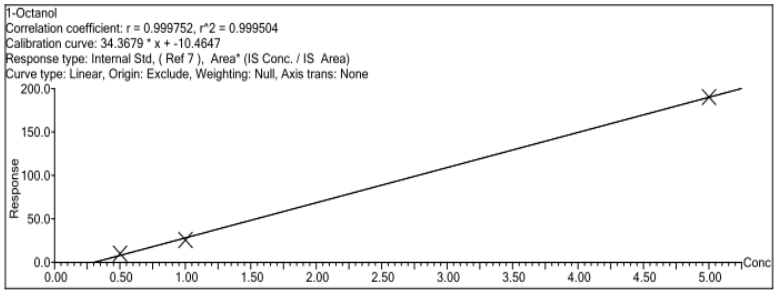


Approved _____ Date _____


Equation – "QualifierSaturated"

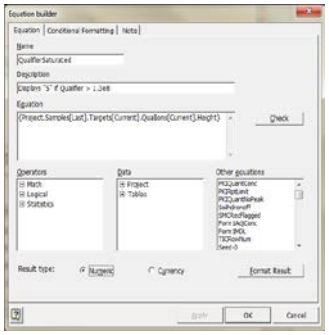

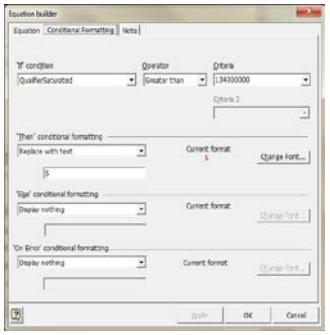

Equation – "PassFail"

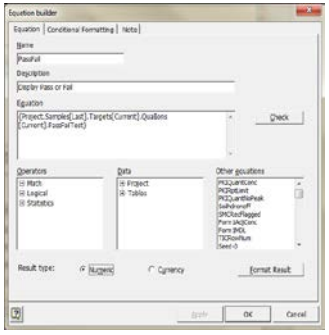

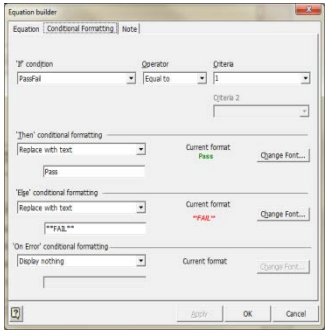

Template: SpectrumQuant Report

Section – "Section1" containing 4 ActiveX Plots, Text box, Equation, 2 Tables, Page Break

- Repeats based on Target Compounds()

Text Box

- Project.Samples(Last).Targets(Current).CompoundNum
- Project.Samples(Last).Targets(Current).Name
- Project.Samples(Last).Targets(Current).Conc
- Project.Samples(Last).Targets(Current).ConcUnits
- Project.Samples(Last).Targets(Current).ActualTime
- Project.Samples(Last).Targets(Current).RetentionTimeDifference
- Project.Samples(Last).Targets(Current).ActualScan
- Project.Samples(Last).Data.Filename
- Project.Samples(Last).Data.ModifyDateTime
- Project.Samples(Last).Targets(Current).QuantifyTrace
- Project.Samples(Last).Targets(Current).Area

ActiveX Plots – "ActiveX1-2"


- Source: Project.Samples(Last).Targets(Current).ActualSpectrum
- Data:
  1. Background Treatment – none
  2. Background Treatment – Background Subtracted

ActiveX Plot – "ActiveX3"


- Source: Project.Samples(Last).Targets(Current).ExpectedSpectrum

Equation – "IonRatiosOverride"

- Shows up between ActiveX3 plot and Table1

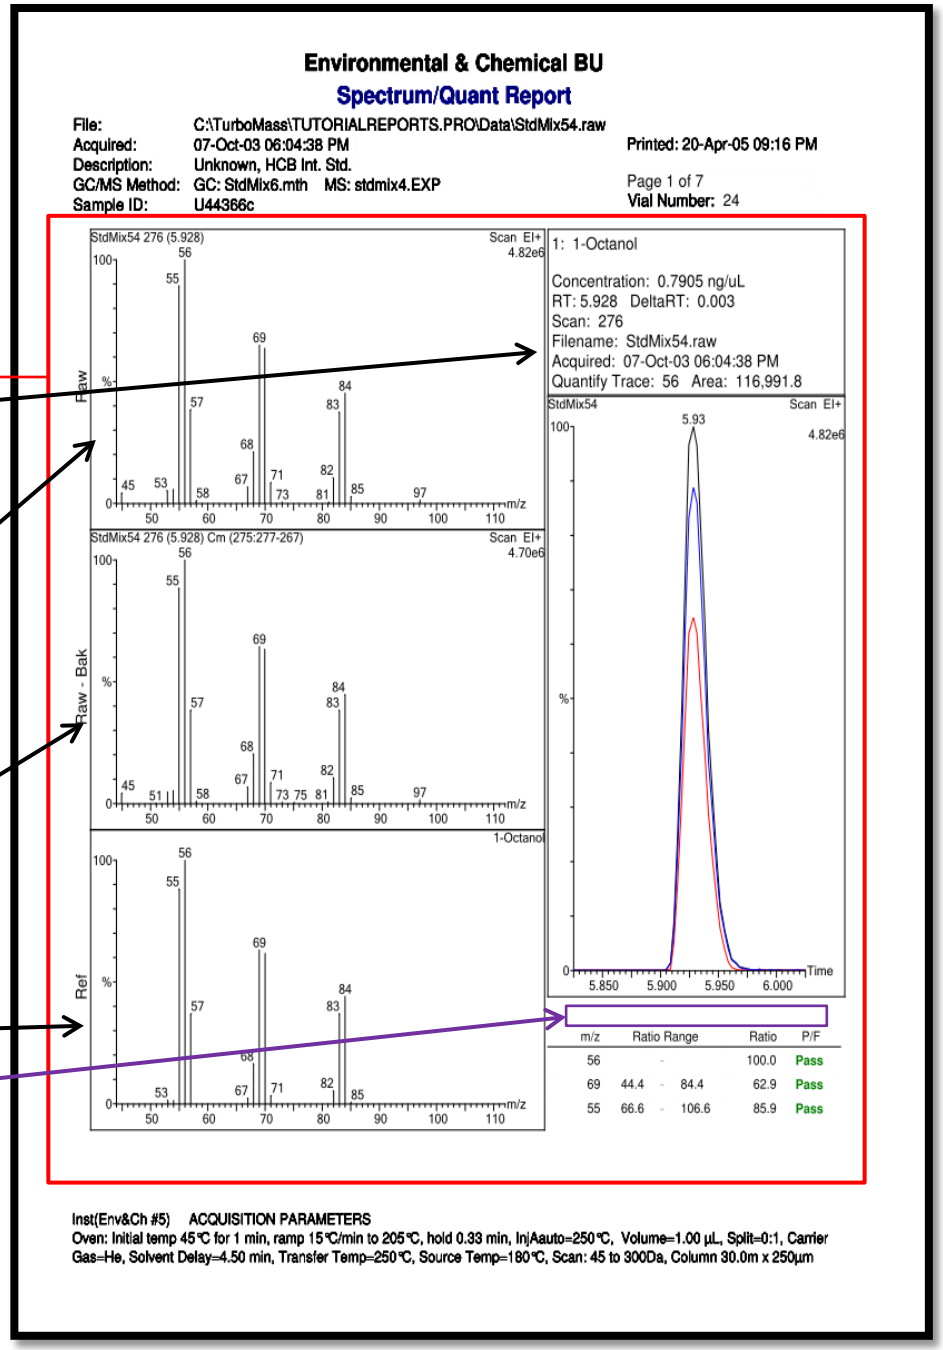

(Continued to next page)

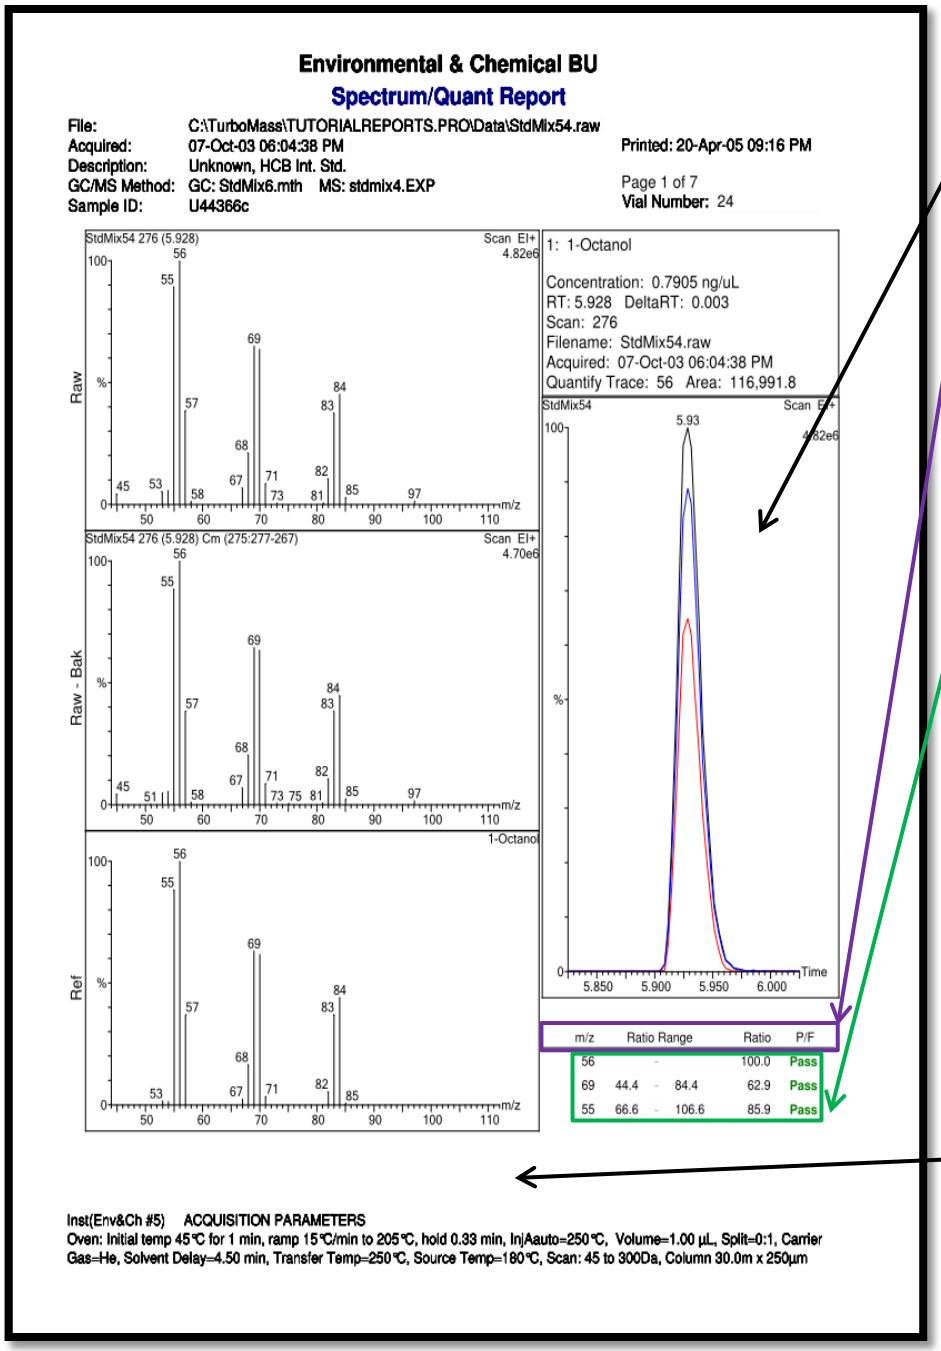

ActiveX Plots – "ActiveX4"

- Source: Project.Samples(Last).Targets(Current).PeakPlot
- Data: Target compound – Overlay Quantify Trace and Qualifier ions

Table – "Table1" (Title Row of Table)


- Does not expand.
- Data items for 1st Row (by column number):
  1. Text – "m/z"
  2. Text – "Ratio Range"
  3. Text – "Ratio"
  4. Text – "P/F"

Table – "Table2" (Body of Table)


- Expands on QualIons().
- Data items for 1st Row (by column number):
  1. Project.Samples(Last).Targets(Current).QuantifyTrace
  2. Project.Samples(Last).Targets(Current).TraceLowLimit
  3. Text – "-"
  4. Project.Samples(Last).Targets(Current).TraceHighLimit
  5. Project.Samples(Last).Targets(Current).TraceRatio
  6. EQUATION: "PassFailTarget1"
- Data items for 2nd Row (by column number):
  1. Project.Samples(Last).QualIons(Current).Mass
  2. Project.Samples(Last). QualIons(Current).LowLimit
  3. Text – "-"
  4. Project.Samples(Last). QualIons(Current).HighLimit
  5. Project.Samples(Last). QualIons(Current).Ratio
  6. EQUATION: "PassFail"

Page Break

(Continued to next page)

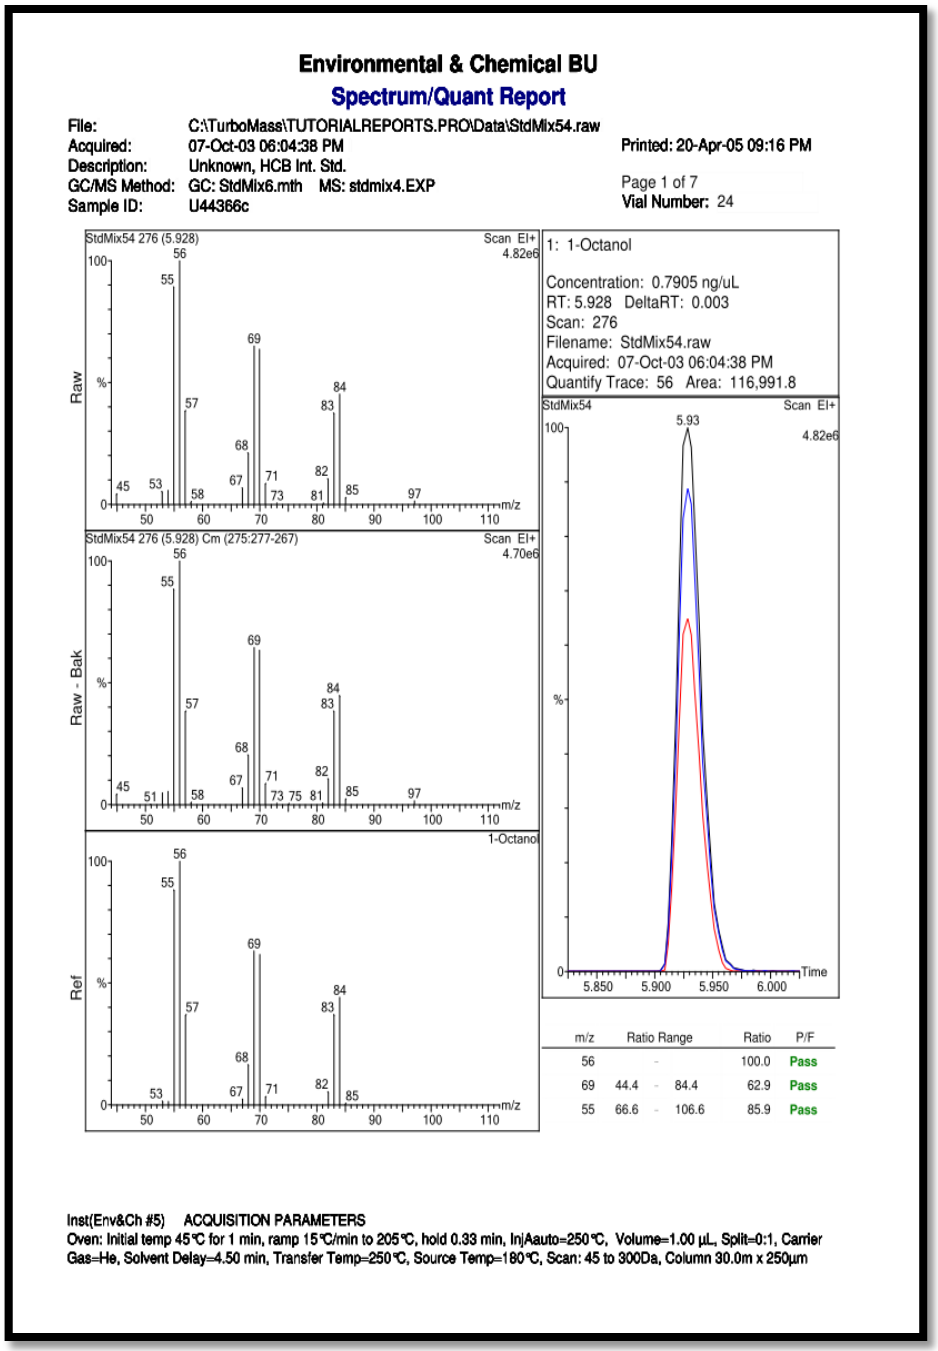



Equation – "IonRatiosOverride"

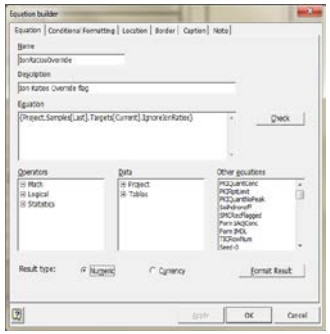



Equation – "PassFailTarget1"

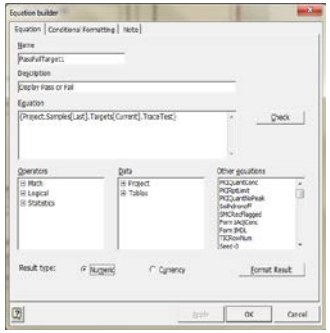

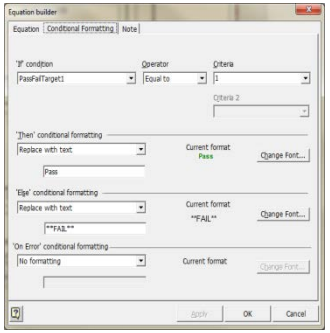

Equation – "PassFail"

