
# BEVERAGE TOWER


CLEAN LOWER VALVE BODY


DIRTY LOWER VALVE BODY

DAILY/RECOVERY

## SUPPLIES:


Valve Cleaning Brush
Inspection Mirror


KAY-5® Sanitizer/ Cleaner


KAY® Rapid Multi Surface Disinfectant Cleaner Solution


KAY® Daily Beverage Tower Drain Cleaner


KAY® QSR Heavy Duty Degreaser (RECOVERY ONLY)

| Franke | H&K | |
|---|---|---|
| #143492 | MEP-18550 | Valve Cleaning Brush |
| #143493 | 15037033 | Mirror Inspection tool |
| #143494 | 15037023 | Pail |
| #143496 | 581996-00 | Squeeze bottle, Heavy Duty Degreaser |
| #143498 | 581999-00 | Squeeze bottle, KAY-5 |


**Other supplies needed:**
Clean, Sanitized Container
Clean, Sanitizer-Soaked Towels
Degreaser, Sanitizer and Water-Only Squeeze Bottles

**IMPORTANT:** Daily procedure should be performed every day, at close or slow volume period, to eliminate the potential for buildup on beverage nozzles and diffusers. If buildup occurs, perform the recovery procedure using Degreaser Solution.


## DAILY





- Gather all cleaning supplies; wash hands before preparing Sanitizer Solution
- Prepare Sanitizer Solution by dissolving 1 packet of KAY-5 Sanitizer/Cleaner in 2.5 gal. (9.5 L) **lukewarm** (85-105°F) water (100ppm); mix thoroughly
- Fill a separate clean and sanitized container and Sanitizer squeeze bottle with KAY-5 Sanitizer Solution

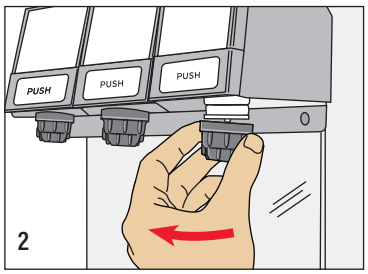



- Remove nozzles and diffusers; place in Sanitizer Solution; allow to soak if needed

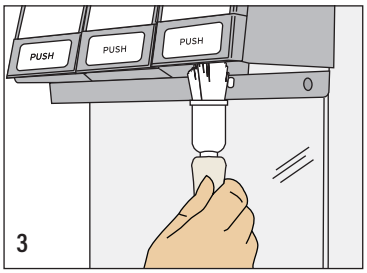



- Use valve cleaning brush dampened with KAY-5 Sanitizer Solution to clean underside of the diffuser and valve area and inside the lower valve body
- Repeat for all valves

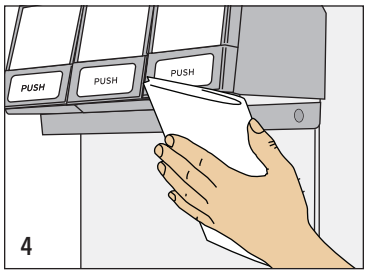



- Wipe diffuser and valve area with a clean sanitizer-soaked towel; discard towel into soiled towel bucket after use

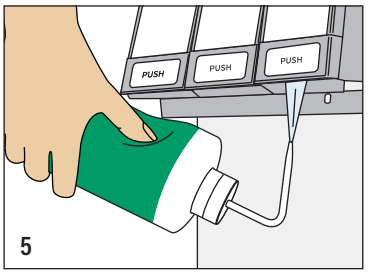


- Squeeze KAY-5 Sanitizer Solution vigorously into lower valve area to sanitize
- Repeat for all valves

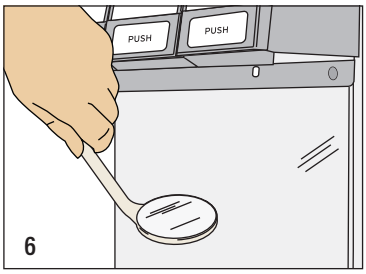


- View each diffuser and valve area with inspection mirror to ensure visual cleanliness; if soil is visible, conduct recovery procedure

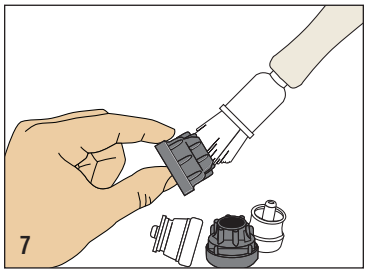



- Use valve brush to clean nozzles and diffusers: rinse at 3-compartment sink
- Place rinsed nozzles and diffusers in a separate clean and sanitized container of KAY-5 Sanitizer Solution; allow to soak for one minute; remove nozzles and diffusers immediately after soaking for one minute

ECOLAB®
Kay Chemical Company
8300 Capital Drive
Greensboro, NC 27409-9790, USA
CUSTOMER SERVICE 800.529.5458


92212274.05 MCD US 40921/8005/1025 ©2025 Ecolab USA Inc. All rights reserved.

# BEVERAGE TOWER (CONTINUED)


DAILY/RECOVERY

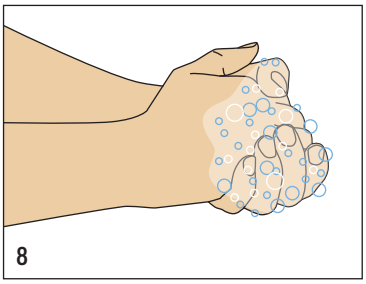



- Wash hands before reinstalling cleaned and sanitized nozzles and diffusers

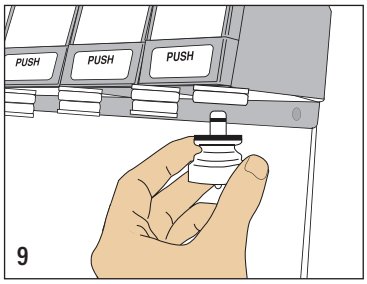


- Replace nozzles and diffusers

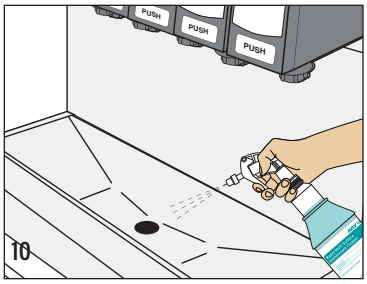



- Clean exterior (including drip tray/pan) using Rapid MSDC Solution and a clean sanitizer-soaked towel
- Discard towel into soiled towel bucket after use

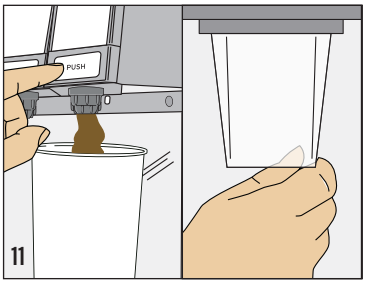



- Dispense beverage for 3 seconds after cleaning/sanitizing equipment; discard liquid
- If ice combo: Remove ice chute and wash rinse and sanitize at 3-compartment sink; re-install

## DRAIN CLEANING—DAILY DURING LOW PEAK HOURS

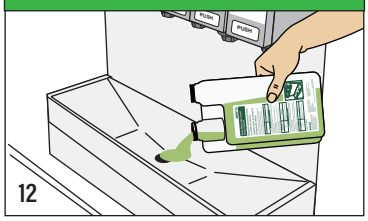



- After beverage tower cleaning is complete, clean beverage drain with Daily Beverage Tower Drain Cleaner
- Follow the BEVERAGE AND FLOOR DRAINS KAY CARD for step by step instructions


## RECOVERY

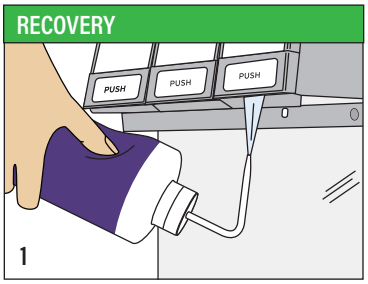


- Fill Degreaser squeeze bottle and a clean container with Degreaser Solution
- Remove nozzles and diffusers; place in container of Degreaser Solution; allow to soak
- Squeeze Degreaser Solution vigorously into lower valve area; repeat for all valves
- Follow step 3 from daily cleaning of valves
- Rinse brush with water after cleaning
- Follow step 6 from daily cleaning to visually inspect valve areas with inspection mirror

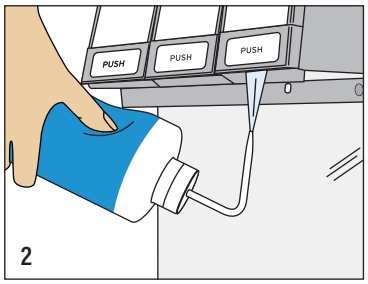


- Fill the water squeeze bottle with **hot** (110-120°F) water
- Squeeze **hot** water vigorously several times into lower valve area to rinse; repeat for all valves
- Wipe diffuser and valve area with a clean sanitizer-soaked towel
- Repeat step 7 from daily cleaning and sanitizing of nozzles and diffusers

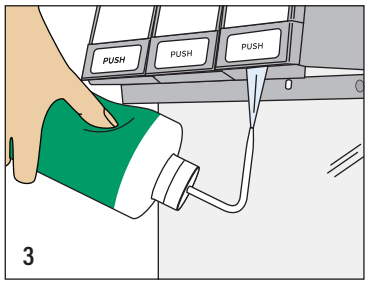


- Fill squeeze bottle with KAY-5 Sanitizer/Cleaner Solution
- Squeeze Sanitizer Solution vigorously into lower valve area to sanitize; repeat for all valves
- Repeat steps 8-12 from daily cleaning



ECOLAB®
Kay Chemical Company
8300 Capital Drive
Greensboro, NC 27409-9790, USA
CUSTOMER SERVICE 800.529.5458

92212274.05 MCD US 40927/8005/1025 ©2025 Ecolab USA Inc. All rights reserved.