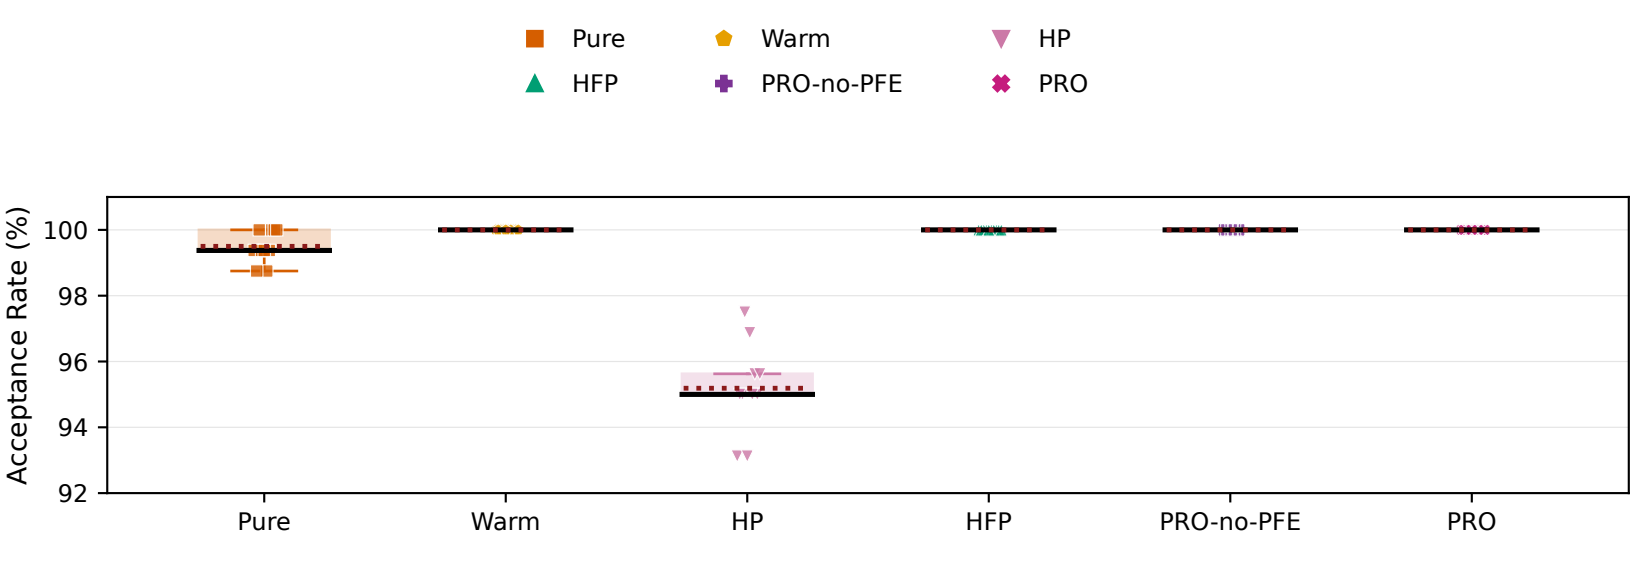


(a) Low Load

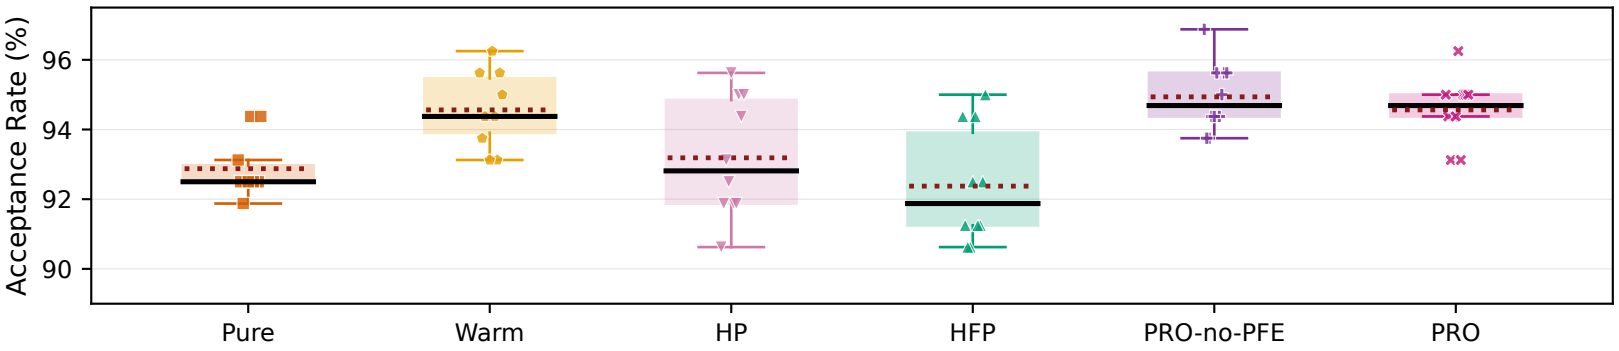


(b) Medium Load

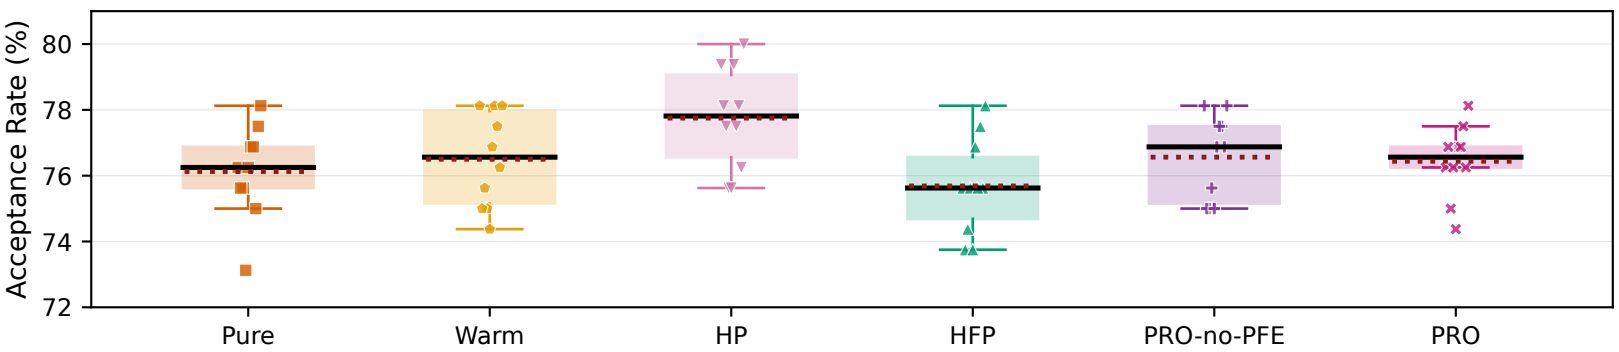


(c) High Load

S40 (|T|=8, |F|=160) Component Ablation