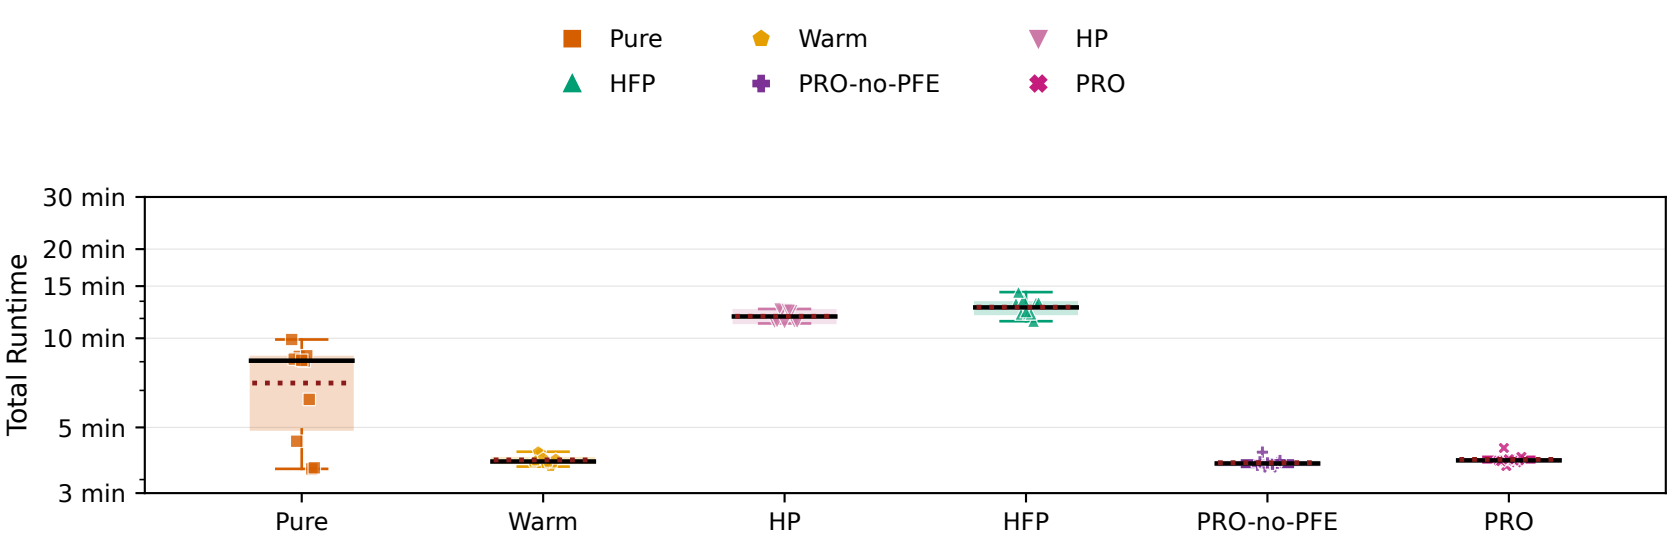

(a) Low Load

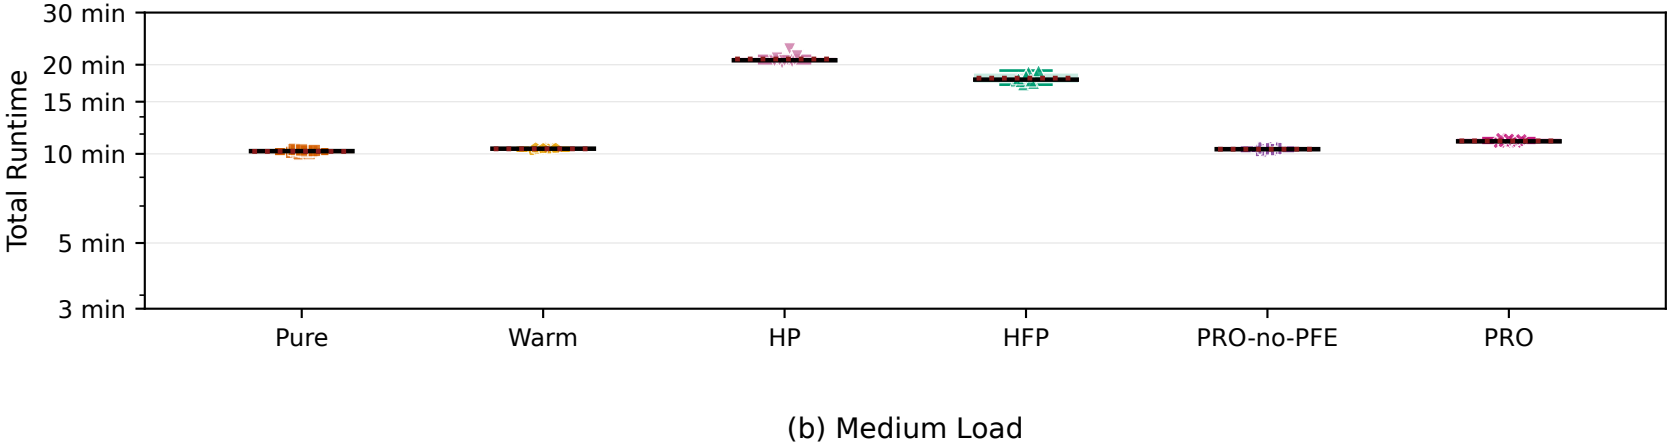

(b) Medium Load

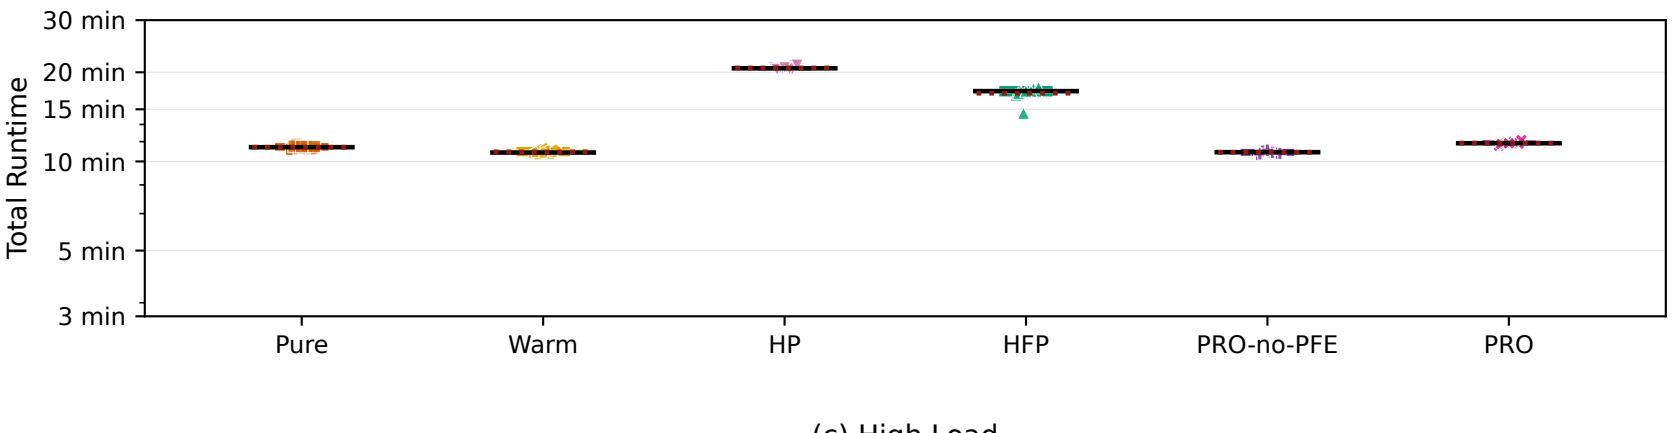

(c) High Load

S40 (|T|=8, |F|=160) Component Ablation