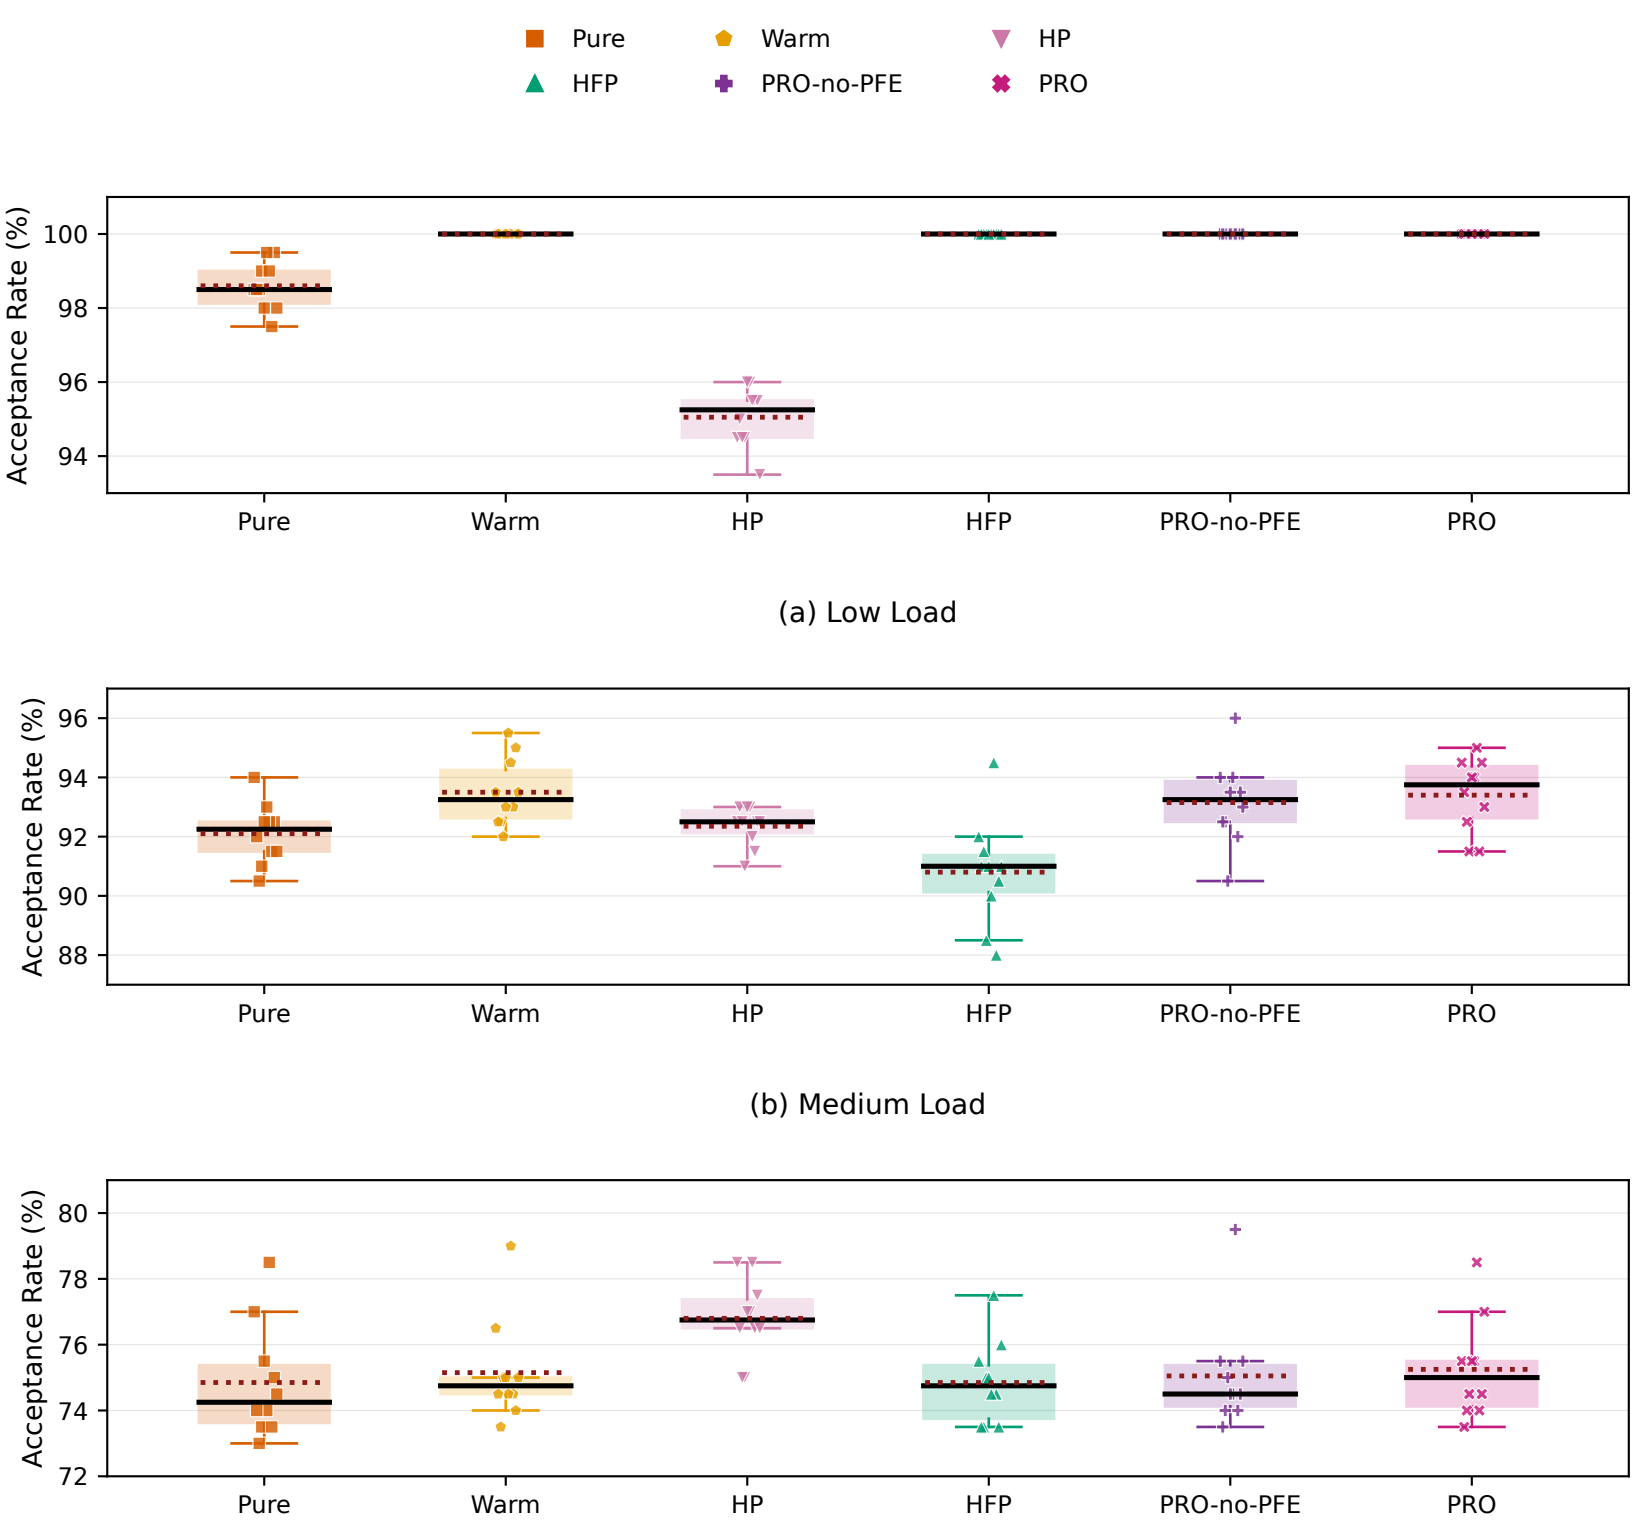

(a) Low Load

(b) Medium Load

(c) High Load

S50 (|T|=8, |F|=200) Component Ablation