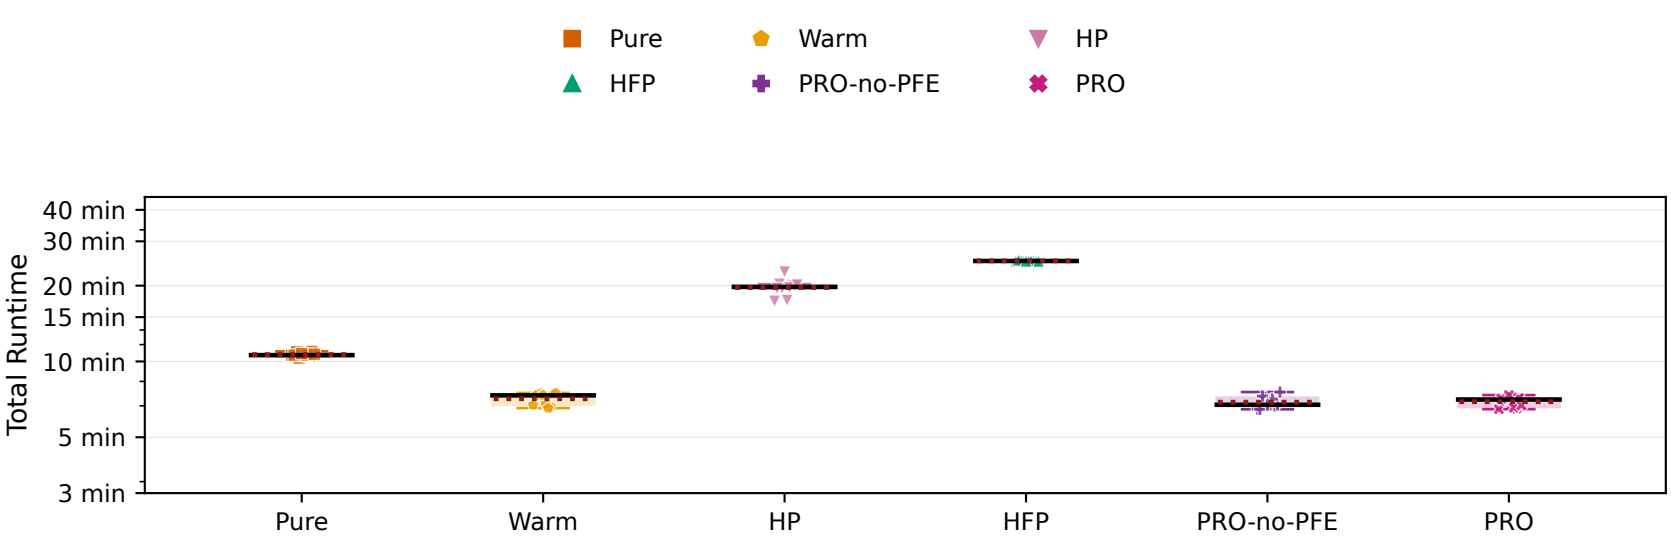

(a) Low Load

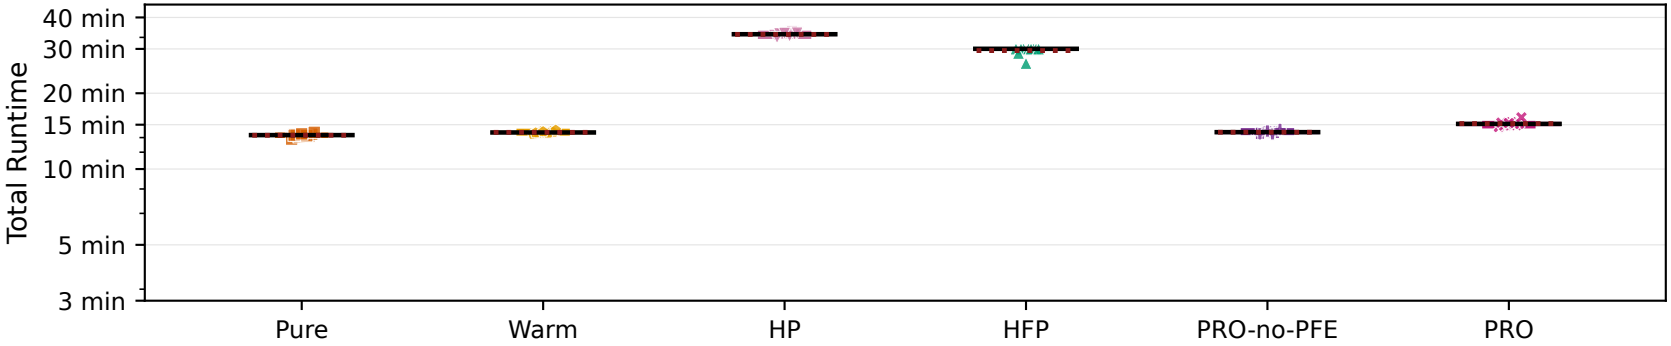

(b) Medium Load

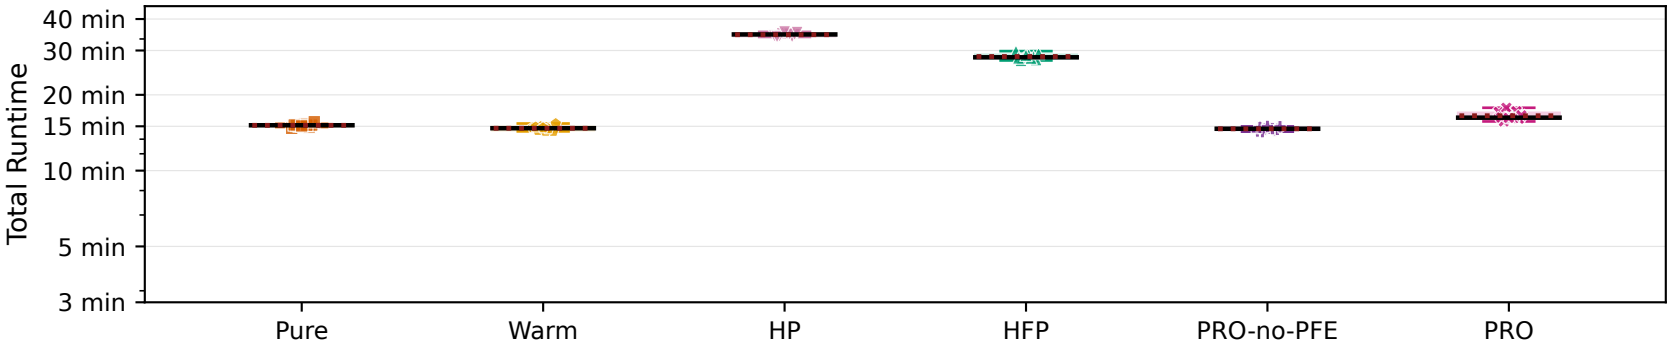

(c) High Load

S50 (|T|=8, |F|=200) Component Ablation