

PRE-TREATMENT REPORTWu xiu ying_UCC, yan gao shu 253406_281299

Clinic: SiChuan Cancer Hospital

Plan: Plan_3

Planned: 2016/7/30 9:37 admin

Measured: 2016/7/30 10:47 admin

Comments:

Treatment Summary

Radiation Device: 2809


Temperature: 22.0 °C

Reference: Planned Dose

Beam	Gantry	Energy	Daily corr factor	Norm dose	Det within acceptance	Median dose dev
Dev	DTA	γ-index				
Fraction				1.09 Gy	53.7%	94.1% 91.7% -1.6%
81	153°	6 MV	1.000	1.03 Gy	97.4% 100.0% 100.0%	-1.0%
82	102°	6 MV	1.000	0.82 Gy	90.1% 99.5% 100.0%	-0.4%
83	51°	6 MV	1.000	0.88 Gy	87.4% 98.7% 99.7%	-0.1%
84	0°	6 MV	1.000	1.23 Gy	90.1% 100.0% 100.0%	-0.0%
85	309°	6 MV	1.000	0.88 Gy	93.0% 100.0% 99.8%	-0.1%
86	258°	6 MV	1.000	1.10 Gy	88.2% 95.3% 99.6%	-0.5%
87	207°	6 MV	1.000	0.72 Gy	84.4% 96.7% 99.0%	-1.1%

Histograms

Reference: Planned dose

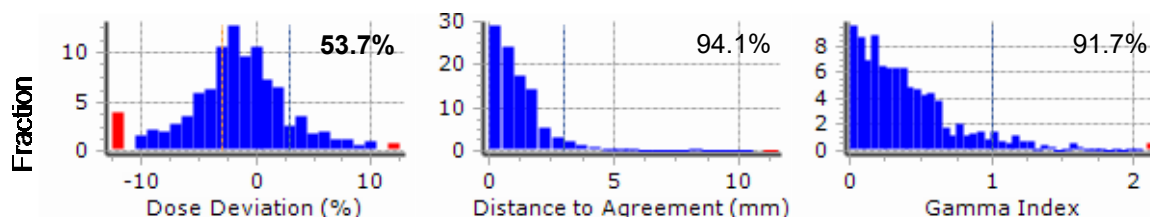

Parameter Definitions & Acceptance Criteria, Detectors

Parameter	Selected Detectors	Δ Dose	Δ Dist	Acceptance Limits
Dose Deviation	Dose from 20% to 500%	n.a.	n.a.	90% within ±3.0%
Dist to Agreement	Gradient >= 1%/mm	n.a.	n.a.	90% with DTA <= 3.0 mm
Gamma Index	Dose from 20% to 500%	±3.0%	3.0 mm	90% with gamma < 1