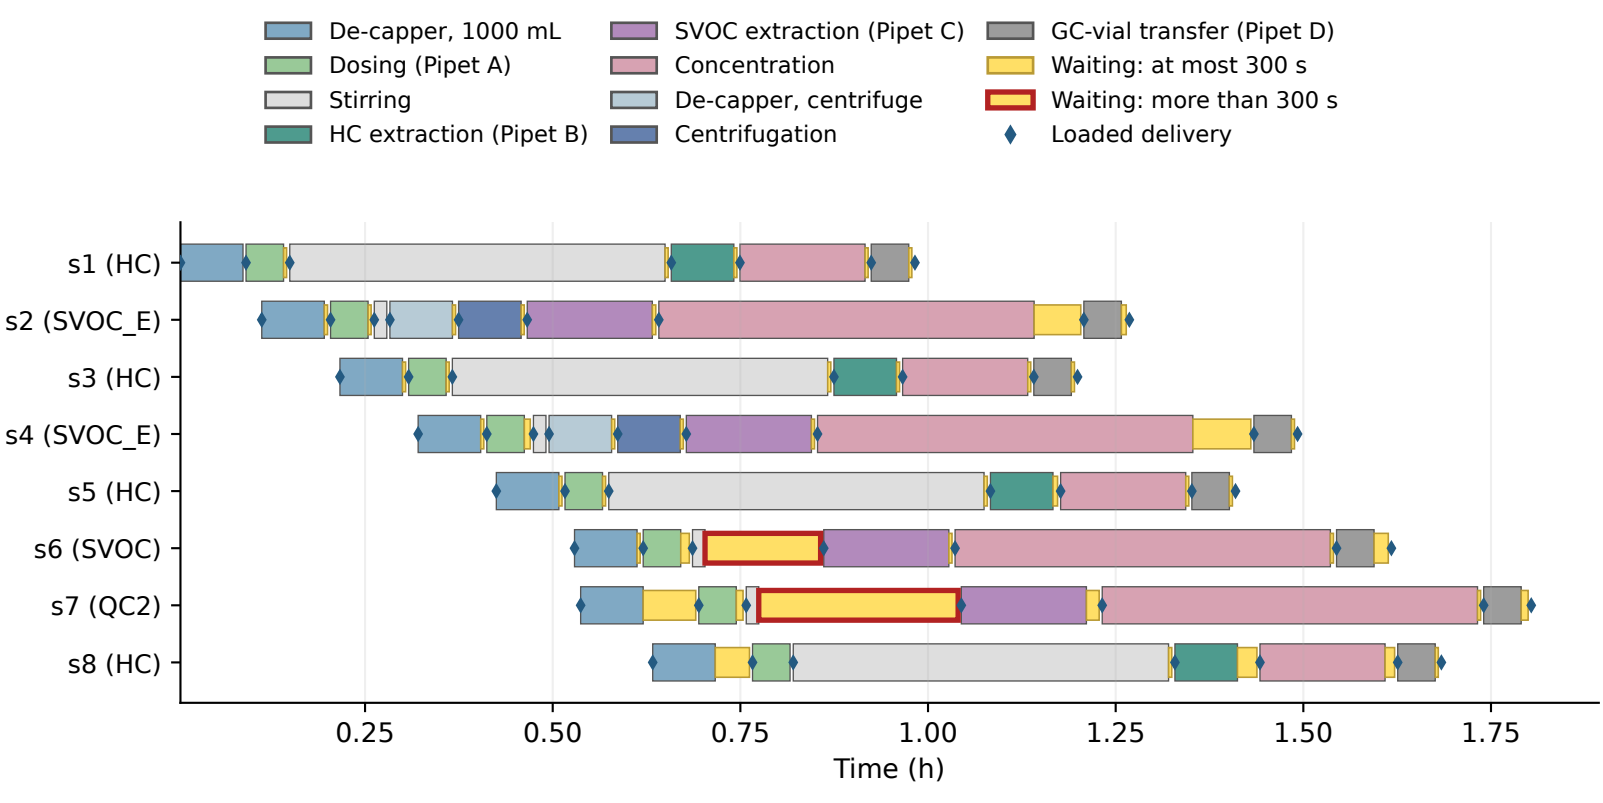
De-capper, 1000 mL
Dosing (Pipet A)
Stirring
HC extraction (Pipet B)
SVOC extraction (Pipet C)
Concentration
De-capper, centrifuge
Centrifugation
GC-vial transfer (Pipet D)
Waiting: at most 300 s
Waiting: more than 300 s
Loaded delivery
s1 (HC)
s2 (SVOC_E)
s3 (HC)
s4 (SVOC_E)
s5 (HC)
s6 (SVOC)
s7 (QC2)
s8 (HC)
0.25
0.50
0.75
1.00
1.25
1.50
1.75
Time (h)