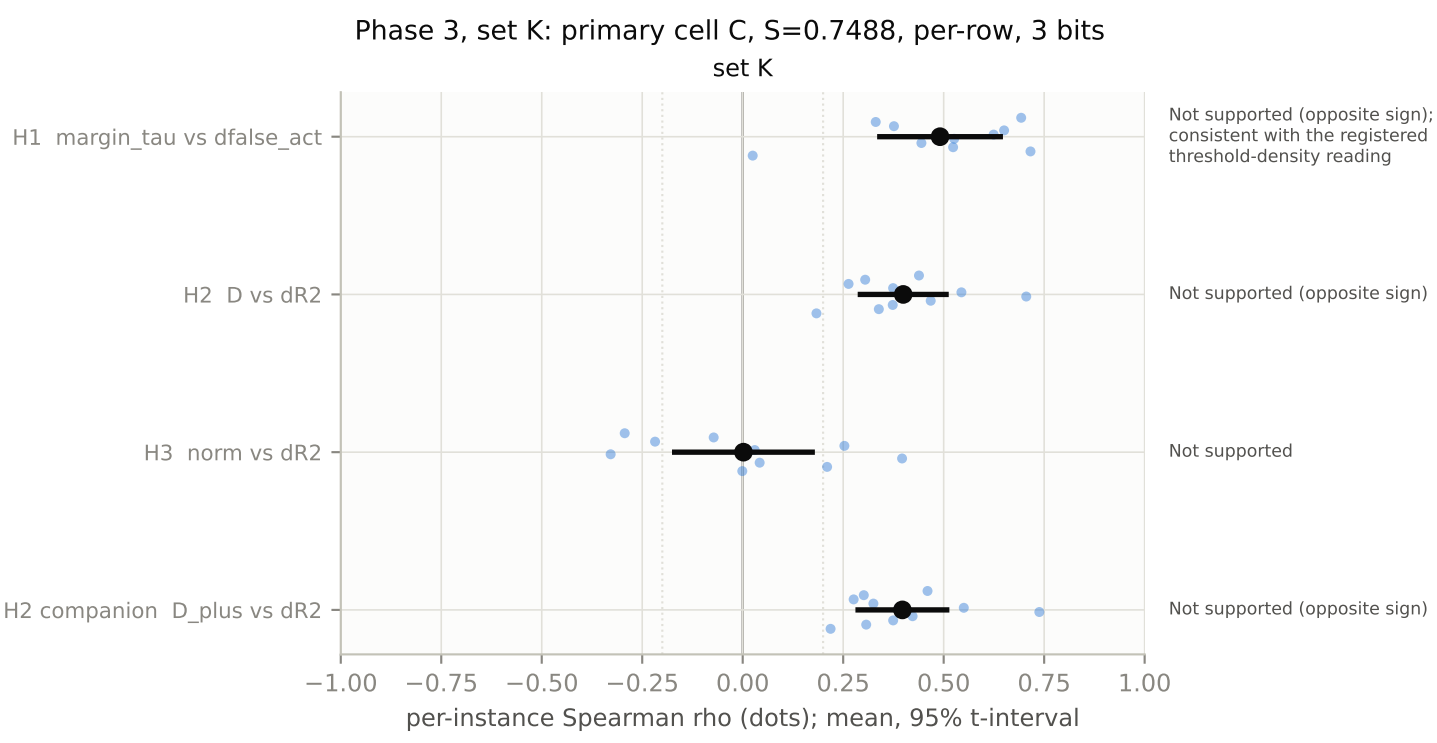
Phase 3, set K: primary cell C, S=0.7488, per-row, 3 bits
set K
H1 margin_tau vs dfalse_act
H2 D vs dR2
H3 norm vs dR2
H2 companion D_plus vs dR2
Not supported (opposite sign); consistent with the registered threshold-density reading
Not supported (opposite sign)
Not supported
Not supported (opposite sign)
−1.00
−0.75
−0.50
−0.25
0.00
0.25
0.50
0.75
1.00
per-instance Spearman rho (dots); mean, 95% t-interval