
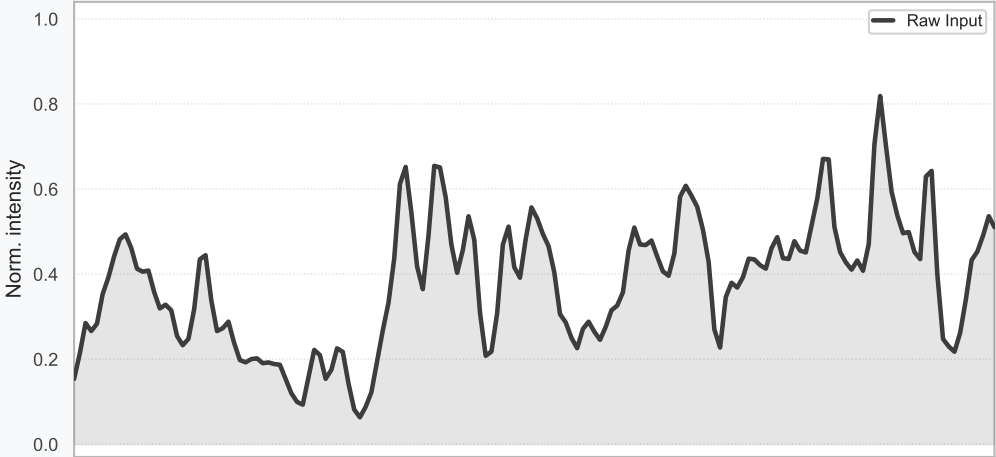




Fluorescence Microscopy · Denoising Benchmark

Anti-diagonal ROI intensity profiles



Raw Input

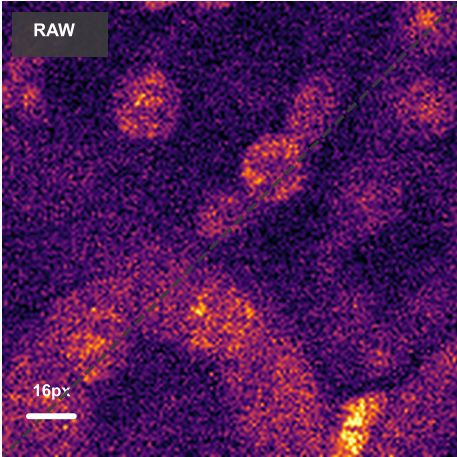

Richardson–Lucy

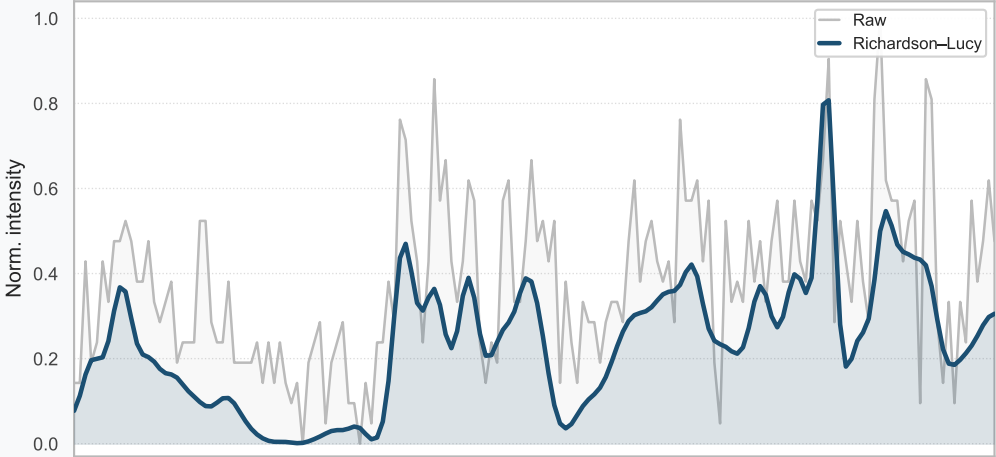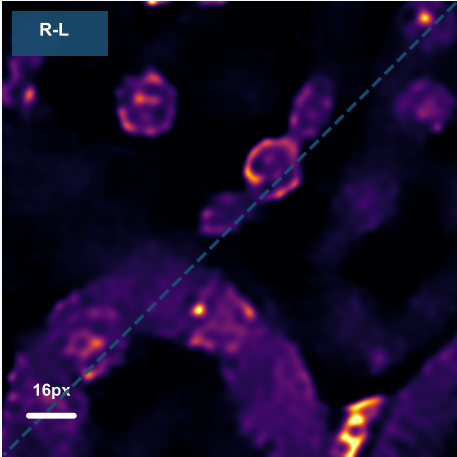

Non-Local Means

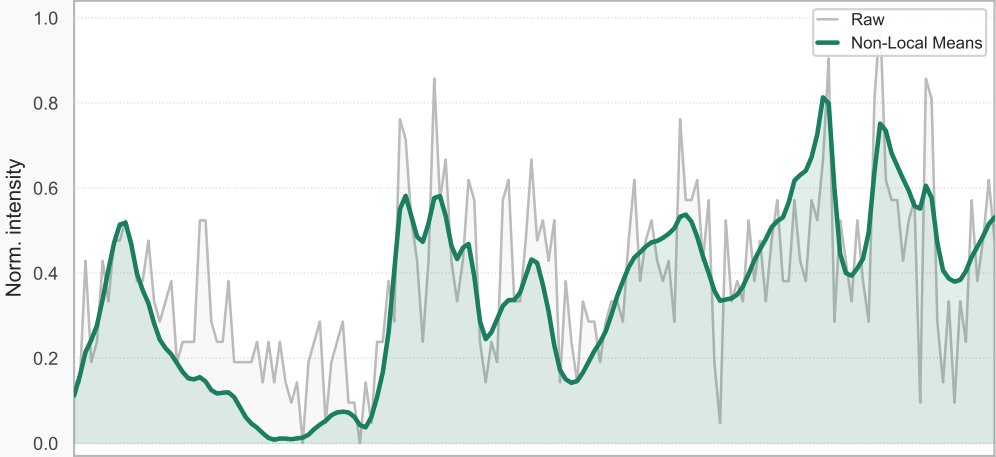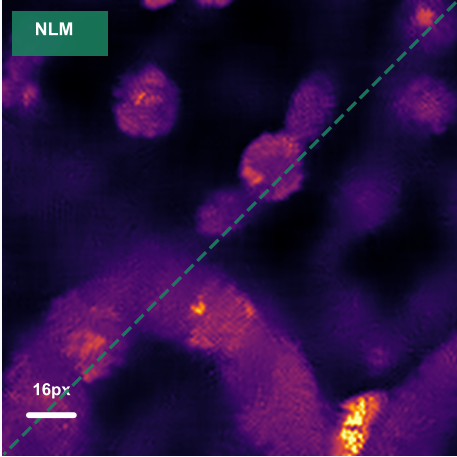

Wavelet · db4

