


# Supplementary Figure S5. Sensitivity of feasibility outputs to the patient-journey calibration

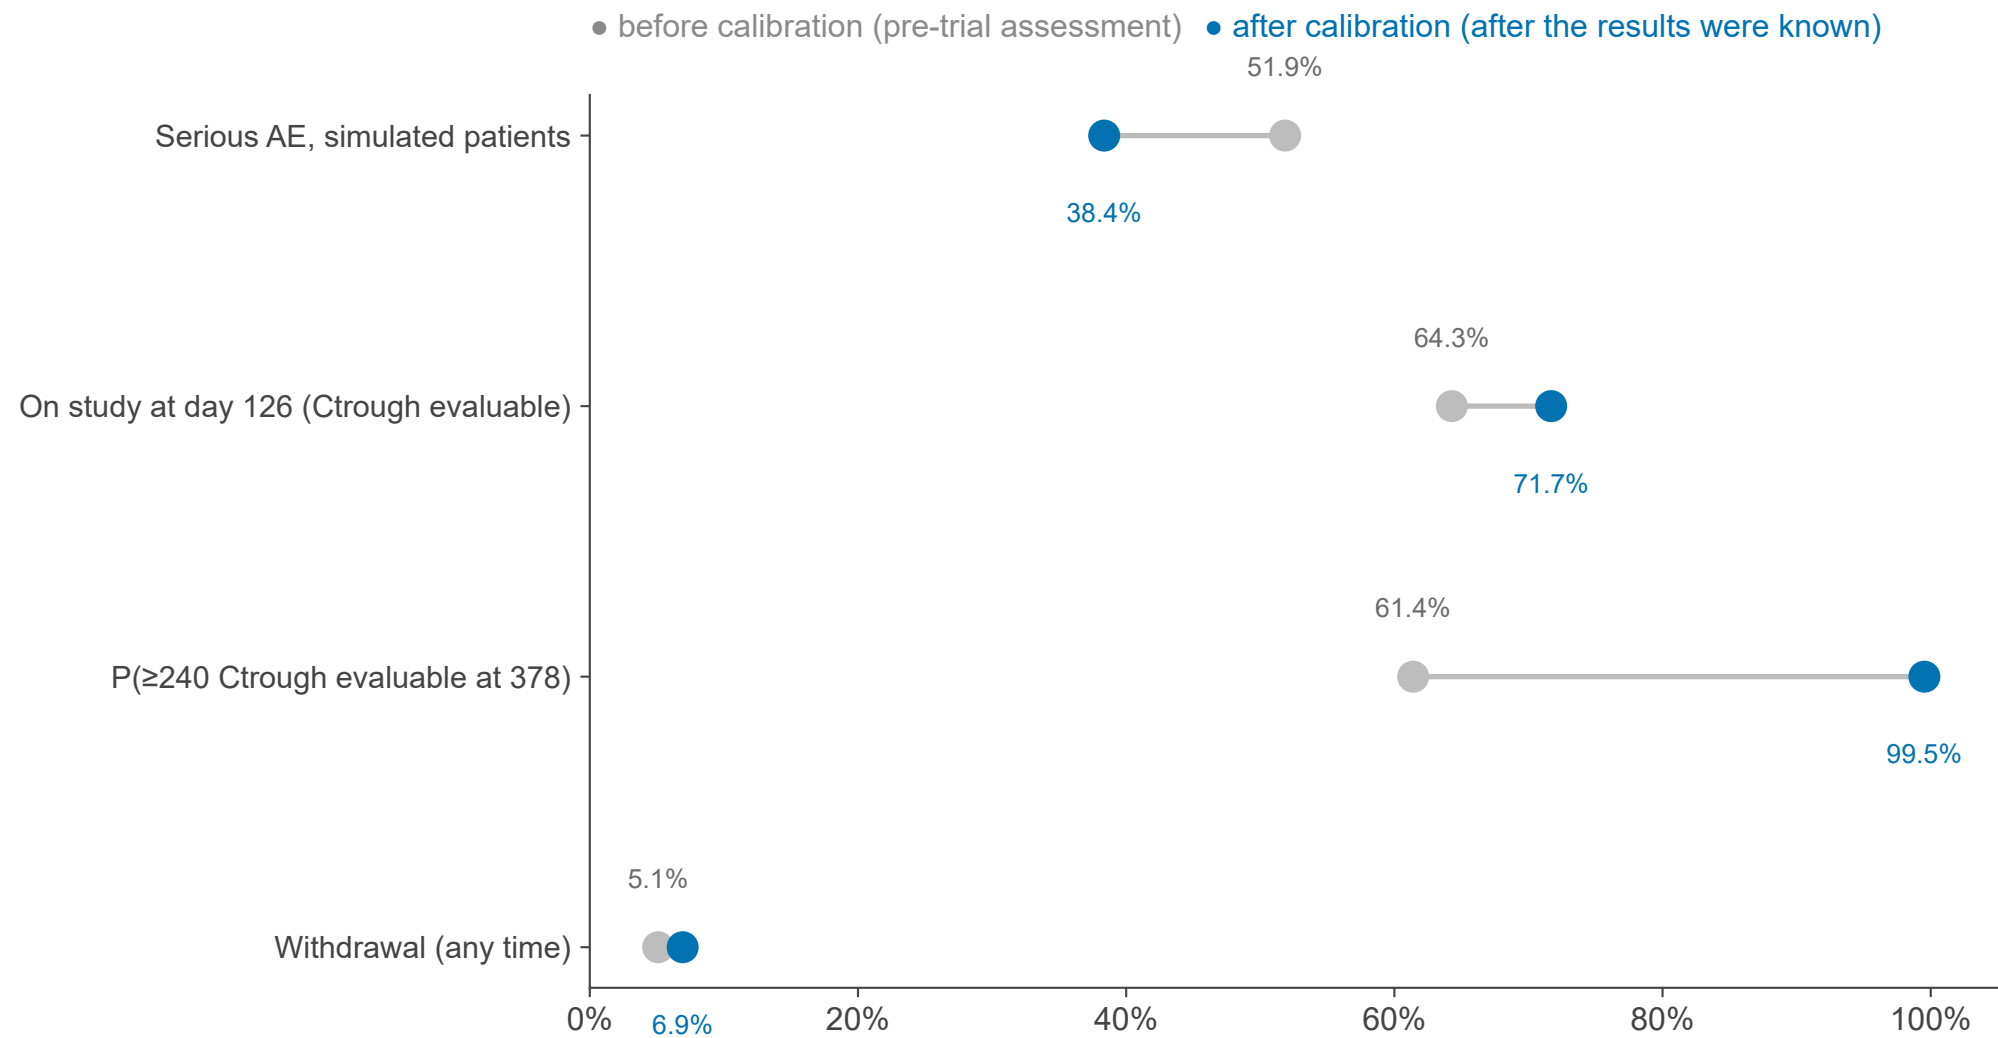

*The calibration anchors serious AEs to the evidence, takes progression from validated evidence and makes withdrawal burden-dependent.*