
Human Reproduction, 2017
doi:10.1093/humrep/dew356

human reproduction

SUPPLEMENTARY DATA

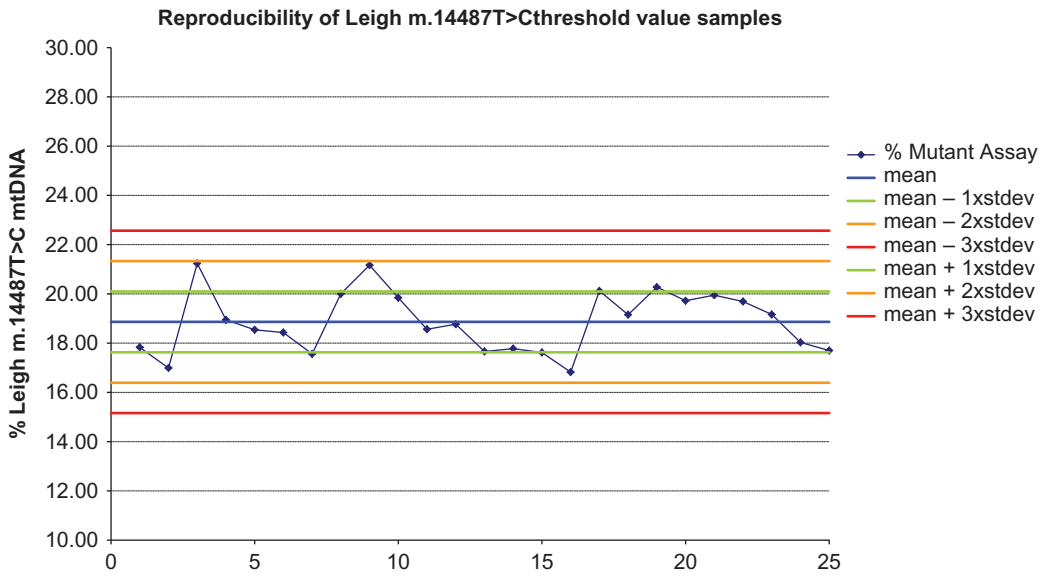

Supplementary Figure S1 Shewhart chart of m.14487 T>C. To demonstrate reproducibility and verify a valid PCR amplification, five reference samples with a mutation load around the threshold value (18% for the Leigh m.14487 T>C) were included in every PCR series for validation. The reference amplicons were diluted to a single blastomere equivalent amount, approximately 12 500–75 000 mtDNA copies. A total of 25 of these reference samples were amplified in five separate PCR runs during protocol setup and the data were used to construct a Shewhart chart which showed the mean, the mean ± 1 SD, the mean ± 2 SD and the mean ± 3 SD. Four of five control observations must fall within the mean ± 2 SD to approve the PGD PCR analysis data with a % mutation load around the threshold value. Data were rejected if more than one control sample exceeded the mean ± 3 SD limit.