Interlaboratory Study - Temperature

General Information

Device Information

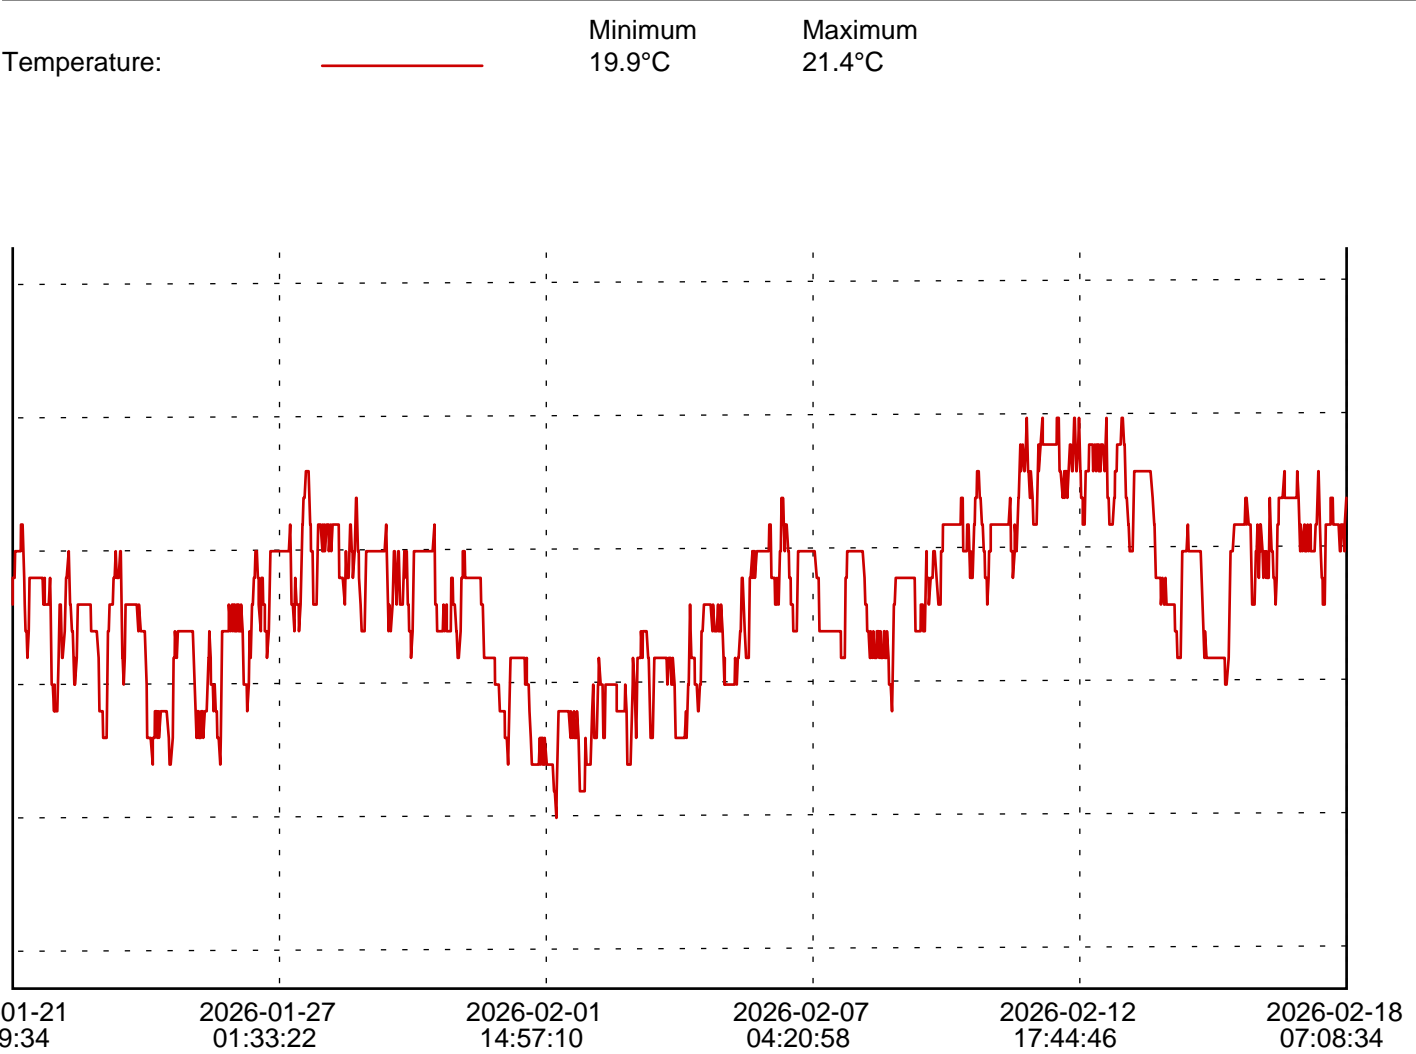|			
Model:	DL-200T	Serial ID:	DL200_2106040081
Owner:		Logger ID:	0000

Data Logger Setting

Record Start Condition:	Immediately until memory full	Start Time:	2026-01-21 12:09:34
Sampling Rate:	1Min,0Sec	Stop Time:	2026-02-18 07:08:34
Data Count:	40020	Recorded Time:	27Days,18Hours,59Min,0Sec

Alarm Status

Alarm:	Enable

Graph

		Minimum	Maximum
Temperature:	——————	19.9°C	21.4°C