

Analysis of Somalogic Plasma Data: Kidney Precision Medicine Project V2

Updated 2024-01-22




Overview

Five samples from each of two participants were included in replicate in these data to check the between run variability. Coefficients of variation (CV) were calculated by measure (n = 7,596 measures) within participant, and the mean CV was then calculated between participants for each measure (e.g. CVs calculated for measure x separately for each participant y_1 and participant y_2 , producing two CVs for measure x , cv_{x1} and cv_{x2} . The mean of the participant specific CVs was taken to provide a measure specific mean CV for measure x , $\overline{cv_x}$).

Results

RAW DATA

Distribution of Mean CVs from Somalogic Plasma Analyses

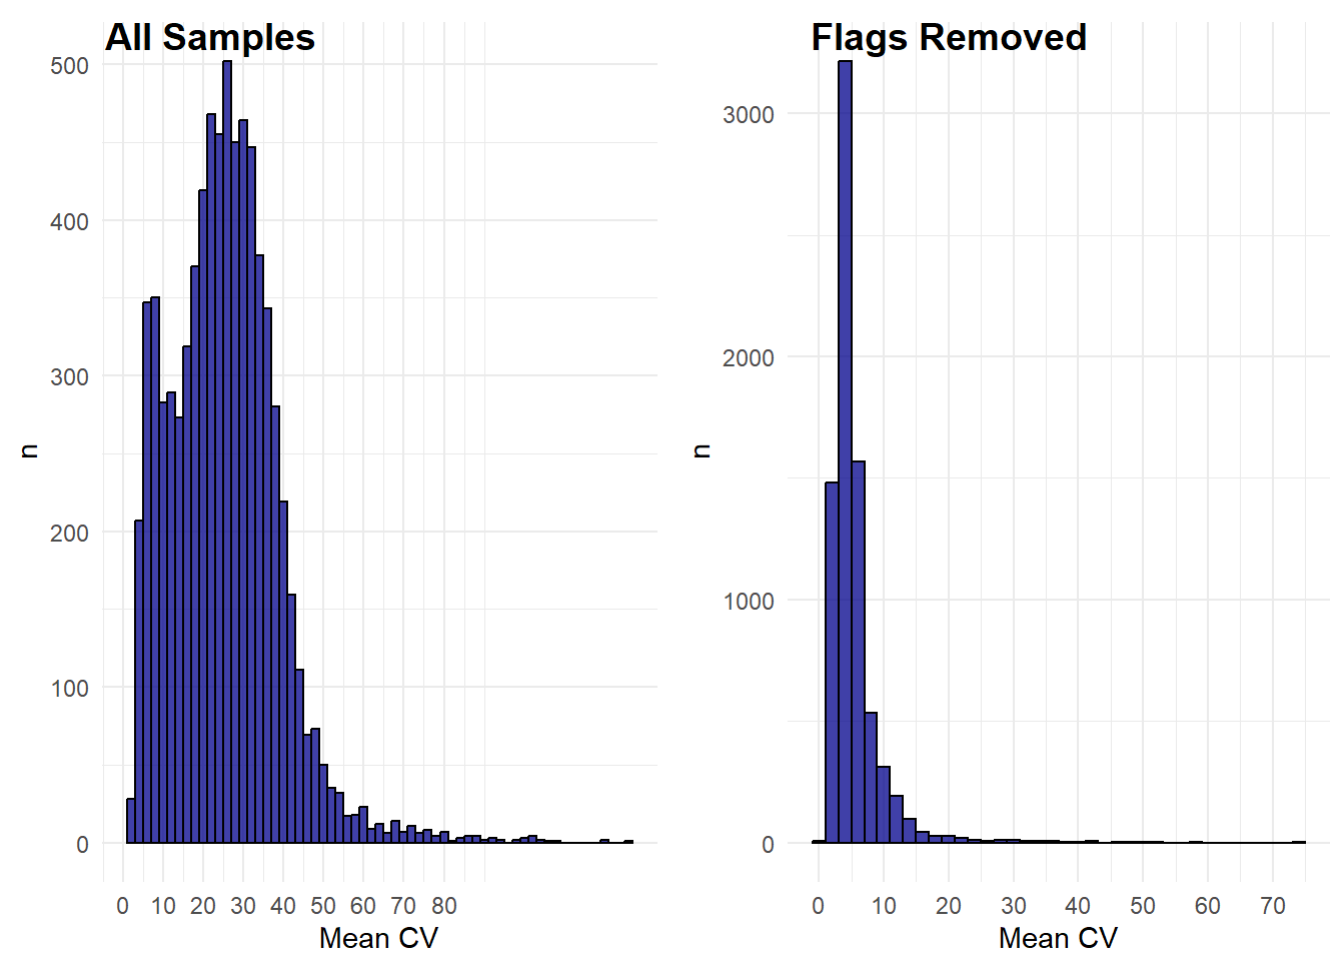

ANML Normalized

Distribution of Mean CVs from Somalogic Plasma Analyses

