
Highly-Accurate Manipulator Calibration via Extended Kalman Filter-Incorporated Residual Neural Network: Supplementary File

This is the supplementary file for the paper entitled *Highly-Accurate Manipulator Calibration via Extended Kalman Filter-Incorporated Residual Neural Network*. It mainly contains a) the evaluation metrics and position accuracy of experimental models on D1 and D2, and b) three supplementary tables recording the performance of the comparison models and calibration results.

PART. I. EVALUATION METRICS AND POSITION ACCURACY

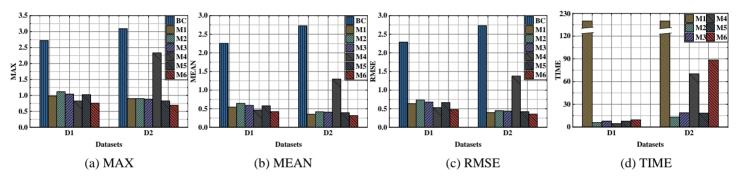

In (d), truncation marker is added to keep the bar graph clear because of the excessive time cost of M1.

Fig. 5. The evaluation metrics of experimental results on D1 and D2.

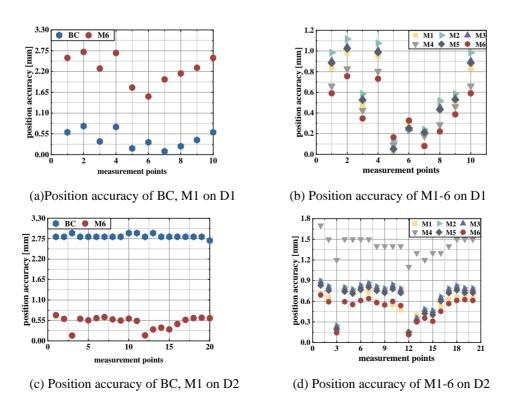


Fig. 6. The position accuracy of the measuring point on D1 and D2 of each algorithm. (a), (c) Compared with BC (before calibration), the position accuracy of D-H parameters compensated by M6 is significantly optimized on both D1 and D2. (b), (d) Moreover, On D1, M6 performs better than other five algorithms 80% of the time and 85% of the time on D2.

PART. II. SUPPLEMENTARY TABLES

 $\label{thm:table} \mbox{TABLE\,III}$ The Comparative Test Error Calibration Results.

| Dataset | Metric(mm) | BC | M1 | M2 | M3 | M4 | M5 | M6 |
|------------|------------|--------|--------|--------|--------|--------|--------|--------|
| | MEAN | 2.2557 | 0.5457 | 0.6444 | 0.5903 | 0.4643 | 0.5781 | 0.4200 |
| D 1 | RMSE | 2.2869 | 0.6364 | 0.7360 | 0.6793 | 0.5277 | 0.6663 | 0.4756 |
| | MAX | 2.7180 | 0.9815 | 1.1150 | 1.0406 | 0.8280 | 1.0226 | 0.7557 |
| D2 | MEAN | 2.7261 | 0.3512 | 0.4179 | 0.4081 | 1.2974 | 0.3921 | 0.3160 |
| | RMSE | 2.7283 | 0.3971 | 0.4471 | 0.4369 | 1.3808 | 0.4209 | 0.3589 |
| | MAX | 3.0906 | 0.8994 | 0.9013 | 0.8822 | 2.3339 | 0.8297 | 0.6921 |

TABLE IV

TIME COST OF METHODS M1-M6 ON RMSE.

| Dataset | Item | M1 | M2 | M3 | M4 | M5 | M6 |
|------------|-----------|----------|---------|---------|---------|---------|---------|
| D1 | Iteration | 40 | 10 | 10 | 14 | 5 | 5 |
| D 1 | Time(s) | 220.9302 | 5.8721 | 7.7915 | 4.4923 | 7.6834 | 9.4193 |
| D2 | Iteration | 50 | 10 | 10 | 15 | 6 | 6 |
| D2 | Time(s) | 220.5976 | 13.1632 | 18.7527 | 70.2240 | 18.3151 | 88.5746 |

 $\label{thm:constraint} TABLE\ V$ D-H Parameter Deviations of ABB IRB120 Manipulator After Calibration.

| | EKF | | | | ResNN | | | | EKF-ResNN Calibrator | | | |
|-------|-----------------------------|------------------------------|--------------------------------------|------------------------|-----------------------------|----------------------------|--------------------------------------|------------------------|------------------------------|----------------------------|----------------------------------|------------------------|
| Joint | $\Delta \alpha_{i-1}/\circ$ | $\Delta a_{i-1}/\mathrm{mm}$ | $\Delta 	heta_{i	ext{-}1}$ / \circ | $\Delta d/\mathrm{mm}$ | Δα _{i-1} /∘ | $\Delta a_{i-1}/\text{mm}$ | $\Delta 	heta_{i	ext{-}1}$ / \circ | $\Delta d/\mathrm{mm}$ | ∆ α _{i-1} /∘ | $\Delta a_{i-1}/\text{mm}$ | $\Delta 	heta_{i	ext{-}1}/\circ$ | $\Delta d/\mathrm{mm}$ |
| 1 | 0.0000 | 0.0003 | 0.0000 | -0.0009 | 0 | 0 | 0.0017 | 0 | 0.0000 | 0.0003 | 0.0002 | -0.0009 |
| 2 | 0.0000 | -0.0009 | 0.0000 | -0.0001 | 0 | 0 | 0.0022 | 0 | 0.0000 | -0.0009 | -0.0005 | -0.0001 |
| 3 | 0.0000 | 0.0000 | 0.0003 | -0.0001 | 0 | 0 | 0.0024 | 0 | 0.0000 | 0.0000 | 0.0010 | -0.0001 |
| 4 | 0.0000 | 0.0000 | 0.0000 | 0.0002 | 0 | 0 | 0.0014 | 0 | 0.0000 | 0.0000 | -0.0001 | 0.0002 |
| 5 | 0.0000 | 0.0000 | 0.0000 | 0.0001 | 0 | 0 | 0.0011 | 0 | 0.0000 | 0.0000 | -0.0009 | 0.0001 |
| 6 | 0.0000 | 0.0001 | 0.0000 | 0.0000 | 0 | 0 | 0.0018 | 0 | 0.0000 | 0.0001 | -0.0008 | 0.0000 |