



ITEM NO.	PartNo	DESCRIPTION	Default/ QTY.
1	2020-10-09 MOUNT YOKE	MOUNT YOKE	1
2	2020-06-17 MOUNT CLAMP	MOUNT CLAMP BODY	2
3	2020-06-17 MOUNT CLAMP	MOUNT CLAMP BODY	2
4	2020-06-17 MOUNT CLAMP KNOB	MOUNT CLAMP KNOB	2
5	2022-05-27 FIBERGLASS THREADED ROD	3/8--16 FIBERGLASS THREADED ROD	2
6	McMASTER-CARR ITEM #9248A247	10-24 x 1" BRASS FLAT HEAD	4
7	McMASTER-CARR #92991A240	10-24 Brass Set Screw	2
8	2022-05-27 STEREOTACTIC PIN	STEREOTACTIC PIN	2
9	McMASTER-CARR #97715A267	1/4"-20 X 1" BRASS BUTTON HEAD	4

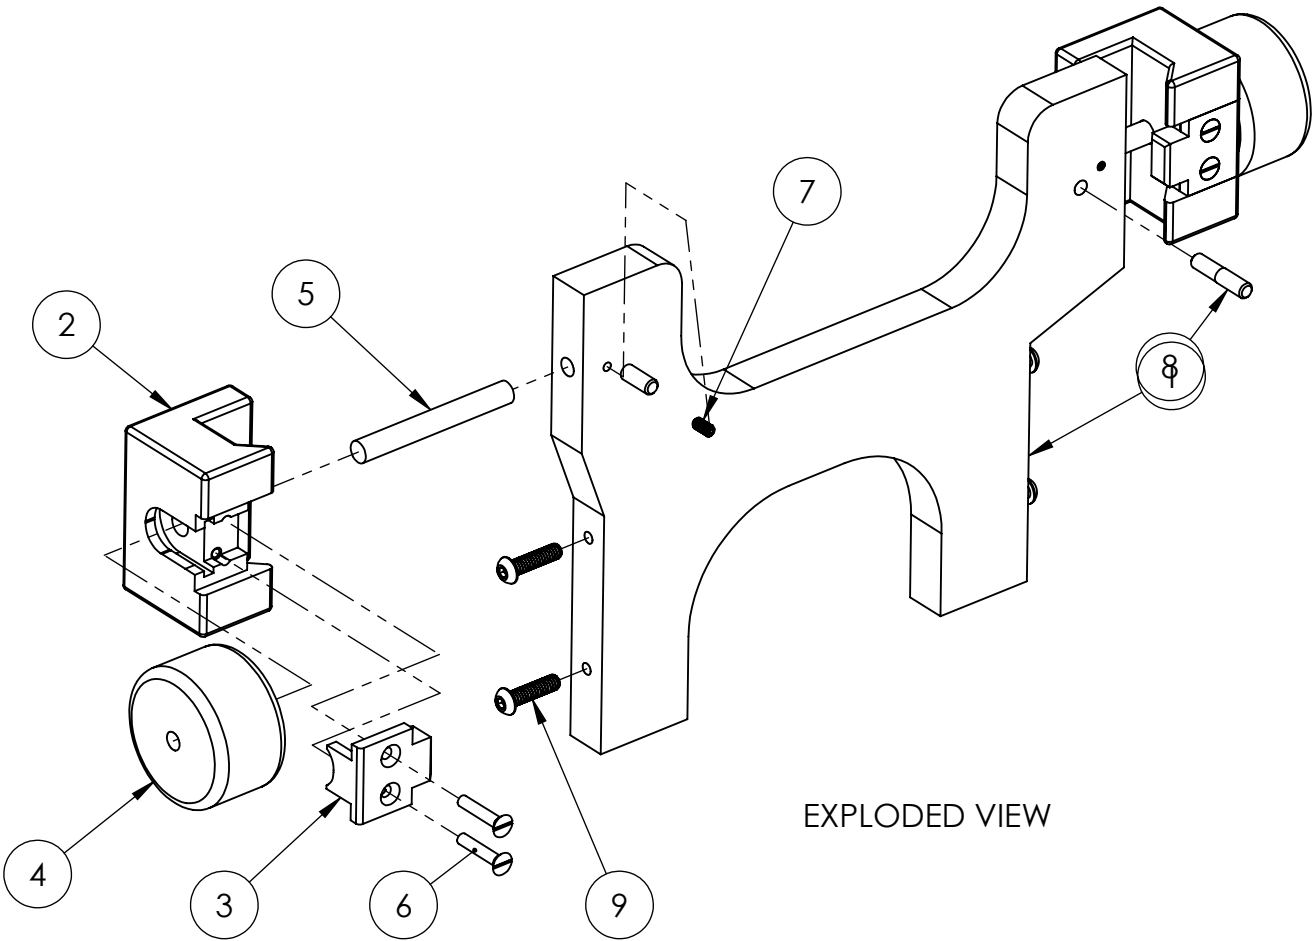


EXPLODED VIEW

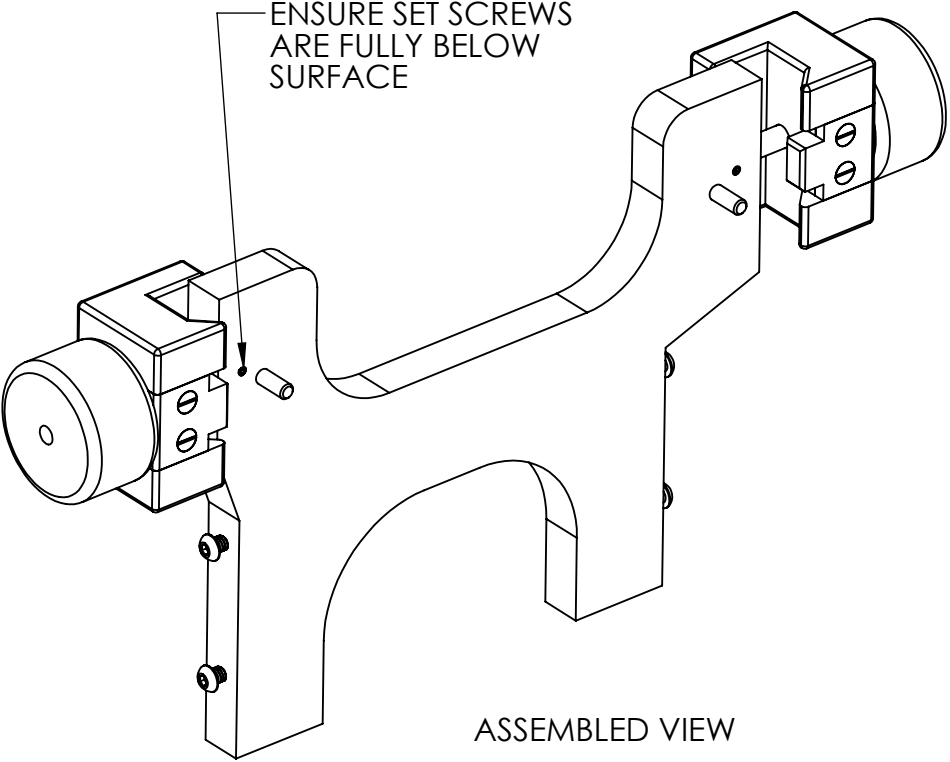

ASSEMBLED VIEW

University of Utah Dept. of Radiology  
729 Arapleen Dr., Salt Lake City, UT 84108  
Phone: (801) 585-7400 Fax: (801) 585-3592

PROPRIETARY AND CONFIDENTIAL THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY IS PROHIBITED.	DRAWN	RM	27 MAY '22	TITLE:	
	CHECKED			2020-10-09 Stereotactic mount Asm	
	UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONAL: $\pm 1/64$ " ANGULAR: $\pm 1^\circ$ TWO PLACE DECIMAL: $\pm 0.015$ THREE PLACE DECIMAL: $\pm 0.003$ FOUR PLACE DECIMAL: $\pm 0.001$			MATERIAL	REV
				--	A
QTY: 1		SCALE: 1:3		SHEET 1 OF 6	





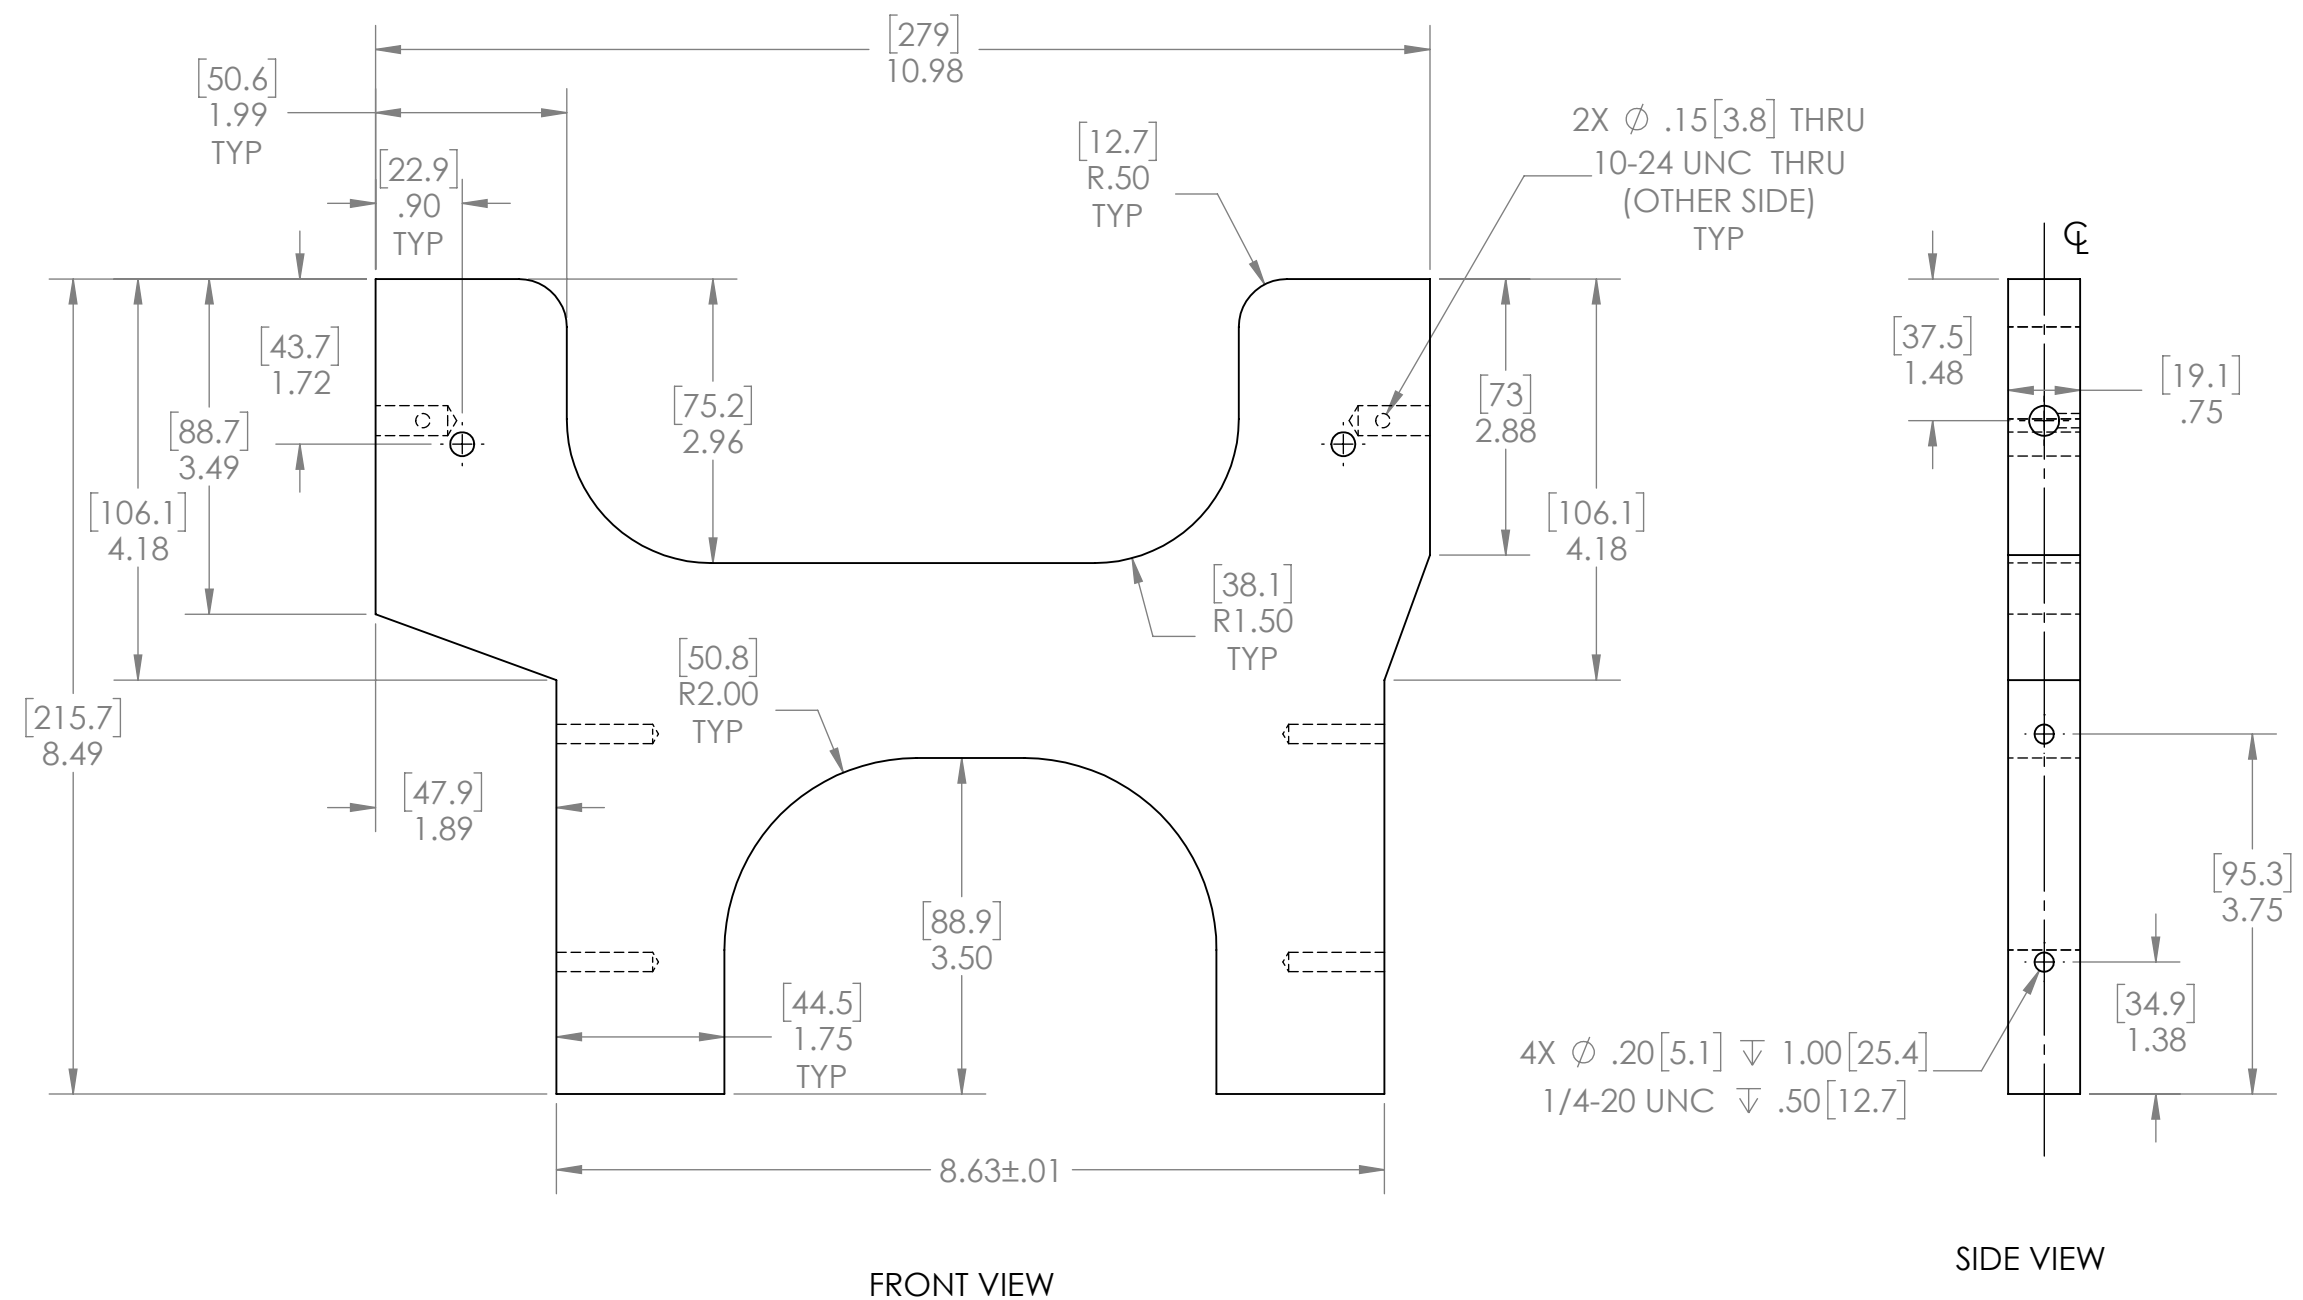


MOUNT YOKE

NOTE: [DUAL-DIMENSION UNITS IN MM]

**University of Utah Dept. of Radiology**  
729 Arapeen Dr., Salt Lake City, UT 84108  
Phone: (801) 585-7400 Fax: (801) 585-3592




<b>PROPRIETARY AND CONFIDENTIAL</b> THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY IS PROHIBITED.	DRAWN	RM	27 MAY '22	TITLE:	
	CHECKED			2020-10-09 Stereotactic mount Asm	
	<u>UNLESS OTHERWISE SPECIFIED:</u> DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONAL: ±1/64" ANGULAR: ± 1° TWO PLACE DECIMAL: ±0.015 THREE PLACE DECIMAL: ±0.003 FOUR PLACE DECIMAL: ±0.001			MATERIAL WHITE DELRIN	REV A
QTY: 1		SCALE: 1:2		SHEET 2 OF 6	

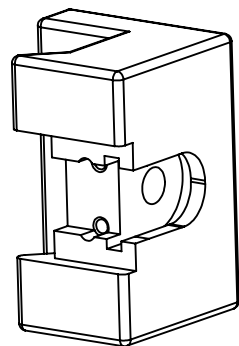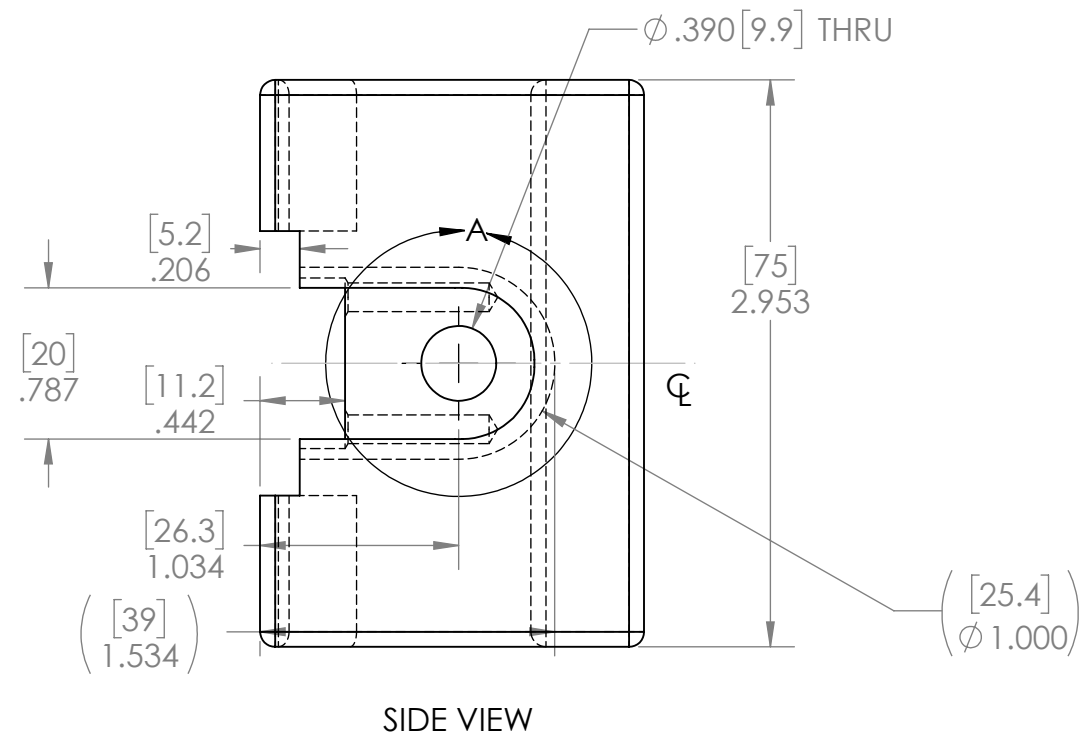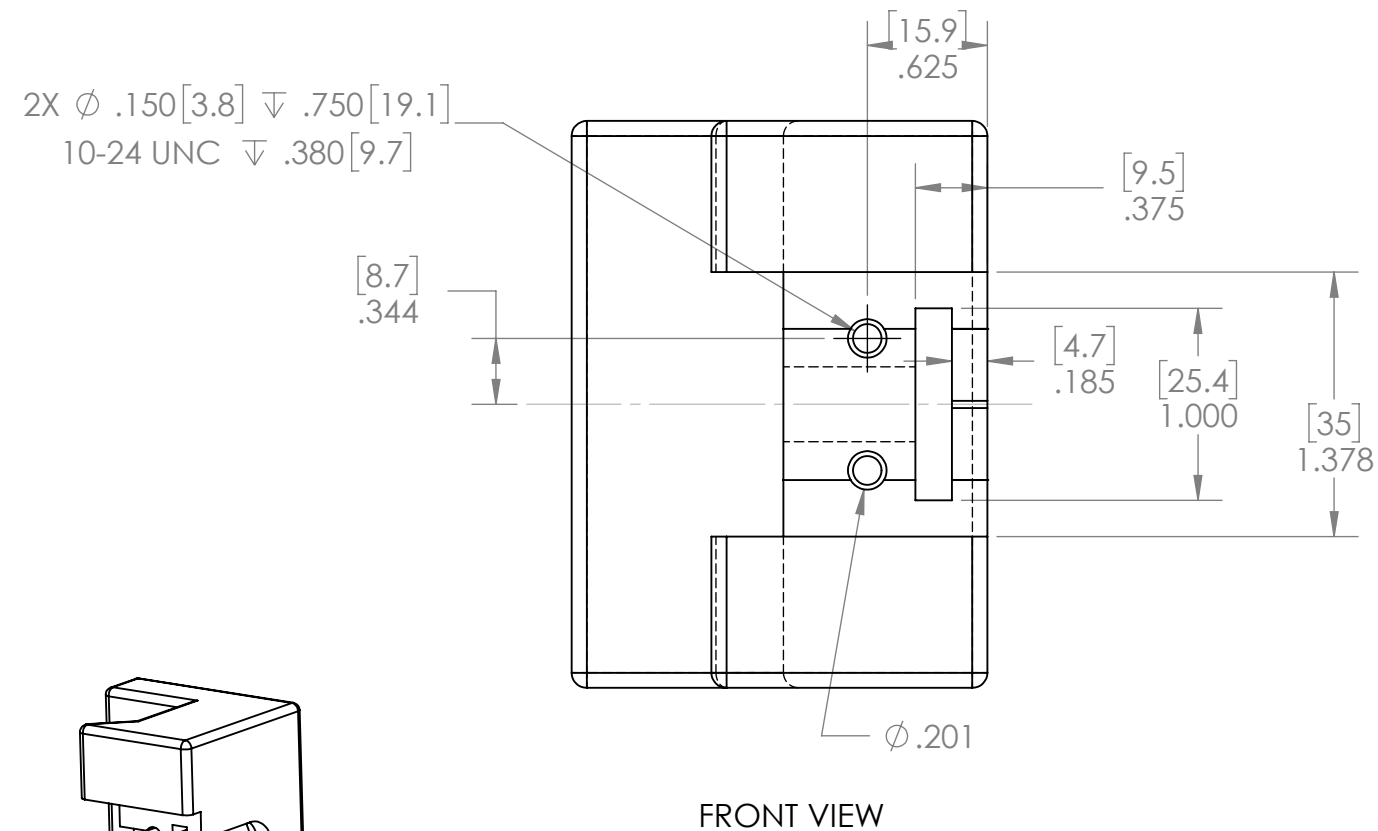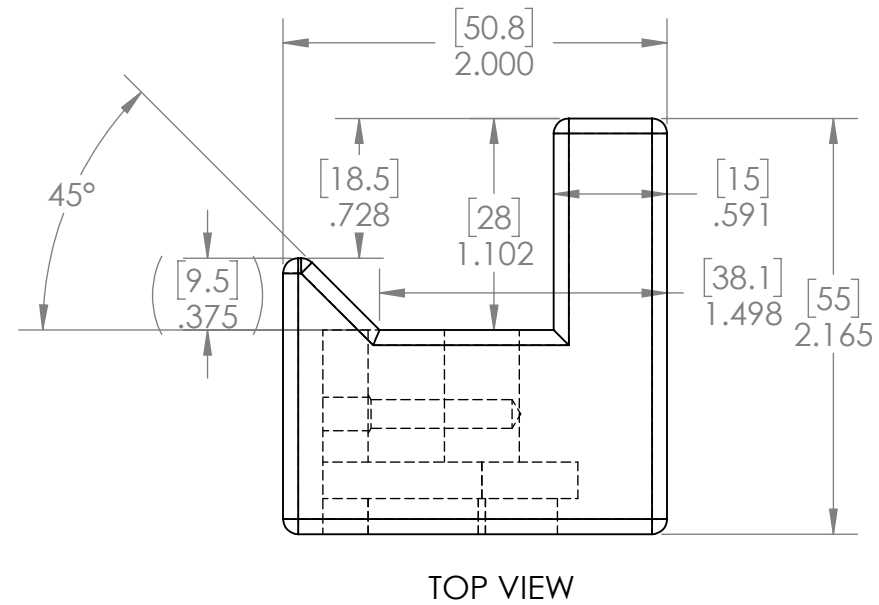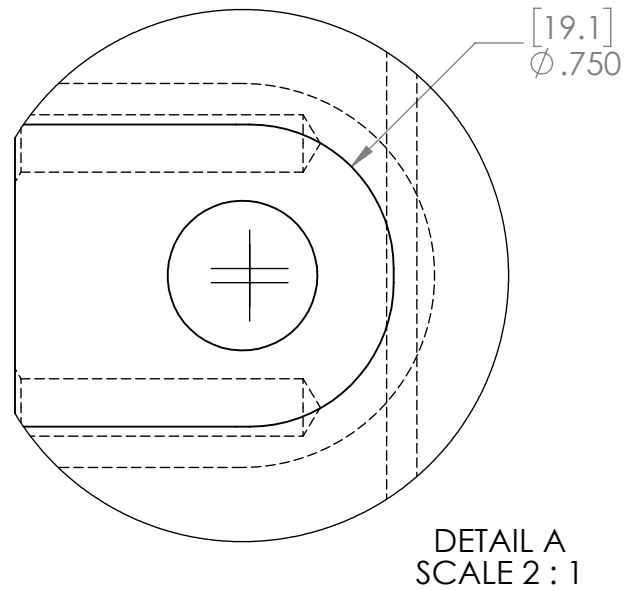

NOTE: [DUAL-DIMENSION UNITS IN MM]

**University of Utah Dept. of Radiology**  
729 Arapleen Dr., Salt Lake City, UT 84108  
Phone: (801) 585-7400 Fax: (801) 585-3592

<b>PROPRIETARY AND CONFIDENTIAL</b> THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY IS PROHIBITED.	DRAWN	RM	27 MAY '22	TITLE:	
	CHECKED			2020-10-09 Stereotactic mount Asm	
	UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONAL: $\pm 1/64$ " ANGULAR: $\pm 1^\circ$ TWO PLACE DECIMAL: $\pm 0.015$ THREE PLACE DECIMAL: $\pm 0.003$ FOUR PLACE DECIMAL: $\pm 0.001$			MATERIAL	REV
				BLACK DELRIN	A
QTY: 2		SCALE: 1:2		SHEET 3 OF 6	

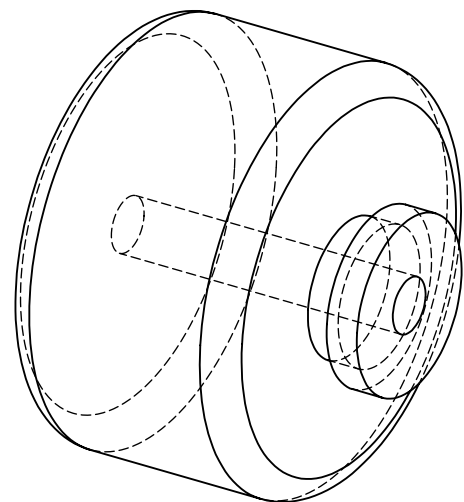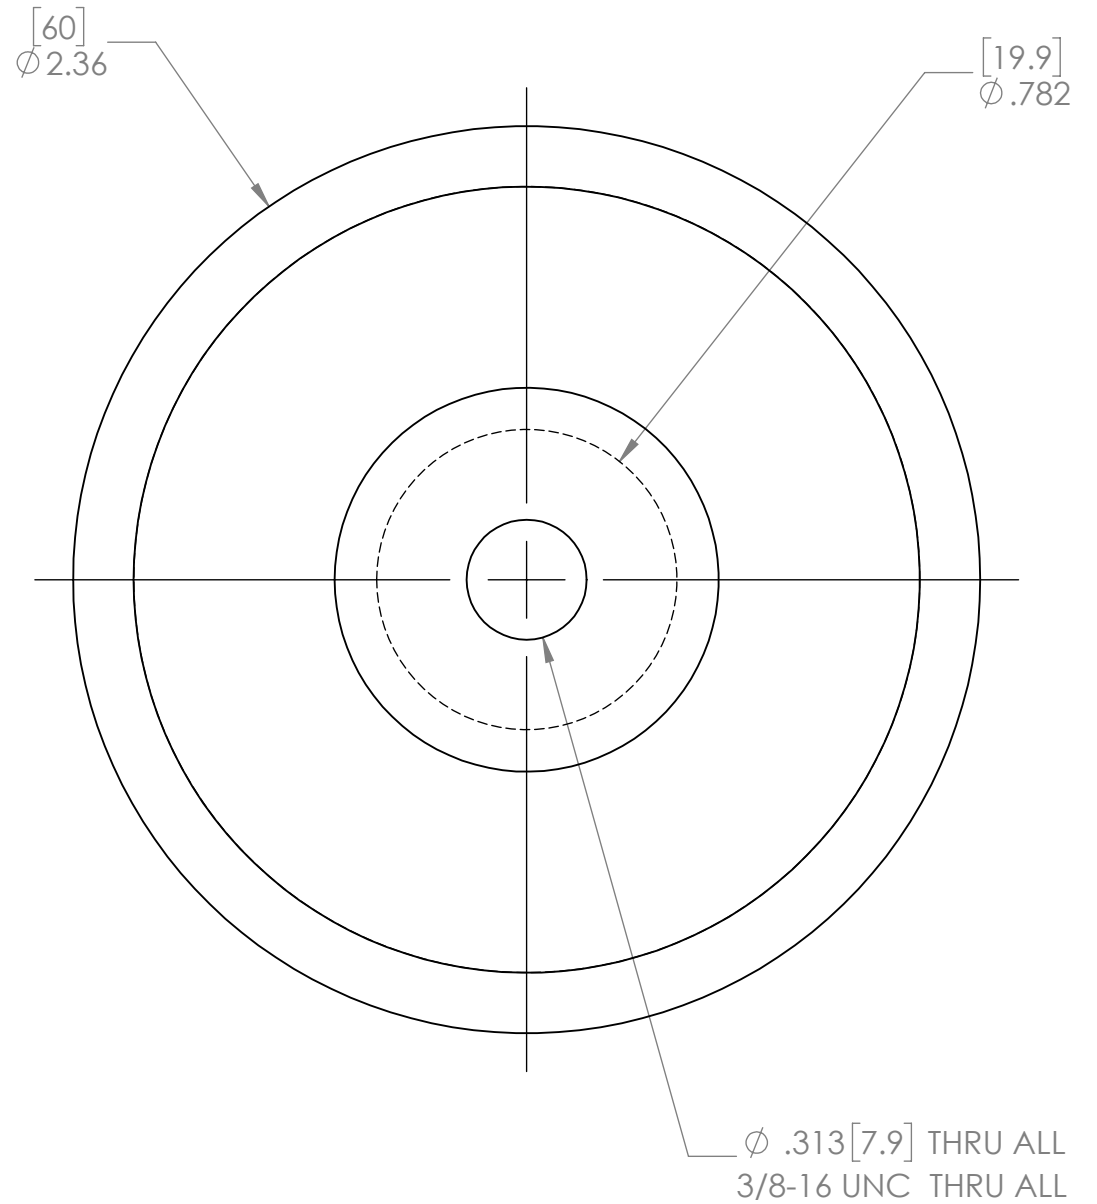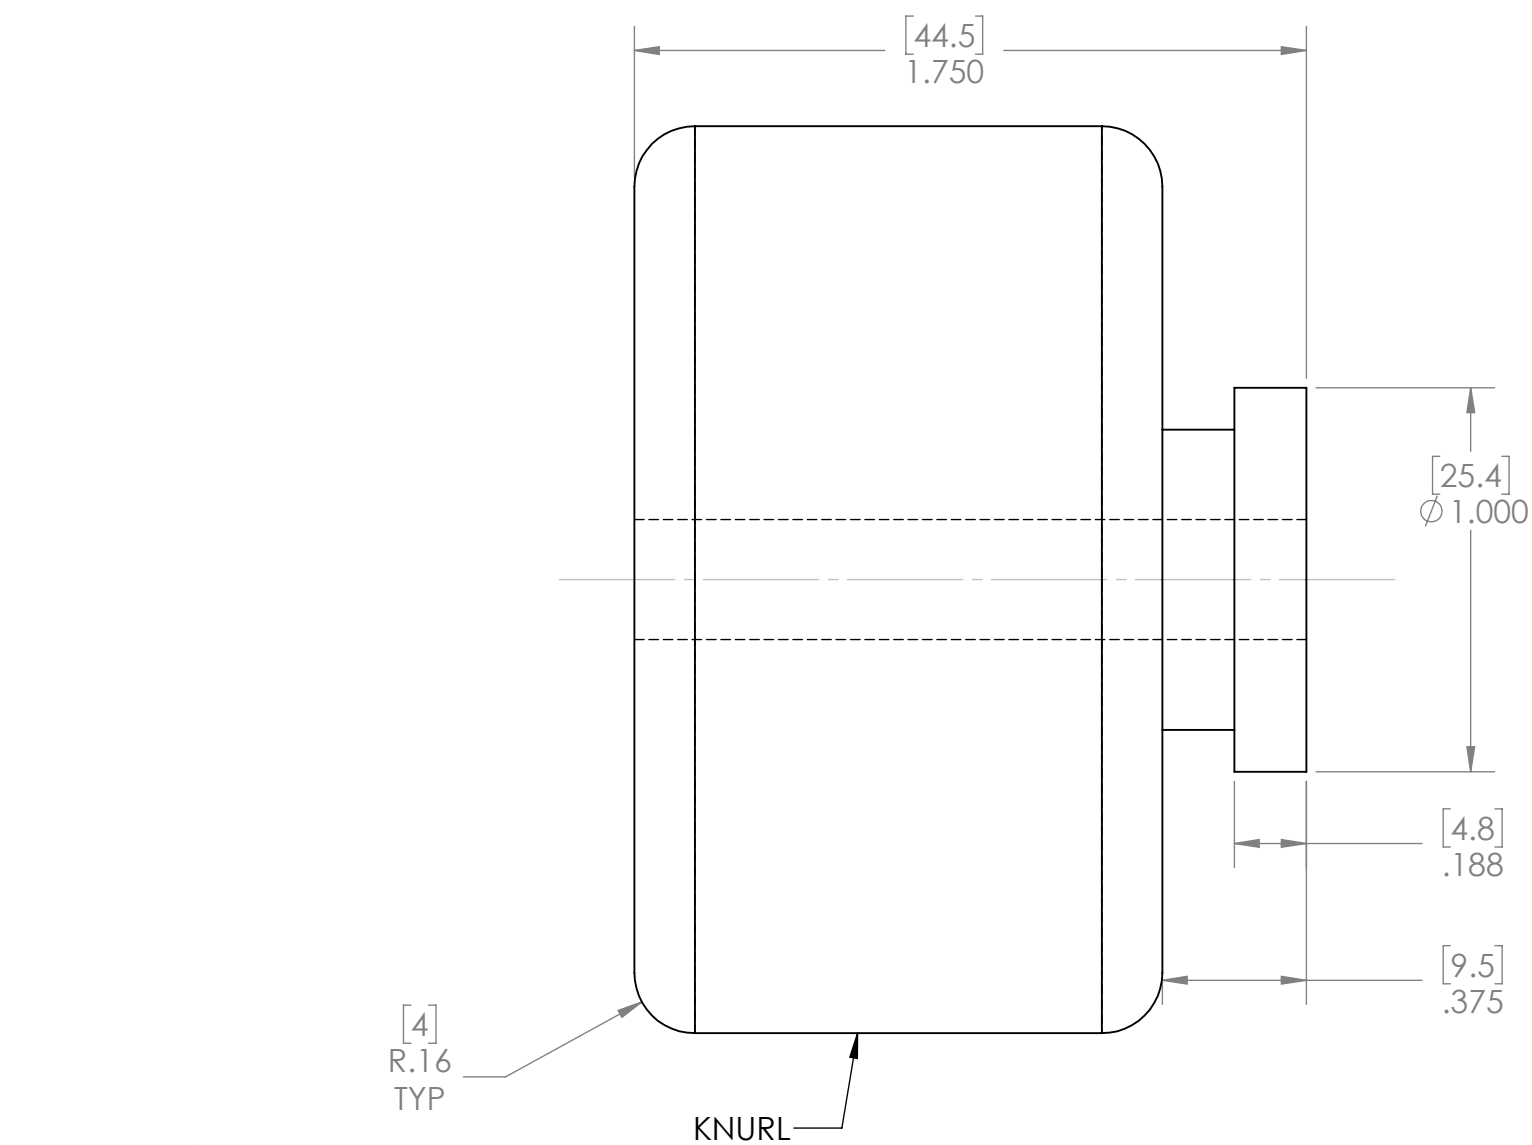


NOTE: [DUAL-DIMENSION UNITS IN MM]


**University of Utah Dept. of Radiology**  
729 Arapeen Dr., Salt Lake City, UT 84108  
Phone: (801) 585-7400 Fax: (801) 585-3592

## MOUNT CLAMP KNOB


<b>PROPRIETARY AND CONFIDENTIAL</b> THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY IS PROHIBITED.	DRAWN	RM	27 MAY '22	TITLE:	
	CHECKED			2020-10-09 Stereotactic mount Asm	
	<u>UNLESS OTHERWISE SPECIFIED:</u> DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONAL: $\pm 1/64"$ ANGULAR: $\pm 1^\circ$ TWO PLACE DECIMAL: $\pm 0.015$ THREE PLACE DECIMAL: $\pm 0.003$ FOUR PLACE DECIMAL: $\pm 0.001$			MATERIAL	REV
				BLACK DELRIN	A
QTY: 2		SCALE: 2:1		SHEET 4 OF 6	

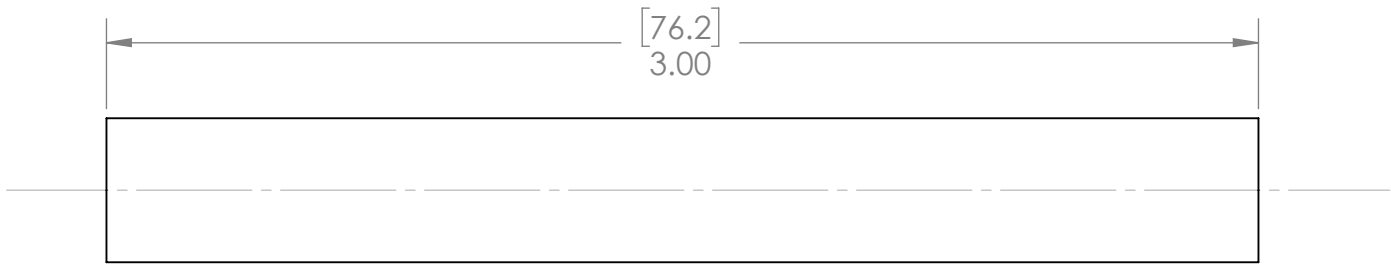

SIDE VIEW



END VIEW



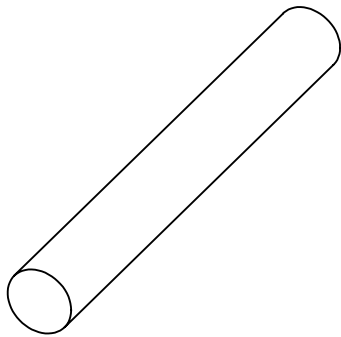


3/8--16 FIBERGLASS THREADED ROD

NOTE: [DUAL-DIMENSION UNITS IN MM]

**University of Utah Dept. of Radiology**  
729 Arapeen Dr., Salt Lake City, UT 84108  
Phone: (801) 585-7400 Fax: (801) 585-3592

PROPRIETARY AND CONFIDENTIAL  THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY IS PROHIBITED.	DRAWN	RM	27 MAY '22	TITLE:		
	CHECKED			2020-10-09 Stereotactic moun		
	<u>UNLESS OTHERWISE SPECIFIED:</u> DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONAL: ±1/64" ANGULAR: ± 1° TWO PLACE DECIMAL: ±0.015 THREE PLACE DECIMAL: ±0.003 FOUR PLACE DECIMAL: ±0.001			MATERIAL		REV
				3/8-16 FIBERGLASS THREADED ROD		A
				QTY: 2	SCALE: 2:1	SHEET 5 OF 6

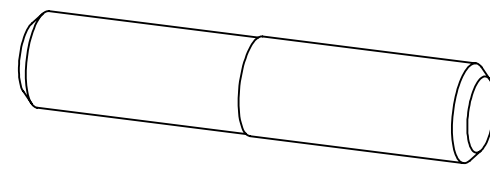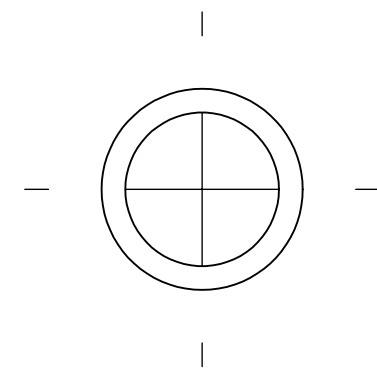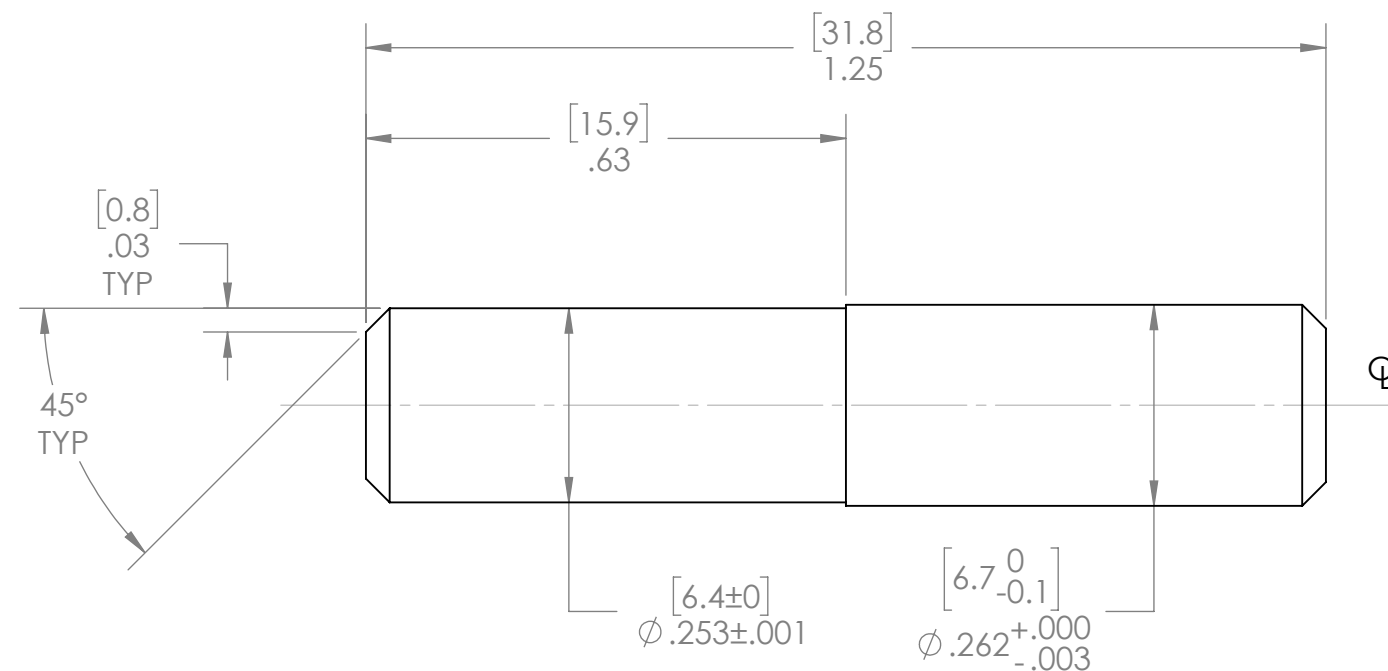

NOTE: [DUAL-DIMENSION UNITS IN MM]

**University of Utah Dept. of Radiology**  
729 Arapeen Dr., Salt Lake City, UT 84108  
Phone: (801) 585-7400 Fax: (801) 585-3592

<b>PROPRIETARY AND CONFIDENTIAL</b>  THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF UNIVERSITY OF UTAH DEPT. OF RADIOLOGY IS PROHIBITED.	DRAWN	RM	27 MAY '22	TITLE:		
	CHECKED			2020-10-09 Stereotactic mount		
	<u>UNLESS OTHERWISE SPECIFIED:</u> DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONAL: ±1/64" ANGULAR: ± 1° TWO PLACE DECIMAL: ±0.015 THREE PLACE DECIMAL: ±0.003 FOUR PLACE DECIMAL: ±0.001					
				MATERIAL		REV
				BRASS		A
QTY: 2		SCALE: 2:1		SHEET 6 OF 6		

STEREOTACTIC PIN