



Utilize the imaging capabilities of IVUS

to assist in reducing radiation during IVUS guided EVAR procedures


Radiopaque and inked catheter shaft markers facilitate low contrast and low radiation procedures

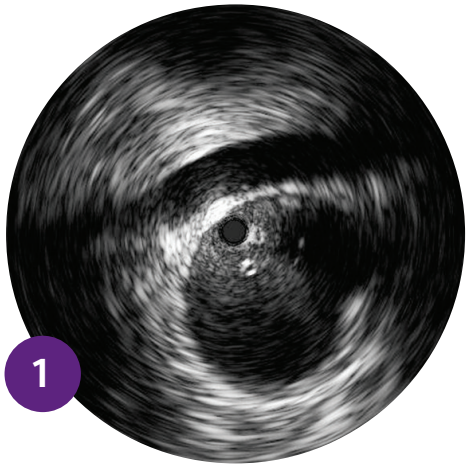

Renal vein and left renal artery

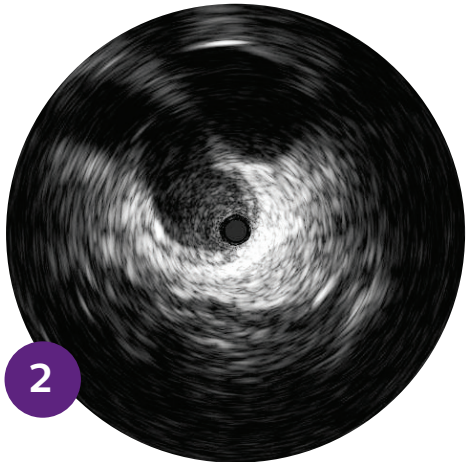

External iliac artery with internal iliac (hypogastric) branch

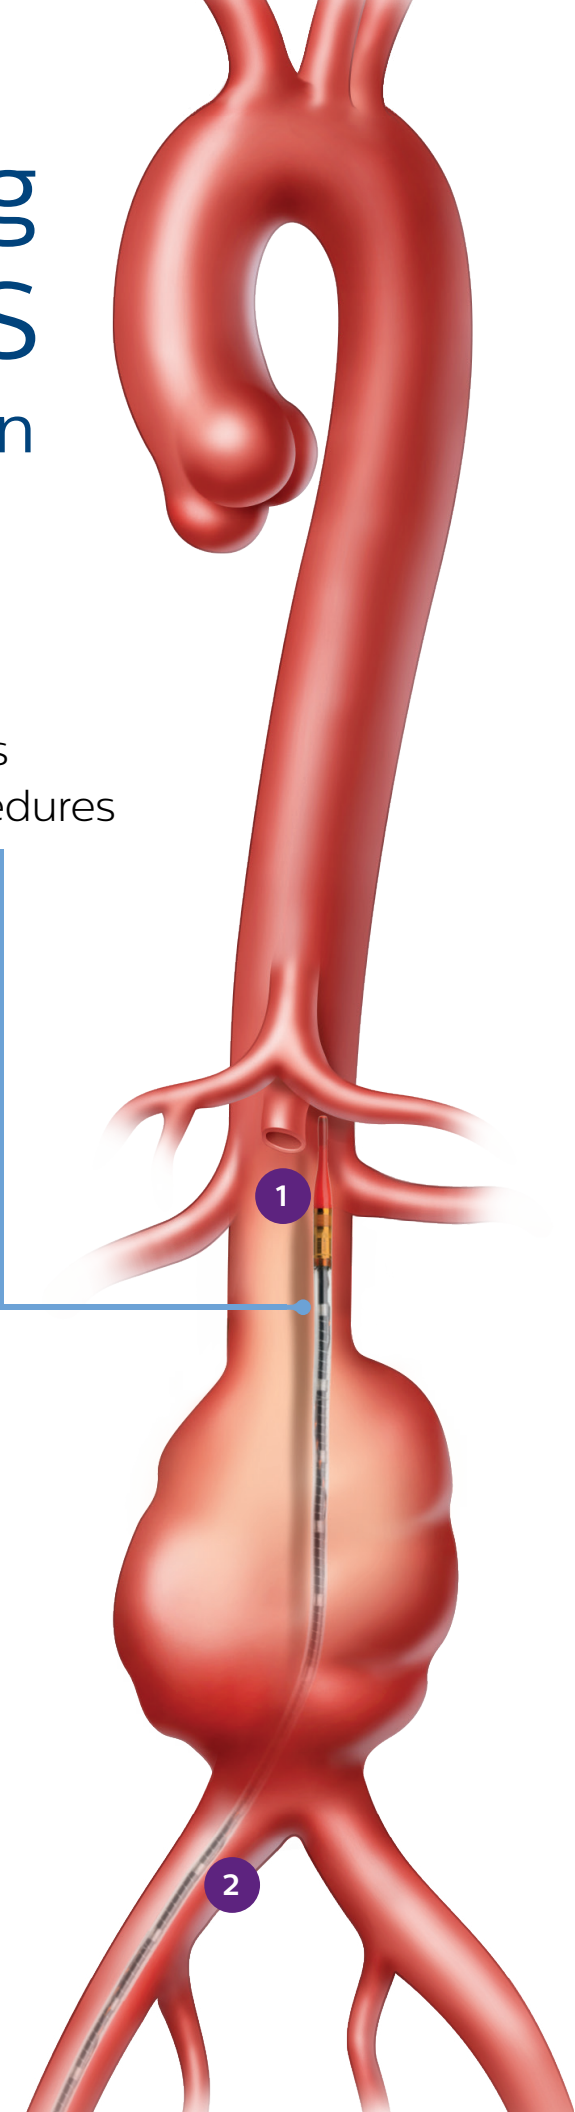

©2019 Koninklijke Philips N.V. All rights reserved.
Approved for external distribution.
D041368-00 012019

Philips
3721 Valley Centre Drive, Suite 500
San Diego, CA 92130 USA
www.philips.com/IGTdevices

PHILIPS


Visions PV .035

Digital IVUS catheter





Help reduce
procedural contrast use
and radiation time
with IVUS guided EVAR procedures

Features and **benefits**

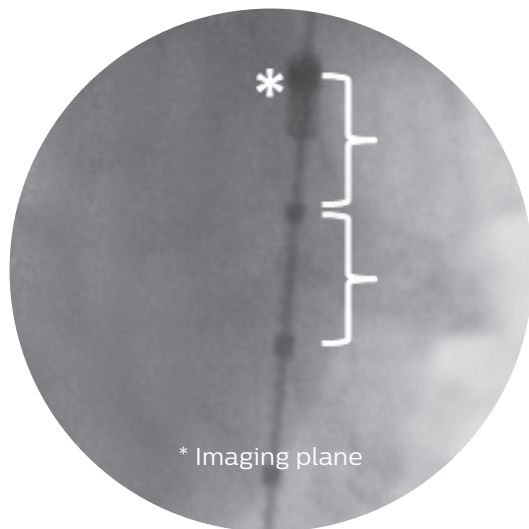

25 radiopaque markers,
1 cm apart, on distal shaft
Visible RO markers spaced 1 cm apart allow for
quick length measurements.

Inked markers,
1 cm apart, on proximal shaft
Pull back the IVUS catheter and count the
external inked markers on proximal shaft to
facilitate length assessments.

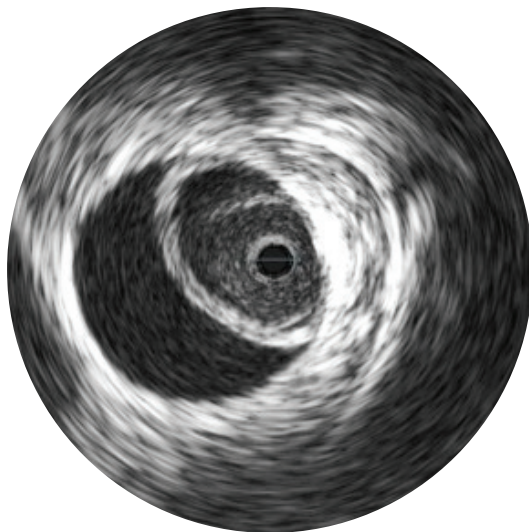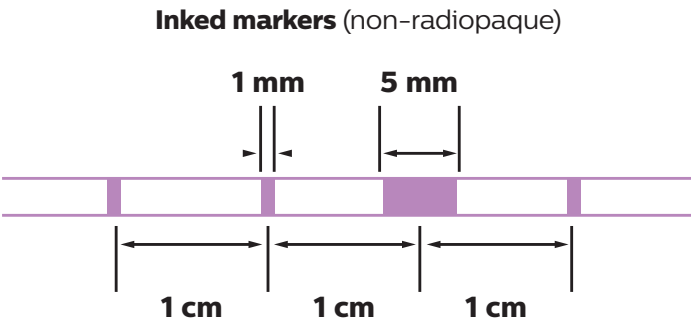


IVUS imaging

- Confirms position in true lumen versus false lumen
- Provides real-time diameter measurements
- Assesses vessel morphology


1. Hoshina, et al. A Retrospective Study of Intravascular Ultrasound use in Patients Undergoing Endovascular Aneurysm Repair: Its Usefulness and a Description of the Procedure. Eur J Vasc Endovasc Surg. 2010;40:559-563.
2. von Segesser, et al. Routine Use of Intravascular Ultrasound for Endovascular Aneurysm Repair: Angiography is not Necessary. Eur J Vasc Endovasc Surg. 2002;23:537-542).

All IVUS images: Data on file.

Study data reported a reduction in contrast¹

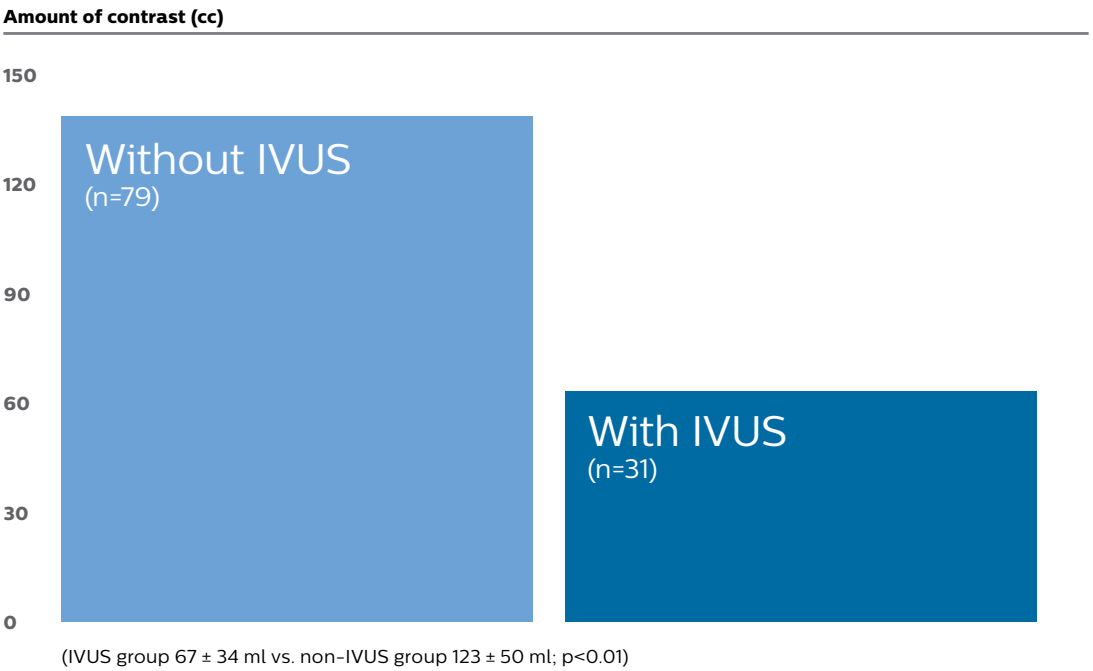

Study data reported a reduction in mean x-ray exposure time
when utilizing adjunctive IVUS vs. angio alone²

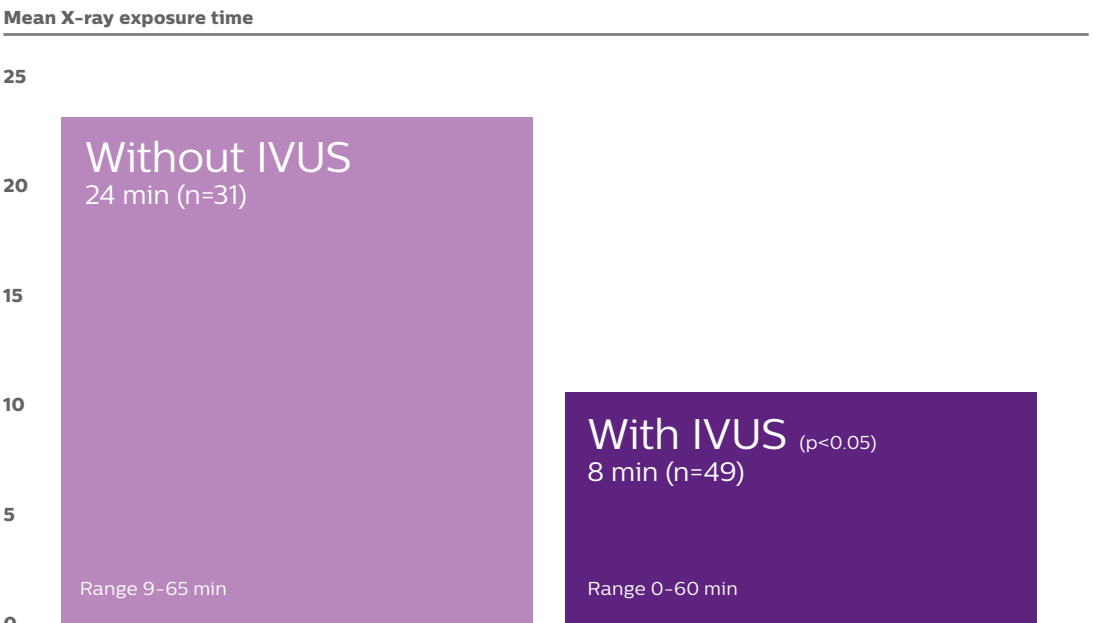

**Help reduce procedural
contrast use and radiation time
with IVUS guided EVAR procedures**